NASA JPL
Data Validation Reports
LDC# 9985

Wet Chemistry

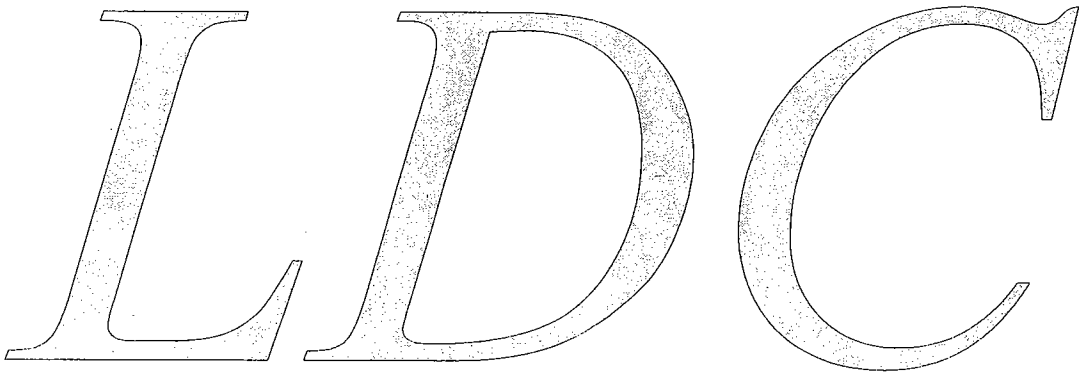

Laboratory Data Consultants, Inc.
Data Validation Report

Project/Site Name: NASA JPL

Collection Date: January 29, 2003

LDC Report Date: March 27, 2003

Matrix: Water

Parameters: Wet Chemistry

Validation Level: EPA Level III

Laboratory: Applied P & Ch Laboratory

Sample Delivery Group (SDG): 03-1369

Sample Identification

EB-1-1/29/03
MW-21-1
MW-21-2
MW-21-3
MW-21-4
MW-21-5
MW-21-5MS
MW-21-5MSD

Introduction

This data review covers 8 water samples listed on the cover sheet including dilutions and reanalysis as applicable. The analyses were per EPA Method 314.0 for Perchlorate, and EPA SW 846 Method 7196 for Hexavalent Chromium.

The review follows a modified outline of the USEPA Contract Laboratory Program National Functional Guidelines for Inorganic Data Review (February 1994) as there are no current guidelines for the methods stated above.

A table summarizing all data qualification is provided at the end of this report. Flags are classified as P (protocol) or A (advisory) to indicate whether the flag is due to a laboratory deviation from a specified protocol or is of technical advisory nature.

Blank results are summarized in Section III.

Field duplicates are summarized in Section IX.

Raw data were not reviewed for this SDG. The review was based on QC data.

The following are definitions of the data qualifiers:

U Indicates the compound or analyte was analyzed for but not detected at or above the stated limit.

J Indicates an estimated value.

R Quality control indicates the data is not usable.

N Presumptive evidence of presence of the constituent.

UJ Indicates the compound or analyte was analyzed for but not detected. The sample detection limit is an estimated value.

A Indicates the finding is based upon technical validation criteria.

P Indicates the finding is related to a protocol/contractual deviation.

None Indicates the data was not significantly impacted by the finding, therefore qualification was not required.

I. Technical Holding Times

All technical holding time requirements were met.

The chain-of-custodies were reviewed for documentation of cooler temperatures. All cooler temperatures met validation criteria.

II. Calibration

a. Initial Calibration

All criteria for the initial calibration of each method were met.

b. Calibration Verification

Calibration verification frequency and analysis criteria were met for each method when applicable.

III. Blanks

Method blanks were reviewed for each matrix as applicable. No contaminant concentrations were found in the method blanks.

IV. Matrix Spike/Matrix Spike Duplicates

Matrix spike (MS) and matrix spike duplicate (MSD) analyses were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

V. Duplicates

Duplicate (DUP) sample analyses were reviewed for each matrix as applicable.

VI. Laboratory Control Samples

Laboratory control samples were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

VII. Sample Result Verification

Raw data were not reviewed for this SDG.

VIII. Overall Assessment of Data

Data flags are summarized at the end of this report.

IX. Field Duplicates

No field duplicates were identified in this SDG.

X. Field Blanks

Sample EB-1-1/29/03 was identified as an equipment blank. No contaminant concentrations were found in this blank.

NASA JPL
Wet Chemistry - Data Qualification Summary - SDG 03-1369

No Sample Data Qualified in this SDG

NASA JPL
Wet Chemistry - Laboratory Blank Data Qualification Summary - SDG 03-1369

No Sample Data Qualified in this SDG

B

Applied P & Ch Laboratory

Wet Analysis Results for Method 7196

Client Name: GEOFON, Inc. Project No: 04-442810 Anal. Method 7196
Project ID: JPL Service ID: 31369 Collected by:

Component Name: Chromium (VI)
CAS No: 1333-82-0

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1369-1	EB-1-1/29/03	Water	01/29/03	01/29/03	01/29/03	03W1295	mg/L	0.01	<0.01	U
03-1369-2	MW-21-1	Water	01/29/03	01/29/03	01/29/03	03W1295	mg/L	0.01	<0.01	U
03-1369-3	MW-21-2	Water	01/29/03	01/29/03	01/29/03	03W1295	mg/L	0.01	<0.01	U
03-1369-4	MW-21-3	Water	01/29/03	01/29/03	01/29/03	03W1295	mg/L	0.01	<0.01	U
03-1369-5	MW-21-4	Water	01/29/03	01/29/03	01/29/03	03W1295	mg/L	0.01	<0.01	U
03-1369-6	MW-21-5	Water	01/29/03	01/29/03	01/29/03	03W1295	mg/L	0.01	<0.01	U
03W1295-MB-01	03W1295-MB-01	Water	01/29/03	01/29/03	01/29/03	03W1295	mg/L	0.01	<0.01	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.
Qualifier: U - Not Detected or less than MDL
B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

2/26/03

Applied P & Ch Laboratory

Wet Analysis Results for Method 314.0

Client Name: GEOFON, Inc. Project No: 04-442810 Anal. Method 314.0

Project ID: JPL Service ID: 31369 Collected by:

Component Name: Perchlorate

CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1369-1	EB-1-1/29/03	Water	01/29/03	01/29/03	01/29/03	03W1286	µg/L	4	<4	U
03-1369-2	MW-21-1	Water	01/29/03	01/29/03	01/29/03	03W1286	µg/L	4	3.1	B
03-1369-3	MW-21-2	Water	01/29/03	01/29/03	01/29/03	03W1286	µg/L	4	<4	U
03-1369-4	MW-21-3	Water	01/29/03	01/29/03	01/29/03	03W1286	µg/L	4	1.9	B
03-1369-5	MW-21-4	Water	01/29/03	01/29/03	01/29/03	03W1286	µg/L	4	1.8	B
03-1369-6	MW-21-5	Water	01/29/03	01/29/03	01/29/03	03W1286	µg/L	4	<4	U
03W1286-MB-01	03W1286-MB-01	Water	01/29/03	01/29/03	01/29/03	03W1286	µg/L	4	<4	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

3/20/03

LDC #: 9985B6 **VALIDATION COMPLETENESS WORKSHEET** Date: 3-27-03
SDG #: 03-1369 Level III Page: 1 of 1
Laboratory: Applied P & Ch Laboratory Reviewer: MG
2nd Reviewer: MD

METHOD: Hexavalent chromium (EPA SW 846 Method 7196) Perchlorate (EPA Method 314.0)

The samples listed below were reviewed for each of the following validation areas. Validation findings are noted in attached validation findings worksheets.

	Validation Area		Comments
I.	Technical holding times	A	Sampling dates: 1-29-03
IIa.	Initial calibration	A	
IIb.	Calibration verification	A	
III.	Blanks	A	
IVa.	Matrix Spike/(Matrix Spike) Duplicates	A	
IVb.	Laboratory control samples	A	LCS/LCSD
V.	Sample result verification	N	
VI.	Overall assessment of data	A	
VII.	Field duplicates	N	
VIII	Field blanks	ND	EB=1

Note: A = Acceptable
N = Not provided/applicable
SW = See worksheet
ND = No compounds detected
R = Rinsate
FB = Field blank
D = Duplicate
TB = Trip blank
EB = Equipment blank

Validated Samples:

1	EB-1-1/29/03 W	11		21		31	
2	MW-21-1	12		22		32	
3	MW-21-2	13		23		33	
4	MW-21-3	14		24		34	
5	MW-21-4	15		25		35	
6	MW-21-5	16		26		36	
7	MW-21-5MS	17		27		37	
8	MW-21-5MSD	18		28		38	
9	PBW	19		29		39	
10		20		30		40	

Notes:

LDC #: 9985B6
SDG #: 03-1369

VALIDATION FINDINGS WORKSHEET
Sample Specific Analysis Reference

Reviewer: MG
2nd reviewer: MH

All circled methods are applicable to each sample.

Sample ID	Parameter
1→6	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) (ClO4) ____ ____ ____
QC 7,8	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____

Comments: _____

Laboratory Data Consultants, Inc.
Data Validation Report

Project/Site Name: NASA JPL

Collection Date: February 3, 2003

LDC Report Date: March 27, 2003

Matrix: Water

Parameters: Wet Chemistry

Validation Level: EPA Level III

Laboratory: Applied P & Ch Laboratory

Sample Delivery Group (SDG): 03-1424

Sample Identification

DUPE-2-1Q03
EB-3-2/3/03
MW-19-1
MW-19-2
MW-19-3
MW-19-4
MW-19-5
DUPE-2-1Q03MS
DUPE-2-1Q03MSD

Introduction

This data review covers 9 water samples listed on the cover sheet including dilutions and reanalysis as applicable. The analyses were per EPA Method 314.0 for Perchlorate, and EPA SW 846 Method 7196 for Hexavalent Chromium.

The review follows a modified outline of the USEPA Contract Laboratory Program National Functional Guidelines for Inorganic Data Review (February 1994) as there are no current guidelines for the methods stated above.

A table summarizing all data qualification is provided at the end of this report. Flags are classified as P (protocol) or A (advisory) to indicate whether the flag is due to a laboratory deviation from a specified protocol or is of technical advisory nature.

Blank results are summarized in Section III.

Field duplicates are summarized in Section IX.

Raw data were not reviewed for this SDG. The review was based on QC data.

The following are definitions of the data qualifiers:

U Indicates the compound or analyte was analyzed for but not detected at or above the stated limit.

J Indicates an estimated value.

R Quality control indicates the data is not usable.

N Presumptive evidence of presence of the constituent.

UJ Indicates the compound or analyte was analyzed for but not detected. The sample detection limit is an estimated value.

A Indicates the finding is based upon technical validation criteria.

P Indicates the finding is related to a protocol/contractual deviation.

None Indicates the data was not significantly impacted by the finding, therefore qualification was not required.

I. Technical Holding Times

All technical holding time requirements were met.

The chain-of-custodies were reviewed for documentation of cooler temperatures. All cooler temperatures met validation criteria.

II. Calibration

a. Initial Calibration

All criteria for the initial calibration of each method were met.

Instrument detection limits, interelement corrections and linear range analysis were performed at the required frequency with the following exceptions:

Analyte	Calibration	Date of Last Report	Report Frequency Requirement	Date of Analysis	Associated Samples	Flag	A or P
Perchlorate	ICAL	7/31/02	Every 6 months	2/3/03	All samples in SDG 03-1424	None	P

b. Calibration Verification

Calibration verification frequency and analysis criteria were met for each method when applicable.

III. Blanks

Method blanks were reviewed for each matrix as applicable. No contaminant concentrations were found in the method blanks.

IV. Matrix Spike/Matrix Spike Duplicates

Matrix spike (MS) and matrix spike duplicate (MSD) analyses were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

V. Duplicates

Duplicate (DUP) sample analyses were reviewed for each matrix as applicable.

VI. Laboratory Control Samples

Laboratory control samples were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

VII. Sample Result Verification

Raw data were not reviewed for this SDG.

VIII. Overall Assessment of Data

Data flags are summarized at the end of this report.

IX. Field Duplicates

Samples DUPE-2-1Q03 and MW-19-4 were identified as field duplicates. No contaminant concentrations were detected in any of the samples.

X. Field Blanks

Sample EB-3-2/3/03 was identified as an equipment blank. No contaminant concentrations were found in this blank.

NASA JPL
Wet Chemistry - Data Qualification Summary - SDG 03-1424

SDG	Sample	Analyte	Flag	A or P	Reason
03-1424	DUPE-2-1Q03 EB-3-2/3/03 MW-19-1 MW-19-2 MW-19-3 MW-19-4 MW-19-5	Perchlorate	None	P	Calibration

NASA JPL
Wet Chemistry - Laboratory Blank Data Qualification Summary - SDG 03-1424

No Sample Data Qualified in this SDG

C

Applied P & Ch Laboratory

Wet Analysis Results for Method 7196

Client Name: GEOFON, Inc. Project No: 04-4428.10 Anal. Method 7196
Project ID: JPL Service ID: 31424 Collected by:

Component Name: Chromium (VI)
CAS No: 1333-82-0

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1424-1	DUPE-2-1Q03	Water	02/03/03	02/03/03	02/03/03	03W1348	mg/L	0.01	<0.01	U
03-1424-2	EB-3-2/3/03	Water	02/03/03	02/03/03	02/03/03	03W1348	mg/L	0.01	<0.01	U
03-1424-3	MW-19-1	Water	02/03/03	02/03/03	02/03/03	03W1348	mg/L	0.01	<0.01	U
03-1424-4	MW-19-2	Water	02/03/03	02/03/03	02/03/03	03W1348	mg/L	0.01	<0.01	U
03-1424-5	MW-19-3	Water	02/03/03	02/03/03	02/03/03	03W1348	mg/L	0.01	<0.01	U
03-1424-6	MW-19-4	Water	02/03/03	02/03/03	02/03/03	03W1348	mg/L	0.01	<0.01	U
03-1424-7	MW-19-5	Water	02/03/03	02/03/03	02/03/03	03W1348	mg/L	0.01	<0.01	U
03W1348-MB-01	03W1348-MB-01	Water	02/03/03	02/03/03	02/03/03	03W1348	mg/L	0.01	<0.01	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.
Qualifier: U - Not Detected or less than MDL
B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

3/28/03

Applied P & Ch Laboratory

Wet Analysis Results for Method 314.0

Client Name: GEOFON, Inc. Project No: 04-4428.10 Anal. Method 314.0

Project ID: JPL Service ID: 31424 Collected by:

Component Name: Perchlorate

CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1424-1	DUPE-2-1Q03	Water	02/03/03	02/03/03	02/03/03	03W1345	µg/L	4	<4	U
03-1424-2	EB-3-2/3/03	Water	02/03/03	02/03/03	02/03/03	03W1345	µg/L	4	<4	U
03-1424-3	MW-19-1	Water	02/03/03	02/03/03	02/03/03	03W1345	µg/L	4	<4	U
03-1424-4	MW-19-2	Water	02/03/03	02/03/03	02/03/03	03W1345	µg/L	4	<4	U
03-1424-5	MW-19-3	Water	02/03/03	02/03/03	02/03/03	03W1345	µg/L	4	<4	U
03-1424-6	MW-19-4	Water	02/03/03	02/03/03	02/03/03	03W1345	µg/L	4	<4	U
03-1424-7	MW-19-5	Water	02/03/03	02/03/03	02/03/03	03W1345	µg/L	4	<4	U
03W1345-MB-01	03W1345-MB-01	Water	02/03/03	02/03/03	02/03/03	03W1345	µg/L	4	<4	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

3/28/03

LDC #: 9985C6
SDG #: 03-1424
Laboratory: Applied P & Ch Laboratory

VALIDATION COMPLETENESS WORKSHEET
Level III

Date: 3-27-03
Page: 1 of 1
Reviewer: MG
2nd Reviewer: MH

METHOD: Hexavalent chromium (EPA SW 846 Method 7196) Perchlorate (EPA Method 314.0)

The samples listed below were reviewed for each of the following validation areas. Validation findings are noted in attached validation findings worksheets.

	Validation Area		Comments
I.	Technical holding times	A	Sampling dates: 2-3-03
IIa.	Initial calibration	SW	
IIb.	Calibration verification	A	
III.	Blanks	A	
IVa.	Matrix Spike/(Matrix Spike) Duplicates	A	MW-20-3 MS/MSD (SDG: 03-1402)
IVb.	Laboratory control samples	A	LCS/LCSD
V.	Sample result verification	N	
VI.	Overall assessment of data	A	
VII.	Field duplicates	ND	D = 1+6
VIII.	Field blanks	ND	EB = 2

Note: A = Acceptable
N = Not provided/applicable
SW = See worksheet
ND = No compounds detected
R = Rinsate
FB = Field blank
D = Duplicate
TB = Trip blank
EB = Equipment blank

Validated Samples:

1	DUPE-2-1Q03 W	11		21		31	
2	EB-3-2/3/03	12		22		32	
3	MW-19-1	13		23		33	
4	MW-19-2	14		24		34	
5	MW-19-3	15		25		35	
6	MW-19-4	16		26		36	
7	MW-19-5	17		27		37	
8	DUPE-2-1Q03MS	18		28		38	
9	DUPE-2-1Q03MSD	19		29		39	
10	PBW	20		30		40	

Notes:

LDC #: 9985C6
SDG #: 03-1424

VALIDATION FINDINGS WORKSHEET
Sample Specific Analysis Reference

Reviewer: MG
2nd reviewer: MM

All circled methods are applicable to each sample.

Sample ID	Parameter
1 → 7	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) (ClO4) ____ ____ ____
QC 8, 9	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____

Comments: _____

LDC #: 998506
SDG #: 03-1424

VALIDATION FINDINGS WORKSHEET
Calibration

Reviewer: MG
2nd Reviewer: MK

METHOD: Inorganics, EPA Method See cover

Please see qualifications below for all questions answered "N". Not applicable questions are identified as "N/A".

Y (N) N/A Were all instruments calibrated daily, each set-up time, and were the proper number of standards used?
(Y) N N/A Were all initial and continuing calibration verification percent recoveries (%R) within the control limits of 90-110% ?
(Y) N N/A Are all correlation coefficients $\geq$0.995 ?

LEVEL IV/D ONLY:

Y N N/A Were recalculated results acceptable? See Level IV Initial and Continuing Calibration Recaluculation Worksheet for recalulations.
Y N N/A Was a balance check conducted prior to the TDS analysis.?
Y N N/A Was the titrant normality checked?

#	Date	Calibration ID	Analyte	%R	Associated Samples	Qualifications
1	7-31-02	ICAL	ClO_4	ICAL > 6 mo. old	all	None / P
				(samples analyzed: 2-3-03)		

Comments:

Laboratory Data Consultants, Inc.
Data Validation Report

Project/Site Name: NASA JPL

Collection Date: February 4, 2003

LDC Report Date: March 27, 2003

Matrix: Water

Parameters: Wet Chemistry

Validation Level: EPA Level III

Laboratory: Applied P & Ch Laboratory

Sample Delivery Group (SDG): 03-1444

Sample Identification

EB-4-2/4/03
MW-17-2
MW-17-3
MW-17-4
MW-17-2MS
MW-17-2MSD

Introduction

This data review covers 6 water samples listed on the cover sheet including dilutions and reanalysis as applicable. The analyses were per EPA Method 314.0 for Perchlorate, and EPA SW 846 Method 7196 for Hexavalent Chromium.

The review follows a modified outline of the USEPA Contract Laboratory Program National Functional Guidelines for Inorganic Data Review (February 1994) as there are no current guidelines for the methods stated above.

A table summarizing all data qualification is provided at the end of this report. Flags are classified as P (protocol) or A (advisory) to indicate whether the flag is due to a laboratory deviation from a specified protocol or is of technical advisory nature.

Blank results are summarized in Section III.

Field duplicates are summarized in Section IX.

Raw data were not reviewed for this SDG. The review was based on QC data.

The following are definitions of the data qualifiers:

U Indicates the compound or analyte was analyzed for but not detected at or above the stated limit.

J Indicates an estimated value.

R Quality control indicates the data is not usable.

N Presumptive evidence of presence of the constituent.

UJ Indicates the compound or analyte was analyzed for but not detected. The sample detection limit is an estimated value.

A Indicates the finding is based upon technical validation criteria.

P Indicates the finding is related to a protocol/contractual deviation.

None Indicates the data was not significantly impacted by the finding, therefore qualification was not required.

I. Technical Holding Times

All technical holding time requirements were met.

The chain-of-custodies were reviewed for documentation of cooler temperatures. All cooler temperatures met validation criteria.

II. Calibration

a. Initial Calibration

All criteria for the initial calibration of each method were met.

Instrument detection limits, interelement corrections and linear range analysis were performed at the required frequency with the following exceptions:

Analyte	Calibration	Date of Last Report	Report Frequency Requirement	Date of Analysis	Associated Samples	Flag	A or P
Perchlorate	ICAL	7/31/02	Every 6 months	2/10-2/11/03	All samples in SDG 03-1444	None	P

b. Calibration Verification

Calibration verification frequency and analysis criteria were met for each method when applicable.

III. Blanks

Method blanks were reviewed for each matrix as applicable. No contaminant concentrations were found in the method blanks.

IV. Matrix Spike/Matrix Spike Duplicates

Matrix spike (MS) and matrix spike duplicate (MSD) analyses were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits with the following exceptions:

Spike ID (Associated Samples)	Analyte	MS (%R) (Limits)	MSD (%R) (Limits)	RPD (Limits)	Flag	A or P
MW-17-2MS/MSD (All samples in SDG 03-1444)	Hexavalent chromium	76 (78-115)	-	-	J (all detects) UJ (all non-detects)	A

V. Duplicates

Duplicate (DUP) sample analyses were reviewed for each matrix as applicable.

VI. Laboratory Control Samples

Laboratory control samples were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

VII. Sample Result Verification

Raw data were not reviewed for this SDG.

VIII. Overall Assessment of Data

Data flags are summarized at the end of this report.

IX. Field Duplicates

No field duplicates were identified in this SDG.

X. Field Blanks

Sample EB-4-2/4/03 was identified as an equipment blank. No contaminant concentrations were found in this blank.

NASA JPL
Wet Chemistry - Data Qualification Summary - SDG 03-1444

SDG	Sample	Analyte	Flag	A or P	Reason
03-1444	EB-4-2/4/03 MW-17-2 MW-17-3 MW-17-4	Perchlorate	None	P	Calibration
03-1444	EB-4-2/4/03 MW-17-2 MW-17-3 MW-17-4	Hexavalent chromium	J (all detects) UJ (all non-detects)	A	Matrix spike/Matrix spike duplicates (%R)

NASA JPL
Wet Chemistry - Laboratory Blank Data Qualification Summary - SDG 03-1444

No Sample Data Qualified in this SDG

D

Applied P & Ch Laboratory

Wet Analysis Results for Method 7196

Client Name: GEOFON, Inc. Project No: 04-4428.10 Anal. Method 7196
Project ID: JPL Service ID: 31444 Collected by:

Component Name: Chromium (VI)
CAS No: 1333-82-0

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1444-1	EB-4-2/4/03	Water	02/04/03	02/04/03	02/04/03	03W1370	mg/L	0.01	<0.01	U UJ
03-1444-2	MW-17-2	Water	02/04/03	02/04/03	02/04/03	03W1370	mg/L	0.01	<0.01	U
03-1444-3	MW-17-3	Water	02/04/03	02/04/03	02/04/03	03W1370	mg/L	0.01	<0.01	U
03-1444-4	MW-17-4	Water	02/04/03	02/04/03	02/04/03	03W1370	mg/L	0.01	<0.01	U
03W1370-MB-01	03W1370-MB-01	Water	02/04/03	02/04/03	02/04/03	03W1370	mg/L	0.01	<0.01	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.
Qualifier: U - Not Detected or less than MDL
B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

3/26/03

Applied P & Ch Laboratory

Wet Analysis Results for Method 314.0

Client Name: GEOFON, Inc. Project No: 04-4428.10 Anal. Method 314.0
Project ID: JPL Service ID: 31444 Collected by:

Component Name: Perchlorate
CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1444-1	EB-4-2/4/03	Water	02/04/03	02/04/03	02/11/03	03W1424	µg/L	4	<4	U
03-1444-2	MW-17-2	Water	02/04/03	02/04/03	02/10/03	03W1424	µg/L	4	3.4	B
03-1444-3	MW-17-3	Water	02/04/03	02/04/03	02/11/03	03W1424	µg/L	8	145	
03-1444-4	MW-17-4	Water	02/04/03	02/04/03	02/10/03	03W1424	µg/L	4	<4	U
03W1424-MB-01	03W1424-MB-01	Water	02/10/03	02/10/03	02/10/03	03W1424	µg/L	4	<4	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.
Qualifier: U - Not Detected or less than MDL
B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

3/28/03

LDC #: 9985D6
SDG #: 03-1444
Laboratory: Applied P & Ch Laboratory

VALIDATION COMPLETENESS WORKSHEET
Level III

Date: 3-27-03
Page: 1 of 1
Reviewer: MG
2nd Reviewer: MB

METHOD: Hexavalent chromium (EPA SW 846 Method 7196) Perchlorate (EPA Method 314.0)

The samples listed below were reviewed for each of the following validation areas. Validation findings are noted in attached validation findings worksheets.

	Validation Area		Comments
I.	Technical holding times	A	Sampling dates: 2-4-03
IIa.	Initial calibration	SW	
IIb.	Calibration verification	A	
III.	Blanks	A	
IVa.	Matrix Spike/(Matrix Spike) Duplicates	SW	
IVb.	Laboratory control samples	A	LCS/LCSD
V.	Sample result verification	N	
VI.	Overall assessment of data	A	
VII.	Field duplicates	N	
VIII.	Field blanks	ND	EB = 1

Note: A = Acceptable
N = Not provided/applicable
SW = See worksheet
ND = No compounds detected
R = Rinsate
FB = Field blank
D = Duplicate
TB = Trip blank
EB = Equipment blank

Validated Samples:

1	EB-4-2/4/03 W	11		21		31	
2	MW-17-2	12		22		32	
3	MW-17-3	13		23		33	
4	MW-17-4	14		24		34	
5	MW-17-2MS	15		25		35	
6	MW-17-2MSD	16		26		36	
7	PBW	17		27		37	
8		18		28		38	
9		19		29		39	
10		20		30		40	

Notes: _____

LDC #: 9985D6
SDG #: 03-1444

VALIDATION FINDINGS WORKSHEET
Sample Specific Analysis Reference

Page: 1 of 1
Reviewer: MG
2nd reviewer: MW

All circled methods are applicable to each sample.

Sample ID	Parameter
1→4	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) (ClO_4) ____ ____ ____
QC 5,6	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) (ClO_4) ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+}

Comments:______________________________

LDC #: 9985D6
SDG #: 03-1444

VALIDATION FINDINGS WORKSHEET
Calibration

Page: 1 of 1
Reviewer: MG
2nd Reviewer: MB

METHOD: Inorganics, EPA Method See cover

Please see qualifications below for all questions answered "N". Not applicable questions are identified as "N/A".

Y (N) N/A Were all instruments calibrated daily, each set-up time, and were the proper number of standards used?
(Y) N N/A Were all initial and continuing calibration verification percent recoveries (%R) within the control limits of 90-110% ?
(Y) N N/A Are all correlation coefficients $\geq$0.995 ?

LEVEL IV/D ONLY:

Y N N/A Were recalculated results acceptable? See Level IV Initial and Continuing Calibration Recaluculation Worksheet for recalulations.
Y N N/A Was a balance check conducted prior to the TDS analysis.?
Y N N/A Was the titrant normality checked?

#	Date	Calibration ID	Analyte	%R	Associated Samples	Qualifications
1	7-31-02	ICAL	ClO4	ICAL > 6 mo. old (samples analyzed: 2-10→2-11-03)	all	None / P

Comments:

LDC #: 9985D6
SDG #: 03-1444

VALIDATION FINDINGS WORKSHEET
Matrix Spike/Matrix Spike Duplicates

Reviewer: MG
2nd Reviewer: MW

METHOD: Inorganics, EPA Method See Cover

Please see qualifications below for all questions answered "N". Not applicable questions are identified as "N/A".

(Y) N N/A Was a matrix spike analyzed for each matrix in this SDG?

Y (N) N/A Were matrix spike percent recoveries (%R) within the control limits of 75-125? If the sample concentration exceeded the spike concentration by a factor of 4 or more, no action was taken.

(Y) N N/A Were all duplicate sample relative percent differences (RPD) ≤ 20% for water samples and ≤35% for soil samples?

LEVEL IV ONLY:

Y N N/A Were recalculated results acceptable? See Level IV Recalculation Worksheet for recalculations.

#	MS/MSD ID	Matrix	Analyte	MS %Recovery	MSD %Recovery	RPD (Limits)	Associated Samples	Qualifications
1	5/6	water	Cr VI	76 (78-115)			all	J/UJ/A

Comments:

Laboratory Data Consultants, Inc.
Data Validation Report

Project/Site Name: NASA JPL

Collection Date: February 5, 2003

LDC Report Date: March 27, 2003

Matrix: Water

Parameters: Wet Chemistry

Validation Level: EPA Level III

Laboratory: Applied P & Ch Laboratory

Sample Delivery Group (SDG): 03-1457

Sample Identification

EB-5-2/5/03
MW-18-2
MW-18-3
MW-18-4
MW-18-5
EB-5-2/5/03MS
EB-5-2/5/03MSD

Introduction

This data review covers 7 water samples listed on the cover sheet including dilutions and reanalysis as applicable. The analyses were per EPA Method 314.0 for Perchlorate, and EPA SW 846 Method 7196 for Hexavalent Chromium.

The review follows a modified outline of the USEPA Contract Laboratory Program National Functional Guidelines for Inorganic Data Review (February 1994) as there are no current guidelines for the methods stated above.

A table summarizing all data qualification is provided at the end of this report. Flags are classified as P (protocol) or A (advisory) to indicate whether the flag is due to a laboratory deviation from a specified protocol or is of technical advisory nature.

Blank results are summarized in Section III.

Field duplicates are summarized in Section IX.

Raw data were not reviewed for this SDG. The review was based on QC data.

The following are definitions of the data qualifiers:

U Indicates the compound or analyte was analyzed for but not detected at or above the stated limit.

J Indicates an estimated value.

R Quality control indicates the data is not usable.

N Presumptive evidence of presence of the constituent.

UJ Indicates the compound or analyte was analyzed for but not detected. The sample detection limit is an estimated value.

A Indicates the finding is based upon technical validation criteria.

P Indicates the finding is related to a protocol/contractual deviation.

None Indicates the data was not significantly impacted by the finding, therefore qualification was not required.

I. Technical Holding Times

All technical holding time requirements were met.

The chain-of-custodies were reviewed for documentation of cooler temperatures. All cooler temperatures met validation criteria.

II. Calibration

a. Initial Calibration

All criteria for the initial calibration of each method were met.

Instrument detection limits, interelement corrections and linear range analysis were performed at the required frequency with the following exceptions:

Analyte	Calibration	Date of Last Report	Report Frequency Requirement	Date of Analysis	Associated Samples	Flag	A or P
Perchlorate	ICAL	7/31/02	Every 6 months	2/10/03	All samples in SDG 03-1457	None	P

b. Calibration Verification

Calibration verification frequency and analysis criteria were met for each method when applicable.

III. Blanks

Method blanks were reviewed for each matrix as applicable. No contaminant concentrations were found in the method blanks.

IV. Matrix Spike/Matrix Spike Duplicates

Matrix spike (MS) and matrix spike duplicate (MSD) analyses were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

V. Duplicates

Duplicate (DUP) sample analyses were reviewed for each matrix as applicable.

VI. Laboratory Control Samples

Laboratory control samples were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

VII. Sample Result Verification

Raw data were not reviewed for this SDG.

VIII. Overall Assessment of Data

Data flags are summarized at the end of this report.

IX. Field Duplicates

No field duplicates were identified in this SDG.

X. Field Blanks

Sample EB-5-2/5/03 was identified as an equipment blank. No contaminant concentrations were found in this blank.

NASA JPL
Wet Chemistry - Data Qualification Summary - SDG 03-1457

SDG	Sample	Analyte	Flag	A or P	Reason
03-1457	EB-5-2/5/03 MW-18-2 MW-18-3 MW-18-4 MW-18-5	Perchlorate	None	P	Calibration

NASA JPL
Wet Chemistry - Laboratory Blank Data Qualification Summary - SDG 03-1457

No Sample Data Qualified in this SDG

E

Applied P & Ch Laboratory

Wet Analysis Results for Method 7196

Client Name: GEOFON, Inc. Project No: 04-4428.10 Anal. Method 7196
Project ID: JPL Service ID: 31457 Collected by:

Component Name: Chromium (VI)
CAS No: 1333-82-0

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1457-1	EB-5-2/5/03	Water	02/05/03	02/05/03	02/05/03	03W1379	mg/L	0.01	<0.01	U
03-1457-2	MW-18-2	Water	02/05/03	02/05/03	02/05/03	03W1379	mg/L	0.01	<0.01	U
03-1457-3	MW-18-3	Water	02/05/03	02/05/03	02/05/03	03W1379	mg/L	0.01	<0.01	U
03-1457-4	MW-18-4	Water	02/05/03	02/05/03	02/05/03	03W1379	mg/L	0.01	<0.01	U
03-1457-5	MW-18-5	Water	02/05/03	02/05/03	02/05/03	03W1379	mg/L	0.01	<0.01	U
03W1379-MB-01	03W1379-MB-01	Water	02/05/03	02/05/03	02/05/03	03W1379	mg/L	0.01	<0.01	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.
Qualifier: U - Not Detected or less than MDL
B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

3/26/03

Applied P & Ch Laboratory

Wet Analysis Results for Method 314.0

Client Name: GEOFON, Inc. Project No: 04-4428.10 Anal. Method 314.0

Project ID: JPL Service ID: 31457 Collected by:

Component Name: Perchlorate

CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1457-1	EB-5-2/5/03	Water	02/05/03	02/05/03	02/10/03	03W1424	µg/L	4	<4	U
03-1457-2	MW-18-2	Water	02/05/03	02/05/03	02/10/03	03W1424	µg/L	4	<4	U
03-1457-3	MW-18-3	Water	02/05/03	02/05/03	02/10/03	03W1424	µg/L	4	<4	U
03-1457-4	MW-18-4	Water	02/05/03	02/05/03	02/10/03	03W1424	µg/L	4	24.6	
03-1457-5	MW-18-5	Water	02/05/03	02/05/03	02/10/03	03W1424	µg/L	4	<4	U
03W1424-MB-01	03W1424-MB-01	Water	02/10/03	02/10/03	02/10/03	03W1424	µg/L	4	<4	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

2/7-8/03

LDC #: 9985E6
SDG #: 03-1457
Laboratory: Applied P & Ch Laboratory

VALIDATION COMPLETENESS WORKSHEET
Level III

Date: 3-27-03
Page: 1 of 1
Reviewer: MG
2nd Reviewer: [illegible]

METHOD: Hexavalent chromium (EPA SW 846 Method 7196) Perchlorate (EPA Method 314.0)

The samples listed below were reviewed for each of the following validation areas. Validation findings are noted in attached validation findings worksheets.

	Validation Area		Comments
I.	Technical holding times	A	Sampling dates: 2-5-03
IIa.	Initial calibration	SW	
IIb.	Calibration verification	A	
III.	Blanks	A	
IVa.	Matrix Spike/(Matrix Spike) Duplicates	A	MW-4-1 MS/MSD (SDG: 03-1501)
IVb.	Laboratory control samples	A	LCS/LCSD
V.	Sample result verification	N	
VI.	Overall assessment of data	A	
VII.	Field duplicates	N	
VIII.	Field blanks	ND	EB = 1

Note: A = Acceptable
N = Not provided/applicable
SW = See worksheet
ND = No compounds detected
R = Rinsate
FB = Field blank
D = Duplicate
TB = Trip blank
EB = Equipment blank

Validated Samples:

1 | EB-5-2/5/03 W		11		21		31	
2 | MW-18-2		12		22		32	
3 | MW-18-3		13		23		33	
4 | MW-18-4		14		24		34	
5 | MW-18-5		15		25		35	
6 | EB-5-2/5/03MS		16		26		36	
7 | EB-5-2/5/03MSD		17		27		37	
8 | PBW		18		28		38	
9		19		29		39	
10		20		30		40	

Notes:

LDC #: 9985E6
SDG #: 03-1457

VALIDATION FINDINGS WORKSHEET
Sample Specific Analysis Reference

Page: 1 of 1
Reviewer: MG
2nd reviewer: MV

All circled methods are applicable to each sample.

Sample ID	Parameter
1→5	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) (ClO4) ____ ____ ____
QC MS 6,7	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____

Comments: _____

LDC #: 9985E6
SDG #: 03-1457

VALIDATION FINDINGS WORKSHEET
Calibration

Reviewer: MG
2nd Reviewer: MB

METHOD: Inorganics, EPA Method See cover

Please see qualifications below for all questions answered "N". Not applicable questions are identified as "N/A".

Y (N) N/A Were all instruments calibrated daily, each set-up time, and were the proper number of standards used?
(Y) N N/A Were all initial and continuing calibration verification percent recoveries (%R) within the control limits of 90-110% ?
(Y) N N/A Are all correlation coefficients ≥0.995 ?

LEVEL IV/D ONLY:

Y N N/A Were recalculated results acceptable? See Level IV Initial and Continuing Calibration Recaluculation Worksheet for recalulations.
Y N N/A Was a balance check conducted prior to the TDS analysis.?
Y N N/A Was the titrant normality checked?

#	Date	Calibration ID	Analyte	%R	Associated Samples	Qualifications
1	7-31-02	ICAL	ClO4	ICAL > 6 mo. old	all	None /P
				(samples analyzed: 2-10-03)		

Comments:

Laboratory Data Consultants, Inc.
Data Validation Report

Project/Site Name: NASA JPL

Collection Date: February 6, 2003

LDC Report Date: March 27, 2003

Matrix: Water

Parameters: Wet Chemistry

Validation Level: EPA Level III

Laboratory: Applied P & Ch Laboratory

Sample Delivery Group (SDG): 03-1501

Sample Identification

EB-6-2/6/03
MW-4-1
MW-4-2
MW-4-3
MW-3-2
MW-3-3
MW-3-4
MW-4-1MS
MW-4-1MSD

Introduction

This data review covers 9 water samples listed on the cover sheet including dilutions and reanalysis as applicable. The analyses were per EPA Method 314.0 for Perchlorate, and EPA SW 846 Method 7196 for Hexavalent Chromium.

The review follows a modified outline of the USEPA Contract Laboratory Program National Functional Guidelines for Inorganic Data Review (February 1994) as there are no current guidelines for the methods stated above.

A table summarizing all data qualification is provided at the end of this report. Flags are classified as P (protocol) or A (advisory) to indicate whether the flag is due to a laboratory deviation from a specified protocol or is of technical advisory nature.

Blank results are summarized in Section III.

Field duplicates are summarized in Section IX.

Raw data were not reviewed for this SDG. The review was based on QC data.

The following are definitions of the data qualifiers:

U Indicates the compound or analyte was analyzed for but not detected at or above the stated limit.

J Indicates an estimated value.

R Quality control indicates the data is not usable.

N Presumptive evidence of presence of the constituent.

UJ Indicates the compound or analyte was analyzed for but not detected. The sample detection limit is an estimated value.

A Indicates the finding is based upon technical validation criteria.

P Indicates the finding is related to a protocol/contractual deviation.

None Indicates the data was not significantly impacted by the finding, therefore qualification was not required.

I. Technical Holding Times

All technical holding time requirements were met.

The chain-of-custodies were reviewed for documentation of cooler temperatures. All cooler temperatures met validation criteria.

II. Calibration

a. Initial Calibration

All criteria for the initial calibration of each method were met.

Instrument detection limits, interelement corrections and linear range analysis were performed at the required frequency with the following exceptions:

Analyte	Calibration	Date of Last Report	Report Frequency Requirement	Date of Analysis	Associated Samples	Flag	A or P
Perchlorate	ICAL	7/31/02	Every 6 months	2/10/03	All samples in SDG 03-1501	None	P

b. Calibration Verification

Calibration verification frequency and analysis criteria were met for each method when applicable.

III. Blanks

Method blanks were reviewed for each matrix as applicable. No contaminant concentrations were found in the method blanks.

IV. Matrix Spike/Matrix Spike Duplicates

Matrix spike (MS) and matrix spike duplicate (MSD) analyses were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

V. Duplicates

Duplicate (DUP) sample analyses were reviewed for each matrix as applicable.

VI. Laboratory Control Samples

Laboratory control samples were reviewed for each matrix as applicable. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

VII. Sample Result Verification

Raw data were not reviewed for this SDG.

VIII. Overall Assessment of Data

Data flags are summarized at the end of this report.

IX. Field Duplicates

No field duplicates were identified in this SDG.

X. Field Blanks

Sample EB-6-2/6/03 was identified as an equipment blank. No contaminant concentrations were found in this blank.

NASA JPL
Wet Chemistry - Data Qualification Summary - SDG 03-1501

SDG	Sample	Analyte	Flag	A or P	Reason
03-1501	EB-6-2/6/03 MW-4-1 MW-4-2 MW-4-3 MW-3-2 MW-3-3 MW-3-4	Perchlorate	None	P	Calibration

NASA JPL
Wet Chemistry - Laboratory Blank Data Qualification Summary - SDG 03-1501

No Sample Data Qualified in this SDG

F

Applied P & Ch Laboratory

Wet Analysis Results for Method 7196

Client Name: GEOFON, Inc. Project No: 04-4428.10 Anal. Method 7196

Project ID: JPL Service ID: 31501 Collected by:

Component Name: Chromium (VI)

CAS No: 1333-82-0

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1501-1	EB-6-2/6/03	Water	02/06/03	02/06/03	02/06/03	03W1392	mg/L	0.01	<0.01	U
03-1501-2	MW-4-1	Water	02/06/03	02/06/03	02/06/03	03W1392	mg/L	0.01	<0.01	U
03-1501-3	MW-4-2	Water	02/06/03	02/06/03	02/06/03	03W1392	mg/L	0.01	<0.01	U
03-1501-4	MW-4-3	Water	02/06/03	02/06/03	02/06/03	03W1392	mg/L	0.01	<0.01	U
03-1501-6	MW-3-2	Water	02/06/03	02/06/03	02/06/03	03W1392	mg/L	0.01	<0.01	U
03-1501-7	MW-3-3	Water	02/06/03	02/06/03	02/06/03	03W1392	mg/L	0.01	<0.01	U
03-1501-8	MW-3-4	Water	02/06/03	02/06/03	02/06/03	03W1392	mg/L	0.01	<0.01	U
03W1392-MB-01	03W1392-MB-01	Water	02/06/03	02/06/03	02/06/03	03W1392	mg/L	0.01	<0.01	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

3/28/03

Applied P & Ch Laboratory

Wet Analysis Results for Method 314.0

Client Name: GEOFON, Inc. Project No: 04-4428.10 Anal. Method 314.0

Project ID: JPL Service ID: 31501 Collected by:

Component Name: Perchlorate

CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-1501-1	EB-6-2/6/03	Water	02/06/03	02/06/03	02/10/03	03W1424	µg/L	4	<4	U
03-1501-2	MW-4-1	Water	02/06/03	02/06/03	02/10/03	03W1424	µg/L	4	2.9	B
03-1501-3	MW-4-2	Water	02/06/03	02/06/03	02/10/03	03W1424	µg/L	4	<4	U
03-1501-4	MW-4-3	Water	02/06/03	02/06/03	02/10/03	03W1424	µg/L	4	<4	U
03-1501-6	MW-3-2	Water	02/06/03	02/06/03	02/10/03	03W1424	µg/L	4	<4	U
03-1501-7	MW-3-3	Water	02/06/03	02/06/03	02/10/03	03W1424	µg/L	4	<4	U
03-1501-8	MW-3-4	Water	02/06/03	02/06/03	02/10/03	03W1424	µg/L	4	<4	U
03W1424-MB-01	03W1424-MB-01	Water	02/10/03	02/10/03	02/10/03	03W1424	µg/L	4	<4	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

3/7/03

LDC #: 9985F6 **VALIDATION COMPLETENESS WORKSHEET** Date: 3-27-03
SDG #: 03-1501 Level III Page: 1 of 1
Laboratory: Applied P & Ch Laboratory Reviewer: MG
2nd Reviewer: MD

METHOD: Hexavalent chromium (EPA SW 846 Method 7196) Perchlorate (EPA Method 314.0)

The samples listed below were reviewed for each of the following validation areas. Validation findings are noted in attached validation findings worksheets.

	Validation Area		Comments
I.	Technical holding times	A	Sampling dates: 2-6-03
IIa.	Initial calibration	SW	
IIb.	Calibration verification	A	
III.	Blanks	A	
IVa.	Matrix Spike/(Matrix Spike) Duplicates	A	
IVb.	Laboratory control samples	A	LCS/LCSD
V.	Sample result verification	N	
VI.	Overall assessment of data	A	
VII.	Field duplicates	N	
VIII.	Field blanks	ND	EB = 1

Note: A = Acceptable
N = Not provided/applicable
SW = See worksheet
ND = No compounds detected
R = Rinsate
FB = Field blank
D = Duplicate
TB = Trip blank
EB = Equipment blank

Validated Samples:

1 | EB-6-2/6/03 W	11		21		31		
2 | MW-4-1	12		22		32		
3 | MW-4-2	13		23		33		
4 | MW-4-3	14		24		34		
5 | MW-3-2	15		25		35		
6 | MW-3-3	16		26		36		
7 | MW-3-4	17		27		37		
8 | MW-4-1MS	18		28		38		
9 | MW-4-1MSD	19		29		39		
10 | PBW	20		30		40		

Notes: _____

LDC #: 9985F6
SDG #: 03-1501

VALIDATION FINDINGS WORKSHEET
Sample Specific Analysis Reference

Page: 1 of 1
Reviewer: MG
2nd reviewer: MM

All circled methods are applicable to each sample.

Sample ID	Parameter
1→7	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) (ClO4) ____ ____ ____
QC 8,9	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC (CR^{6+}) (ClO4) ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____
	pH TDS Cl F NO_3 NO_2 SO_4 PO_4 ALK CN^- NH_3 TKN TOC CR^{6+} ____ ____ ____ ____

Comments: _____

LDC #: 9985F6
SDG #: 03-1501

VALIDATION FINDINGS WORKSHEET
Calibration

Page: 1 of 1
Reviewer: MG
2nd Reviewer: [illegible]

METHOD: Inorganics, EPA Method See cover

Please see qualifications below for all questions answered "N". Not applicable questions are identified as "N/A".

Y (N) N/A Were all instruments calibrated daily, each set-up time, and were the proper number of standards used?
(Y) N N/A Were all initial and continuing calibration verification percent recoveries (%R) within the control limits of 90-110% ?
(Y) N N/A Are all correlation coefficients ≥0.995 ?

LEVEL IV/D ONLY:

Y N N/A Were recalculated results acceptable? See Level IV Initial and Continuing Calibration Recaluculation Worksheet for recalulations.
Y N N/A Was a balance check conducted prior to the TDS analysis.?
Y N N/A Was the titrant normality checked?

#	Date	Calibration ID	Analyte	%R	Associated Samples	Qualifications
1	7-31-02	ICAL	ClO4	ICAL > 6 mo. old	all	None /P
				(samples analyzed: 2-10-03)		

Comments:

TARGET COMPOUND WORKSHEET

ETHOD: VOA (EPA Method TO-14/TO-14A)

A. Chloromethane*	S. Trichloroethene	KK. Trichlorofluoromethane	CCC. tert-Butylbenzene	UUU. Benzyl chloride
B. Bromomethane	T. Dibromochloromethane	LL. Methyl-tert-butyl ether	DDD. 1,2,4-Trimethylbenzene	VVV. 4-Ethyltoluene
C. Vinyl choride**	U. 1,1,2-Trichloroethane	MM. 1,2-Dibromo-3-chloropropane	EEE. sec-Butylbenzene	WWW. Ethanol
D. Chloroethane	V. Benzene	NN. Diethyl ether	FFF. 1,3-Dichlorobenzene	XXX. Ethyl ether
E. Methylene chloride	W. trans-1,3-Dichloropropene	OO. 2,2-Dichloropropane	GGG. p-Isopropyltoluene	YYY. tert-Butanol
F. Acetone	X. Bromoform*	PP. Bromochloromethane	HHH. 1,4-Dichlorobenzene	ZZZ. tert-Butyl alcohol
G. Carbon disulfide	Y. 4-Methyl-2-pentanone	QQ. 1,1-Dichloropropene	III. n-Butylbenzene	AAAA. Ethyl tert-butyl ether
H. 1,1-Dichloroethene**	Z. 2-Hexanone	RR. Dibromomethane	JJJ. 1,2-Dichlorobenzene	BBBB. tert-Amyl methyl ether
I. 1,1-Dichloroethane*	AA. Tetrachloroethene	SS. 1,3-Dichloropropane	KKK. 1,2,4-Trichlorobenzene	CCCC.1-Chlorohexane
J. 1,2-Dichloroethene, total	BB. 1,1,2,2-Tetrachloroethane*	TT. 1,2-Dibromoethane	LLL. Hexachlorobutadiene	DDDD. Isopropyl alcohol
K. Chloroform**	CC. Toluene**	UU. 1,1,1,2-Tetrachloroethane	MMM. Naphthalene	EEEE. Acetonitrile
L. 1,2-Dichloroethane	DD. Chlorobenzene*	VV. Isopropylbenzene	NNN. 1,2,3-Trichlorobenzene	FFFF. Acrolein
M. 2-Butanone	EE. Ethylbenzene**	WW. Bromobenzene	OOO. 1,3,5-Trichlorobenzene	GGGG. Acrylonitrile
N. 1,1,1-Trichloroethane	FF. Styrene	XX. 1,2,3-Trichloropropane	PPP. trans-1,2-Dichloroethene	HHHH. 1,4-Dioxane
O. Carbon tetrachloride	GG. Xylenes, total	YY. n-Propylbenzene	QQQ. cis-1,2-Dichloroethene	IIII. Isobutyl alcohol
P. Bromodichloromethane	HH. Vinyl acetate	ZZ. 2-Chlorotoluene	RRR. m,p-Xylenes	JJJJ. Methacrylonitrile
Q. 1,2-Dichloropropane**	II. 2-Chloroethylvinyl ether	AAA. 1,3,5-Trimethylbenzene	SSS. o-Xylene	KKKK. Propionitrile
R. cis-1,3-Dichloropropene	JJ. Dichlorodifluoromethane	BBB. 4-Chlorotoluene	TTT. 1,1,2-Trichloro-1,2,2-trifluoroethane	LLLL.

= System performance check compounds (SPCC) for RRF ; ** = Calibration check compounds (CCC) for %RSD.

LDC #: 9985A48
SDG #: 0302376

VALIDATION FINDINGS WORKSHEET
Initial Calibration

Reviewer: DM
2nd Reviewer: ____

METHOD: GC/MS VOA (EPA TO-14/TO-14A)

Please see qualifications below for all questions answered "N". Not applicable questions are identified as "N/A".

(Y) N N/A Did the laboratory perform a 5 point calibration prior to sample analysis?

Y (N) N/A Were all percent relative standard deviations (%RSD) $\leq$ 30% and relative response factors (RRF) $\geq$ 0.05?

#	Date	Standard ID	Compound	Finding %RSD (Limit: $\leq$30.0%)	Finding RRF (Limit: $\geq$0.05)	Associated Samples	Qualifications
	1-22-03	ICAL	A	35.435		All + BLKS	J/UJ/A
	to		C	30.158			↓
	2-12-03						

LDC #: 9985A48
SDG #: 0302376

VALIDATION FINDINGS WORKSHEET
Laboratory Control Samples (LCS)

Reviewer: DM
2nd Reviewer:

METHOD: GC/MS VOA (EPA TO-14/TO-14A)

Please see qualifications below for all questions answered "N". Not applicable questions are identified as "N/A".

Y N N/A Was a LCS required?
Y N N/A Were the LCS percent recoveries (%R) and relative percent difference (RPD) within the QC limits?

#	Date	LCS/LCSD ID	Compound	LCS %R (Limits)	LCSD %R (Limits)	RPD (Limits)	Associated Samples	Qualifications
		0302376-05A-LCS/D	C	146 (70-130)	147 (70-130)	( )	1 + 0302376A MB	J dets / P
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
		0302376-05B-LCS/D	C	142 (70-130)	142 (70-130)	( )	2 + 0302376B-MB	J dets / P
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		
				( )	( )	( )		

LABORATORY DATA CONSULTANTS, INC.
7750 El Camino Real, Suite 2L Carlsbad, CA 92009 Phone: 760/634-0437 Fax: 760/634-0439

Geofon, Inc.
22632 Golden Springs Drive, Suite 270
Diamond Bar, CA 91765
ATTN: Mr. Leo Williamson

March 28, 2003

SUBJECT: NASA JPL, DO #01, Data Validation

Dear Mr. Williamson,

Enclosed are the final validation reports for the fractions listed below. These SDGs were received on March 19, 2003. Attachment 1 is a summary of the samples that were reviewed for each analysis.

LDC Project # 10006:

SDG #	Fraction
03-1402, 03-1425, 03-1534	Volatiles (524.2), Chromium, Wet Chemistry

The data validation was performed under EPA Level III guidelines. The analyses were validated using the following documents, as applicable to each method:

- USEPA, Contract Laboratory Program National Functional Guidelines for Organic Data Review, October 1999
- USEPA, Contract Laboratory Program National Functional Guidelines for Inorganic Data Review, February 1994
- EPA SW 846, Third Edition, Test Methods for Evaluating Solid Waste, update 1, July 1992; update IIA, August 1993; update II, September 1994; update IIB, January 1995; update III, December 1996

Please feel free to contact us if you have any questions.

Sincerely,

Erlinda T. Rauto
Operations Manager/Senior Chemist

Attachment 1

LDC #10006 (Geofon, Inc.-Diamond Bar / NASA Jet Propulsion Laboratory, DO#001)

LDC	SDG#	DATE REC'D	DATE DUE	VOA (524.2)		Cr (200.8)		Cr(VI) (7196)		CLO_4 (314.0)																									
Matrix:	Water/Soil			W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S	W	S
A	03-1402	3/19/03	4/9/03	10	0	-	-	9	0	9	0																								
B	03-1425	3/19/03	4/9/03	-	-	24	0	-	-	-	-																								
C	03-1534	3/19/03	4/9/03	8	0	-	-	9	0	7	0																								
Total	B			18	0	24	0	18	0	16	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0

Shaded cells indicate Level IV validation (all other cells are Level III validation).

NASA JPL
Data Validation Reports
LDC# 10006

Volatiles

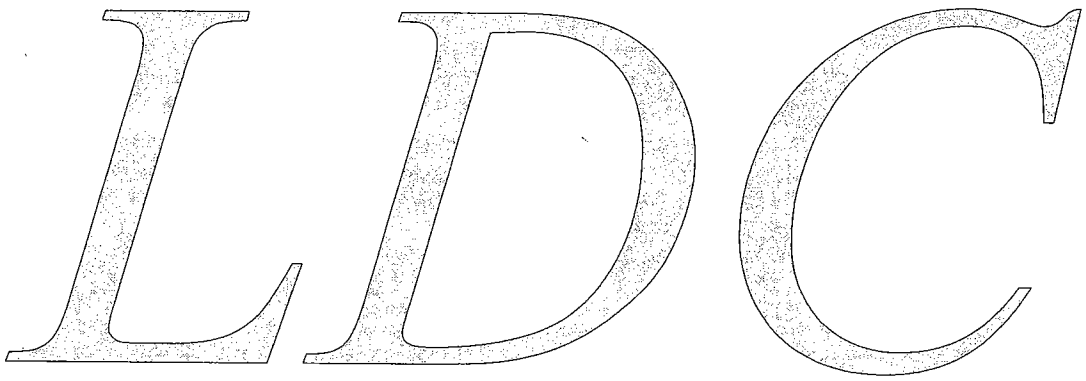

Laboratory Data Consultants, Inc.
Data Validation Report

Project/Site Name: NASA JPL

Collection Date: January 30, 2003

LDC Report Date: March 27, 2003

Matrix: Water

Parameters: Volatiles

Validation Level: EPA Level III

Laboratory: Applied P & Ch Laboratory

Sample Delivery Group (SDG): 03-1402

Sample Identification

DUPE-1-1Q03
EB-2-1/30/03
MW-20-1
MW-20-2
MW-20-3
MW-20-4
MW-20-5
TB-2-1/30/03
MW-20-3MS
MW-20-3MSD

Introduction

This data review covers 10 water samples listed on the cover sheet including dilutions and reanalysis as applicable. The analyses were per EPA Method 524.2 for Volatiles.

This review follows a modified outline of the USEPA Contract Laboratory Program National Functional Guidelines for Organic Data Review (October 1999) as there are no current guidelines for the method stated above.

A table summarizing all data qualification is provided at the end of this report. Flags are classified as P (protocol) or A (advisory) to indicate whether the flag is due to a laboratory deviation from a specified protocol or is of technical advisory nature.

Blank results are summarized in Section V.

Field duplicates are summarized in Section XVI.

Raw data were not reviewed for this SDG. The review was based on QC data.

The following are definitions of the data qualifiers:

U Indicates the compound or analyte was analyzed for but not detected at or above the stated limit.

J Indicates an estimated value.

R Quality control indicates the data is not usable.

N Presumptive evidence of presence of the constituent.

UJ Indicates the compound or analyte was analyzed for but not detected. The sample detection limit is an estimated value.

A Indicates the finding is based upon technical validation criteria.

P Indicates the finding is related to a protocol/contractual deviation.

None Indicates the data was not significantly impacted by the finding, therefore qualification was not required.

I. Technical Holding Times

All technical holding time requirements were met.

The chain-of-custodies were reviewed for documentation of cooler temperatures. All cooler temperatures met validation criteria.

II. GC/MS Instrument Performance Check

Instrument performance was checked at 12 hour intervals.

All ion abundance requirements were met.

III. Initial Calibration

Initial calibration was performed using required standard concentrations.

Percent relative standard deviations (%RSD) were less than or equal to 20.0% for selected compounds.

A curve fit, based on the initial calibration, was established for quantitation for selected compounds. The coefficient of determination (r^2) was greater than or equal to 0.990 .

IV. Continuing Calibration

Continuing calibration was performed at the required frequencies.

All of the continuing calibration percent differences (%D) between the initial calibration RRF and the continuing calibration RRF were less than or equal to 30.0% .

V. Blanks

Method blanks were reviewed for each matrix as applicable. No volatile contaminants were found in the method blanks.

VI. Surrogate Spikes

Surrogates were added to all samples and blanks as required by the method. All surrogate recoveries (%R) were within QC limits.

VII. Matrix Spike/Matrix Spike Duplicates

Although matrix spike (MS) and matrix spike duplicate (MSD) samples were not required by the method, MS and MSD samples were reported by the laboratory. Percent recoveries (%R) and relative percent differences (RPD) were within QC limits.

VIII. Laboratory Control Samples (LCS)

Laboratory control samples were reviewed for each matrix as applicable. Percent recoveries (%R) were within QC limits.

IX. Regional Quality Assurance and Quality Control

Not applicable.

X. Internal Standards

All internal standard areas and retention times were within QC limits.

XI. Target Compound Identifications

Raw data were not reviewed for this SDG.

XII. Compound Quantitation and CRQLs

Raw data were not reviewed for this SDG.

XIII. Tentatively Identified Compounds (TICs)

Raw data were not reviewed for this SDG.

XIV. System Performance

Raw data were not reviewed for this SDG.

XV. Overall Assessment of Data

Data flags have been summarized at the end of the report.

XVI. Field Duplicates

Samples DUPE-1-1Q03 and MW-20-1 were identified as field duplicates. No volatiles were detected in any of the samples.

XVII. Field Blanks

Sample TB-2-1/30/03 was identified as a trip blank. No volatile contaminants were found in this blank.

Sample EB-2-1/30/03 was identified as an equipment blank. No volatile contaminants were found in this blank.

NASA JPL
Volatiles - Data Qualification Summary - SDG 03-1402

No Sample Data Qualified in this SDG

NASA JPL
Volatiles - Laboratory Blank Data Qualification Summary - SDG 03-1402

No Sample Data Qualified in this SDG

100016A

Applied P & Ch Laboratory

Organic Analysis Results for Method 524.2

Client Name:	GEOFON, Inc.	Project No:	04-4428.10	Collection Date:	01/30/2003
Project ID:	JPL	Service ID:	31402	Collected by:	
		Lab Sample ID:	03-1402-1	Received Date:	01/30/2003
Sample ID:	**DUPE-1-1Q03**	Sample Matrix	Water	Moisture %:	–
Sample Type:	Field Sample	Prep. Method:	5030	Instrument ID:	GC/MS: G
Anal. Method:	524.2	Prep. Date:	02/03/03	Anal. Date:	02/03/03
Batch No:	03G1286	Prep. No:	–	Anal. Time:	17:50
Data File Name:	1402-01	Sample Amount:	25 mL	Dilution Factor:	1
Methanol Vol.	–				
Test Level:	Low	Sparge Size:	25 mL	Heated Purge: (Y/N)	N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	0.3	J
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE	98-82-8	µg/L	0.5	<0.5	U

3/26/03

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE (PCE)	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE (TCE)	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	TRICHLOROTRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
58	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates			Control Limit, %	Surro. Rec.%
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL	460-00-4	70-129	107
2	DIBROMOFLUOROMETHANE	1868-53-7	70-129	99
3	1,2-DICHLOROETHANE-D4	17060-07-0	70-122	90
4	TOLUENE-D8	2037-26-5	73-129	102
# of out-of-control				0

Internal Standard			Control Limit, %	IS Rec.%
1	CHLOROBENZENE-D5	3114-55-4	50-200	136
2	1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	136
3	FLUOROBENZENE	462-06-6	50-200	140
# of out-of-control				0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
E - Exceed calibration range
B - A positive value was found in the method blank
D - Diluted

3/28/03

Applied P & Ch Laboratory

Organic Analysis Results for Method 524.2

Client Name:	GEOFON, Inc.	Project No:	04-4428.10	Collection Date:	01/30/2003
Project ID:	JPL	Service ID:	31402	Collected by:	
		Lab Sample ID:	03-1402-2	Received Date:	01/30/2003
Sample ID:	**EB-2-1/30/03**	Sample Matrix	Water	Moisture %:	–
Sample Type:	Field Sample	Prep. Method:	5030	Instrument ID:	GC/MS: G
Anal. Method:	524.2	Prep. Date:	02/03/03	Anal. Date:	02/03/03
Batch No:	03G1286	Prep. No:	–	Anal. Time:	18:19
Data File Name:	1402-02	Sample Amount:	25 mL	Dilution Factor:	1
Methanol Vol.	–				
Test Level:	Low	Sparge Size:	25 mL	Heated Purge: (Y/N)	N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE	98-82-8	µg/L	0.5	<0.5	U

3/28/03

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE (PCE)	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE (TCE)	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	TRICHLOROTRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
58	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates			Control Limit, %	Surro. Rec.%
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL	460-00-4	70-129	112
2	DIBROMOFLUOROMETHANE	1868-53-7	70-129	105
3	1,2-DICHLOROETHANE-D4	17060-07-0	70-122	92
4	TOLUENE-D8	2037-26-5	73-129	110
# of out-of-control				0

Internal Standard			Control Limit, %	IS Rec.%
1	CHLOROBENZENE-D5	3114-55-4	50-200	127
2	1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	131
3	FLUOROBENZENE	462-06-6	50-200	128
# of out-of-control				0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
E - Exceed calibration range
B - A positive value was found in the method blank
D - Diluted

3/28/03

Applied P & Ch Laboratory

Organic Analysis Results for Method 524.2

Client Name:	GEOFON, Inc.	Project No:	04-4428.10	Collection Date:	01/30/2003
Project ID:	JPL	Service ID:	31402	Collected by:	
		Lab Sample ID:	03-1402-3	Received Date:	01/30/2003
Sample ID:	**MW-20-1**	Sample Matrix	Water	Moisture %:	–
Sample Type:	Field Sample	Prep. Method:	5030	Instrument ID:	GC/MS: G
Anal. Method:	524.2	Prep. Date:	02/03/03	Anal. Date:	02/03/03
Batch No:	03G1286	Prep. No:	–	Anal. Time:	18:48
Data File Name:	1402-03	Sample Amount:	25 mL	Dilution Factor:	1
Methanol Vol.	–				
Test Level:	Low	Sparge Size:	25 mL	Heated Purge: (Y/N)	N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE	98-82-8	µg/L	0.5	<0.5	U

3/28/03

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE (PCE)	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE (TCE)	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	TRICHLOROTRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
58	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates			Control Limit, %	Surro. Rec.%
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL	460-00-4	70-129	105
2	DIBROMOFLUOROMETHANE	1868-53-7	70-129	98
3	1,2-DICHLOROETHANE-D4	17060-07-0	70-122	87
4	TOLUENE-D8	2037-26-5	73-129	101
# of out-of-control				0

Internal Standard			Control Limit, %	IS Rec.%
1	CHLOROBENZENE-D5	3114-55-4	50-200	133
2	1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	135
3	FLUOROBENZENE	462-06-6	50-200	132
# of out-of-control				0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
E - Exceed calibration range
B - A positive value was found in the method blank
D - Diluted

3/28/03

Applied P & Ch Laboratory

Organic Analysis Results for Method 524.2

Client Name:	GEOFON, Inc.	Project No:	04-4428.10	Collection Date:	01/30/2003
Project ID:	JPL	Service ID:	31402	Collected by:	
		Lab Sample ID:	03-1402-4	Received Date:	01/30/2003
Sample ID:	**MW-20-2**	Sample Matrix	Water	Moisture %:	–
Sample Type:	Field Sample	Prep. Method:	5030	Instrument ID:	GC/MS: G
Anal. Method:	524.2	Prep. Date:	02/03/03	Anal. Date:	02/03/03
Batch No:	03G1286	Prep. No:	–	Anal. Time:	19:16
Data File Name:	1402-04	Sample Amount:	25 mL	Dilution Factor:	1
Methanol Vol.	–				
Test Level:	Low	Sparge Size:	25 mL	Heated Purge: (Y/N)	N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	1.3	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE	98-82-8	µg/L	0.5	<0.5	U

2/28/03

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE (PCE)	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE (TCE)	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	TRICHLOROTRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
58	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates		Control Limit, %	Surro. Rec.%
1 1-BROMO-4-FLUOROBENZENE (4-BROMOFL	460-00-4	70-129	100
2 DIBROMOFLUOROMETHANE	1868-53-7	70-129	93
3 1,2-DICHLOROETHANE-D4	17060-07-0	70-122	84
4 TOLUENE-D8	2037-26-5	73-129	96
# of out-of-control			0

Internal Standard		Control Limit, %	IS Rec.%
1 CHLOROBENZENE-D5	3114-55-4	50-200	144
2 1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	144
3 FLUOROBENZENE	462-06-6	50-200	142
# of out-of-control			0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
E - Exceed calibration range
B - A positive value was found in the method blank
D - Diluted

3/28/03

Applied P & Ch Laboratory

Organic Analysis Results for Method 524.2

Client Name:	GEOFON, Inc.	Project No:	04-4428.10	Collection Date:	01/30/2003
Project ID:	JPL	Service ID:	31402	Collected by:	
		Lab Sample ID:	03-1402-5	Received Date:	01/30/2003
Sample ID:	**MW-20-3**	Sample Matrix	Water	Moisture %:	–
Sample Type:	Field Sample	Prep. Method:	5030	Instrument ID:	GC/MS: G
Anal. Method:	524.2	Prep. Date:	02/03/03	Anal. Date:	02/03/03
Batch No:	03G1286	Prep. No:	–	Anal. Time:	19:45
Data File Name:	1402-05	Sample Amount:	25 mL	Dilution Factor:	1
Methanol Vol.	–				
Test Level:	Low	Sparge Size:	25 mL	Heated Purge: (Y/N)	N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE	98-82-8	µg/L	0.5	<0.5	U

3/28/03

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE (PCE)	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE (TCE)	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	TRICHLOROTRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
58	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates			Control Limit, %	Surro. Rec.%
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL	460-00-4	70-129	100
2	DIBROMOFLUOROMETHANE	1868-53-7	70-129	100
3	1,2-DICHLOROETHANE-D4	17060-07-0	70-122	90
4	TOLUENE-D8	2037-26-5	73-129	104
# of out-of-control				0

Internal Standard			Control Limit, %	IS Rec.%
1	CHLOROBENZENE-D5	3114-55-4	50-200	137
2	1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	138
3	FLUOROBENZENE	462-06-6	50-200	130
# of out-of-control				0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
E - Exceed calibration range
B - A positive value was found in the method blank
D - Diluted

3/28/03

Applied P & Ch Laboratory

Organic Analysis Results for Method 524.2

Client Name:	GEOFON, Inc.	Project No:	04-4428.10	Collection Date:	01/30/2003
Project ID:	JPL	Service ID:	31402	Collected by:	
		Lab Sample ID:	03-1402-6	Received Date:	01/30/2003
Sample ID:	**MW-20-4**	Sample Matrix	Water	Moisture %:	–
Sample Type:	Field Sample	Prep. Method:	5030	Instrument ID:	GC/MS: G
Anal. Method:	524.2	Prep. Date:	02/03/03	Anal. Date:	02/03/03
Batch No:	03G1286	Prep. No:	–	Anal. Time:	20:15
Data File Name:	1402-06	Sample Amount:	25 mL	Dilution Factor:	1
Methanol Vol.	–				
Test Level:	Low	Sparge Size:	25 mL	Heated Purge: (Y/N)	N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE	98-82-8	µg/L	0.5	<0.5	U

3/28/03

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE (PCE)	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE (TCE)	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	TRICHLOROTRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
58	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates		Control Limit, %	Surro. Rec.%
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL	460-00-4	70-129	110
2	DIBROMOFLUOROMETHANE	1868-53-7	70-129	99
3	1,2-DICHLOROETHANE-D4	17060-07-0	70-122	89
4	TOLUENE-D8	2037-26-5	73-129	102
# of out-of-control				0

Internal Standard		Control Limit, %	IS Rec.%
1	CHLOROBENZENE-D5	3114-55-4	50-200	131
2	1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	131
3	FLUOROBENZENE	462-06-6	50-200	135
# of out-of-control				0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
E - Exceed calibration range
B - A positive value was found in the method blank
D - Diluted

3/28/03

Applied P & Ch Laboratory

Organic Analysis Results for Method 524.2

Client Name:	GEOFON, Inc.	Project No:	04-4428.10	Collection Date:	01/30/2003
Project ID:	JPL	Service ID:	31402	Collected by:	
		Lab Sample ID:	03-1402-7	Received Date:	01/30/2003
Sample ID:	**MW-20-5**	Sample Matrix	Water	Moisture %:	–
Sample Type:	Field Sample	Prep. Method:	5030	Instrument ID:	GC/MS: G
Anal. Method:	524.2	Prep. Date:	02/03/03	Anal. Date:	02/03/03
Batch No:	03G1286	Prep. No:	–	Anal. Time:	20:43
Data File Name:	1402-07	Sample Amount:	25 mL	Dilution Factor:	1
Methanol Vol.	–				
Test Level:	Low	Sparge Size:	25 mL	Heated Purge: (Y/N)	N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	3	J
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE	98-82-8	µg/L	0.5	<0.5	U

3/28/03

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	0.6	
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE (PCE)	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE (TCE)	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	TRICHLOROTRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
58	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates		Control Limit, %	Surro. Rec.%
1 1-BROMO-4-FLUOROBENZENE (4-BROMOFL	460-00-4	70-129	106
2 DIBROMOFLUOROMETHANE	1868-53-7	70-129	104
3 1,2-DICHLOROETHANE-D4	17060-07-0	70-122	92
4 TOLUENE-D8	2037-26-5	73-129	107
# of out-of-control			0

Internal Standard		Control Limit, %	IS Rec.%
1 CHLOROBENZENE-D5	3114-55-4	50-200	125
2 1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	131
3 FLUOROBENZENE	462-06-6	50-200	125
# of out-of-control			0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
E - Exceed calibration range
B - A positive value was found in the method blank
D - Diluted

3/28/03

Applied P & Ch Laboratory

Organic Analysis Results for Method 524.2

Client Name:	GEOFON, Inc.	Project No:	04-4428.10	Collection Date:	01/30/2003
Project ID:	JPL	Service ID:	31402	Collected by:	
		Lab Sample ID:	03-1402-8	Received Date:	01/30/2003
Sample ID:	**TB-2-1/30/03**	Sample Matrix	Water	Moisture %:	–
Sample Type:	Field Sample	Prep. Method:	5030	Instrument ID:	GC/MS: G
Anal. Method:	524.2	Prep. Date:	02/03/03	Anal. Date:	02/03/03
Batch No:	03G1286	Prep. No:	–	Anal. Time:	21:11
Data File Name:	1402-08	Sample Amount:	25 mL	Dilution Factor:	1
Methanol Vol.	–				
Test Level:	Low	Sparge Size:	25 mL	Heated Purge: (Y/N)	N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE	98-82-8	µg/L	0.5	<0.5	U

3/28/03

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE (PCE)	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE (TCE)	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	TRICHLOROTRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
58	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates		Control Limit, %	Surro. Rec.%
1 1-BROMO-4-FLUOROBENZENE (4-BROMOFL	460-00-4	70-129	101
2 DIBROMOFLUOROMETHANE	1868-53-7	70-129	93
3 1,2-DICHLOROETHANE-D4	17060-07-0	70-122	85
4 TOLUENE-D8	2037-26-5	73-129	97
# of out-of-control			0

Internal Standard		Control Limit, %	IS Rec.%
1 CHLOROBENZENE-D5	3114-55-4	50-200	139
2 1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	140
3 FLUOROBENZENE	462-06-6	50-200	140
# of out-of-control			0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
E - Exceed calibration range
B - A positive value was found in the method blank
D - Diluted

3/28/03

LDC #: 10006A1 **VALIDATION COMPLETENESS WORKSHEET** Date: 3-21-03
SDG #: 03-1402 Level III Page: 1 of 1
Laboratory: Applied P & Ch Laboratory Reviewer: DM
2nd Reviewer:

METHOD: GC/MS Volatiles (EPA Method 524.2)

The samples listed below were reviewed for each of the following validation areas. Validation findings are noted in attached validation findings worksheets.

	Validation Area		Comments
I.	Technical holding times	A	Sampling dates: 1-30-03
II.	GC/MS Instrument performance check	A	
III.	Initial calibration	A	%RSD, r2
IV.	Continuing calibration	A	
V.	Blanks	A	
VI.	Surrogate spikes	A	
VII.	Matrix spike/Matrix spike duplicates	A	
VIII.	Laboratory control samples	A	LCS
IX.	Regional Quality Assurance and Quality Control	N	
X.	Internal standards	A	
XI.	Target compound identification	N	
XII.	Compound quantitation/CRQLs	N	
XIII.	Tentatively identified compounds (TICs)	N	
XIV.	System performance	N	
XV.	Overall assessment of data	A	
XVI.	Field duplicates	SW	D=1+3
XVII.	Field blanks	ND	TB=8 EB=2

Note: A = Acceptable
N = Not provided/applicable
SW = See worksheet
ND = No compounds detected
R = Rinsate
FB = Field blank
D = Duplicate
TB = Trip blank
EB = Equipment blank

Validated Samples: All thOs

1	DUPE-1-1Q03	11	03G1286MB01	21		31	
2	EB-2-1/30/03	12		22		32	
3	MW-20-1	13		23		33	
4	MW-20-2	14		24		34	
5	MW-20-3	15		25		35	
6	MW-20-4	16		26		36	
7	MW-20-5	17		27		37	
8	TB-2-1/30/03	18		28		38	
9	MW-20-3MS	19		29		39	
10	MW-20-3MSD	20		30		40	

TARGET COMPOUND WORKSHEET

METHOD: VOA (EPA Method 524.2)

A. Chloromethane	Q. 1,2-Dichloropropane	GG. Xylenes, total	WW. Bromobenzene	MMM. Naphthalene
B. Bromomethane	R. cis-1,3-Dichloropropene	HH. Vinyl acetate	XX. 1,2,3-Trichloropropane	NNN. 1,2,3-Trichlorobenzene
C. Vinyl choride	S. Trichloroethene	II. 2-Chloroethylvinyl ether	YY. n-Propylbenzene	OOO. 1,3,5-Trichlorobenzene
D. Chloroethane	T. Dibromochloromethane	JJ. Dichlorodifluoromethane	ZZ. 2-Chlorotoluene	PPP. trans-1,2-Dichloroethene
E. Methylene chloride	U. 1,1,2-Trichloroethane	KK. Trichlorofluoromethane	AAA. 1,3,5-Trimethylbenzene	QQQ. cis-1,2-Dichloroethene
F. Acetone	V. Benzene	LL. Methyl-tert-butyl ether	BBB. 4-Chlorotoluene	RRR. m,p-Xylenes
G. Carbon disulfide	W. trans-1,3-Dichloropropene	MM. 1,2-Dibromo-3-chloropropane	CCC. tert-Butylbenzene	SSS. o-Xylene
H. 1,1-Dichloroethene	X. Bromoform	NN. Diethyl ether	DDD. 1,2,4-Trimethylbenzene	TTT. 1,1,2-Trichloro-1,2,2-trifluoroethane
I. 1,1-Dichloroethane	Y. 4-Methyl-2-pentanone	OO. 2,2-Dichloropropane	EEE. sec-Butylbenzene	UUU. Benzyl chloride
J. 1,2-Dichloroethene, total	Z. 2-Hexanone	PP. Bromochloromethane	FFF. 1,3-Dichlorobenzene	VVV. 4-Ethyltoluene
K. Chloroform	AA. Tetrachloroethene	QQ. 1,1-Dichloropropene	GGG. p-Isopropyltoluene	WWW. Ethanol
L. 1,2-Dichloroethane	BB. 1,1,2,2-Tetrachloroethane	RR. Dibromomethane	HHH. 1,4-Dichlorobenzene	XXX. Ethyl ether
M. 2-Butanone	CC. Toluene	SS. 1,3-Dichloropropane	III. n-Butylbenzene	
N. 1,1,1-Trichloroethane	DD. Chlorobenzene	TT. 1,2-Dibromoethane	JJJ. 1,2-Dichlorobenzene	
O. Carbon tetrachloride	EE. Ethylbenzene	UU. 1,1,1,2-Tetrachloroethane	KKK. 1,2,4-Trichlorobenzene	
P. Bromodichloromethane	FF. Styrene	VV. Isopropylbenzene	LLL. Hexachlorobutadiene	

Notes:_____

LDC #: 10006A1
SDG #: 03-1402

VALIDATION FINDINGS WORKSHEET
Field Duplicates

Page: 1 of 1
Reviewer: DM
2nd reviewer:

METHOD: GC/MS VOA (EPA Method 524.2)

(Y) N N/A Were field duplicate pairs identified in this SDG?
(Y) N N/A Were target compounds detected in the field duplicate pairs?

Compound	Concentration (ug/L)		RPD
	1	3	
K	0.3	0.5U	—

Compound	Concentration ( )		RPD

Compound	Concentration ( )		RPD