



A P C L

Applied Physics & Chemistry Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel. (909) 590-1828 Fax (909) 590-1498

December 8, 2003

GEOFON, Inc.

Attention: Brad Shojaee

22632 Golden Spring Dr Ste 270

Diamond Bar CA 91765

Dear Brad,

This package contains samples in our Service ID 03-5951 and your project : 04-4428.10 JPL

Enclosed please find:

- (1) Original analytical report.
- (2) Original Chain of Custody.
- (3) One diskette containing EDD deliverable.
- (4) One original Level C Data Package Deliverable.

If anything is missing or you have any questions, please feel free to contact me.

Respectfully submitted,

Regina Kirakozova

Associate QA/QC Director

Applied P & Ch Laboratory

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Submitted to:
GEOFON, Inc.

Attention: Brad Shojaee
22632 Golden Spring Dr Ste 270

Diamond Bar CA 91765

Tel: (909)396-7662 Fax: (909)396-1455

APCL Analytical Report

Service ID #: 801-035951

Collected by: JR

Collected on: 11/04/03

Received: 11/04/03

Extracted: N/A

Tested: 11/04-10/03

Reported: 11/11/03

Sample Description: Water from MW-17,14.

Project Description: 04-4428.10 JPL

Analysis of Water Samples

| Component Analyzed | Method | Unit | PQL | Analysis Result | | | |
|-----------------------------------|--------|------|------|-----------------|--------------|------------|------------|
| | | | | DUPE-5-4-Q03 | EB-9-11-4-03 | MW-14-1 | MW-14-2 |
| | | | | 03-05951-1 | 03-05951-2 | 03-05951-3 | 03-05951-4 |
| CHROMIUM (VI) | 7196 | mg/L | 0.01 | <0.01 | <0.01 | <0.01 | <0.01 |
| Dilution Factor | | | | 5 | 1 | 1 | 1 |
| PERCHLORATE | 314.0 | µg/L | 4 | 193 | <4 | 6.6 | 4.7 |
| VOLATILE ORGANIC COMPOUNDS | | | | | | | |
| Dilution Factor | | | | 1 | 1 | 1 | 1 |
| BENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| BROMOBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| BROMOCHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| BROMODICHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| BROMOFORM | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| BROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| N-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| SEC-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| TERT-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 2-BUTANONE | 524.2 | µg/L | 10 | <10 | <10 | <10 | <10 |
| CARBON TETRACHLORIDE | 524.2 | µg/L | 0.5 | 13.7 | <0.5 | <0.5 | <0.5 |
| CHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| CHLORODIBROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROFORM | 524.2 | µg/L | 0.5 | 3.1 | <0.5 | <0.5 | 0.5J |
| CHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 2-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 4-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DIBROMO-3-CHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DIBROMOETHANE (EDB) | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| DIBROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,3-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,4-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| DICHLORODIFLUOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | 0.5J | <0.5 |
| 1,2-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| CIS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | | |
|---|--------|------|-----|-----------------|--------------|------------|------------|
| | | | | DUPE-5-4-Q03 | EB-9-11-4-03 | MW-14-1 | MW-14-2 |
| | | | | 03-05951-1 | 03-05951-2 | 03-05951-3 | 03-05951-4 |
| TRANS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,3-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 2,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| CIS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| TRANS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| ETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| HEXACHLOROBUTADIENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| ISOPROPYLBENZENE (CUMENE) | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| P-ISOPROPYLTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| METHYLENE CHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| METHYL-T-BUTYL ETHER (MTBE) | 524.2 | µg/L | 1 | <1 | <1 | <1 | <1 |
| 4-METHYL-2-PENTANONE (MIBK) | 524.2 | µg/L | 10 | <10 | <10 | <10 | <10 |
| NAPHTHALENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| N-PROPYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| STYRENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,1,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| TETRACHLOROETHENE | 524.2 | µg/L | 0.5 | 0.6 | <0.5 | 0.4J | 0.7 |
| TOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,3-TRICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,4-TRICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,1-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| TRICHLOROETHENE | 524.2 | µg/L | 0.5 | 3.8 | <0.5 | <0.5 | 4.6 |
| TRICHLOROFLUOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,3-TRICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,4-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| 1,3,5-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| VINYL CHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| O-XYLENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |
| M/P-XYLENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 | <0.5 |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|-----------------------------------|--------|------|------|-----------------------|-----------------------|-----------------------|
| | | | | MW-14-3 03-05951-5 | MW-14-4 03-05951-6 | MW-14-5 03-05951-7 |
| CHROMIUM (VI) | 7196 | mg/L | 0.01 | < 0.01 | < 0.01 | < 0.01 |
| Dilution Factor | | | | 1 | 1 | 1 |
| PERCHLORATE | 314.0 | µg/L | 4 | 7.2 | 4.4 | < 4 |
| VOLATILE ORGANIC COMPOUNDS | | | | | | |
| Dilution Factor | | | | 1 | 1 | 1 |
| BENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMOBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMOCHLOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMODICHLOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMOFORM | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMOMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| N-BUTYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| SEC-BUTYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TERT-BUTYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 2-BUTANONE | 524.2 | µg/L | 10 | < 10 | < 10 | < 10 |
| CARBON TETRACHLORIDE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CHLORODIBROMOMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CHLOROFORM | 524.2 | µg/L | 0.5 | 0.4J | < 0.5 | < 0.5 |
| CHLOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 2-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 4-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DIBROMO-3-CHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DIBROMOETHANE (EDB) | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| DIBROMOMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,3-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,4-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| DICHLORODIFLUOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1-DICHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DICHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1-DICHLOROETHENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CIS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TRANS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,3-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 2,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CIS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TRANS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|---|--------|------|-----|-----------------|------------|------------|
| | | | | MW-14-3 | MW-14-4 | MW-14-5 |
| | | | | 03-05951-5 | 03-05951-6 | 03-05951-7 |
| ETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| HEXACHLOROBUTADIENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| ISOPROPYLBENZENE (CUMENE) | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| P-ISOPROPYLTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| METHYLENE CHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| METHYL-T-BUTYL ETHER (MTBE) | 524.2 | µg/L | 1 | <1 | <1 | <1 |
| 4-METHYL-2-PENTANONE (MIBK) | 524.2 | µg/L | 10 | <10 | <10 | <10 |
| NAPHTHALENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| N-PROPYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| STYRENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,1,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TETRACHLOROETHENE | 524.2 | µg/L | 0.5 | 0.6 | <0.5 | <0.5 |
| TOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,3-TRICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,4-TRICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,1-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TRICHLOROETHENE | 524.2 | µg/L | 0.5 | 0.8 | <0.5 | <0.5 |
| TRICHLOROFLUOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,3-TRICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,4-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,3,5-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| VINYL CHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| O-XYLENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| M/P-XYLENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|----------------------|--------|------|------|-----------------|------------|-------------|
| | | | | MW-17-1 | MW-17-2 | MW-17-3 |
| | | | | 03-05951-8 | 03-05951-9 | 03-05951-10 |
| CHROMIUM (VI) | 7196 | mg/L | 0.01 | <0.01 | <0.01 | <0.01 |
| Dilution Factor | | | | 1 | 1 | 5 |
| PERCHLORATE | 314.0 | µg/L | 4 | <4 | 15.7 | 199 |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|-----------------------------------|--------|------|-----|-----------------------|-----------------------|------------------------|
| | | | | MW-17-1 03-05951-8 | MW-17-2 03-05951-9 | MW-17-3 03-05951-10 |
| VOLATILE ORGANIC COMPOUNDS | | | | | | |
| Dilution Factor | | | | 1 | 1 | 1 |
| BENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMOBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMOCHLOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMODICHLOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMOFORM | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| BROMOMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| N-BUTYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| SEC-BUTYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TERT-BUTYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 2-BUTANONE | 524.2 | µg/L | 10 | < 10 | < 10 | < 10 |
| CARBON TETRACHLORIDE | 524.2 | µg/L | 0.5 | < 0.5 | 1.0 | 11.0 |
| CHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CHLORODIBROMOMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CHLOROFORM | 524.2 | µg/L | 0.5 | < 0.5 | 1.1 | 2.6 |
| CHLOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 2-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 4-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DIBROMO-3-CHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DIBROMOETHANE (EDB) | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| DIBROMOMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,3-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,4-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| DICHLORODIFLUOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1-DICHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DICHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1-DICHLOROETHENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CIS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TRANS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,3-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 2,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| CIS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TRANS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| ETHYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| HEXACHLOROBUTADIENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| ISOPROPYLBENZENE (CUMENE) | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|---|--------|------|-----|-----------------|------------|-------------|
| | | | | MW-17-1 | MW-17-2 | MW-17-3 |
| | | | | 03-05951-8 | 03-05951-9 | 03-05951-10 |
| P-ISOPROPYLTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| METHYLENE CHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| METHYL-T-BUTYL ETHER (MTBE) | 524.2 | µg/L | 1 | <1 | <1 | <1 |
| 4-METHYL-2-PENTANONE (MIBK) | 524.2 | µg/L | 10 | <10 | <10 | <10 |
| NAPHTHALENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| N-PROPYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| STYRENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,1,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TETRACHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | 0.4J | 0.4J |
| TOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,3-TRICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,4-TRICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,1-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TRICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | 6.2 | 3.1 |
| TRICHLOROFUOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,3-TRICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,4-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,3,5-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| VINYL CHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| O-XYLENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| M/P-XYLENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|----------------------|--------|------|------|-----------------|-------------|--------------|
| | | | | MW-17-4 | MW-17-5 | TB-9-11-4-03 |
| | | | | 03-05951-11 | 03-05951-12 | 03-05951-13 |
| CHROMIUM (VI) | 7196 | mg/L | 0.01 | <0.01 | <0.01 | - |
| Dilution Factor | | | | 1 | 1 | 1 |
| PERCHLORATE | 314.0 | µg/L | 4 | <4 | <4 | - |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|-----------------------------------|--------|------|-----|------------------------|------------------------|-----------------------------|
| | | | | MW-17-4 03-05951-11 | MW-17-5 03-05951-12 | TB-9-11-4-03 03-05951-13 |
| VOLATILE ORGANIC COMPOUNDS | | | | | | |
| Dilution Factor | | | | 1 | 1 | 1 |
| BENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMOBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMOCHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMODICHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMOFORM | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| N-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| SEC-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TERT-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 2-BUTANONE | 524.2 | µg/L | 10 | <10 | <10 | <10 |
| CARBON TETRACHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLORODIBROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROFORM | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 2-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 4-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DIBROMO-3-CHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DIBROMOETHANE (EDB) | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| DIBROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,3-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,4-DICHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| DICHLORODIFLUOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CIS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TRANS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,3-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 2,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CIS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TRANS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| ETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| HEXACHLOROBUTADIENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| ISOPROPYLBENZENE (CUMENE) | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|---|--------|------|-----|-----------------|-------------|--------------|
| | | | | MW-17-4 | MW-17-5 | TB-9-11-4-03 |
| | | | | 03-05951-11 | 03-05951-12 | 03-05951-13 |
| P-ISOPROPYLTOLUENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| METHYLENE CHLORIDE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | 0.4J |
| METHYL-T-BUTYL ETHER (MTBE) | 524.2 | µg/L | 1 | < 1 | < 1 | < 1 |
| 4-METHYL-2-PENTANONE (MIBK) | 524.2 | µg/L | 10 | < 10 | < 10 | < 10 |
| N-PROPYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| NAPHTHALENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| STYRENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1,1,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1,2,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TETRACHLOROETHENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TOLUENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2,3-TRICHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2,4-TRICHLOROBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1,1-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1,2-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| TRICHLOROETHENE | 524.2 | µg/L | 0.5 | 0.8 | < 0.5 | < 0.5 |
| TRICHLOROFLUOROMETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2,3-TRICHLOROPROPANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,1,2,2,3,3,3-HEPTACHLORO-1,1,2,2,3,3,3-TRIFLUOROETHANE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,2,4-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| 1,3,5-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| VINYL CHLORIDE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| O-XYLENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |
| M/P-XYLENE | 524.2 | µg/L | 0.5 | < 0.5 | < 0.5 | < 0.5 |


PQL: Practical Quantitation Limit. MDL: Method Detection Limit. CRDL: Contract Required Detection Limit

N.D.: Not Detected or less than the practical quantitation limit. "-": Analysis is not required.

J: Reported between PQL and MDL.

Listed Dilution Factors (DF) are relative to the method default DF. All unlisted DFs are 1.0

Respectfully submitted,

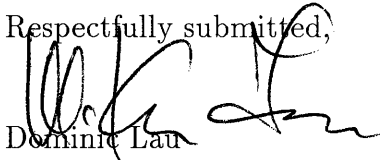
 Dominic Lau
 Laboratory Director
 Applied P & Ch Laboratory

Level C Data Package Deliverables

General Information

Project: 04-4428.10 JPL

APCL Service ID: 03-5951



Applied P & Ch Laboratory
13760 Magnolia Ave. Chino, CA 91710
Telephone (909)590-1828
Fax (909)590-1498

Case Narrative

Project: JPL/MW-17,14./04-4428.10

For GEOFON, Inc.

APCL Service No: 03-5951

1. Sample Identification

The sample identifications are listed in the following table:

| GEOFON, Inc. Sample ID | APCL Sample ID |
|------------------------|----------------|
| MW-17-5 | 03-05951-12 |
| MW-17-4 | 03-05951-11 |
| MW-17-3 | 03-05951-10 |
| MW-17-2 | 03-05951-9 |
| MW-17-1 | 03-05951-8 |
| DUPE-5-4-Q03 | 03-05951-1 |
| MW-14-5 | 03-05951-7 |
| MW-14-4 | 03-05951-6 |
| MW-14-3 | 03-05951-5 |
| MW-14-2 | 03-05951-4 |
| MW-14-1 | 03-05951-3 |
| EB-9-11-4-03 | 03-05951-2 |
| TB-9-11-4-03 | 03-05951-13 |

2. Analytical Methodology

Samples are analyzed by EPA methods

524.2 (Volatile Organic Compounds),

7196 (Chromium (VI)),

314.0 (Perchlorate, low level),

3. Holding Time

All samples were extracted, digested and analyzed within the holding times defined by the appropriate EPA methods of the analyses.

4. Preservation

All samples were preserved and stored according to the appropriate EPA methods.

5. Tele-log

None

6. Anomaly

None

"I certify that these data are technically accurate, complete, and in compliance with the terms and conditions of the contract, for other than the conditions detailed above. Release of the data contained in the hardcopy data package and its electronic data deliverable submitted on diskette had been authorized by the Laboratory Manager or her/his designee, as verified by the following signature."

Respectfully submitted,

A handwritten signature in black ink, appearing to read 'R. Kirakozova', written in a cursive style.

Regina Kirakozova
Associate QA/QC Director
Applied P & Ch Laboratory



INCORPORATED
 22632 GOLDEN SPRINGS DR., SUITE 270
 DIAMOND BAR, CA 91785 • (909) 396-7662 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

0063

MUS-17

| | | | | | | | | | | | |
|---|--|---|--|---------------------------------------|--|---|--|---|--|--|--|
| GEOFON'S LAB COORDINATOR Scott Buhner | | LAB COORDINATOR'S PHONE 909 396 7662 | | LAB COORDINATOR'S FAX 909 396 1455 | | LABORATORY SERVICE ID | | LABORATORY CONTACT Kenny Chan | | MAIL REPORT (COMPANY NAME) Geofon | |
| PROJECT NAME SPL Goldstone-1803 | | PROJECT LOCATION MUS-17 | | PROJECT NUMBER 07-4428.10 | | LABORATORY PHONE 909 596 1828 | | LABORATORY FAX 909 596 1498 | | RECIPIENT NAME Tommy Ford | |
| PROJECT CONTACT Brend Shapiro | | PROJECT PHONE NUMBER 909 396 7662 | | PROJECT FAX 909 396 1455 | | LABORATORY ADDRESS 13710 Magnolia Ave. | | LABORATORY CITY, STATE AND ZIP CODE Clino, CA 91710 | | ADDRESS 22632 | |
| PROJECT ADDRESS 4800 Oak Grove Dr. | | CITY, STATE AND ZIP CODE Pasadena, CA | | CLIENT US NAVY SUBVIV | | LABORATORY CITY, STATE AND ZIP CODE Clino, CA 91710 | | LABORATORY CITY, STATE AND ZIP CODE Clino, CA 91710 | | CITY, STATE AND ZIP CODE Diamond Bar, CA 91765 | |
| PROJECT MANAGER Tommy Ford | | PROJECT MANAGER'S PHONE 909 396 7662 | | PROJECT MANAGER'S FAX 909 396 1455 | | LABORATORY CITY, STATE AND ZIP CODE Clino, CA 91710 | | LABORATORY CITY, STATE AND ZIP CODE Clino, CA 91710 | | CITY, STATE AND ZIP CODE Diamond Bar, CA 91765 | |

| Item | Sample Identifier | Matrix | Date | Time | HCl HNO3 H2O2 | Preserved | # of Cont. | QC Level | T.A.T | Analyses | | |
|------|------------------------------------|--------|----------|------|---------------------|-----------|------------|----------|-------|--------------|--------------|------------------|
| | | | | | | | | | | 529.2 (Vols) | 314.0 (ClO4) | 208.8 (Total Cr) |
| 1 | MUS-17-5 | W | 10/16/03 | 0958 | None | S | III | Normal | X | X | X | |
| 2 | MUS-17-4 | | 10/22 | | | | | | X | X | X | |
| 3 | MUS-17-3 | | 10/16 | | | | | | X | X | X | |
| 4 | MUS-17-2 | | 11/28 | | | | | | X | X | X | |
| 5 | MUS-17-1 | | 11/18 | | | | | | X | X | X | |
| 6 | MUS-17-1 SPL-5-4-003 | W | 11/07 | | | | IV | | X | X | X | |
| 7 | | | | | | | | | | | | |
| 8 | | | | | | | | | | | | |
| 9 | | | | | | | | | | | | |
| 10 | | | | | | | | | | | | |

| | | | | | | |
|---------------------------------------|-----------------------------|-----------------------------------|-------------------------|---------------------|---------------------------------|---------------------------------|
| SAMPLES COLLECTED BY SN | COURIER AND AIR BILL NUMBER | RECEIVED BY [Signature] | DATE 11/05/03 | TIME 1245 | COOLER TEMPERATURE UPON RECEIPT | SAMPLE'S CONDITION UPON RECEIPT |
| RELINQUISHED BY [Signature] | | RECEIVED BY [Signature] | DATE 11/05/03 | TIME 1345 | | |

5951
Comments

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager



GEOFON
INCORPORATED
22692 GOLDEN SPRINGS DR., SUITE 270
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

0062

GEOFON'S LAB COORDINATOR: Scott Buhman LAB COORDINATOR'S PHONE: 909 396 7662 LAB COORDINATOR'S FAX: 909 396 1455

PROJECT NAME: SPC Gas Mon-1003 PROJECT LOCATION: HWS-14 PROJECT NUMBER: 07-4428.10 LABORATORY SERVICE ID: 909 590 1828 LABORATORY CONTACT: Kimmey Chan MAIL REPORT (COMPANY NAME): GEOFON

PROJECT CONTACT: Brad Shapiro PROJECT PHONE NUMBER: 909-396 7662 PROJECT FAX: 909 396 1455 LABORATORY PHONE: 909 590 1828 LABORATORY FAX: 909 590 1498 RECIPIENT NAME: Tony Ford

PROJECT ADDRESS: 4800 Oak Grove Dr. City, State and Zipcode: Pasadena, CA 91710 CLIENT: US NAVY SUBSTV LABORATORY ADDRESS: 13760 Magnolia Ave. City, State and Zipcode: Chino, CA 91710 ADDRESS: 22432 Diamond Bar, CA 91765

PROJECT MANAGER: Tony Ford PROJECT MANAGER'S PHONE: 909 396 7662 PROJECT MANAGER'S FAX: 909 396 1455

| Item | Sample Identifier | Matrix | Date | Time | Preserved | # of Cont. | QC Level | T.A.T | Analyses | | | Comments |
|------|-------------------|--------|----------|------|-----------|------------|----------|-------|-----------|---------------|-----------|----------|
| | | | | | | | | | 200.8 (L) | 2196 (C) (IE) | 221.2 (V) | |
| 1 | HWS-14-5 | UD | 11/16/03 | 0719 | 8 | III | Normal | X | X | X | | |
| 2 | HWS-14-4 | | | 0739 | 5 | III | | X | X | X | | |
| 3 | HWS-14-3 | | | 0800 | | | | X | X | X | | |
| 4 | HWS-14-2 | | | 0819 | | | | X | X | X | | |
| 5 | HWS-14-1 | | | 0845 | | | | X | X | X | | |
| 6 | TR-9-11-4-03 | | | - | 2 | | | X | X | X | | |
| 7 | =B-9-11-4-03 | | | 0834 | 5 | | | X | X | X | | |
| 8 | | | | | | | | | | | | |
| 9 | | | | | | | | | | | | |
| 10 | | | | | | | | | | | | |

SAMPLES COLLECTED BY: SN COURIER AND AIR BILL NUMBER: RECEIVED BY: DATE: TIME: COOLER TEMPERATURE UPON RECEIPT: SAMPLE'S CONDITION UPON RECEIPT:

REINQUISHED BY: 11-04-03 1245 11-4-03 1445

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager

Sample Receiving Checklist

APCL ServiceID: **5951** Client Name/Project: Geofon

1. Sample Arrival

Date/Time Received 11/4/03 1345 Date/Time Opened 11/4/03 1345 By (name): Jason

Custody Transfer: Client Golden State UPS US Mail FedEx APCL Empl: Richard

2. Chain-of-Custody (CoC)

With Samples? Faxed? Client has Copy? Signed, dated? By: _____
 Project ID? Analyses Clear? Hold Samples? #on Hold _____ # Received _____
 CoC/Docs Zip-Locked under lid? Compos. #: _____ #Samples OK? _____
 Discrepancies? Client notified? Response (attach docs): _____

3. Shipping Container/Cooler

Cooler Used? # of 1 Cooled by: Ice Blue Ice Dry Ice None
Temp °C 3.4

(Cooler temperature measured from temp blank if present, otherwise measured from the cooler).

Cooler Custody Seal? Absent Intact Tampered?

4. Sample Preservation

pH <2 pH >12
If Not, pH = _____ Preserved by: Client APCL Third Party _____

5. Holding-time Requirements

pH 24hr BACT 6/24hr Cr^{VI} 24hr NO₃⁻ 48hr BOD 48hr
 Cl₂ ASAP Turbidity 48hr DO ASAP Fe(II) ASAP
 HT Expired? Client notified?

6. Sample Container Condition

Intact? Broken? Documented? Number: _____
Type: plastic glass Tube: brass/SS Tedlar Bag
 Quantity OK? Leaking? Anomaly?
 Caps tight? Air Bubbles? Anomaly?
Labels: Unique ID? Date/Time Preserved?

7. Turn Around Time

RUSH TAT: 5 days Std (7-10 days) Not Marked

8. Sample Matrix

Drinking H₂O Other Liq Soil Wipe Polymer Air Other: _____
 Ground H₂O Sludge Filter Oil/Petro Paint W. Water Extract Unknown

9. Pre-Login Check List Completed & OK?

ALL OK? (if not, attach docs) Client Contact? (Name: _____) Date/Time: _____

Received/Checked by: [Signature] Printed: 4 Nov 2003 9:21 a.m.

*HT: Samples must be analyzed for results to reflect total concentrations. Results generated outside required of holding times are considered minimal values and may be used to define waste as hazardous but not as non-hazardous.

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Sample Login: Check List

03-05951 (0470_ 186) (2202777_ 186)

11/04/03

Part 1: General Information

| | | | |
|--------------------------|--------------------------|----------------------|--|
| <input type="checkbox"/> | Company Information | Name: | <i>GEOFON, Inc.</i> |
| | | Address: | <i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i> |
| <input type="checkbox"/> | Project Information | Project Description: | <i>JPL</i> |
| | | Project #: | <i>04-4428.10</i> |
| <input type="checkbox"/> | Billing Information | P.O. #: | |
| | | Bill Address: | <i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i> |
| | | Lab Project ID: | |
| | | Client Database #: | <i>3</i> |
| <input type="checkbox"/> | Receiving Information | Who Received Sample? | <i>Jason N.</i> |
| | | Receiving Date/Time: | <i>11/04/03 1345</i> |
| | | COC No. | <i>0063 0062</i> |
| <input type="checkbox"/> | Shipping Information | Shipping Company | <i>APCL pick up</i> |
| | | Packing Information: | <i>Cooler/Ice Chester</i> |
| | | Cooler Temperature: | <i>3.6 °C</i> |
| <input type="checkbox"/> | Container Information | Container Provider: | <i>Client</i> |
| <input type="checkbox"/> | Sampling Information | Sampling Person: | <i>JR</i> |
| | | Sampling Company: | <i>Client</i> |
| <input type="checkbox"/> | Turn-Around-Time Option: | | <i>Rush 5 working day(s)</i> |
| <input type="checkbox"/> | QC Option: | | <i>NEESA C</i> |
| <input type="checkbox"/> | Disposal Option: | | <i>Not specify</i> |

Part 2: Sample Information

| Seq. # | Sample ID (on COC) | Sample Sub-ID | APCL Sample ID | Matrix | Cont- tainer | Preser- vative | Vol, ml Am. g | # of Replica | Condition G, L, B | Collected mmmddyy | Hold ? | Composite Group | TAT Days | |
|--------|--------------------|---------------|-----------------------|--------|--------------|----------------|---------------|--------------|-------------------|-------------------|--------|-----------------|----------|--------------------------|
| 1 | MW-17-5 | 524.2 | 03-05951-12- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-17-5 | CrVI | 03-05951-12- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 2 | MW-17-4 | 524.2 | 03-05951-11- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-17-4 | CrVI | 03-05951-11- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 3 | MW-17-3 | 524.2 | 03-05951-10- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-17-3 | CrVI | 03-05951-10- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 4 | MW-17-2 | 524.2 | 03-05951-9- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-17-2 | CrVI | 03-05951-9- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 5 | MW-17-1 | 524.2 | 03-05951-8- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-17-1 | CrVI | 03-05951-8- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 6 | DUPE-5-4-Q03 | 524.2 | 03-05951-1- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | DUPE-5-4-Q03 | CrVI | 03-05951-1- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 7 | MW-14-5 | 524.2 | 03-05951-7- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-14-5 | CrVI | 03-05951-7- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 8 | MW-14-4 | 524.2 | 03-05951-6- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-14-4 | CrVI | 03-05951-6- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 9 | MW-14-3 | 524.2 | 03-05951-5- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-14-3 | CrVI | 03-05951-5- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 10 | MW-14-2 | 524.2 | 03-05951-4- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-14-2 | CrVI | 03-05951-4- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 11 | MW-14-1 | 524.2 | 03-05951-3- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | MW-14-1 | CrVI | 03-05951-3- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 12 | EB-9-11-4-03 | 524.2 | 03-05951-2- α | W | V | C | 40 | 3 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| | EB-9-11-4-03 | CrVI | 03-05951-2- β | W | P | | 500 | 1 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |
| 13 | TB-9-11-4-03 | 524.2 | 03-05951-13 | W | V | C | 40 | 2 | G | 110403 | N | 0 | 7 | <input type="checkbox"/> |

Part 3: Analysis Information

Test Items:

- 524.2 Volatile Organic Compounds
- 7196A Chromium (VI)
- 314.0/300.0 Perchlorate, low level
- 300.0 Chloride Cl^- by IC
- 300.0 Sulfate (SO_4^{--}), by IC
- 300.0/ $\text{SM}_4500\text{NO}_3^-$ Nitrate (NO_3^-) as N by IC
- SM_2320B Carbonate
- SM_2320B Bicarbonate
- 9040B/150.1 pH
- 160.1 Solids, Total Dissolved (TDS)

Level C Data Package Deliverables

Volatile Organics



Applied P & Ch Laboratory

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------------|------------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/06/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: |
| Sample ID: 03G4717-MB-01 | Lab Sample ID: 03G4717-MB-01 | Received Date: 11/06/2003 |
| Sample Type: Method Blank | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: G4717K01 | Prep. No: - | Anal. Time: 13:54 |
| Methanol Vol: - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | < 0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | < 0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | < 0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | < 0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | < 0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | < 0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | < 0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | < 0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | < 0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | < 10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | < 0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | < 0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | < 0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | < 0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | < 0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | < 0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | < 0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | < 0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | < 0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | < 0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | < 0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | < 0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | < 0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | < 0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | < 0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | < 0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | < 0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | < 0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | < 0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | < 0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | < 0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | < 0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | < 0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | < 0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | < 0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | < 0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | < 0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | < 0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | < 0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROBENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROBENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 112TRICHLORO-122TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | | Control Limit, % | Surro. Rec.% |
|---------------------|-----------------------------|------------|------------------|--------------|
| 1 | 4-BROMO-FLUOROBENZENE (BFB) | 460-00-4 | 70-129 | 108 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 108 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 107 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 108 |
| # of out-of-control | | | | 0 |

Internal Standard

| | | | Control Limit, % | IS Rec.% |
|---------------------|-----------------------|-----------|------------------|----------|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 99 |
| 2 | 1,4-DICHLOROETHANE-D4 | 3855-82-1 | 50-200 | 97 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 102 |
| # of out-of-control | | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQ, or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717K01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 13:54 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:12 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:12 2003
 Miscleaneous :


| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | c,ppb | Quality | Note |
|--------------------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.64 | 7.64 | 0.000 | 96 | 70 | 664.922 | 10.00 | | 0.00 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 492.340 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.85 | 13.85 | 0.000 | 152 | 150 | 294.801 | 10.00 | | 0.00 | |


| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|-------------------|-------|-------|-------|-----|-----|----------|-------|--|------|---------|
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.60 | 0.000 | 111 | 113 | 333.019 | 21.33 | | 21.3 | 106.65% |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.10 | 7.11 | 0.000 | 65 | 102 | 299.810 | 21.56 | | 21.6 | 107.79% |
| 55 | toluene-d8 | 9.91 | 9.91 | 0.000 | 98 | 100 | 1175.143 | 21.62 | | 21.6 | 108.12% |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 428.526 | 21.45 | | 21.5 | 107.26% |

| Target Compounds | | | | | | | | | | | |
|------------------|-------------------|-------|-------|-------|-----|-----|-------|------|--|-----|--------|
| <<< | I1 : ISTD ID = 1 | >>> | | | | | | | | | Qvalue |
| 33 | 2-butanoneMEK X10 | 5.95 | 5.95 | 0.000 | 43 | 72 | 2.021 | 0.58 | | 0.6 | 83% |
| 101 | TAME | 7.65 | 7.41 | 0.031 | 73 | 43 | 9.851 | 1.15 | | 1.1 | 46% |
| <<< | I2 : ISTD ID = 47 | >>> | | | | | | | | | |
| 54 | MIBK | 9.91 | 9.77 | 0.012 | 43 | 58 | 4.718 | 2.01 | | 2.0 | 1% |
| 57 | 2-hexanone X5 | 10.78 | 10.76 | 0.002 | 43 | 58 | 0.293 | 5.06 | | 5.1 | 93% |
| <<< | I3 : ISTD ID = 62 | >>> | | | | | | | | | |
| 88 | naphthalene | 15.80 | 15.78 | 0.000 | 128 | 129 | 2.394 | 1.18 | | 1.2 | 71% |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06





Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717K01.D
Method : C:\MSDCHEM\1\METHODS\E524A003.M
Acq. Time : Nov 6 13:54 2003
Method Update: Mon Oct 27 14:05 2003
Quant. Time : Nov 07 11:12 2003
Print Time : Fri Nov 07 11:12 2003
Miscellaneous :
Sample : F=1
Inst. : GCMS-A
RF via : Multiple Level Calibration
Operator: zou
Multiplr: 1.000000

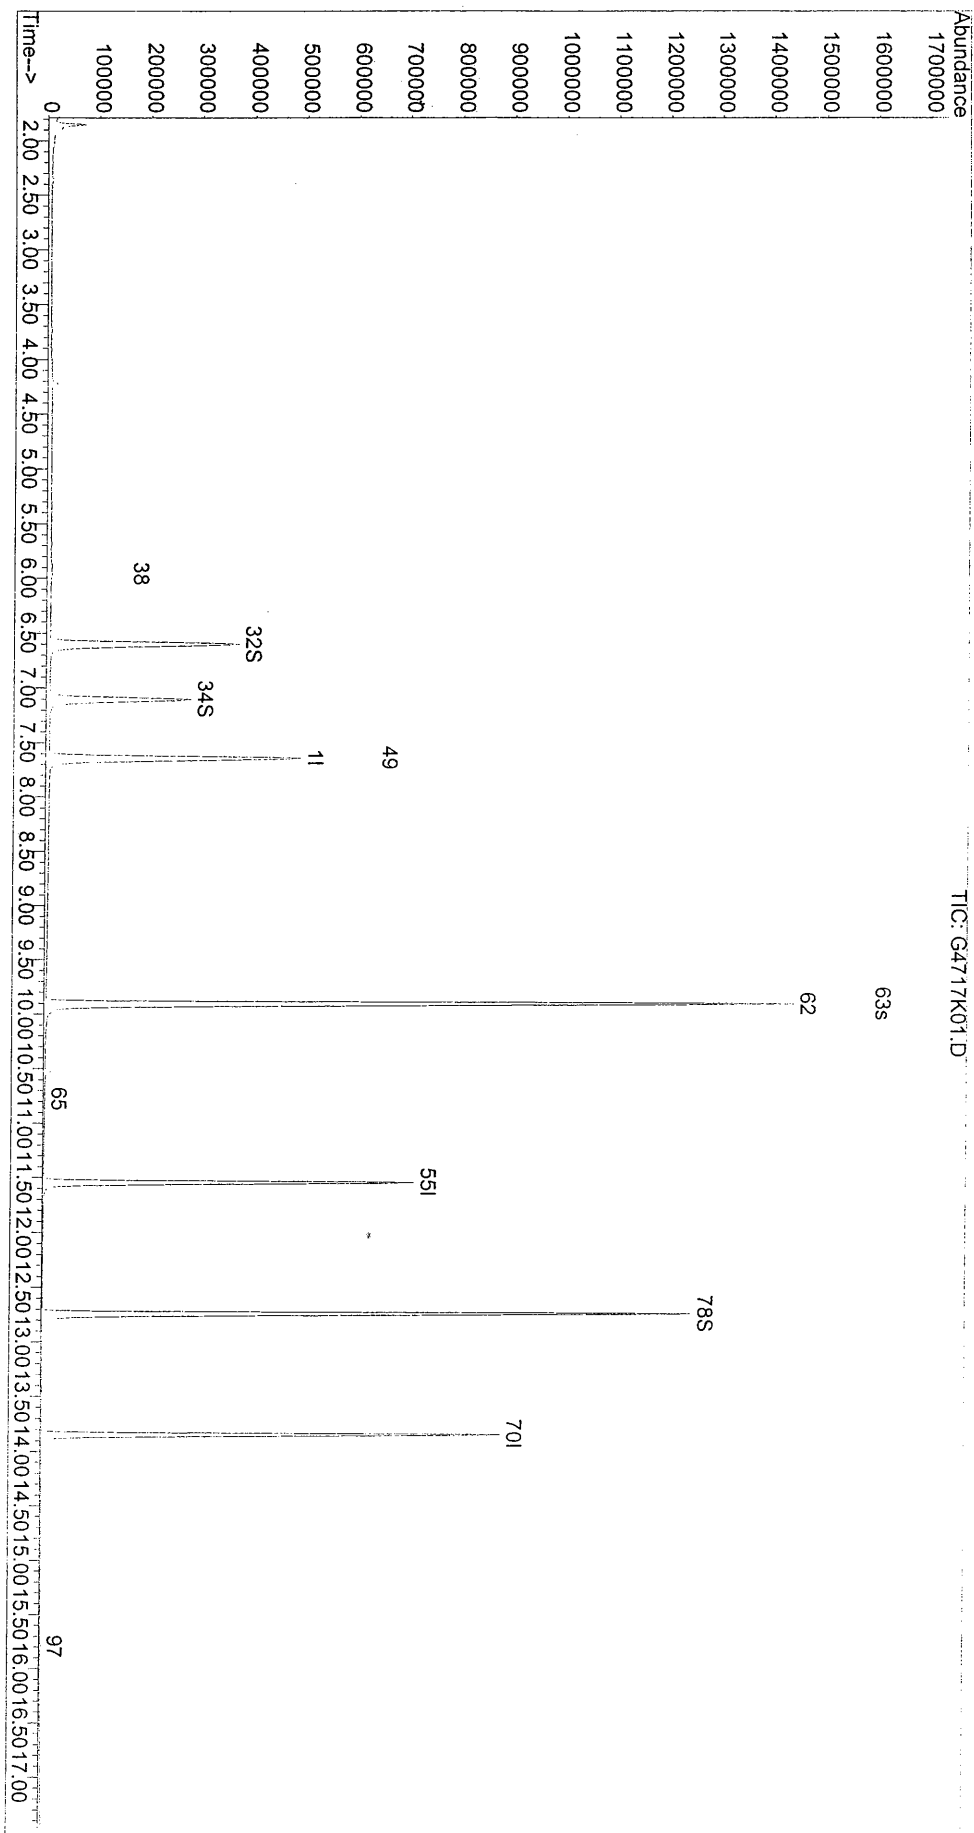

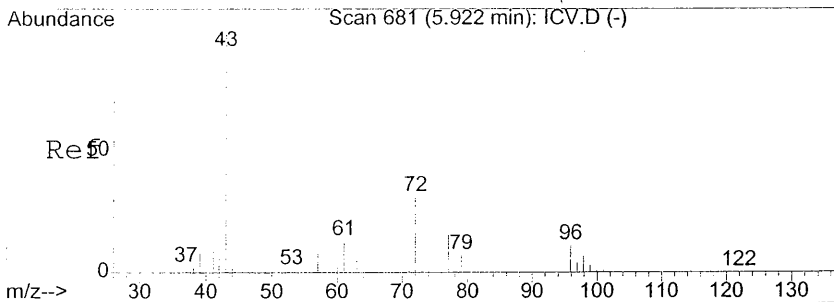




#38
 33 2-butanoneMEK X10
 Concen: 0.58 ppb
 RT: 5.95 min Scan# 686
 Delta R.T. 0.01 min
 Lab File: G4717K01.D
 Acq: 6 Nov 2003 1:54 pm


| Tgt Ion | Resp | Lower | Upper |
|---------|------|-------|-------|
| 43 | 2021 | 100 | |
| 72 | 23.3 | 13.1 | 53.1 |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

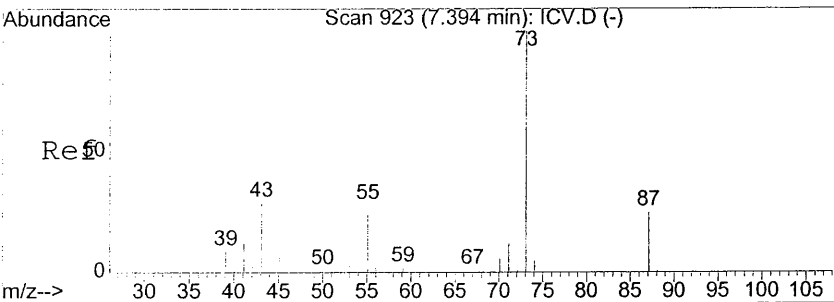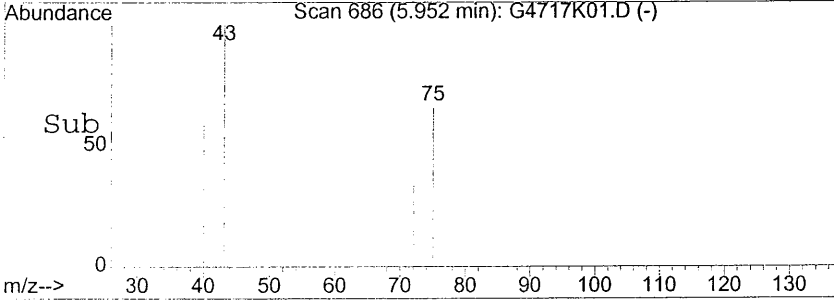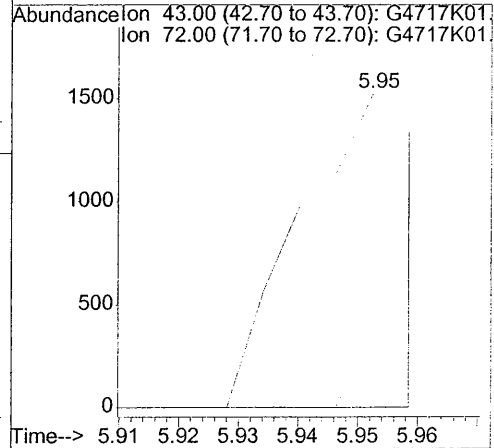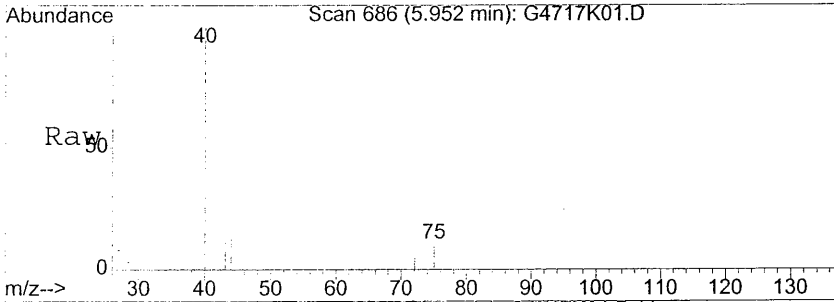


#49
 101 TAME
 Concen: 1.15 ppb
 RT: 7.65 min Scan# 965
 Delta R.T. 0.24 min
 Lab File: G4717K01.D
 Acq: 6 Nov 2003 1:54 pm

| Tgt Ion | Resp | Lower | Upper |
|---------|------|-------|-------|
| 73 | 9851 | 100 | |
| 43 | 0.0 | 22.7 | 34.1# |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

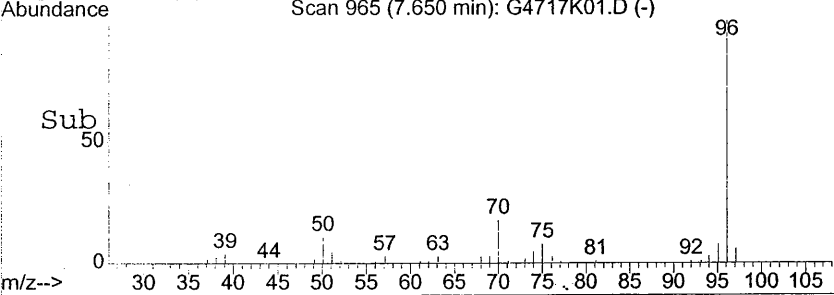
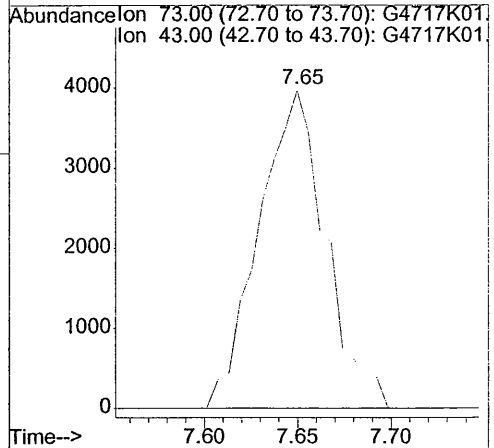
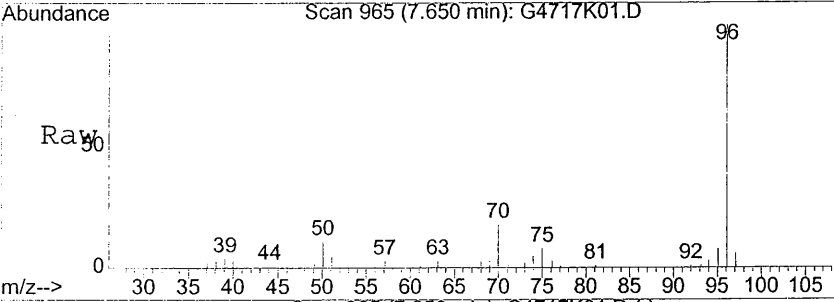


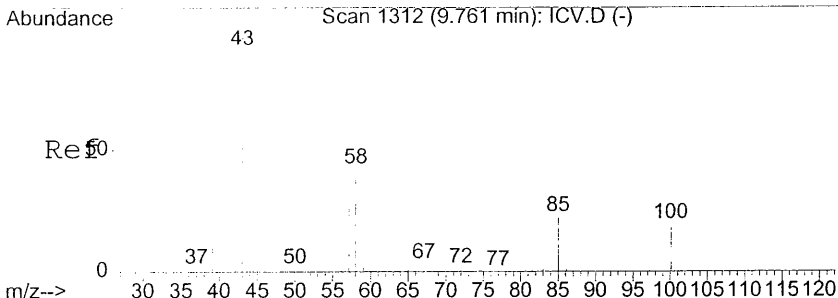


#62
 54 MIBK
 Concen: 2.01 ppb
 RT: 9.91 min Scan# 1336
 Delta R.T. 0.14 min
 Lab File: G4717K01.D
 Acq: 6 Nov 2003 1:54 pm

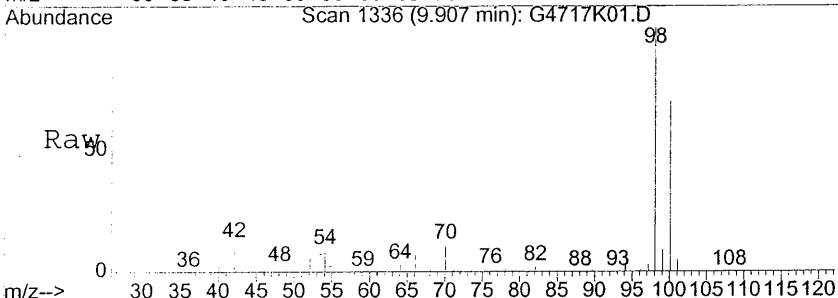



| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 43 | 100 | | |
| 58 | 202.5 | 20.1 | 60.1# |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

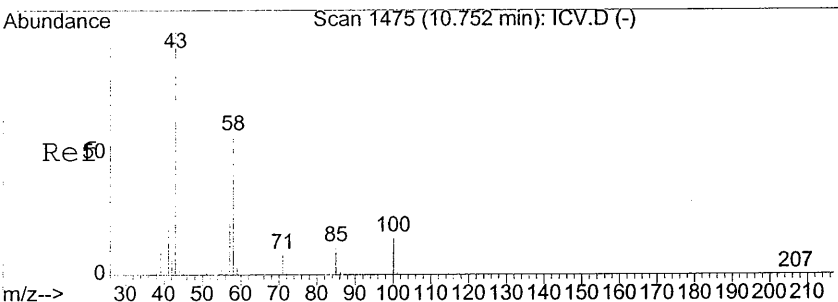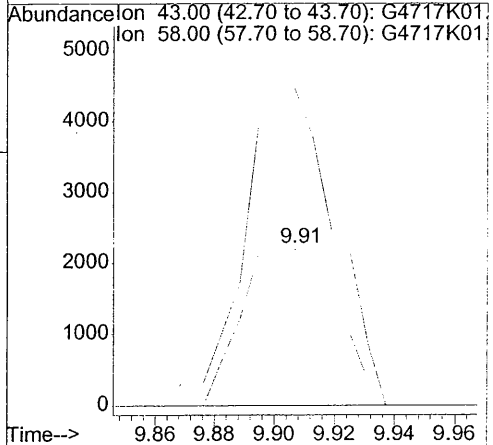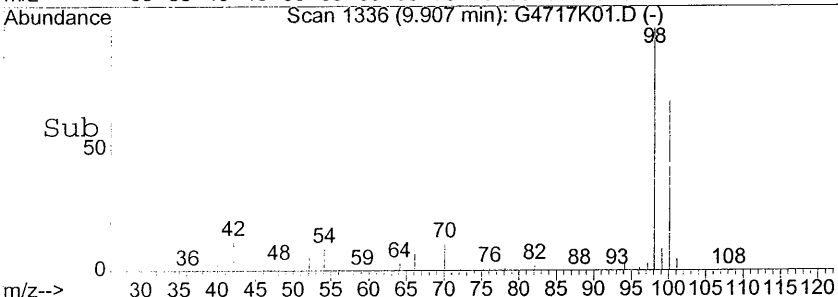


#65
 57 2-hexanone X5
 Concen: 5.06 ppb
 RT: 10.78 min Scan# 1480
 Delta R.T. 0.02 min
 Lab File: G4717K01.D
 Acq: 6 Nov 2003 1:54 pm

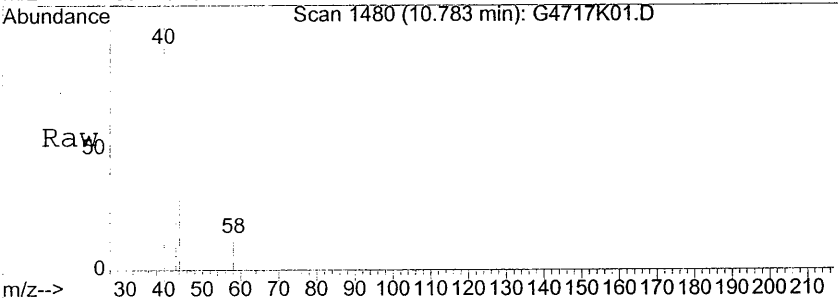


| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 43 | 100 | | |
| 58 | 63.6 | 38.4 | 78.4 |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

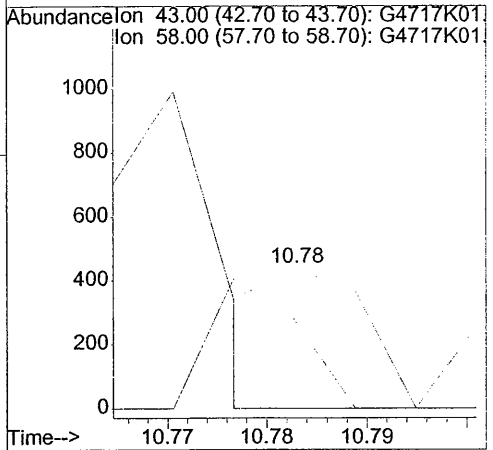
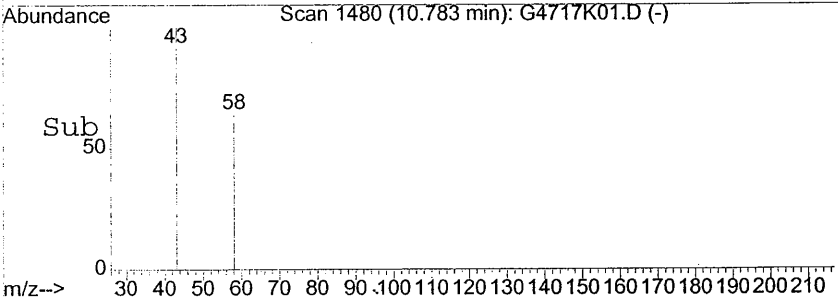


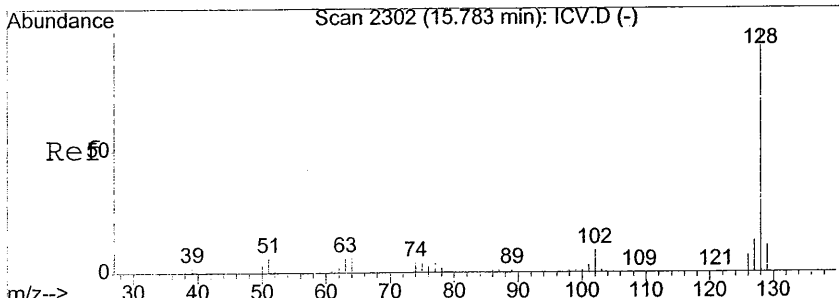

#97
 88 naphthalene
 Concen: 1.18 ppb
 RT: 15.80 min Scan# 2304
 Delta R.T. 0.01 min
 Lab File: G4717K01.D
 Acq: 6 Nov 2003 1:54 pm

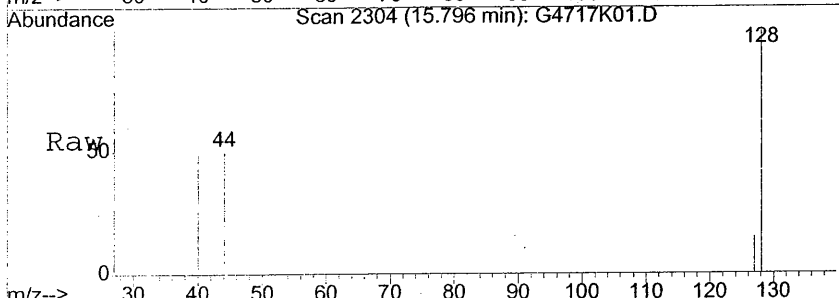

| Tgt Ion | 128 | 129 | 0 | 0 | Resp: | 2394 | Lower | Upper |
|-----------|-----|-----|-----|-----|-------|------|-------|-------|
| Ion Ratio | 100 | 0.0 | 0.0 | 0.0 | | | | |
| | | 0.0 | 0.0 | 0.0 | | 31.1 | | |
| | | 0.0 | 0.0 | 0.0 | | 0.0 | | |

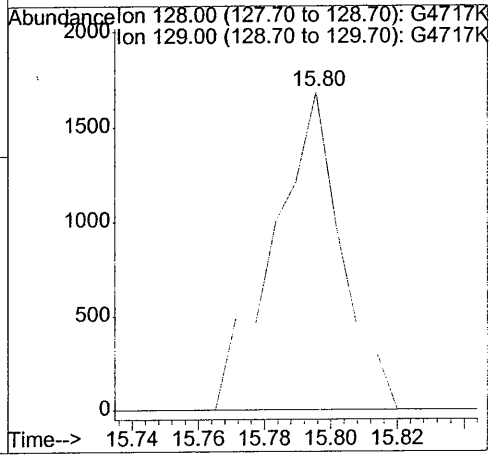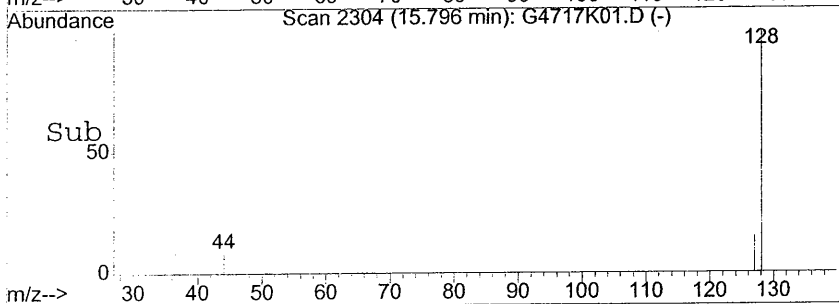

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|--------------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: DUPE-5-4-Q03 | Lab Sample ID: 03-5951-1 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-01 | Prep. No: - | Anal. Time: 16:30 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | 13.7 | |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | 3.1 | |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | 0.6 | |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | 3.8 | |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 112TRICHLORO-122TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | | Control Limit, % | Surro. Rec.% |
|---|-------------------------------------|------------|------------------|--------------|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 108 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 108 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 107 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 108 |
| # | of out-of-control | | | 0 |

Internal Standard

| | | | Control Limit, % | IS Rec.% |
|---|-----------------------|-----------|------------------|----------|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 96 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 92 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 99 |
| # | of out-of-control | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Data Filename: C:\MSDCHEM\1\DATA\03G4717\5951-01.D
 Method : C:\MSDCHEM\1\METHODS\E524A003.M
 Acq. Time : Nov 6 16:30 2003
 Method Update: Mon Oct 27 14:05 2003
 Quant. Time : Nov 07 10:24 2003
 Print Time : Fri Nov 07 10:24 2003
 Miscellaneous :

Sample : F=1 dup
 Inst. : GCMS-A
 RF via : Multiple Level Calibration
 Operator: zou
 Multiplr: 1.000000

1615

ID Component Name R.T. RT0 DRRT Qion Q1 RF/1000 C0,ppb C,ppb Quality Note

Internal Standards
 1 .1 Fluorobenzene 7.65 7.64 0.000 96 70 644.992 10.00
 47 47 Chlorobenzene-d5 11.54 11.54 0.000 117 82 476.399 10.00
 62 62 1,4-Dichlorobenze 13.85 13.85 0.000 152 150 281.619 10.00

System Monitoring Compounds (Surrogate)
 27 27 Di-Br-F-Me (surr) 6.60 6.60 0.000 111 113 322.579 21.30 21.3 106.50%
 29 29 1,2-Di-Cl-Et-d4 (7.10 7.11 0.000 65 102 291.233 21.59 21.6 107.95%
 55 55 toluene-d8 9.91 9.91 0.000 98 100 1130.676 21.50 21.5 107.51%
 70 70 4-Br-1-F-Bz (S3) 12.74 12.74 0.000 174 95 410.381 21.50 21.5 107.52%


Qvalue


Target Compounds
 <<< I1 : ISTD ID = 1 >>>
 95 95 Tert butyl alcohol 4.41 4.51 -0.013 59 57 0.289 0.68 0.7 100
 25 25 chloroform 6.37 6.37 0.000 83 85 84.198 3.14 3.1 97
 37 37 CCl4 6.91 6.91 0.000 117 119 284.222 13.71 13.7 98
 40 40 trichloroethene 8.25 8.24 0.000 130 132 66.795 3.82 3.8 88
 101 101 TAME 7.64 7.41 0.030 73 43 8.707 1.11 1.1 46
 <<< I2 : ISTD ID = 47 >>>
 54 54 MIBK 9.91 9.77 0.012 43 58 5.012 2.05 2.1 1
 59 59 tetra-Cl-ethene 10.65 10.64 0.000 166 168 9.914 0.56 0.6 93
 <<< I3 : ISTD ID = 62 >>>
 88 88 naphthalene 15.79 15.78 0.000 128 129 0.394 1.14 1.1 71

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Quantitation Report: **Applied P & Ch Lab** EPA 524.2





Data Filename: C:\MSDCHEM\1\DATA\03G4717\5951-01.D
Method : C:\MSDCHEM\1\METHODS\E524A003.M
Acq. Time : Nov 6 16:30 2003
Method Update: Mon Oct 27 14:05 2003
Quant. Time : Nov 07 10:24 2003
Print Time : Fri Nov 07 10:24 2003
Miscellaneous :
Sample : F=1 dup
Inst. : GCMS-A
RF via : Multiple Level Calibration
Operator: zou
Multiplier: 1.000000

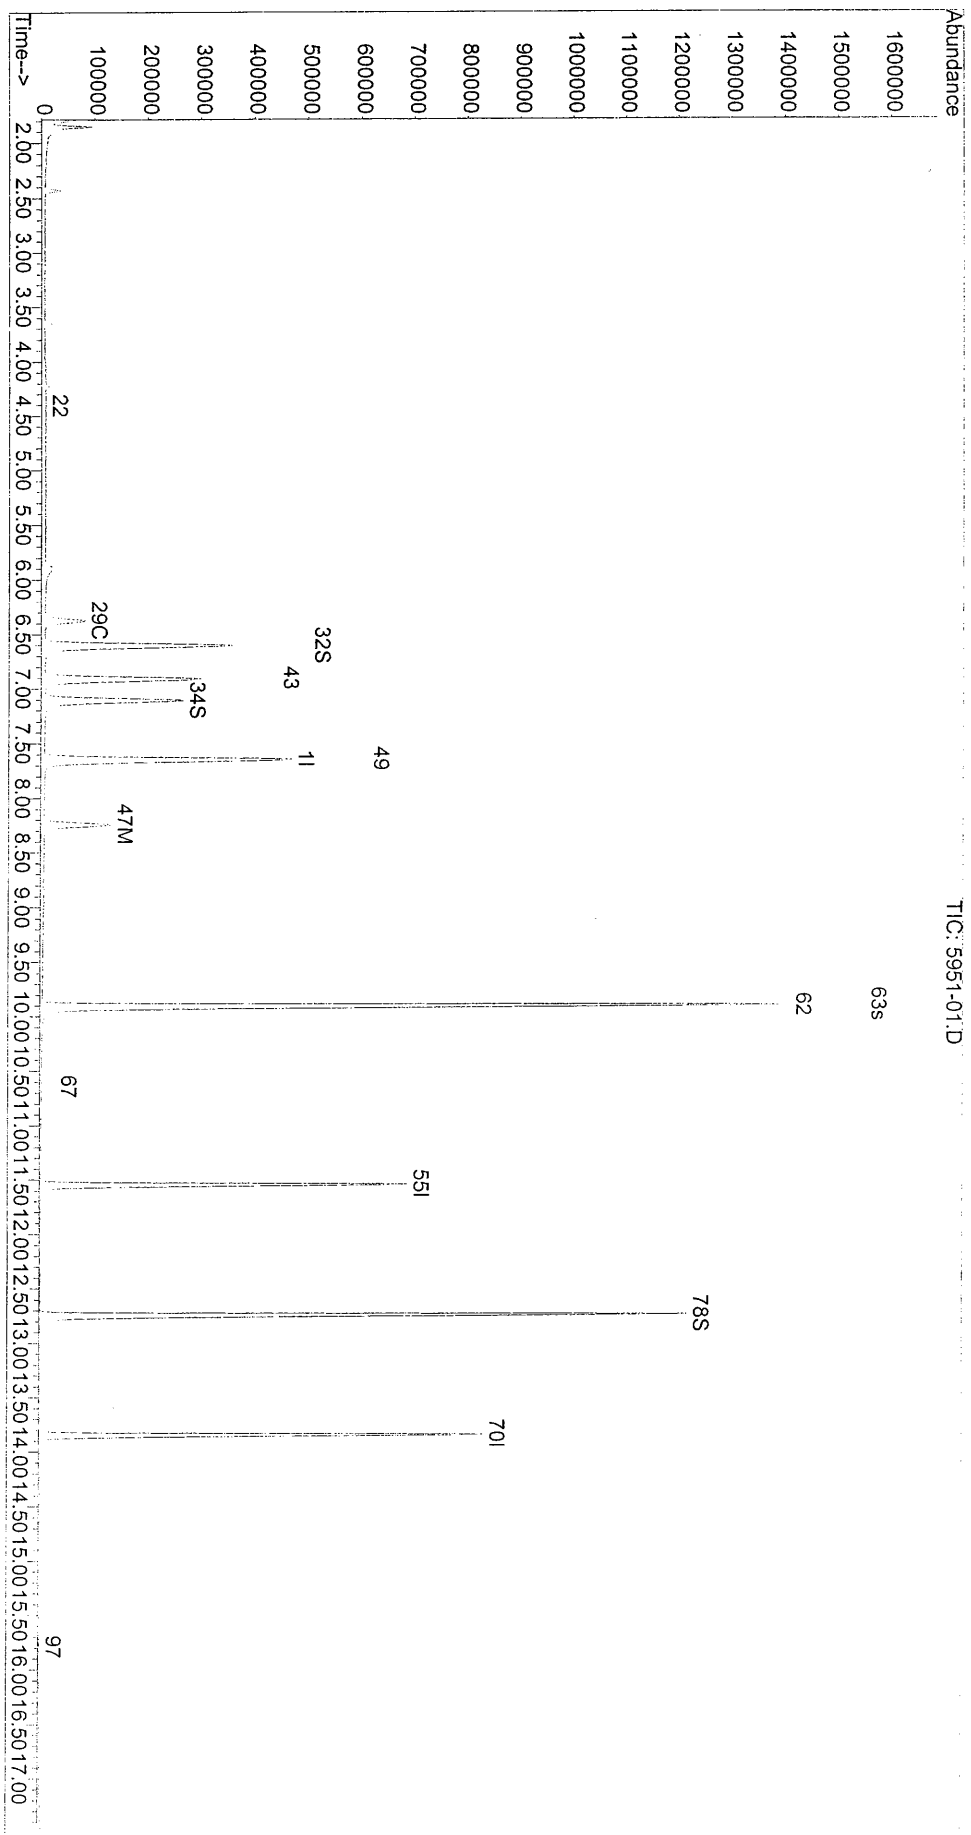

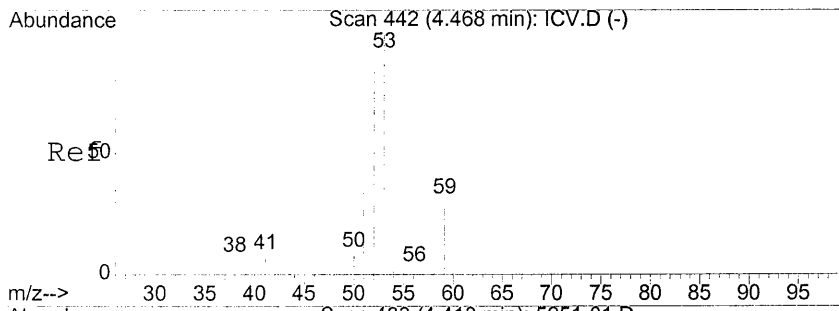




#22
 95 Tert butyl alcoholx10
 Concen: 0.68 ppb
 RT: 4.41 min Scan# 433
 Delta R.T. -0.10 min
 Lab File: 5951-01.D
 Acq: 6 Nov 2003 4:30 pm


| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 59 | 100 | | |
| 57 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

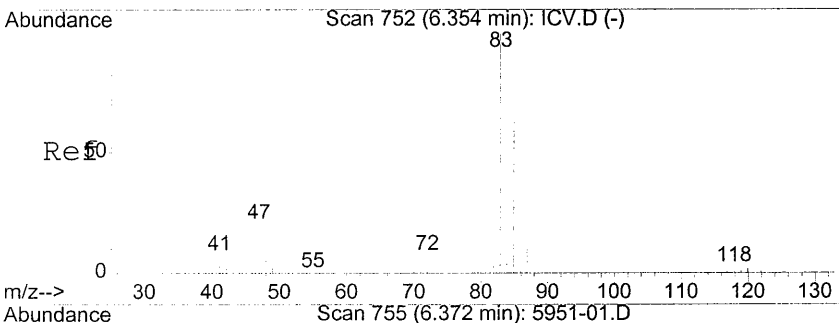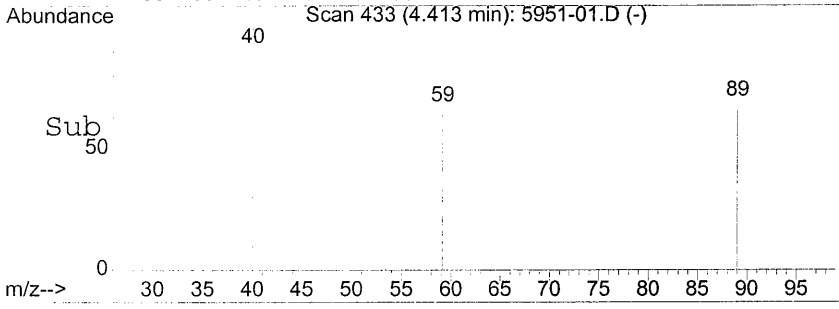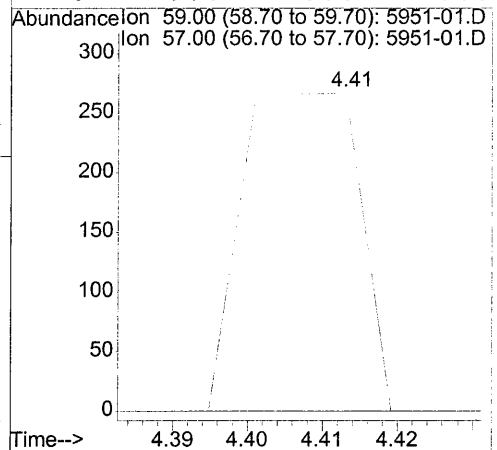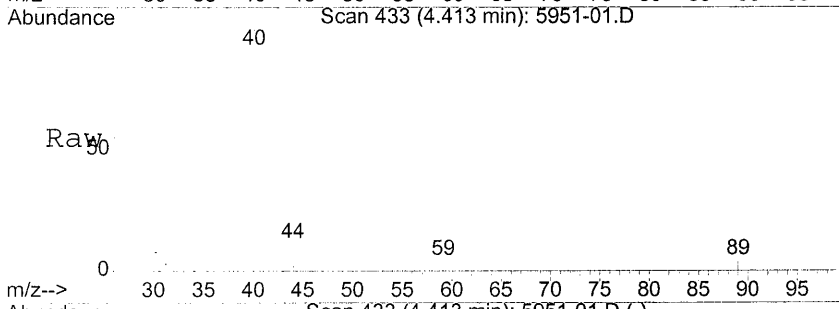

#29
 25 chloroform
 Concen: 3.14 ppb
 RT: 6.37 min Scan# 755
 Delta R.T. 0.00 min
 Lab File: 5951-01.D
 Acq: 6 Nov 2003 4:30 pm


| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 83 | 100 | | |
| 85 | 66.6 | 43.9 | 83.9 |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

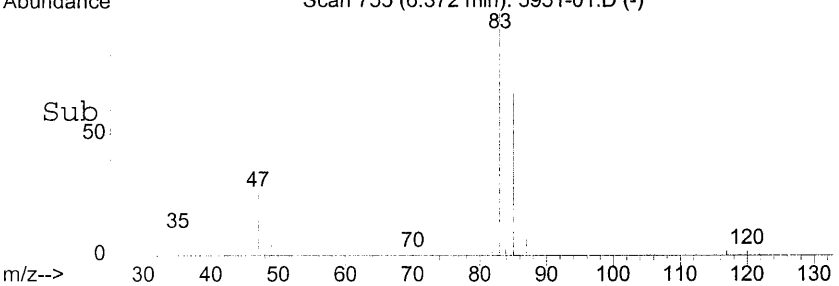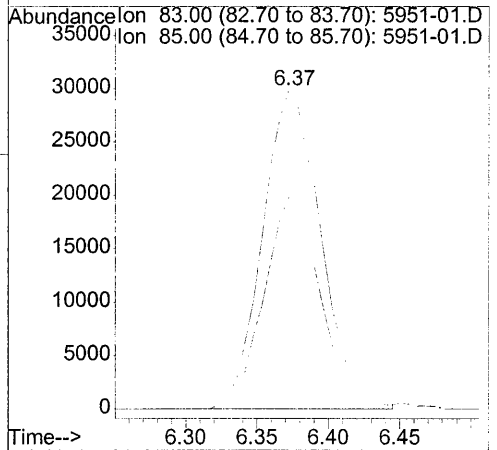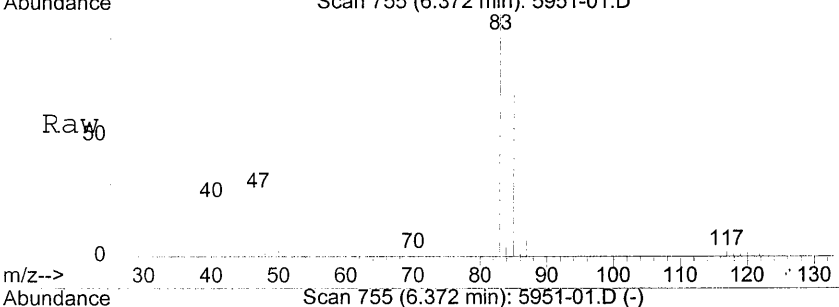



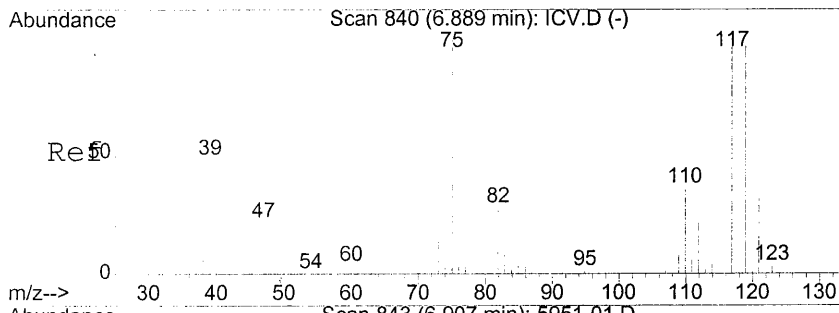


#43
 37 CCl4
 Concen: 13.71 ppb
 RT: 6.91 min Scan# 843
 Delta R.T. -0.01 min
 Lab File: 5951-01.D
 Acq: 6 Nov 2003 4:30 pm

| Tgt Ion | Resp | Lower | Upper |
|---------|--------|-------|-------|
| 117 | 284222 | | |
| 119 | 94.9 | 77.2 | 117.2 |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

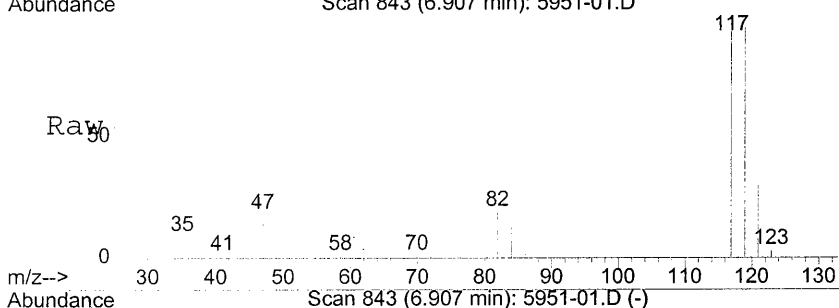


Abundance Ion 117.00 (116.70 to 117.70): 5951-01
 Ion 119.00 (118.70 to 119.70): 5951-01

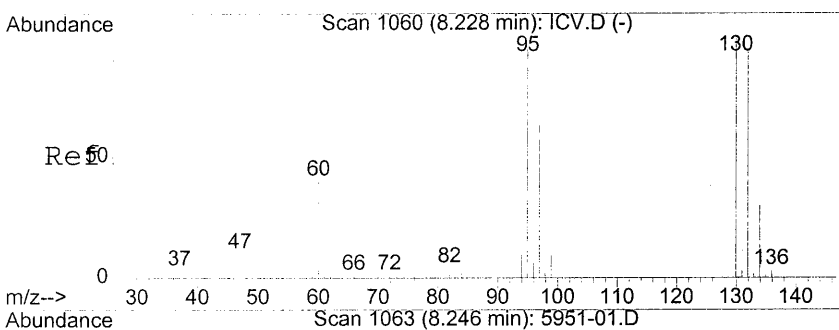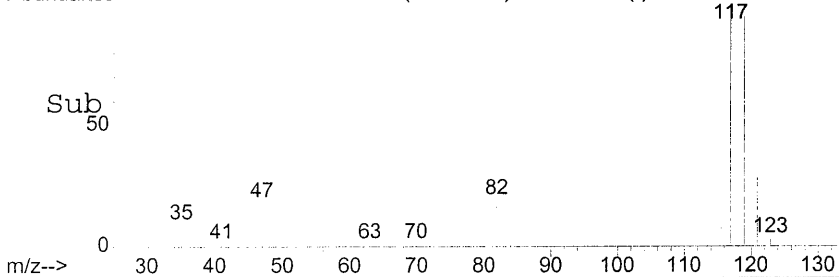
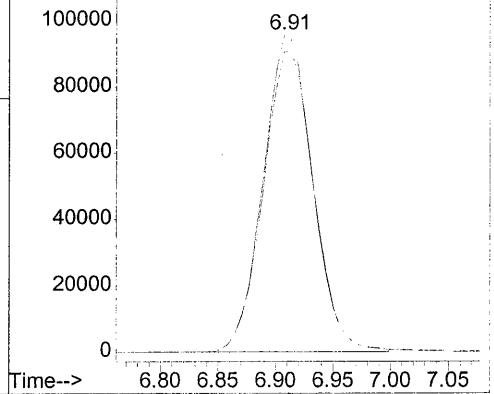



#47
 40 trichloroethene
 Concen: 3.82 ppb
 RT: 8.25 min Scan# 1063
 Delta R.T. 0.01 min
 Lab File: 5951-01.D
 Acq: 6 Nov 2003 4:30 pm

| Tgt Ion | Resp | Lower | Upper |
|---------|-------|-------|-------|
| 130 | 66795 | | |
| 132 | 105.4 | 73.5 | 113.5 |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

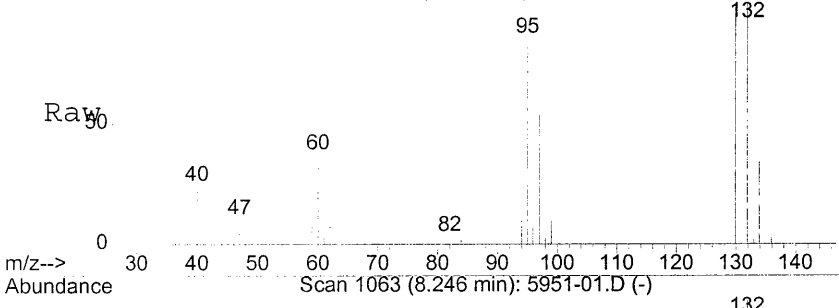


Abundance Ion 130.00 (129.70 to 130.70): 5951-01
 Ion 132.00 (131.70 to 132.70): 5951-01


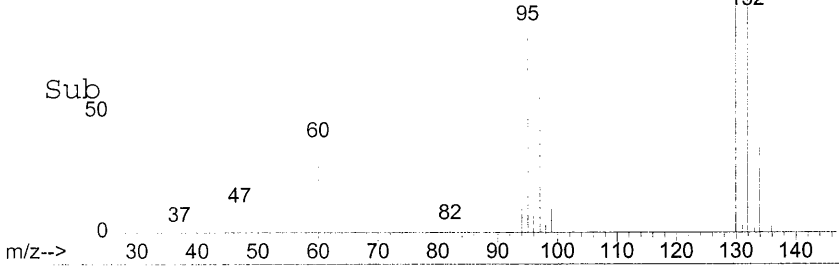
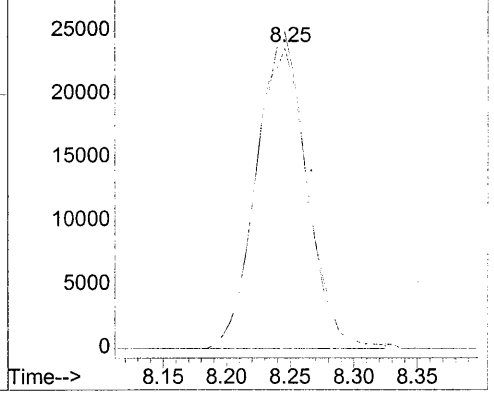


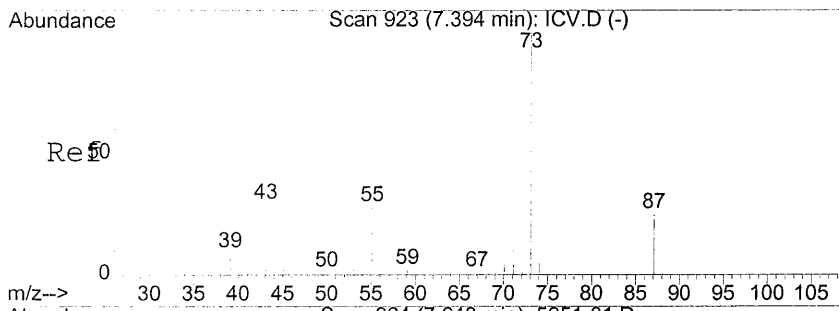


#49
 101 TAME
 Concen: 1.11 ppb
 RT: 7.64 min Scan# 964
 Delta R.T. 0.23 min
 Lab File: 5951-01.D
 Acq: 6 Nov 2003 4:30 pm

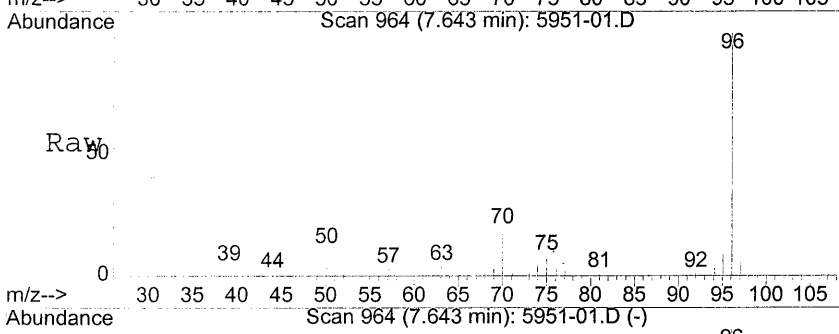



| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 73 | 100 | | |
| 43 | 0.0 | 22.7 | 34.1# |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

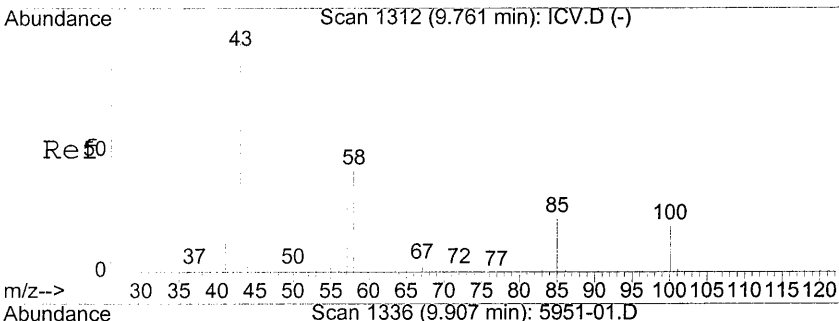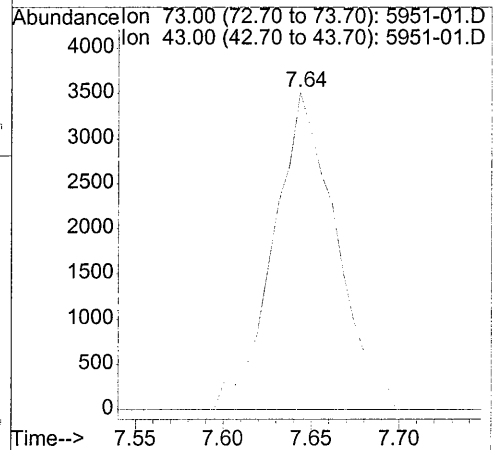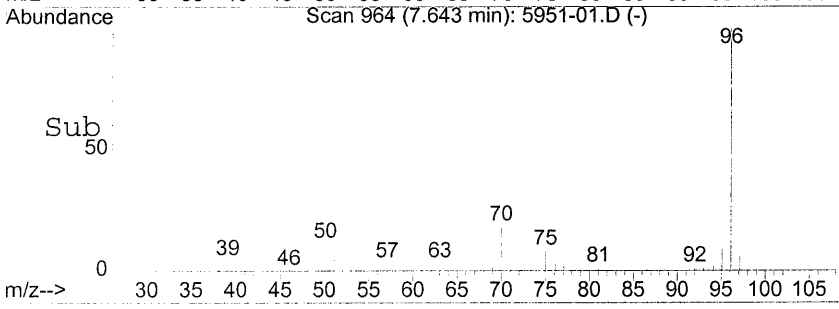


#62
 54 MIBK
 Concen: 2.05 ppb
 RT: 9.91 min Scan# 1336
 Delta R.T. 0.14 min
 Lab File: 5951-01.D
 Acq: 6 Nov 2003 4:30 pm

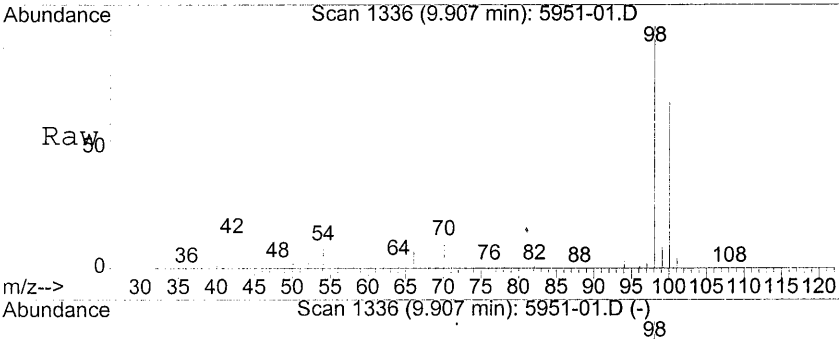


| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 43 | 100 | | |
| 58 | 150.0 | 20.1 | 60.1# |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

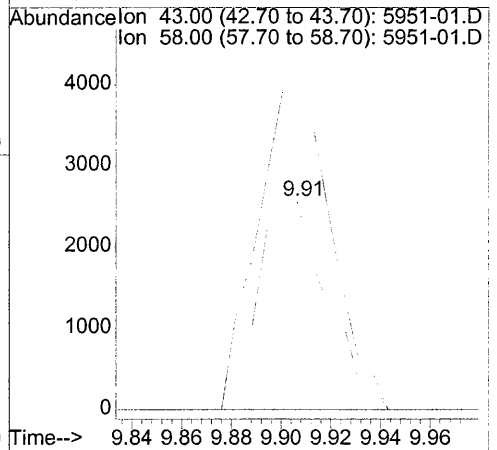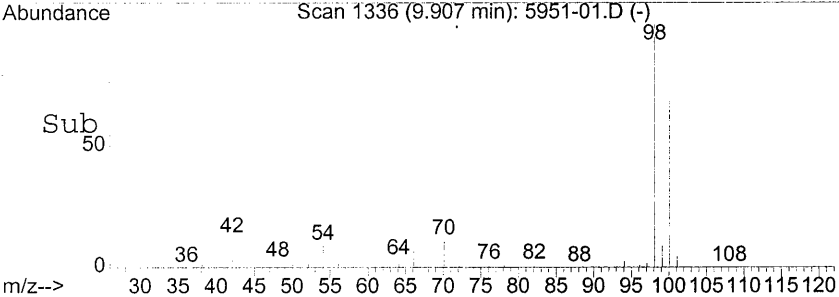



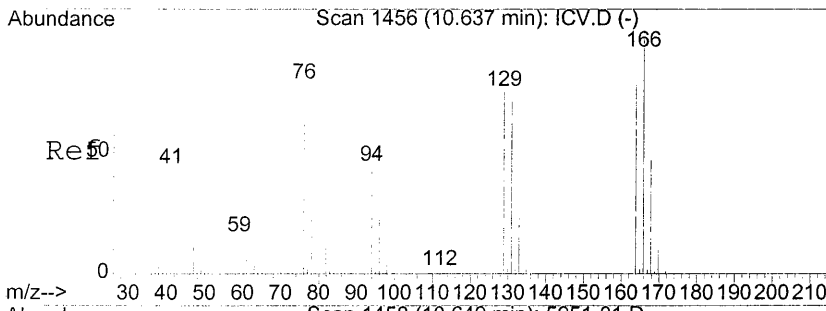


#67
 59 tetra-Cl-ethene
 Concen: 0.56 ppb
 RT: 10.65 min Scan# 1458
 Delta R.T. 0.01 min
 Lab File: 5951-01.D
 Acq: 6 Nov 2003 4:30 pm

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 166 | 100 | | |
| 168 | 40.0 | 24.9 | 64.9 |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

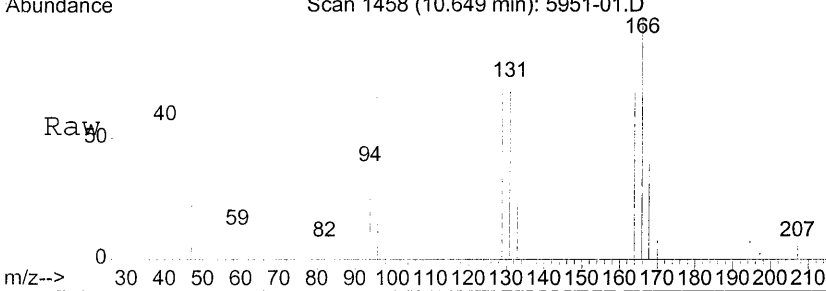


Abundance Ion 166.00 (165.70 to 166.70): 5951-01
 Ion 168.00 (167.70 to 168.70): 5951-01

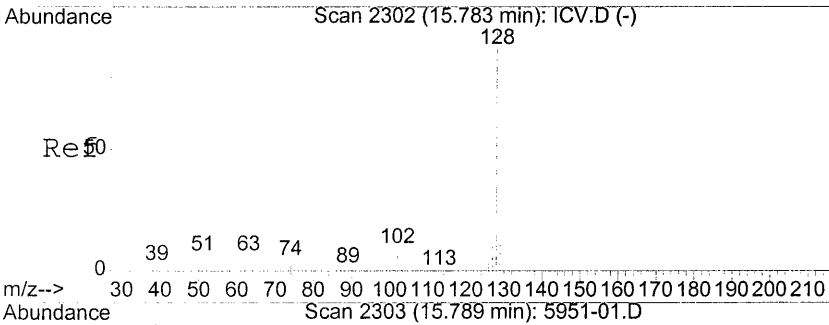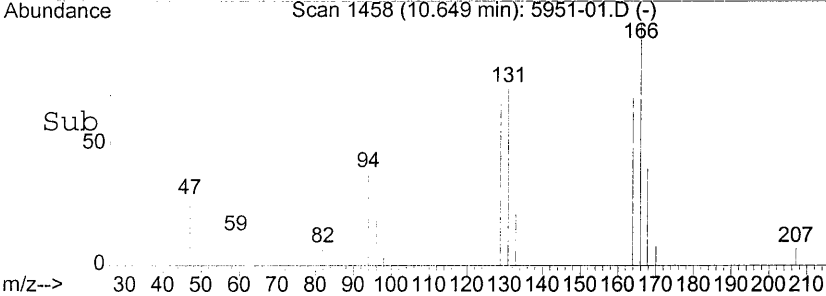
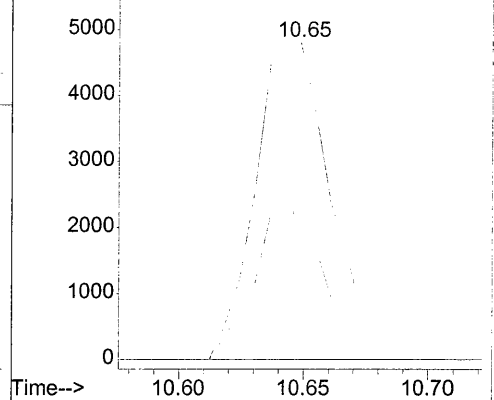


#97
 88 naphthalene
 Concen: 1.14 ppb
 RT: 15.79 min Scan# 2303
 Delta R.T. 0.01 min
 Lab File: 5951-01.D
 Acq: 6 Nov 2003 4:30 pm

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 128 | 100 | | |
| 129 | 0.0 | 0.0 | 31.1 |
| 0 | 0.0 | 0.0 | 0.0 |
| 0 | 0.0 | 0.0 | 0.0 |

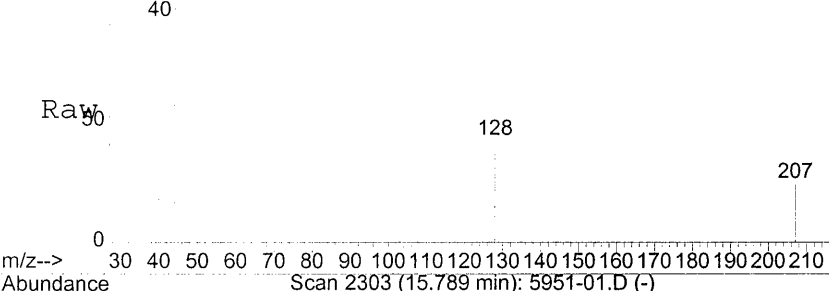

Abundance Ion 128.00 (127.70 to 128.70): 5951-01
 Ion 129.00 (128.70 to 129.70): 5951-01

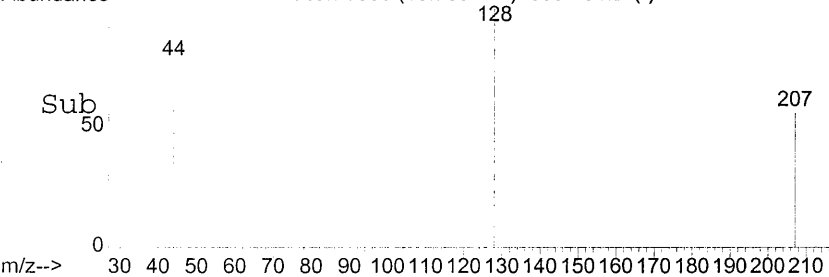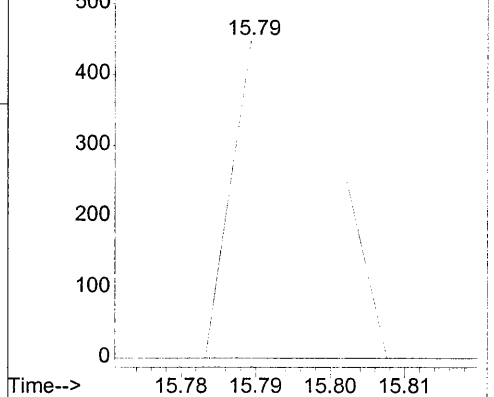

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|--------------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: EB-9-11-4-03 | Lab Sample ID: 03-5951-2 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-02 | Prep. No: - | Anal. Time: 16:57 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | <0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROBENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROBENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2,2-TETRACHLOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | Control Limit, % | Surro. Rec.% | |
|---|-------------------------------------|------------------|--------------|-----|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 108 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 108 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 107 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 109 |
| # | of out-of-control | | | 0 |

Internal Standard

| | | Control Limit, % | IS Rec.% | |
|---|-----------------------|------------------|----------|-----|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 96 |
| 2 | 1,4-DICHLOROETHANE-D4 | 3855-82-1 | 50-200 | 94 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 100 |
| # | of out-of-control | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-14-1 | Lab Sample ID: 03-5951-3 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-03 | Prep. No: - | Anal. Time: 17:23 |
| Methanol Vol: - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | <0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | 0.5 | J |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | 0.4 | J |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROBENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROBENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | Control Limit, % | Surro. Rec.% | |
|---|-------------------------------------|------------------|--------------|-----|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 108 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 108 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 106 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 108 |
| # | of out-of-control | | | 0 |

Internal Standard

| | | Control Limit, % | IS Rec.% | |
|---|-----------------------|------------------|----------|----|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 94 |
| 2 | 1,4-DICHLOROETHANE-D4 | 3855-82-1 | 50-200 | 90 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 97 |
| # | of out-of-control | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-14-2 | Lab Sample ID: 03-5951-4 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-04 | Prep. No: - | Anal. Time: 17:49 |
| Methanol Vol: - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | 0.5 | J |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | 0.7 | |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | 4.6 | |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 112TRICHLORO-122TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | Control Limit, % | Surro. Rec.% | |
|---------------------|------------------------------------|------------------|--------------|-----|
| 1 | 1-BROMO-4-FLUOROENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 110 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 106 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 108 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 107 |
| # of out-of-control | | | | 0 |

Internal Standard

| | | Control Limit, % | IS Rec.% | |
|---------------------|-----------------------|------------------|----------|----|
| 1 | CHLOROENZENE-D5 | 3114-55-4 | 50-200 | 96 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 91 |
| 3 | FLUROENZENE | 462-06-6 | 50-200 | 99 |
| # of out-of-control | | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-14-3 | Lab Sample ID: 03-5951-5 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-05 | Prep. No: - | Anal. Time: 18:15 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | 0.4 | J |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | 0.6 | |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | 0.8 | |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | | Control Limit, % | Surro. Rec.% |
|---------------------|-------------------------------------|------------|------------------|--------------|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 109 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 109 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 107 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 109 |
| # of out-of-control | | | | 0 |

Internal Standard

| | | | Control Limit, % | IS Rec.% |
|---------------------|-----------------------|-----------|------------------|----------|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 94 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 92 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 98 |
| # of out-of-control | | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-14-4 | Lab Sample ID: 03-5951-6 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-06 | Prep. No: - | Anal. Time: 18:41 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | <0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 112TRICHLORO-122TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | | Control Limit, % | Surro. Rec.% |
|---|-------------------------------------|------------|------------------|--------------|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 109 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 109 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 108 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 109 |
| # | of out-of-control | | | 0 |

Internal Standard

| | | | Control Limit, % | IS Rec.% |
|---|-----------------------|-----------|------------------|----------|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 93 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 90 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 96 |
| # | of out-of-control | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-14-5 | Lab Sample ID: 03-5951-7 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-07 | Prep. No: - | Anal. Time: 19:07 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | < 0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | < 0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | < 0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | < 0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | < 0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | < 0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | < 0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | < 0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | < 0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | < 10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | < 0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | < 0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | < 0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | < 0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | < 0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | < 0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | < 0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | < 0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | < 0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | < 0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | < 0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | < 0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | < 0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | < 0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | < 0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | < 0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | < 0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | < 0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | < 0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | < 0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | < 0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | < 0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | < 0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | < 0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | < 0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | < 0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | < 0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | < 0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | < 0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 112TRICHLORO-122TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | Control Limit, % | Surro. Rec.% | |
|---|-------------------------------------|------------------|--------------|-----|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 110 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 108 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 108 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 107 |
| # | of out-of-control | | | 0 |

Internal Standard

| | | Control Limit, % | IS Rec.% | |
|---|-----------------------|------------------|----------|----|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 94 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 91 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 98 |
| # | of out-of-control | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-17-1 | Lab Sample ID: 03-5951-8 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-08 | Prep. No: - | Anal. Time: 19:33 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | <0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 112TRICHLORO-122TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | Control Limit, % | Surro. Rec.% | |
|---|-------------------------------------|------------------|--------------|-----|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 108 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 109 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 109 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 108 |
| # | of out-of-control | | | 0 |

Internal Standard

| | | Control Limit, % | IS Rec.% | |
|---|-----------------------|------------------|----------|----|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 94 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 91 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 97 |
| # | of out-of-control | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-17-2 | Lab Sample ID: 03-5951-9 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-09 | Prep. No: - | Anal. Time: 19:59 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | < 0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | < 0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | < 0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | < 0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | < 0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | < 0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | < 0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | < 0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | < 0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | < 10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | 1.0 | |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | < 0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | < 0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | < 0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | 1.1 | |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | < 0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | < 0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | < 0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | < 0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | < 0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | < 0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | < 0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | < 0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | < 0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | < 0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | < 0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | < 0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | < 0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | < 0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | < 0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | < 0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | < 0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | < 0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | < 0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | < 0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | < 0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | < 0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | < 0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | < 0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|--------------------------|---|------------|------|-------------------------|---------------------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | 0.4 | J |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | 6.2 | |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2,2-TETRACHLORO-1,1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |
| Surrogates | | | | Control Limit, % | Surro. Rec.% | |
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | | 70-129 | 109 | |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | | 70-129 | 111 | |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | | 70-122 | 107 | |
| 4 | TOLUENE-D8 | 2037-26-5 | | 73-129 | 108 | |
| # of out-of-control | | | | | 0 | |
| Internal Standard | | | | Control Limit, % | IS Rec.% | |
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | | 50-200 | 95 | |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | | 50-200 | 92 | |
| 3 | FLUOROBENZENE | 462-06-6 | | 50-200 | 98 | |
| # of out-of-control | | | | | 0 | |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|---------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-17-3 | Lab Sample ID: 03-5951-10 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-10 | Prep. No: - | Anal. Time: 20:25 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | < 0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | < 0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | < 0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | < 0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | < 0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | < 0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | < 0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | < 0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | < 0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | < 10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | 11.0 | |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | < 0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | < 0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | < 0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | 2.6 | |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | < 0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | < 0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | < 0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | < 0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | < 0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | < 0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | < 0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | < 0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | < 0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | < 0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | < 0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | < 0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | < 0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | < 0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | < 0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | < 0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | < 0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | < 0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | < 0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | < 0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | < 0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | < 0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | < 0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | < 0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | 0.4 | J |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | 3.1 | |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 112TRICHLORO-122TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | Control Limit, % | Surro. Rec.% | |
|---------------------|-------------------------------------|------------------|--------------|-----|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 107 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 111 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 108 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 105 |
| # of out-of-control | | | | 0 |

Internal Standard

| | | Control Limit, % | IS Rec.% | |
|---------------------|-----------------------|------------------|----------|----|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 96 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 94 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 98 |
| # of out-of-control | | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQ, or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|---------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-17-4 | Lab Sample ID: 03-5951-11 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-11 | Prep. No: - | Anal. Time: 20:51 |
| Methanol Vol: - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | <0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | 0.8 | |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | Control Limit, % | Surro. Rec.% | |
|---|-------------------------------------|------------------|--------------|-----|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 109 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 110 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 109 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 107 |
| # | of out-of-control | | | 0 |

Internal Standard

| | | Control Limit, % | IS Rec.% | |
|---|-----------------------|------------------|----------|----|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 95 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 91 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 96 |
| # | of out-of-control | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|---------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: MW-17-5 | Lab Sample ID: 03-5951-12 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-12 | Prep. No: - | Anal. Time: 21:17 |
| Methanol Vol: - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | <0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | <0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|--------------------------|---|------------|------|-------------------------|---------------------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | <0.5 | U |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |
| Surrogates | | | | Control Limit, % | Surro. Rec.% | |
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | | 70-129 | 106 | |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | | 70-129 | 110 | |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | | 70-122 | 107 | |
| 4 | TOLUENE-D8 | 2037-26-5 | | 73-129 | 107 | |
| # of out-of-control | | | | | 0 | |
| Internal Standard | | | | Control Limit, % | IS Rec.% | |
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | | 50-200 | 97 | |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | | 50-200 | 94 | |
| 3 | FLUOROBENZENE | 462-06-6 | | 50-200 | 99 | |
| # of out-of-control | | | | | 0 | |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|--------------------------------|---------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 11/04/2003 |
| Project ID: JPL | Service ID: 35951 | Collected by: JR |
| Sample ID: TB-9-11-4-03 | Lab Sample ID: 03-5951-13 | Received Date: 11/04/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: A |
| Batch No: 03G4717 | Prep. Date: 11/06/03 | Anal. Date: 11/06/03 |
| Data File Name: 5951-13 | Prep. No: - | Anal. Time: 14:20 |
| Methanol Vol. - | Sample Amount: 25.0 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | < 0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | < 0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | < 0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | < 0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | < 0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | < 0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | < 0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | < 0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | < 0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | < 10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | < 0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | < 0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | < 0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | < 0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | < 0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | < 0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | < 0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | < 0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 0.5 | < 0.5 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | < 0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | < 0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | < 0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | < 0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | < 0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | < 0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | < 0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | < 0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | < 0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | < 0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | < 0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | < 0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | < 0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | < 0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | < 0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | < 0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | < 0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | < 0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | < 0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | < 0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 0.5 | 0.4 | J |
| 42 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 43 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 112TRICHLORO-122TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | | Control Limit, % | Surro. Rec.% |
|---|-------------------------------------|------------|------------------|--------------|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 109 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 107 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 105 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 107 |
| # | of out-of-control | | | 0 |

Internal Standard

| | | | Control Limit, % | IS Rec.% |
|---|-----------------------|-----------|------------------|----------|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 100 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 97 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 104 |
| # | of out-of-control | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

FORM-2A

Applied P & Ch Laboratory

Surrogate Recovery Summary for Method 524.2

Client Name: GEOFON, Inc.

Contract No:

Lab Code: APCL

Case No:

SAS No:

SDG Number: 035951

Project ID: JPL

Project No: 04-4428.10

Sample Matrix: Water

Batch No: 03G4717

| # | Client Sample No | Lab Sample ID | S1 % # | S2 % # | S3 % # | S4 % # | TOT OUT |
|----|------------------|----------------|--------|--------|--------|--------|---------|
| 1 | 03G4717-LCS-01 | 03G4717-LCS-01 | 96 | 98 | 97 | 96 | 0 |
| 2 | MW-3-1MS | 03-5973-2MS | 98 | 97 | 97 | 94 | 0 |
| 3 | MW-3-1MSD | 03-5973-2MSD | 92 | 97 | 95 | 92 | 0 |
| 4 | 03G4717-MB-01 | 03G4717-MB-01 | 108 | 108 | 107 | 108 | 0 |
| 5 | TB-9-11-4-03 | 03-5951-13 | 109 | 107 | 105 | 107 | 0 |
| 6 | DUPE-5-4-Q03 | 03-5951-1 | 108 | 108 | 107 | 108 | 0 |
| 7 | EB-9-11-4-03 | 03-5951-2 | 108 | 108 | 107 | 109 | 0 |
| 8 | MW-14-1 | 03-5951-3 | 108 | 108 | 106 | 108 | 0 |
| 9 | MW-14-2 | 03-5951-4 | 110 | 106 | 108 | 107 | 0 |
| 10 | MW-14-3 | 03-5951-5 | 109 | 109 | 107 | 109 | 0 |
| 11 | MW-14-4 | 03-5951-6 | 109 | 109 | 108 | 109 | 0 |
| 12 | MW-14-5 | 03-5951-7 | 110 | 108 | 108 | 107 | 0 |
| 13 | MW-17-1 | 03-5951-8 | 108 | 109 | 109 | 108 | 0 |
| 14 | MW-17-2 | 03-5951-9 | 109 | 111 | 107 | 108 | 0 |
| 15 | MW-17-3 | 03-5951-10 | 107 | 111 | 108 | 105 | 0 |
| 16 | MW-17-4 | 03-5951-11 | 109 | 110 | 109 | 107 | 0 |
| 17 | MW-17-5 | 03-5951-12 | 106 | 110 | 107 | 107 | 0 |
| 18 | | | | | | | |
| 19 | | | | | | | |
| 20 | | | | | | | |
| 21 | | | | | | | |
| 22 | | | | | | | |
| 23 | | | | | | | |
| 24 | | | | | | | |
| 25 | | | | | | | |

QC Control Limit

S1 = 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) 70-129
 S2 = 1,2-DICHLOROETHANE-D4 70-129
 S3 = DIBROMOFLUOROMETHANE 70-122
 S4 = TOLUENE-D8 73-129

Column to be used to flag recovery values:

* - Values outside of contract required QC Limits D - Surrogate diluted out I - Matrix Interference

FORM-3A

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 524.2

| | | |
|---------------------------|------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 35951 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03G4717 | |
| LCS Filename: G4717L01 | Date Analyzed: 110603 | Time Analyzed: 10:53 |
| LCSD Filename: - | Date Analyzed: - | Time Analyzed: - |

| Spiked Components | Unit | Spike Added | Concentration | | LCS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|------|------------|-----------------|
| | | | Unspiked | LCS | | |
| BENZENE | µg/L | 20 | 0 | 17.9 | 90 | 65-120 |
| CHLOROBENZENE | µg/L | 20 | 0 | 18.9 | 95 | 65-134 |
| 1,1-DICHLOROETHENE | µg/L | 20 | 0 | 20.8 | 104 | 65-127 |
| TOLUENE | µg/L | 20 | 0 | 17.8 | 89 | 65-134 |
| TRICHLOROETHENE | µg/L | 20 | 0 | 19.6 | 98 | 67-122 |
| # of Out-of-control | | | | | 0 | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717L01.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:53 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:54 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:54 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------------------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.64 | 7.64 | 0.000 | 96 | 70 | 654.113 | 10.00 | | 0.00 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 497.611 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.84 | 13.85 | 0.000 | 152 | 150 | 302.374 | 10.00 | | 0.00 | |

| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|-------------------|-------|-------|-------|-----|-----|----------|-------|--|------|--------|
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.60 | 0.000 | 111 | 113 | 299.152 | 19.48 | | 19.5 | 97.39% |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.10 | 7.11 | 0.000 | 65 | 102 | 268.993 | 19.66 | | 19.7 | 98.31% |
| 55 | toluene-d8 | 9.91 | 9.91 | 0.000 | 98 | 100 | 1053.107 | 19.17 | | 19.2 | 95.87% |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 394.058 | 19.23 | | 19.2 | 96.16% |

| Target Compounds | | | | | | | | | | | | |
|------------------|----------------------|------|------|-------|-----|-----|---------|--------|--|-------|-----|--------|
| <<< I1 | : ISTD ID = 1 | >>> | | | | | | | | | | Qvalue |
| 3 | 3 di-Cl-di-F-methan | 1.89 | 1.89 | 0.000 | 85 | 87 | 248.211 | 18.87 | | 18.9 | 97 | |
| 4 | 4 Chloromethane | 2.11 | 2.11 | 0.000 | 50 | 52 | 186.734 | 14.29 | | 14.3 | 99 | |
| 2 | 2 F114 | 2.03 | 2.03 | 0.000 | 85 | 135 | 128.811 | 20.83 | | 20.8 | 31 | |
| 5 | 5 vinyl chloride | 2.22 | 2.22 | 0.000 | 62 | 64 | 198.734 | 17.82 | | 17.8 | 100 | |
| 6 | 6 bromomethane | 2.61 | 2.61 | 0.000 | 94 | 96 | 95.361 | 15.05 | | 15.1 | 96 | |
| 7 | 7 chloroethane | 2.73 | 2.73 | 0.000 | 64 | 66 | 116.949 | 19.47 | | 19.5 | 94 | |
| 8 | 8 tri-Cl-F-methane | 3.03 | 3.03 | 0.000 | 101 | 103 | 421.221 | 22.84 | | 22.8 | 99 | |
| 91 | 91 Acetonitrile X10 | 4.07 | 4.07 | 0.000 | 41 | 40 | 484.281 | 171.84 | | 171.8 | 87 | |
| 9 | 9 acrolein X10 | 3.51 | 3.51 | 0.000 | 56 | 55 | 249.577 | 180.31 | | 180.3 | 100 | |
| 11 | 11 acetone X10 | 3.72 | 3.73 | 0.000 | 43 | 58 | 390.766 | 186.99 | | 187.0 | 80 | |
| 12 | 12 ethyl ether X5 | 3.37 | 3.37 | 0.000 | 59 | 74 | 574.360 | 92.42 | | 92.4 | 78 | |
| 13 | 13 11-dichloroethene | 3.63 | 3.64 | 0.000 | 61 | 96 | 322.800 | 20.77 | | 20.8 | 78 | |
| 14 | 14 Iodomethane | 3.81 | 3.81 | 0.000 | 142 | 127 | 209.713 | 16.56 | | 16.6 | 93 | |
| 15 | 15 F-113 | 3.65 | 3.65 | 0.000 | 101 | 151 | 216.447 | 22.96 | | 23.0 | 83 | |
| 16 | 16 acrylonitrile X10 | 4.52 | 4.52 | 0.000 | 53 | 52 | 475.092 | 169.31 | | 169.3 | 93 | |
| 17 | 17 carbon disulfide | 3.90 | 3.90 | 0.000 | 76 | 78 | 504.418 | 17.05 | | 17.0 | 100 | |
| 94 | 94 Isopropyl Alcohol | 4.09 | 4.10 | 0.000 | 45 | 43 | 60.696 | 453.21 | | 453.2 | 100 | |
| 18 | 18 methylene chlorid | 4.22 | 4.22 | 0.000 | 84 | 49 | 248.714 | 17.89 | | 17.9 | 78 | |
| 19 | 19 t-12-di-Cl-ethene | 4.58 | 4.58 | 0.000 | 96 | 61 | 268.036 | 18.35 | | 18.4 | 94 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

m
11/06/03
m
4/6/03
 # ?
 # ?
 # ?

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717L01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\F524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:53 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:54 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:54 2003
 Miscleaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|--------------------|-------|-------|--------|------|-----|----------|--------|-------|---------|------|
| 20 | t-Bu-Me-ether | 4.59 | 4.59 | 0.000 | 73 | 57 | 516.132 | 20.08 | 20.1 | 94 | ? |
| 95 | Tert butyl alcoho | 4.50 | 4.51 | -0.002 | 59 | 57 | 80.352 | 187.21 | 187.2 | 100 | #? |
| 94 | allyl chloride | 4.07 | 4.07 | 0.000 | 41 | 76 | 484.281 | 16.79 | 16.8 | 77 | #? |
| 21 | 11-dichloroethane | 5.12 | 5.12 | 0.000 | 63 | 83 | 449.390 | 18.58 | 18.6 | 98 | |
| 97 | propionitrile | 6.02 | 6.02 | 0.000 | 54 | 51 | 20.048 | 17.39 | 17.4 | 100 | #? |
| 22 | c-12-di-Cl-ethene | 5.92 | 5.92 | 0.000 | 96 | 61 | 280.411 | 18.41 | 18.4 | 86 | ? |
| 23 | 22-Dichloropropan | 5.92 | 5.92 | 0.000 | 77 | 97 | 407.456 | 26.40 | 26.4 | 97 | ? |
| 24 | Br-Cl-methane | 6.25 | 6.25 | 0.000 | 128 | 130 | 139.016 | 18.05 | 18.0 | 94 | ? |
| 25 | chloroform | 6.37 | 6.37 | 0.000 | 83 | 85 | 507.072 | 18.65 | 18.6 | 99 | ? |
| 26 | tetrahydrofuranX5 | 6.35 | 6.35 | 0.000 | 42 | 72 | 188.090 | 83.00 | 83.0 | 87 | ? |
| 98 | Disopropyl ether | 5.24 | 5.24 | 0.000 | 45 | 87 | 842.567 | 18.14 | 18.1 | 90 | ? |
| 99 | ETBE | 5.74 | 5.74 | 0.000 | 59 | 87 | 624.966 | 21.34 | 21.3 | 92 | |
| 30 | 12-dichloroethane | 7.22 | 7.22 | 0.000 | 64 | 62 | 105.192 | 19.84 | 19.8 | 98 | ? |
| 32 | vinyl acetate X5 | 5.19 | 5.20 | 0.000 | 43 | 86 | 2184.800 | 96.40 | 96.4 | 94 | |
| 92 | Nitro Methane (x10 | 5.82 | 5.84 | -0.002 | 61 | 46 | 57.142 | 74.80 | 74.8 | 93 | |
| 33 | 2-butanoneMEK X10 | 5.94 | 5.95 | 0.000 | 43 | 72 | 604.599 | 177.16 | 177.2 | 84 | ? |
| 93 | Ethyl Acetate x2 | 6.04 | 6.04 | 0.000 | 43 | 61 | 288.825 | 34.18 | 34.2 | 99 | ? |
| 34 | 111-trichloroetha | 6.65 | 6.65 | 0.000 | 97 | 99 | 512.630 | 22.42 | 22.4 | 99 | |
| 35 | 11-Di-Cl-propene | 6.90 | 6.90 | 0.000 | 75 | 110 | 364.102 | 21.10 | 21.1 | 93 | ? |
| 36 | benzene | 7.21 | 7.21 | 0.000 | 78 | 52 | 989.572 | 17.89 | 17.9 | 90 | ? |
| 37 | CCl4 | 6.91 | 6.91 | 0.000 | 117 | 119 | 507.164 | 24.12 | 24.1 | 99 | ? |
| 100 | Isobutyl alcohol | 7.41 | 7.41 | 0.000 | 43 | 42 | 169.487 | 201.78 | 201.8 | 93 | ? |
| 38 | thiophene | 7.53 | 7.53 | 0.000 | 84 | 58 | 535.721 | 18.60 | 18.6 | 95 | |
| 39 | 12-di-Cl-propane | 8.56 | 8.56 | 0.000 | 63 | 76 | 223.117 | 17.63 | 17.6 | 84 | |
| 40 | trichloroethene | 8.24 | 8.24 | 0.000 | 130 | 132 | 346.430 | 19.55 | 19.5 | 90 | |
| 41 | dibromomethane | 8.73 | 8.73 | 0.000 | 174 | 172 | 164.273 | 18.66 | 18.7 | 98 | |
| 101 | TAME | 7.41 | 7.41 | 0.000 | 73 | 43 | 495.323 | 18.40 | 18.4 | 89 | #? |
| 42 | Br-di-Cl-methane | 8.96 | 8.96 | 0.000 | 83 | 85 | 382.675 | 19.20 | 19.2 | 100 | |
| 43 | Me-methacrylate | 8.76 | 8.76 | 0.000 | 69 | 100 | 116.698 | 16.52 | 16.5 | 93 | |
| 44 | 2-ClEt-VI-ether10 | 9.38 | 9.38 | 0.000 | 63 | 43 | 283.135 | 131.35 | 131.4 | 81 | |
| 45 | C-13-di-Cl-propen | 9.56 | 9.56 | 0.000 | 75 | 110 | 402.940 | 20.07 | 20.1 | 93 | |
| 46 | t-1,3-dichloropro | 10.25 | 10.25 | 0.000 | 75 | 110 | 345.424 | 19.26 | 19.3 | 96 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717L01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:53 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:54 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:54 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------|--------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| <<< I2 | : ISTD ID = 47 >>> | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.46 | 10.45 | 0.000 | 97 | 83 | 200.584 | 18.21 | 18.2 | 91 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.65 | 0.000 | 76 | 78 | 307.311 | 18.18 | 18.2 | 96 | ? |
| 50 | Et methacrylate | 10.38 | 10.37 | 0.000 | 69 | 99 | 256.371 | 16.69 | 16.7 | 89 | |
| 51 | di-Br-Cl-methane | 10.90 | 10.91 | 0.000 | 129 | 127 | 302.283 | 19.34 | 19.3 | 99 | |
| 52 | bromoform | 12.42 | 12.42 | 0.000 | 173 | 174 | 179.277 | 19.50 | 19.5 | 100 | |
| 53 | 1,4-dichlorobutan | 12.67 | 12.67 | 0.000 | 55 | 41 | 339.964 | 18.26 | 18.3 | 97 | |
| 54 | MIBK | 9.77 | 9.77 | 0.000 | 43 | 58 | 145.001 | 15.15 | 15.2 | 97 | |
| 56 | toluene | 9.99 | 9.99 | 0.000 | 91 | 92 | 1202.310 | 17.84 | 17.8 | 98 | |
| 57 | 2-hexanone X5 | 10.76 | 10.76 | 0.000 | 43 | 58 | 496.288 | 80.68 | 80.7 | 90 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 208.064 | 18.43 | 18.4 | 99 | |
| 59 | tetra-Cl-ethene | 10.64 | 10.64 | 0.000 | 166 | 168 | 392.179 | 21.14 | 21.1 | 96 | ? |
| 60 | chlorobenzene | 11.58 | 11.57 | 0.000 | 112 | 77 | 870.455 | 18.93 | 18.9 | 91 | ? |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 346.269 | 20.23 | 20.2 | 96 | |
| <<< I3 | : ISTD ID = 62 >>> | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 144.169 | 20.88 | 20.9 | 56 | #? |
| 64 | Et-Bz | 11.70 | 11.70 | 0.000 | 91 | 106 | 1498.568 | 19.50 | 19.5 | 95 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 2346.934 | 39.47 | 39.5 | 100 | |
| 66 | styrene | 12.24 | 12.24 | 0.000 | 104 | 78 | 963.705 | 19.25 | 19.2 | 97 | ? |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 1182.078 | 19.69 | 19.7 | 100 | ? |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 210.930 | 17.62 | 17.6 | 97 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.92 | 0.000 | 110 | 97 | 76.274 | 19.19 | 19.2 | 88 | ? |
| 71 | isopropylbenzene | 12.60 | 12.60 | 0.000 | 105 | 120 | 1668.917 | 20.79 | 20.8 | 98 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 401.987 | 19.79 | 19.8 | 99 | ? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 42.712 | 18.04 | 18.0 | 77 | #? |
| 73 | n-propylbenzene | 13.00 | 13.00 | 0.000 | 120 | 78 | 487.694 | 20.98 | 21.0 | 96 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 395.108 | 20.05 | 20.0 | 99 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.19 | 0.000 | 126 | 128 | 394.939 | 19.50 | 19.5 | 99 | ? |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 1462.003 | 20.66 | 20.7 | 94 | ? |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 1622.064 | 21.27 | 21.3 | 97 | ? |
| 78 | 124-tri-Me-Benzen | 13.51 | 13.52 | 0.000 | 105 | 120 | 1488.780 | 20.09 | 20.1 | 98 | ? |
| 79 | tert-butylbenzene | 13.47 | 13.47 | 0.000 | 119 | 91 | 1336.133 | 21.50 | 21.5 | 99 | |


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717L01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\F524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:53 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:54 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:54 2003
 Miscleaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.79 | 0.000 | 146 | 148 | 827.005 | 19.59 | 19.6 | 100 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 1953.543 | 21.05 | 21.1 | 97 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 845.036 | 19.13 | 19.1 | 95 | |
| 83 | Cl-benzyl | 13.98 | 13.98 | 0.000 | 126 | 91 | 92.328 | 20.02 | 20.0 | 84 | # |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 743.785 | 19.24 | 19.2 | 99 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 443.002 | 22.00 | 22.0 | 77 | #? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 54.565 | 18.97 | 19.0 | 97 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 514.934 | 21.39 | 21.4 | 99 | |
| 88 | naphthalene | 15.78 | 15.78 | 0.000 | 128 | 129 | 810.232 | 18.28 | 18.3 | 98 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 324.000 | 23.52 | 23.5 | 99 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 441.734 | 21.25 | 21.3 | 99 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717L01.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:53 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:54 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:54 2003
 Miscleaneous :

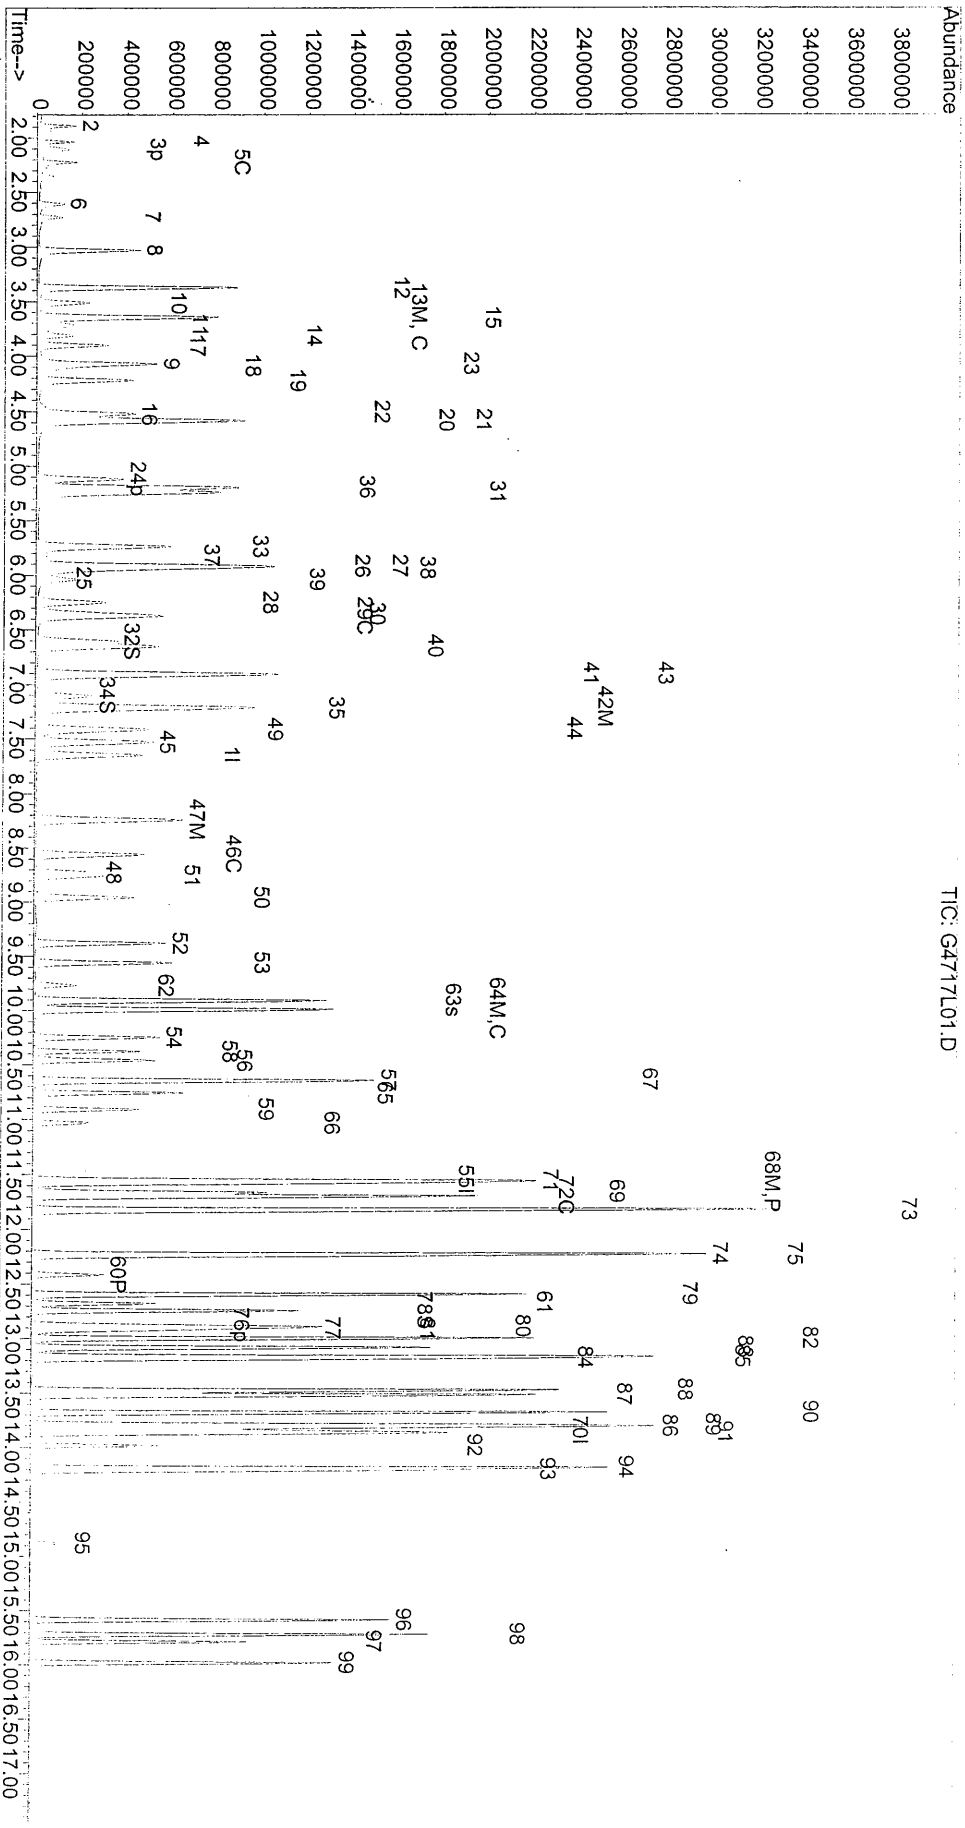

FORM-3A

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 524.2

| | | |
|---------------------------|--------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 35951 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03G4717 | |
| MS Filename: G4717M01 | Date Analyzed: 110603 | Time Analyzed: 11:19 |
| MSD Filename: G4717N01 | Date Analyzed: 110603 | Time Analyzed: 11:44 |
| MS Sample No: MW-3-1 | Sample Lab ID: 03-5973-2 | |

| Spiked Components | Unit | Spike Added | Concentration | | MS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|------|-----------|-----------------|
| | | | Unspiked | MS | | |
| BENZENE | µg/L | 20 | 0 | 17.9 | 90 | 65-121 |
| CHLOROBENZENE | µg/L | 20 | 0 | 18.6 | 93 | 65-134 |
| 1,1-DICHLOROETHENE | µg/L | 20 | 0 | 21.1 | 106 | 65-127 |
| TOLUENE | µg/L | 20 | 0 | 17.6 | 88 | 65-134 |
| TRICHLOROETHENE | µg/L | 20 | 0 | 19.5 | 98 | 65-125 |
| # of Out-of-control | | | | | 0 | |

| Spiked Components | Unit | Spike Added | MSD Concentration | MSD Rec% # | RPD% # | QC Limit, % | |
|---------------------|------|-------------|-------------------|------------|--------|-------------|--------|
| | | | | | | RPD | REC |
| BENZENE | µg/L | 20 | 17.6 | 88 | 2 | 28 | 65-121 |
| CHLOROBENZENE | µg/L | 20 | 18.1 | 91 | 2 | 35 | 65-134 |
| 1,1-DICHLOROETHENE | µg/L | 20 | 20.9 | 105 | 1 | 31 | 65-127 |
| TOLUENE | µg/L | 20 | 17.3 | 87 | 1 | 35 | 65-134 |
| TRICHLOROETHENE | µg/L | 20 | 19.6 | 98 | 0 | 30 | 65-125 |
| # of Out-of-control | | | | 0 | 0 | | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717M01.D Sample : F=1 \$5973-02
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 11:19 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:01 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:01 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | QIon | QI | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|-------------------|-------|-------|--------|------|-----|----------|--------|-------|---------|--------------|
| 20 | t-Bu-Me-ether | 4.59 | 4.59 | 0.000 | 73 | 57 | 535.612 | 20.07 | 20.1 | 95 | ? |
| 95 | Tert butyl alcoho | 4.43 | 4.51 | -0.011 | 59 | 57 | 156.314 | 350.81 | 350.8 | 100 | ? |
| 94 | allyl chloride | 4.07 | 4.07 | 0.000 | 41 | 76 | 488.801 | 16.33 | 16.3 | 78 | #? (1/13/03) |
| 21 | 11-dichloroethane | 5.12 | 5.12 | 0.000 | 63 | 83 | 464.011 | 18.48 | 18.5 | 98 | # |
| 97 | propionitrile | 6.00 | 6.02 | -0.002 | 54 | 51 | 18.040 | 15.07 | 15.1 | 100 | ? |
| 22 | c-12-di-Cl-ethene | 5.92 | 5.92 | 0.000 | 96 | 61 | 290.894 | 18.40 | 18.4 | 90 | ? |
| 23 | 22-Dichloropropan | 5.92 | 5.92 | 0.000 | 77 | 97 | 420.309 | 26.23 | 26.2 | 99 | ? |
| 24 | Br-Cl-methane | 6.25 | 6.25 | 0.000 | 128 | 130 | 142.089 | 17.77 | 17.8 | 99 | ? |
| 25 | chloroform | 6.37 | 6.37 | 0.000 | 83 | 85 | 530.573 | 18.80 | 18.8 | 99 | ? |
| 26 | tetrahydrofuranX5 | 6.34 | 6.35 | -0.002 | 42 | 72 | 192.907 | 82.00 | 82.0 | 87 | ? |
| 98 | Diisopropyl ether | 5.24 | 5.24 | 0.000 | 45 | 87 | 882.221 | 18.30 | 18.3 | 90 | ? |
| 99 | ETBE | 5.74 | 5.74 | 0.000 | 59 | 87 | 655.767 | 21.57 | 21.6 | 92 | ? |
| 30 | 12-dichloroethane | 7.22 | 7.22 | 0.000 | 64 | 62 | 108.399 | 19.69 | 19.7 | 94 | ? |
| 32 | vinyl acetate X5 | 5.19 | 5.20 | 0.000 | 43 | 86 | 2217.900 | 94.26 | 94.3 | 93 | ? |
| 92 | Nitro Methane(x10 | 5.80 | 5.84 | -0.005 | 61 | 46 | 63.495 | 80.06 | 80.1 | 95 | ? |
| 33 | 2-butanoneMEK X10 | 5.93 | 5.95 | -0.002 | 43 | 72 | 591.593 | 166.98 | 167.0 | 86 | ? |
| 93 | Ethyl Acetate x2 | 6.03 | 6.04 | 0.000 | 43 | 61 | 288.696 | 32.91 | 32.9 | 98 | ? |
| 34 | 111-trichloroetha | 6.65 | 6.65 | 0.000 | 97 | 99 | 529.885 | 22.32 | 22.3 | 97 | ? |
| 35 | 11-Di-Cl-propene | 6.90 | 6.90 | 0.000 | 75 | 110 | 376.938 | 21.04 | 21.0 | 91 | ? |
| 36 | benzene | 7.21 | 7.21 | 0.000 | 78 | 52 | 1028.062 | 17.90 | 17.9 | 91 | ? |
| 37 | CCl4 | 6.91 | 6.91 | 0.000 | 117 | 119 | 519.514 | 23.80 | 23.8 | 100 | ? |
| 100 | Isobutyl alcohol | 7.41 | 7.41 | 0.000 | 43 | 42 | 178.736 | 204.97 | 205.0 | 95 | ? |
| 38 | thiophene | 7.53 | 7.53 | 0.000 | 84 | 58 | 552.850 | 18.49 | 18.5 | 93 | ? |
| 39 | 12-di-Cl-propane | 8.56 | 8.56 | 0.000 | 63 | 76 | 236.529 | 18.00 | 18.0 | 89 | ? |
| 40 | trichloroethene | 8.24 | 8.24 | 0.000 | 130 | 132 | 359.212 | 19.52 | 19.5 | 89 | ? |
| 41 | dibromomethane | 8.73 | 8.73 | 0.000 | 174 | 172 | 168.466 | 18.43 | 18.4 | 100 | ? |
| 101 | TAME | 7.41 | 7.41 | 0.000 | 73 | 43 | 517.988 | 18.52 | 18.5 | 88 | ? |
| 42 | Br-di-Cl-methane | 8.96 | 8.96 | 0.000 | 83 | 85 | 390.857 | 18.90 | 18.9 | 98 | ? |
| 43 | Me-methacrylate | 8.76 | 8.76 | 0.000 | 69 | 100 | 121.981 | 16.63 | 16.6 | 88 | ? |
| 44 | 2-ClEt-Vl-ether10 | 9.57 | 9.38 | 0.026 | 63 | 43 | 1.826 | 11.01 | 11.0 | 28 | ? |
| 45 | c-13-di-Cl-propen | 9.56 | 9.56 | 0.000 | 75 | 110 | 402.551 | 19.32 | 19.3 | 91 | ? |
| 46 | t-1,3-dichloropro | 10.25 | 10.25 | 0.000 | 75 | 110 | 354.172 | 19.03 | 19.0 | 94 | ? |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717M01.D Sample : F=1 \$5973-02
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 11:19 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:01 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:01 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------|--------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| <<< 12 | : ISTD ID = 47 >>> | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.46 | 10.45 | 0.000 | 97 | 83 | 202.321 | 17.47 | 17.5 | 91 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.65 | 0.000 | 76 | 78 | 317.369 | 17.86 | 17.9 | 99 | |
| 50 | Et methacrylate | 10.38 | 10.37 | 0.000 | 69 | 99 | 268.457 | 16.62 | 16.6 | 90 | ? |
| 51 | di-Br-Cl-methane | 10.91 | 10.91 | 0.000 | 129 | 127 | 307.731 | 18.72 | 18.7 | 99 | |
| 52 | bromoform | 12.41 | 12.42 | 0.000 | 173 | 174 | 184.577 | 19.09 | 19.1 | 99 | |
| 53 | 1,4-dichlorobutan | 12.68 | 12.67 | 0.000 | 55 | 41 | 344.879 | 17.62 | 17.6 | 96 | |
| 54 | MIBK | 9.77 | 9.77 | 0.000 | 43 | 58 | 152.137 | 15.12 | 15.1 | 92 | |
| 56 | toluene | 9.99 | 9.99 | 0.000 | 91 | 92 | 1245.193 | 17.57 | 17.6 | 100 | |
| 57 | 2-hexanone X5 | 10.75 | 10.76 | 0.000 | 43 | 58 | 519.883 | 80.40 | 80.4 | 91 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 214.882 | 18.10 | 18.1 | 98 | |
| 59 | tetra-Cl-ethene | 10.64 | 10.64 | 0.000 | 166 | 168 | 406.399 | 20.84 | 20.8 | 99 | ? |
| 60 | chlorobenzene | 11.58 | 11.57 | 0.000 | 112 | 77 | 898.462 | 18.58 | 18.6 | 91 | ? |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 354.682 | 19.71 | 19.7 | 98 | |
| <<< 13 | : ISTD ID = 62 >>> | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 147.123 | 20.64 | 20.6 | 58 | #? |
| 64 | Et-Bz | 11.70 | 11.70 | 0.000 | 91 | 106 | 1555.794 | 19.60 | 19.6 | 97 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 2430.038 | 39.58 | 39.6 | 99 | |
| 66 | styrene | 12.24 | 12.24 | 0.000 | 104 | 78 | 983.514 | 19.03 | 19.0 | 100 | ? |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 1220.460 | 19.69 | 19.7 | 96 | ? |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 216.361 | 17.50 | 17.5 | 99 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.92 | 0.000 | 110 | 97 | 78.915 | 19.23 | 19.2 | 93 | ? |
| 71 | isopropylbenzene | 12.60 | 12.60 | 0.000 | 105 | 120 | 1719.600 | 20.75 | 20.7 | 99 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 414.967 | 19.78 | 19.8 | 100 | ? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 44.590 | 18.23 | 18.2 | 81 | #? |
| 73 | n-propylbenzene | 13.00 | 13.00 | 0.000 | 120 | 78 | 507.852 | 21.16 | 21.2 | 94 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 411.509 | 20.22 | 20.2 | 100 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.19 | 0.000 | 126 | 128 | 407.564 | 19.49 | 19.5 | 100 | ? |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 1498.752 | 20.51 | 20.5 | 93 | ? |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 1659.868 | 21.08 | 21.1 | 98 | ? |
| 78 | 124-tri-Me-Benzen | 13.52 | 13.52 | 0.000 | 105 | 120 | 1531.880 | 20.02 | 20.0 | 97 | |
| 79 | tert-butylbenzene | 13.47 | 13.47 | 0.000 | 119 | 91 | 1377.295 | 21.47 | 21.5 | 97 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06


Quantitation Report: **Applied P & Ch Lab** EPA 524.2

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717M01.D Sample : F=1 \$5973-02
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 11:19 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:01 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:01 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.79 | 0.000 | 146 | 148 | 865.438 | 19.86 | 19.9 | 96 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 1994.589 | 20.82 | 20.8 | 98 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 863.158 | 18.92 | 18.9 | 97 | |
| 83 | Cl-benzy1 | 13.98 | 13.98 | 0.000 | 126 | 91 | 94.449 | 19.86 | 19.9 | 80 | # |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 764.744 | 19.16 | 19.2 | 99 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 446.733 | 21.49 | 21.5 | 86 | #? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 56.260 | 18.94 | 18.9 | 95 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 521.917 | 20.99 | 21.0 | 99 | |
| 88 | naphthalene | 15.78 | 15.78 | 0.000 | 128 | 129 | 837.480 | 18.30 | 18.3 | 100 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 331.844 | 23.33 | 23.3 | 99 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 455.972 | 21.25 | 21.2 | 100 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717M01.D Sample : F=1 \$5973-02
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 11:19 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:01 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:01 2003
 Miscleaneous :

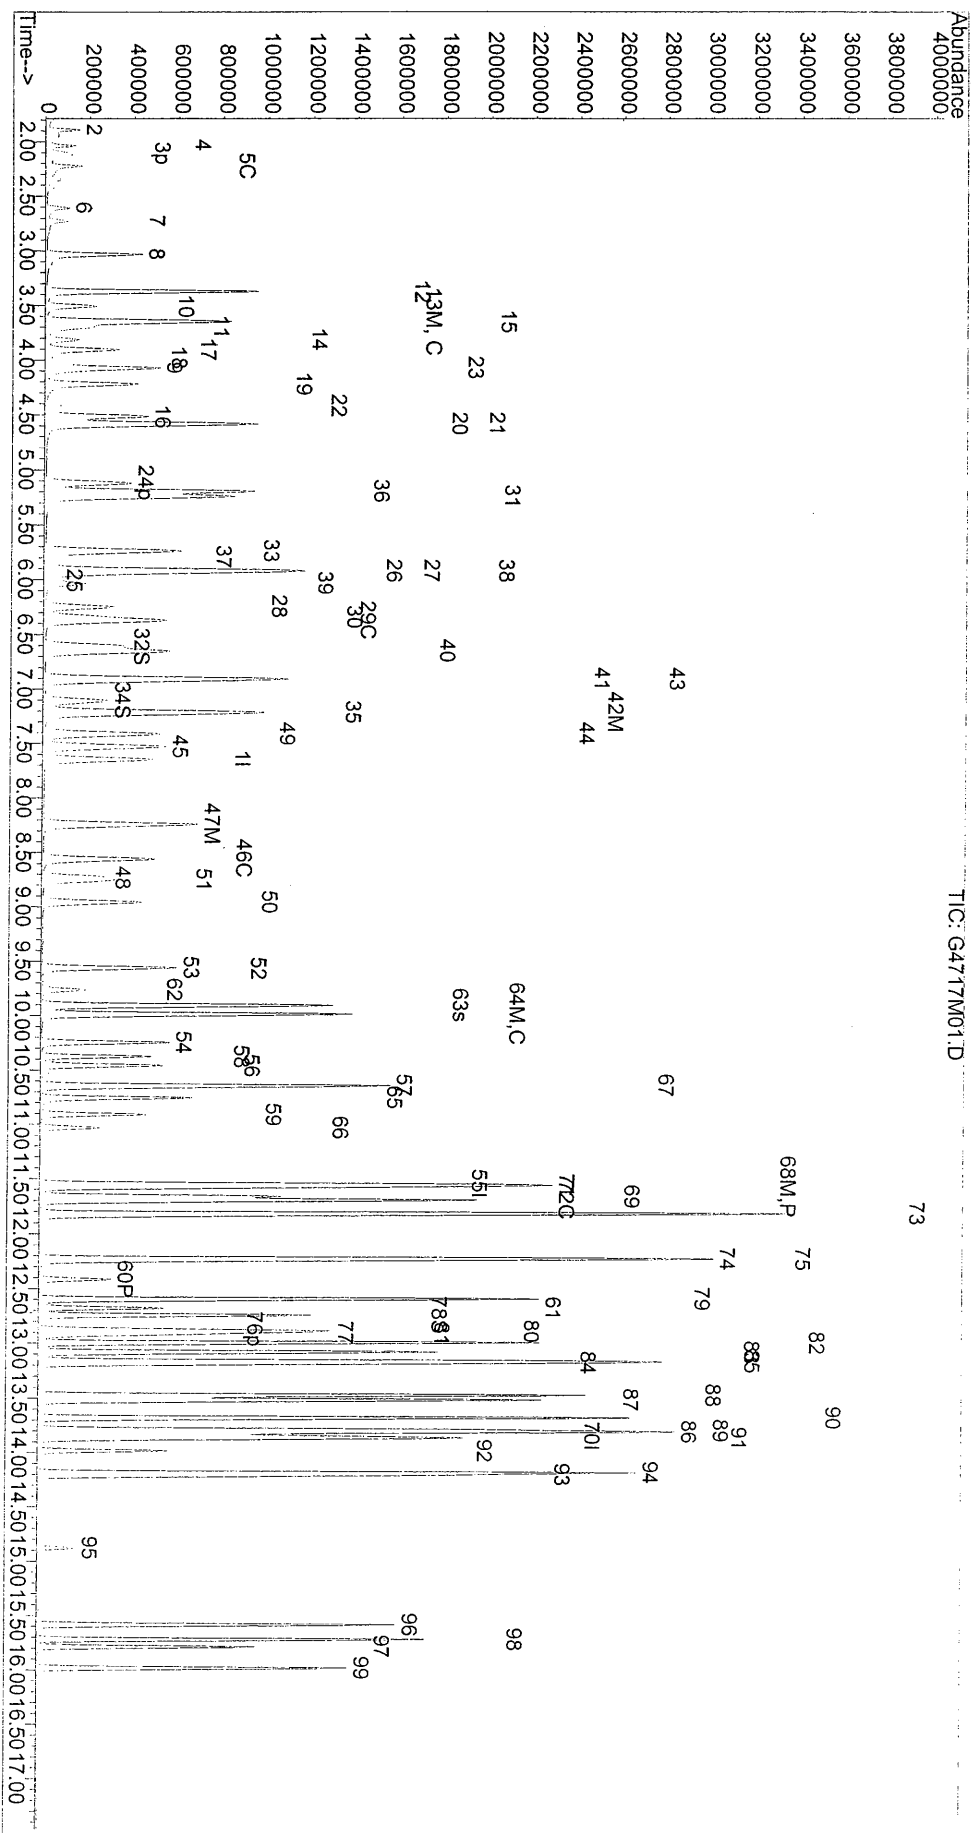

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717N01.D Sample : F=1 \$5973-02
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 11:44 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:02 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:02 2003
 Miscelaneous :

Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------------------|---------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.64 | 7.64 | 0.000 | 96 | 70 | 690.552 | 10.00 | | 0.00 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 531.594 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenzene | 13.84 | 13.85 | 0.000 | 152 | 150 | 325.550 | 10.00 | | 0.00 | |

| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|-------------------|-------|-------|-------|-----|-----|----------|-------|--|------|--------|
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.60 | 0.000 | 111 | 113 | 308.413 | 19.02 | | 19.0 | 95.10% |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.10 | 7.11 | 0.000 | 65 | 102 | 278.767 | 19.30 | | 19.3 | 96.51% |
| 55 | toluene-d8 | 9.91 | 9.91 | 0.000 | 98 | 100 | 1078.908 | 18.39 | | 18.4 | 91.94% |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 407.624 | 18.48 | | 18.5 | 92.39% |

| Target Compounds | | | | | | | | | | | |
|------------------|-------------------|------|------|--------|-----|-----|---------|--------|--|-------|-----|
| <<< 11 | : ISTD ID = 1 | >>> | | | | | | | | | |
| 3 | di-Cl-di-F-methan | 1.89 | 1.89 | 0.000 | 85 | 87 | 241.045 | 17.36 | | 17.4 | 100 |
| 4 | Chloromethane | 2.11 | 2.11 | 0.000 | 50 | 52 | 198.736 | 14.41 | | 14.4 | 96 |
| 2 | F114 | 2.03 | 2.03 | 0.000 | 85 | 135 | 126.997 | 19.43 | | 19.4 | 49 |
| 5 | vinyl chloride | 2.22 | 2.22 | 0.000 | 62 | 64 | 211.003 | 17.92 | | 17.9 | 98 |
| 6 | bromomethane | 2.61 | 2.61 | 0.000 | 94 | 96 | 95.757 | 14.32 | | 14.3 | 96 |
| 7 | chloroethane | 2.73 | 2.73 | 0.000 | 64 | 66 | 110.621 | 17.44 | | 17.4 | 93 |
| 8 | tri-Cl-F-methane | 3.03 | 3.03 | 0.000 | 101 | 103 | 449.633 | 23.09 | | 23.1 | 98 |
| 91 | Acetonitrile X10 | 4.07 | 4.07 | 0.000 | 41 | 40 | 490.974 | 165.02 | | 165.0 | 88 |
| 9 | acrolein X10 | 3.51 | 3.51 | 0.000 | 56 | 55 | 230.312 | 157.62 | | 157.6 | 99 |
| 11 | acetone X10 | 3.70 | 3.73 | -0.003 | 43 | 58 | 370.261 | 167.83 | | 167.8 | 81 |
| 12 | ethyl ether X5 | 3.37 | 3.37 | 0.000 | 59 | 74 | 615.330 | 93.79 | | 93.8 | 79 |
| 13 | 11-dichloroethene | 3.64 | 3.64 | 0.000 | 61 | 96 | 342.975 | 20.91 | | 20.9 | 86 |
| 14 | Iodomethane | 3.81 | 3.81 | 0.000 | 142 | 127 | 216.577 | 16.20 | | 16.2 | 92 |
| 15 | F-113 | 3.65 | 3.65 | 0.000 | 101 | 151 | 227.035 | 22.82 | | 22.8 | 85 |
| 16 | acrylonitrile X10 | 4.52 | 4.52 | 0.000 | 53 | 52 | 495.027 | 167.11 | | 167.1 | 96 |
| 17 | carbon disulfide | 3.90 | 3.90 | 0.000 | 76 | 78 | 540.419 | 17.30 | | 17.3 | 100 |
| 94 | Isopropyl Alcohol | 4.01 | 4.10 | -0.011 | 45 | 43 | 39.122 | 276.71 | | 276.7 | 100 |
| 18 | methylene chlorid | 4.22 | 4.22 | 0.000 | 84 | 49 | 250.906 | 17.05 | | 17.1 | 78 |
| 19 | t-12-di-Cl-ethene | 4.58 | 4.58 | 0.000 | 96 | 61 | 276.332 | 17.92 | | 17.9 | 90 |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

De
De 11/17/03
De
 # 11/17/03
 ?
 ?
 ?
 ?

Quantitation Report: **Applied P & Ch Lab** EPA 524.2

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717N01.D Sample : f=1 \$5973-02
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 11:44 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:02 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:02 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|-------------------|-------|-------|--------|------|-----|----------|--------|-------|---------|-------------------|
| 20 | t-Bu-Me-ether | 4.59 | 4.59 | 0.000 | 73 | 57 | 551.105 | 20.31 | 20.3 | 94 | ? |
| 95 | Tert butyl alcoho | 4.45 | 4.51 | -0.008 | 59 | 57 | 170.506 | 376.29 | 376.3 | 100 | <i>me</i> |
| 94 | allyl chloride | 4.07 | 4.07 | 0.000 | 41 | 76 | 490.974 | 16.13 | 16.1 | 78 | #? <i>11/6/03</i> |
| 21 | 11-dichloroethane | 5.12 | 5.12 | 0.000 | 63 | 83 | 460.225 | 18.02 | 18.0 | 99 | |
| 97 | propionitrile | 6.01 | 6.02 | -0.002 | 54 | 51 | 19.058 | 15.66 | 15.7 | 100 | # |
| 22 | c-12-di-Cl-ethene | 5.92 | 5.92 | 0.000 | 96 | 61 | 290.447 | 18.06 | 18.1 | 88 | ? |
| 23 | 22-Dichloropropan | 5.92 | 5.92 | 0.000 | 77 | 97 | 419.465 | 25.74 | 25.7 | 99 | ? |
| 24 | Br-Cl-methane | 6.25 | 6.25 | 0.000 | 128 | 130 | 144.349 | 17.75 | 17.8 | 100 | |
| 25 | chloroform | 6.37 | 6.37 | 0.000 | 83 | 85 | 533.193 | 18.57 | 18.6 | 99 | |
| 26 | tetrahydrofuranX5 | 6.34 | 6.35 | -0.002 | 42 | 72 | 199.109 | 83.22 | 83.2 | 82 | |
| 98 | Diisopropyl ether | 5.24 | 5.24 | 0.000 | 45 | 87 | 883.130 | 18.01 | 18.0 | 89 | |
| 99 | ETBE | 5.74 | 5.74 | 0.000 | 59 | 87 | 667.266 | 21.58 | 21.6 | 92 | |
| 30 | 12-dichloroethane | 7.22 | 7.22 | 0.000 | 64 | 62 | 109.026 | 19.48 | 19.5 | 98 | ? |
| 32 | vinyl acetate X5 | 5.19 | 5.20 | 0.000 | 43 | 86 | 2217.532 | 92.68 | 92.7 | 92 | |
| 92 | Nitro Methane(x10 | 5.81 | 5.84 | -0.004 | 61 | 46 | 66.370 | 82.29 | 82.3 | 100 | |
| 33 | 2-butanoneMEK X10 | 5.93 | 5.95 | -0.002 | 43 | 72 | 606.948 | 168.46 | 168.5 | 83 | ? |
| 93 | Ethyl Acetate x2 | 6.04 | 6.04 | 0.000 | 43 | 61 | 288.984 | 32.39 | 32.4 | 95 | |
| 34 | 111-trichloroetha | 6.65 | 6.65 | 0.000 | 97 | 99 | 532.576 | 22.06 | 22.1 | 98 | |
| 35 | 11-Di-Cl-propene | 6.90 | 6.90 | 0.000 | 75 | 110 | 379.287 | 20.82 | 20.8 | 91 | ? |
| 36 | benzene | 7.21 | 7.21 | 0.000 | 78 | 52 | 1029.360 | 17.63 | 17.6 | 92 | ? |
| 37 | CCl4 | 6.91 | 6.91 | 0.000 | 117 | 119 | 535.020 | 24.10 | 24.1 | 98 | ? |
| 100 | Isobutyl alcohol | 7.41 | 7.41 | 0.000 | 43 | 42 | 185.791 | 209.51 | 209.5 | 98 | ? |
| 38 | thiophene | 7.53 | 7.53 | 0.000 | 84 | 58 | 553.963 | 18.22 | 18.2 | 91 | |
| 39 | 12-di-Cl-propane | 8.56 | 8.56 | 0.000 | 63 | 76 | 233.184 | 17.45 | 17.4 | 90 | |
| 40 | trichloroethene | 8.25 | 8.24 | 0.000 | 130 | 132 | 367.448 | 19.64 | 19.6 | 92 | |
| 41 | dibromomethane | 8.73 | 8.73 | 0.000 | 174 | 172 | 169.541 | 18.24 | 18.2 | 100 | |
| 101 | TAME | 7.41 | 7.41 | 0.000 | 73 | 43 | 532.815 | 18.73 | 18.7 | 88 | #? |
| 42 | Br-di-Cl-methane | 8.96 | 8.96 | 0.000 | 83 | 85 | 387.504 | 18.42 | 18.4 | 98 | |
| 43 | Me-methacrylate | 8.76 | 8.76 | 0.000 | 69 | 100 | 125.497 | 16.81 | 16.8 | 86 | |
| 44 | 2-ClEt-Vi-ether10 | 9.56 | 9.38 | 0.024 | 63 | 43 | 1.759 | 10.97 | 11.0 | 28 | #? |
| 45 | c-13-di-Cl-propen | 9.56 | 9.56 | 0.000 | 75 | 110 | 408.164 | 19.26 | 19.3 | 91 | ? |
| 46 | t-1,3-dichloropro | 10.25 | 10.25 | 0.000 | 75 | 110 | 358.856 | 18.96 | 19.0 | 94 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717N01.D Sample : F=1 \$5973-02
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 11:44 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:02 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:02 2003
 Miscleaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------|--------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| <<< I2 | : ISTD ID = 47 >>> | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.46 | 10.45 | 0.000 | 97 | 83 | 206.856 | 17.58 | 17.6 | 94 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.65 | 0.000 | 76 | 78 | 324.067 | 17.95 | 17.9 | 97 | |
| 50 | Et methacrylate | 10.38 | 10.37 | 0.000 | 69 | 99 | 274.831 | 16.74 | 16.7 | 88 | ? |
| 51 | di-Br-Cl-methane | 10.90 | 10.91 | 0.000 | 129 | 127 | 311.794 | 18.67 | 18.7 | 100 | |
| 52 | bromoform | 12.41 | 12.42 | 0.000 | 173 | 174 | 183.463 | 18.68 | 18.7 | 100 | |
| 53 | 1,4-dichlorobutan | 12.67 | 12.67 | 0.000 | 55 | 41 | 348.870 | 17.54 | 17.5 | 97 | |
| 54 | MIBK | 9.76 | 9.77 | 0.000 | 43 | 58 | 157.915 | 15.42 | 15.4 | 100 | |
| 56 | toluene | 9.99 | 9.99 | 0.000 | 91 | 92 | 1242.000 | 17.25 | 17.3 | 99 | |
| 57 | 2-hexanone X5 | 10.76 | 10.76 | 0.000 | 43 | 58 | 533.717 | 81.18 | 81.2 | 91 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 213.632 | 17.71 | 17.7 | 95 | |
| 59 | tetra-Cl-ethene | 10.64 | 10.64 | 0.000 | 166 | 168 | 398.513 | 20.11 | 20.1 | 95 | ? |
| 60 | chlorobenzene | 11.57 | 11.57 | 0.000 | 112 | 77 | 888.636 | 18.09 | 18.1 | 93 | ? |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 358.043 | 19.58 | 19.6 | 93 | |
| <<< I3 | : ISTD ID = 62 >>> | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 150.050 | 20.18 | 20.2 | 56 | #? |
| 64 | Et-Bz | 11.70 | 11.70 | 0.000 | 91 | 106 | 1542.753 | 18.64 | 18.6 | 93 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 2397.720 | 37.46 | 37.5 | 99 | |
| 66 | styrene | 12.24 | 12.24 | 0.000 | 104 | 78 | 985.299 | 18.28 | 18.3 | 99 | ? |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 1215.585 | 18.81 | 18.8 | 99 | ? |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 219.652 | 17.04 | 17.0 | 97 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.92 | 0.000 | 110 | 97 | 79.877 | 18.66 | 18.7 | 90 | ? |
| 71 | isopropylbenzene | 12.60 | 12.60 | 0.000 | 105 | 120 | 1701.832 | 19.69 | 19.7 | 100 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 418.715 | 19.14 | 19.1 | 100 | ? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 45.317 | 17.80 | 17.8 | 84 | #? |
| 73 | n-propylbenzene | 13.00 | 13.00 | 0.000 | 120 | 78 | 506.191 | 20.23 | 20.2 | 95 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 410.935 | 19.37 | 19.4 | 100 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.19 | 0.000 | 126 | 128 | 405.945 | 18.62 | 18.6 | 99 | ? |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 1502.067 | 19.71 | 19.7 | 93 | ? |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 1670.563 | 20.35 | 20.4 | 99 | ? |
| 78 | 124-tri-Me-Benzen | 13.51 | 13.52 | 0.000 | 105 | 120 | 1524.936 | 19.11 | 19.1 | 97 | ? |
| 79 | tert-butylbenzene | 13.47 | 13.47 | 0.000 | 119 | 91 | 1368.252 | 20.45 | 20.5 | 98 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717N01.D Sample : F=1 \$5973-02
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 11:44 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 11:02 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:02 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.79 | 0.000 | 146 | 148 | 853.198 | 18.77 | 18.8 | 98 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 2006.778 | 20.09 | 20.1 | 98 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 855.000 | 17.98 | 18.0 | 98 | |
| 83 | Cl-benzyl | 13.98 | 13.98 | 0.000 | 126 | 91 | 95.230 | 19.28 | 19.3 | 83 | # |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 761.712 | 18.30 | 18.3 | 99 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 443.628 | 20.46 | 20.5 | 81 | #? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 57.305 | 18.50 | 18.5 | 95 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 519.294 | 20.03 | 20.0 | 99 | |
| 88 | naphthalene | 15.78 | 15.78 | 0.000 | 128 | 129 | 863.437 | 18.10 | 18.1 | 99 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 328.067 | 22.12 | 22.1 | 100 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 450.225 | 20.12 | 20.1 | 99 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\5973-02.D Sample : f=1 ms
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 15:12 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 07 10:25 2003 Multiplr: 1.000000
 Print Time : Fri Nov 07 11:12 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | QIon | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------------------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.64 | 7.64 | 0.000 | 96 | 70 | 652.896 | 10.00 | | 0.00 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 482.809 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.85 | 13.85 | 0.000 | 152 | 150 | 287.868 | 10.00 | | 0.00 | |


| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|--------------------|-------|-------|-------|-----|-----|----------|-------|--|------|---------|
| 27 | Di-Br-F-Me (surrr) | 6.60 | 6.60 | 0.000 | 111 | 113 | 320.403 | 20.90 | | 20.9 | 104.50% |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.11 | 7.11 | 0.000 | 65 | 102 | 292.499 | 21.42 | | 21.4 | 107.10% |
| 55 | toluene-d8 | 9.91 | 9.91 | 0.000 | 98 | 100 | 1136.525 | 21.33 | | 21.3 | 106.63% |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 418.877 | 21.47 | | 21.5 | 107.37% |

| Target Compounds | | | | | | | | | | | |
|------------------|-------------------|-------|-------|-------|-----|-----|-------|------|--|-----|----|
| <<< | I1 : ISTD ID = 1 | >>> | | | | | | | | | |
| 92 | Nitro Methane(x10 | 5.89 | 5.84 | 0.006 | 61 | 46 | 0.457 | 0.60 | | 0.6 | 16 |
| 101 | TAME | 7.64 | 7.41 | 0.030 | 73 | 43 | 8.317 | 1.10 | | 1.1 | 46 |
| <<< | I2 : ISTD ID = 47 | >>> | | | | | | | | | |
| 54 | MIBK | 9.90 | 9.77 | 0.012 | 43 | 58 | 4.512 | 2.00 | | 2.0 | 1 |
| <<< | I3 : ISTD ID = 62 | >>> | | | | | | | | | |
| 88 | naphthalene | 15.79 | 15.78 | 0.000 | 128 | 129 | 0.717 | 1.14 | | 1.1 | 71 |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\5973-02.D
Method : C:\MSDCHEM\1\METHODS\E524A003.M
Acq. Time : Nov 6 15:12 2003
Method Update: Mon Oct 27 14:05 2003
Quant. Time : Nov 07 10:25 2003
Print Time : Fri Nov 07 11:12 2003
Miscellaneous :

Sample : F=1 ms
Inst. : GCMS-A
RF via : Multiple Level Calibration
Operator: zou
Multiplr: 1.000000

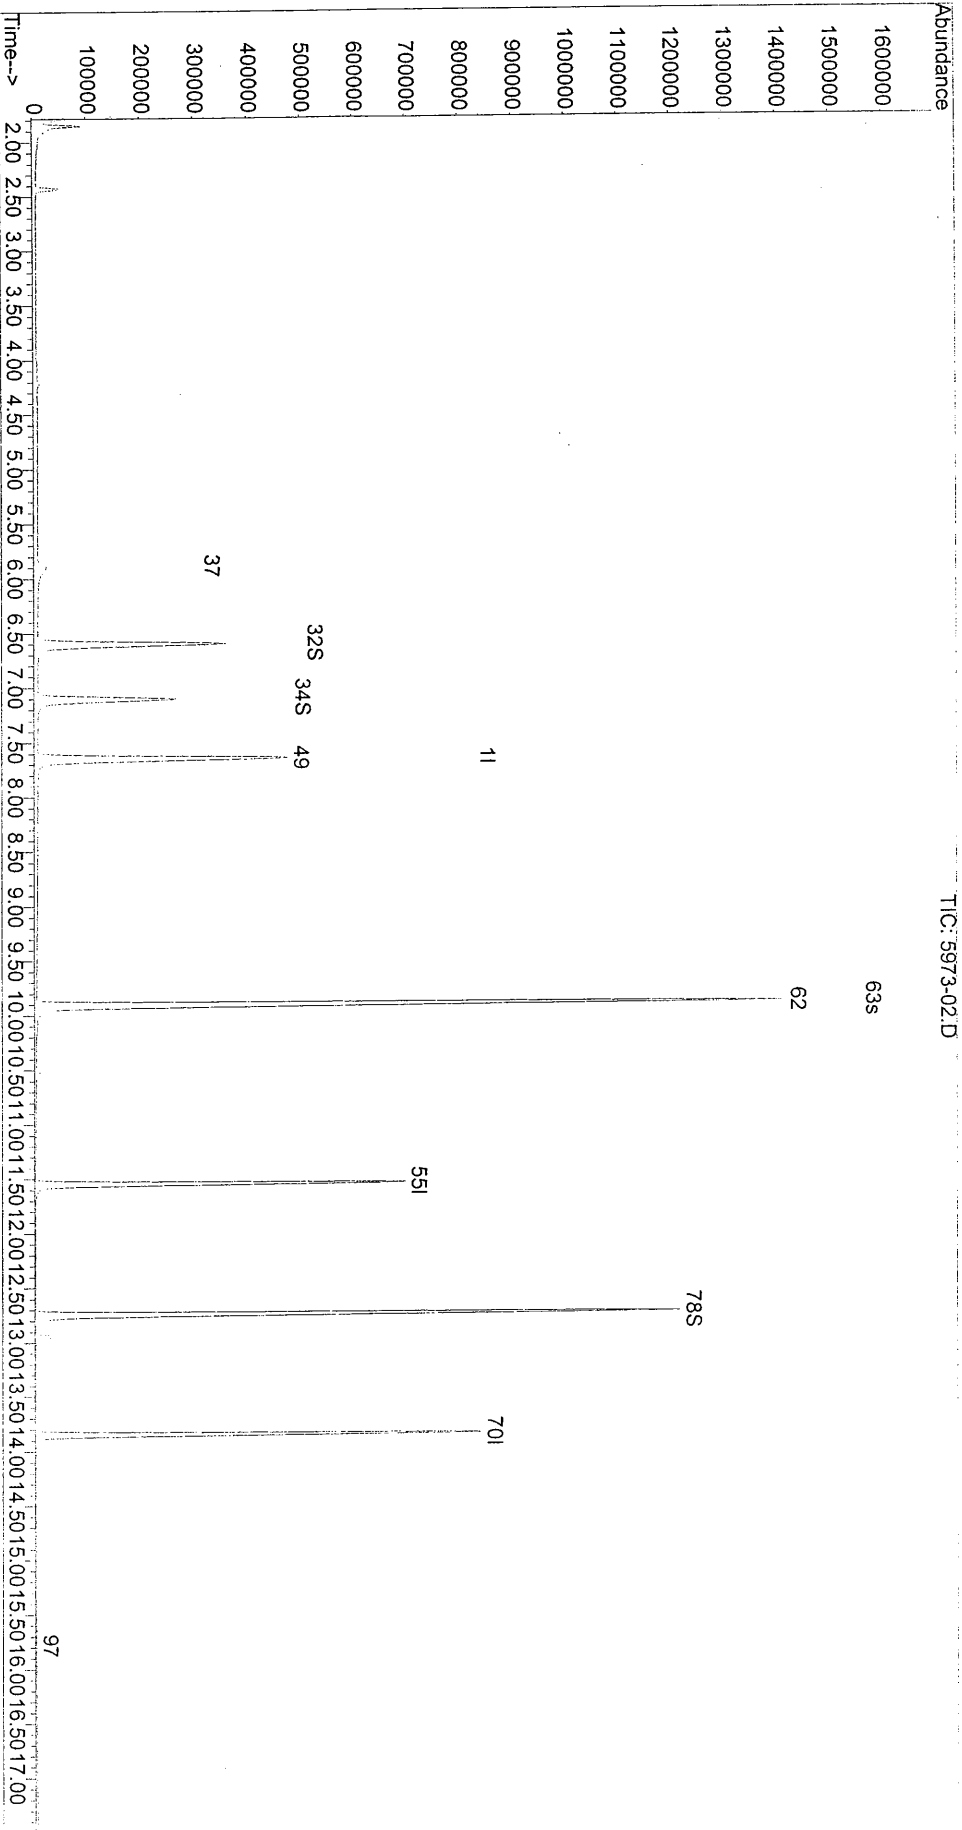

FORM-4A

Applied P & Ch Laboratory


Method Blank Summary for Method 524.2

| | | |
|---------------------------------|--------------------------|-------------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 35951 |
| Project ID: JPL | Project No: 04-4428.10 | Analysis Date: 11/06/03 |
| Sample ID: 03G4717-MB-01 | Sample Matrix: Water | Analysis Time: 13:54 |
| Lab Sample ID: 03G4717-MB-01 | Batch No: 03G4717 | Instrument ID: GC/MS: A |
| | Data File Name: G4717K01 | GC Column: HP-VOC |
| | Heated Purge: (Y/N) N | Column ID: 0.20 mm |

This Method Blank applies to the following samples and QC samples:

| # | Client Sample No | Lab Sample ID | Sample Type | Data Filename | Analysis Date | Analysis Time |
|----|------------------|----------------|------------------------|---------------|---------------|---------------|
| 1 | 03G4717-LCS-01 | 03G4717-LCS-01 | Lab Control Spike | G4717L01 | 11/06/03 | 10:53 |
| 2 | MW-3-1MS | 03-5973-2MS | Matrix Spike | G4717M01 | 11/06/03 | 11:19 |
| 3 | MW-3-1MSD | 03-5973-2MSD | Matrix Spike Duplicate | G4717N01 | 11/06/03 | 11:44 |
| 4 | TB-9-11-4-03 | 03-5951-13 | Field Sample | 5951-13 | 11/06/03 | 14:20 |
| 5 | DUPE-5-4-Q03 | 03-5951-1 | Field Sample | 5951-01 | 11/06/03 | 16:30 |
| 6 | EB-9-11-4-03 | 03-5951-2 | Field Sample | 5951-02 | 11/06/03 | 16:57 |
| 7 | MW-14-1 | 03-5951-3 | Field Sample | 5951-03 | 11/06/03 | 17:23 |
| 8 | MW-14-2 | 03-5951-4 | Field Sample | 5951-04 | 11/06/03 | 17:49 |
| 9 | MW-14-3 | 03-5951-5 | Field Sample | 5951-05 | 11/06/03 | 18:15 |
| 10 | MW-14-4 | 03-5951-6 | Field Sample | 5951-06 | 11/06/03 | 18:41 |
| 11 | MW-14-5 | 03-5951-7 | Field Sample | 5951-07 | 11/06/03 | 19:07 |
| 12 | MW-17-1 | 03-5951-8 | Field Sample | 5951-08 | 11/06/03 | 19:33 |
| 13 | MW-17-2 | 03-5951-9 | Field Sample | 5951-09 | 11/06/03 | 19:59 |
| 14 | MW-17-3 | 03-5951-10 | Field Sample | 5951-10 | 11/06/03 | 20:25 |
| 15 | MW-17-4 | 03-5951-11 | Field Sample | 5951-11 | 11/06/03 | 20:51 |
| 16 | MW-17-5 | 03-5951-12 | Field Sample | 5951-12 | 11/06/03 | 21:17 |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

Data File : C:\MSDCHEM\1\DATA\03G4612\G4612P01.D Vial: 1
 Acq On : 21 Oct 2003 9:14 am Operator: zou
 Sample : ##03g4565,w 50ng Inst : GCMS-A
 Misc : Multiplr: 1.00
 MS Integration Params: Lscint.p
 Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
 Title : **Applied P &h Lab** EPA 524.2

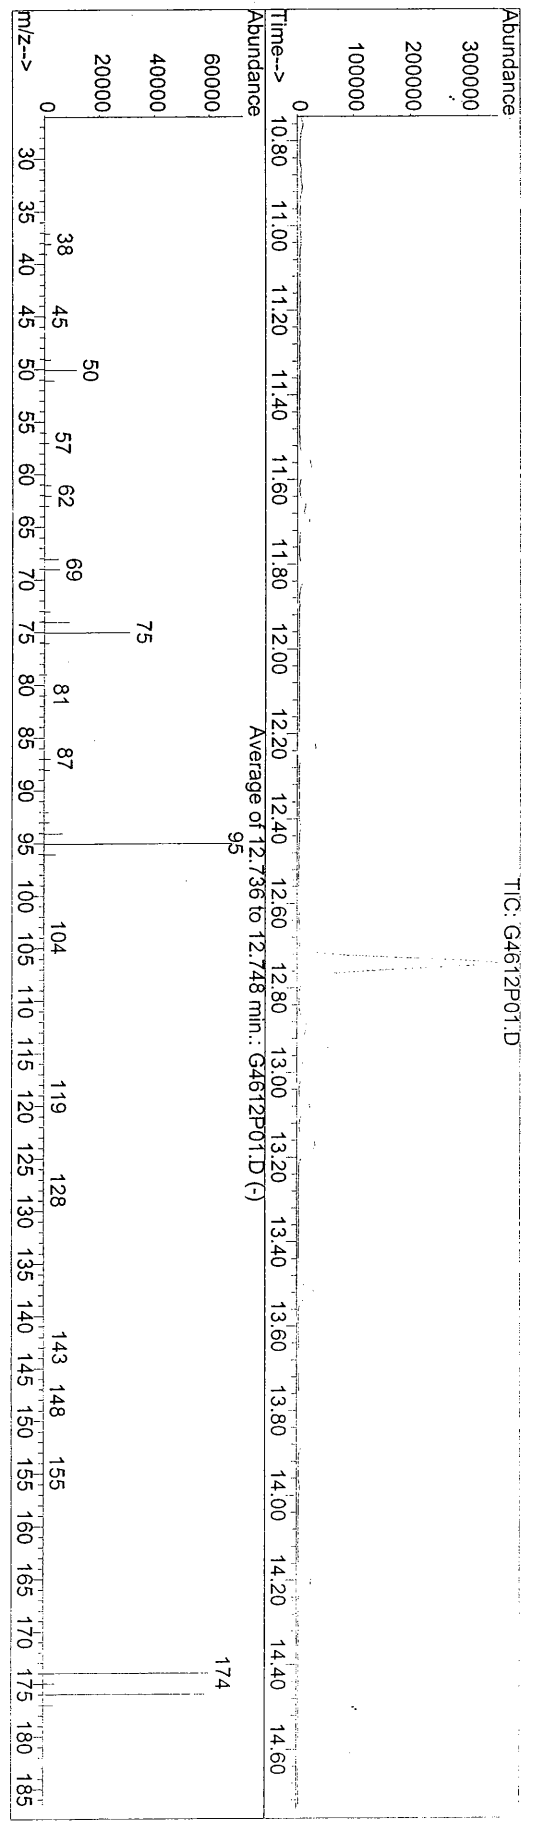

Spectrum Information: Average of 12.736 to 12.748 min.

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result |
|-------------|--------------|--------------|--------------|-----------|---------|--------|
| 50 | 95 | 15 | 40 | 17.0 | 11745 | PASS |
| 75 | 95 | 30 | 60 | 45.0 | 31162 | PASS |
| 95 | 95 | 100 | 100 | 100.0 | 69181 | PASS |
| 96 | 95 | 5 | 9 | 6.6 | 4558 | PASS |
| 173 | 174 | 0.00 | 2 | 0.5 | 275 | PASS |
| 174 | 95 | 50 | 100 | 87.4 | 60456 | PASS |
| 175 | 174 | 5 | 9 | 7.7 | 4634 | PASS |
| 176 | 174 | 95 | 101 | 98.1 | 59312 | PASS |
| 177 | 176 | 5 | 9 | 7.0 | 4135 | PASS |

5A
VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name : APPLIED P & CH LAB Contract: _____
 Lab Code: _____ Case No.: _____ SAS No.: _____ SDG No.: 035951
 Lab File ID: G 4612 P01 BFB Injection Date: 10/21/2003
 Instrument ID: GCMS-A BFB Injection Time: 0914
 GC Column: HP-VOC ID: 0.20 (mm) Heated Purge: (Y/N) N

| m/e | ION ABUNDANCE CRITERIA | %RELATIVE ABUNDANCE |
|-----|------------------------------------|---------------------|
| 50 | 15.0 - 40.0% of mass 95 | 17.0 |
| 75 | 30.0 - 60.0% of mass 95 | 45.0 |
| 95 | Base peak, 100% relative abundance | 100.0 |
| 96 | 5.0 - 9.0% of mass 95 | 6.6 |
| 173 | Less than 2.0% of mass 174 | 0.4 (0.5)1 |
| 174 | 50.0 - 100.0% of mass 95 | 87.4 |
| 175 | 5.0 - 9.0% of mass 174 | 6.7 (7.7)1 |
| 176 | 95.0 - 101.0% of mass 174 | 85.7 (98.1)1 |
| 177 | 5.0 - 9.0% of mass 176 | 6.0 (7.0)2 |

1-Value is % mass 174

2-Value is % mass 176

This check applies to the following SAMPLES, MS, MSD, BLANKS and STANDARDS:

| | EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|----------------|---------------|-------------|---------------|---------------|
| 01 | VSTD0003 | 3-A0003 | 3-A0003.D | 10/21/2003 | 1005 |
| 02 | VSTD002 | 3-0002 | 3-0002.D | 10/21/2003 | 1031 |
| 03 | VSTD010 | 3-0010 | 3-0010.D | 10/21/2003 | 1056 |
| 04 | VSTD020 | 3-0020 | 3-0020.D | 10/21/2003 | 1122 |
| 05 | VSTD040 | 3-0040 | 3-0040.D | 10/21/2003 | 1147 |
| 06 | VSTD060 | 3-0060 | 3-0060.D | 10/21/2003 | 1214 |
| 07 | | | | | |
| 08 | | | | | |
| 09 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

INITIAL CALIBRATION SUMMARY

Method File e524a003
 Last Calibration Update Mon Oct 27 13:56:31 2003
 Level 1 File Name 3-A0003.D Level 1 ID 3
 Level 2 File Name 3-002.D Level 2 ID 2
 Level 3 File Name 3-0010.D Level 3 ID 10
 Level 4 File Name 3-0020.D Level 4 ID 20
 Level 5 File Name 3-0040.D Level 5 ID 40
 Level 6 File Name 3-0060.D Level 6 ID 60
 Level 7 File Name 3-0020.D Level 7 ID CC

| Compound Name | Level 1 Response | Level 2 Response | Level 3 Response | Level 4 Response | Level 5 Response | Level 6 Response | Level 7 Response | Coeff X ⁰ | Coeff X ⁻¹ / ave RF | Coeff X ² | R ² / RSD |
|--------------------------|------------------|------------------|------------------|------------------|------------------|------------------|------------------|----------------------|--------------------------------|----------------------|----------------------|
| 1 Fluorobenzene | 920067 | 916201 | 919392 | 955116 | 907151 | 1006211 | -1 | ----- | ----- | ----- | ----- |
| 3 di-Cl-di-F-methane | 6437 | 39097 | 199979 | 303885 | 731076 | 1099511 | -1 | 0.0000 | 0.2011 | 0.0000 | 0.1330 |
| 4 Chloromethane | 6136 | 37417 | 181676 | 348991 | 739859 | 1132557 | -1 | 0.0000 | 0.1997 | 0.0000 | 0.0704 |
| 2 F114 | 1527 | 19306 | 101058 | 155932 | 367886 | 551592 | -1 | 0.0028 | 0.0932 | 0.0000 | 0.9919 |
| 5 vinyl chloride | 4876 | 33446 | 161213 | 285451 | 640709 | 982033 | -1 | 0.0000 | 0.1705 | 0.0000 | 0.0717 |
| 6 bromomethane | 2539 | 18408 | 87613 | 168214 | 383891 | 601141 | -1 | 0.0000 | 0.0969 | 0.0000 | 0.0659 |
| 7 chloroethane | 2197 | 17752 | 90280 | 159905 | 376464 | 536590 | -1 | 0.0000 | 0.0918 | 0.0000 | 0.1013 |
| 8 tri-Cl-F-methane | 8394 | 56082 | 277768 | 461283 | 1030751 | 1532166 | -1 | 0.0000 | 0.2819 | 0.0000 | 0.0992 |
| 91 Acetonitrile X10 | 10689 | 82041 | 382813 | 794170 | 1713507 | 2428244 | -1 | 0.0000 | 0.0431 | 0.0000 | 0.0662 |
| 9 acrolein X10 | 5645 | 40130 | 201945 | 381523 | 807796 | 1232252 | -1 | 0.0000 | 0.0212 | 0.0000 | 0.0467 |
| 11 acetone X10 | -1 | 64324 | 288996 | 538495 | 1267205 | 1816586 | -1 | 0.0000 | 0.0319 | 0.0000 | 0.0947 |
| 12 ethyl ether X5 | 13693 | 93915 | 436367 | 874255 | 1704647 | 2654028 | -1 | 0.0000 | 0.0950 | 0.0000 | 0.0552 |
| 13 11-dichloroethene | 6637 | 46215 | 229524 | 410040 | 877445 | 1367991 | -1 | 0.0000 | 0.2376 | 0.0000 | 0.0605 |
| 14 iodomethane | 3461 | 29384 | 183879 | 356970 | 751141 | 1123042 | -1 | 0.0038 | 0.1913 | 0.0000 | 0.9951 |
| 15 F-113 | 4492 | 28088 | 146108 | 224035 | 516639 | 784890 | -1 | 0.0000 | 0.1441 | 0.0000 | 0.1231 |
| 16 acrylonitrile X10 | 10574 | 78358 | 419836 | 794346 | 1709905 | 2532493 | -1 | 0.0000 | 0.0429 | 0.0000 | 0.0731 |
| 17 carbon disulfide | 13839 | 85463 | 420250 | 772812 | 1671671 | 2561651 | -1 | 0.0000 | 0.4524 | 0.0000 | 0.0750 |
| 94 Isopropyl AlcoholX10 | 331 | 1284 | 1238 | 28714 | 240070 | 128634 | -1 | 0.0000 | 0.0020 | 0.0000 | 1.1427 |
| 18 methylene chloride | 10278 | 48191 | 203033 | 407143 | 804880 | 1192483 | -1 | 0.0203 | 0.2012 | 0.0000 | 0.9947 |
| 19 t-12-di-Cl-ethene | 6615 | 45733 | 217854 | 407874 | 774111 | 1126298 | -1 | 0.0000 | 0.2233 | 0.0000 | 0.1039 |
| 20 t-Bu-Me-ether | 9529 | 70095 | 362056 | 751228 | 1592599 | 2437498 | -1 | 0.0000 | 0.3929 | 0.0000 | 0.0773 |
| 95 Tert butyl alcoholX10 | 1332 | 4624 | 88338 | 76985 | 452680 | 251872 | -1 | 0.0000 | 0.0066 | 0.0000 | 0.6496 |

| | | | | | | | | | | | |
|-------------------------|-------|--------|---------|---------|---------|----------|----|--------|--------|--------|--------|
| 94 allyl chloride | 10689 | 82041 | 426268 | 794170 | 1724483 | 2428244 | -1 | 0.0000 | 0.4409 | 0.0000 | 0.0706 |
| 21 11-dichloroethane | 10035 | 71189 | 342138 | 689918 | 1398310 | 2101878 | -1 | 0.0000 | 0.3698 | 0.0000 | 0.0415 |
| 97 propionitrile | 103 | 3119 | 18745 | 29270 | 62391 | 109975 | -1 | 0.0000 | 0.0176 | 0.0000 | 0.1055 |
| 22 c-12-di-Cl-ethene | 6459 | 46844 | 225560 | 436935 | 845644 | 1210430 | -1 | 0.0000 | 0.2329 | 0.0000 | 0.0801 |
| 23 22-Dichloropropane | 5693 | 38859 | 218612 | 456844 | 979998 | 1513030 | -1 | 0.0000 | 0.2360 | 0.0000 | 0.1011 |
| 24 Br-Cl-methane | 3294 | 23046 | 109590 | 215148 | 438926 | 655419 | -1 | 0.0000 | 0.1177 | 0.0000 | 0.0523 |
| 25 chloroform | 13164 | 80631 | 375460 | 741683 | 1492648 | 2229387 | -1 | 0.0000 | 0.4157 | 0.0000 | 0.0920 |
| 26 tetrahydrofuranX5 | 4044 | 28808 | 169729 | 317711 | 726346 | 1114014 | -1 | 0.0000 | 0.0346 | 0.0000 | 0.1155 |
| 98 Diisopropyl ether | 16931 | 136442 | 688556 | 1387177 | 2723439 | 4088155 | -1 | 0.0000 | 0.7101 | 0.0000 | 0.0772 |
| 27 Di-Br-F-Me (surr) | 6137 | 45047 | 218874 | 439096 | 880145 | 1314263 | -1 | 0.0000 | 0.2348 | 0.0000 | 0.0481 |
| 99 ETBE | 9591 | 74005 | 411030 | 879689 | 1934215 | 2984281 | -1 | 0.0000 | 0.4477 | 0.0000 | 0.1468 |
| 29 1,2-Di-Cl-Et-d4 (S1) | 5167 | 39287 | 192209 | 385356 | 801084 | 1206050 | -1 | 0.0000 | 0.2091 | 0.0000 | 0.0418 |
| 30 12-dichloroethane | 2318 | 14864 | 77221 | 146461 | 303955 | 463659 | -1 | 0.0000 | 0.0811 | 0.0000 | 0.0434 |
| 32 vinyl acetate X5 | 36279 | 291623 | 1683396 | 3463521 | 7301957 | 11062661 | -1 | 0.0000 | 0.3465 | 0.0000 | 0.1412 |
| 92 Nitro Methane(X10) | 1574 | 10571 | 358371 | 95786 | 134103 | 298076 | -1 | 0.0000 | 0.0117 | 0.0000 | 1.3083 |
| 33 2-butanone/MEK X10 | 14739 | 98541 | 459782 | 956754 | 2014463 | 3034414 | -1 | 0.0000 | 0.0522 | 0.0000 | 0.0453 |
| 93 Ethyl Acetate x2 | 6463 | 37342 | 237607 | 465630 | 1199719 | 1687653 | -1 | 0.0000 | 0.1292 | 0.0000 | 0.1682 |
| 34 111-trichloroethane | 9393 | 63933 | 333945 | 629233 | 1352461 | 2070811 | -1 | 0.0000 | 0.3496 | 0.0000 | 0.0454 |
| 35 11-Di-Cl-propene | 6749 | 49362 | 260487 | 484228 | 1020849 | 1516179 | -1 | 0.0000 | 0.2639 | 0.0000 | 0.0625 |
| 36 benzene | 23536 | 167998 | 811668 | 1581767 | 3067808 | 4519766 | -1 | 0.0000 | 0.8457 | 0.0000 | 0.0673 |
| 37 CCl4 | 9052 | 59763 | 312695 | 555550 | 1228562 | 1842053 | -1 | 0.0000 | 0.3215 | 0.0000 | 0.0608 |

| Compound Name | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | Level 7 | Coeff X^0 | Coeff X^1 / ave RF | Coeff X^2 | R^2 / RSD |
|--------------------------|----------|----------|----------|----------|----------|----------|----------|-----------|--------------------|-----------|-----------|
| | Response | Response | Response | Response | Response | Response | Response | | | | |
| 100 Isobutyl alcoholX10 | 2932 | 21047 | 112031 | 247109 | 552842 | 880424 | -1 | ----- | ----- | ----- | ----- |
| 38 thiophene | 10222 | 83170 | 428533 | 868274 | 1718044 | 2554816 | -1 | 0.0000 | 0.4403 | 0.0000 | 0.0870 |
| 39 12-di-Cl-propane | 4815 | 37555 | 178169 | 370946 | 752605 | 1124998 | -1 | 0.0000 | 0.1935 | 0.0000 | 0.0628 |
| 40 trichloroethene | 7696 | 50098 | 255616 | 501517 | 1020048 | 1520360 | -1 | 0.0000 | 0.2710 | 0.0000 | 0.0423 |
| 41 dibromomethane | 3770 | 26033 | 124373 | 247759 | 508912 | 747601 | -1 | 0.0000 | 0.1346 | 0.0000 | 0.0506 |
| 101 TAME | 7879 | 59032 | 335735 | 716981 | 1622049 | 2525816 | -1 | -0.0345 | 0.4304 | 0.0000 | 0.9963 |
| 42 Br-di-Cl-methane | 9392 | 56733 | 274489 | 546104 | 1129675 | 1703118 | -1 | 0.0000 | 0.3046 | 0.0000 | 0.0694 |
| 43 Me-methacrylate | 1457 | 14747 | 87065 | 188318 | 435160 | 662734 | -1 | -0.0095 | 0.1138 | 0.0000 | 0.9946 |
| 44 2-ClEt-Vi-ether10 | 4887 | 45249 | 275793 | 591932 | 1294105 | 1950851 | -1 | -0.0367 | 0.0357 | 0.0000 | 0.9955 |
| 45 c-13-di-Cl-propene | 6769 | 54923 | 293425 | 608486 | 1252896 | 1891415 | -1 | 0.0000 | 0.3069 | 0.0000 | 0.1096 |
| 46 t-1,3-dichloropropene | 5153 | 40425 | 231011 | 505285 | 1067475 | 1638452 | -1 | -0.0097 | 0.2792 | 0.0000 | 0.9968 |
| 47 Chlorobenzene-d5 | 745928 | 732691 | 724575 | 731811 | 659336 | 705610 | -1 | 0.0000 | 1.0000 | 0.0000 | 0.0000 |

| Compound Name | Level 1 | | Level 2 | | Level 3 | | Level 4 | | Level 5 | | Level 6 | | Level 7 | | Coeff Xv0 | Coeff Xv1 / ave RF | Coeff Xv2 | Rv2 / RSD |
|----------------------------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|-----------|--------------------|-----------|-----------|
| | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | | | | |
| 48 112-tri-Cl-Et | 4896 | 31570 | 158039 | 308164 | 644393 | 936372 | -1 | 0.0000 | 0.2214 | 0.0000 | 0.0533 | | | | | | | |
| 49 13-di-Cl-propane | 7569 | 48826 | 251096 | 479955 | 958048 | 1392110 | -1 | 0.0000 | 0.3397 | 0.0000 | 0.0396 | | | | | | | |
| 50 Et methacrylate | 2785 | 29334 | 189197 | 404574 | 897662 | 1374874 | -1 | -0.0430 | 0.3345 | 0.0000 | 0.9960 | | | | | | | |
| 51 di-Br-Cl-methane | 7359 | 44728 | 219307 | 430191 | 895491 | 1332246 | -1 | 0.0000 | 0.3141 | 0.0000 | 0.0548 | | | | | | | |
| 52 bromoform | 4029 | 26611 | 127022 | 257402 | 537161 | 813031 | -1 | 0.0000 | 0.1848 | 0.0000 | 0.0599 | | | | | | | |
| 53 1,4-dichlorobutane-2 | 7248 | 52525 | 270048 | 530472 | 1118631 | 1708578 | -1 | 0.0000 | 0.3742 | 0.0000 | 0.0947 | | | | | | | |
| 54 MIBK | 2727 | 20267 | 114402 | 244409 | 567049 | 883730 | -1 | -0.0334 | 0.2144 | 0.0000 | 0.9947 | | | | | | | |
| 55 toluene-d8 | 22176 | 162055 | 811859 | 1597728 | 3175057 | 4699033 | -1 | 0.0000 | 1.1038 | 0.0000 | 0.0617 | | | | | | | |
| 56 toluene | 32453 | 204349 | 957684 | 1867212 | 3679239 | 5453434 | -1 | 0.0000 | 1.3542 | 0.0000 | 0.0513 | | | | | | | |
| 57 2-hexanone X5 | 8296 | 70148 | 400071 | 806303 | 1789801 | 2714840 | -1 | -0.0660 | 0.1318 | 0.0000 | 0.9958 | | | | | | | |
| 58 12-dibromoethane | 4393 | 32436 | 159989 | 322735 | 683020 | 1029927 | -1 | 0.0000 | 0.2269 | 0.0000 | 0.0954 | | | | | | | |
| 59 tetra-Cl-ethene | 8603 | 59173 | 281865 | 498130 | 1001817 | 1436032 | -1 | 0.0000 | 0.3728 | 0.0000 | 0.0719 | | | | | | | |
| 60 chlorobenzene | 21200 | 144953 | 676974 | 1307160 | 2492370 | 3536493 | -1 | 0.0000 | 0.9241 | 0.0000 | 0.0576 | | | | | | | |
| 61 1112-tetra-Cl-Et | 7365 | 51367 | 249086 | 487380 | 969491 | 1437439 | -1 | 0.0000 | 0.3439 | 0.0000 | 0.0403 | | | | | | | |
| 62 1,4-Dichlorobenzene-d4 | 436784 | 441685 | 431820 | 433290 | 398842 | 428493 | -1 | 0.0000 | 1.0000 | 0.0000 | 0.0000 | | | | | | | |
| 63 1-chlorohexane | 3125 | 20185 | 105292 | 181129 | 379300 | 546400 | -1 | 0.0000 | 0.2284 | 0.0000 | 0.0636 | | | | | | | |
| 64 Et-Bz | 31613 | 225200 | 1128701 | 2162672 | 4307205 | 6378701 | -1 | 0.0000 | 2.5420 | 0.0000 | 0.0404 | | | | | | | |
| 65 m/p-Xylenes X2 | 51588 | 364290 | 1753788 | 3322945 | 6407191 | 9314343 | -1 | 0.0000 | 1.9663 | 0.0000 | 0.0463 | | | | | | | |
| 66 styrene | 19899 | 158986 | 755749 | 1448349 | 2712603 | 3842415 | -1 | 0.0000 | 1.6558 | 0.0000 | 0.0748 | | | | | | | |
| 67 o-xylene | 25030 | 181225 | 888564 | 1715323 | 3289680 | 4761198 | -1 | 0.0000 | 1.9855 | 0.0000 | 0.0445 | | | | | | | |
| 68 1122-Tetra-Cl-Et | 4786 | 35408 | 176142 | 333638 | 679431 | 1005365 | -1 | 0.0000 | 0.3960 | 0.0000 | 0.0524 | | | | | | | |
| 69 123-tri-Cl-Pr | 1463 | 11857 | 58506 | 111098 | 231129 | 345542 | -1 | 0.0000 | 0.1315 | 0.0000 | 0.0844 | | | | | | | |
| 70 4-Br-1-F-Bz (S3) | 9236 | 60769 | 292727 | 571173 | 1114624 | 1638683 | -1 | 0.0000 | 0.6776 | 0.0000 | 0.0376 | | | | | | | |
| 71 isopropylbenzene | 31809 | 228075 | 1204677 | 2257352 | 4576796 | 6821750 | -1 | 0.0000 | 2.6544 | 0.0000 | 0.0592 | | | | | | | |
| 72 bromobenzene | 8279 | 62596 | 299551 | 577972 | 1123002 | 1610222 | -1 | 0.0000 | 0.6719 | 0.0000 | 0.0539 | | | | | | | |
| 92 t-1,4-dichloro-2-butene | 370 | 3850 | 26890 | 58909 | 138278 | 214154 | -1 | -0.0139 | 0.0860 | 0.0000 | 0.9950 | | | | | | | |
| 73 n-propylbenzene | 9091 | 70513 | 355352 | 656540 | 1290074 | 1877926 | -1 | 0.0000 | 0.7686 | 0.0000 | 0.0653 | | | | | | | |
| 74 2-Cl-Toluene | 7570 | 61543 | 297725 | 558317 | 1084812 | 1601091 | -1 | 0.0000 | 0.6518 | 0.0000 | 0.0707 | | | | | | | |
| 75 4-Cl-Toluene | 9182 | 64367 | 296683 | 566381 | 1062470 | 1497703 | -1 | 0.0000 | 0.6698 | 0.0000 | 0.0750 | | | | | | | |
| 76 135-tri-Me-Benzene | 28727 | 213694 | 1063069 | 2008540 | 3906361 | 5670674 | -1 | 0.0000 | 2.3409 | 0.0000 | 0.0517 | | | | | | | |
| 77 4-iso-Pr-toluene | 31720 | 226621 | 1149787 | 2111126 | 4215398 | 61774914 | -1 | 0.0000 | 2.5215 | 0.0000 | 0.0463 | | | | | | | |
| 78 124-tri-Me-Benzene | 29971 | 222021 | 1078747 | 2103275 | 4147713 | 6124395 | -1 | 0.0000 | 2.4513 | 0.0000 | 0.0448 | | | | | | | |
| 79 tert-butylbenzene | 24279 | 177466 | 929162 | 1736357 | 3598467 | 5289165 | -1 | 0.0000 | 2.0550 | 0.0000 | 0.0671 | | | | | | | |

| | | | | | | | | | | | |
|---------------------|-------|--------|---------|---------|---------|---------|----|---------|--------|--------|--------|
| 80 13-DCB | 19447 | 131664 | 611576 | 1176380 | 2227519 | 3166301 | -1 | 0.0000 | 1.3960 | 0.0000 | 0.0684 |
| 81 sec-butylbenzene | 38627 | 268975 | 1387531 | 2530666 | 5231475 | 7732088 | -1 | 0.0000 | 3.0688 | 0.0000 | 0.0475 |
| 82 14-DCB | 21754 | 133604 | 619366 | 1184125 | 2334471 | 3417867 | -1 | 0.0000 | 1.4610 | 0.0000 | 0.0806 |
| 83 Cl-benzyl | 871 | 5857 | 44122 | 106539 | 268318 | 431461 | -1 | -0.0412 | 0.1731 | 0.0000 | 0.9920 |
| 84 12-DCB | 17721 | 121367 | 559240 | 1055514 | 2046326 | 2953834 | -1 | 0.0000 | 1.2785 | 0.0000 | 0.0657 |
| 85 n-butylbenzene | 8164 | 59910 | 307483 | 567085 | 1127859 | 1596385 | -1 | 0.0000 | 0.6659 | 0.0000 | 0.0599 |
| 86 12-diBr-2-Cl-Pra | 1032 | 7477 | 40003 | 83208 | 177685 | 276212 | -1 | 0.0000 | 0.0951 | 0.0000 | 0.1330 |
| 87 124-tri-Cl-Bz | 9169 | 66792 | 354819 | 702123 | 1402301 | 2085639 | -1 | 0.0000 | 0.7963 | 0.0000 | 0.0771 |
| 88 naphthalene | 11079 | 87277 | 545491 | 1159824 | 2506296 | 3927146 | -1 | -0.1762 | 1.5623 | 0.0000 | 0.9976 |
| 89 hx-Cl-butadiene | 6445 | 40287 | 205532 | 360400 | 746186 | 1096494 | -1 | 0.0000 | 0.4557 | 0.0000 | 0.0644 |
| 90 123-Tri-Cl-Bz | 7754 | 57941 | 307963 | 600915 | 1229181 | 1798500 | -1 | 0.0000 | 0.6874 | 0.0000 | 0.0870 |

1671



Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
Title : **Applied P & Ch Lab** EPA 524.2
Last Update : Mon Oct 27 13:56:31 2003
Response via : Initial Calibration

Calibration Files
.3 =3-A0003.D 2 =3-002.D 10 =3-0010.D
20 =3-0020.D 40 =3-0040.D 60 =3-0060.D

| Compound | .3 | 2 | 10 | 20 | 40 | 60 | Avg | %RSD | | |
|------------|--------------|---------------|-------|-------|-------|-------|-------|-------|--------|-------|
| 1) I | 1 | Fluorobenzene | 0.233 | 0.213 | 0.218 | 0.159 | 0.201 | 0.182 | 0.201 | 13.30 |
| 2) 3 | di-Cl-di-F-m | 0.222 | 0.204 | 0.198 | 0.183 | 0.204 | 0.188 | 0.200 | 7.04 | |
| 3) P | 4 | Chloromethan | 0.055 | 0.105 | 0.110 | 0.082 | 0.101 | 0.091 | 0.091 | 22.20 |
| 4) 2 | F114 | 0.177 | 0.183 | 0.175 | 0.149 | 0.177 | 0.163 | 0.171 | 7.17 | |
| 5) C | 5 | vinyl chlori | 0.092 | 0.100 | 0.095 | 0.088 | 0.106 | 0.100 | 0.097 | 6.59 |
| 6) 6 | bromomethane | 0.080 | 0.097 | 0.098 | 0.084 | 0.104 | 0.089 | 0.092 | 10.13 | |
| 7) 7 | chloroethane | 0.304 | 0.306 | 0.302 | 0.241 | 0.284 | 0.254 | 0.282 | 9.92 | |
| 8) 8 | tri-Cl-F-met | 0.020 | 0.022 | 0.022 | 0.020 | 0.022 | 0.020 | 0.021 | 4.67 | |
| 9) 9 | Acetonitrile | 0.035 | 0.031 | 0.028 | 0.035 | 0.030 | 0.032 | 9.47 | | |
| 10) 9 | acrolein | 0.099 | 0.103 | 0.095 | 0.092 | 0.094 | 0.088 | 0.095 | 5.52 | |
| 11) 11 | acetone | 0.240 | 0.252 | 0.250 | 0.215 | 0.242 | 0.227 | 0.238 | 6.05# | |
| 12) 12 | ethyl ether | 0.125 | 0.160 | 0.200 | 0.187 | 0.207 | 0.186 | 0.178 | 16.98 | |
| 13) M, C13 | 11-dichloroe | 0.163 | 0.153 | 0.159 | 0.117 | 0.142 | 0.130 | 0.144 | 12.31 | |
| 14) 14 | Iodomethane | 0.038 | 0.043 | 0.046 | 0.042 | 0.047 | 0.042 | 0.043 | 7.31 | |
| 15) 15 | F-113 | 0.501 | 0.466 | 0.457 | 0.405 | 0.461 | 0.424 | 0.452 | 7.50 | |
| 16) 16 | acrylonitril | 0.001 | 0.001 | 0.000 | 0.002 | 0.007 | 0.002 | 0.002 | 114.27 | |
| 17) 17 | carbon disul | 0.372 | 0.263 | 0.221 | 0.213 | 0.222 | 0.198 | 0.248 | 26.04 | |
| 18) 18 | Isopropyl Al | 0.240 | 0.250 | 0.237 | 0.214 | 0.213 | 0.187 | 0.223 | 10.39 | |
| 19) 19 | methylene ch | 0.345 | 0.383 | 0.394 | 0.393 | 0.439 | 0.404 | 0.393 | 7.73 | |
| 20) 20 | t-12-di-Cl-e | 0.003 | 0.010 | 0.004 | 0.012 | 0.004 | 0.004 | 0.007 | 64.96 | |
| 21) 21 | t-Bu-Me-ethe | 0.448 | 0.464 | 0.464 | 0.416 | 0.475 | 0.402 | 0.441 | 7.06 | |
| 22) 22 | Tert butyl a | 0.364 | 0.389 | 0.372 | 0.361 | 0.385 | 0.348 | 0.370 | 4.15 | |
| 23) 23 | allyl chlori | 0.017 | 0.020 | 0.015 | 0.017 | 0.018 | 0.018 | 0.018 | 10.55 | |
| 24) P | 11-dichloroe | 0.234 | 0.256 | 0.245 | 0.229 | 0.233 | 0.200 | 0.233 | 8.01 | |
| 25) 25 | propionitril | 0.206 | 0.212 | 0.238 | 0.239 | 0.270 | 0.251 | 0.236 | 10.11 | |
| 26) 26 | c-12-di-Cl-e | 0.119 | 0.126 | 0.119 | 0.113 | 0.121 | 0.109 | 0.118 | 5.23 | |
| 27) 27 | 22-Dichlorop | | | | | | | | | |
| 28) 28 | Br-Cl-methan | | | | | | | | | |

Handwritten mark resembling a checkmark or '2'.

0.995

0.995

0.990

(#) = Out of Range
E524A003.M

Mon Oct 27 13:57:06 2003

Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Mon Oct 27 13:56:31 2003
 Response via : Initial Calibration

Calibration Files
 .3 =3-A0003.D 2 =3-002.D 10 =3-0010.D
 20 =3-0020.D 40 =3-0040.D 60 =3-0060.D

| Compound | .3 | 2 | 10 | 20 | 40 | 60 | Avg | %RSD |
|--------------------------|-------|-------|-------|-------|-------|-------|-------|--------|
| 29) C 25 chloroform | 0.477 | 0.440 | 0.408 | 0.388 | 0.411 | 0.369 | 0.416 | 9.20 |
| 30) 26 tetrahydrofu | 0.029 | 0.031 | 0.037 | 0.033 | 0.040 | 0.037 | 0.035 | 11.55 |
| 31) 98 Diisopropyl | 0.613 | 0.745 | 0.749 | 0.726 | 0.751 | 0.677 | 0.710 | 7.72 |
| 32) S 27 Di-Br-F-Me (| 0.246 | 0.238 | 0.230 | 0.243 | 0.218 | 0.235 | 0.235 | 4.81 |
| 33) 99 ETBE | 0.347 | 0.404 | 0.447 | 0.461 | 0.533 | 0.494 | 0.448 | 14.68 |
| 34) S 29 1,2-Di-Cl-Et | 0.214 | 0.209 | 0.202 | 0.221 | 0.200 | 0.209 | 0.209 | 4.18 |
| 35) 30 12-dichloroe | 0.084 | 0.081 | 0.084 | 0.077 | 0.084 | 0.077 | 0.081 | 4.34 |
| 36) 32 vinyl acetat | 0.263 | 0.318 | 0.366 | 0.363 | 0.402 | 0.366 | 0.346 | 14.12 |
| 37) 92 Nitro Methan | 0.006 | 0.039 | 0.005 | 0.004 | 0.004 | 0.005 | 0.012 | 130.83 |
| 38) 33 2-butanoneME | 0.053 | 0.054 | 0.050 | 0.050 | 0.056 | 0.050 | 0.052 | 4.53 |
| 39) 93 Ethyl Acetat | 0.117 | 0.102 | 0.129 | 0.122 | 0.165 | 0.140 | 0.129 | 16.82 |
| 40) 34 111-trichlor | 0.340 | 0.349 | 0.363 | 0.329 | 0.373 | 0.343 | 0.350 | 4.54 |
| 41) 35 11-Di-Cl-pro | 0.245 | 0.269 | 0.283 | 0.253 | 0.281 | 0.251 | 0.264 | 6.25 |
| 42) M 36 benzene | 0.853 | 0.917 | 0.883 | 0.828 | 0.845 | 0.749 | 0.846 | 6.73 |
| 43) 37 CCl4 | 0.328 | 0.326 | 0.340 | 0.291 | 0.339 | 0.305 | 0.321 | 6.08 |
| 44) 100 Isobutyl al | 0.011 | 0.011 | 0.012 | 0.013 | 0.015 | 0.015 | 0.013 | 13.92 |
| 45) 38 thiophene | 0.370 | 0.454 | 0.466 | 0.455 | 0.473 | 0.423 | 0.440 | 8.70 |
| 46) C 39 12-di-Cl-pro | 0.174 | 0.205 | 0.194 | 0.194 | 0.207 | 0.186 | 0.194 | 6.28# |
| 47) M 40 trichloroeth | 0.279 | 0.273 | 0.278 | 0.263 | 0.281 | 0.252 | 0.271 | 4.23 |
| 48) 41 dibromometha | 0.137 | 0.142 | 0.135 | 0.130 | 0.140 | 0.124 | 0.135 | 5.06 |
| 49) 101 TAME | 0.285 | 0.322 | 0.365 | 0.375 | 0.447 | 0.418 | 0.369 | 16.15 |
| 50) 42 Br-di-Cl-met | 0.340 | 0.310 | 0.299 | 0.286 | 0.311 | 0.282 | 0.305 | 6.94 |
| 51) 43 Me-methacryl | 0.053 | 0.080 | 0.095 | 0.099 | 0.120 | 0.110 | 0.093 | 25.59 |
| 52) 44 2-ClEt-Vi-et | 0.018 | 0.025 | 0.030 | 0.031 | 0.036 | | 0.028 | 24.68 |
| 53) 45 C-13-di-Cl-p | 0.245 | 0.300 | 0.319 | 0.319 | 0.345 | 0.313 | 0.307 | 10.96 |
| 54) 46 t-1,3-dichlo | 0.187 | 0.221 | 0.251 | 0.265 | 0.294 | 0.271 | 0.248 | 15.58 |
| 55) I 47 Chlorobezene-d5 | 0.219 | 0.215 | 0.218 | 0.211 | 0.244 | 0.221 | 0.221 | 5.33 |
| 56) 48 112-tri-Cl-E | | | | | | | | |

0.994
 0.994
 0.994
 0.994

(#) = Out of Range
 E524A003.M Mon Oct 27 13:57:07 2003



Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
Title : **Applied P &ch Lab** EPA 524.2
Last Update : Mon Oct 27 13:56:31 2003
Response via : Initial Calibration

Calibration Files
.3 =3-A0003.D 2 =3-002.D 10 =3-0010.D
20 =3-0020.D 40 =3-0040.D 60 =3-0060.D

| Compound | .3 | 2 | 10 | 20 | 40 | 60 | Avg | %RSD |
|-----------------------------|----------------|-------|-------|-------|-------|-------|-------|-------|
| 57) 49 13-di-Cl-pro | 0.338 | 0.333 | 0.347 | 0.328 | 0.363 | 0.329 | 0.340 | 3.96 |
| 58) 50 Et methacryl | 0.124 | 0.200 | 0.261 | 0.276 | 0.340 | 0.325 | 0.255 | 31.77 |
| 59) 51 di-Br-Cl-met | 0.329 | 0.305 | 0.303 | 0.294 | 0.340 | 0.315 | 0.314 | 5.48 |
| 60) P 52 bromoform | 0.180 | 0.182 | 0.175 | 0.176 | 0.204 | 0.192 | 0.185 | 5.99 |
| 61) 53 1,4-dichloro | 0.324 | 0.358 | 0.373 | 0.362 | 0.424 | 0.404 | 0.374 | 9.47 |
| 62) 54 MIBK | 0.122 | 0.138 | 0.158 | 0.167 | 0.215 | 0.209 | 0.168 | 22.23 |
| 63) s 55 toluene-d8 | 0.991 | 1.106 | 1.120 | 1.092 | 1.204 | 1.110 | 1.104 | 6.17 |
| 64) M,C 56 toluene | 1.450 | 1.395 | 1.322 | 1.276 | 1.395 | 1.288 | 1.354 | 5.13 |
| 65) 57 2-hexanone X | 0.074 | 0.096 | 0.110 | 0.110 | 0.136 | 0.128 | 0.109 | 20.41 |
| 66) 58 12-dibromoet | 0.196 | 0.221 | 0.221 | 0.221 | 0.259 | 0.243 | 0.227 | 9.54 |
| 67) 59 tetra-Cl-eth | 0.384 | 0.404 | 0.389 | 0.340 | 0.380 | 0.339 | 0.373 | 7.19 |
| 68) M,P 60 chlorobenzen | 0.947 | 0.989 | 0.934 | 0.893 | 0.945 | 0.835 | 0.924 | 5.76 |
| 69) 61 1112-tetra-C | 0.329 | 0.351 | 0.344 | 0.333 | 0.368 | 0.340 | 0.344 | 4.03 |
| 70) I 62 1,4-Dichlorobenzen | -----ISTD----- | | | | | | | |
| 71) 63 1-chlorohexa | 0.238 | 0.228 | 0.244 | 0.209 | 0.238 | 0.213 | 0.228 | 6.36 |
| 72) C 64 Et-Bz | 2.413 | 2.549 | 2.614 | 2.496 | 2.700 | 2.481 | 2.542 | 4.04# |
| 73) 65 m/p-Xylenes | 1.968 | 2.062 | 2.031 | 1.917 | 2.008 | 1.811 | 1.966 | 4.63 |
| 74) 66 styrene | 1.519 | 1.800 | 1.750 | 1.671 | 1.700 | 1.495 | 1.656 | 7.48 |
| 75) 67 o-xylene | 1.910 | 2.052 | 2.058 | 1.979 | 2.062 | 1.852 | 1.985 | 4.45 |
| 76) P 68 1122-Tetra-C | 0.365 | 0.401 | 0.408 | 0.385 | 0.426 | 0.391 | 0.396 | 5.24 |
| 77) 69 123-tri-Cl-P | 0.112 | 0.134 | 0.135 | 0.128 | 0.145 | 0.134 | 0.131 | 8.44 |
| 78) S 70 4-Br-1-F-Bz | 0.705 | 0.688 | 0.678 | 0.659 | 0.699 | 0.637 | 0.678 | 3.76 |
| 79) 71 isopropylben | 2.428 | 2.582 | 2.790 | 2.605 | 2.869 | 2.653 | 2.654 | 5.92 |
| 80) 72 bromobenzene | 0.632 | 0.709 | 0.694 | 0.667 | 0.704 | 0.626 | 0.672 | 5.39 |
| 81) 92 t-1,4-dichlo | 0.028 | 0.044 | 0.062 | 0.068 | 0.087 | 0.083 | 0.062 | 36.62 |
| 82) 73 n-propylbenz | 0.694 | 0.798 | 0.823 | 0.758 | 0.809 | 0.730 | 0.769 | 6.53 |
| 83) 74 2-Cl-Toluene | 0.578 | 0.697 | 0.689 | 0.644 | 0.680 | 0.623 | 0.652 | 7.07 |
| 84) 75 4-Cl-Toluene | 0.701 | 0.729 | 0.687 | 0.654 | 0.666 | 0.583 | 0.670 | 7.50 |

0.993

0.994

0.992

0.995

(#) = Out of Range
E524A003.M Mon Oct 27 13:57:07 2003



Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Mon Oct 27 13:56:31 2003
 Response via : Initial Calibration

Calibration Files
 .3 =3-A0003.D 2 =3-002.D 10 =3-0010.D
 20 =3-0020.D 40 =3-0040.D 60 =3-0060.D

| Compound | .3 | 2 | 10 | 20 | 40 | 60 | Avg | %RSD |
|---------------------|-------|-------|-------|-------|-------|-------|-------|-------|
| 85) 76 135-tri-Me-B | 2.192 | 2.419 | 2.462 | 2.318 | 2.449 | 2.206 | 2.341 | 5.17 |
| 86) 77 4-Iso-Pr-tol | 2.421 | 2.565 | 2.663 | 2.436 | 2.642 | 2.402 | 2.522 | 4.63 |
| 87) 78 124-tri-Me-B | 2.287 | 2.513 | 2.498 | 2.427 | 2.600 | 2.382 | 2.451 | 4.48 |
| 88) 79 tert-butylbe | 1.853 | 2.009 | 2.152 | 2.004 | 2.256 | 2.057 | 2.055 | 6.71 |
| 89) 80 13-DCB | 1.484 | 1.490 | 1.416 | 1.357 | 1.396 | 1.232 | 1.396 | 6.84 |
| 90) 81 sec-butylben | 2.948 | 3.045 | 3.213 | 2.920 | 3.279 | 3.007 | 3.069 | 4.75 |
| 91) 82 14-DCB | 1.660 | 1.512 | 1.434 | 1.366 | 1.463 | 1.329 | 1.461 | 8.06 |
| 92) 83 Cl-benzyl | 0.066 | 0.066 | 0.102 | 0.123 | 0.168 | 0.168 | 0.116 | 39.76 |
| 93) 84 12-DCB | 1.352 | 1.374 | 1.295 | 1.218 | 1.283 | 1.149 | 1.278 | 6.57 |
| 94) 85 n-butylbenze | 0.623 | 0.678 | 0.712 | 0.654 | 0.707 | 0.621 | 0.666 | 5.99 |
| 95) 86 12-diBr-2-Cl | 0.079 | 0.085 | 0.093 | 0.096 | 0.111 | 0.107 | 0.095 | 13.30 |
| 96) 87 124-tri-Cl-B | 0.700 | 0.756 | 0.822 | 0.810 | 0.879 | 0.811 | 0.796 | 7.71 |
| 97) 88 naphthalene | 0.845 | 0.988 | 1.263 | 1.338 | 1.571 | 1.528 | 1.256 | 23.09 |
| 98) 89 hx-Cl-butadi | 0.492 | 0.456 | 0.476 | 0.416 | 0.468 | 0.426 | 0.456 | 6.44 |
| 99) 90 123-Tri-Cl-B | 0.592 | 0.656 | 0.713 | 0.693 | 0.770 | 0.700 | 0.687 | 8.70 |

0.989

0.997

(#) = Out of Range
E524A003.M

Mon Oct 27 13:57:08 2003

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-A0003.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:05 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:33 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------------------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.64 | 7.63 | 0.002 | 96 | 70 | 920.067 | 10.00 | | 0.02 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 745.928 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.84 | 13.84 | 0.000 | 152 | 150 | 436.784 | 10.00 | | 0.00 | |

| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|-------------------|-------|-------|-------|-----|-----|--------|------|-----|-------|--|
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.58 | 0.002 | 111 | 113 | 6.137 | 0.27 | 0.3 | 1.34% | |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.11 | 7.08 | 0.002 | 65 | 102 | 5.167 | 0.28 | 0.3 | 1.39% | |
| 55 | toluene-d8 | 9.90 | 9.89 | 0.000 | 98 | 100 | 22.176 | 0.24 | 0.2 | 1.18% | |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 9.236 | 0.26 | 0.3 | 1.28% | |

| Target Compounds | <<< I1 : ISTD ID = 1 >>> | Qvalue |
|------------------|--------------------------|--|
| 3 | di-Cl-di-F-methan | 1.89 1.85 0.005 85 87 6.437 0.28 0.3 96 |
| 4 | Chloromethane | 2.11 2.07 0.006 50 52 6.136 0.28 0.3 85 |
| 2 | F114 | 2.04 2.00 0.006 85 135 1.527 0.13 0.1 99 |
| 5 | vinyl chloride | 2.23 2.19 0.005 62 64 4.876 0.22 0.2 74 |
| 6 | bromomethane | 2.60 2.58 0.003 94 96 2.539 0.24 0.2 69 |
| 7 | chloroethane | 2.72 2.70 0.003 64 66 2.197 0.17 0.2 0 |
| 8 | tri-Cl-F-methane | 3.03 3.00 0.004 101 103 8.394 0.25 0.3 100 |
| 91 | Acetonitrile X10 | 4.07 4.04 0.003 41 40 10.689 2.65 2.6 80 |
| 9 | acrolein X10 | 3.52 3.48 0.006 56 55 5.645 2.22 2.2 0 |
| 11 | acetone X10 | 3.71 3.69 0.002 43 58 18.756 4.78 4.8 80 |
| 12 | ethyl ether X5 | 3.37 3.34 0.005 59 74 13.693 1.17 1.2 79 |
| 13 | 11-dichloroethene | 3.63 3.60 0.004 61 96 6.637 0.25 0.3 0 |
| 14 | Iodomethane | 3.81 3.78 0.004 142 127 3.461 0.15 0.1 95 |
| 15 | F-113 | 3.65 3.62 0.004 101 151 4.492 0.22 0.2 0 |
| 16 | acrylonitrile X10 | 4.52 4.49 0.003 53 52 10.574 2.57 2.6 85 |
| 17 | carbon disulfide | 3.90 3.87 0.004 76 78 13.839 0.21 0.2 99 |
| 94 | Isopropyl Alcohol | 4.04 4.01 0.003 45 43 0.331 0.47 0.5 100 |
| 18 | methylene chlorid | 4.22 4.19 0.004 84 49 10.278 0.24 0.2 72 |
| 19 | t-12-di-Cl-ethene | 4.58 4.55 0.004 96 61 6.615 0.27 0.3 88 |

Handwritten signature and date: m/27/03

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-A0003.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:05 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:33 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscleous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|-------------------|-------|-------|--------|------|-----|---------|--------|-------|---------|------|
| 20 | t-Bu-Me-ether | 4.59 | 4.56 | 0.004 | 73 | 57 | 9.529 | 0.23 | 0.2 | 67 | ? |
| 95 | Tert butyl alcoho | 4.45 | 4.47 | -0.002 | 59 | 57 | 1.332 | 1.21 | 1.2 | 100 | # |
| 94 | allyl chloride | 4.07 | 4.04 | 0.003 | 41 | 76 | 10.689 | 0.30 | 0.3 | 56 | #? |
| 21 | 11-dichloroethane | 5.12 | 5.09 | 0.005 | 63 | 83 | 10.035 | 0.25 | 0.3 | 97 | #? |
| 22 | c-12-di-Cl-ethene | 5.93 | 5.89 | 0.005 | 96 | 61 | 6.459 | 0.26 | 0.3 | 86 | #? |
| 23 | 22-Dichloropropan | 5.92 | 5.89 | 0.004 | 77 | 97 | 5.693 | 0.20 | 0.2 | 90 | #? |
| 24 | Br-Cl-methane | 6.26 | 6.23 | 0.004 | 128 | 130 | 3.294 | 0.27 | 0.3 | 87 | #? |
| 25 | chloroform | 6.37 | 6.35 | 0.003 | 83 | 85 | 13.164 | 0.30 | 0.3 | 82 | #? |
| 26 | tetrahydrofuranX5 | 6.35 | 6.32 | 0.004 | 42 | 72 | 4.044 | 1.34 | 1.3 | 73 | #? |
| 98 | Diisopropyl ether | 5.24 | 5.22 | 0.003 | 45 | 87 | 16.931 | 0.28 | 0.3 | 93 | #? |
| 99 | ETBE | 5.73 | 5.72 | 0.002 | 59 | 87 | 9.591 | 0.20 | 0.2 | 95 | m |
| 30 | 12-dichloroethane | 7.23 | 7.20 | 0.004 | 64 | 62 | 2.318 | 0.32 | 0.3 | 46 | m? |
| 32 | vinyl acetate X5 | 5.20 | 5.17 | 0.004 | 43 | 86 | 36.279 | 1.26 | 1.3 | 95 | m |
| 92 | Nitro Methane(x10 | 5.81 | 5.80 | 0.000 | 61 | 46 | 1.574 | 3.08 | 3.1 | 16 | m |
| 33 | 2-butanoneMEK X10 | 5.94 | 5.92 | 0.003 | 43 | 72 | 14.739 | 3.08 | 3.1 | 87 | #? |
| 93 | Ethyl Acetate x2 | 6.04 | 6.02 | 0.003 | 43 | 61 | 6.463 | 0.57 | 0.6 | 79 | # |
| 34 | 111-trichloroetha | 6.65 | 6.63 | 0.002 | 97 | 99 | 9.393 | 0.25 | 0.3 | 85 | # |
| 35 | 11-Di-Cl-propene | 6.91 | 6.88 | 0.004 | 75 | 110 | 6.749 | 0.24 | 0.2 | 89 | # |
| 36 | benzene | 7.21 | 7.19 | 0.002 | 78 | 52 | 23.536 | 0.25 | 0.3 | 87 | # |
| 37 | CCl4 | 6.91 | 6.89 | 0.002 | 117 | 119 | 9.052 | 0.26 | 0.3 | 90 | # |
| 100 | Isobutyl alcohol | 7.42 | 7.39 | 0.003 | 43 | 42 | 2.932 | 7.75 | 7.8 | 61 | #? |
| 38 | thiophene | 7.54 | 7.51 | 0.004 | 84 | 58 | 10.222 | 0.22 | 0.2 | 75 | #? |
| 39 | 12-di-Cl-propane | 8.56 | 8.54 | 0.002 | 63 | 76 | 4.815 | 0.23 | 0.2 | 95 | m |
| 40 | trichloroethene | 8.25 | 8.23 | 0.002 | 130 | 132 | 7.696 | 0.26 | 0.3 | 95 | m |
| 41 | dibromomethane | 8.72 | 8.71 | 0.000 | 174 | 172 | 3.770 | 0.28 | 0.3 | 83 | m |
| 101 | TAME | 7.41 | 7.39 | 0.002 | 73 | 43 | 7.879 | 0.19 | 0.2 | 52 | m? |
| 42 | Br-di-Cl-methane | 8.95 | 8.95 | 0.000 | 83 | 85 | 9.392 | 0.31 | 0.3 | 94 | m? |
| 43 | Me-methacrylate | 8.76 | 8.75 | 0.002 | 69 | 100 | 1.457 | 0.15 | 0.2 | 34 | m |
| 44 | 2-ClEt-Vi-ether10 | 9.38 | 9.37 | 0.000 | 63 | 43 | 4.887 | 2.69 | 2.7 | 93 | m |
| 45 | c-13-di-Cl-propen | 9.57 | 9.55 | 0.002 | 75 | 110 | 6.769 | 0.22 | 0.2 | 89 | m |
| 46 | t-1,3-dichloropro | 10.25 | 10.24 | 0.000 | 75 | 110 | 5.153 | 0.21 | 0.2 | 89 | m |

Handwritten notes:
 101-7/13
 101-7/13

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-A0003.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:05 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:33 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscelaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|---------------------------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| 49 | 13-di-Cl-propane | 10.65 | 10.64 | 0.001 | 76 | 78 | 7.569 | 0.27 | 0.3 | 85 | ? |
| 50 | Et methacrylate | 10.38 | 10.37 | 0.000 | 69 | 99 | 2.785 | 0.14 | 0.1 | 83 | |
| 51 | di-Br-Cl-methane | 10.91 | 10.90 | 0.000 | 129 | 127 | 7.359 | 0.30 | 0.3 | 83 | |
| 52 | bromofom | 12.41 | 12.41 | 0.000 | 173 | 174 | 4.029 | 0.29 | 0.3 | 95 | |
| 53 | 1,4-dichlorobutan | 12.68 | 12.67 | 0.000 | 55 | 41 | 7.248 | 0.27 | 0.3 | 90 | |
| 54 | MIBK | 9.77 | 9.76 | 0.001 | 43 | 58 | 2.727 | 0.25 | 0.3 | 63 | |
| 56 | toluene | 9.99 | 9.98 | 0.001 | 91 | 92 | 32.453 | 0.30 | 0.3 | 96 | |
| 57 | 2-hexanone X5 | 10.76 | 10.75 | 0.001 | 43 | 58 | 8.296 | 1.13 | 1.1 | 89 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 4.393 | 0.25 | 0.2 | 83 | |
| 59 | tetra-Cl-ethene | 10.64 | 10.64 | 0.000 | 166 | 168 | 8.603 | 0.27 | 0.3 | 96 | |
| 60 | chlorobenzene | 11.57 | 11.57 | 0.000 | 112 | 77 | 21.200 | 0.28 | 0.3 | 95 | |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 7.365 | 0.27 | 0.3 | 93 | |
| <<< I3 : ISTD ID = 62 >>> | | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 3.125 | 0.22 | 0.2 | 17 | #? |
| 64 | Et-Bz | 11.70 | 11.69 | 0.000 | 91 | 106 | 31.613 | 0.23 | 0.2 | 94 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 51.588 | 0.50 | 0.5 | 98 | |
| 66 | styrene | 12.24 | 12.23 | 0.000 | 104 | 78 | 19.899 | 0.25 | 0.3 | 94 | |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 25.030 | 0.24 | 0.2 | 96 | |
| 68 | 1122-Tetra-Cl-Et | 12.88 | 12.87 | 0.000 | 83 | 85 | 4.786 | 0.21 | 0.2 | 86 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.91 | 0.000 | 110 | 97 | 1.463 | 0.21 | 0.2 | 75 | |
| 71 | isopropylbenzene | 12.60 | 12.59 | 0.000 | 105 | 120 | 31.809 | 0.24 | 0.2 | 99 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 8.279 | 0.23 | 0.2 | 74 | #? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 0.370 | 0.11 | 0.1 | 84 | #? |
| 73 | n-propylbenzene | 13.00 | 12.99 | 0.000 | 120 | 78 | 9.091 | 0.22 | 0.2 | 91 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 7.570 | 0.21 | 0.2 | 93 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.18 | 0.000 | 126 | 128 | 9.182 | 0.25 | 0.2 | 95 | |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 28.727 | 0.25 | 0.3 | 90 | |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 31.720 | 0.25 | 0.2 | 99 | |
| 78 | 124-tri-Me-Benzen | 13.52 | 13.51 | 0.000 | 105 | 120 | 29.971 | 0.25 | 0.3 | 99 | |
| 79 | tert-butylbenzene | 13.48 | 13.47 | 0.000 | 119 | 91 | 24.279 | 0.22 | 0.2 | 91 | |
| 80 | 13-DCB | 13.79 | 13.78 | 0.000 | 146 | 148 | 19.447 | 0.26 | 0.3 | 91 | |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 38.627 | 0.25 | 0.3 | 96 | |

Mr 10/27/03


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-A0003.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:05 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:33 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscelleneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 21.754 | 0.28 | 0.3 | 84 | |
| 83 | Cl-benzy1 | 13.98 | 13.98 | 0.000 | 126 | 91 | 0.871 | 0.12 | 0.1 | 35 | # |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 17.721 | 0.27 | 0.3 | 90 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 8.164 | 0.24 | 0.2 | 80 | #? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 1.032 | 0.22 | 0.2 | 75 | |
| 87 | 124-tri-Cl-Bz | 15.59 | 15.58 | 0.000 | 180 | 182 | 9.169 | 0.21 | 0.2 | 96 | |
| 88 | naphthalene | 15.79 | 15.78 | 0.000 | 128 | 129 | 11.079 | 0.14 | 0.1 | 91 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 6.445 | 0.25 | 0.2 | 81 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 7.754 | 0.20 | 0.2 | 97 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-A0003.D
 Method : C:\MSDCHEM\1\METHODS\E524A003.M
 Acq. Time : Oct 21 10:05 2003
 Method Update: Mon Oct 27 13:48 2003
 Quant. Time : Oct 27 13:33 2003
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :
 Sample : F=1
 Inst. : GCMS-A
 RF via : Multiple Level Calibration
 Operator: zou
 Multiplr: 1.000000

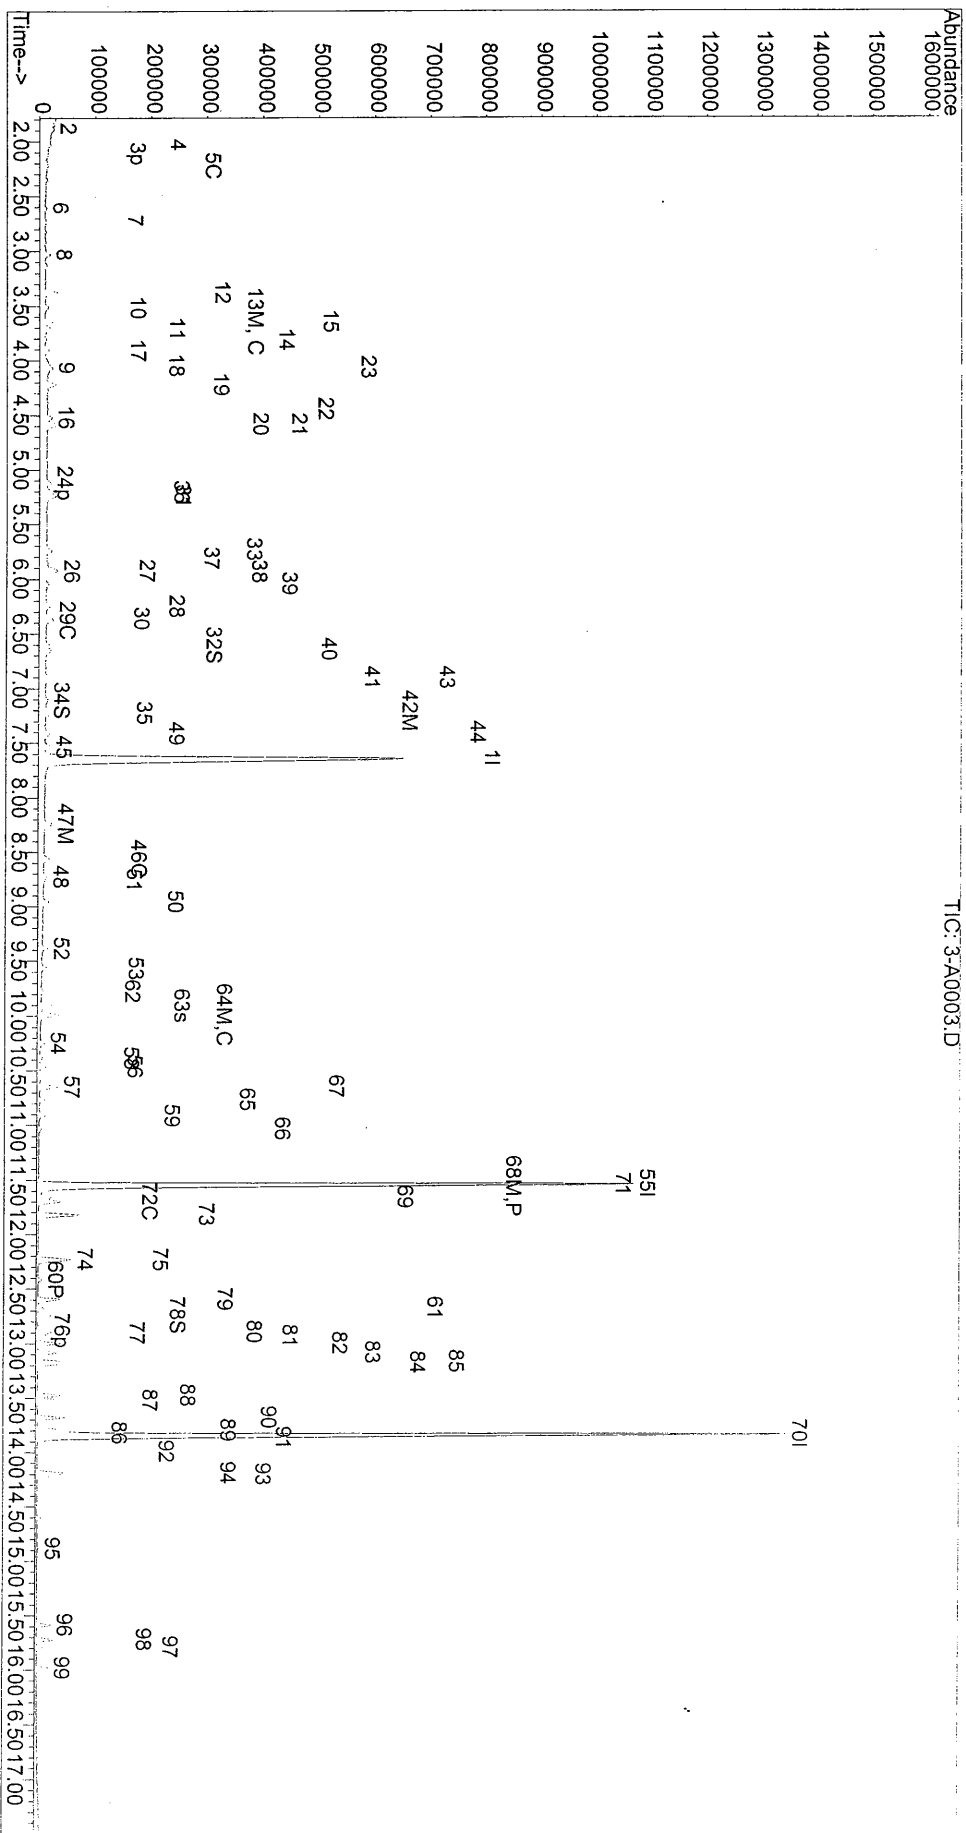

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-002.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:31 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:36 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------------------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.65 | 7.63 | 0.003 | 96 | 70 | 916.201 | 10.00 | | 0.02 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 732.691 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.84 | 13.84 | 0.000 | 152 | 150 | 441.685 | 10.00 | | 0.00 | |

| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|-------------------|-------|-------|-------|-----|-----|---------|------|--|-----|--------|
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.58 | 0.002 | 111 | 113 | 45.047 | 1.97 | | 2.0 | 9.86% |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.11 | 7.08 | 0.002 | 65 | 102 | 39.287 | 2.12 | | 2.1 | 10.62% |
| 55 | toluene-d8 | 9.91 | 9.89 | 0.000 | 98 | 100 | 162.055 | 1.75 | | 1.8 | 8.77% |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 60.769 | 1.66 | | 1.7 | 8.32% |

| Target Compounds | <<< 11 : ISTD ID = 1 >>> | Qvalue |
|------------------|--------------------------|--|
| 3 | di-Cl-di-F-methan | 1.89 1.85 0.005 85 87 39.097 1.70 1.7 95 |
| 4 | Chloromethane | 2.11 2.07 0.005 50 52 37.417 1.74 1.7 92 |
| 2 | F114 | 2.03 2.00 0.005 85 135 19.306 1.61 1.6 55 |
| 5 | vinyl chloride | 2.22 2.19 0.004 62 64 33.446 1.51 1.5 95 |
| 6 | bromomethane | 2.61 2.58 0.005 94 96 18.408 1.73 1.7 96 |
| 7 | chloroethane | 2.73 2.70 0.004 64 66 17.752 1.34 1.3 88 |
| 8 | tri-Cl-F-methane | 3.03 3.00 0.005 101 103 56.082 1.70 1.7 99 |
| 91 | Acetonitrile X10 | 4.07 4.04 0.004 41 40 82.041 20.41 20.4 96 |
| 9 | acrolein X10 | 3.52 3.48 0.006 56 55 40.130 15.88 15.9 98 |
| 11 | acetone X10 | 3.71 3.69 0.002 43 58 64.324 16.47 16.5 79 |
| 12 | ethyl ether X5 | 3.37 3.34 0.005 59 74 93.915 8.07 8.1 81 |
| 13 | 11-dichloroethene | 3.64 3.60 0.005 61 96 46.215 1.76 1.8 85 |
| 14 | Iodomethane | 3.82 3.78 0.005 142 127 29.384 1.27 1.3 99 |
| 15 | F-113 | 3.65 3.62 0.004 101 151 28.088 1.36 1.4 90 |
| 16 | acrylonitrile X10 | 4.52 4.49 0.004 53 52 78.358 19.13 19.1 95 |
| 17 | carbon disulfide | 3.91 3.87 0.005 76 78 85.463 1.28 1.3 99 |
| 94 | Isopropyl Alcohol | 4.04 4.01 0.004 45 43 1.284 1.83 1.8 100 |
| 18 | methylene chlorid | 4.22 4.19 0.005 84 49 48.191 1.13 1.1 94 |
| 19 | t-12-di-Cl-ethene | 4.58 4.55 0.005 96 61 45.733 1.85 1.8 96 |

10/27/23

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-002.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:31 2003 RF via : Multiple Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:36 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | QIon | QI | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|-----------|
| 20 | t-Bu-Me-ether | 4.59 | 4.56 | 0.004 | 73 | 57 | 70.095 | 1.70 | 1.7 | 90 | ? |
| 95 | Tert butyl alcoho | 4.46 | 4.47 | 0.000 | 59 | 57 | 4.624 | 4.22 | 4.2 | 100 | # |
| 94 | allyl chloride | 4.07 | 4.04 | 0.004 | 41 | 76 | 82.041 | 2.28 | 2.3 | 71 | #? |
| 21 | 11-dichloroethane | 5.12 | 5.09 | 0.004 | 63 | 83 | 71.189 | 1.79 | 1.8 | 96 | 2 |
| 97 | propionitrile | 6.03 | 5.99 | 0.004 | 54 | 51 | 3.119 | 2.03 | 2.0 | 100 | m? 2/2/13 |
| 22 | c-12-di-Cl-ethene | 5.91 | 5.89 | 0.002 | 96 | 61 | 46.844 | 1.88 | 1.9 | 91 | ? |
| 23 | 22-Dichloropropan | 5.92 | 5.89 | 0.003 | 77 | 97 | 38.859 | 1.37 | 1.4 | 94 | ? |
| 24 | Br-Cl-methane | 6.25 | 6.23 | 0.003 | 128 | 130 | 23.046 | 1.90 | 1.9 | 96 | ? |
| 25 | chloroform | 6.38 | 6.35 | 0.003 | 83 | 85 | 80.631 | 1.84 | 1.8 | 95 | ? |
| 26 | tetrahydrofuranX5 | 6.35 | 6.32 | 0.003 | 42 | 72 | 28.808 | 9.57 | 9.6 | 83 | ? |
| 98 | Diisopropyl ether | 5.25 | 5.22 | 0.004 | 45 | 87 | 136.442 | 2.23 | 2.2 | 88 | ? |
| 99 | ETBE | 5.74 | 5.72 | 0.003 | 59 | 87 | 74.005 | 1.58 | 1.6 | 93 | ? |
| 30 | 12-dichloroethane | 7.22 | 7.20 | 0.002 | 64 | 62 | 14.864 | 2.08 | 2.1 | 93 | ? |
| 32 | vinyl acetate X5 | 5.20 | 5.17 | 0.004 | 43 | 86 | 291.623 | 10.20 | 10.2 | 95 | # |
| 92 | Nitro Methane(x10 | 5.82 | 5.80 | 0.002 | 61 | 46 | 10.571 | 20.78 | 20.8 | 63 | #? |
| 33 | 2-butanoneMEK X10 | 5.94 | 5.92 | 0.003 | 43 | 72 | 98.541 | 20.66 | 20.7 | 83 | #? |
| 93 | Ethyl Acetate x2 | 6.05 | 6.02 | 0.004 | 43 | 61 | 37.342 | 3.29 | 3.3 | 91 | ? |
| 34 | 111-trichloroetha | 6.65 | 6.63 | 0.002 | 97 | 99 | 63.933 | 1.73 | 1.7 | 97 | ? |
| 35 | 11-Di-Cl-propene | 6.90 | 6.88 | 0.002 | 75 | 110 | 49.362 | 1.77 | 1.8 | 85 | ? |
| 36 | benzene | 7.21 | 7.19 | 0.003 | 78 | 52 | 167.998 | 1.81 | 1.8 | 94 | ? |
| 37 | CCl4 | 6.91 | 6.89 | 0.002 | 117 | 119 | 59.763 | 1.76 | 1.8 | 98 | ? |
| 100 | Isobutyl alcohol | 7.42 | 7.39 | 0.003 | 43 | 42 | 21.047 | 55.87 | 55.9 | 81 | #? |
| 38 | thiophene | 7.53 | 7.51 | 0.003 | 84 | 58 | 83.170 | 1.80 | 1.8 | 95 | ? |
| 39 | 12-di-Cl-propane | 8.56 | 8.54 | 0.002 | 63 | 76 | 37.555 | 1.80 | 1.8 | 93 | ? |
| 40 | trichloroethene | 8.24 | 8.23 | 0.002 | 130 | 132 | 50.098 | 1.73 | 1.7 | 82 | ? |
| 41 | dibromomethane | 8.73 | 8.71 | 0.002 | 174 | 172 | 26.033 | 1.97 | 2.0 | 87 | ? |
| 101 | TAME | 7.42 | 7.39 | 0.004 | 73 | 43 | 59.032 | 1.46 | 1.5 | 92 | m? |
| 42 | Br-di-Cl-methane | 8.96 | 8.95 | 0.002 | 83 | 85 | 56.733 | 1.89 | 1.9 | 97 | ? |
| 43 | Me-methacrylate | 8.76 | 8.75 | 0.002 | 69 | 100 | 14.747 | 1.57 | 1.6 | 91 | ? |
| 44 | 2-ClEt-VI-ether10 | 9.38 | 9.37 | 0.000 | 63 | 43 | 45.249 | 24.99 | 25.0 | 84 | ? |
| 45 | C-13-di-Cl-propen | 9.56 | 9.55 | 0.002 | 75 | 110 | 54.923 | 1.82 | 1.8 | 94 | ? |
| 46 | t-1,3-dichloropro | 10.25 | 10.24 | 0.000 | 75 | 110 | 40.425 | 1.68 | 1.7 | 98 | ? |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-002.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:31 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:36 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| <<< I2 : | ISTD ID = 47 >>> | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.46 | 10.45 | 0.000 | 97 | 83 | 31.570 | 1.79 | 1.8 | 94 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.64 | 0.000 | 76 | 78 | 48.826 | 1.75 | 1.8 | 84 | |
| 50 | Et methacrylate | 10.38 | 10.37 | 0.000 | 69 | 99 | 29.334 | 1.47 | 1.5 | 96 | |
| 51 | di-Br-Cl-methane | 10.91 | 10.90 | 0.000 | 129 | 127 | 44.728 | 1.88 | 1.9 | 100 | |
| 52 | bromoform | 12.42 | 12.41 | 0.000 | 173 | 174 | 26.611 | 1.96 | 2.0 | 98 | |
| 53 | 1,4-dichlorobutan | 12.67 | 12.67 | 0.000 | 55 | 41 | 52.525 | 2.02 | 2.0 | 98 | |
| 54 | MIBK | 9.77 | 9.76 | 0.000 | 43 | 58 | 20.267 | 1.90 | 1.9 | 91 | |
| 56 | toluene | 9.99 | 9.98 | 0.000 | 91 | 92 | 204.349 | 1.93 | 1.9 | 97 | |
| 57 | 2-hexanone X5 | 10.76 | 10.75 | 0.000 | 43 | 58 | 70.148 | 9.69 | 9.7 | 85 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 32.436 | 1.86 | 1.9 | 94 | |
| 59 | tetra-Cl-ethene | 10.65 | 10.64 | 0.001 | 166 | 168 | 59.173 | 1.87 | 1.9 | 98 | |
| 60 | chlorobenzene | 11.57 | 11.57 | 0.000 | 112 | 77 | 144.953 | 1.92 | 1.9 | 94 | |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 51.367 | 1.90 | 1.9 | 98 | |
| <<< I3 : | ISTD ID = 62 >>> | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 20.185 | 1.40 | 1.4 | 69 | #? |
| 64 | Et-Bz | 11.70 | 11.69 | 0.000 | 91 | 106 | 225.200 | 1.63 | 1.6 | 92 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 364.290 | 3.49 | 3.5 | 99 | |
| 66 | styrene | 12.24 | 12.23 | 0.000 | 104 | 78 | 158.986 | 2.00 | 2.0 | 95 | |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 181.225 | 1.73 | 1.7 | 92 | |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 35.408 | 1.52 | 1.5 | 99 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.91 | 0.000 | 110 | 97 | 11.857 | 1.70 | 1.7 | 94 | |
| 71 | isopropylbenzene | 12.60 | 12.59 | 0.000 | 105 | 120 | 228.075 | 1.70 | 1.7 | 97 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 62.596 | 1.74 | 1.7 | 97 | |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 3.850 | 1.13 | 1.1 | 71 | #? |
| 73 | n-propylbenzene | 13.00 | 12.99 | 0.000 | 120 | 78 | 70.513 | 1.68 | 1.7 | 96 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 61.543 | 1.66 | 1.7 | 96 | |
| 75 | 4-Cl-Toluene | 13.18 | 13.18 | 0.000 | 126 | 128 | 64.367 | 1.70 | 1.7 | 100 | |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 213.694 | 1.85 | 1.8 | 96 | |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 226.621 | 1.76 | 1.8 | 97 | |
| 78 | 124-tri-Me-Benzen | 13.51 | 13.51 | 0.000 | 105 | 120 | 222.021 | 1.84 | 1.8 | 99 | |
| 79 | tert-butylbenzene | 13.48 | 13.47 | 0.000 | 119 | 91 | 177.466 | 1.61 | 1.6 | 90 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06


Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-002.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:31 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:36 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.78 | 0.000 | 146 | 148 | 131.664 | 1.74 | 1.7 | 94 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 268.975 | 1.73 | 1.7 | 95 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 133.604 | 1.73 | 1.7 | 94 | |
| 83 | Cl-benzy1 | 13.98 | 13.98 | 0.000 | 126 | 91 | 5.857 | 0.80 | 0.8 | 61 | # |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 121.367 | 1.80 | 1.8 | 96 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 59.910 | 1.74 | 1.7 | 82 | #? |
| 86 | 12-diBr-2-Cl-PrA | 14.88 | 14.88 | 0.000 | 157 | 155 | 7.477 | 1.57 | 1.6 | 89 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 66.792 | 1.53 | 1.5 | 94 | |
| 88 | naphthalene | 15.79 | 15.78 | 0.000 | 128 | 129 | 87.277 | 1.10 | 1.1 | 99 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 40.287 | 1.52 | 1.5 | 96 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 57.941 | 1.48 | 1.5 | 93 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-002.D
 Method : C:\MSDCHEM\1\METHODS\E524A003.M
 Acq. Time : Oct 21 10:31 2003
 Method Update: Mon Oct 27 13:48 2003
 Quant. Time : Oct 27 13:36 2003
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

Sample : f=1
 Inst. : GCMS-A
 RF via : Multiple Level Calibration
 Operator: zou
 Multiplr: 1.000000

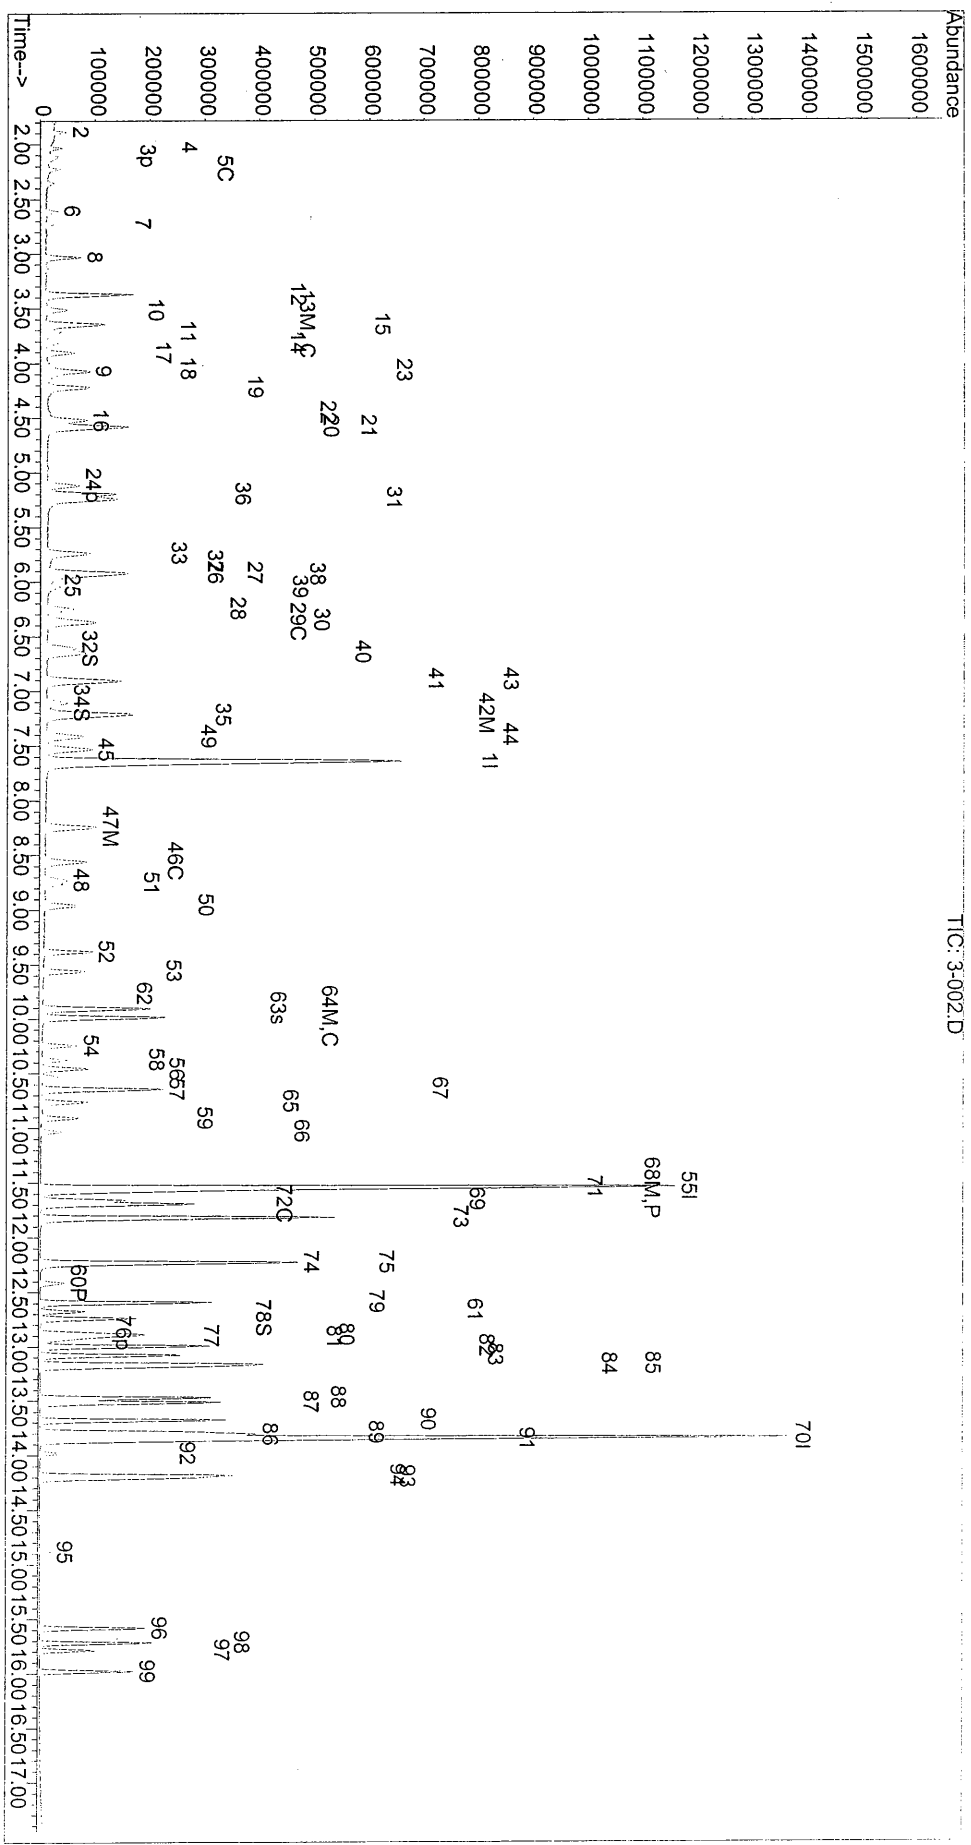

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0010.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:56 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:38 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

ID Component Name R.T. RT0 DRRT Qion Q1 RF/1000 C0,ppb C,ppb Quality Note

Internal Standards

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|----------|
| 1 | Fluorobenzene | 7.65 | 7.63 | 0.003 | 96 | 70 | 919.392 | 10.00 | | 0.02 | Dev(Min) |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 724.575 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.84 | 13.84 | 0.000 | 152 | 150 | 431.820 | 10.00 | | 0.00 | |

System Monitoring Compounds (Surrogate)

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|--------|
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.58 | 0.002 | 111 | 113 | 218.874 | 9.55 | | 9.6 | 47.76% |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.10 | 7.08 | 0.001 | 65 | 102 | 192.209 | 10.36 | | 10.4 | 51.79% |
| 55 | toluene-d8 | 9.91 | 9.89 | 0.000 | 98 | 100 | 811.859 | 8.89 | | 8.9 | 44.45% |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 292.727 | 8.20 | | 8.2 | 40.98% |

Target Compounds <<< I1 : ISTD ID = 1 >>> Qvalue

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|-------------------|------|------|-------|------|-----|---------|--------|-------|---------|------|
| 3 | di-Cl-di-F-methan | 1.89 | 1.85 | 0.005 | 85 | 87 | 199.979 | 8.66 | | 8.7 | 93 |
| 4 | Chloromethane | 2.11 | 2.07 | 0.005 | 50 | 52 | 181.676 | 8.40 | | 8.4 | 99 |
| 2 | F114 | 2.03 | 2.00 | 0.005 | 85 | 135 | 101.058 | 8.37 | | 8.4 | 67 |
| 5 | vinyl chloride | 2.23 | 2.19 | 0.005 | 62 | 64 | 161.213 | 7.23 | | 7.2 | 98 |
| 6 | bromomethane | 2.61 | 2.58 | 0.005 | 94 | 96 | 87.613 | 8.18 | | 8.2 | 98 |
| 7 | chloroethane | 2.73 | 2.70 | 0.004 | 64 | 66 | 90.280 | 6.81 | | 6.8 | 100 |
| 8 | tri-Cl-F-methane | 3.04 | 3.00 | 0.006 | 101 | 103 | 277.768 | 8.41 | | 8.4 | 98 |
| 91 | Acetonitrile X10 | 4.07 | 4.04 | 0.004 | 41 | 40 | 382.813 | 94.91 | | 94.9 | 92 |
| 9 | acrolein X10 | 3.52 | 3.48 | 0.006 | 56 | 55 | 201.945 | 79.64 | | 79.6 | 100 |
| 11 | acetone X10 | 3.75 | 3.69 | 0.008 | 43 | 58 | 288.996 | 73.75 | | 73.8 | 0 |
| 12 | ethyl ether X5 | 3.37 | 3.34 | 0.005 | 59 | 74 | 436.367 | 37.37 | | 37.4 | 80 |
| 13 | 11-dichloroethene | 3.64 | 3.60 | 0.005 | 61 | 96 | 229.524 | 8.71 | | 8.7 | 83 |
| 14 | Iodomethane | 3.82 | 3.78 | 0.005 | 142 | 127 | 183.879 | 7.89 | | 7.9 | 97 |
| 15 | F-113 | 3.65 | 3.62 | 0.005 | 101 | 151 | 146.108 | 7.05 | | 7.1 | 89 |
| 16 | acrylonitrile X10 | 4.53 | 4.49 | 0.005 | 53 | 52 | 419.836 | 102.15 | | 102.1 | 98 |
| 17 | carbon disulfide | 3.90 | 3.87 | 0.004 | 76 | 78 | 420.250 | 6.27 | | 6.3 | 99 |
| 94 | Isopropyl Alcohol | 4.04 | 4.01 | 0.004 | 45 | 43 | 1.238 | 1.76 | | 1.8 | 100 |
| 18 | methylene chlorid | 4.22 | 4.19 | 0.004 | 84 | 49 | 203.033 | 4.73 | | 4.7 | 78 |
| 19 | t-12-di-Cl-ethene | 4.58 | 4.55 | 0.004 | 96 | 61 | 217.854 | 8.77 | | 8.8 | 93 |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Handwritten signature and date: 10/27/03

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0010.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:56 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:38 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0, ppb | C, ppb | Quality | Note |
|-----|--------------------|-------|-------|-------|------|-----|----------|---------|--------|---------|--------------|
| 20 | t-Bu-Me-ether | 4.60 | 4.56 | 0.005 | 73 | 57 | 362.056 | 8.76 | 8.8 | 94 | |
| 95 | Tert butyl alcohol | 4.58 | 4.47 | 0.015 | 59 | 57 | 88.338 | 80.34 | 80.3 | 100 | m? (ok) 10/3 |
| 94 | allyl chloride | 4.07 | 4.04 | 0.004 | 41 | 76 | 426.268 | 11.79 | 11.8 | 75 | m? |
| 21 | 11-dichloroethane | 5.12 | 5.09 | 0.005 | 63 | 83 | 342.138 | 8.58 | 8.6 | 99 | |
| 97 | propionitrile | 6.04 | 5.99 | 0.006 | 54 | 51 | 18.745 | 12.15 | 12.2 | 100 | m? |
| 22 | c-12-di-Cl-ethene | 5.92 | 5.89 | 0.003 | 96 | 61 | 225.560 | 9.01 | 9.0 | 93 | ? |
| 23 | 22-Dichloropropan | 5.92 | 5.89 | 0.004 | 77 | 97 | 218.612 | 7.67 | 7.7 | 98 | ? |
| 24 | Br-Cl-methane | 6.25 | 6.23 | 0.003 | 128 | 130 | 109.590 | 9.03 | 9.0 | 100 | |
| 25 | chloroform | 6.38 | 6.35 | 0.003 | 83 | 85 | 375.460 | 8.54 | 8.5 | 96 | ? |
| 26 | tetrahydrofuranX5 | 6.36 | 6.32 | 0.005 | 42 | 72 | 169.729 | 56.21 | 56.2 | 82 | m? |
| 98 | Diisopropyl ether | 5.24 | 5.22 | 0.003 | 45 | 87 | 688.556 | 11.22 | 11.2 | 90 | |
| 99 | ETBE | 5.74 | 5.72 | 0.003 | 59 | 87 | 411.030 | 8.76 | 8.8 | 90 | |
| 30 | 12-dichloroethane | 7.22 | 7.20 | 0.003 | 64 | 62 | 77.221 | 10.78 | 10.8 | 91 | ? |
| 32 | vinyl acetate X5 | 5.20 | 5.17 | 0.004 | 43 | 86 | 1683.396 | 58.68 | 58.7 | 93 | |
| 92 | Nitro Methane(x10 | 5.92 | 5.80 | 0.015 | 61 | 46 | 358.371 | 701.91 | 701.9 | 16 | #? |
| 33 | 2-butanoneMEK X10 | 5.96 | 5.92 | 0.005 | 43 | 72 | 459.782 | 96.08 | 96.1 | 86 | |
| 93 | Ethyl Acetate x2 | 6.05 | 6.02 | 0.004 | 43 | 61 | 237.607 | 20.85 | 20.8 | 100 | ? |
| 34 | 111-trichloroetha | 6.65 | 6.63 | 0.002 | 97 | 99 | 333.945 | 9.02 | 9.0 | 98 | |
| 35 | 11-Di-Cl-propene | 6.91 | 6.88 | 0.003 | 75 | 110 | 260.487 | 9.31 | 9.3 | 88 | ? |
| 36 | benzene | 7.21 | 7.19 | 0.003 | 78 | 52 | 811.668 | 8.70 | 8.7 | 93 | ? |
| 37 | CCl4 | 6.91 | 6.89 | 0.002 | 117 | 119 | 312.695 | 9.16 | 9.2 | 95 | ? |
| 100 | Isobutyl alcohol | 7.42 | 7.39 | 0.003 | 43 | 42 | 112.031 | 296.35 | 296.4 | 81 | #? |
| 38 | thiophene | 7.53 | 7.51 | 0.003 | 84 | 58 | 428.533 | 9.24 | 9.2 | 98 | |
| 39 | 12-di-Cl-propane | 8.56 | 8.54 | 0.002 | 63 | 76 | 178.169 | 8.53 | 8.5 | 97 | |
| 40 | trichloroethene | 8.24 | 8.23 | 0.002 | 130 | 132 | 255.616 | 8.79 | 8.8 | 93 | |
| 41 | dibromomethane | 8.72 | 8.71 | 0.000 | 174 | 172 | 124.373 | 9.39 | 9.4 | 96 | |
| 101 | TAME | 7.41 | 7.39 | 0.002 | 73 | 43 | 335.735 | 8.25 | 8.3 | 91 | ? |
| 42 | Br-di-Cl-methane | 8.96 | 8.95 | 0.002 | 83 | 85 | 274.489 | 9.12 | 9.1 | 98 | |
| 43 | Me-methacrylate | 8.76 | 8.75 | 0.002 | 69 | 100 | 87.065 | 9.25 | 9.3 | 97 | |
| 44 | 2-ClEt-Vi-ether10 | 9.38 | 9.37 | 0.002 | 63 | 43 | 275.793 | 151.78 | 151.8 | 84 | |
| 45 | c-13-di-Cl-propen | 9.56 | 9.55 | 0.002 | 75 | 110 | 293.425 | 9.67 | 9.7 | 91 | |
| 46 | t-1,3-dichloropro | 10.25 | 10.24 | 0.000 | 75 | 110 | 231.011 | 9.57 | 9.6 | 91 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-00.L.D
 Method : C:\MSDCHEM\1\METHODS\E524A003.M
 Acq. Time : Oct 21 10:56 2003
 Method Update: Mon Oct 27 13:48 2003
 Quant. Time : Oct 27 13:38 2003
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------|--------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| <<< 12 | : ISTD ID = 47 >>> | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.46 | 10.45 | 0.000 | 97 | 83 | 158.039 | 9.04 | 9.0 | 98 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.64 | 0.000 | 76 | 78 | 251.096 | 9.10 | 9.1 | 100 | ? |
| 50 | Et methacrylate | 10.37 | 10.37 | 0.000 | 69 | 99 | 189.197 | 9.56 | 9.6 | 95 | |
| 51 | di-Br-Cl-methane | 10.91 | 10.90 | 0.000 | 129 | 127 | 219.307 | 9.33 | 9.3 | 95 | |
| 52 | bromofom | 12.42 | 12.41 | 0.000 | 173 | 174 | 127.022 | 9.46 | 9.5 | 100 | |
| 53 | 1,4-dichlorobutan | 12.68 | 12.67 | 0.000 | 55 | 41 | 270.048 | 10.52 | 10.5 | 94 | |
| 54 | MIBK | 9.77 | 9.76 | 0.000 | 43 | 58 | 114.402 | 10.84 | 10.8 | 95 | |
| 56 | toluene | 9.99 | 9.98 | 0.000 | 91 | 92 | 957.684 | 9.13 | 9.1 | 98 | |
| 57 | 2-hexanone X5 | 10.76 | 10.75 | 0.000 | 43 | 58 | 400.071 | 55.86 | 55.9 | 90 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 159.989 | 9.27 | 9.3 | 95 | |
| 59 | tetra-Cl-ethene | 10.65 | 10.64 | 0.001 | 166 | 168 | 281.865 | 8.99 | 9.0 | 97 | ? |
| 60 | chlorobenzene | 11.58 | 11.57 | 0.000 | 112 | 77 | 676.974 | 9.05 | 9.1 | 90 | ? |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 249.086 | 9.33 | 9.3 | 98 | |
| <<< 13 | : ISTD ID = 62 >>> | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 105.292 | 7.48 | 7.5 | 60 | #? |
| 64 | Et-Bz | 11.70 | 11.69 | 0.000 | 91 | 106 | 1128.701 | 8.35 | 8.4 | 94 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 1753.788 | 17.17 | 17.2 | 97 | |
| 66 | styrene | 12.24 | 12.23 | 0.000 | 104 | 78 | 755.749 | 9.73 | 9.7 | 95 | ? |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 888.564 | 8.67 | 8.7 | 95 | ? |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 176.142 | 7.72 | 7.7 | 100 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.91 | 0.000 | 110 | 97 | 58.506 | 8.57 | 8.6 | 97 | ? |
| 71 | isopropylbenzene | 12.60 | 12.59 | 0.000 | 105 | 120 | 1204.677 | 9.18 | 9.2 | 99 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 299.551 | 8.50 | 8.5 | 98 | ? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 26.890 | 8.11 | 8.1 | 75 | #? |
| 73 | n-propylbenzene | 13.00 | 12.99 | 0.000 | 120 | 78 | 355.352 | 8.64 | 8.6 | 92 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 297.725 | 8.19 | 8.2 | 100 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.18 | 0.000 | 126 | 128 | 296.683 | 8.03 | 8.0 | 98 | ? |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 1063.069 | 9.41 | 9.4 | 98 | ? |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 1149.787 | 9.11 | 9.1 | 97 | ? |
| 78 | 124-tri-Me-Benzen | 13.51 | 13.51 | 0.000 | 105 | 120 | 1078.747 | 9.17 | 9.2 | 98 | |
| 79 | tert-butylbenzene | 13.47 | 13.47 | 0.000 | 119 | 91 | 929.162 | 8.61 | 8.6 | 97 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06


Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-00.LV.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 10:56 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:38 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscleous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.78 | 0.000 | 146 | 148 | 611.576 | 8.25 | 8.3 | 97 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 1387.531 | 9.14 | 9.1 | 98 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 619.366 | 8.20 | 8.2 | 96 | |
| 83 | Cl-benzyl | 13.98 | 13.98 | 0.000 | 126 | 91 | 44.122 | 6.18 | 6.2 | 94 | |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 559.240 | 8.47 | 8.5 | 99 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 307.483 | 9.14 | 9.1 | 90 | #? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 40.003 | 8.61 | 8.6 | 96 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 354.819 | 8.30 | 8.3 | 98 | |
| 88 | naphthalene | 15.78 | 15.78 | 0.000 | 128 | 129 | 545.491 | 7.03 | 7.0 | 99 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 205.532 | 7.94 | 7.9 | 99 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 307.963 | 8.03 | 8.0 | 97 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0010.D
 Method : C:\MSDCHEM\1\METHODS\E524A003.M
 Acq. Time : Oct 21 10:56 2003
 Method Update: Mon Oct 27 13:48 2003
 Quant. Time : Oct 27 13:38 2003
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

Sample : F=1
 Inst. : GCMS-A
 RF via : Multiple Level Calibration
 Operator: zou
 Multiplr: 1.000000

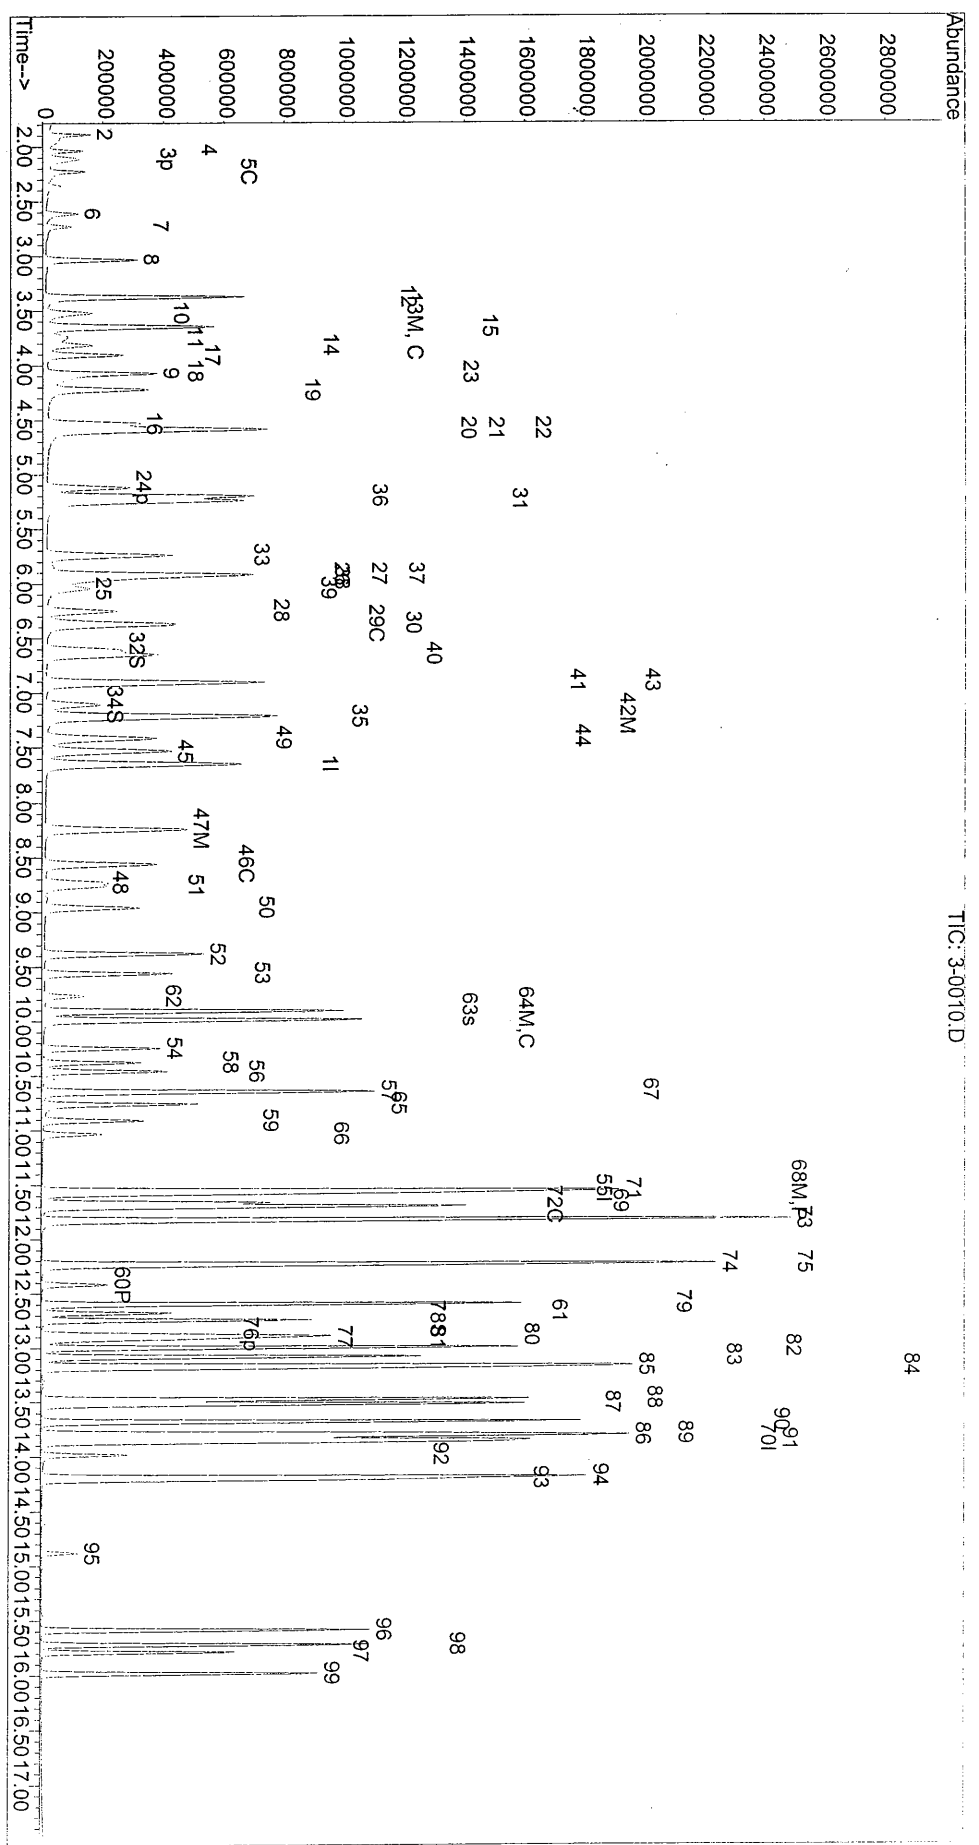

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0020.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 11:22 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:40 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscelaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------------------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.65 | 7.63 | 0.003 | 96 | 70 | 955.116 | 10.00 | | 0.02 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 731.811 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.84 | 13.84 | 0.000 | 152 | 150 | 433.290 | 10.00 | | 0.00 | |

| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|-------------------|-------|-------|-------|-----|-----|----------|-------|--|------|--------|
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.58 | 0.002 | 111 | 113 | 439.096 | 18.45 | | 18.4 | 92.24% |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.10 | 7.08 | 0.001 | 65 | 102 | 385.356 | 19.99 | | 20.0 | 99.95% |
| 55 | toluene-d8 | 9.91 | 9.89 | 0.000 | 98 | 100 | 1597.728 | 17.32 | | 17.3 | 86.62% |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 571.173 | 15.94 | | 15.9 | 79.69% |

| Target Compounds | <<< I1 : ISTD ID = 1 >>> | Qvalue |
|------------------|--------------------------|--------|
| 3 | di-Cl-di-F-methan | 1.89 |
| 4 | Chloromethane | 2.11 |
| 2 | F114 | 2.03 |
| 5 | vinyl chloride | 2.22 |
| 6 | bromomethane | 2.61 |
| 7 | chloroethane | 2.73 |
| 8 | tri-Cl-F-methane | 3.03 |
| 91 | Acetonitrile X10 | 4.07 |
| 9 | acrolein X10 | 3.51 |
| 11 | acetone X10 | 3.71 |
| 12 | ethyl ether X5 | 3.37 |
| 13 | 11-dichloroethene | 3.64 |
| 14 | Iodomethane | 3.81 |
| 15 | F-113 | 3.65 |
| 16 | acrylonitrile X10 | 4.52 |
| 17 | carbon disulfide | 3.90 |
| 94 | Isopropyl Alcohol | 4.01 |
| 18 | methylene chlorid | 4.22 |
| 19 | t-12-di-Cl-ethene | 4.58 |

Handwritten signature/initials

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0020.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 11:22 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:40 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|--------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 20 | t-Bu-Me-ether | 4.59 | 4.56 | 0.004 | 73 | 57 | 751.228 | 17.49 | 17.5 | 93 | ? |
| 95 | Tert butyl alcohol | 4.47 | 4.47 | 0.000 | 59 | 57 | 76.985 | 67.40 | 67.4 | 100 | # |
| 94 | allyl chloride | 4.07 | 4.04 | 0.004 | 41 | 76 | 794.170 | 21.14 | 21.1 | 75 | #? |
| 21 | 11-dichloroethane | 5.12 | 5.09 | 0.004 | 63 | 83 | 689.918 | 16.66 | 16.7 | 98 | # |
| 97 | propionitrile | 6.01 | 5.99 | 0.002 | 54 | 51 | 29.270 | 18.27 | 18.3 | 100 | # |
| 22 | c-12-di-Cl-ethene | 5.92 | 5.89 | 0.003 | 96 | 61 | 436.935 | 16.80 | 16.8 | 90 | ? |
| 23 | 22-Dichloropropan | 5.92 | 5.89 | 0.004 | 77 | 97 | 456.844 | 15.42 | 15.4 | 97 | ? |
| 24 | Br-Cl-methane | 6.25 | 6.23 | 0.003 | 128 | 130 | 215.148 | 17.06 | 17.1 | 93 | ? |
| 25 | chloroform | 6.37 | 6.35 | 0.003 | 83 | 85 | 741.683 | 16.23 | 16.2 | 99 | ? |
| 26 | tetrahydrofuranX5 | 6.34 | 6.32 | 0.002 | 42 | 72 | 317.711 | 101.28 | 101.3 | 84 | ? |
| 98 | Diisopropyl ether | 5.24 | 5.22 | 0.003 | 45 | 87 | 1387.177 | 21.76 | 21.8 | 89 | ? |
| 99 | ETBE | 5.74 | 5.72 | 0.003 | 59 | 87 | 879.689 | 18.05 | 18.1 | 91 | ? |
| 30 | 12-dichloroethane | 7.22 | 7.20 | 0.002 | 64 | 62 | 146.461 | 19.69 | 19.7 | 97 | ? |
| 32 | vinyl acetate X5 | 5.19 | 5.17 | 0.003 | 43 | 86 | 3463.521 | 116.23 | 116.2 | 93 | ? |
| 92 | Nitro Methane (x10 | 5.81 | 5.80 | 0.002 | 61 | 46 | 95.786 | 180.59 | 180.6 | 50 | # |
| 33 | 2-butanoneMEK X10 | 5.94 | 5.92 | 0.003 | 43 | 72 | 956.754 | 192.46 | 192.5 | 86 | ? |
| 93 | Ethyl Acetate x2 | 6.04 | 6.02 | 0.002 | 43 | 61 | 465.630 | 39.33 | 39.3 | 97 | ? |
| 34 | 111-trichloroetha | 6.65 | 6.63 | 0.002 | 97 | 99 | 629.233 | 16.35 | 16.4 | 100 | ? |
| 35 | 11-Di-Cl-propene | 6.90 | 6.88 | 0.002 | 75 | 110 | 484.228 | 16.65 | 16.7 | 89 | ? |
| 36 | benzene | 7.21 | 7.19 | 0.003 | 78 | 52 | 1581.767 | 16.32 | 16.3 | 90 | ? |
| 37 | CCl4 | 6.91 | 6.89 | 0.002 | 117 | 119 | 555.550 | 15.66 | 15.7 | 98 | ? |
| 100 | Isobutyl alcohol | 7.41 | 7.39 | 0.002 | 43 | 42 | 247.109 | 629.22 | 629.2 | 82 | #? |
| 38 | thiophene | 7.53 | 7.51 | 0.002 | 84 | 58 | 868.274 | 18.02 | 18.0 | 92 | ? |
| 39 | 12-di-Cl-propane | 8.56 | 8.54 | 0.002 | 63 | 76 | 370.946 | 17.10 | 17.1 | 99 | ? |
| 40 | trichloroethene | 8.24 | 8.23 | 0.002 | 130 | 132 | 501.517 | 16.60 | 16.6 | 90 | ? |
| 41 | dibromomethane | 8.73 | 8.71 | 0.002 | 174 | 172 | 247.759 | 18.01 | 18.0 | 99 | ? |
| 101 | TAME | 7.41 | 7.39 | 0.002 | 73 | 43 | 716.981 | 16.97 | 17.0 | 89 | #? |
| 42 | Br-di-Cl-methane | 8.96 | 8.95 | 0.002 | 83 | 85 | 546.104 | 17.46 | 17.5 | 99 | ? |
| 43 | Me-methacrylate | 8.76 | 8.75 | 0.000 | 69 | 100 | 188.318 | 19.26 | 19.3 | 88 | ? |
| 44 | 2-ClEt-Vi-ether10 | 9.38 | 9.37 | 0.000 | 63 | 43 | 591.932 | 313.58 | 313.6 | 85 | ? |
| 45 | c-13-di-Cl-propen | 9.56 | 9.55 | 0.002 | 75 | 110 | 608.486 | 19.30 | 19.3 | 91 | ? |
| 46 | t-1,3-dichloropro | 10.25 | 10.24 | 0.000 | 75 | 110 | 505.285 | 20.16 | 20.2 | 93 | ? |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Date: C:\MSDCHEM\1\DATA\03G4612\3-0020.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 11:22 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:40 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|---------------------------|-------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| <<< I2 : ISTD ID = 47 >>> | | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.45 | 10.45 | 0.000 | 97 | 83 | 308.164 | 17.45 | 17.4 | 96 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.64 | 0.000 | 76 | 78 | 479.955 | 17.23 | 17.2 | 99 | |
| 50 | Et methacrylate | 10.38 | 10.37 | 0.000 | 69 | 99 | 404.574 | 20.25 | 20.2 | 91 | ? |
| 51 | di-Br-Cl-methane | 10.91 | 10.90 | 0.000 | 129 | 127 | 430.191 | 18.11 | 18.1 | 99 | |
| 52 | bromoform | 12.41 | 12.41 | 0.000 | 173 | 174 | 257.402 | 18.99 | 19.0 | 100 | |
| 53 | 1,4-dichlorobutan | 12.67 | 12.67 | 0.000 | 55 | 41 | 530.472 | 20.46 | 20.5 | 97 | |
| 54 | MIBK | 9.77 | 9.76 | 0.000 | 43 | 58 | 244.409 | 22.93 | 22.9 | 97 | |
| 56 | toluene | 9.99 | 9.98 | 0.000 | 91 | 92 | 1867.212 | 17.62 | 17.6 | 99 | |
| 57 | 2-hexanone X5 | 10.76 | 10.75 | 0.000 | 43 | 58 | 806.303 | 111.46 | 111.5 | 96 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 322.735 | 18.52 | 18.5 | 93 | |
| 59 | tetra-Cl-ethene | 10.64 | 10.64 | 0.000 | 166 | 168 | 498.130 | 15.73 | 15.7 | 97 | ? |
| 60 | chlorobenzene | 11.58 | 11.57 | 0.000 | 112 | 77 | 1307.160 | 17.31 | 17.3 | 92 | ? |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 487.380 | 18.07 | 18.1 | 99 | |
| <<< I3 : ISTD ID = 62 >>> | | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 181.129 | 12.82 | 12.8 | 74 | #? |
| 64 | Et-Bz | 11.70 | 11.69 | 0.000 | 91 | 106 | 2162.672 | 15.95 | 16.0 | 95 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 3322.945 | 32.42 | 32.4 | 97 | |
| 66 | styrene | 12.24 | 12.23 | 0.000 | 104 | 78 | 1448.349 | 18.59 | 18.6 | 95 | ? |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 1715.323 | 16.68 | 16.7 | 97 | ? |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 333.638 | 14.58 | 14.6 | 99 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.91 | 0.000 | 110 | 97 | 111.098 | 16.21 | 16.2 | 97 | ? |
| 71 | isopropylbenzene | 12.60 | 12.59 | 0.000 | 105 | 120 | 2257.352 | 17.14 | 17.1 | 99 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 577.972 | 16.34 | 16.3 | 99 | ? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 58.909 | 17.70 | 17.7 | 85 | ? |
| 73 | n-propylbenzene | 13.00 | 12.99 | 0.000 | 120 | 78 | 656.540 | 15.91 | 15.9 | 94 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 558.317 | 15.31 | 15.3 | 100 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.18 | 0.000 | 126 | 128 | 566.381 | 15.27 | 15.3 | 99 | ? |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 2008.540 | 17.71 | 17.7 | 96 | ? |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 2111.126 | 16.67 | 16.7 | 98 | ? |
| 78 | 124-tri-Me-Benzen | 13.51 | 13.51 | 0.000 | 105 | 120 | 2103.275 | 17.81 | 17.8 | 97 | ? |
| 79 | tert-butylbenzene | 13.47 | 13.47 | 0.000 | 119 | 91 | 1736.357 | 16.03 | 16.0 | 97 | |


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0020.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 11:22 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:40 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.78 | 0.000 | 146 | 148 | 1176.380 | 15.82 | 15.8 | 97 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 2530.666 | 16.61 | 16.6 | 98 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 1184.125 | 15.62 | 15.6 | 96 | |
| 83 | Cl-benzyl | 13.98 | 13.98 | 0.000 | 126 | 91 | 106.539 | 14.86 | 14.9 | 84 | # |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 1055.514 | 15.94 | 15.9 | 97 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 567.085 | 16.79 | 16.8 | 82 | ##? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 83.208 | 17.84 | 17.8 | 98 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 702.123 | 16.37 | 16.4 | 99 | |
| 88 | naphthalene | 15.78 | 15.78 | 0.000 | 128 | 129 | 1159.824 | 14.90 | 14.9 | 99 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 360.400 | 13.88 | 13.9 | 98 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 600.915 | 15.62 | 15.6 | 97 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0020.D
Method : C:\MSDCHEM\1\METHODS\E524A003.M
Acq. Time : Oct 21 11:22 2003
Method Update: Mon Oct 27 13:48 2003
Quant. Time : Oct 27 13:40 2003
Print Time : Mon Oct 27 13:50 2003
Miscellaneous :
Sample : F=1
Inst. : GCMS-A
RF via : Multiple Level Calibration
Operator: zou
Multiplier: 1.000000

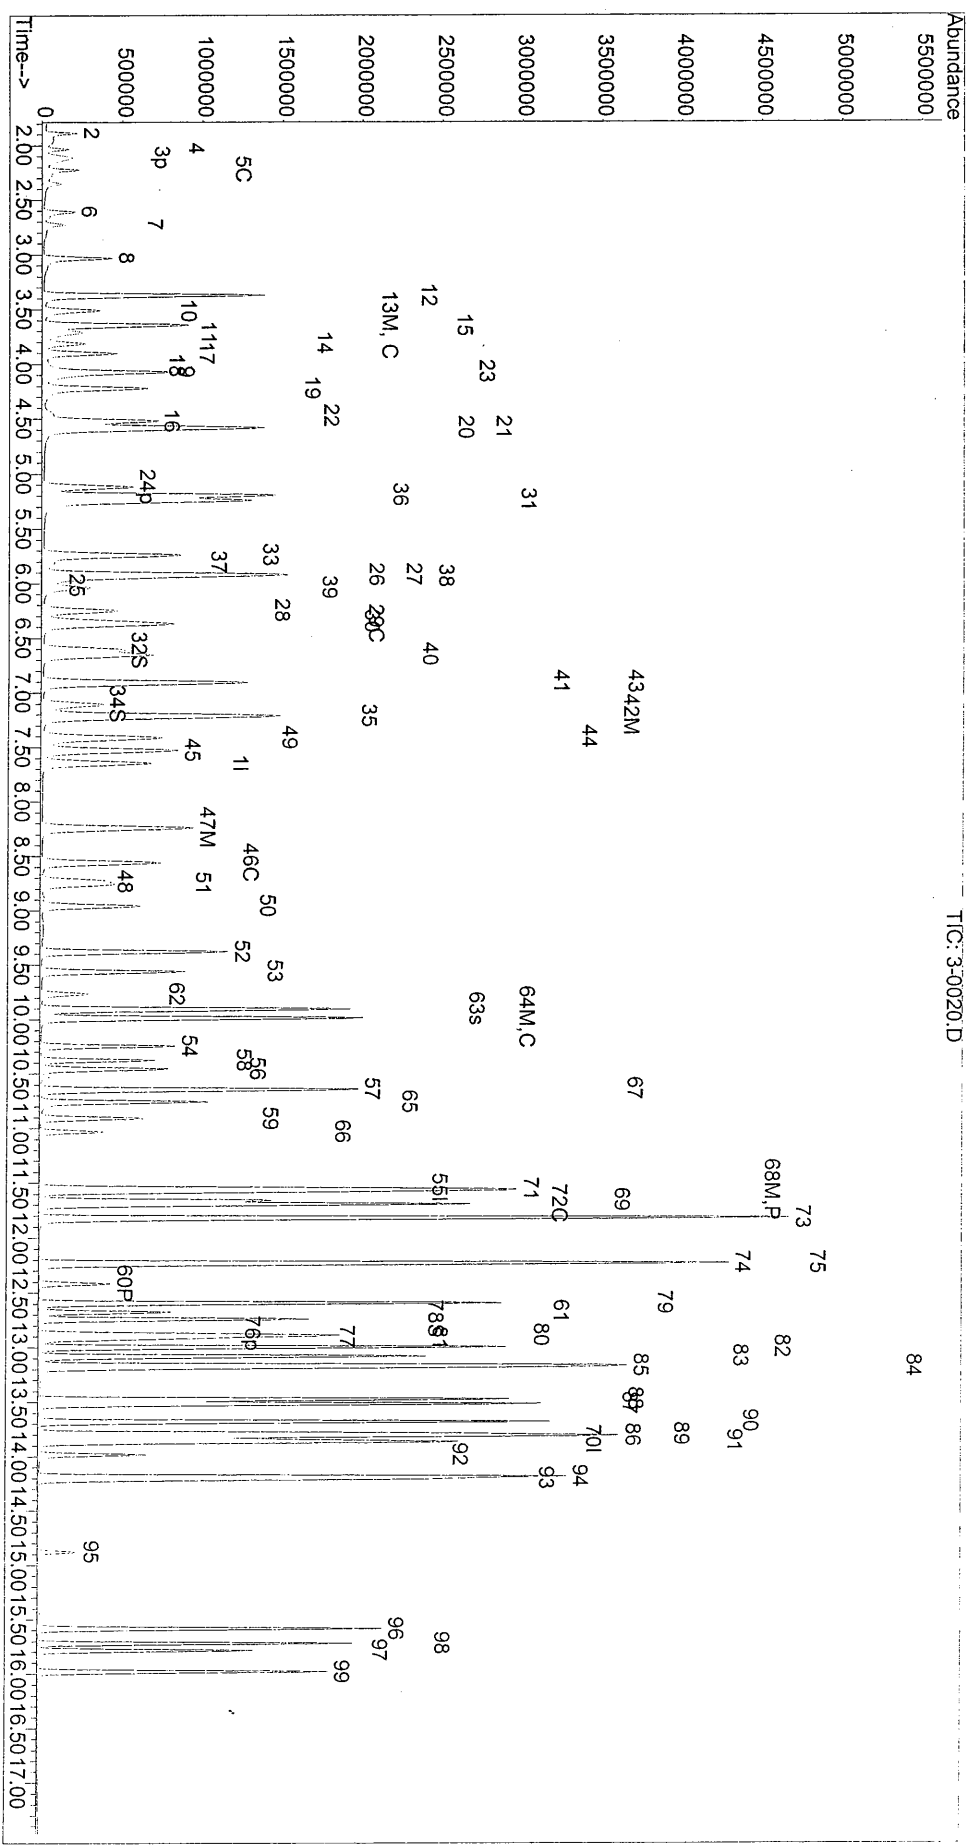

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0040.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E5224A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 11:47 2003 RF Via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:43 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | QIon | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|--------------------|-------|-------|-------|------|-----|----------|---------|--------|---------|------------------|
| 20 | t-Bu-Me-ether | 4.60 | 4.56 | 0.005 | 73 | 57 | 1592.599 | 39.05 | 39.0 | 94 | |
| 95 | Tert butyl alcohol | 4.58 | 4.47 | 0.014 | 59 | 57 | 452.680 | 417.24 | 417.2 | 100 | |
| 94 | allyl chloride | 4.07 | 4.04 | 0.004 | 41 | 76 | 1724.483 | 48.32 | 48.3 | 72 | #26 #10/27/03 |
| 21 | 11-dichloroethane | 5.12 | 5.09 | 0.004 | 63 | 83 | 1398.310 | 35.56 | 35.6 | 99 | |
| 97 | propionitrile | 6.03 | 5.99 | 0.004 | 54 | 51 | 62.391 | 41.00 | 41.0 | 100 | #? |
| 22 | c-12-di-Cl-ethene | 5.92 | 5.89 | 0.003 | 96 | 61 | 845.644 | 34.23 | 34.2 | 94 | ?? |
| 23 | 22-Dichloropropan | 5.92 | 5.89 | 0.004 | 77 | 97 | 979.998 | 34.83 | 34.8 | 100 | ?? |
| 24 | Br-Cl-methane | 6.25 | 6.23 | 0.003 | 128 | 130 | 438.926 | 36.64 | 36.6 | 96 | |
| 25 | chloroform | 6.38 | 6.35 | 0.003 | 83 | 85 | 1492.648 | 34.39 | 34.4 | 99 | |
| 26 | tetrahydrofuranX5 | 6.35 | 6.32 | 0.003 | 42 | 72 | 726.346 | 243.80 | 243.8 | 81 | |
| 98 | Diisopropyl ether | 5.24 | 5.22 | 0.003 | 45 | 87 | 2723.439 | 44.98 | 45.0 | 88 | |
| 99 | ETBE | 5.74 | 5.72 | 0.003 | 59 | 87 | 1934.215 | 41.79 | 41.8 | 90 | |
| 30 | 12-dichloroethane | 7.22 | 7.20 | 0.003 | 64 | 62 | 303.955 | 43.02 | 43.0 | 92 | ?? |
| 32 | vinyl acetate X5 | 5.20 | 5.17 | 0.004 | 43 | 86 | 7301.957 | 257.99 | 258.0 | 91 | |
| 92 | Nitro Methane(x10 | 5.84 | 5.80 | 0.006 | 61 | 46 | 134.103 | 266.20 | 266.2 | 67 | # |
| 33 | 2-butanoneMEK X10 | 5.95 | 5.92 | 0.004 | 43 | 72 | 2014.463 | 426.65 | 426.7 | 85 | |
| 93 | Ethyl Acetate x2 | 6.04 | 6.02 | 0.003 | 43 | 61 | 1199.719 | 106.69 | 106.7 | 99 | ?? |
| 34 | 111-trichloroetha | 6.65 | 6.63 | 0.002 | 97 | 99 | 1352.461 | 37.01 | 37.0 | 99 | |
| 35 | 11-Di-Cl-propene | 6.90 | 6.88 | 0.002 | 75 | 110 | 1020.849 | 36.97 | 37.0 | 92 | ?? |
| 36 | benzene | 7.21 | 7.19 | 0.003 | 78 | 52 | 3067.808 | 33.32 | 33.3 | 92 | ?? |
| 37 | CCl4 | 6.91 | 6.89 | 0.003 | 117 | 119 | 1228.562 | 36.46 | 36.5 | 99 | ?? |
| 100 | Isobutyl alcohol | 7.41 | 7.39 | 0.002 | 43 | 42 | 552.842 | 1482.14 | 1482.1 | 86 | #? |
| 38 | thiophene | 7.53 | 7.51 | 0.003 | 84 | 58 | 1718.044 | 37.54 | 37.5 | 92 | |
| 39 | 12-di-Cl-propane | 8.56 | 8.54 | 0.002 | 63 | 76 | 752.605 | 36.53 | 36.5 | 96 | |
| 40 | trichloroethene | 8.24 | 8.23 | 0.002 | 130 | 132 | 1020.048 | 35.54 | 35.5 | 90 | |
| 41 | dibromomethane | 8.73 | 8.71 | 0.002 | 174 | 172 | 508.912 | 38.94 | 38.9 | 100 | |
| 101 | TAME | 7.41 | 7.39 | 0.002 | 73 | 43 | 1622.049 | 40.42 | 40.4 | 89 | #? |
| 42 | Br-di-Cl-methane | 8.96 | 8.95 | 0.002 | 83 | 85 | 1129.675 | 38.03 | 38.0 | 100 | |
| 43 | Me-methacrylate | 8.76 | 8.75 | 0.002 | 69 | 100 | 435.160 | 46.87 | 46.9 | 88 | |
| 44 | 2-ClEt-Vi-ether10 | 9.38 | 9.37 | 0.002 | 63 | 43 | 1294.105 | 721.80 | 721.8 | 82 | |
| 45 | c-13-di-Cl-propen | 9.56 | 9.55 | 0.002 | 75 | 110 | 1252.896 | 41.84 | 41.8 | 91 | |
| 46 | t-1,3-dichloropro | 10.25 | 10.24 | 0.000 | 75 | 110 | 1067.475 | 44.83 | 44.8 | 93 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0040.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 11:47 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:43 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|---------------------------|-------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| <<< I2 : ISTD ID = 47 >>> | | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.46 | 10.45 | 0.000 | 97 | 83 | 644.393 | 40.50 | 40.5 | 94 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.64 | 0.001 | 76 | 78 | 958.048 | 38.17 | 38.2 | 100 | ? |
| 50 | Et methacrylate | 10.37 | 10.37 | 0.000 | 69 | 99 | 897.662 | 49.86 | 49.9 | 91 | |
| 51 | di-Br-Cl-methane | 10.91 | 10.90 | 0.000 | 129 | 127 | 895.491 | 41.85 | 41.8 | 99 | |
| 52 | bromoform | 12.42 | 12.41 | 0.000 | 173 | 174 | 537.161 | 43.98 | 44.0 | 100 | |
| 53 | 1,4-dichlorobutan | 12.67 | 12.67 | 0.000 | 55 | 41 | 1118.631 | 47.88 | 47.9 | 96 | |
| 54 | MIBK | 9.77 | 9.76 | 0.000 | 43 | 58 | 567.049 | 59.05 | 59.1 | 97 | |
| 56 | toluene | 9.99 | 9.98 | 0.001 | 91 | 92 | 3679.239 | 38.53 | 38.5 | 100 | |
| 57 | 2-hexanone X5 | 10.76 | 10.75 | 0.000 | 43 | 58 | 1789.801 | 274.61 | 274.6 | 92 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 683.020 | 43.51 | 43.5 | 98 | |
| 59 | tetra-Cl-ethene | 10.65 | 10.64 | 0.001 | 166 | 168 | 1001.817 | 35.11 | 35.1 | 98 | ? |
| 60 | chlorobenzene | 11.58 | 11.57 | 0.000 | 112 | 77 | 2492.370 | 36.63 | 36.6 | 93 | ? |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 969.491 | 39.89 | 39.9 | 97 | |
| <<< I3 : ISTD ID = 62 >>> | | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 379.300 | 29.16 | 29.2 | 63 | #? |
| 64 | Et-Bz | 11.70 | 11.69 | 0.000 | 91 | 106 | 4307.205 | 34.51 | 34.5 | 97 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 6407.191 | 67.91 | 67.9 | 98 | |
| 66 | styrene | 12.24 | 12.23 | 0.000 | 104 | 78 | 2712.603 | 37.82 | 37.8 | 99 | ? |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 3289.680 | 34.76 | 34.8 | 100 | ? |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 679.431 | 32.25 | 32.2 | 98 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.91 | 0.000 | 110 | 97 | 231.129 | 36.65 | 36.6 | 92 | ? |
| 71 | isopropylbenzene | 12.60 | 12.59 | 0.000 | 105 | 120 | 4576.796 | 37.74 | 37.7 | 96 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 1123.002 | 34.48 | 34.5 | 98 | ? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 138.278 | 45.13 | 45.1 | 84 | #? |
| 73 | n-propylbenzene | 13.00 | 12.99 | 0.000 | 120 | 78 | 1290.074 | 33.97 | 34.0 | 96 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 1084.812 | 32.32 | 32.3 | 98 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.18 | 0.000 | 126 | 128 | 1062.470 | 31.12 | 31.1 | 99 | ? |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 3906.361 | 37.42 | 37.4 | 94 | ? |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 4215.398 | 36.16 | 36.2 | 99 | ? |
| 78 | 124-tri-Me-Benzen | 13.52 | 13.51 | 0.000 | 105 | 120 | 4147.713 | 38.15 | 38.2 | 94 | ? |
| 79 | tert-butylbenzene | 13.48 | 13.47 | 0.000 | 119 | 91 | 3598.467 | 36.10 | 36.1 | 96 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06


Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-004.v.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 11:47 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:43 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.78 | 0.000 | 146 | 148 | 2227.519 | 32.53 | 32.5 | 98 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 5231.475 | 37.29 | 37.3 | 100 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 2334.471 | 33.46 | 33.5 | 96 | |
| 83 | Cl-benzy1 | 13.98 | 13.98 | 0.000 | 126 | 91 | 268.318 | 40.67 | 40.7 | 84 | # |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 2046.326 | 33.56 | 33.6 | 99 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 1127.859 | 36.28 | 36.3 | 87 | #? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 177.685 | 41.39 | 41.4 | 99 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 1402.301 | 35.52 | 35.5 | 100 | |
| 88 | naphthalene | 15.78 | 15.78 | 0.000 | 128 | 129 | 2506.296 | 34.99 | 35.0 | 99 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 746.186 | 31.22 | 31.2 | 97 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 1229.181 | 34.70 | 34.7 | 97 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0040.D
Method : C:\MSDCHEM\1\METHODS\E524A003.M
Acq. Time : Oct 21 11:47 2003
Method Update: Mon Oct 27 13:48 2003
Quant. Time : Oct 27 13:43 2003
Print Time : Mon Oct 27 13:50 2003
Miscellaneous :

Sample : F=1
Inst. : GCMS-A
RF via : Multiple Level Calibration
Operator: zou
Multiplier: 1.000000

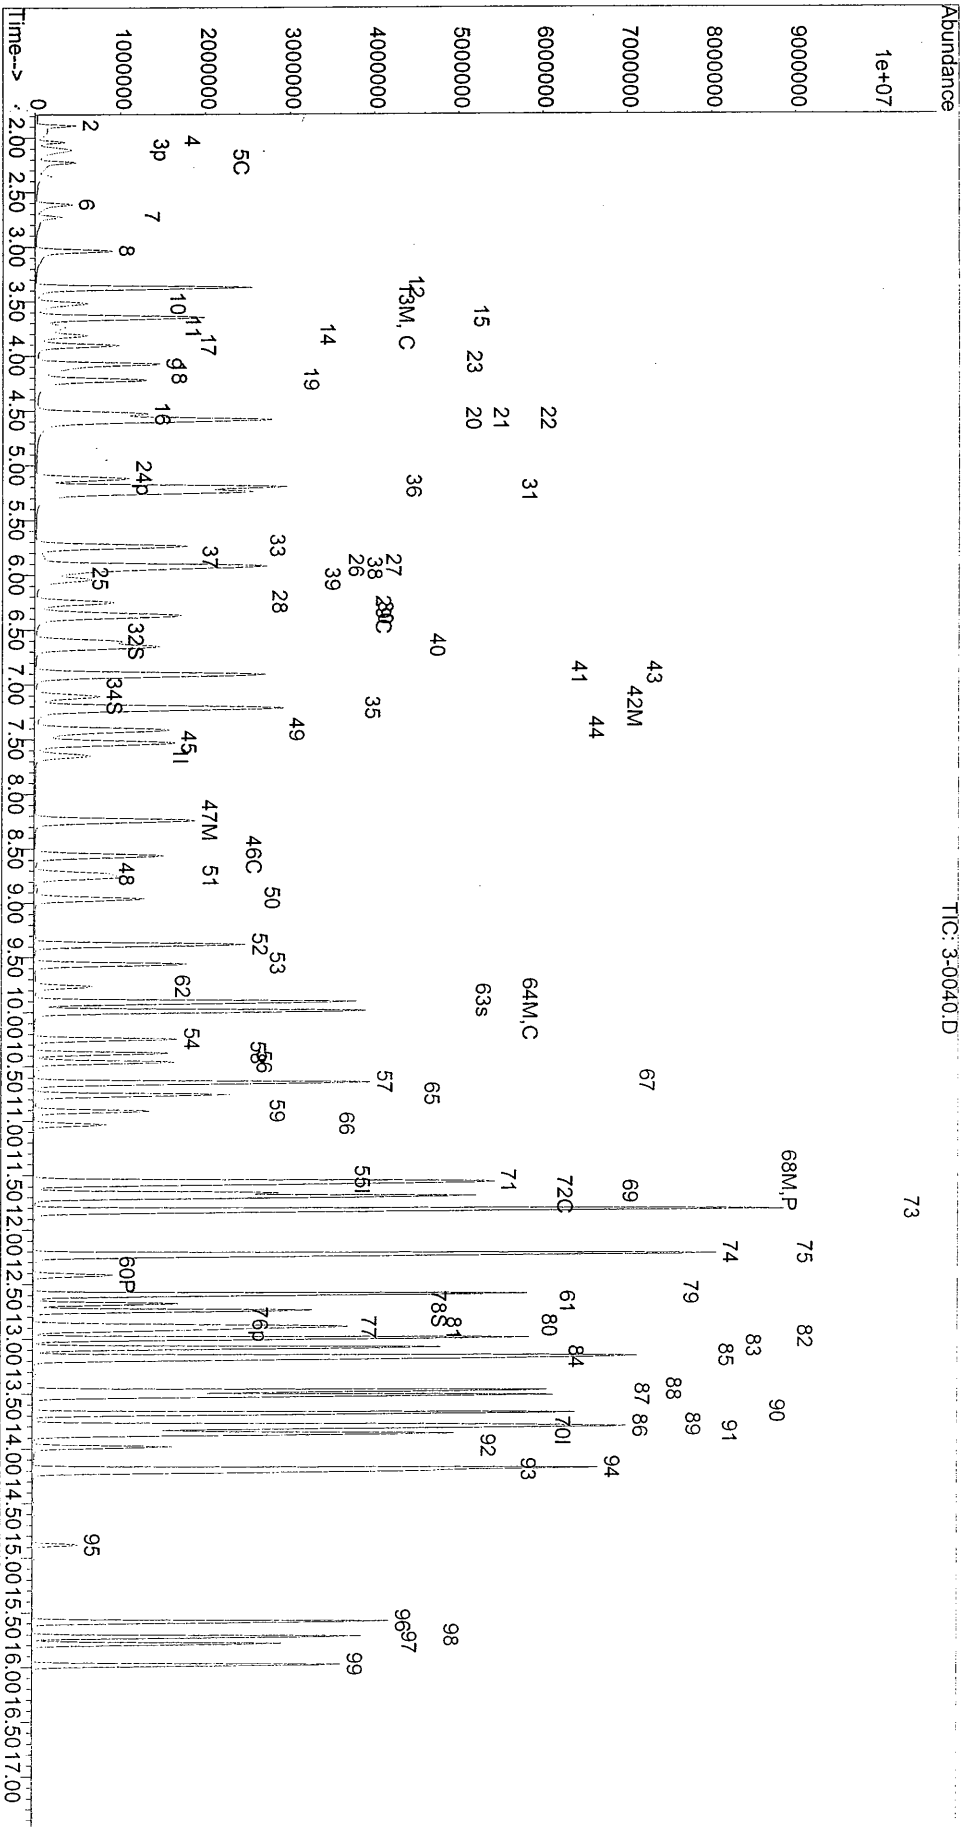

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0060.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 12:14 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:45 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------------------|-------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.65 | 7.63 | 0.003 | 96 | 70 | 1006.211 | 10.00 | | 0.02 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 705.610 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.85 | 13.84 | 0.000 | 152 | 150 | 428.493 | 10.00 | | 0.00 | |

| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|-------------------|-------|-------|-------|-----|-----|----------|-------|--|------|---------|
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.58 | 0.002 | 111 | 113 | 1314.263 | 52.41 | | 52.4 | 262.06% |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.11 | 7.08 | 0.002 | 65 | 102 | 1206.050 | 59.38 | | 59.4 | 296.92% |
| 55 | toluene-d8 | 9.91 | 9.89 | 0.000 | 98 | 100 | 4699.033 | 52.84 | | 52.8 | 264.21% |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 1638.683 | 46.24 | | 46.2 | 231.18% |

| Target Compounds | <<< I1 : ISTD ID = 1 >>> | Qvalue |
|------------------|--------------------------|---|
| 3 | di-Cl-di-F-methan | 1.89 1.85 0.005 85 87 1099.511 43.53 43.5 100 |
| 4 | Chloromethane | 2.11 2.07 0.005 50 52 1132.557 54.69 54.7 98 |
| 2 | F114 | 2.03 2.00 0.005 85 135 551.592 41.76 41.8 32 |
| 5 | vinyl chloride | 2.22 2.19 0.004 62 64 982.033 40.26 40.3 99 |
| 6 | bromomethane | 2.61 2.58 0.005 94 96 601.141 51.30 51.3 98 |
| 7 | chloroethane | 2.73 2.70 0.004 64 66 536.590 36.96 37.0 0 |
| 8 | tri-Cl-F-methane | 3.03 3.00 0.005 101 103 1532.166 42.41 42.4 99 |
| 91 | Acetonitrile X10 | 4.07 4.04 0.004 41 40 2428.244 550.07 550.1 95 |
| 9 | acrolein X10 | 3.51 3.48 0.005 56 55 1232.252 535.84 535.8 100 |
| 11 | acetone X10 | 3.72 3.69 0.004 43 58 1816.586 837.75 837.8 0 |
| 12 | ethyl ether X5 | 3.37 3.34 0.004 59 74 2654.028 257.12 257.1 77 |
| 13 | 11-dichloroethene | 3.64 3.60 0.005 61 96 1367.991 47.43 47.4 0 |
| 14 | Iodomethane | 3.81 3.78 0.004 142 127 1123.042 44.04 44.0 95 |
| 15 | F-113 | 3.65 3.62 0.005 101 151 784.890 40.46 40.5 86 |
| 16 | acrylonitrile X10 | 4.52 4.49 0.004 53 52 2532.493 563.01 563.0 97 |
| 17 | carbon disulfide | 3.90 3.87 0.004 76 78 2561.651 34.93 34.9 100 |
| 94 | Isopropyl Alcohol | 4.05 4.01 0.006 45 43 128.634 203.26 203.3 100 |
| 18 | methylene chlorid | 4.22 4.19 0.004 84 49 1192.483 48.64 48.6 74 |
| 19 | t-12-di-Cl-ethene | 4.58 4.55 0.004 96 61 1126.298 41.44 41.4 84 |

Handwritten signature and date: 10/27/03

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0060.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 12:14 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:45 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscelaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|-------------------|-------|-------|-------|------|-----|-----------|---------|--------|---------|------|
| 20 | t-Bu-Me-ether | 4.59 | 4.56 | 0.004 | 73 | 57 | 2437.498 | 53.88 | 53.9 | 92 | ? |
| 95 | Tert butyl alcoho | 4.48 | 4.47 | 0.002 | 59 | 57 | 251.872 | 209.71 | 209.7 | 100 | # |
| 94 | allyl chloride | 4.07 | 4.04 | 0.004 | 41 | 76 | 2428.244 | 61.34 | 61.3 | 72 | #? |
| 21 | 11-dichloroethane | 5.12 | 5.09 | 0.004 | 63 | 83 | 2101.878 | 48.19 | 48.2 | 100 | #? |
| 97 | propionitrile | 6.01 | 5.99 | 0.002 | 54 | 51 | 109.975 | 65.15 | 65.2 | 100 | #? |
| 22 | c-12-di-Cl-ethene | 5.92 | 5.89 | 0.003 | 96 | 61 | 1210.430 | 44.17 | 44.2 | 93 | ? |
| 23 | 22-Dichloropropan | 5.92 | 5.89 | 0.003 | 77 | 97 | 1513.030 | 56.27 | 56.3 | 98 | ? |
| 24 | Br-Cl-methane | 6.25 | 6.23 | 0.003 | 128 | 130 | 655.419 | 49.32 | 49.3 | 97 | ? |
| 25 | chloroform | 6.37 | 6.35 | 0.002 | 83 | 85 | 2229.387 | 54.70 | 54.7 | 99 | ? |
| 26 | tetrahydrofuranX5 | 6.34 | 6.32 | 0.002 | 42 | 72 | 1114.014 | 337.11 | 337.1 | 81 | # |
| 98 | Diisopropyl ether | 5.24 | 5.22 | 0.003 | 45 | 87 | 4088.155 | 60.87 | 60.9 | 87 | # |
| 99 | ETBE | 5.74 | 5.72 | 0.003 | 59 | 87 | 2984.281 | 58.13 | 58.1 | 90 | # |
| 30 | 12-dichloroethane | 7.22 | 7.20 | 0.003 | 64 | 62 | 463.659 | 65.98 | 66.0 | 99 | ? |
| 32 | vinyl acetate X5 | 5.20 | 5.17 | 0.004 | 43 | 86 | 11062.661 | 352.38 | 352.4 | 90 | ? |
| 92 | Nitro Methane(x10 | 5.82 | 5.80 | 0.002 | 61 | 46 | 298.076 | 533.44 | 533.4 | 95 | ? |
| 33 | 2-butanoneMEK X10 | 5.95 | 5.92 | 0.003 | 43 | 72 | 3034.414 | 734.41 | 734.4 | 85 | ? |
| 93 | Ethyl Acetate x2 | 6.04 | 6.02 | 0.002 | 43 | 61 | 1687.653 | 154.04 | 154.0 | 98 | ? |
| 34 | 111-trichloroetha | 6.65 | 6.63 | 0.002 | 97 | 99 | 2070.811 | 51.08 | 51.1 | 98 | ? |
| 35 | 11-Di-Cl-propene | 6.91 | 6.88 | 0.003 | 75 | 110 | 1516.179 | 49.50 | 49.5 | 88 | ? |
| 36 | benzene | 7.21 | 7.19 | 0.003 | 78 | 52 | 4519.766 | 44.25 | 44.3 | 90 | ? |
| 37 | CCl4 | 6.91 | 6.89 | 0.003 | 117 | 119 | 1842.053 | 49.28 | 49.3 | 99 | ? |
| 100 | Isobutyl alcohol | 7.41 | 7.39 | 0.002 | 43 | 42 | 880.424 | 1806.00 | 1806.0 | 99 | ? |
| 38 | thiophene | 7.53 | 7.51 | 0.003 | 84 | 58 | 2554.816 | 50.32 | 50.3 | 93 | ? |
| 39 | 12-di-Cl-propane | 8.56 | 8.54 | 0.002 | 63 | 76 | 1124.998 | 49.23 | 49.2 | 97 | ? |
| 40 | trichloroethene | 8.24 | 8.23 | 0.002 | 130 | 132 | 1520.360 | 47.76 | 47.8 | 92 | ? |
| 41 | dibromomethane | 8.73 | 8.71 | 0.002 | 174 | 172 | 747.601 | 51.57 | 51.6 | 99 | ? |
| 101 | TAME | 7.41 | 7.39 | 0.002 | 73 | 43 | 2525.816 | 56.74 | 56.7 | 88 | #? |
| 42 | Br-di-Cl-methane | 8.96 | 8.95 | 0.002 | 83 | 85 | 1703.118 | 57.00 | 57.0 | 99 | ? |
| 43 | Me-methacrylate | 8.76 | 8.75 | 0.002 | 69 | 100 | 662.734 | 54.98 | 55.0 | 88 | ? |
| 44 | 2-ClEt-Vi-ether10 | 9.38 | 9.37 | 0.002 | 63 | 43 | 1950.851 | 684.59 | 684.6 | 82 | ? |
| 45 | c-13-di-Cl-propen | 9.56 | 9.55 | 0.002 | 75 | 110 | 1891.415 | 56.95 | 57.0 | 94 | ? |
| 46 | t-1,3-dichloropro | 10.25 | 10.24 | 0.000 | 75 | 110 | 1638.452 | 62.04 | 62.0 | 94 | ? |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-006v.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 12:14 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:45 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscleous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------|--------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| <<< I2 | : ISTD ID = 47 >>> | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.46 | 10.45 | 0.000 | 97 | 83 | 936.372 | 54.99 | 55.0 | 95 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.64 | 0.001 | 76 | 78 | 1392.110 | 51.83 | 51.8 | 100 | |
| 50 | Et methacrylate | 10.38 | 10.37 | 0.000 | 69 | 99 | 1374.874 | 61.96 | 62.0 | 92 | ? |
| 51 | di-Br-Cl-methane | 10.91 | 10.90 | 0.000 | 129 | 127 | 1332.246 | 61.52 | 61.5 | 99 | |
| 52 | bromofom | 12.41 | 12.41 | 0.000 | 173 | 174 | 813.031 | 62.20 | 62.2 | 100 | |
| 53 | 1,4-dichlorobutan | 12.68 | 12.67 | 0.000 | 55 | 41 | 1708.578 | 68.33 | 68.3 | 98 | |
| 54 | MIBK | 9.77 | 9.76 | 0.000 | 43 | 58 | 883.730 | 86.00 | 86.0 | 98 | |
| 56 | toluene | 9.99 | 9.98 | 0.001 | 91 | 92 | 5453.434 | 53.36 | 53.4 | 99 | |
| 57 | 2-hexanone X5 | 10.76 | 10.75 | 0.000 | 43 | 58 | 2714.840 | 389.23 | 389.2 | 91 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 1029.927 | 61.31 | 61.3 | 98 | |
| 59 | tetra-Cl-ethene | 10.64 | 10.64 | 0.000 | 166 | 168 | 1436.032 | 47.03 | 47.0 | 97 | ? |
| 60 | chlorobenzene | 11.58 | 11.57 | 0.000 | 112 | 77 | 3536.493 | 53.79 | 53.8 | 95 | ? |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 1437.439 | 55.27 | 55.3 | 95 | |
| <<< I3 | : ISTD ID = 62 >>> | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 546.400 | 39.10 | 39.1 | 57 | #? |
| 64 | Et-Bz | 11.70 | 11.69 | 0.000 | 91 | 106 | 6378.701 | 47.58 | 47.6 | 98 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 9314.343 | 91.90 | 91.9 | 94 | |
| 66 | styrene | 12.24 | 12.23 | 0.000 | 104 | 78 | 3842.415 | 49.86 | 49.9 | 98 | ? |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 4761.198 | 46.82 | 46.8 | 98 | ? |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 1005.365 | 44.41 | 44.4 | 99 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.91 | 0.000 | 110 | 97 | 345.542 | 51.00 | 51.0 | 95 | ? |
| 71 | Isopropylbenzene | 12.60 | 12.59 | 0.000 | 105 | 120 | 6821.750 | 52.36 | 52.4 | 95 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 1610.222 | 46.02 | 46.0 | 100 | ? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 214.154 | 53.26 | 53.3 | 84 | #? |
| 73 | n-propylbenzene | 13.00 | 12.99 | 0.000 | 120 | 78 | 1877.926 | 46.02 | 46.0 | 95 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 1601.091 | 44.40 | 44.4 | 98 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.18 | 0.000 | 126 | 128 | 1497.703 | 40.83 | 40.8 | 99 | ? |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 5670.674 | 50.56 | 50.6 | 91 | ? |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 6174.914 | 49.30 | 49.3 | 97 | ? |
| 78 | 124-tri-Me-Benzen | 13.52 | 13.51 | 0.000 | 105 | 120 | 6124.395 | 52.44 | 52.4 | 93 | |
| 79 | tert-butylbenzene | 13.48 | 13.47 | 0.000 | 119 | 91 | 5289.165 | 49.39 | 49.4 | 98 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06


Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0060.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Oct 21 12:14 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 13:48 2003 Operator: zou
 Quant. Time : Oct 27 13:45 2003 Multiplr: 1.000000
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.78 | 0.000 | 146 | 148 | 3166.301 | 43.04 | 43.0 | 97 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 7732.088 | 51.30 | 51.3 | 99 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 3417.867 | 48.86 | 48.9 | 95 | |
| 83 | Cl-benzyl | 13.98 | 13.98 | 0.000 | 126 | 91 | 431.461 | 60.87 | 60.9 | 98 | |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 2953.834 | 45.10 | 45.1 | 97 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 1596.385 | 43.23 | 43.2 | 93 | ? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 276.212 | 59.89 | 59.9 | 99 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 2085.639 | 49.18 | 49.2 | 96 | |
| 88 | naphthalene | 15.78 | 15.78 | 0.000 | 128 | 129 | 3927.146 | 51.03 | 51.0 | 99 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 1096.494 | 42.70 | 42.7 | 100 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 1798.500 | 47.26 | 47.3 | 99 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4612\3-0060.D
 Method : C:\MSDCHEM\1\METHODS\E524A003.M
 Acq. Time : Oct 21 12:14 2003
 Method Update: Mon Oct 27 13:48 2003
 Quant. Time : Oct 27 13:45 2003
 Print Time : Mon Oct 27 13:50 2003
 Miscellaneous :

Sample : f=1
 Inst. : GCMS-A
 RF via : Multiple Level Calibration
 Operator: zou
 Multiplr: 1.000000

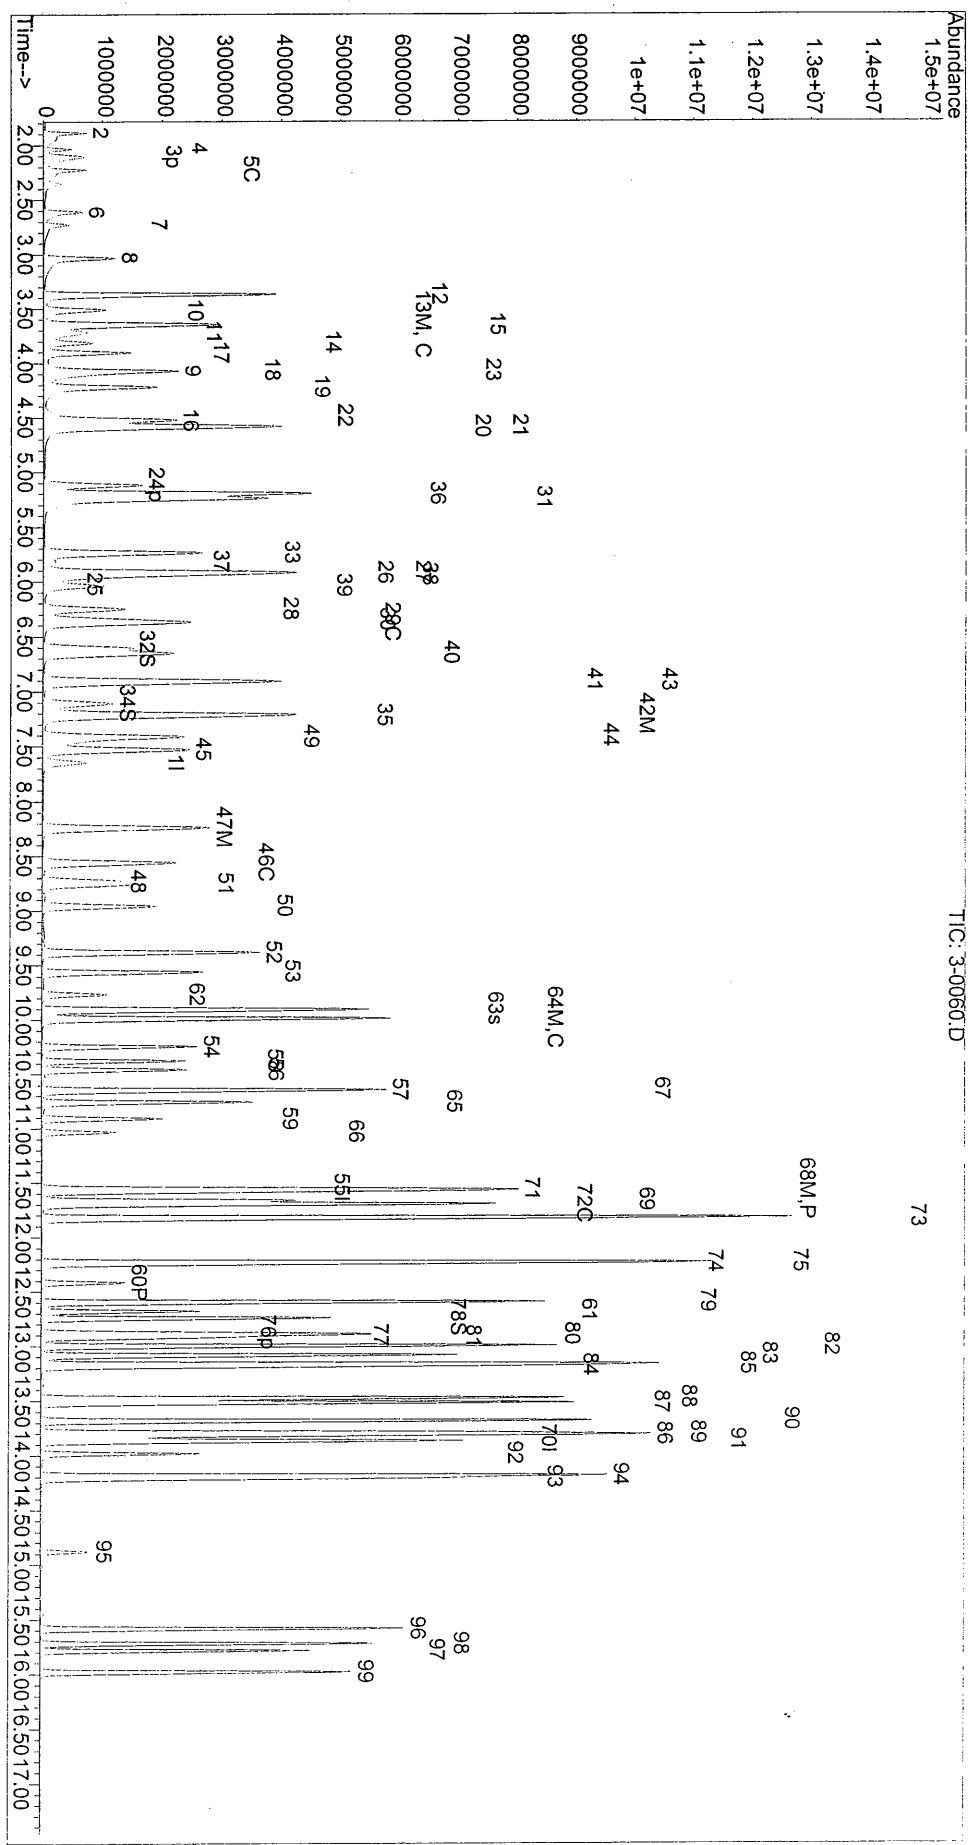


Data File : C:\MSDCHEM\1\DATA\03G4717\G4717P01.D

Vial: 1
Operator: zou
Inst : GCMS-A
Multiplier: 1.00

Acq On : 6 Nov 2003 10:02 am
Sample : ##03g4717, w 50 ng
Misc :

MS Integration Params: Lscint.p
Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
Title : **Applied P & Ch Lab** EPA 524.2

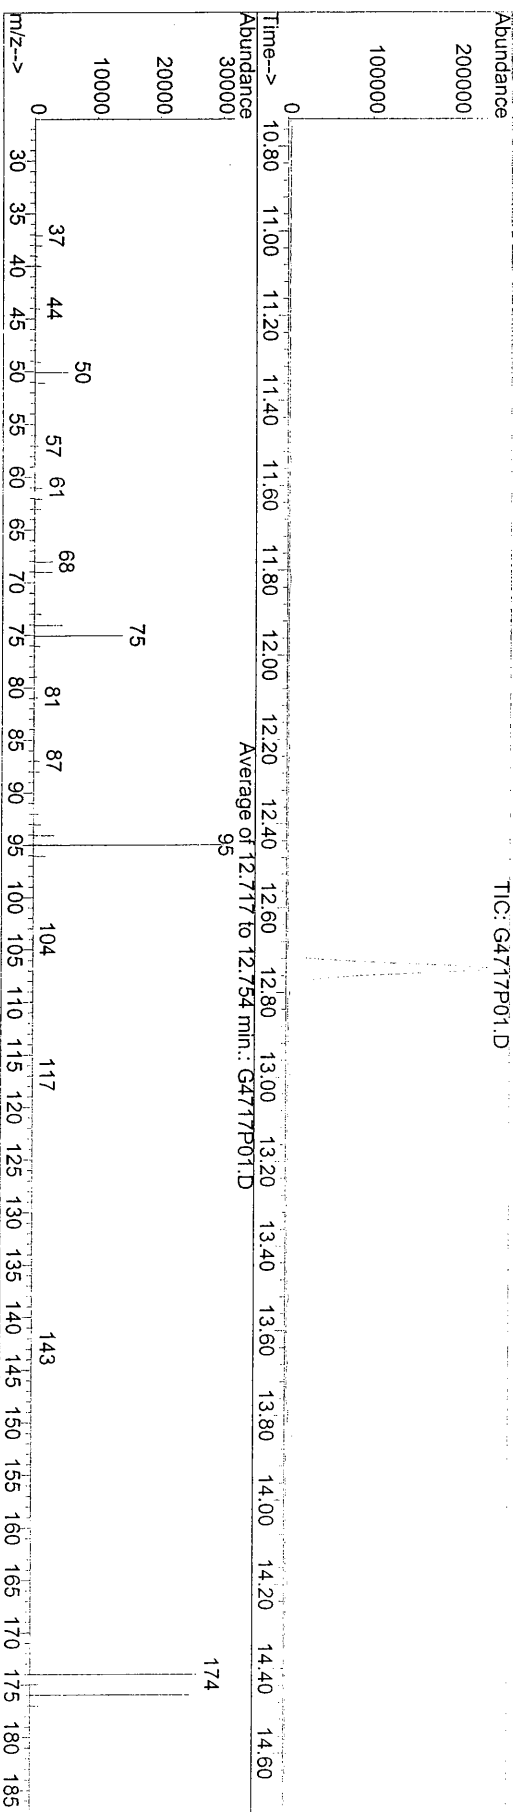

Spectrum Information: Average of 12.717 to 12.754 min.

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result |
|-------------|--------------|--------------|--------------|-----------|---------|--------|
| 50 | 95 | 15 | 40 | 17.7 | 5373 | PASS |
| 75 | 95 | 30 | 60 | 46.6 | 14115 | PASS |
| 95 | 95 | 100 | 100 | 100.0 | 30317 | PASS |
| 96 | 95 | 5 | 9 | 6.7 | 2038 | PASS |
| 173 | 174 | 0.00 | 2 | 0.5 | 124 | PASS |
| 174 | 95 | 50 | 100 | 88.2 | 26740 | PASS |
| 175 | 174 | 5 | 9 | 7.7 | 2050 | PASS |
| 176 | 174 | 95 | 101 | 96.2 | 25730 | PASS |
| 177 | 176 | 5 | 9 | 6.2 | 1595 | PASS |

FORM-5A

Applied P & Ch Laboratory

Volatile Organic Instrument Performance Check for Method 524.2

Bromofluorobenzene (BFB), Part II

| | | | | | |
|-----------------|--------------|----------------|-----------------|--------------|---------|
| Client Name: | GEOFON, Inc. | Contract No: | | Lab Code: | APCL |
| Case No: | | SAS No: | | Service ID: | 035951 |
| Project ID: | JPL | BFB Inj. Date: | <u>11/06/03</u> | Batch No: | 03G4717 |
| | | BFB Inj. Time: | <u>10:02</u> | Sequence No: | 03G4717 |
| Project No: | 04-4428.10 | Instrument ID: | A | GC Column: | HP-VOC |
| Data File Name: | G4717P01 | Heated Purge: | (Y/N) N | Column ID: | 0.20 mm |

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS AND STANDARDS:

| # | Client Sample No | Lab Sample ID | Data File Name | Date Analyzed | Time Analyzed |
|----|------------------|----------------|----------------|---------------|---------------|
| 1 | 03G4717-CCV-01 | 03G4717-CCV-01 | G4717Q01 | 11/06/03 | 10:27 |
| 2 | 03G4717-LCS-01 | 03G4717-LCS-01 | G4717L01 | 11/06/03 | 10:53 |
| 3 | MW-3-1MS | 03-5973-2MS | G4717M01 | 11/06/03 | 11:19 |
| 4 | MW-3-1MSD | 03-5973-2MSD | G4717N01 | 11/06/03 | 11:44 |
| 5 | 03G4717-MB-01 | 03G4717-MB-01 | G4717K01 | 11/06/03 | 13:54 |
| 6 | TB-9-11-4-03 | 03-5951-13 | 5951-13 | 11/06/03 | 14:20 |
| 7 | DUPE-5-4-Q03 | 03-5951-1 | 5951-01 | 11/06/03 | 16:30 |
| 8 | EB-9-11-4-03 | 03-5951-2 | 5951-02 | 11/06/03 | 16:57 |
| 9 | MW-14-1 | 03-5951-3 | 5951-03 | 11/06/03 | 17:23 |
| 10 | MW-14-2 | 03-5951-4 | 5951-04 | 11/06/03 | 17:49 |
| 11 | MW-14-3 | 03-5951-5 | 5951-05 | 11/06/03 | 18:15 |
| 12 | MW-14-4 | 03-5951-6 | 5951-06 | 11/06/03 | 18:41 |
| 13 | MW-14-5 | 03-5951-7 | 5951-07 | 11/06/03 | 19:07 |
| 14 | MW-17-1 | 03-5951-8 | 5951-08 | 11/06/03 | 19:33 |
| 15 | MW-17-2 | 03-5951-9 | 5951-09 | 11/06/03 | 19:59 |
| 16 | MW-17-3 | 03-5951-10 | 5951-10 | 11/06/03 | 20:25 |
| 17 | MW-17-4 | 03-5951-11 | 5951-11 | 11/06/03 | 20:51 |
| 18 | MW-17-5 | 03-5951-12 | 5951-12 | 11/06/03 | 21:17 |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |
| 23 | | | | | |
| 24 | | | | | |
| 25 | | | | | |

Continuing Calibration Concentration Summary

Data File G4717Q01
Method File E524A003

| <u>Compound Name</u> | <u>Amount</u> | <u>Actual</u> | <u>Units</u> | <u>%Dev</u> | <u>Target Response</u> |
|--------------------------|---------------|---------------|--------------|-------------|------------------------|
| 1 Fluorobenzene | 10 | 10.00 | ppb | 0.00 | 650919 |
| 3 di-Cl-di-F-methane | 20 | 18.22 | ppb | 8.88 | 238592 |
| 4 Chloromethane | 20 | 13.80 | ppb | 30.98 | 179442 |
| 2 F114 | 20 | 20.05 | ppb | 0.27 | 123464 |
| 5 vinyl chloride | 20 | 17.07 | ppb | 14.66 | 189466 |
| 6 bromomethane | 20 | 11.10 | ppb | 44.52 | 69956 |
| 7 chloroethane | 20 | 17.89 | ppb | 10.54 | 106954 |
| 8 tri-Cl-F-methane | 20 | 22.97 | ppb | 14.84 | 421501 |
| 91 Acetonitrile X10 | 200 | 164.55 | ppb | 17.72 | 461496 |
| 9 acrolein X10 | 200 | 164.28 | ppb | 17.86 | 226269 |
| 11 acetone X10 | 200 | 241.05 | ppb | 20.52 | 501271 |
| 12 ethyl ether X5 | 100 | 88.59 | ppb | 11.41 | 547856 |
| 13 1,1-dichloroethane | 20 | 20.53 | ppb | 2.64 | 317434 |
| 14 Iodomethane | 20 | 12.52 | ppb | 37.42 | 158325 |
| 15 F-113 | 20 | 23.05 | ppb | 15.26 | 216223 |
| 16 acrylonitrile X10 | 200 | 157.84 | ppb | 21.08 | 440756 |
| 17 carbon disulfide | 20 | 16.93 | ppb | 15.35 | 498576 |
| 94 Isopropyl Alcoholx10 | 200 | 265.70 | ppb | 32.85 | 35410 |
| 18 methylene chloride | 20 | 17.33 | ppb | 13.37 | 240082 |
| 19 t-1,2-di-Cl-ethene | 20 | 18.20 | ppb | 9.01 | 264471 |
| 20 t-Bu-Me-ether | 20 | 19.39 | ppb | 3.05 | 495885 |
| 95 Tert butyl alcoholx10 | 200 | 319.44 | ppb | 59.72 | 136440 |
| 94 allyl chloride | 20 | 12.76 | ppb | 36.19 | 366268 |
| 21 1,1-dichloroethane | 20 | 18.11 | ppb | 9.43 | 436044 |
| 97 propionitrile | 20 | 16.83 | ppb | 15.84 | 19315 |
| 22 c-1,2-di-Cl-ethene | 20 | 17.76 | ppb | 11.21 | 269178 |
| 23 2,2-Dichloropropane | 20 | 26.43 | ppb | 32.14 | 405964 |
| 24 Br-Cl-methane | 20 | 17.74 | ppb | 11.32 | 135937 |
| 25 chloroform | 20 | 18.79 | ppb | 6.03 | 508556 |
| 26 tetrahydrofuranX5 | 100 | 76.20 | ppb | 23.80 | 171834 |
| 98 Diisopropyl ether | 20 | 17.49 | ppb | 12.54 | 808540 |
| 27 Di-Br-F-Me (surr) | 20 | 19.14 | ppb | 4.30 | 292546 |
| 99 ETBE | 20 | 20.53 | ppb | 2.65 | 598312 |
| 29 1,2-Di-Cl-Et-d4 (S1) | 20 | 19.72 | ppb | 1.38 | 268507 |
| 30 1,1-dichloroethane | 20 | 19.68 | ppb | 1.60 | 103834 |
| 32 vinyl acetate X5 | 100 | 93.02 | ppb | 6.98 | 2098034 |
| 92 Nitro Methane(x10) | 200 | 76.72 | ppb | 61.64 | 58322 |
| 33 2-butanoneMEK X10 | 200 | 191.23 | ppb | 4.39 | 649430 |
| 93 Ethyl Acetate x2 | 40 | 31.52 | ppb | 21.20 | 265051 |
| 34 1,1,1-trichloroethane | 20 | 22.51 | ppb | 12.57 | 512316 |
| 35 1,1-Di-Cl-propene | 20 | 20.75 | ppb | 3.77 | 356458 |
| 36 benzene | 20 | 17.70 | ppb | 11.52 | 974138 |
| 37 CCl4 | 20 | 24.14 | ppb | 20.69 | 505080 |

| <u>Compound Name</u> | <u>Amount</u> | <u>Actual</u> | <u>Units</u> | <u>%Dev</u> | <u>Target Response</u> |
|--------------------------|---------------|---------------|--------------|-------------|------------------------|
| 100 Isobutyl alcoholx10 | 200 | 195.71 | ppb | 2.15 | 163588 |
| 38 thiophene | 20 | 18.31 | ppb | 8.47 | 524615 |
| 39 12-di-Cl-propane | 20 | 17.31 | ppb | 13.47 | 217989 |
| 40 trichloroethene | 20 | 19.19 | ppb | 4.05 | 338447 |
| 41 dibromomethane | 20 | 18.41 | ppb | 7.94 | 161333 |
| 101 TAME | 20 | 18.08 | ppb | 9.61 | 483990 |
| 42 Br-di-Cl-methane | 20 | 19.01 | ppb | 4.97 | 376858 |
| 43 Me-methacrylate | 20 | 15.75 | ppb | 21.26 | 110408 |
| 44 2-ClEt-Vi-ether10 | 200 | 127.89 | ppb | 36.06 | 273681 |
| 45 c-13-di-Cl-propene | 20 | 19.44 | ppb | 2.79 | 388349 |
| 46 t-1,3-dichloropropene | 20 | 19.12 | ppb | 4.39 | 341152 |
| 47 Chlorobezene-d5 | 10 | 10.00 | ppb | 0.00 | 496725 |
| 48 112-tri-Cl-Et | 20 | 17.71 | ppb | 11.45 | 194772 |
| 49 13-di-Cl-propane | 20 | 17.89 | ppb | 10.53 | 301908 |
| 50 Et methacrylate | 20 | 15.88 | ppb | 20.59 | 242544 |

| <u>Compound Name</u> | <u>Amount</u> | <u>Actual</u> | <u>Units</u> | <u>%Dev</u> | <u>Target Response</u> |
|----------------------------|---------------|---------------|--------------|-------------|------------------------|
| 51 di-Br-Cl-methane | 20 | 18.97 | ppb | 5.15 | 296008 |
| 52 bromoform | 20 | 19.27 | ppb | 3.64 | 176864 |
| 53 1,4-dichlorobutane-2 | 20 | 17.76 | ppb | 11.22 | 330045 |
| 54 MIBK | 20 | 14.24 | ppb | 28.78 | 135067 |
| 55 toluene-d8 | 20 | 18.89 | ppb | 5.57 | 1035489 |
| 56 toluene | 20 | 17.78 | ppb | 11.08 | 1196236 |
| 57 2-hexanone X5 | 100 | 82.32 | ppb | 17.68 | 506148 |
| 58 12-dibromoethane | 20 | 18.00 | ppb | 10.02 | 202794 |
| 59 tetra-Cl-ethene | 20 | 21.23 | ppb | 6.16 | 393147 |
| 60 chlorobenzene | 20 | 18.89 | ppb | 5.56 | 866936 |
| 61 1112-tetra-Cl-Et | 20 | 20.40 | ppb | 1.99 | 348480 |
| 62 1,4-Dichlorobenzene-d4 | 10 | 10.00 | ppb | 0.00 | 305376 |
| 63 1-chlorohexane | 20 | 20.02 | ppb | 0.08 | 139579 |
| 64 Et-Bz | 20 | 19.02 | ppb | 4.88 | 1476804 |
| 65 m/p-Xylenes X2 | 40 | 38.77 | ppb | 3.07 | 2328165 |
| 66 styrene | 20 | 18.95 | PPB | 5.23 | 958401 |
| 67 o-xylene | 20 | 19.41 | ppb | 2.93 | 1177124 |
| 68 1122-Tetra-Cl-Et | 20 | 17.06 | ppb | 14.68 | 206349 |
| 69 123-tri-Cl-Pr | 20 | 18.84 | ppb | 5.78 | 75659 |
| 70 4-Br-1-F-Bz (S3) | 20 | 19.24 | ppb | 3.80 | 398140 |
| 71 isopropylbenzene | 20 | 20.42 | ppb | 2.12 | 1655609 |
| 72 bromobenzene | 20 | 19.65 | ppb | 1.74 | 403196 |
| 92 t-1,4-dichloro-2-butene | 20 | 17.50 | ppb | 12.50 | 41711 |
| 73 n-propylbenzene | 20 | 20.72 | ppb | 3.61 | 486356 |
| 74 2-Cl-Toluene | 20 | 19.73 | ppb | 1.37 | 392657 |
| 75 4-Cl-Toluene | 20 | 19.22 | ppb | 3.89 | 393162 |
| 76 135-tri-Me-Benzene | 20 | 20.43 | ppb | 2.15 | 1460395 |
| 77 4-iso-Pr-toluene | 20 | 20.99 | ppb | 4.94 | 1616052 |
| 78 124-tri-Me-Benzene | 20 | 19.88 | ppb | 0.58 | 1488485 |
| 79 tert-butylbenzene | 20 | 21.12 | ppb | 5.59 | 1325271 |
| 80 13-DCB | 20 | 19.38 | ppb | 3.08 | 826362 |
| 81 sec-butylbenzene | 20 | 20.81 | ppb | 4.06 | 1950300 |

| | | | | | |
|---------------------|----|-------|-----|-------|--------|
| 82 14-DCB | 20 | 18.58 | ppb | 7.11 | 828869 |
| 83 Cl-benzyl | 20 | 19.80 | ppb | 0.99 | 92095 |
| 84 12-DCB | 20 | 19.06 | ppb | 4.69 | 744207 |
| 85 n-butylbenzene | 20 | 20.97 | ppb | 4.86 | 426496 |
| 86 12-diBr-2-Cl-Pra | 20 | 18.03 | ppb | 9.85 | 52386 |
| 87 124-tri-Cl-Bz | 20 | 20.36 | ppb | 1.78 | 495011 |
| 88 naphthalene | 20 | 15.77 | ppb | 21.16 | 698457 |
| 89 hx-Cl-butadiene | 20 | 23.45 | ppb | 17.23 | 326253 |
| 90 123-Tri-Cl-Bz | 20 | 20.11 | ppb | 0.57 | 422215 |

Average D % 10.906831

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D
 Acq On : 6 Nov 2003 10:27 am
 Sample : f=1
 Misc :
 MS Integration Params: Lscint.p

Vial: 2
 Operator: zou
 Inst : GCMS-A
 Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Mon Oct 27 14:05:06 2003
 Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 20% Max. Rel. Area : 200%

| Compound | Avgrf | CCRF | %Dev | Area# | Dev(min) |
|----------|-------|-------|--------|-------|----------|
| 1 I | 1.000 | 1.000 | 0.0 | 68 | 0.00 |
| 2 | 0.201 | 0.183 | 9.0 | 79 | 0.00 |
| 3 p | 0.200 | 0.138 | 31.0# | 51 | 0.00 |
| 4 | 0.091 | 0.095 | -4.4 | 79 | 0.00 |
| 5 C | 0.171 | 0.146 | 14.6 | 66 | 0.00 |
| 6 | 0.097 | 0.054 | 44.3# | 42# | 0.00 |
| 7 | 0.092 | 0.082 | 10.9 | 67 | 0.00 |
| 8 | 0.282 | 0.324 | -14.9 | 91 | 0.00 |
| 9 | 0.043 | 0.035 | 18.6 | 58 | 0.00 |
| 10 | 0.021 | 0.017 | 19.0 | 59 | 0.00 |
| 11 | 0.032 | 0.039 | -21.9# | 93 | -0.03 |
| 12 | 0.095 | 0.084 | 11.6 | 63 | 0.00 |
| 13 M, C | 0.238 | 0.244 | -2.5 | 77 | 0.00 |
| 14 | 0.178 | 0.122 | 31.5# | 44# | 0.00 |
| 15 | 0.144 | 0.166 | -15.3 | 97 | 0.00 |
| 16 | 0.043 | 0.034 | 20.9# | 55 | -0.01 |
| 17 | 0.452 | 0.383 | 15.3 | 65 | 0.00 |
| 18 | 0.002 | 0.003 | -50.0# | 123 | -0.17 |
| 19 | 0.248 | 0.184 | 25.8# | 59 | 0.00 |
| 20 | 0.223 | 0.203 | 9.0 | 65 | 0.00 |
| 21 | 0.393 | 0.381 | 3.1 | 66 | 0.00 |
| 22 | 0.007 | 0.010 | -42.9# | 177 | -0.10 |
| 23 | 0.441 | 0.281 | 36.3# | 46# | 0.00 |
| 24 p | 0.370 | 0.335 | 9.5 | 63 | 0.00 |
| 25 | 0.018 | 0.015 | 16.7 | 66 | -0.02 |
| 26 | 0.233 | 0.207 | 11.2 | 62 | 0.00 |

(#) = Out of Range
 G4717Q01.D E524A003.M Thu Nov 06 17:52:21 2003

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D
 Acq On : 6 Nov 2003 10:27 am
 Sample : f=1
 Misc :
 MS Integration Params: Lscint.p
 Vial: 2
 Operator: zou
 Inst : GCMS-A
 Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Mon Oct 27 14:05:06 2003
 Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 20% Max. Rel. Area : 200%

| Compound | AvgrRF | CCRF | %Dev | Area | % Dev | (min) |
|----------|-------------------------|-------|-------|--------|-------|-------|
| 27 | 23 22-Dichloropropane | 0.236 | 0.312 | -32.2# | 89 | 0.00 |
| 28 | 24 Br-Cl-methane | 0.118 | 0.104 | 11.9 | 63 | 0.00 |
| 29 C | 25 chloroform | 0.416 | 0.391 | 6.0 | 69 | 0.00 |
| 30 | 26 tetrahydrofuranX5 | 0.035 | 0.026 | 25.7# | 54 | -0.01 |
| 31 | 98 Diisopropyl ether | 0.710 | 0.621 | 12.5 | 58 | 0.00 |
| 32 S | 27 Di-Br-F-Me (surr) | 0.235 | 0.225 | 4.3 | 67 | 0.00 |
| 33 | 99 ETBE | 0.448 | 0.460 | -2.7 | 68 | 0.00 |
| 34 S | 29 1,2-Di-Cl-Et-d4 (S1) | 0.209 | 0.206 | 1.4 | 70 | 0.00 |
| 35 | 30 12-dichloroethane | 0.081 | 0.080 | 1.2 | 71 | 0.00 |
| 36 | 32 vinyl acetate X5 | 0.346 | 0.322 | 6.9 | 61 | 0.00 |
| 37 | 92 Nitro Methane(x10) | 0.012 | 0.004 | 66.7# | 61 | -0.04 |
| 38 | 33 2-butanoneMEK X10 | 0.052 | 0.050 | 3.8 | 68 | -0.02 |
| 39 | 93 Ethyl Acetate x2 | 0.129 | 0.102 | 20.9# | 57 | 0.00 |
| 40 | 34 111-trichloroethane | 0.350 | 0.394 | -12.6 | 81 | 0.00 |
| 41 | 35 11-Di-Cl-propene | 0.264 | 0.274 | -3.8 | 74 | 0.00 |
| 42 M | 36 benzene | 0.846 | 0.748 | 11.6 | 62 | 0.00 |
| 43 | 37 CCl4 | 0.321 | 0.388 | -20.9# | 91 | 0.00 |
| 44 | 100 Isobutyl alcoholx10 | 0.013 | 0.013 | 0.0 | 66 | 0.00 |
| 45 | 38 thiophene | 0.440 | 0.403 | 8.4 | 60 | 0.00 |
| 46 C | 39 12-di-Cl-propane | 0.194 | 0.167 | 13.9 | 59 | 0.00 |
| 47 M | 40 trichloroethene | 0.271 | 0.260 | 4.1 | 67 | 0.00 |
| 48 | 41 dibromomethane | 0.135 | 0.124 | 8.1 | 65 | 0.00 |
| 49 | 101 TAME | 0.369 | 0.372 | -0.8 | 68 | 0.00 |
| 50 | 42 Br-di-Cl-methane | 0.305 | 0.289 | 5.2 | 69 | 0.00 |
| 51 | 43 Me-methacrylate | 0.093 | 0.085 | 8.6 | 59 | 0.00 |
| 52 | 44 2-ClEt-Vi-ether10 | 0.028 | 0.021 | 25.0# | 46# | 0.00 |

(#) = Out of Range
 G4717Q01.D E524A003.M Thu Nov 06 17:52:22 2003

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D
 Acq On : 6 Nov 2003 10:27 am
 Sample : f=1
 Misc :
 MS Integration Params: Lscint.p
 Vial: 2
 Operator: zou
 Inst : GCMS-A
 Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Mon Oct 27 14:05:06 2003
 Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 20% Max. Rel. Area : 200%

| Compound | AvgrRF | CCRF | %Dev Area | Dev (min) | | |
|----------|---------------------------|-------|-----------|-----------|----|------|
| 53 | 45 c-13-di-Cl-propene | 0.307 | 0.298 | 2.9 | 64 | 0.00 |
| 54 | 46 t-1,3-dichloropropene | 0.248 | 0.262 | -5.6 | 68 | 0.00 |
| 55 I | 47 Chlorobenzene-d5 | 1.000 | 1.000 | 0.0 | 68 | 0.00 |
| 56 | 48 112-tri-Cl-Et | 0.221 | 0.196 | 11.3 | 63 | 0.00 |
| 57 | 49 13-di-Cl-propane | 0.340 | 0.304 | 10.6 | 63 | 0.00 |
| 58 | 50 Et methacrylate | 0.255 | 0.244 | 4.3 | 60 | 0.00 |
| 59 | 51 di-Br-Cl-methane | 0.314 | 0.298 | 5.1 | 69 | 0.00 |
| 60 P | 52 bromoform | 0.185 | 0.178 | 3.8 | 69 | 0.00 |
| 61 | 53 1,4-dichlorobutane-2 | 0.374 | 0.332 | 11.2 | 62 | 0.00 |
| 62 | 54 MIBK | 0.168 | 0.136 | 19.0 | 55 | 0.00 |
| 63 s | 55 toluene-d8 | 1.104 | 1.042 | 5.6 | 65 | 0.00 |
| 64 M,C | 56 toluene | 1.354 | 1.204 | 11.1 | 64 | 0.00 |
| 65 | 57 2-hexanone X5 | 0.109 | 0.102 | 6.4 | 63 | 0.00 |
| 66 | 58 12-dibromoethane | 0.227 | 0.204 | 10.1 | 63 | 0.00 |
| 67 | 59 tetra-Cl-ethene | 0.373 | 0.396 | -6.2 | 79 | 0.00 |
| 68 M,P | 60 chlorobenzene | 0.924 | 0.873 | 5.5 | 66 | 0.00 |
| 69 | 61 1112-tetra-Cl-Et | 0.344 | 0.351 | -2.0 | 72 | 0.00 |
| 70 I | 62 1,4-Dichlorobenzene-d4 | 1.000 | 1.000 | 0.0 | 70 | 0.00 |
| 71 | 63 1-chlorohexane | 0.228 | 0.229 | -0.4 | 77 | 0.00 |
| 72 C | 64 Et-Bz | 2.542 | 2.418 | 4.9 | 68 | 0.00 |
| 73 | 65 m/p-Xylenes X2 | 1.966 | 1.906 | 3.1 | 70 | 0.00 |
| 74 | 66 styrene | 1.656 | 1.569 | 5.3 | 66 | 0.00 |
| 75 | 67 o-xylene | 1.985 | 1.927 | 2.9 | 69 | 0.00 |
| 76 p | 68 1122-Tetra-Cl-Et | 0.396 | 0.338 | 14.6 | 62 | 0.00 |

(#) = Out of Range
 G4717Q01.D E524A003.M Thu Nov 06 17:52:22 2003

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D Vial: 2
 Acq On : 6 Nov 2003 10:27 am Operator: zou
 Sample : f=1 Inst : GCMS-A
 Misc : Multiplr: 1.00
 MS Integration Params: Lscint.p

Method : C:\MSDCHEM\1\METHODS\E524A003.M (RTE Integrator)
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Mon Oct 27 14:05:06 2003
 Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 20% Max. Rel. Area : 200%

| Compound | AvgRF | CCRF | %Dev Area | Dev (min) | | | |
|----------|-------|-------------------------|-----------|-----------|--------|----|------|
| 77 | 69 | 123-tri-Cl-Pr | 0.131 | 0.124 | 5.3 | 68 | 0.00 |
| 78 | 70 | 4-Br-1-F-Bz (S3) | 0.678 | 0.652 | 3.8 | 70 | 0.00 |
| 79 | 71 | isopropylbenzene | 2.654 | 2.711 | -2.1 | 73 | 0.00 |
| 80 | 72 | bromobenzene | 0.672 | 0.660 | 1.8 | 70 | 0.00 |
| 81 | 92 | t-1,4-dichloro-2-butene | 0.062 | 0.068 | -9.7 | 71 | 0.00 |
| 82 | 73 | n-propylbenzene | 0.769 | 0.796 | -3.5 | 74 | 0.00 |
| 83 | 74 | 2-Cl-Toluene | 0.652 | 0.643 | 1.4 | 70 | 0.00 |
| 84 | 75 | 4-Cl-Toluene | 0.670 | 0.644 | 3.9 | 69 | 0.00 |
| 85 | 76 | 135-tri-Me-Benzene | 2.341 | 2.391 | -2.1 | 73 | 0.00 |
| 86 | 77 | 4-iso-Pr-toluene | 2.522 | 2.646 | -4.9 | 77 | 0.00 |
| 87 | 78 | 124-tri-Me-Benzene | 2.451 | 2.437 | 0.6 | 71 | 0.00 |
| 88 | 79 | tert-butylbenzene | 2.055 | 2.170 | -5.6 | 76 | 0.00 |
| 89 | 80 | 13-DCB | 1.396 | 1.353 | 3.1 | 70 | 0.00 |
| 90 | 81 | sec-butylbenzene | 3.069 | 3.193 | -4.0 | 77 | 0.00 |
| 91 | 82 | 14-DCB | 1.461 | 1.357 | 7.1 | 70 | 0.00 |
| 92 | 83 | Cl-benzyl | 0.116 | 0.151 | -30.2# | 86 | 0.00 |
| 93 | 84 | 12-DCB | 1.278 | 1.219 | 4.6 | 71 | 0.00 |
| 94 | 85 | n-butylbenzene | 0.666 | 0.698 | -4.8 | 75 | 0.00 |
| 95 | 86 | 12-diBr-2-Cl-Pra | 0.095 | 0.086 | 9.5 | 63 | 0.00 |
| 96 | 87 | 124-tri-Cl-Bz | 0.796 | 0.810 | -1.8 | 71 | 0.00 |
| 97 | 88 | naphthalene | 1.256 | 1.144 | 8.9 | 60 | 0.00 |
| 98 | 89 | hx-Cl-butadiene | 0.456 | 0.534 | -17.1 | 91 | 0.00 |
| 99 | 90 | 123-Tri-Cl-Bz | 0.687 | 0.691 | -0.6 | 70 | 0.00 |

(#) = Out of Range SPCC's out = 0 CCC's out = 0
 G4717Q01.D E524A003.M Thu Nov 06 17:52:23 2003

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:27 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:50 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:51 2003
 Miscelaneous :

| ID | Component Name | R.T. | RT0 | DRRT | QIon | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------------------|-------------------|-------|-------|-------|------|-----|---------|--------|-------|---------|------|
| Internal Standards | | | | | | | | | | | |
| 1 | Fluorobenzene | 7.65 | 7.64 | 0.000 | 96 | 70 | 650.919 | 10.00 | | 0.00 | |
| 47 | Chlorobenzene-d5 | 11.54 | 11.54 | 0.000 | 117 | 82 | 496.725 | 10.00 | | 0.00 | |
| 62 | 1,4-Dichlorobenze | 13.84 | 13.85 | 0.000 | 152 | 150 | 305.376 | 10.00 | | 0.00 | |

| System Monitoring Compounds (Surrogate) | | | | | | | | | | | |
|---|-------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| ID | Component Name | R.T. | RT0 | DRRT | QIon | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
| 27 | Di-Br-F-Me (surr) | 6.60 | 6.60 | 0.000 | 111 | 113 | 292.546 | 19.14 | 19.1 | 95.70% | |
| 29 | 1,2-Di-Cl-Et-d4 (| 7.10 | 7.11 | 0.000 | 65 | 102 | 268.507 | 19.72 | 19.7 | 98.62% | |
| 55 | toluene-d8 | 9.91 | 9.91 | 0.000 | 98 | 100 | 1035.489 | 18.89 | 18.9 | 94.43% | |
| 70 | 4-Br-1-F-Bz (S3) | 12.74 | 12.74 | 0.000 | 174 | 95 | 398.140 | 19.24 | 19.2 | 96.20% | |

| Target Compounds | | | | | | | | | | | | |
|------------------|-------------------|------|------|--------|-----|-----|---------|--------|-------|-----|--|--------|
| <<< ID | : ISTD ID = 1 | >>> | | | | | | | | | | Qvalue |
| 3 | di-Cl-di-F-methan | 1.89 | 1.89 | 0.000 | 85 | 87 | 238.592 | 18.22 | 18.2 | 100 | | |
| 4 | Chloromethane | 2.11 | 2.11 | 0.000 | 50 | 52 | 179.442 | 13.80 | 13.8 | 99 | | |
| 2 | F114 | 2.03 | 2.03 | 0.000 | 85 | 135 | 123.464 | 20.05 | 20.1 | 49 | | |
| 5 | vinyl chloride | 2.22 | 2.22 | 0.000 | 62 | 64 | 189.466 | 17.07 | 17.1 | 100 | | |
| 6 | bromomethane | 2.61 | 2.61 | 0.000 | 94 | 96 | 69.956 | 11.10 | 11.1 | 91 | | |
| 7 | chloroethane | 2.73 | 2.73 | 0.000 | 64 | 66 | 106.954 | 17.89 | 17.9 | 88 | | |
| 8 | tri-Cl-F-methane | 3.03 | 3.03 | 0.000 | 101 | 103 | 421.501 | 22.97 | 23.0 | 98 | | |
| 91 | Acetonitrile X10 | 4.07 | 4.07 | 0.000 | 41 | 40 | 461.496 | 164.55 | 164.6 | 82 | | |
| 9 | acrolein X10 | 3.51 | 3.51 | 0.000 | 56 | 55 | 226.269 | 164.28 | 164.3 | 95 | | |
| 11 | acetone X10 | 3.70 | 3.73 | -0.004 | 43 | 58 | 501.271 | 241.05 | 241.0 | 81 | | |
| 12 | ethyl ether X5 | 3.37 | 3.37 | 0.000 | 59 | 74 | 547.856 | 88.59 | 88.6 | 80 | | |
| 13 | 11-dichloroethene | 3.64 | 3.64 | 0.000 | 61 | 96 | 317.434 | 20.53 | 20.5 | 80 | | |
| 14 | Iodomethane | 3.81 | 3.81 | 0.000 | 142 | 127 | 158.325 | 12.52 | 12.5 | 90 | | |
| 15 | F-113 | 3.65 | 3.65 | 0.000 | 101 | 151 | 216.223 | 23.05 | 23.1 | 85 | | |
| 16 | acrylonitrile X10 | 4.51 | 4.52 | -0.002 | 53 | 52 | 440.756 | 157.84 | 157.8 | 94 | | |
| 17 | carbon disulfide | 3.90 | 3.90 | 0.000 | 76 | 78 | 498.576 | 16.93 | 16.9 | 100 | | |
| 94 | Isopropyl Alcohol | 3.93 | 4.10 | -0.022 | 45 | 43 | 35.410 | 265.70 | 265.7 | 100 | | |
| 18 | methylene chlorid | 4.22 | 4.22 | 0.000 | 84 | 49 | 240.082 | 17.33 | 17.3 | 76 | | |
| 19 | t-12-di-Cl-ethene | 4.58 | 4.58 | 0.000 | 96 | 61 | 264.471 | 18.20 | 18.2 | 95 | | |

De
11/06/03
m
De
11/06/03
m

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:27 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:50 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:51 2003
 Miscleous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|-----|-------------------|-------|-------|--------|------|-----|----------|--------|-------|---------|-----------------|
| 20 | t-Bu-Me-ether | 4.59 | 4.59 | 0.000 | 73 | 57 | 495.885 | 19.39 | 19.4 | 93 | ? |
| 95 | Tert butyl alcoho | 4.41 | 4.51 | -0.013 | 59 | 57 | 136.440 | 319.44 | 319.4 | 100 | ? |
| 94 | allyl chloride | 4.07 | 4.07 | 0.000 | 41 | 76 | 366.268 | 12.76 | 12.8 | 89 | me ? 11/6/03 |
| 21 | 11-dichloroethane | 5.12 | 5.12 | 0.000 | 63 | 83 | 436.044 | 18.11 | 18.1 | 97 | # |
| 97 | propionitrile | 6.00 | 6.02 | -0.002 | 54 | 51 | 19.315 | 16.83 | 16.8 | 100 | # |
| 22 | c-12-di-Cl-ethene | 5.92 | 5.92 | 0.000 | 96 | 61 | 269.178 | 17.76 | 17.8 | 79 | #? |
| 23 | 22-Dichloropropan | 5.92 | 5.92 | 0.000 | 77 | 97 | 405.964 | 26.43 | 26.4 | 98 | ? |
| 24 | Br-Cl-methane | 6.24 | 6.25 | 0.000 | 128 | 130 | 135.937 | 17.74 | 17.7 | 99 | |
| 25 | chloroform | 6.37 | 6.37 | 0.000 | 83 | 85 | 508.556 | 18.79 | 18.8 | 100 | |
| 26 | tetrahydrofuranX5 | 6.34 | 6.35 | -0.002 | 42 | 72 | 171.834 | 76.20 | 76.2 | 85 | |
| 98 | Diisopropyl ether | 5.24 | 5.24 | 0.000 | 45 | 87 | 808.540 | 17.49 | 17.5 | 91 | |
| 99 | ETBE | 5.74 | 5.74 | 0.000 | 59 | 87 | 598.312 | 20.53 | 20.5 | 93 | |
| 30 | 12-dichloroethane | 7.22 | 7.22 | 0.000 | 64 | 62 | 103.834 | 19.68 | 19.7 | 98 | ? |
| 32 | vinyl acetate X5 | 5.19 | 5.20 | 0.000 | 43 | 86 | 2098.034 | 93.02 | 93.0 | 92 | |
| 92 | Nitro Methane(x10 | 5.79 | 5.84 | -0.006 | 61 | 46 | 58.322 | 76.72 | 76.7 | 97 | |
| 33 | 2-butanoneMEK X10 | 5.93 | 5.95 | -0.002 | 43 | 72 | 649.430 | 191.23 | 191.2 | 85 | ? |
| 93 | Ethyl Acetate x2 | 6.03 | 6.04 | 0.000 | 43 | 61 | 265.051 | 31.52 | 31.5 | 98 | |
| 34 | 111-trichloroetha | 6.65 | 6.65 | 0.000 | 97 | 99 | 512.316 | 22.51 | 22.5 | 100 | |
| 35 | 11-Di-Cl-propene | 6.90 | 6.90 | 0.000 | 75 | 110 | 356.458 | 20.75 | 20.8 | 92 | ? |
| 36 | benzene | 7.21 | 7.21 | 0.000 | 78 | 52 | 974.138 | 17.70 | 17.7 | 88 | ? |
| 37 | CCl4 | 6.91 | 6.91 | 0.000 | 117 | 119 | 505.080 | 24.14 | 24.1 | 99 | ? |
| 100 | Isobutyl alcohol | 7.41 | 7.41 | 0.000 | 43 | 42 | 163.588 | 195.71 | 195.7 | 88 | #? |
| 38 | thiophene | 7.53 | 7.53 | 0.000 | 84 | 58 | 524.615 | 18.31 | 18.3 | 93 | |
| 39 | 12-di-Cl-propane | 8.56 | 8.56 | 0.000 | 63 | 76 | 217.989 | 17.31 | 17.3 | 86 | |
| 40 | trichloroethene | 8.24 | 8.24 | 0.000 | 130 | 132 | 338.447 | 19.19 | 19.2 | 94 | |
| 41 | dibromomethane | 8.73 | 8.73 | 0.000 | 174 | 172 | 161.333 | 18.41 | 18.4 | 99 | |
| 101 | TAME | 7.41 | 7.41 | 0.000 | 73 | 43 | 483.990 | 18.08 | 18.1 | 90 | ? |
| 42 | Br-di-Cl-methane | 8.96 | 8.96 | 0.000 | 83 | 85 | 376.858 | 19.01 | 19.0 | 99 | |
| 43 | Me-methacrylate | 8.76 | 8.76 | 0.000 | 69 | 100 | 110.408 | 15.75 | 15.7 | 87 | |
| 44 | 2-ClEt-Vi-ether10 | 9.38 | 9.38 | 0.000 | 63 | 43 | 273.681 | 127.89 | 127.9 | 83 | |
| 45 | c-13-di-Cl-propen | 9.56 | 9.56 | 0.000 | 75 | 110 | 388.349 | 19.44 | 19.4 | 92 | |
| 46 | t-1,3-dichloropro | 10.24 | 10.25 | 0.000 | 75 | 110 | 341.152 | 19.12 | 19.1 | 94 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:27 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:50 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:51 2003
 Miscelaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|--------|--------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| <<< I2 | : ISTD ID = 47 >>> | | | | | | | | | | |
| 48 | 112-tri-Cl-Et | 10.45 | 10.45 | 0.000 | 97 | 83 | 194.772 | 17.71 | 17.7 | 95 | |
| 49 | 13-di-Cl-propane | 10.65 | 10.65 | 0.000 | 76 | 78 | 301.908 | 17.89 | 17.9 | 99 | |
| 50 | Et methacrylate | 10.38 | 10.37 | 0.000 | 69 | 99 | 242.544 | 15.88 | 15.9 | 89 | ? |
| 51 | di-Br-Cl-methane | 10.90 | 10.91 | 0.000 | 129 | 127 | 296.008 | 18.97 | 19.0 | 99 | |
| 52 | bromoform | 12.41 | 12.42 | 0.000 | 173 | 174 | 176.864 | 19.27 | 19.3 | 99 | |
| 53 | 1,4-dichlorobutan | 12.67 | 12.67 | 0.000 | 55 | 41 | 330.045 | 17.76 | 17.8 | 96 | |
| 54 | MIBK | 9.76 | 9.77 | 0.000 | 43 | 58 | 135.067 | 14.24 | 14.2 | 96 | |
| 56 | toluene | 9.99 | 9.99 | 0.000 | 91 | 92 | 1196.236 | 17.78 | 17.8 | 97 | |
| 57 | 2-hexanone X5 | 10.75 | 10.76 | 0.000 | 43 | 58 | 506.148 | 82.32 | 82.3 | 89 | |
| 58 | 12-dibromoethane | 11.03 | 11.03 | 0.000 | 107 | 109 | 202.794 | 18.00 | 18.0 | 99 | |
| 59 | tetra-Cl-ethene | 10.64 | 10.64 | 0.000 | 166 | 168 | 393.147 | 21.23 | 21.2 | 97 | ? |
| 60 | chlorobenzene | 11.57 | 11.57 | 0.000 | 112 | 77 | 866.936 | 18.89 | 18.9 | 94 | ? |
| 61 | 1112-tetra-Cl-Et | 11.66 | 11.66 | 0.000 | 131 | 133 | 348.480 | 20.40 | 20.4 | 98 | |
| <<< I3 | : ISTD ID = 62 >>> | | | | | | | | | | |
| 63 | 1-chlorohexane | 11.56 | 11.56 | 0.000 | 93 | 55 | 139.579 | 20.02 | 20.0 | 49 | #? |
| 64 | Et-Bz | 11.70 | 11.70 | 0.000 | 91 | 106 | 1476.804 | 19.02 | 19.0 | 97 | |
| 65 | m/p-Xylenes X2 | 11.82 | 11.82 | 0.000 | 91 | 106 | 2328.165 | 38.77 | 38.8 | 100 | |
| 66 | styrene | 12.24 | 12.24 | 0.000 | 104 | 78 | 958.401 | 18.95 | 19.0 | 100 | ? |
| 67 | o-xylene | 12.22 | 12.22 | 0.000 | 91 | 106 | 1177.124 | 19.41 | 19.4 | 98 | ? |
| 68 | 1122-Tetra-Cl-Et | 12.87 | 12.87 | 0.000 | 83 | 85 | 206.349 | 17.06 | 17.1 | 94 | |
| 69 | 123-tri-Cl-Pr | 12.91 | 12.92 | 0.000 | 110 | 97 | 75.659 | 18.84 | 18.8 | 92 | ? |
| 71 | isopropylbenzene | 12.60 | 12.60 | 0.000 | 105 | 120 | 1655.609 | 20.42 | 20.4 | 97 | |
| 72 | bromobenzene | 12.89 | 12.89 | 0.000 | 156 | 158 | 403.196 | 19.65 | 19.7 | 98 | ? |
| 92 | t-1,4-dichloro-2- | 12.92 | 12.92 | 0.000 | 89 | 53 | 41.711 | 17.50 | 17.5 | 83 | #? |
| 73 | n-propylbenzene | 13.00 | 13.00 | 0.000 | 120 | 78 | 486.356 | 20.72 | 20.7 | 95 | |
| 74 | 2-Cl-Toluene | 13.08 | 13.08 | 0.000 | 126 | 128 | 392.657 | 19.73 | 19.7 | 99 | |
| 75 | 4-Cl-Toluene | 13.19 | 13.19 | 0.000 | 126 | 128 | 393.162 | 19.22 | 19.2 | 98 | ? |
| 76 | 135-tri-Me-Benzen | 13.16 | 13.16 | 0.000 | 105 | 120 | 1460.395 | 20.43 | 20.4 | 95 | ? |
| 77 | 4-iso-Pr-toluene | 13.81 | 13.81 | 0.000 | 119 | 134 | 1616.052 | 20.99 | 21.0 | 100 | ? |
| 78 | 124-tri-Me-Benzen | 13.51 | 13.52 | 0.000 | 105 | 120 | 1488.485 | 19.88 | 19.9 | 96 | |
| 79 | tert-butylbenzene | 13.47 | 13.47 | 0.000 | 119 | 91 | 1325.271 | 21.12 | 21.1 | 97 | |


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:27 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:50 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:51 2003
 Miscelaneous :

| ID | Component Name | R.T. | RT0 | DRRT | Qion | Q1 | RF/1000 | C0,ppb | C,ppb | Quality | Note |
|----|------------------|-------|-------|-------|------|-----|----------|--------|-------|---------|------|
| 80 | 13-DCB | 13.79 | 13.79 | 0.000 | 146 | 148 | 826.362 | 19.38 | 19.4 | 99 | ? |
| 81 | sec-butylbenzene | 13.68 | 13.68 | 0.000 | 105 | 134 | 1950.300 | 20.81 | 20.8 | 98 | |
| 82 | 14-DCB | 13.87 | 13.87 | 0.000 | 146 | 148 | 828.869 | 18.58 | 18.6 | 98 | |
| 83 | Cl-benzyl | 13.98 | 13.98 | 0.000 | 126 | 91 | 92.095 | 19.80 | 19.8 | 86 | # |
| 84 | 12-DCB | 14.21 | 14.21 | 0.000 | 146 | 148 | 744.207 | 19.06 | 19.1 | 98 | ? |
| 85 | n-butylbenzene | 14.18 | 14.18 | 0.000 | 134 | 91 | 426.496 | 20.97 | 21.0 | 81 | #? |
| 86 | 12-diBr-2-Cl-Pra | 14.88 | 14.88 | 0.000 | 157 | 155 | 52.386 | 18.03 | 18.0 | 98 | |
| 87 | 124-tri-Cl-Bz | 15.58 | 15.58 | 0.000 | 180 | 182 | 495.011 | 20.36 | 20.4 | 99 | |
| 88 | naphthalene | 15.78 | 15.78 | 0.000 | 128 | 129 | 698.457 | 15.77 | 15.8 | 98 | |
| 89 | hx-Cl-butadiene | 15.72 | 15.72 | 0.000 | 225 | 258 | 326.253 | 23.45 | 23.4 | 97 | |
| 90 | 123-Tri-Cl-Bz | 15.98 | 15.98 | 0.000 | 180 | 182 | 422.215 | 20.11 | 20.1 | 99 | |

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G4717\G4717Q01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A003.M Inst. : GCMS-A
 Acq. Time : Nov 6 10:27 2003 RF via : Multiple Level Calibration
 Method Update: Mon Oct 27 14:05 2003 Operator: zou
 Quant. Time : Nov 06 17:50 2003 Multiplr: 1.000000
 Print Time : Thu Nov 06 17:51 2003
 Miscelaneous :

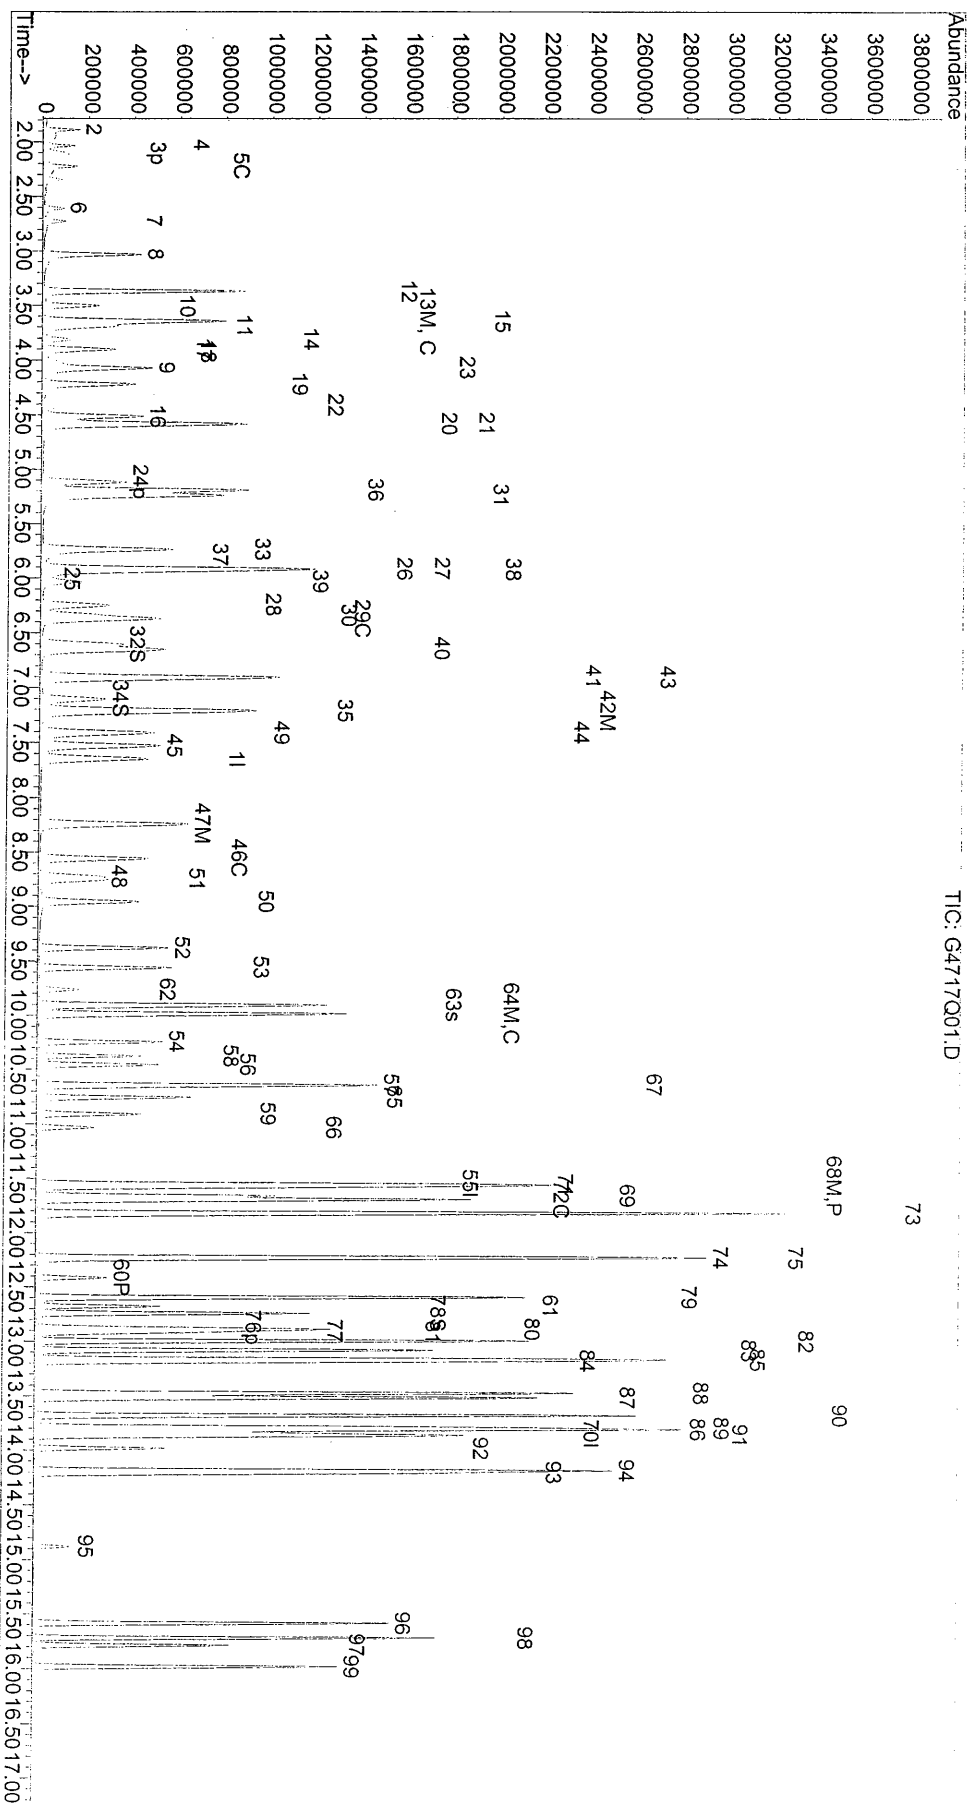

FORM-8A

Applied P & Ch Laboratory

Internal Standard Area and RT Summary for Method 524.2

Client Name: GEOFON, Inc. Contract No: Lab Code: APCL
 Case No: SAS No: Service ID: 035951
 Project ID: JPL Project No: 04-4428.10 Sample Matrix: Water
 CCV Data File: G4717Q01 Instrument ID: A
 Batch No: 03G4717

| # | Client Sample No | Lab Sample ID | Analysis Date & Time | IS-1 | | IS-2 | | IS-3 | |
|-----------------|------------------|----------------|----------------------|---------|------|--------|-------|--------|-------|
| | | | | Area # | RT # | Area # | RT # | Area # | RT # |
| 12 Hour CCV STD | | | 11/06/03 10:27 | 650919 | 7.65 | 496725 | 11.54 | 305376 | 13.84 |
| CCV Upper Limit | | | | 1301838 | 8.15 | 993450 | 12.04 | 610752 | 14.34 |
| CCV Lower Limit | | | | 325459 | 7.15 | 248362 | 11.04 | 152688 | 13.34 |
| 1 | 03G4717-LCS-01 | 03G4717-LCS-01 | 11/06/03 10:53 | 654113 | 7.64 | 497611 | 11.54 | 302374 | 13.84 |
| 2 | MW-3-1MS | 03-5973-2MS | 11/06/03 11:19 | 679050 | 7.65 | 523203 | 11.54 | 312211 | 13.84 |
| 3 | MW-3-1MSD | 03-5973-2MSD | 11/06/03 11:44 | 690552 | 7.64 | 531594 | 11.54 | 325550 | 13.84 |
| 4 | 03G4717-MB-01 | 03G4717-MB-01 | 11/06/03 13:54 | 664923 | 7.64 | 492340 | 11.54 | 294801 | 13.85 |
| 5 | TB-9-11-4-03 | 03-5951-13 | 11/06/03 14:20 | 674960 | 7.64 | 498096 | 11.55 | 295897 | 13.85 |
| 6 | DUPE-5-4-Q03 | 03-5951-1 | 11/06/03 16:30 | 644992 | 7.65 | 476399 | 11.54 | 281619 | 13.85 |
| 7 | EB-9-11-4-03 | 03-5951-2 | 11/06/03 16:57 | 651961 | 7.64 | 478094 | 11.54 | 287454 | 13.85 |
| 8 | MW-14-1 | 03-5951-3 | 11/06/03 17:23 | 632576 | 7.64 | 469145 | 11.54 | 274279 | 13.85 |
| 9 | MW-14-2 | 03-5951-4 | 11/06/03 17:49 | 647229 | 7.64 | 477270 | 11.54 | 278778 | 13.85 |
| 10 | MW-14-3 | 03-5951-5 | 11/06/03 18:15 | 638481 | 7.65 | 468972 | 11.54 | 279778 | 13.84 |
| 11 | MW-14-4 | 03-5951-6 | 11/06/03 18:41 | 626843 | 7.64 | 459535 | 11.54 | 276318 | 13.85 |
| 12 | MW-14-5 | 03-5951-7 | 11/06/03 19:07 | 636531 | 7.64 | 468573 | 11.55 | 277618 | 13.85 |
| 13 | MW-17-1 | 03-5951-8 | 11/06/03 19:33 | 631650 | 7.64 | 465910 | 11.55 | 278661 | 13.85 |
| 14 | MW-17-2 | 03-5951-9 | 11/06/03 19:59 | 636151 | 7.65 | 473543 | 11.54 | 282429 | 13.85 |
| 15 | MW-17-3 | 03-5951-10 | 11/06/03 20:25 | 638237 | 7.65 | 476913 | 11.55 | 287702 | 13.85 |
| 16 | MW-17-4 | 03-5951-11 | 11/06/03 20:51 | 627311 | 7.65 | 469574 | 11.54 | 277534 | 13.85 |
| 17 | MW-17-5 | 03-5951-12 | 11/06/03 21:17 | 645260 | 7.65 | 480046 | 11.54 | 288566 | 13.85 |
| 18 | | | | | | | | | |
| 19 | | | | | | | | | |
| 20 | | | | | | | | | |
| 21 | | | | | | | | | |
| 22 | | | | | | | | | |

IS-1 = FLUOROBENZENE
 IS-2 = CHLOROBENZENE-D5
 IS-3 = 1,4-DICHLOROBENZENE-D4

Area Upper Limit = +100% of CCV internal standard area
 Area Lower Limit = - 50% of CCV internal standard area
 RT Upper Limit = +0.50 minutes of CCV internal standard RT
 RT Lower Limit = - 0.50 minutes of CCV internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits

A
 Applied P & Ch Laboratory
 10 Magnolia Ave. Chino CA 91710
 (909) 590-1828 Fax: (909) 590-1498

VOC Analysis General Logbook

License # 0384717 Batch # 0384717 Matrix: W Date: 11/06/03 Analyst: Zac
 #: IS/Surrogate: GC-1576/1576 Methanol(mark-M): _____ PEG (mark-PEG): _____ Defoaming(mark-DF): _____

Calib. + Ini. Batch Initial Batch; Middle Batch; Final Batch. Internal Study Datafile Path: _____

| # | Type | Sample ID | Method | V/X=f ₁ | V _j /V _i =f ₂ | V _{spg} /V _{inj} =f ₃ | F | A-# | Datafile | Note | pH |
|------|--------|-----------|--------------|--------------------|--|--|---|-----|----------|-----------|---------|
| 77 | SP | 64717P01 | ES24A 003 | 25/25 = 1 | / = | / = | 1 | | 64717P01 | 11/06/03 | 10.020m |
| 778 | CCV | Q01 | | / = 1 | / = | / = | | | Q01 | GC15796 | |
| 779 | LCS | L01 | | / = 1 | / = | / = | | | L01 | | |
| 780 | MS | M01 | | / = | / = | / = | | | M01 | \$5973-02 | <2 |
| 781 | MSD | N01 | | / = | / = | / = | | | N01 | ↓ | ↓ |
| 782 | MB | √ K01 | | / = | / = | / = | | | √ K01 | | |
| 783 | Sample | 5951-13 | | / = | / = | / = | | | 5951-13 | tb | <2 |
| 784 | | 5973-04 | | / = | / = | / = | | | 5973-04 | tb | |
| 785 | | 02 | | / = | / = | / = | | | 02 | ms | |
| 786 | | 01 | | / = | / = | / = | | | 01 | | |
| 787 | | √ 03 | | / = | / = | / = | | | √ 03 | | |
| 788 | | 5951-01 | | / = | / = | / = | | | 5951-01 | | |
| 789 | | 02 | | / = | / = | / = | | | 02 | | |
| 790 | | 03 | | / = | / = | / = | | | 03 | | |
| 791 | | 04 | | / = | / = | / = | | | 04 | | |
| 792 | | 05 | | / = | / = | / = | | | 05 | | |
| 793 | | 06 | | / = | / = | / = | | | 06 | | |
| 794 | | 07 | | / = | / = | / = | | | 07 | | |
| 795 | | 08 | | / = | / = | / = | | | 08 | | |
| 796 | | 09 | | / = | / = | / = | | | 09 | | |
| 797 | | 10 | | / = | / = | / = | | | 10 | | |
| 798 | | 11 | | / = | / = | / = | | | 11 | | |
| 799 | ↓ | √ 12 | √ | √ / = √ | / = | / = | √ | | √ 12 | | √ |
| 4800 | | | | / = | / = | / = | | | | | |
| 4801 | | | | / = | / = | / = | | | | | |
| 4802 | | | | / = | / = | / = | | | | | |
| 4803 | | | | / = | / = | / = | | | | | |
| 4804 | | | | / = | / = | / = | | | | | |
| 4805 | | | | / = | / = | / = | | | | | |
| 4806 | | | | / = | / = | / = | | | | | |
| 4807 | | | | / = | / = | / = | | | | | |
| 4808 | | | | / = | / = | / = | | | | | |

| Type | Op # | STD Lot # | C _{std} (ng/μL) × V _{std} (μL) / X(g or mL) = T | Op # | STD Lot # | C _{std} (ng/μL) × V _{std} (μL) / X(g or mL) = T |
|----------|-----------|-----------|---|------|-----------|---|
| LCS/LCSD | 4779 | GC-15797 | 200 × 2.5 / X = ppb | | GC- | x / X = ppb |
| MS/MSD | 4780/4781 | GC- | x / X = ppb | | GC- | x / X = ppb |

Footnote/Anomaly: _____

VOC Analysis General Logbook

Sequence # 0364612 Batch # 0364612 Matrix: W Date: 10/21/03 Analyst: Eddie

Lot #: IS/Surrogate: GC1514/1515 Methanol(mark-M): _____ PEG (mark-PEG): _____ Defoaming(mark-DF): _____

Calib. + Ini. Batch - Initial Batch; Middle Batch; Final Batch. Internal Study Datafile Path: _____

| Op. # | Type | Sample ID | Method | $V_1/X=f_1$ | $V_1/V_i=f_2$ | $V_{spg}/V_{inj}=f_3$ | F | A-# | Datafile | Note | pH |
|-------|-------|-----------|--------|-------------|---------------|-----------------------|---|-----|----------|--------------------|----|
| 4201 | SP | 64612 P01 | E524A | 25/25 = 1 | / = | / = | 1 | | 64612P01 | 10/21/03 9:14am | |
| 4202 | Calib | 3-A003 | 003 | / = | / = | / = | | | 3-A003 | gc15731 | |
| 4203 | | 3-002 | | / = | / = | / = | | | 3-002 | | |
| 4204 | | 3-0010 | | / = | / = | / = | | | 3-0010 | | |
| 4205 | | 3-0020 | | / = | / = | / = | | | 3-0020 | | |
| 4206 | | 3-0040 | | / = | / = | / = | | | 3-0040 | | |
| 4207 | | 3-0060 | | / = | / = | / = | | | 3-0060 | | |
| 4208 | ICV | ICV | | / = | / = | / = | | | ICV | gc15732 | |
| 4209 | | | | / = | / = | / = | | | | | |
| 4210 | | | | / = | / = | / = | | | | | |
| 4211 | | | | / = | / = | / = | | | | | |
| 4212 | | | | / = | / = | / = | | | | | |
| 4213 | | | | / = | / = | / = | | | | | |
| 4214 | | | | / = | / = | / = | | | | | |
| 4215 | | | | / = | / = | / = | | | | | |
| 4216 | | | | / = | / = | / = | | | | | |
| 4217 | | | | / = | / = | / = | | | | | |
| 4218 | | | | / = | / = | / = | | | | | |
| 4219 | | | | / = | / = | / = | | | | | |
| 4220 | | | | / = | / = | / = | | | | | |
| 4221 | | | | / = | / = | / = | | | | | |
| 4222 | | | | / = | / = | / = | | | | | |
| 4223 | | | | / = | / = | / = | | | | | |
| 4224 | | | | / = | / = | / = | | | | | |
| 4225 | | | | / = | / = | / = | | | | | |
| 4226 | | | | / = | / = | / = | | | | | |
| 4227 | | | | / = | / = | / = | | | | | |
| 4228 | | | | / = | / = | / = | | | | | |
| 4229 | | | | / = | / = | / = | | | | | |
| 4230 | | | | / = | / = | / = | | | | | |
| 4231 | | | | / = | / = | / = | | | | | |
| 4232 | | | | / = | / = | / = | | | | | |

| Type | Op # | STD Lot # | $C_{std}(ng/\mu L) \times V_{std}(\mu L) / X(g \text{ or mL}) = T$ | Op # | STD Lot # | $C_{std}(ng/\mu L) \times V_{std}(\mu L) / X(g \text{ or mL}) = T$ |
|----------|------|-----------|--|------|-----------|--|
| LCS/LCSD | | GC- | x / X = ppb | | GC- | x / X = ppb |
| MS/MSD | | GC- | x / X = ppb | | GC- | x / X = ppb |

Footnote/Anomaly: