

Level C Data Package Deliverables

Wet Chemistry



Applied P & Ch Laboratory

Applied P & Ch Laboratory
Wet Analysis Results for Method SM2320B

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 32933

Anal. Method: SM2320B
 Collected by: Leo Williamson

Component Name: Bicarbonate
 CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	05/01/03	03W2665	mg/L	2	< 2	U
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	05/01/03	03W2665	mg/L	2	176	
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	05/01/03	03W2665	mg/L	2	164	
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	05/01/03	03W2665	mg/L	2	167	
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	05/01/03	03W2665	mg/L	2	137	
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	05/01/03	03W2665	mg/L	2	156	
03W2665-MB-01	03W2665-MB-01	Water	05/01/03	05/01/03	05/01/03	03W2665	mg/L	2	< 2	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method SM2320B

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 32933

Anal. Method: SM2320B
 Collected by: Leo Williamson

Component Name: Carbonate
 CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	05/01/03	03W2665	mg-CaCO ₃ /L	2	<2	U
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	05/01/03	03W2665	mg-CaCO ₃ /L	2	<2	U
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	05/01/03	03W2665	mg-CaCO ₃ /L	2	<2	U
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	05/01/03	03W2665	mg-CaCO ₃ /L	2	<2	U
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	05/01/03	03W2665	mg-CaCO ₃ /L	2	<2	U
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	05/01/03	03W2665	mg-CaCO ₃ /L	2	<2	U
03W2665-MB-01	03W2665-MB-01	Water	05/01/03	05/01/03	05/01/03	03W2665	mg-CaCO ₃ /L	2	<2	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method 9040B

Client Name: GEOFON, Inc.
Project ID: JPL

Project No: 04-4428.10
Service ID: 32933

Anal. Method: 9040B
Collected by: Leo Williamson

Component Name: pH
CAS No: 10-29-7

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	04/28/03	03W2592	pH unit	0.01	6.54	
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	04/28/03	03W2592	pH unit	0.01	7.44	
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	04/28/03	03W2592	pH unit	0.01	7.97	
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	04/28/03	03W2592	pH unit	0.01	8.08	
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	04/28/03	03W2592	pH unit	0.01	8.01	
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	04/28/03	03W2592	pH unit	0.01	8.17	
03W2592-MB-01	03W2592-MB-01	Water	04/28/03	04/28/03	04/28/03	03W2592	pH unit	0.01	6.87	

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method 160.1

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 32933

Anal. Method: 160.1
 Collected by: Leo Williamson

Component Name: Solids, Total Dissolved (TDS)
 CAS No: 10-33-3

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	04/28/03	03W2607	mg/L	10	<10	U
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	04/28/03	03W2607	mg/L	10	253	
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	04/28/03	03W2607	mg/L	10	250	
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	04/28/03	03W2607	mg/L	10	247	
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	04/28/03	03W2607	mg/L	10	198	
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	04/28/03	03W2607	mg/L	10	219	
03W2607-MB-01	03W2607-MB-01	Water	04/28/03	04/28/03	04/28/03	03W2607	mg/L	10	<10	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method 7196

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 32933

Anal. Method: 7196
 Collected by: Leo Williamson

Component Name: Chromium (VI)
 CAS No: 1333-82-0

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	04/28/03	03W2603	mg/L	0.01	<0.01	U
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	04/28/03	03W2603	mg/L	0.01	<0.01	U
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	04/28/03	03W2603	mg/L	0.01	<0.01	U
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	04/28/03	03W2603	mg/L	0.01	<0.01	U
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	04/28/03	03W2603	mg/L	0.01	<0.01	U
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	04/28/03	03W2603	mg/L	0.01	<0.01	U
03W2603-MB-01	03W2603-MB-01	Water	04/28/03	04/28/03	04/28/03	03W2603	mg/L	0.01	<0.01	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method 314.0

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 32933

Anal. Method 314.0
 Collected by: Leo Williamson

Component Name: Perchlorate
 CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	04/29/03	03W2612	µg/L	4	<4	U
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	04/29/03	03W2612	µg/L	4	<4	U
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	04/29/03	03W2612	µg/L	4	4.1	
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	04/29/03	03W2612	µg/L	8	126	
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	04/29/03	03W2612	µg/L	4	6.5	
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	04/29/03	03W2612	µg/L	4	3.6	B
03W2612-MB-01	03W2612-MB-01	Water	04/29/03	04/29/03	04/29/03	03W2612	µg/L	4	<4	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method 300.0

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 32933

Anal. Method: 300.0
 Collected by: Leo Williamson

Component Name: Chloride Cl⁻
 CAS No: 16887-00-6

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.25	0.20	B
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.4	13.3	
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.4	19.6	
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.4	12.5	
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.4	11.4	
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.4	11.2	
03W2610-MB-01	03W2610-MB-01	Water	04/29/03	04/29/03	04/29/03	03W2610	mg/L	0.2	<0.2	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method 300.0

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 32933

Anal. Method: 300.0
 Collected by: Leo Williamson

Component Name: Nitrate as N
 CAS No: 14797-55-8

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.05	0.071	
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.08	1.3	
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.08	2.0	
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.08	1.5	
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.08	0.70	
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.08	0.64	
03W2610-MB-01	03W2610-MB-01	Water	04/29/03	04/29/03	04/29/03	03W2610	mg/L	0.04	<0.04	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method 300.0

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 32933

Anal. Method 300.0
 Collected by: Leo Williamson

Component Name: Sulfate SO_4^{--}
 CAS No: 14808-79-8

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-2933-1	EB-6-4/28/03	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	0.63	<0.63	U
03-2933-2	MW-17-1	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	1	36.5	
03-2933-3	MW-17-2	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	1	34.7	
03-2933-4	MW-17-3	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	1	31.7	
03-2933-5	MW-17-4	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	1	25.5	
03-2933-6	MW-17-5	Water	04/28/03	04/28/03	04/29/03	03W2610	mg/L	1	18.8	
03W2610-MB-01	03W2610-MB-01	Water	04/29/03	04/29/03	04/29/03	03W2610	mg/L	0.5	<0.5	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

FORM-3

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 300.0

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 32933
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W2610	
LCS Filename: -	Date Analyzed: 042903	Time Analyzed: 10:33
LCSD Filename: -	Date Analyzed: 042903	Time Analyzed: 10:46

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
CHLORIDE CL ⁻	mg/L	4.0	0	3.88	97	80-120
NITRATE AS N	mg/L	1.5	0	1.49	99	80-120
SULFATE SO ₄ ⁻	mg/L	15	0	14.7	98	80-120
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	LCSD Concentration	LCSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
CHLORIDE CL ⁻	mg/L	4.0	3.90	98	1	20	80-120
NITRATE AS N	mg/L	1.5	1.50	100	1	20	80-120
SULFATE SO ₄ ⁻	mg/L	15	14.8	99	1	25	80-120
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 300.0

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 32933
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W2610	
MS Filename: -	Date Analyzed: 042903	Time Analyzed: 15:02
MSD Filename: -	Date Analyzed: 042903	Time Analyzed: 15:14
MS Sample No: MW-17-2	Sample Lab ID: 03-2933-3	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
CHLORIDE CL ⁻	mg/L	16.0	19.6	35.2	98	75-125
NITRATE AS N	mg/L	6.00	2.0	8.18	103	75-125
SULFATE SO ₄ ⁻²	mg/L	60.0	34.7	98.4	106	75-125
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
CHLORIDE CL ⁻	mg/L	16.0	35.2	98	0	20	75-125
NITRATE AS N	mg/L	6.00	8.12	102	1	20	75-125
SULFATE SO ₄ ⁻²	mg/L	60.0	97.4	105	1	25	75-125
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 314.0

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 32933
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W2612	
LCS Filename: -	Date Analyzed: 042903	Time Analyzed: 10:20
LCSD Filename: -	Date Analyzed: -	Time Analyzed: -

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
PERCHLORATE	µg/L	25	0	23.4	94	80-120
# of Out-of-control					0	

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 314.0

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 32933
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W2612	
MS Filename: -	Date Analyzed: 042903	Time Analyzed: 14:07
MSD Filename: -	Date Analyzed: 042903	Time Analyzed: 14:26
MS Sample No: MW-17-2	Sample Lab ID: 03-2933-3	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
PERCHLORATE	µg/L	50	4.1	54.6	101	75-125
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
PERCHLORATE	µg/L	50	54.2	100	1	20	75-125
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 160.1

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 32933
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W2607	
LCS Filename: -	Date Analyzed: 042803	Time Analyzed: 17:19
LCSD Filename: -	Date Analyzed: 042803	Time Analyzed: 17:19

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
SOLIDS, TOTAL DISSOLVED (TDS)	mg/L	400	0	396	99	88-108
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	LCSD Concentration	LCSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
SOLIDS, TOTAL DISSOLVED (TDS)	mg/L	400	412	103	4	20	88-108
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 160.1

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 32933
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W2607	
MS Filename: -	Date Analyzed: 042803	Time Analyzed: 17:19
MSD Filename: -	Date Analyzed: 042803	Time Analyzed: 17:19
MS Sample No: MW-17-2	Sample Lab ID: 03-2933-3	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
SOLIDS, TOTAL DISSOLVED (TDS)	mg/L	400	250	679	107	80-119
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
SOLIDS, TOTAL DISSOLVED (TDS)	mg/L	400	652	101	6	20	80-119
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 7196

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 32933
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W2603	
LCS Filename: -	Date Analyzed: 042803	Time Analyzed: 16:53
LCSD Filename: -	Date Analyzed: 042803	Time Analyzed: 16:53

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
CHROMIUM (VI)	mg/L	0.25	0	0.239	96	80-115
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	LCSD Concentration	LCSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
CHROMIUM (VI)	mg/L	0.25	0.251	100	4	19	80-115
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 7196

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 32933
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W2603	
MS Filename: -	Date Analyzed: 042803	Time Analyzed: 16:53
MSD Filename: -	Date Analyzed: 042803	Time Analyzed: 16:53
MS Sample No: MW-17-2	Sample Lab ID: 03-2933-3	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
CHROMIUM (VI)	mg/L	0.25	0	0.238	95	78-115
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
CHROMIUM (VI)	mg/L	0.25	0.243	97	2	19	78-115
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

Wet Chemistry QC Report B
Duplicate Results

Matrix: Water

APCL Service ID: 03-2933

Analysis	Batch ID	Analysis Date	Sample Name	Unit	Result	Duplicate Result	RPD %	RPD Control limit
Bicarbonate	03W2665	05/01/2003	MW-17-1	mg/L	176	175	1	20
Carbonate	03W2665	05/01/2003	MW-17-1	mg-CaCO ₃ /L	ND	ND	NC	20
pH	03W2592	04/28/2003	03-2940-2	pH unit	7.58	7.58	0	20

Note: N/A = Not applicable; NR: Not requested; NC= Not Calculated; ND: Not detected.

6A
INITIAL CALIBRATION DATA

Lab Name: Applied P & Ch Lab Contract: _____

Analysis: Chromium (VI) Calibration Date: 01/29/2003

Concentration (mg/L)	0.000	0.0125	0.050	0.125	0.250	0.50
Absorbance	0.000	0.006	0.041	0.109	0.214	0.415

A = 0.000 + 0.836C

A = Absorbance

C = Concentration (mg/L)

r = 0.9997

DIONEX METHOD PARAMETERS - E300-063.MET

Method Comment: APCL EPA 300 ANALYSIS DX-100
 Column ID: Dionex AS4A-SC
 Analyst ID: David

System Parameters

System Name: DX-100	
Number of Detectors.....	1
Run Time (minutes).....	10.00
Sampling Rate (seconds).....	0.20
Detector 1 Type.....	COND
Detector 1 real time plot scale maximum (uS).....	30.000
minimum.....	-3.000
Detector 1 Output Equivalent to 1 Volt (in uS).....	30.00
Detector 1 ACI Analog Input Connection.....	DET1
Save Data File.....	Yes
Data File Name: C:\DX\DATA\03W1991\W1991Q01.D10	

-- DETECTOR 1 PARAMETERS --

Report Options

Create ASCII Report File.....	No
Print Report.....	Yes
Print All Components.....	Yes
Print Components Found.....	No
Print Missing Components.....	No
Print All Peaks.....	No
Print Unknown Peaks.....	No
Print Chromatogram.....	Yes
Autoscale Chromatogram Maximum.....	No
Autoscale Chromatogram Minimum.....	No
Fill Peaks with Color.....	No
Draw Grid Lines on Chromatogram.....	No
Show Component Fraction Numbers.....	No
Label with Peak Number.....	No
Label with Retention Times on Chromatogram.....	Yes
Label with Component Name.....	Yes
Format File Name: C:\DX\METHOD\DEFAULT.PRF	

Integration Parameters

Starting Peak Width (seconds).....	10.0
Peak Threshold.....	2.000
Peak Area Reject.....	1000
Area Reject for Reference Peaks.....	1000

Data Events

Time	Description

0.13	Start peak detection
10.00	Stop peak detection

Calibration Parameters

Number Of Levels for Calibration.....	6
Force Calibration Curve Through Origin.....	No
Calibration Fit Type.....	Linear
Replace Or Average Calibrations.....	Replace
External or Internal Calibration.....	External
Calculate Unknowns by Area or Height.....	Area
Default Sample Volume.....	1.0
Default Dilution Factor.....	1.0
Default Response Factor for Unknown Peaks.....	0.0
Calibration Standard Volume	1.0
Internal Standard Amount in Samples	1.0
Amount Units	ppm

Component # 4 Bromide Retention Time 3.45
 Reference Comp. Nitrate-N Window Size 0.20 min.
 Amount = $K0 + K1 \cdot \text{Area}$
 K0 = 4.58974E-002
 K1 = 4.83279E-006

Level	Amount	Area	Height
1	7.50000E-002	13830	1488
2	1.50000E+000	298206	30100
3	3.00000E+000	591234	61776
4	6.00000E+000	1219933	128845
5	7.50000E+000	1559887	166594
6	0.00000E+000	0	0

Component # 5 Nitrate-N Retention Time 3.87
 Reference Comp. Nitrate-N Window Size 0.25 min.
 Amount = $K0 + K1 \cdot \text{Area}$
 K0 = 4.24689E-002
 K1 = 8.05553E-007

Level	Amount	Area	Height
1	3.75000E-002	40157	3802
2	7.50000E-001	849179	77129
3	1.50000E+000	1713421	152776
4	3.00000E+000	3610927	313707
5	3.75000E+000	4688990	396441
6	0.00000E+000	0	0

Component # 6 Phosphate-P Retention Time 6.38
 Reference Comp. Phosphate-P Window Size 0.60 min.
 Amount = $K0 + K1 \cdot \text{Area}$
 K0 = 8.68926E-002
 K1 = 2.12227E-006

Level	Amount	Area	Height
1	7.50000E-002	24783	1450
2	1.50000E+000	642376	38579
3	3.00000E+000	1301126	79971
4	6.00000E+000	2756481	168994
5	7.50000E+000	3546397	217521
6	0.00000E+000	0	0

Component Table -- Last Modified: 17:42 on Fri, 21 Mar 2003

Component # 1 Fluoride Retention Time 1.32
Reference Comp. Fluoride Window Size 0.15 min.
Amount = K0 + K1*Area
K0 = -9.62851E-004
K1 = 1.37614E-006

Level	Amount	Area	Height
1	2.50000E-002	28534	2732
2	5.00000E-001	373164	44629
3	1.00000E+000	707646	82595
4	2.00000E+000	1435865	173007
5	2.50000E+000	1837162	220914
6	0.00000E+000	0	0

Component # 2 Chloride Retention Time 1.97
Reference Comp. Chloride Window Size 0.15 min.
Amount = K0 + K1*Area
K0 = 1.28188E-001
K1 = 1.95287E-006

Level	Amount	Area	Height
1	1.00000E-001	51206	7044
2	2.00000E+000	909455	126181
3	4.00000E+000	1856586	261681
4	8.00000E+000	3987563	585791
5	1.00000E+001	5142155	754321
6	0.00000E+000	0	0

Component # 3 Nitrite-N Retention Time 2.33
Reference Comp. Chloride Window Size 0.15 min.
Amount = K0 + K1*Area
K0 = 2.38085E-002
K1 = 9.76240E-007

Level	Amount	Area	Height
1	3.75000E-002	30884	3582
2	7.50000E-001	734006	79701
3	1.50000E+000	1468106	162005
4	3.00000E+000	3021523	336616
5	3.75000E+000	3856614	429219
6	0.00000E+000	0	0


Component # 7 Sulfate Retention Time 7.92
 Reference Comp. Sulfate Window Size 0.90 min.
 Amount = K0 + K1*Area
 K0 = 5.32283E-001
 K1 = 2.53252E-006

Level	Amount	Area	Height
1	3.76000E-001	129999	6524
2	7.50000E+000	2598757	138579
3	1.50000E+001	5330209	287851
4	3.00000E+001	11507107	615917
5	3.75000E+001	14859049	776426
6	0.00000E+000	0	0

Timed Events File: C:\DX\METHOD\W761CAL.TE


Step	Time	Description
Init		ACI Autosmp OFF
Init		ACI pump st ON
Init		ACI inject OFF
Init		ACI auto zer OFF
Init		ACI TTL 1 OFF
Init		ACI TTL 2 OFF
Init		ACI TTL 3 OFF
Init		ACI TTL 4 OFF
Init		ACI OFF
Init		ACI OFF
1	0.0	ACI Autosmp ON
1	0.0	ACI auto zer ON
2	2.5	ACI Autosmp OFF
2	2.5	ACI inject ON
2	2.5	ACI TTL 1 ON
2	2.5	Start Sampling

Component: Fluoride
Fit Type: Linear
 $r^2 = 0.999552$
Amt = Resp * $1.376e-006$ + -0.000962
Resp = Amt * $-7.267e+005$ + 699.7
Standardization: External
Calibration: Area

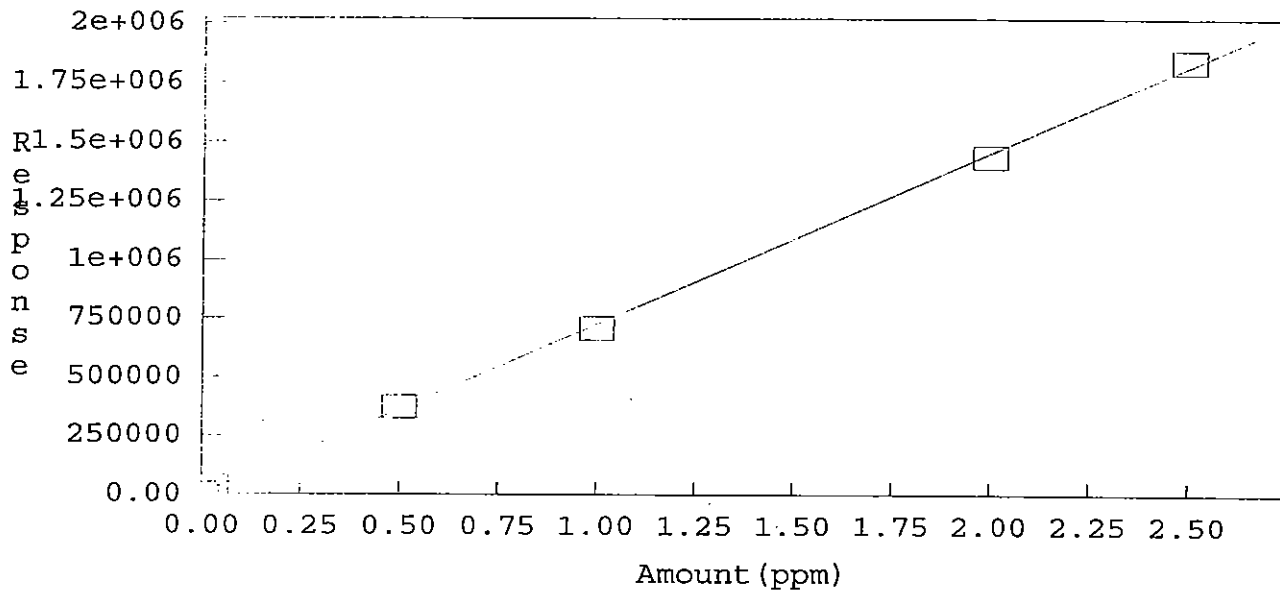

Method: C:\DX\METHOD\E300-063.MET

Component: Chloride
Fit Type: Linear
 $r^2 = 0.998409$
Amt = Resp * $1.953e-006$ + 0.1282
Resp = Amt * $5.121e+005$ + $-6.564e+00$
Standardization: External
Calibration: Area

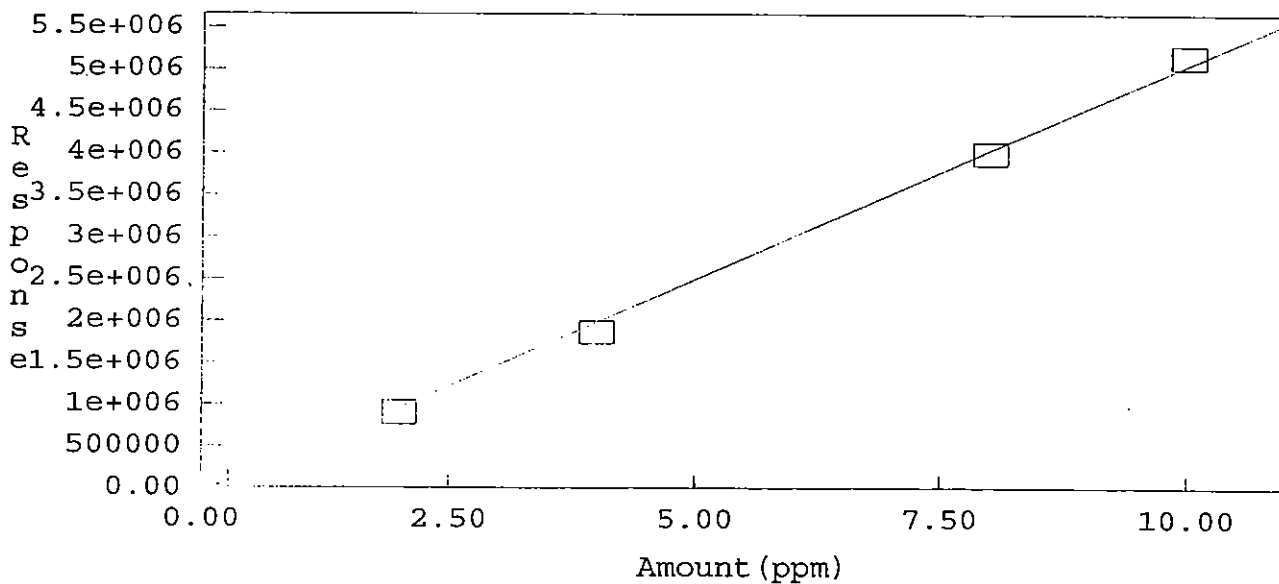

Method: C:\DX\METHOD\E300-063.MET

Component: Nitrite-N

Fit Type: Linear


$r^2 = 0.999594$

Amt = Resp * $9.762e-007$ + 0.02381

Resp = Amt * $1.024e+006$ + -2.439e+00

Standardization: External

Calibration: Area

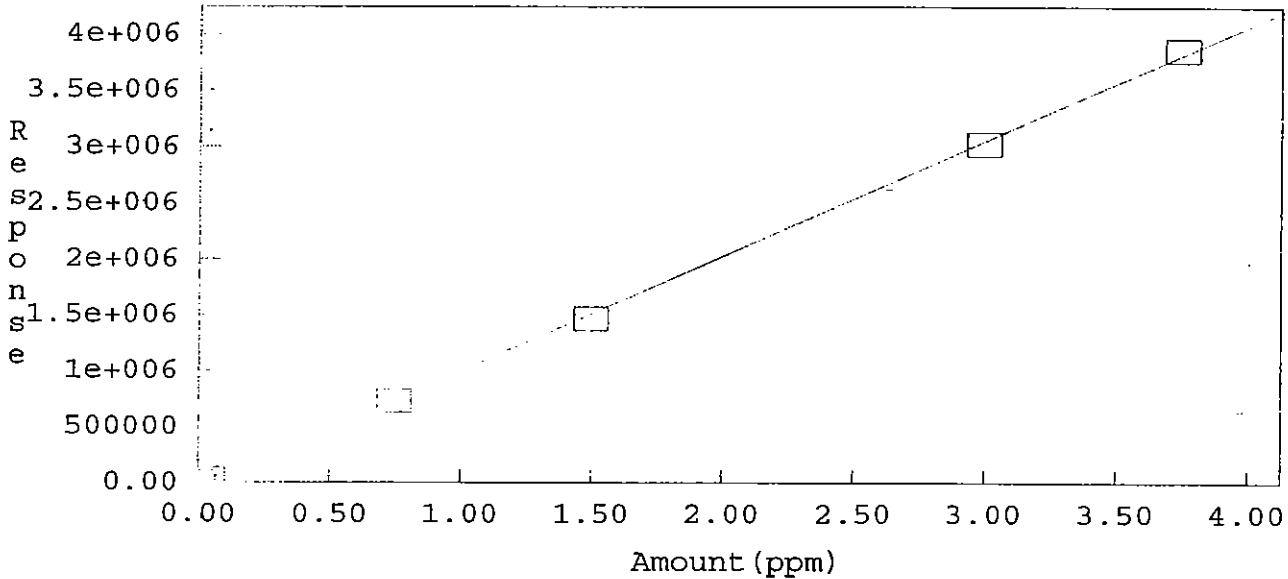

Method: C:\DX\METHOD\E300-063.MET

Component: Bromide

Fit Type: Linear


$r^2 = 0.999518$

Amt = Resp * $4.833e-006$ + 0.0459

Resp = Amt * $2.069e+005$ + -9497

Standardization: External

Calibration: Area

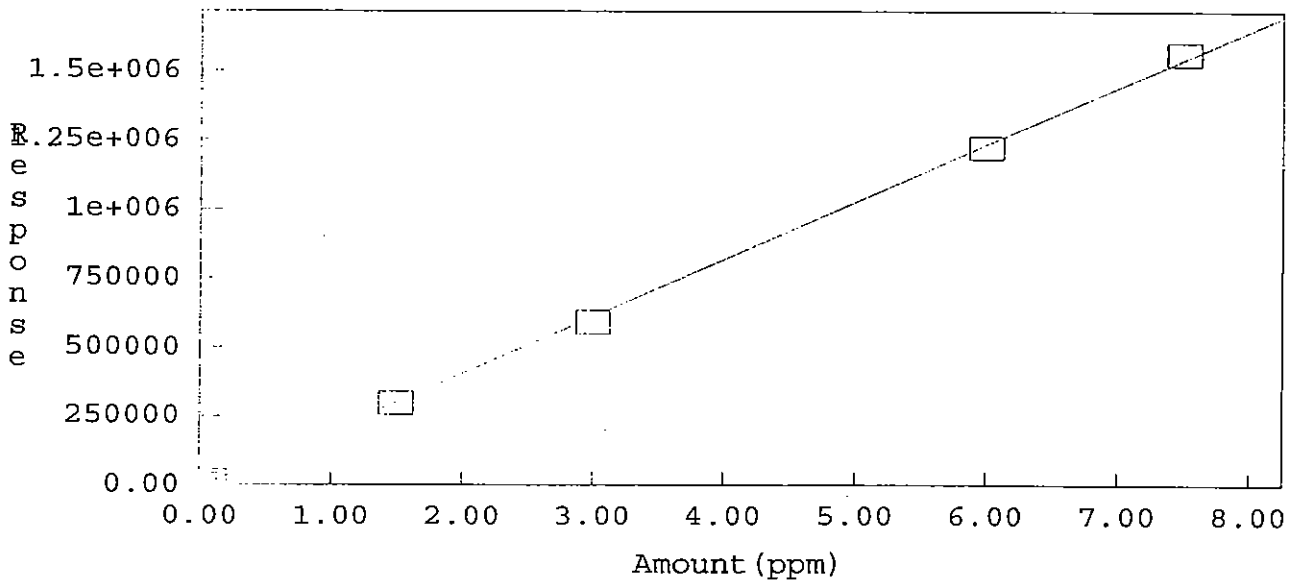

Method: C:\DX\METHOD\E300-063.MET

Component: Nitrate-N

Fit Type: Linear


$r^2 = 0.998618$

Amt = Resp * $8.056e-007$ + 0.04247

Resp = Amt * $1.241e+006$ + $-5.272e+00$

Standardization: External

Calibration: Area

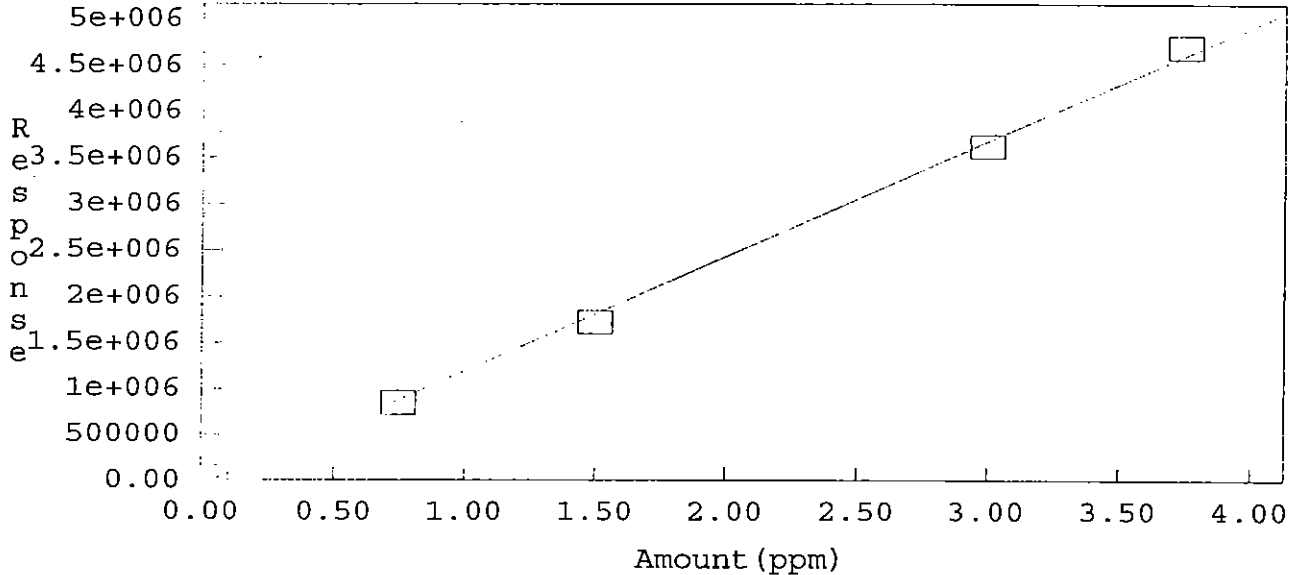

Method: C:\DX\METHOD\E300-063.MET

Component: Phosphate-P

Fit Type: Linear


$r^2 = 0.998898$

Amt = Resp * $2.122e-006$ + 0.08689

Resp = Amt * $4.712e+005$ + $-4.094e+00$

Standardization: External

Calibration: Area

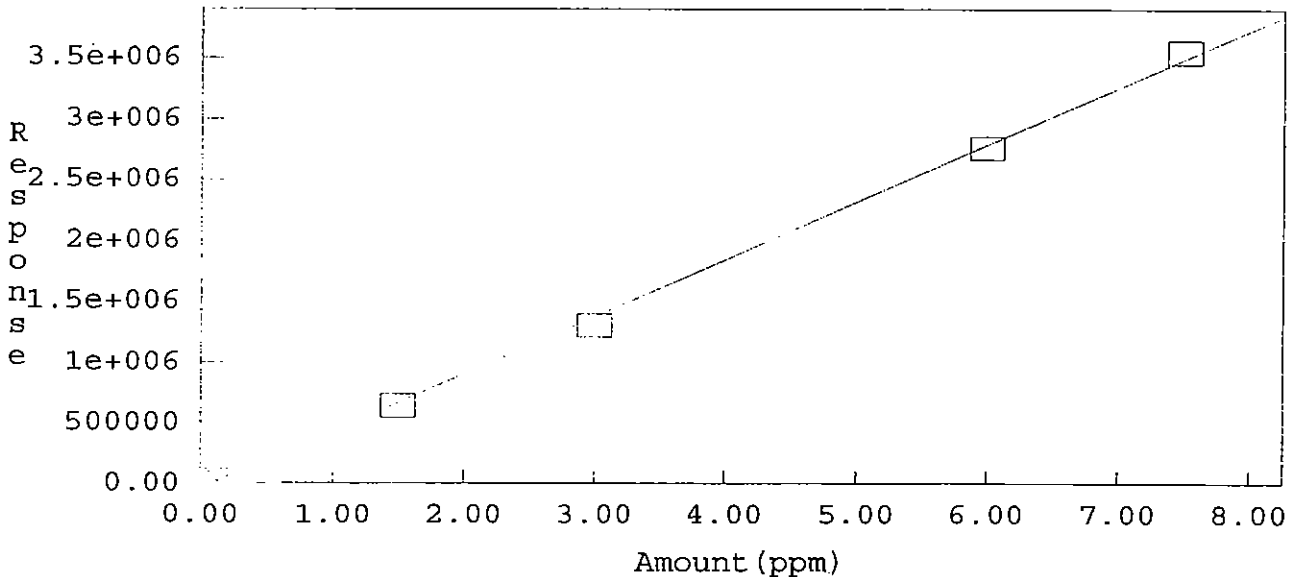

Method: C:\DX\METHOD\E300-063.MET

Component: Sulfate

Fit Type: Linear


$r^2 = 0.998245$

$Amt = Resp * 2.533e-006 + 0.5323$


$Resp = Amt * 3.949e+005 + -2.102e+00$

Standardization: External

Calibration: Area

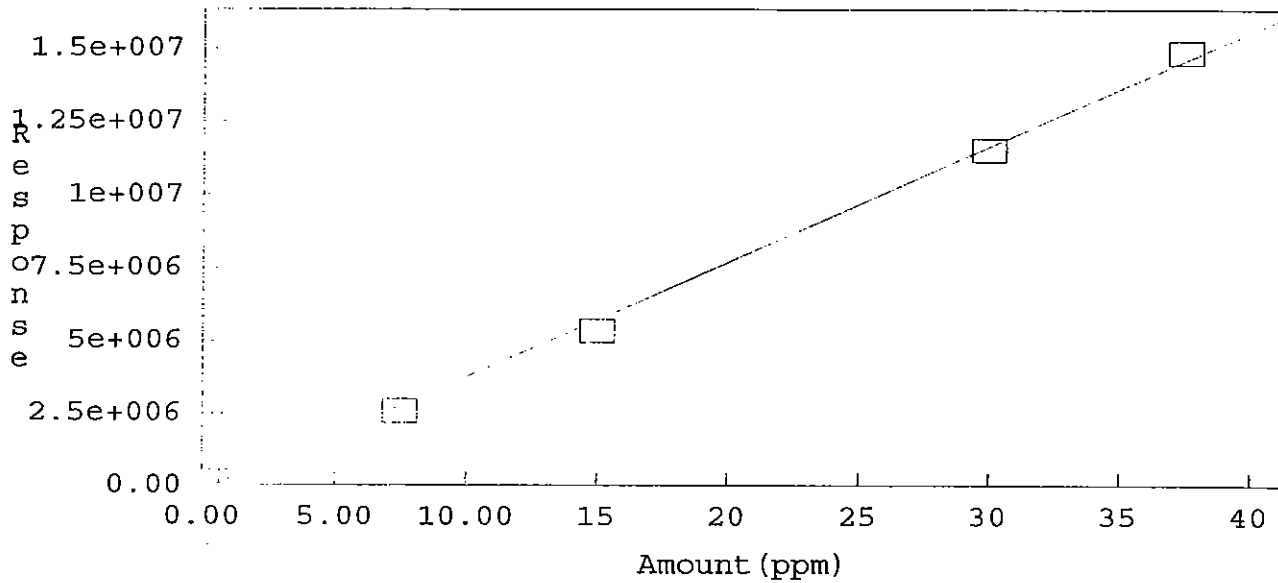

1. Component: perchlorate
Standard: External Fit Type: Linear
Origin: Force Calibration: Area
 $r^2=0.999492$
Amt= $0.0005893 * Resp + 0$

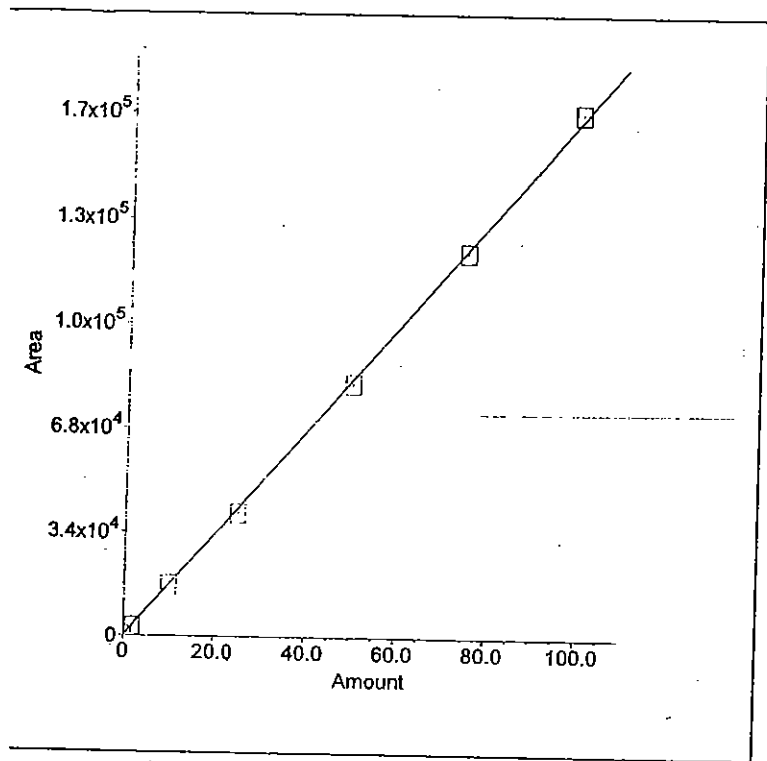

Calibration : 7 points , 0, 2, 10, 25, 50, 75, 100 ppb

Analyst C.W
Date 03/12/03
Instrument LC-10

FORM-7
Applied P & Ch Laboratory
CCV Recovery for Wet Analysis

Client Name: GEOFON, Inc.
Case No:
Project ID: JPL

Contract No.:
SAS No.:
Project No.: 04-4428.10

Lab Code: APCL
Service ID: 32933

#	Component Name	Method	Batch No.	Unit	Expected	Test Result	Rec. %	Dev. %	Flag	Control Limit, %	Test Date
1	Chloride Cl ⁻	300.0	03W2610	mg/L	4.0	3.79	95	-5	✓	90-110	04/29/2003
	NITRATE as N-NO ₃ ⁻ , BY	300.0	03W2610	mg/L	1.5	1.45	96	-4	✓	90-110	04/29/2003
	SULFATE SO ₄ ⁻ , BY I	300.0	03W2610	mg/L	15	14.3	95	-5	✓	90-110	04/29/2003
	Chloride Cl ⁻	300.0	03W2610	mg/L	4.0	3.91	98	-2	✓	90-110	04/29/2003
	NITRATE as N-NO ₃ ⁻ , BY	300.0	03W2610	mg/L	1.5	1.49	99	-1	✓	90-110	04/29/2003
	SULFATE SO ₄ ⁻ , BY I	300.0	03W2610	mg/L	15	15.0	100	0	✓	90-110	04/29/2003
	Chloride Cl ⁻	300.0	03W2610	mg/L	4.0	3.93	98	-2	✓	90-110	04/29/2003
	NITRATE as N-NO ₃ ⁻ , BY	300.0	03W2610	mg/L	1.5	1.52	101	1	✓	90-110	04/29/2003
	SULFATE SO ₄ ⁻ , BY I	300.0	03W2610	mg/L	15	14.9	99	-1	✓	90-110	04/29/2003
	Chloride Cl ⁻	300.0	03W2610	mg/L	4.0	3.88	97	-3	✓	90-110	04/29/2003
	NITRATE as N-NO ₃ ⁻ , BY	300.0	03W2610	mg/L	1.5	1.50	100	0	✓	90-110	04/29/2003
	SULFATE SO ₄ ⁻ , BY I	300.0	03W2610	mg/L	15	14.7	98	-2	✓	90-110	04/29/2003
2	Perchlorate	314.0	03W2612	μg/L	50	53.1	106	6	✓	90-110	04/29/2003
	Perchlorate	314.0	03W2612	μg/L	50	49.8	100	0	✓	90-110	04/29/2003
	Perchlorate	314.0	03W2612	μg/L	50	50.8	102	2	✓	90-110	04/29/2003
	Perchlorate	314.0	03W2612	μg/L	50	48.9	98	-2	✓	90-110	04/29/2003
3	Chromium (VI)	7196	03W2603	mg/L	0.25	0.255	102	2	✓	90-110	04/28/2003
	Chromium (VI)	7196	03W2603	mg/L	0.25	0.250	100	0	✓	90-110	04/28/2003

Applied P & Ch Laboratory
 Magnolia Ave. Chino CA 91710
 (909) 590-1828 Fax: (909) 590-1498

Conductance (120.1) Worksheet

06

for reference: W
 Matrix: W
 Constant _____ Calibration STD: 0.0100M KCl

Test Date: 6/30/03 Analyst: ww

SOP: G-4

Sample ID	Treatment V/X=f ₀	Dilution V _f /V _i =f ₁	Temperature T, °C	C ₂₅ = C _T f ₁ /[1-0.0191(25-T)] C _T , μmhos/cm	C ₂₅ , μmhos/cm	ρ=1/C ₂₅ MΩ cm	Note & Anomaly
Gal. Lot #:	-	-	25°C				C ₂₅ =1,413±20
MB	/ =	/ =	↓				for cell
1 2833-1	/ =	/ =		21.6			
2 -2	/ =	/ =		437			
3 -3	/ =	/ =		364			
4 -4	/ =	/ =		404			
5 -5	/ =	/ =		302			
6 -6	/ =	/ =		349			
7 2864-1	/ =	/ =		412			
8 -2	/ =	/ =		25.2			
9 -3	/ =	/ =		538			
10 -4	/ =	/ =		364			
11 -5	/ =	/ =		360			
12 -6	/ =	/ =		297			
13 -7	/ =	/ =	401				
14	/ =	/ =					
15	/ =	/ =					
16	/ =	/ =					
17	/ =	/ =					
18	/ =	/ =					
19	/ =	/ =					
20	/ =	/ =					
Dup.	/ =	/ =					

13780 Magnolia Ave. Chino CA 91710

TDS
Solid Analysis (160.1, 160.2, 160.3) Worksheet

Tel: (909) 590-1828 Fax: (909) 590-1498

Batch # 03W260 Matrix W Method: 160.1 Balance No. _____

Date: 4/28/03 Analyst: DC

EPA 160.1 TDS - Total Dissolved (filterable) Solids - Dry for 1hr. or more at 180 °C

EPA 160.2 TSS - Total Suspended (nonfilterable) Solids - Dry for 1hr. or more at 103-105 °C

EPA 160.3 TS - Total Solids - Dry for 1hr. or more at 103-105 °C

Other method (specify):

Result = $10^6 \times \Delta W \times J_1 / V$

SOP: G-81

#	Analysis Type	Sample ID (STD Lot #)	Treatment Ratio $V_1/X=f_1$	Volume V, mL	W ₁ g	W ₂ 1st, g	W ₂ 2nd, g	Δ W = W ₂ -W ₁ , g	Results (ppm)	Note
1	Blank	T1116	1 =	100	111.7909	111.7908	111.7909	0.0000	0	R
2	LCS	T1116	1 =		113.859	113.8989	113.8987	0.0396	396	6
3	Sample-1	2866-1	1 =		103.944	103.974	103.974	0.0298	298	14
4	MS on S-1	2933-3	1 =		111.2769	111.3486	111.3448	0.0679	679	J
5	MSD on S-1	3	1 =		114.307	114.372	114.3723	0.0652	652	H
6	Sample-2	2866-2	1 =		104.307	104.3076	104.3078	0.0001	1	3
7	Sample-3	3	1 =		115.1364	115.1614	115.1615	0.0251	251	10
8	Sample-4	4	1 =		114.369	114.3928	114.3929	0.0235	235	A
9	Sample-5	5	1 =		115.911	115.9449	115.9450	0.0333	333	Y9
10	Sample-6	6	1 =		116.9493	116.9693	116.9694	0.0201	201	W
11	Sample-7	7	1 =		115.7069	115.741	115.7416	0.0347	347	HKS
12	Sample-8	2881-1	1 =		106.324	106.340	106.3400	0.0155	155	8
13	Sample-9	2	1 =		107.7107	107.7356	107.7357	0.0250	250	0
14	Sample-10	3	1 =		105.312	105.366	105.3669	0.0544	544	12
15	LCSD	T1116	1 =		112.9002	112.942	112.944	0.0412	412	*
16	Sample-11	4	1 =		121.3177	121.3567	121.356	0.0388	388	I
17	Sample-12	5	1 =		105.352	105.3998	105.3996	0.0421	421	W1
18	Sample-13	6	1 =		99.0757	99.0946	99.0945	0.0188	188	Y2
19	Sample-14	2933-1	1 =		103.5328	103.5328	103.5328	0.0000	0	26
20	Sample-15	2	1 =		115.1082	115.1334	115.1335	0.0253	253	G
21	Sample-16	3	1 =		115.3468	115.371	115.3718	0.0250	250	J
22	Sample-17	4	1 =		116.6429	116.675	116.672	0.0247	247	ZJ
23	Sample-18	5	1 =		105.8998	105.929	105.9296	0.0198	198	19
24	Sample-19	6	1 =		115.8730	115.8948	115.8949	0.0219	219	CK
25	Sample-20	2948-1	1 =							
26	Mix Dup.		1 =							

Type	STD Lot #	CSTD(μs/mL) × V _{STD} (mL) / X(g or mL) = T	Spike Rec.	Ctl Limit (W/S)	PQL/MDL (in ppm)
MS	W-7618	x / = 4000 ppm	%	85-115 % / 80-120 %	PQL(w) 10
MSD	W-	x / = ppm	%	PQL(s) 50
LCS	W-7619	x / = ppm	%	90-110 % / 85-115 %	MDL(w) 4
LCSD	W-	x / = ppm	%	MDL(s) 20

Balance Daily Calibration Worksheet

Weight Set S/N: 12006

085
485

Calib. Date	Lab Balance					Digital Balance					Analytical Balance					Calib. by
	Balance #	1 g ±0.05g	10 g ±0.1g	200 g ±0.5g	Note (C)	Balance #	1 g ±0.02g	10 g ±0.05g	200 g ±0.10g	Note (D) (C) (AR)	Balance #	1 g ±0.0002g	10 g ±0.0005g	200 g ±0.0010g	Note (D) (C) (AR)	
4/25/03	A-01	Net	W	W	✓	B-01	1.00	10.00	200.00	✓ ✓ ✓	C-01	1.0000	10.0000	200.0000	✓ ✓ ✓	
	A-02					B-05	1.00	9.99	199.99	✓ ✓ ✓	C-02	1.0000	10.0000	200.0000	✓ ✓ ✓	
	A-03	1.00	9.99	200.00	✓	B-06	1.00	10.00	200.00	✓ ✓ ✓						
	A-04	1.00	9.99	200.00	✓	B-07	1.00	9.99	199.99	✓ ✓ ✓						
4/29/03	A-	4/29/03				B-	4/29/03				C-	4/29/03				
	A-01	Net	W	W	✓	B-01	1.00	10.01	200.00	✓ ✓ ✓	C-01	1.0000	10.0000	200.0000	✓ ✓ ✓	
	A-02					B-05	1.00	9.99	199.99	✓ ✓ ✓	C-02	1.0000	10.0000	200.0000	✓ ✓ ✓	
	A-03	1.00	9.99	200.00	✓	B-06	1.00	10.00	200.00	✓ ✓ ✓						
4/30/03	A-04	1.00	9.99	200.00	✓	B-07	1.00	9.99	199.99	✓ ✓ ✓						
	A-	4/30/03				B-	4/30/03				C-	4/30/03				
	A-01	Net	W	W	✓	B-01	1.00	10.01	200.00	✓ ✓ ✓	C-01	1.0000	10.0000	200.0000	✓ ✓ ✓	
	A-02					B-05	1.00	9.99	199.99	✓ ✓ ✓	C-02	1.0000	10.0000	200.0000	✓ ✓ ✓	

Notation: (C) - Cleanliness; (D) - Display; (AR) - Auto Zeroing.
 APCL form 4213, March 30, 1995, Ver. 4.0 No pencil. Use blue pen for record. Use red pen for correction.
 PRT-INST-DOC-LAB/BAL-CAL-TEX Root-File: BAL-CAL-FOOT-TEX 1-Page-File: BAL-CALI-1-TEX

Alkalinity / OH / CO₃ / HCO₃ (310.1 / SM2320B) Worksheet 02h

Batch # D302661 Matrix: W Titrant H₂SO₄ Lot # W7900 Concentration (CO₂) 0.025% Test Date: 5/1/03 Analyst: RL SOP: G-51

#	Sample ID	Dilution V ₁ /V ₂ =f ₁	Smp Amt V ₁ , mL	H ₂ SO ₄ (mL) by Phnh		H ₂ SO ₄ (mL) by MR-BCG		Phnh-Alk., P (in unit of mgCaCO ₃ /L)	Tot. Alk., T	OH ⁻	CO ₃ ²⁻	HCO ₃ ⁻	Note & Anomaly
				S _A	E _A	S _B	E _B						
1	MB: T111	1 =	100	0		0		0	0	0	0		
2	LS	1 =	100	7.90		100.9		100.9	0	0	0		
3	165D	1 =	100	8.60		102.2		102.2	0	0	0		
4	2933-1	1 =	10.0	0		0		0	0	0	0		
5	-2	1 =	10.0	0		0		0	0	0	0		
6	-3	1 =	10.0	0		0		0	0	0	0		
7	-4	1 =	10.0	0		0		0	0	0	0		
8	-5	1 =	10.0	0		0		0	0	0	0		
9	-6	1 =	10.0	0		0		0	0	0	0		
10	2015-1	1 =	10.0	0		0		0	0	0	0		
11	-2	1 =	10.0	0		0		0	0	0	0		
12	-3	1 =	10.0	0		0		0	0	0	0		
13	-4	1 =	10.0	0		0		0	0	0	0		
14	-5	1 =	10.0	0		0		0	0	0	0		
15	-6	1 =	10.0	0.10		5.10		143.1	0	0	143.1		
16	-7	1 =	10.0	0.80		4.25		132.9	0	0	132.9		
17	2964-1	1 =	10.0	0.20		4.60		122.6	0	0	122.6		
18	2964-2	1 =	10.0	0		0		0	0	0	0		
19	-3	1 =	10.0	0		0		0	0	0	0		
20	-4	1 =	10.0	0.2		4.65		123.9	0	0	123.9		
Dup.	2933-2	1 =	10.0	0		6.85		175.6	0	0	175.6		

Calculations:
 A = 5 · A · E_A
 B = 5 · B · E_B
 P = 50,000 f₁ A C / V
 T = 50,000 f₁ (A+B) C / V

Titration Results	OH ⁻ (CaCO ₃ mg/L)	CO ₃ ²⁻ (CaCO ₃ mg/L)	HCO ₃ ⁻ (CaCO ₃ mg/L)
P=0	0	0	T
P<T/2	0	2P	T-2P
P=T/2	0	2P	0
P>T/2	2P-T	2(T-P)	0
P=T	T	0	0

Temperature compensation must be performed by the instrument automatically.

Analyst DL

SOP: G-44

Batch # <u>03W2592</u>	Analysis Date: <u>4/28/03</u>	Batch # <u>03W2631</u>	Analysis Date: <u>4/29/03</u>				
Starting Time: <u>16:22</u>	Ending Time: _____	Starting Time: <u>16:10</u>	Ending Time: _____				
Matrix <input checked="" type="checkbox"/> Aqueous <input type="checkbox"/> Soil		Matrix <input checked="" type="checkbox"/> Aqueous <input type="checkbox"/> Soil					
Standard	4.00	7.00	10.00	Standard	4.00	7.00	10.00
Lot #		<u>2120</u>	<u>030659-24</u>	Lot #		<u>2120</u>	<u>030659-24</u>
Temperature °C		<u>24.2</u>	<u>24.2</u>	Temperature °C		<u>24.0</u>	<u>24.0</u>
pH Reading		<u>7.07</u>	<u>10.02</u>	pH Reading		<u>6.49</u>	<u>10.00</u>
T-corrected pH		<u>7.00</u>	<u>10.07</u>	T-corrected pH		<u>7.00</u>	<u>10.07</u>
Control Limit	±0.05 pH unit			Control Limit	±0.05 pH unit		

#	Sample ID	Pre-treat	pH	Note	#	Sample ID	Pre-treat	pH	Note
MB	<u>T1116</u>		<u>6.87</u>		MB	<u>T1116</u>		<u>6.85</u>	
1	<u>2940-2</u>		<u>7.58</u>		1	<u>2959-2</u>		<u>8.65</u>	
2	<u>2933-1</u>		<u>6.54</u>		2	<u>2961-2</u>		<u>8.10</u>	
3	<u>-2</u>		<u>7.44</u>		3	<u>2964-1</u>		<u>8.22</u>	
4	<u>-3</u>		<u>7.97</u>		4	<u>-2</u>		<u>7.77</u>	
5	<u>-4</u>		<u>8.68</u>		5	<u>-3</u>		<u>7.90</u>	
6	<u>-5</u>		<u>8.07</u>		6	<u>-4</u>		<u>8.40</u>	
7	<u>-6</u>		<u>8.17</u>		7	<u>-5</u>		<u>8.89</u>	
8					8	<u>-6</u>		<u>9.01</u>	
9					9	<u>-7</u>		<u>8.04</u>	
10					10				
11					11				
12					12				
13					13				
14					14				
15					15				
16					16				
17					17				
18					18				
19					19				
20					20				
Dup.	<u>2940-2</u>		<u>7.58</u>		Dup.	<u>2964-7</u>		<u>8.09</u>	

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710
Tel: (909) 590-1828 Fax: (909) 590-1498

Chromium (VI) (7196) Worksheet

Batch # 03W2603 Matrix: u

[Holding Time: 24 hours!!]

Test Date: 4/28/03 Analyst: R

Lot #: Reagent Water _____ Diphenylcazide solution _____ Test Time: 16:53 SOP: G-22

Calibration	STD Lot #	$C_{std} \times V_{std} / V_f = C_i$	A_i	$RF_i = A_i / C_i$	Calibration results	Note
STD-1	W-	x / = mg/L			Least Square [RF]=	Cal. Code:
STD-2	W-	x / = mg/L			Average RF=	
STD-3	W-	x / = mg/L			C.C. = <u>0.9997</u> ≥ 0.995	
STD-4	W-	x / = mg/L			RSD = % (< 15%)	
STD-5	W-	x / = mg/L			Ref. page	
STD-6	W-	x / = mg/L				

A = 0.000 + 0.836C

Analysis Type	Sample ID or Lot #	Samp. Amnt X ₀ (g or mL)	Dilu./Ext X/X ₀ =f ₁	Treat. Ratio V/X=f ₂	540 nm A	Concentration C' = A/RF	C (Sample) C=f ₁ f ₂ C'	Anomaly Note
CCV	Lot: W- <u>7853</u>	Expected Conc.: x	1	= <u>0.25</u> mg/L	<u>0.23</u>	<u>0.25</u> mg/L	REC. %	90-110 %
Method Blank	Bl. Lot: <u>T1116</u>		X ₀ = 1	95.0/ =	<u>0.000</u>	mg/L	<u>0.000</u> ppm	
LCS1	Bl. Lot: <u>1</u>		X ₀ =	95.0/ =	<u>0.200</u>	mg/L	<u>0.229</u> ppm	
Sample-1	<u>2933-1</u>		X ₀ =	95.0/ =	<u>0.003</u>	mg/L	<u>0.003</u> ppm	
MS on S-1	<u>3</u>		X ₀ =	95.0/ =	<u>0.199</u>	mg/L	<u>0.238</u> ppm	
MSD on S-1	<u>3</u>		X ₀ =	95.0/ =	<u>0.203</u>	mg/L	<u>0.743</u> ppm	
Sample 2	<u>2</u>		X ₀ =	95.0/ =	<u>0.002</u>	mg/L	<u>0.002</u> ppm	
Sample 3	<u>3</u>		X ₀ =	95.0/ =	<u>0.002</u>	mg/L	<u>0.002</u> ppm	
Sample 4	<u>4</u>		X ₀ =	95.0/ =	<u>0.001</u>	mg/L	<u>0.001</u> ppm	
Sample 5	<u>5</u>		X ₀ =	95.0/ =	<u>0.001</u>	mg/L	<u>0.001</u> ppm	
Sample 6	<u>6</u>		X ₀ =	95.0/ =	<u>0.001</u>	mg/L	<u>0.001</u> ppm	
Sample 7			X ₀ =	95.0/ =		mg/L	ppm	
Sample 8			X ₀ =	95.0/ =		mg/L	ppm	
Sample 9			X ₀ =	95.0/ =		mg/L	ppm	
Sample 10			X ₀ =	95.0/ =		mg/L	ppm	
Blank	Lot:		X ₀ =	95.0/ =		mg/L	ppm	
LCS2	Bl. Lot: <u>T1116</u>		X ₀ = 1	95.0/ =	<u>0.210</u>	mg/L	<u>0.25</u> ppm	
Sample 11			X ₀ =	95.0/ =		mg/L	ppm	
Sample 12			X ₀ =	95.0/ =		mg/L	ppm	
Sample 13			X ₀ =	95.0/ =		mg/L	ppm	
Sample 14			X ₀ =	95.0/ =		mg/L	ppm	
Sample 15			X ₀ =	95.0/ =		mg/L	ppm	
Sample 16			X ₀ =	95.0/ =		mg/L	ppm	
Sample 17			X ₀ =	95.0/ =		mg/L	ppm	
Sample 18			X ₀ =	95.0/ =		mg/L	ppm	
Sample 19			X ₀ =	95.0/ =		mg/L	ppm	
Sample 20			X ₀ =	95.0/ =		mg/L	ppm	
MEX Dup.	<u>03W2603</u>		X ₀ =	95.0/ =	<u>0.209</u>	mg/L	ppm	

STD Lot #	CSTD (μg/mL) × VSTD (mL) / X (g or mL) = T	Spike Rec.	Ctl Limit (W/S)	PQL/MDL (in ppm)
W- <u>7759</u>	x / = <u>0.25</u> ppm	%	80-120 %/80-120 %	PQL(w) 0.01
W- <u>1</u>	x / = ppm	%	PQL(s) 0.05
W- <u>7853</u>	x / = ppm	%	80-120 %/80-120 %	MDL(w) 0.005
W- <u>1</u>	x / = ppm	%	MDL(s) 0.025

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710
Tel: (909) 590-1828 Fax: (909) 590-1498

Chromium (VI) (7196) Worksheet

Batch # 03W1295 Matrix: W

[Holding Time: 24 hours!!]

Test Date: 1/29/03 Analyst: B.V.

Lot #: Reagent Water _____ Diphenylcazide solution _____ Test Time: _____ SOP: G-22

Calibration	STD Lot #	$C_{std} \times V_{std} / V_f = C_i$	A_i	$RF_i = A_i / C_i$	Calibration results	Note
STD-1	W-7191	x / = 0.000 mg/L	0.000		Least Square [RF]=	Cal. Code:
STD-2	W-	x / = 0.012 mg/L	0.006		Average RF=	A=0.000+0.836c
STD-3	W-	x / = 0.050 mg/L	0.041		C.C.=0.977 (> 0.995)	
STD-4	W-	x / = 0.175 mg/L	0.109		RSD= % (< 15%)	
STD-5	W-	x / = 0.250 mg/L	0.214		Ref. page	
STD-6	W- ✓	x / = 0.50 mg/L	0.415		A=0.003+0.836c	

Analysis Type	Sample ID or Lot #	Samp. Amnt X ₀ (g or mL)	Dilu./Ext X/X ₀ =f ₁	Treat. Ratio V/X=f ₂	540 nm A	Concentration C'=A/RF	C (Sample) C=f ₁ f ₂ C'	Anomaly Note
CCV	Lot: W-7076	Expected Conc.: x	/	= 0.25 mg/L	0.216	0.258 mg/L	REC. %	90-110 %
Method Blank	Bl. Lot: T1115		/X ₀ = 1	95.0/ =	0.000	mg/L	0.00 ppm	
LCS1	Bl. Lot: 4		/X ₀ =	95.0/ =	0.209	mg/L	0.244 ppm	
Sample-1	1369-1		/X ₀ =	95.0/ =	0.000	mg/L	0.00 ppm	
MS on S-1	6		/X ₀ =	95.0/ =	0.223	mg/L	0.266 ppm	
MSD on S-1	6		/X ₀ =	95.0/ =	0.230	mg/L	0.275 ppm	
Sample 2	12		/X ₀ =	95.0/ =	0.004	mg/L	0.005 ppm	
Sample 3	3		/X ₀ =	95.0/ =	0.002	mg/L	0.002 ppm	
Sample 4	4		/X ₀ =	95.0/ =	0.001	mg/L	0.001 ppm	
Sample 5	5		/X ₀ =	95.0/ =	0.002	mg/L	0.002 ppm	
Sample 6	6		/X ₀ = ✓	95.0/ =	0.004	mg/L	0.005 ppm	
Sample 7			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 8			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 9			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 10			/X ₀ =	95.0/ =		mg/L	ppm	
Blank	Lot:		/X ₀ =	95.0/ =		mg/L	ppm	
LCS2	Bl. Lot: T1115		/X ₀ = 1	95.0/ =	0.210	mg/L	0.251 ppm	
Sample 11			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 12			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 13			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 14			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 15			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 16			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 17			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 18			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 19			/X ₀ =	95.0/ =		mg/L	ppm	
Sample 20			/X ₀ =	95.0/ =		mg/L	ppm	
MTX Dup.	losing 0.25 mg/L		/X ₀ =	95.0/ =	0.204	mg/L	0.244 ppm	

Type	STD Lot #	$C_{STD}(\mu\text{g/mL}) \times V_{STD}(\text{mL}) / X(\text{g or mL}) = T$	Spike Rec.	Ctl Limit (W/S)	PQL/MDL (in ppm)
MS	W- 7076	x / = 0.25 ppm	%	80-120 %/80-120 %	PQL(w) 0.01
MSD	W- ✓	x / = ppm	%	PQL(s) 0.05
LCS	W- 7191	x / = ppm	%	80-120 %/80-120 %	MDL(w) 0.005
LCSD	W- ✓	x / = ppm	%	MDL(s) 0.025

DIONEX SCHEDULE - C:\DX\SCHEDULE\E300-063.SCH

Inj#	Sample Name	Method	Data File	Vol.	Dil.	Int.Std.
1	autocal1r	..\E300-063	..\W7767Q01.D01	1	1	1
2	autocal2r	..\E300-063	..\W7767Q01.D02	1	1	1
3	autocal3r	..\E300-063	..\W7767Q01.D03	1	1	1
4	autocal4r	..\E300-063	..\W7767Q01.D04	1	1	1
5	autocal5r	..\E300-063	..\W7767Q01.D05	1	1	1
6	autocal6r	..\E300-063	..\W7767Q01.D06	1	1	1
7	icv-w7768-100X	..\E300-063	..\W7768Q01.D07	1	1	1
8	icb	..\E300-063	..\W7767Q01.D08	1	1	1

Comment :

Analyst *DN*
 Date 3/21/03
 Instrument J

DIONEX SCHEDULE - C:\DX\SCHEDULE\03W2610.SCH

Inj#	Sample Name	Method	Data File	Vol.	Dil.	Int.Std.
1	##03W2610, W CCVW77	.. \E300-063	.. \W2610Q01.D01	1	1	1
2	MB RW1409	.. \E300-063	.. \W2610K11.D02	1	1	1
3	LCS W7768-100X	.. \E300-063	.. \W2610L01.D03	1	1	1
4	LCSD W7768-100X	.. \E300-063	.. \W2610J01.D04	1	1	1
5	2933-2 F=2	.. \E300-063	.. \2933-201.D05	1	2	1
6	2933-3 F=2	.. \E300-063	.. \2933-301.D06	1	2	1
7	2933-4 F=2	.. \E300-063	.. \2933-401.D07	1	2	1
8	2933-5 F=2	.. \E300-063	.. \2933-501.D08	1	2	1
9	2933-6 F=2	.. \E300-063	.. \2933-601.D09	1	2	1
10	2936-1 F=200	.. \E300-063	.. \2936-101.D10	1	200	1
11	2933-1 F=1.25	.. \E300-063	.. \2933-101.D11	1	1.25	1
12	CCV2W7767-100X	.. \E300-063	.. \W2610Q01.D12	1	1	1
13	MB RW1409	.. \E300-063	.. \W2610K01.D13	1	1	1
14	\$2933-3 MS F=4	.. \E300-063	.. \W2610M01.D14	1	4	1
15	\$2933-3 MSD F=4	.. \E300-063	.. \W2610N01.D15	1	4	1
16	2933-3 F=2	.. \E300-063	.. \2933-301.D16	1	2	1
17	CCV3W7767-100X	.. \E300-063	.. \W2610Q01.D17	1	1	1
18	MB RW1409	.. \E300-063	.. \W2610K11.D18	1	1	1
19	2964-1 F=8	.. \E300-063	.. \2964-101.D19	1	8	1
20	2964-3 F=5	.. \E300-063	.. \2964-301.D20	1	5	1
21	2964-4 F=8	.. \E300-063	.. \2964-401.D21	1	8	1
22	2964-5 F=4	.. \E300-063	.. \2964-501.D22	1	4	1
23	2964-6 F=2	.. \E300-063	.. \2964-601.D23	1	2	1
24	2964-7 F=2	.. \E300-063	.. \2964-701.D24	1	2	1
25	2964-2 F=1.25	.. \E300-063	.. \2964-201.D25	1	1.25	1
26	CCV4W7767-100X	.. \E300-063	.. \W2610Q01.D26	1	1	1
27		.. \STOP.MET		1	1	1

Comment :

LCS/LCSD LOT # W7768

MS/MSD LOT # W7767

ELUENT LOT # W7868

ANALYTICAL METHOD 9056/E300 MATRIX W

Analyst TR

Date 4/29/03

Instrument I

e	Sample	Sample Type	Level	Method	Data File	Volume	Dilution
	##03w2612kw ipc 25ppb w7759	Sample		e314-011.met	c:\data\03w2612kw2612k ipc 25ppb	1	1
	ccv 50ppb w7827e	Sample		e314-011.met	c:\data\03w2612kw2612k q01	1	1
	ccb	Sample		e314-011.met	c:\data\03w2612kw2612k ccb01	1	1
	ics 25ppb w7827d	Sample		e314-011.met	c:\data\03w2612kw2612k i01	1	1
	LCS 18PPB W7685D	Sample		e314-011.met	c:\data\03w2612kw2612k j01	1	1
	ICCS 4ppb w7827b	Sample		e314-011.met	c:\data\03w2612kw2612k iccs 4ppb	1	1
	mb	Sample		e314-011.met	c:\data\03w2612kw2612k k01	1	1
	2866-05 F=1	Sample		e314-011.met	c:\data\03w2612k\2866-05	1	1
	2866-06 f=1	Sample		e314-011.met	c:\data\03w2612k\2866-06	1	1
	2866-07 F=1	Sample		e314-011.met	c:\data\03w2612k\2866-07	1	1
	2933-03 F=1	Sample		e314-011.met	c:\data\03w2612k\2933-03	1	1
	2933-01 f=1	Sample		e314-011.met	c:\data\03w2612k\2933-01	1	1
	ccv 50ppb w7827e	Sample		e314-011.met	c:\data\03w2612kw2612k q02	1	1
	ccb	Sample		e314-011.met	c:\data\03w2612kw2612k k02	1	1
	2933-02 f=1	Sample		e314-011.met	c:\data\03w2612k\2933-02	1	1
	2933-03 ms 50ppb f=1	Sample		e314-011.met	c:\data\03w2612kw2612k m01	1	1
	2933-03 msd 50ppb f=1	Sample		e314-011.met	c:\data\03w2612kw2612k n01	1	1
	2933-04 F=1	Sample		e314-011.met	c:\data\03w2612k\2933-04	1	1
	2933-05 F=1	Sample		e314-011.met	c:\data\03w2612k\2933-05	1	1
	2933-06 F=1	Sample		e314-011.met	c:\data\03w2612k\2933-06	1	1
	2881-01 F=1	Sample		e314-011.met	c:\data\03w2612k\2881-01	1	1
	2881-02 F=1	Sample		e314-011.met	c:\data\03w2612k\2881-02	1	1
	2881-03 F=1	Sample		e314-011.met	c:\data\03w2612k\2881-03	1	1
	ccv 50ppb w7827e	Sample		e314-011.met	c:\data\03w2612kw2612k q03	1	1
	CCB	Sample		e314-011.met	c:\data\03w2612kw2612k k03	1	1
	2881-04 F=1	Sample		e314-011.met	c:\data\03w2612k\2881-04	1	1
	2881-05 F=1	Sample		e314-011.met	c:\data\03w2612k\2881-05	1	1
	2881-06 F=1	Sample		e314-011.met	c:\data\03w2612k\2881-06	1	1
	2866-06 md f=2	Sample		e314-011.met	c:\data\03w2612kw2612k d01	1	2
	2933-04 f=2	Sample		e314-011.met	c:\data\03w2612k\2933-04a	1	2
	ccv 50ppb w7827e	Sample		e314-011.met	c:\data\03w2612kw2612k q04	1	1
	ccb	Sample		e314-011.met	c:\data\03w2612kw2612k k04	1	1
	2964-01 f=1	Sample		e314-011.met	c:\data\03w2612k\2964-01	1	1
	2964-02 f=1	Sample		e314-011.met	c:\data\03w2612k\2964-02	1	1
	2964-03 f=1	Sample		e314-011.met	c:\data\03w2612k\2964-03	1	1
	2964-04 f=1	Sample		e314-011.met	c:\data\03w2612k\2964-04	1	1
	2964-05 f=1	Sample		e314-011.met	c:\data\03w2612k\2964-05	1	1
	ccv 50ppb w7827e	Sample		e314-011.met	c:\data\03w2612kw2612k q05	1	1
	ccv 50ppb w7827e	Sample		e314-011.met	c:\data\03w2612kw2612k q06	1	1
	ccb	Sample		e314-011.met	c:\data\03w2612kw2612k k05	1	1
	2964-01 f=4	Sample		e314-011.met	c:\data\03w2612k\2964-01	1	4
	2964-04 f=4	Sample		e314-011.met	c:\data\03w2612k\2964-04	1	4
	2964-03 f=20	Sample		e314-011.met	c:\data\03w2612k\2964-03	1	20
	ccv 50ppb w7827e	Sample		e314-011.met	c:\data\03w2612kw2612k q07	1	1
		Sample		aastopcl.met		1	1

Analyst Wei Wang
 Date 4/29-30/03
 Instrument IC-K

Line	Sample	Sample Type	Level	Method	Data File	Volume	Dilution
1	Cal blank	Sample		e314-011.met	c:\data\314-01\1\mb_001.dxd	1	1
2	cal standard 2ppb W7827a	Sample		e314-011.met	c:\data\314-01\1\std-2pb_002.dxd	1	1
3	cal standard 4ppb W7827b	Sample		e314-011.met	c:\data\314-01\1\std-4pb_003.dxd	1	1
4	cal standard 10ppb W7827c	Sample		e314-011.met	c:\data\314-01\1\std-10pb_004.dxd	1	1
5	cal standard 25ppb W7827d	Sample		e314-011.met	c:\data\314-01\1\std-25pb_005.dxd	1	1
6	cal standard 50ppb W7827e	Sample		e314-011.met	c:\data\314-01\1\std-50pb_006.dxd	1	1
7	cal standard 75ppb W7827f	Sample		e314-011.met	c:\data\314-01\1\std-75pb_007.dxd	1	1
8	cal standard 100ppb W7827g	Sample		e314-011.met	c:\data\314-01\1\std-100pb_008.dxd	1	1
9	ICV 50 ppb w7828a	Sample		e314-011.met	c:\data\314-01\1\cv-50pb_009.dxd	1	1
0	icb	Sample		e314-011.met	c:\data\314-01\1\icb_010.dxd	1	1
1	anion 100pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\1\mct-100_011.dxd	1	1
2	anion 200pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\1\mct-200_012.dxd	1	1
3	anion 300pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\1\mct-300_013.dxd	1	1
4	anion 400pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\1\mct-400_014.dxd	1	1
5	anion 500pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\1\mct-500_015.dxd	1	1
6	anion 600pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\1\mct-600_016.dxd	1	1
7	anion 800pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\1\mct-800_017.dxd	1	1
8	anion 1000pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\1\mct-1000_018.dxd	1	1
9	anion 400pm each 2pb	Sample		e314-011.met	c:\data\314-01\1\ipc-2pb_019.dxd	1	1
0	anion 400pm each 4pb	Sample		e314-011.met	c:\data\314-01\1\ipc-4pb_020.dxd	1	1
1	anion 400pm each 25pb	Sample		e314-011.met	c:\data\314-01\1\ipc-25pb_021.dxd	1	1
2	ICV 50 ppb	Sample		e314-011.met	c:\data\314-01\1\ccv-50pb	1	1
3	MDL 4pb	Sample		e314-011.met	c:\data\314-01\1\mdl-02_023.dxd	1	1
4	MDL 4pb	Sample		e314-011.met	c:\data\314-01\1\mdl-03_024.dxd	1	1
5	MDL 4pb	Sample		e314-011.met	c:\data\314-01\1\mdl-04	1	1
6	MDL 4pb	Sample		e314-011.met	c:\data\314-01\1\mdl-05	1	1
7	MDL 4pb	Sample		e314-011.met	c:\data\314-01\1\mdl-06	1	1
8	MDL 4pb	Sample		e314-011.met	c:\data\314-01\1\mdl-07	1	1
9	MDL 4pb	Sample		e314-011.met	c:\data\314-01\1\mdl-08	1	1
0	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\1\idap-25pb	1	1
1	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\1\idap-25pb	1	1
2	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\1\idap-25pb	1	1
3	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\1\idap-25pb	1	1
4	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\1\idap-25pb	1	1
5	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\1\idap-25pb	1	1
6	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\1\idap-25pb	1	1
7	MCT anion 800pm each, 25pbCLO4	Sample		e314-011.met	c:\data\314-01\1\ipc-25pb	1	1
8	MCT anion 800pm each, 25pbCLO4	Sample		e314-011.met	c:\data\314-01\1\ipc-25pb	1	1
9	MCT anion 800pm each, 4pbCLO4	Sample		e314-011.met	c:\data\314-01\1\ipc-4pb	1	1
0	MCT anion 800pm each, 4pbCLO4	Sample		e314-011.met	c:\data\314-01\1\ipc-4pb	1	1
1	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\1\mdl-s01	1	5
2	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\1\mdl-s02	1	5
3	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\1\mdl-s03	1	5
4	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\1\mdl-s04	1	5
5	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\1\mdl-s05	1	5
6	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\1\mdl-s06	1	5
7	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\1\mdl-s07	1	5
8	standard 25ppb W7827d	Sample		e314-011.met	c:\data\314-01\1\std-25pb	1	1
9	anion 100pm each,4pb CLO4	Sample		e314-011.met	c:\data\314-01\1\am-100-4pb	1	1
0	anion 200pm each ,4pb CLO4	Sample		e314-011.met	c:\data\314-01\1\am-200-4pb	1	1
1	anion 300pm each ,4pb CLO4	Sample		e314-011.met	c:\data\314-01\1\am-300-4pb	1	1
2	anion 100pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-01\1\am-100-2pb	1	1
3	anion 200pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-01\1\am-200-2pb	1	1
4	anion 300pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-01\1\am-300-2pb	1	1
5	1982-01 B S.C 4450us/cm	Sample		e314-011.met	c:\data\314-01\1\1982-01	1	1
6	1982-01 B S.C 4450us/cm	Sample		e314-011.met	c:\data\314-01\1\1982-01	1	2
7	1982-02 F=10	Sample		e314-011.met	c:\data\314-01\1\1982-02_057.dxd	1	10
8		Sample		aastopcl.met		1	1



Applied Physics & Chemistry Laboratory

13760 Magnolia Ave. Chino CA 91710
Tel. (909) 590-1828 Fax (909) 590-1498

June 17, 2003

GEOFON, Inc.
Attention: Leo Williamson
22632 Golden Spring Dr Ste 270
Diamond Bar CA 91765

Dear Leo Williamson,

This package contains samples in our Service ID 03-3205 and your project : 04-4304.10 JPL GW
Mon-2Q0.3

Enclosed please find:

- (1) Original analytical report.
- (2) Original Chain of Custody.
- (3) One diskette containing EDD deliverable.
- (4) One original Level C Data Package Deliverable.

If anything is missing or you have any questions, please feel free to contact me.

Respectfully submitted,

A handwritten signature in black ink, appearing to read 'R. Kirakozova', is written over the printed name.

Regina Kirakozova
Associate QA/QC Director
Applied P & Ch Laboratory



GEOFON CORPORATION
 22632 GOLDEN SPRINGS DR., SUITE 270
 DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

MW-18 0032

Item	Sample Identifier	Matrix			Time			Preserved			QC Level	T.A.T	LABORATORY SERVICE ID	LABORATORY CONTACT		MAIL REPORT (COMPANY NAME)	
		Date	Date	HCl Name	Time	Time	Time	Lab. Contact	Lab. Fax	Recipient Name				Address			
1	MW-18-5	H ₂ O	5/13/03	810	None	3+1	III	Norm		X	X	X	Kenny Chan	Geofon, INC.	22632 Golden Springs Dr. #270	Diamond Bar, CA 91765	
2	MW-18-4			925		1+1				X	X	X	(909) 590-1828	Leo W. Williamson			
3	MW-18-3			1010						X	X	X	(909) 590-1496				
4	MW-18-2			1050						X	X	X	13760 Magnolia Ave.				
5	MW-18-1			1130						X	X	X	Ching, CA				
6																	
7	EB-13-5/13/03	H ₂ O	5/13/03	1020	HCl Name	3+1	III	Normal		X	X	X	(909) 590-1455				
8	TB-13-5/13/03				HCl Name	2				X							
9	DUPE-7-2203			9/13/03	HCl Name	3+1	IV			X	X	X					
10					HCl Name	1-1				X	X	X					

MINERALS: Na/K/Ca/As/Mg/Fe

ANALYSES: 5247 (NO3), 5248 (Cl), 5249 (NO2+NO3), 5250 (NO3), 5251 (NO3), 5252 (NO3), 5253 (NO3), 5254 (NO3), 5255 (NO3), 5256 (NO3), 5257 (NO3), 5258 (NO3), 5259 (NO3), 5260 (NO3)

3205

COOLER TEMPERATURE UPON RECEIPT

SAMPLE'S CONDITION UPON RECEIPT

COURIER AND AIR BILL NUMBER.

SAMPLES COLLECTED BY: Leo W. Williamson

RELINQUISHED BY: Leo W. Williamson

RECEIVED BY: [Signature]

DATE: 5/13/03

TIME: 1528

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Submitted to:

GEOFON, Inc.

Attention: Leo W. Williamson

22632 Golden Spring Dr Ste 270

Diamond Bar CA 91765

Tel: (909)396-7662 Fax: (909)396-1455

APCL Analytical Report

Service ID #: 801-033205

Received: 05/13/03

Collected by: Leo W. Williamson

Extracted: N/A

Collected on: 05/13/03

Tested: 05/13-20/03

Reported: 05/22/03

Sample Description: Water from MW-18

Project Description: 04-4428.10 JPL GW Mon-2Q03

Analysis of Water Samples

Component Analyzed	Method	Unit	PQL	Analysis Result			
				DUPE-7-2Q03 03-03205-1	EB-13-5/13/03 03-03205-2	MW-18-1 03-03205-3	MW-18-2 03-03205-4
BICARBONATE	SM2320B	mg/L	2	155	<2	133	120
CARBONATE	SM2320B	mg-CaCO ₃ /L	2	<2	<2	<2	<2
PH	9040B	pH unit	0.01	7.93	7.25	7.14	7.75
SOLIDS, TOTAL DISSOLVED (TDS)	160.1	mg/L	10	227	8.0J	263	277
CHROMIUM (VI)	7196	mg/L	0.01	<0.01	<0.01	<0.01	<0.01
Dilution Factor				1	1	1	1
PERCHLORATE	314.0	µg/L	4	23.8	<4	<4	<4
Dilution Factor				2	1.25	2	2
CHLORIDE CL ⁻	300.0	mg/L	0.2	10.8	0.37	11.3	11.2
NITRATE N-NO ₃ ⁻ AS N	300.0	mg/L	0.04	1.3	0.16	1.3	0.86
SULFATE SO ₄ ⁻²	300.0	mg/L	0.5	26.0	0.84	42.9	30.9
Dilution Factor				1	1	1	1
ARSENIC	200.9	µg/L	5	<5	<5	<5	<5
CALCIUM	200.7	µg/L	200	37,700	<200	48,100	53,200
IRON	200.7	µg/L	50	184	31.5J	138	176
MAGNESIUM	200.7	µg/L	100	13,400	85.8J	15,500	17,500
POTASSIUM	200.7	µg/L	400	1,540	172J	2,340	2,460
SODIUM	200.7	µg/L	2000	24,300	1,000J	15,600	19,400
VOLATILE ORGANIC COMPOUNDS							
Dilution Factor				1	1	1	1
BENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOCHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMODICHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOFORM	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2-BUTANONE	524.2	µg/L	10	<10	<10	<10	<10
N-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
SEC-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TERT-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CARBON TETRACHLORIDE	524.2	µg/L	0.5	2.4	<0.5	<0.5	<0.5
CHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLORODIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROFORM	524.2	µg/L	0.5	0.8	<0.5	<0.5	<0.5
CHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5

APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result			
				DUPE-7-2Q03	EB-13-5/13/03	MW-18-1	MW-18-2
				03-03205-1	03-03205-2	03-03205-3	03-03205-4
4-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DIBROMO-3-CHLOROPROPANE	524.2	µg/L	1.1 (a)	<1.1	<1.1	<1.1	<1.1
1,2-DIBROMOETHANE (EDB)	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
DIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,4-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
DICHLORODIFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CIS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TRANS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CIS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TRANS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
ETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
HEXACHLOROBUTADIENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
ISOPROPYLBENZENE (CUMENE)	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
P-ISOPROPYLTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
4-METHYL-2-PENTANONE (MIBK)	524.2	µg/L	10	6J	4J	4J	4J
METHYLENE CHLORIDE	524.2	µg/L	1.8 (a)	<1.8	<1.8	<1.8	<1.8
METHYL-T-BUTYL ETHER (MTBE)	524.2	µg/L	1	<1	<1	<1	<1
NAPHTHALENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
N-PROPYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
STYRENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,1,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TETRACHLOROETHENE	524.2	µg/L	0.5	1.9	<0.5	<0.5	<0.5
TOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,4-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,1-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TRICHLOROETHENE	524.2	µg/L	0.5	0.9	<0.5	<0.5	<0.5
TRICHLOROFUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,4-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3,5-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
VINYL CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
O-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
M/P-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5

APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result			
				MW-18-3 03-03205-5	MW-18-4 03-03205-6	MW-18-5 03-03205-7	TB-13-5/13/03 03-03205-8
BICARBONATE	SM2320B	mg/L	2	210	159	132	-
CARBONATE	SM2320B	mg-CaCO ₃ /L	2	<2	<2	<2	-
PH	9040B	pH unit	0.01	7.78	7.94	8.76	-
SOLIDS, TOTAL DISSOLVED (TDS)	160.1	mg/L	10	325	229	188	-
CHROMIUM (VI)	7196	mg/L	0.01	<0.01	<0.01	<0.01	-
Dilution Factor				1	1	1	1
PERCHLORATE	314.0	µg/L	4	1.3J	23.9	<4	-
Dilution Factor				2	2	2	1
CHLORIDE CL ⁻	300.0	mg/L	0.2	18.4	10.6	9.8	-
NITRATE AS N	300.0	mg/L	0.04	1.1	1.3	0.13	-
SULFATE SO ₄ ⁻²	300.0	mg/L	0.5	40.8	25.3	4.8	-
Dilution Factor				1	1	1	1
ARSENIC	200.9	µg/L	5	<5	<5	<5	-
CALCIUM	200.7	µg/L	200	71,600	41,600	8,960	-
IRON	200.7	µg/L	50	58.0	169	206	-
MAGNESIUM	200.7	µg/L	100	20,400	13,800	4,660	-
POTASSIUM	200.7	µg/L	400	3,050	1,960	1,830	-
SODIUM	200.7	µg/L	2000	23,600	28,800	52,800	-
VOLATILE ORGANIC COMPOUNDS							
Dilution Factor				1	1	1	1
BENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOCHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMODICHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOFORM	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2-BUTANONE	524.2	µg/L	10	<10	<10	<10	<10
N-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
SEC-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TERT-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CARBON TETRACHLORIDE	524.2	µg/L	0.5	<0.5	2.4	<0.5	<0.5
CHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLORODIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROFORM	524.2	µg/L	0.5	1.2	0.9	<0.5	<0.5
CHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
4-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DIBROMO-3-CHLOROPROPANE	524.2	µg/L	1.1 (a)	<1.1	<1.1	<1.1	<1.1
1,2-DIBROMOETHANE (EDB)	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
DIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,4-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
DICHLORODIFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5

APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result			
				MW-18-3 03-03205-5	MW-18-4 03-03205-6	MW-18-5 03-03205-7	TB-13-5/13/03 03-03205-8
1,1-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CIS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TRANS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CIS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TRANS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
ETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
HEXACHLOROBUTADIENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
ISOPROPYLBENZENE (CUMENE)	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
P-ISOPROPYLTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
4-METHYL-2-PENTANONE (MIBK)	524.2	µg/L	10	4J	7J	5J	6J
METHYLENE CHLORIDE	524.2	µg/L	1.8 ^(a)	<1.8	<1.8	<1.8	3.9
METHYL-T-BUTYL ETHER (MTBE)	524.2	µg/L	1	<1	<1	<1	<1
NAPHTHALENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
N-PROPYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
STYRENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,1,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TETRACHLOROETHENE	524.2	µg/L	0.5	<0.5	2.1	<0.5	<0.5
TOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,4-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,1-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TRICHLOROETHENE	524.2	µg/L	0.5	0.4J	1.0	<0.5	<0.5
TRICHLOROFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2,2,2-TRICHLORO-1,1,1,2,2,2-TRIFLUOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,4-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3,5-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
VINYL CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
O-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
M/P-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5

PQL: Practical Quantitation Limit. MDL: Method Detection Limit. CRDL: Contract Required Detection Limit

N.D.: Not Detected or less than the practical quantitation limit.


"-": Analysis is not required.

J: Reported between PQL and MDL.

Listed Dilution Factors (DF) are relative to the method default DF. All unlisted DFs are 1.0

(^a) MDL reported.

Respectfully submitted,

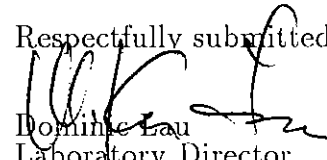
 Dominic Lau
 Laboratory Director
 Applied P & Ch Laboratory

Level C Data Package Deliverables

General Information

Project: 04-4428.10 JPL GW Mon-2Q03

APCL Service ID: 03-3205



Applied Earth Sciences Laboratory

13760 Magnolia Ave. Chino, CA 91710

Telephone (909)590-1828

Fax (909)590-1498

Case Narrative

Project: JPL GW Mon-2Q03/MW-18/04-4428.10

For GEOFON, Inc.

APCL Service No: 03-3205

1. Sample Identification

The sample identifications are listed in the following table:

GEOFON, Inc. Sample ID	APCL Sample ID
MW-18-5	03-03205-7
MW-18-4	03-03205-6
MW-18-3	03-03205-5
MW-18-2	03-03205-4
MW-18-1	03-03205-3
EB-13-5/13/03	03-03205-2
TB-13-5/13/03	03-03205-8
DUPE-7-2Q03	03-03205-1

2. Analytical Methodology

Samples are analyzed by EPA methods

- 524.2 (Volatile Organic Compounds),
- 7196A (Chromium (VI)),
- 314.0 (Perchlorate, low level),
- 300.0 (Anions by IC),
- SM2320B (Bicarbonate),
- SM2320B (Carbonate),
- 9040B (pH),
- 160.1 (Solids, Total Dissolved (TDS)),
- 200.7 (Metals by ICP),
- 200.9 (Arsenic, As, by GFAA),

3. Holding Time

All samples were extracted, digested and analyzed within the holding times defined by the appropriate EPA methods of the analyses.

4. Preservation

All samples were preserved and stored according to the appropriate EPA methods.

5. Tele-log


None

6. Anomaly

None

"I certify that these data are technically accurate, complete, and in compliance with the terms and conditions of the contract, for other than the conditions detailed above. Release of the data contained in the hardcopy data package and its electronic data deliverable submitted on diskette had been authorized by the Laboratory Manager or her/his designee, as verified by the following signature."

Respectfully submitted,



Regina Kirakozova
Associate QA/QC Director
Applied P & Ch Laboratory

Sample Receiving Checklist

APCL ServiceID: **3205** Client Name/Project: Geolon

1. Sample Arrival

Date/Time Received 5/13/03 1528 Date/Time Opened 5/13/03 1600 By (name): Kenny Chan
Custody Transfer: Client Golden State UPS US Mail FedEx APCL Empl: Kenny Chan

2. Chain-of-Custody (CoC)

With Samples? Faxed? Client has Copy? Signed, dated? By: _____
 Project ID? Analyses Clear? Hold Samples? # on Hold _____ # Received 8
 CoC/Docs Zip-Locked under lid? Compos. #: _____ #Samples OK?
 Discrepancies? Client notified? Response (attach docs): _____

3. Shipping-Container/Cooler

Cooler Used? # of 1 Cooled by: Ice Blue Ice Dry Ice None
Temp °C 30
(Cooler temperature measured from temp blank if present, otherwise measured from the cooler).
Cooler Custody Seal? Absent Intact Tampered?

4. Sample Preservation

pH <2 pH >12
If Not, pH = _____ Preserved by: Client APCL Third Party _____

5. Holding-time Requirements

pH 24hr BACT 6/24hr Cr^{VI} 24hr NO₃⁻ 48hr BOD 48hr
 Cl₂ ASAP Turbidity 48hr DO ASAP Fe(II) ASAP
 HT Expired? Client notified?

6. Sample Container Condition

Intact? Broken? Documented? Number: _____
Type: plastic glass Tube: brass/SS Tedlar Bag
 Quantity OK? Leaking? Anomaly?
 Caps tight? Air Bubbles? Anomaly?
Labels: Unique ID? Date/Time Preserved?

7. Turn Around Time

RUSH TAT: _____ Std (7-10 days) Not Marked

8. Sample Matrix

Drinking H₂O Other Liq Soil Wipe Polymer Air Other: _____
 Ground H₂O Sludge Filter Oil/Petro Paint W. Water Extract Unknown

9. Pre-Login Check List Completed & OK?

ALL OK? (if not, attach docs) Client Contact? (Name: _____) Date/Time: _____
Received/Checked by: Kenny Chan Date: 13 May 2003 Time: 7:46 a.m.

*HT: Samples must be analyzed for results to reflect total concentrations. Results generated outside required of holding times are considered minimal values and may be used to define waste as hazardous but not as non-hazardous.

Sample Login: Check List

03-03205 (0470_ 147) (2202777_ 147)

05/13/03

Part 1: General Information

-
- | | | |
|---|----------------------|--|
| <input type="checkbox"/> Company Information | Name: | <i>GEOFON, Inc.</i> |
| | Address: | <i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i> |
| <input type="checkbox"/> Project Information | Project Description: | <i>JPL</i> |
| | Project #: | <i>04-4428.10</i> |
| <input type="checkbox"/> Billing Information | P.O. #: | |
| | Bill Address: | <i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i> |
| | Lab Project ID: | |
| | Client Database #: | <i>3</i> |
| <input type="checkbox"/> Receiving Information | Who Received Sample? | <i>Kenny Chan</i> |
| | Receiving Date/Time: | <i>05/19/03 1528</i> |
| | COC No. | |
| <input type="checkbox"/> Shipping Information | Shipping Company | <i>APCL pick up</i> |
| | Packing Information: | <i>Cooler/Ice Chester</i> |
| | Cooler Temperature: | <i>3.0 °C</i> |
| <input type="checkbox"/> Container Information | Container Provider: | <i>Client</i> |
| <input type="checkbox"/> Sampling Information | Sampling Person: | |
| | Sampling Company: | <i>Client</i> |
| <input type="checkbox"/> Turn-Around-Time Option: | | <i>Rush 5 working day(s)</i> |
| <input type="checkbox"/> QC Option: | | <i>NEESA C</i> |
| <input type="checkbox"/> Disposal Option: | | <i>Not specify</i> |
-

Part 2: Sample Information

Seq. #	Sample ID (on COC)	Sample Sub-ID	APCL Sample ID	Matrix	Cont. tainer	Preser- vative	Vol, ml Am. g	# of Replica	Condition G, L, B	Collected mmddyy	Hold ?	Compositè Group	TAT Days
1	MW-18-5	VOC	03-03205-7- α	W	V	C	40	3	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-5	Metal	03-03205-7- β	W	P	N	500	1	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-5	300	03-03205-7- γ	W	P		1000	1	G	051303	N	0	7 <input type="checkbox"/>
2	MW-18-4	VOC	03-03205-6- α	W	V	C	40	3	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-4	Metal	03-03205-6- β	W	P	N	500	1	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-4	300	03-03205-6- γ	W	P		1000	1	G	051303	N	0	7 <input type="checkbox"/>
3	MW-18-3	VOC	03-03205-5- α	W	V	C	40	3	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-3	Metal	03-03205-5- β	W	P	N	500	1	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-3	300	03-03205-5- γ	W	P		1000	1	G	051303	N	0	7 <input type="checkbox"/>
4	MW-18-2	VOC	03-03205-4- α	W	V	C	40	3	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-2	Metal	03-03205-4- β	W	P	N	500	1	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-2	300	03-03205-4- γ	W	P		1000	1	G	051303	N	0	7 <input type="checkbox"/>
5	MW-18-1	VOC	03-03205-3- α	W	V	C	40	3	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-1	Metal	03-03205-3- β	W	P	N	500	1	G	051303	N	0	7 <input type="checkbox"/>
	MW-18-1	300	03-03205-3- γ	W	P		1000	1	G	051303	N	0	7 <input type="checkbox"/>
6	EB-13-5/13/03	VOC	03-03205-2- α	W	V	C	40	3	G	051303	N	0	7 <input type="checkbox"/>
	EB-13-5/13/03	Metal	03-03205-2- β	W	P	N	500	1	G	051303	N	0	7 <input type="checkbox"/>
	EB-13-5/13/03	300	03-03205-2- γ	W	P		1000	1	G	051303	N	0	7 <input type="checkbox"/>
7	TB-13-5/13/03	VOC	03-03205-8	W	V	C	40	2	G	051303	N	0	7 <input type="checkbox"/>
8	DUPE-7-2Q03	VOC	03-03205-1- α	W	V	C	40	3	G	051303	N	0	7 <input type="checkbox"/>
	DUPE-7-2Q03	Metal	03-03205-1- β	W	P	N	500	1	G	051303	N	0	7 <input type="checkbox"/>
	DUPE-7-2Q03	300	03-03205-1- γ	W	P		1000	1	G	051303	N	0	7 <input type="checkbox"/>

Part 3: Analysis Information

- Test Items:
- 524.2 Volatile Organic Compounds
 - 7196A Chromium (VI)
 - 314.0/300.0 Perchlorate, low level
 - 300.0 Chloride Cl^- by IC
 - 300.0 Sulfate (SO_4^{--}), by IC
 - 300.0/SM4500NO3 Nitrate (NO_3^-) as N by IC
 - SM2320B Carbonate
 - SM2320B Bicarbonate
 - 9040B/150.1 pH
 - 160.1 Solids, Total Dissolved (TDS)
 - 200.7/6010B Sodium, Na, by ICP
 - 200.7/6010B Calcium, Ca, by ICP

Level C Data Package Deliverables

Volatile Organics



Applied P & Ch Laboratory

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/19/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: 03G2534-MB-01	Lab Sample ID: 03G2534-MB-01	Received Date: 05/19/2003
Sample Type: Method Blank	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/19/03	Anal. Date: 05/19/03
Data File Name: G2534K01	Prep. No: -	Anal. Time: 20:12
Methanol Vol. -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8	4.7	
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TETRACHLOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	4-BROMO-FLUOROBENZENE (BFB)	460-00-4		70-129	107	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	98	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	104	
4	TOLUENE-D8	2037-26-5		73-129	107	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	85	
2	1,4-DICHLOROETHANE-D4	3855-82-1		50-200	89	
3	FLUOROBENZENE	462-06-6		50-200	93	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Data Filename: C:\HPCHEM\1\DATA\03G2534\G2534K01.D
 Method : C:\HPCHEM\1\METHODS\E524G004.M
 Acq. Time : May 19 20:12 2003
 Method Update: Fri May 16 12:11 2003
 Quant. Time : May 20 09:45 2003
 Print Time : Tue May 20 09:45 2003
 Miscellaneous :
 Sample : F=1
 Inst. : GCMS-G
 RF via : Multiple Level Calibration
 Operator: Eddie
 Multiplr: 1.000000

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
Internal Standards											
1	1 Fluorobenzene I1	9.50	9.52	-0.002	96	70	648.041	10.00		-0.02	
47	47 Cl-benzene-d5, I2	13.11	13.12	-0.001	82	119	183.940	10.00		-0.02	
62	62 1,4-DCB-d4 150 15	15.62	15.63	0.000	152	150	165.027	10.00		-0.01	

System Monitoring Compounds (Surrogate)											
27	27 Di-Br-F-Methane (7.96	7.97	0.000	111	113	499.235	20.75		20.7	103.74%
29	29 1,2-di-Cl-ethane-	8.54	8.54	0.000	65	102	213.264	19.50		19.5	97.50%
55	55 toluene-d8(S2)	11.59	11.61	-0.001	100	99	695.105	21.29		21.3	106.46%
70	70 4-Br-1-F-Bz (S3)	14.34	14.36	0.000	174	95	291.442	21.43		21.4	107.15%

Target Compounds												
<<< I1	: ISTD ID = 1	>>>										Qvalue
111	111 isopropyl alcoho	4.77	4.76	0.002	45	43	2.823	10.88		10.9	38	
102	102 Acrolein x10	4.45	4.67	-0.023	56	55	0.246	4.52		4.5	9	
101	101 Acetonitrilex10	4.72	4.71	0.000	41	40	1.218	12.37		12.4	82	
113	113 Tert butyl alcoh	5.39	5.38	0.000	59	57	0.738	1.24		1.2	24	
18	18 methylene chlorid	5.51	5.50	0.000	84	49	73.920	4.65		4.7	97	
98	98 Vinyl acetate x5	6.95	6.97	-0.002	43	86	0.918	12.56		12.6	69	
201	201 Ethyl acetate x2	7.85	7.83	0.002	43	61	1.903	4.54		4.5	52	
117	117 Iso-butyl alcoho	7.85	7.83	0.002	43	42	2.159	14.94		14.9	59	
26	26 tetrahydrofuranx5	8.23	8.23	0.000	72	42	0.268	0.39		0.4	36	
107	107 Et methacrylate	11.60	11.80	-0.021	69	99	1.309	1.73		1.7	1	
93	93 2-Hexanone x5	12.01	11.93	0.008	43	58	0.573	5.77		5.8	95	
48	48 112-tri-Cl-Et	11.61	11.49	0.012	97	83	21.204	2.80		2.8	8	
<<< I2	: ISTD ID = 47	>>>										
54	54 MIBK	11.02	10.99	0.002	43	58	4.098	0.63		0.6	72	
49	49 1,3-di-cl-propane	11.61	11.75	-0.011	76	78	8.271	0.63		0.6	68	


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Quantitation Report


Data File : C:\HPCHEM\1\DATA\03G2534\G2534K01.D
Acq On : 19 May 03 8:12 pm
Sample : f=1
Misc :
Quant Time: May 20 9:45 2003

Vial: 12
Operator: Eddie
Inst : GCMS-G
Multiplier: 1.00
Quant Results File: quant.res

Method : C:\HPCHEM\1\METHODS\E524G004.M
Title : **Applied P & Ch Lab** EPA 524.2
Last Update : Fri May 16 12:11:07 2003
Response via : Multiple Level Calibration

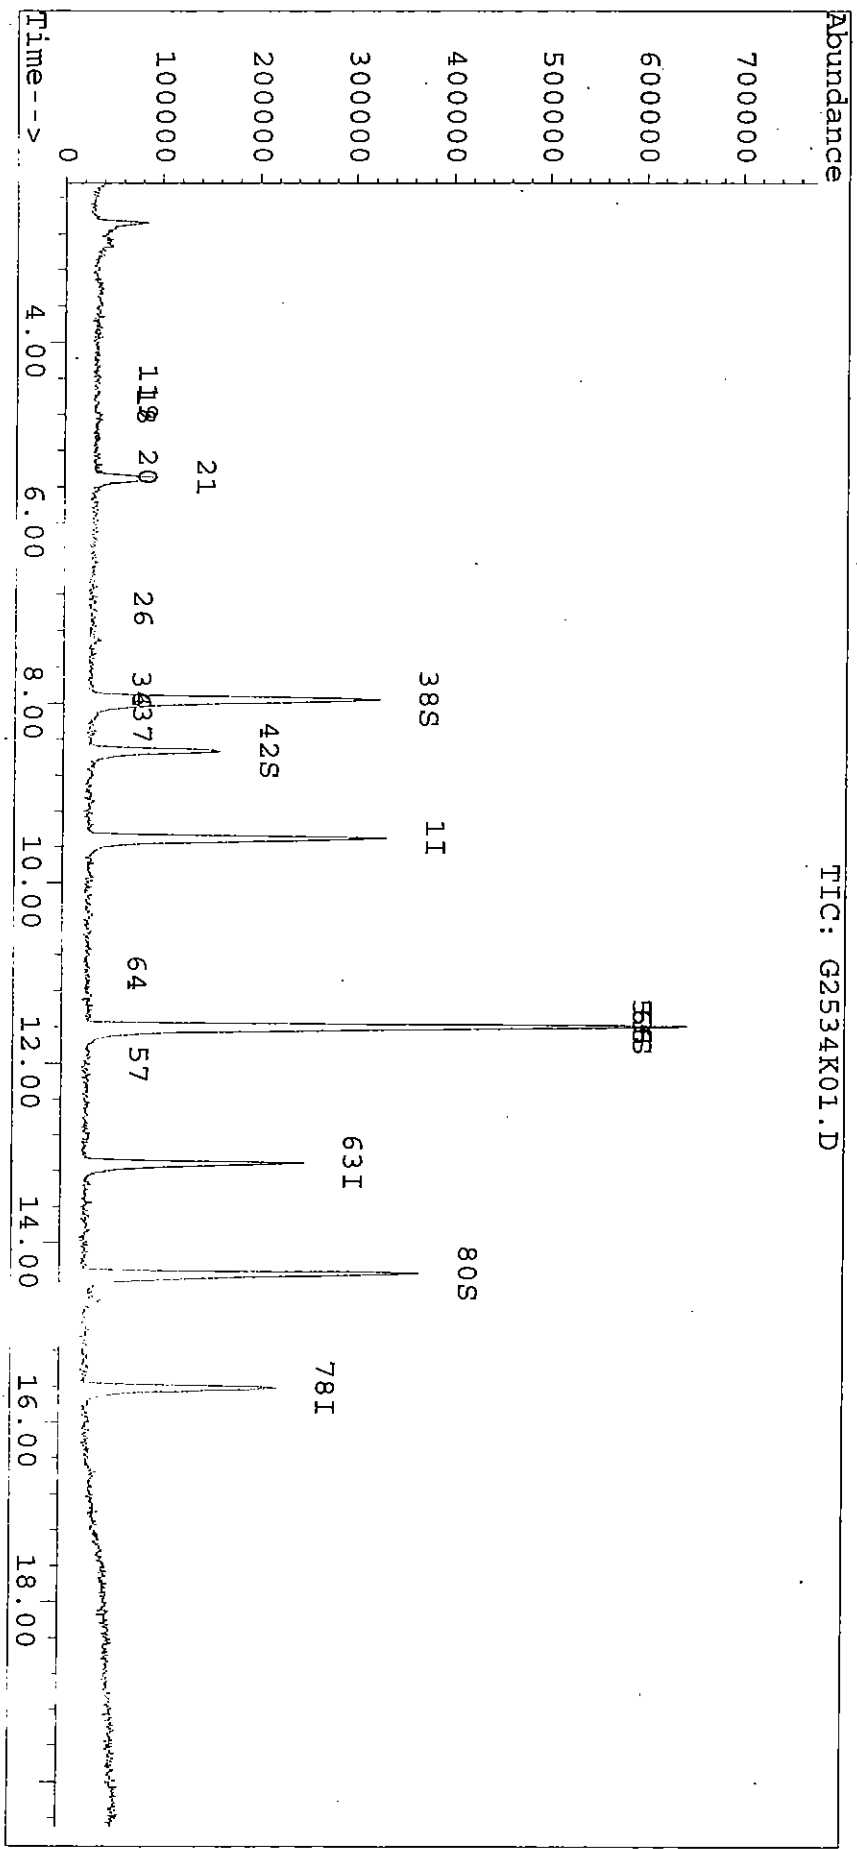


AbundanceScan 261 (4.297 min): G2317Q01.D (

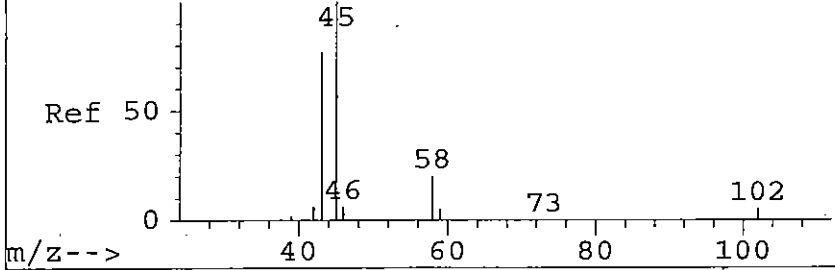


#9
 111 isopropyl alcohol x10
 Concen: 10.88 ppb
 RT: 4.77 min Scan# 321
 Delta R.T. 0.02 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Ratio	Lower	Upper
45	100		
43	31.5	77.0	115.5#
39	0.0	13.3	19.9#
0	0.0	0.0	0.0


AbundanceScan 321 (4.771 min): G2534K01.D (

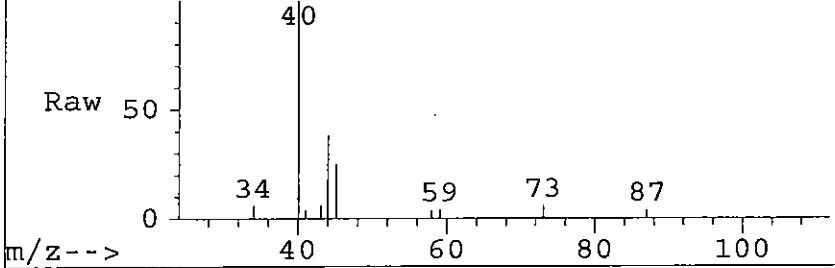


Abundance	Ion	Label
6000	45.00	(44.
	43.00	(42.
	39.00	(38.

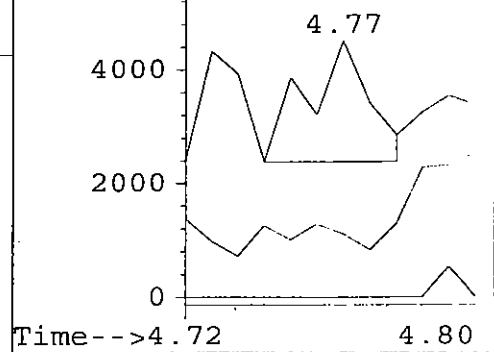

AbundanceScan 321 (4.771 min): G2534K01.D (

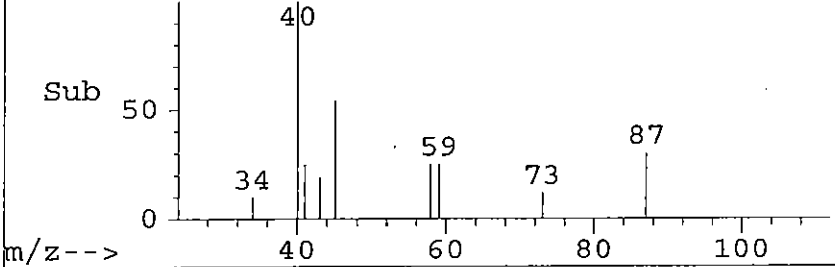


AbundanceScan 249 (4.202 min): G2317Q01.D (

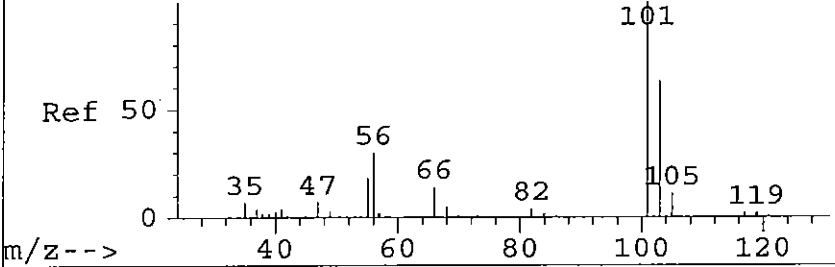


#11
 102 Acrolein x10
 Concen: 4.52 ppb
 RT: 4.45 min Scan# 280
 Delta R.T. -0.22 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Ratio	Lower	Upper
56	100		
55	126.4	29.2	87.5#
0	0.0	0.0	0.0
0	0.0	0.0	0.0


AbundanceScan 280 (4.447 min): G2534K01.D (

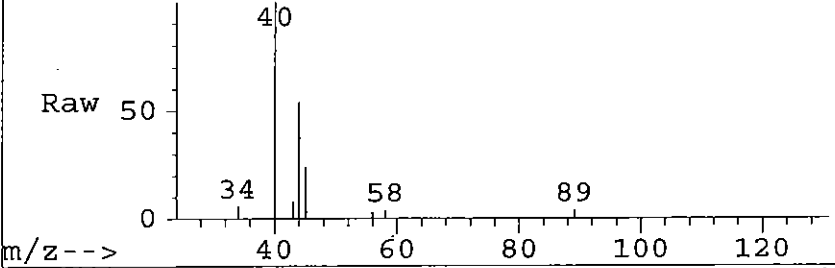


Abundance	Ion	Label
600	56.00	(55.
	55.00	(54.

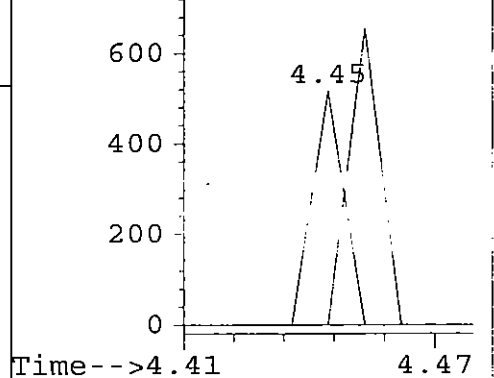


AbundanceScan 280 (4.447 min): G2534K01.D (

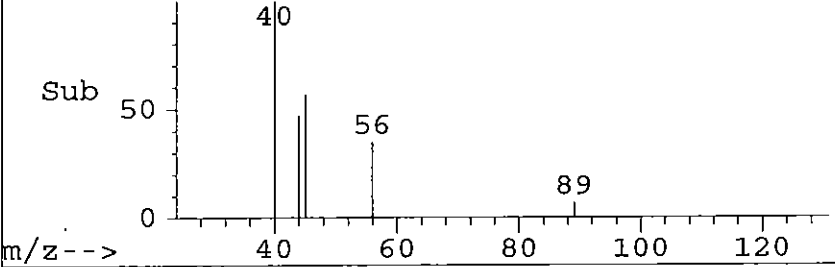



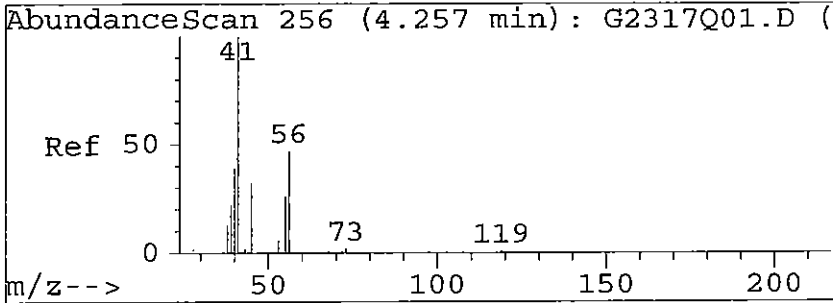


#18
 101 Acetonitrilex10
 Concen: 12.37 ppb
 RT: 4.72 min Scan# 314
 Delta R.T. 0.00 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Resp	Lower	Upper
41	1218		
41	100		
40	212.0	151.7	227.5
39	0.0	17.3	25.9#
0	0.0	0.0	0.0

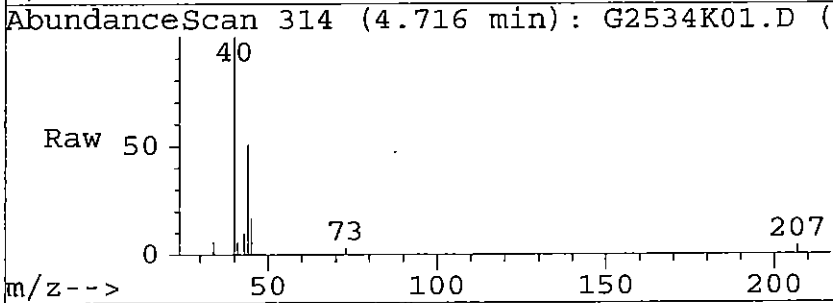


Abundance	Ion	Ion	Ion
41.00	(40.		
40.00	(39.		
39.00	(38.		

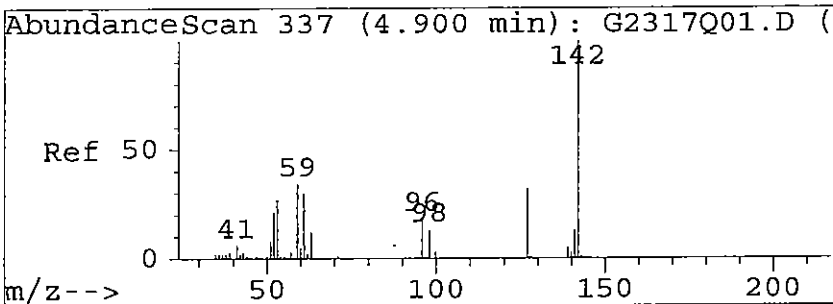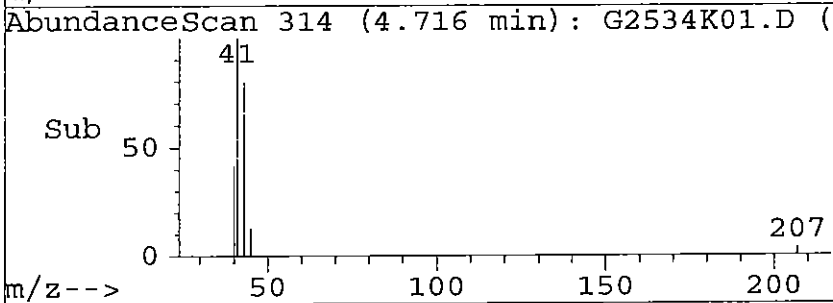
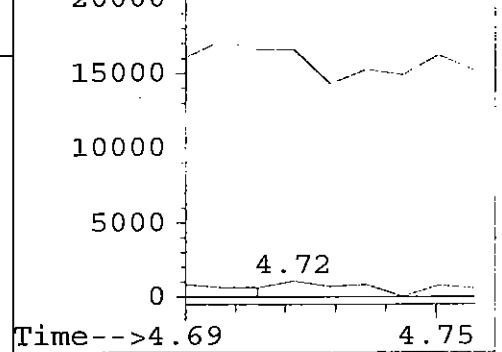



#20
 113 Tert butyl alcohol x10
 Concen: 1.24 ppb
 RT: 5.39 min Scan# 399
 Delta R.T. 0.01 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Resp	Lower	Upper
59	738		
59	100		
57	33.6	5.8	8.7#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

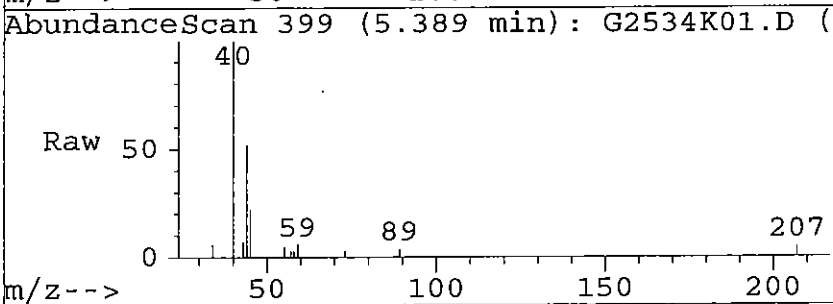


Abundance	Ion	Ion
59.00	(58.	
57.00	(56.	
5.39		


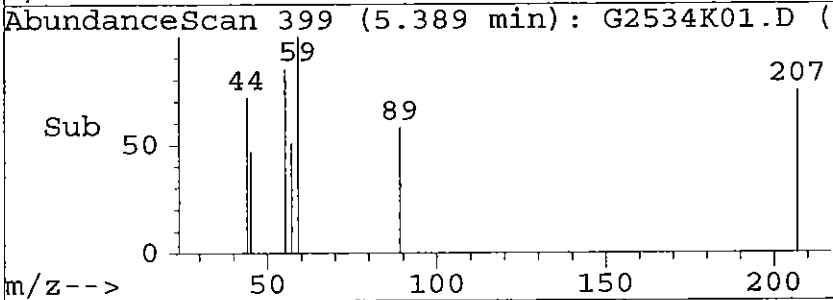
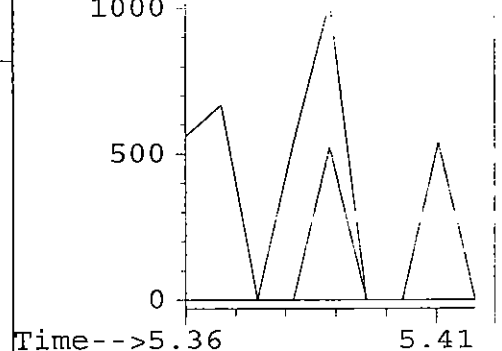


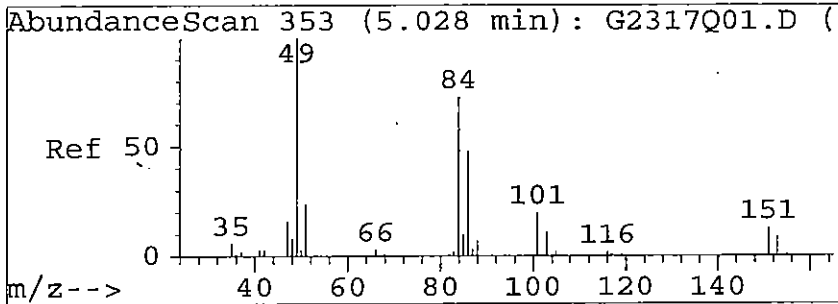


#21
 18 methylene chloride 49 84
 Concen: 4.65 ppb
 RT: 5.51 min Scan# 414
 Delta R.T. 0.00 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

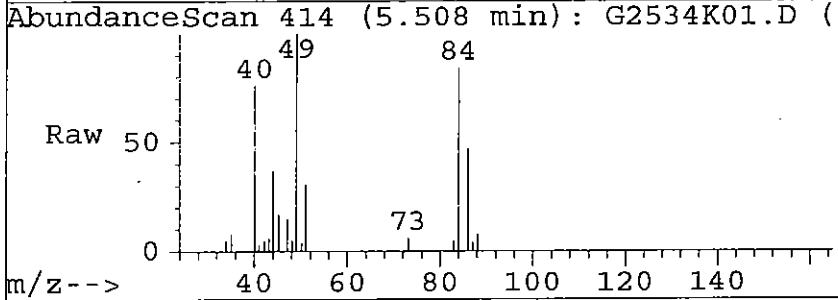



Tgt Ion	Resp	Lower	Upper
84	73920		
49	121.9	62.9	188.5
0	0.0	0.0	0.0
0	0.0	0.0	0.0

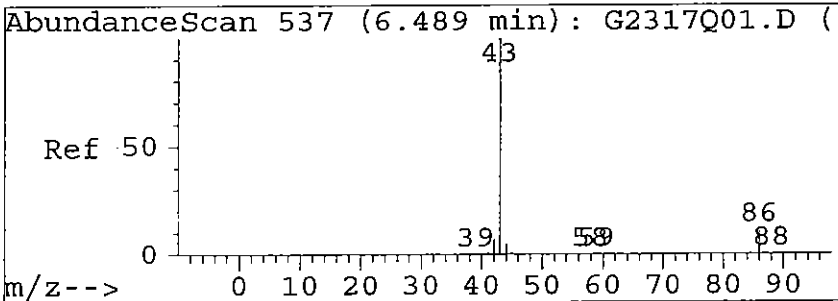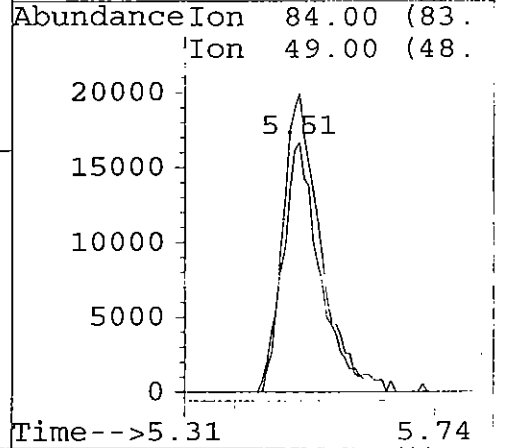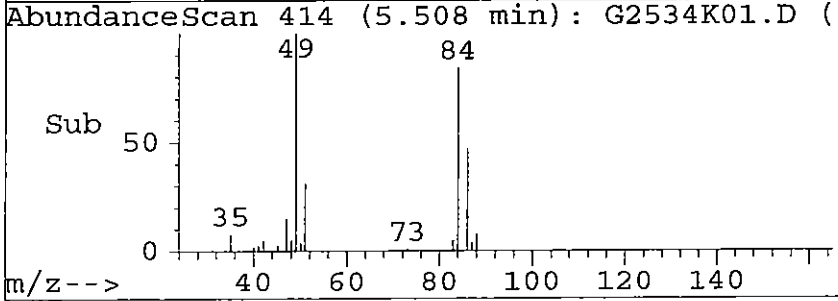


#26
 98 Vinyl acetate x5
 Concen: 12.56 ppb
 RT: 6.95 min Scan# 596
 Delta R.T. -0.02 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

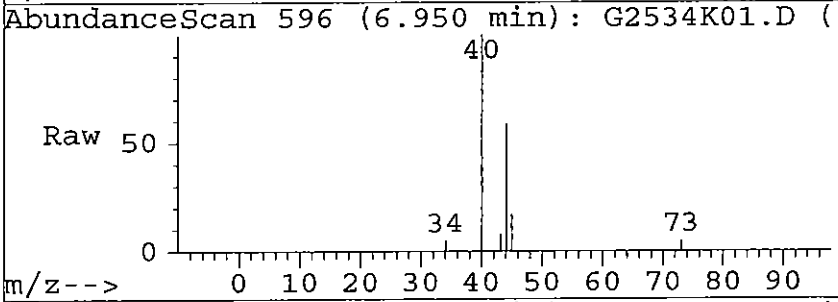





Tgt Ion	Resp	Lower	Upper
43	918		
86	0.0	9.5	14.2#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

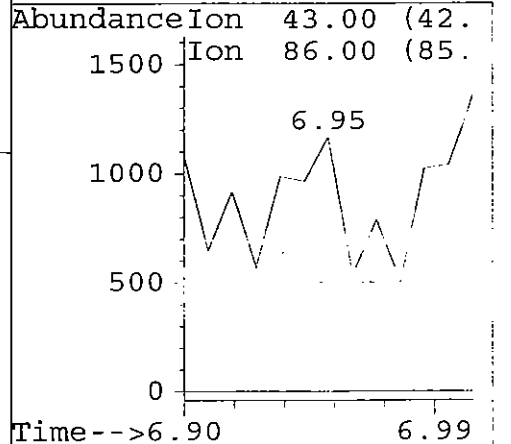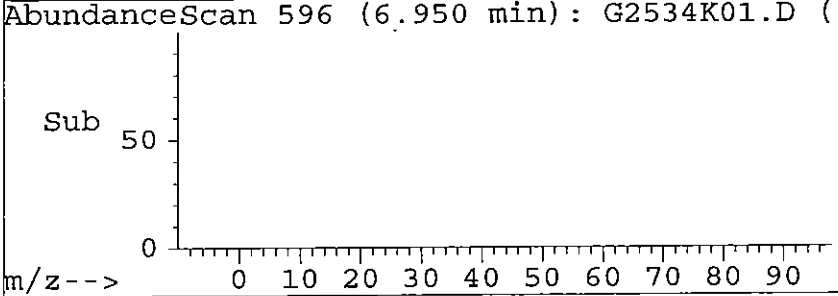

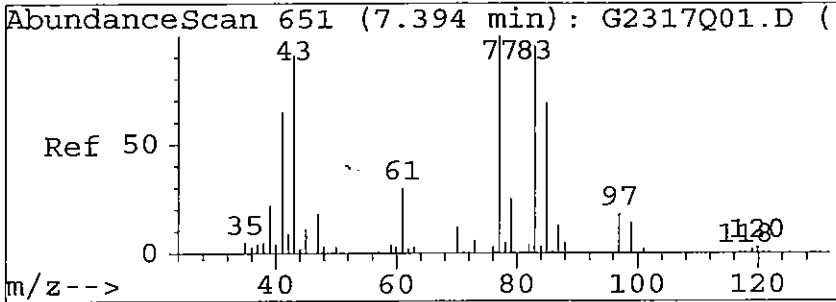




#34
 201 Ethyl acetate x2
 Concen: 4.54 ppb
 RT: 7.85 min Scan# 709
 Delta R.T. 0.01 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Resp	Lower	Upper
43	1903		
61	0.0	19.1	28.6#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

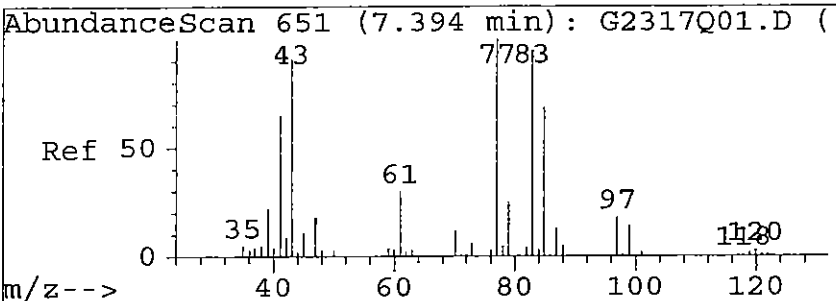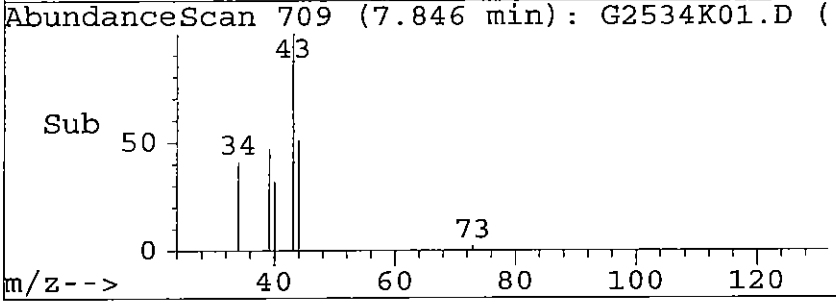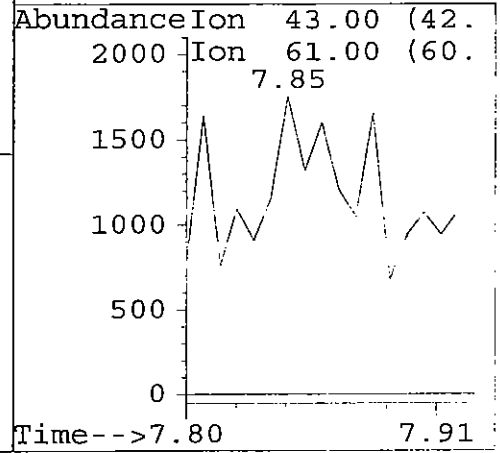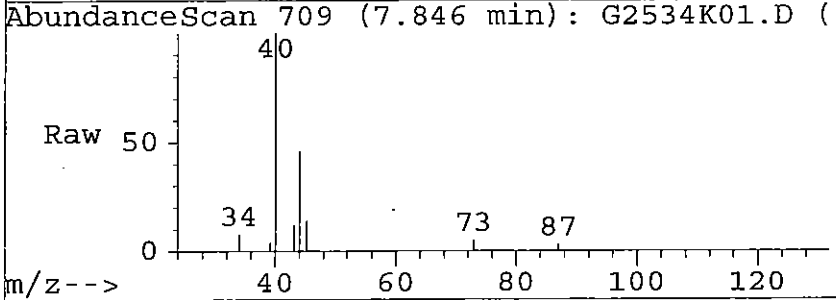


#36
 117 Iso-butyl alcohol X10
 Concen: 14.94 ppb
 RT: 7.85 min Scan# 709
 Delta R.T. 0.01 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Resp	Lower	Upper
43	2159		
42	12.0	7.3	10.9#
41	17.1	39.7	59.5#
0	0.0	0.0	0.0

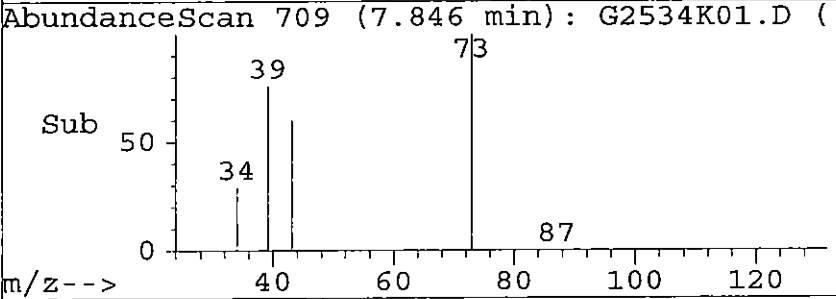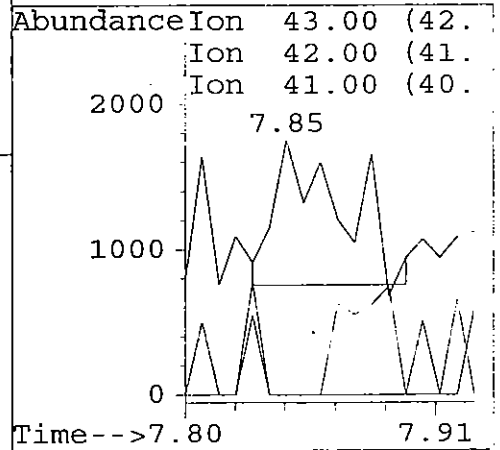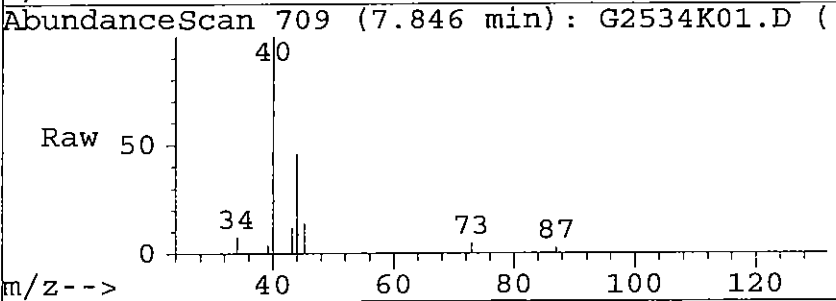

AbundanceScan 702 (7.799 min): G2317Q01.D (


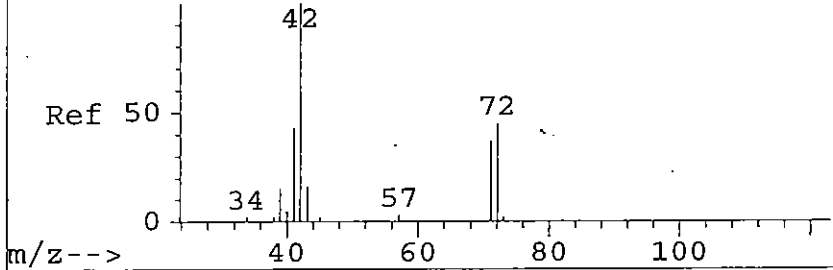


#37


26 tetrahydrofuranx5
 Concen: 0.39 ppb
 RT: 8.23 min Scan# 758
 Delta R.T. 0.01 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Resp	Lower	Upper
72	100		
42	101.9	99.5	298.3
0	0.0	0.0	0.0
0	0.0	0.0	0.0


AbundanceScan 758 (8.234 min): G2534K01.D (

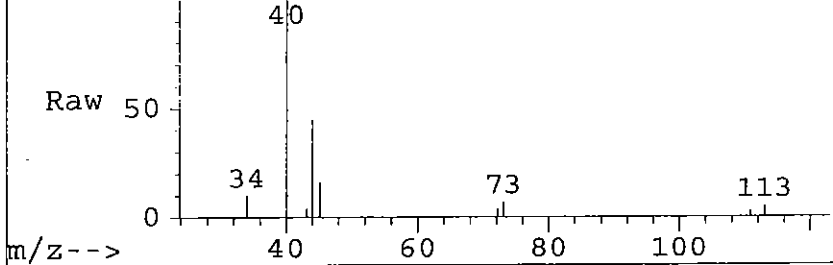

AbundanceScan 758 (8.234 min): G2534K01.D (

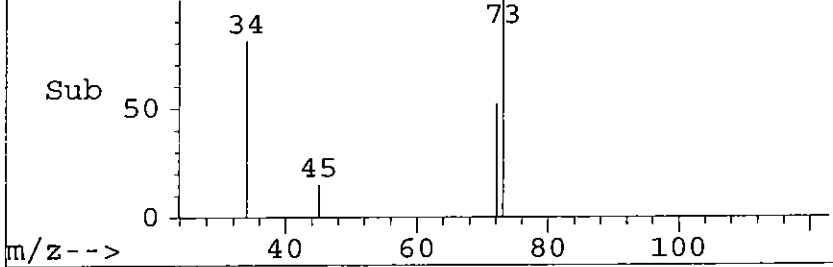

AbundanceScan 1162 (11.452 min): G2317Q01.D


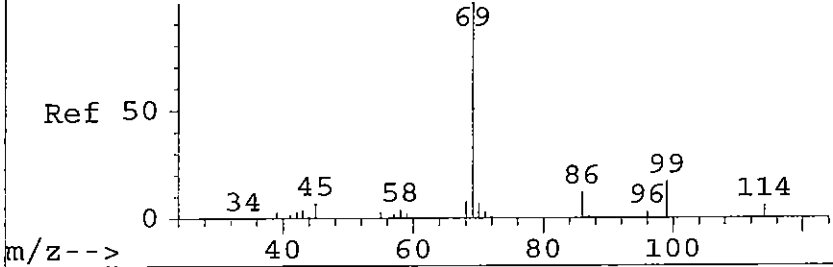


#56


107 Et methacrylate
 Concen: 1.73 ppb
 RT: 11.60 min Scan# 1183
 Delta R.T. -0.20 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Resp	Lower	Upper
69	100		
99	7171.3	9.4	28.0#
0	0.0	0.0	0.0
0	0.0	0.0	0.0


AbundanceScan 1183 (11.602 min): G2534K01.D

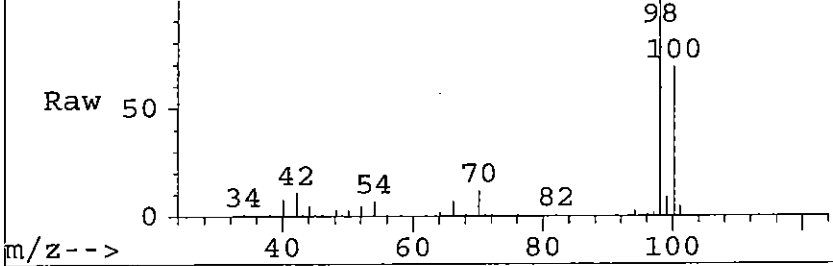

AbundanceScan 1183 (11.602 min): G2534K01.D

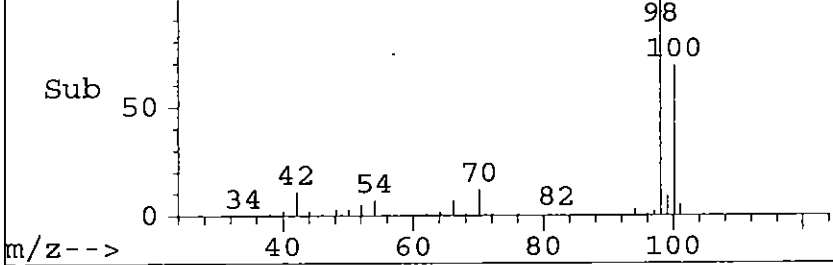


AbundanceScan 1178 (11.579 min): G2317Q01.D

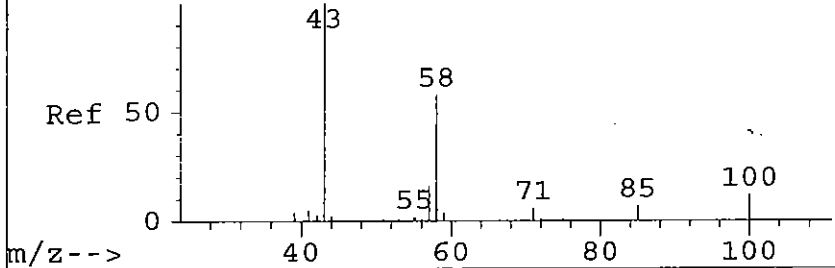


#57
 93 2-Hexanone x5
 Concen: 5.77 ppb
 RT: 12.01 min Scan# 1234
 Delta R.T. 0.08 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	43	58	0	0	Resp:	573	Lower	Upper
Ion Ratio	100	51.8	0.0	0.0				
		44.5	0.0	0.0				
		66.8	0.0	0.0				


AbundanceScan 1234 (12.006 min): G2534K01.D

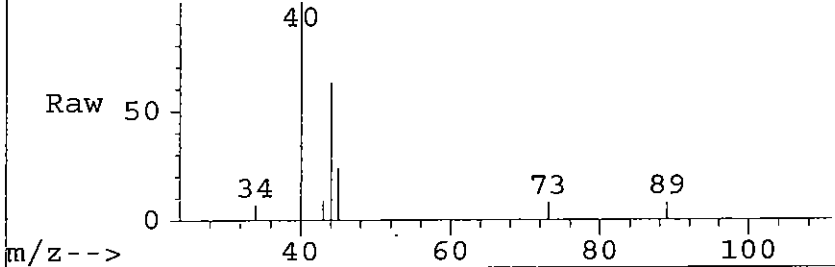


Abundance Ion 43.00 (42.
 Ion 58.00 (57.

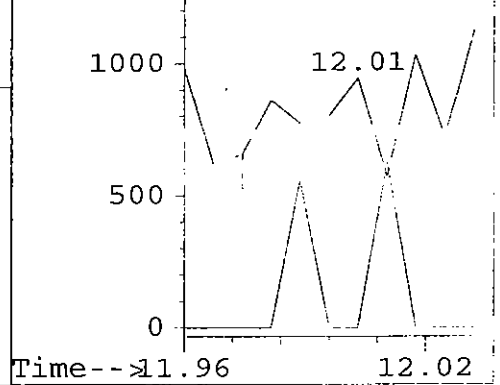

AbundanceScan 1234 (12.006 min): G2534K01.D

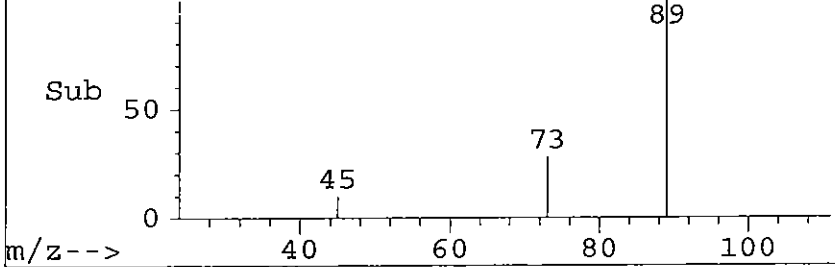


AbundanceScan 1121 (11.126 min): G2317Q01.D

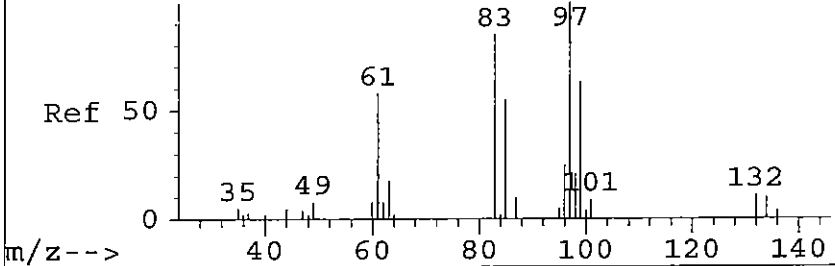


#58
 48 112-tri-Cl-Et 97 83
 Concen: 2.80 ppb
 RT: 11.61 min Scan# 1184
 Delta R.T. 0.12 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	97	83	0	0	Resp:	21204	Lower	Upper
Ion Ratio	100	0.0	0.0	0.0				
		41.5	0.0	0.0				
		124.4#	0.0	0.0				


AbundanceScan 1184 (11.610 min): G2534K01.D

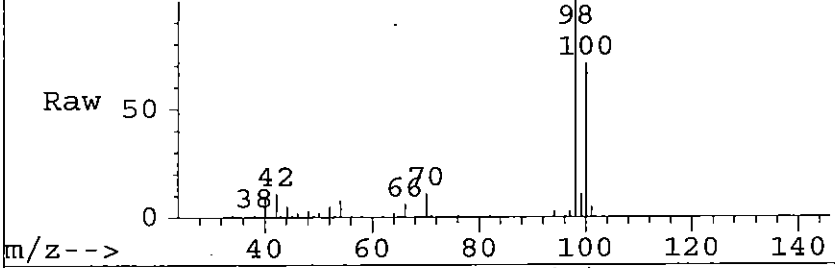


Abundance Ion 97.00 (96.
 8000 Ion 83.00 (82.
 11.61

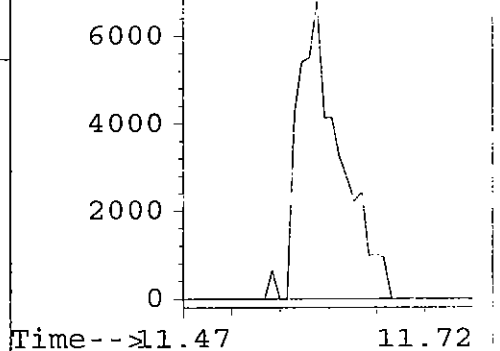


AbundanceScan 1184 (11.610 min): G2534K01.D

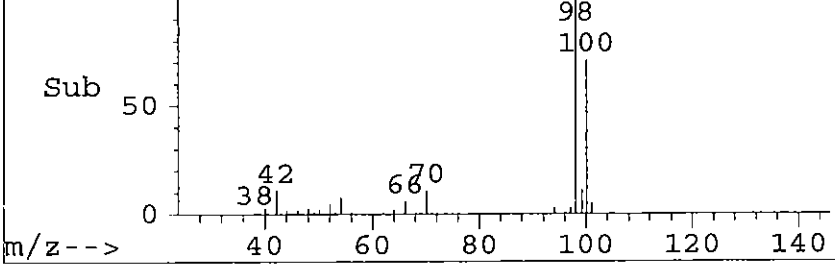


AbundanceScan 1056 (10.610 min): G2317Q01.D

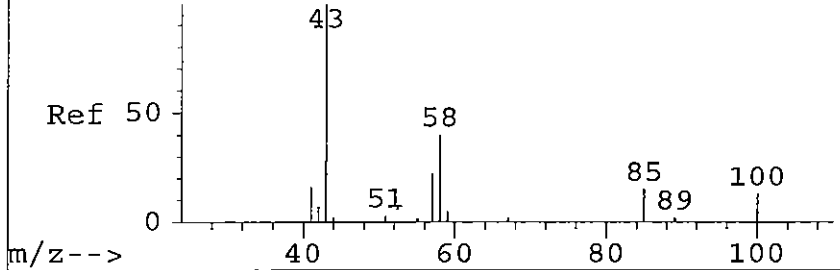

AbundanceScan 1109 (11.015 min): G2534K01.D

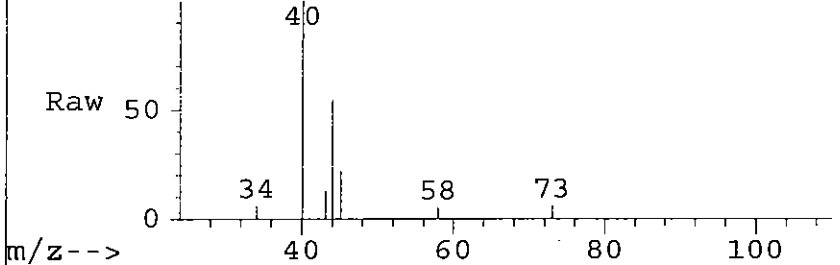


AbundanceScan 1109 (11.015 min): G2534K01.D

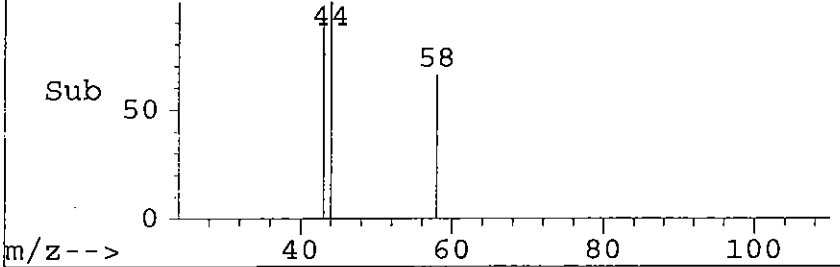


#64
 54 MIBK
 Concen: 0.63 ppb
 RT: 11.02 min Scan# 1109
 Delta R.T. 0.02 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm


Tgt Ion	Resp	Lower	Upper
43	4098		
58	20.5	17.5	57.5
0	0.0	0.0	0.0
0	0.0	0.0	0.0

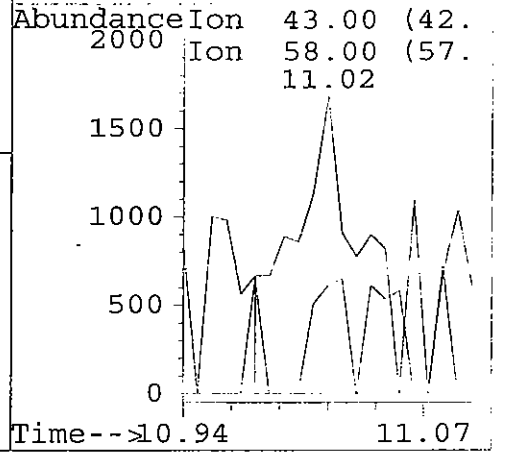


AbundanceScan 1154 (11.388 min): G2317Q01.D

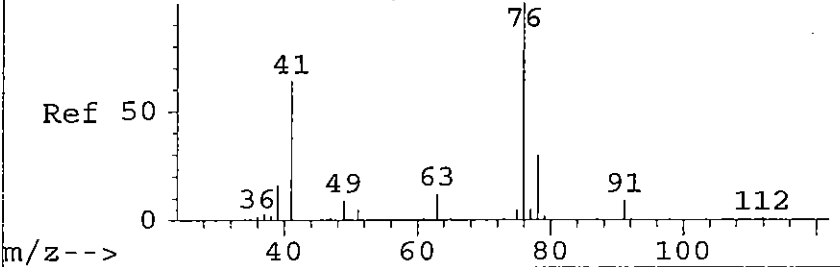

AbundanceScan 1184 (11.610 min): G2534K01.D

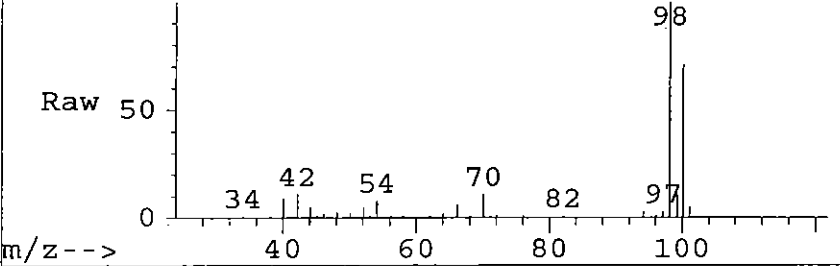


AbundanceScan 1184 (11.610 min): G2534K01.D

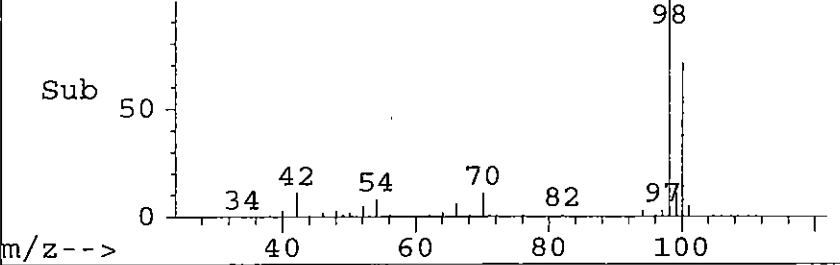

#65
 49 1,3-di-cl-propane 76 78
 Concen: 0.63 ppb
 RT: 11.61 min Scan# 1184
 Delta R.T. -0.14 min
 Lab File: G2534K01.D
 Acq: 19 May 03 8:12 pm

Tgt Ion	Resp	Lower	Upper
76	8271		
78	16.2	27.9	41.8#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

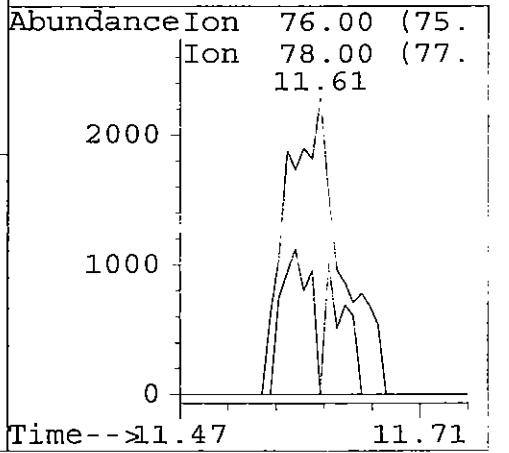

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/13/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: DUPE-7-2Q03	Lab Sample ID: 03-3205-1	Received Date: 05/13/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/20/03	Anal. Date: 05/20/03
Data File Name: 3205-01	Prep. No: -	Anal. Time: 00:32
Methanol Vol. -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	2.4	
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	0.8	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1 (a)	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	6	J
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8 (a)	<1.8	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	1.9	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	0.9	
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TETRACHLOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	112	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	99	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	107	
4	TOLUENE-D8	2037-26-5		73-129	111	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	79	
2	1,4-DICHLOROBENZENE-D4	3855-82-1		50-200	88	
3	FLUOROBENZENE	462-06-6		50-200	89	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

(a)MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Data Filename: C:\HPCHEM\1\DATA\03G2534\3205-01.D Sample : f=1 9
 Method : C:\HPCHEM\1\METHODS\E524G004.M Inst. : GCMS-G
 Acq. Time : May 20 00:32 2003 RF via : Multiple Level Calibration
 Method Update: Fri May 16 12:11 2003 Operator: Eddie
 Quant. Time : May 20 09:41 2003 Multiplr: 1.000000
 Print Time : Tue May 20 09:41 2003
 Miscellaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
Internal Standards											
1	Fluorobenzene I1	9.49	9.52	-0.002	96	70	620.688	10.00		-0.02	
47	Cl-benzene-d5, I2	13.10	13.12	-0.002	82	119	171.702	10.00		-0.02	
62	1,4-DCB-d4 150 15	15.61	15.63	-0.001	152	150	163.610	10.00		-0.02	

System Monitoring Compounds (Surrogate)											
27	Di-Br-F-Methane (7.94	7.97	-0.002	111	113	494.375	21.45		21.5	107.26%
29	1,2-di-Cl-ethane-	8.51	8.54	-0.002	65	102	206.483	19.71		19.7	98.56%
55	toluene-d8(S2)	11.59	11.61	-0.002	100	99	694.175	22.20		22.2	111.00%
70	4-Br-1-F-Bz (S3)	14.34	14.36	-0.001	174	95	301.532	22.36		22.4	111.82%

Target Compounds
 <<< I1 : ISTD ID = 1 >>>
 Qvalue

111	111 isopropyl alcoho	4.75	4.76	0.000	45	43	3.735	15.02		15.0	56	#
102	102 Acrolein x10	4.78	4.67	0.012	56	55	0.265	4.56		4.6	16	#
104	104 Carbon disulfide	5.74	5.74	0.000	76	78	25.145	0.65		0.7	84	#
101	101 Acetonitrilex10	4.72	4.71	0.000	41	40	0.606	11.01		11.0	1	#
113	113 Tert butyl alcoh	5.38	5.38	0.000	59	57	0.371	0.65		0.6	79	#
18	18 methylene chlorid	5.49	5.50	-0.001	84	49	19.560	1.29		1.3	94	#
200	200 Nitro methane x1	6.36	6.38	-0.002	61	46	1.087	0.45		0.4	8	#
98	98 Vinyl acetate x5	6.96	6.97	-0.002	43	86	1.559	12.61		12.6	69	#
91	91 2-butanone MEKx10	7.32	7.37	-0.005	43	72	6.433	1.10		1.1	82	#
25	25 chloroform	7.78	7.81	-0.003	83	85	24.164	0.76		0.8	91	#
201	201 Ethyl acetate x2	7.82	7.83	0.000	43	61	1.626	4.52		4.5	52	#?
117	117 Iso-butyl alcoho	7.82	7.83	0.000	43	42	1.626	14.66		14.7	55	#?
26	26 tetrahydrofuranx5	8.22	8.23	0.000	72	42	0.246	0.37		0.4	30	#
30	30 12-dichloroethane	8.61	8.63	-0.002	62	64	0.243	0.90		0.9	40	#
37	37 CCl4	9.18	9.19	-0.002	117	119	52.742	2.37		2.4	94	#
40	40 trichloroethene	10.00	10.02	-0.002	130	132	16.550	0.88		0.9	78	#
107	107 Et methacrylate	11.63	11.80	-0.017	69	99	0.499	1.65		1.6	58	#
93	93 2-Hexanone x5	11.93	11.93	0.000	43	58	2.160	6.21		6.2	40	#
48	48 112-tri-Cl-Et	11.59	11.49	0.010	97	83	24.201	3.30		3.3	8	#?

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\HPCHEM\1\DATA\03G2534\3205-01.D Sample : f=1 9
 Method : C:\HPCHEM\1\METHODS\E524G004.M Inst. : GCMS-G
 Acq. Time : May 20 00:32 2003 RF Via : Multiple Level Calibration
 Method Update: Fri May 16 12:11 2003 Operator: Eddie
 Quant. Time : May 20 09:41 2003 Multiplr: 1.000000
 Print Time : Tue May 20 09:41 2003
 Miscellaneous :


ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
<<<	I2 : ISTD ID = 47	>>>									
54	MIBK	10.96	10.99	-0.003	43	58	33.262	6.04	6.0	99	
49	1,3-di-cl-propane	11.59	11.75	-0.013	76	78	7.263	0.60	0.6	77	#?
59	tetra-cl-ethene	12.43	12.46	-0.002	166	168	27.911	1.90	1.9	97	


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Quantitation Report

Data File : C:\HPCHEM\1\DATA\03G2534\3205-01.D
Acq On : 20 May 03 12:32 am
Sample : F=1 9
Misc :
Quant Time: May 20 9:41 2003
Operator: Eddie
Inst : GCMS-G
Multiplier: 1.00
Quant Results File: quant.res





Method : C:\HPCHEM\1\METHODS\E524G004.M
Title : **Applied P & Ch Lab** EPA 524.2
Last Update : Fri May 16 12:11:07 2003
Response via : Multiple Level Calibration

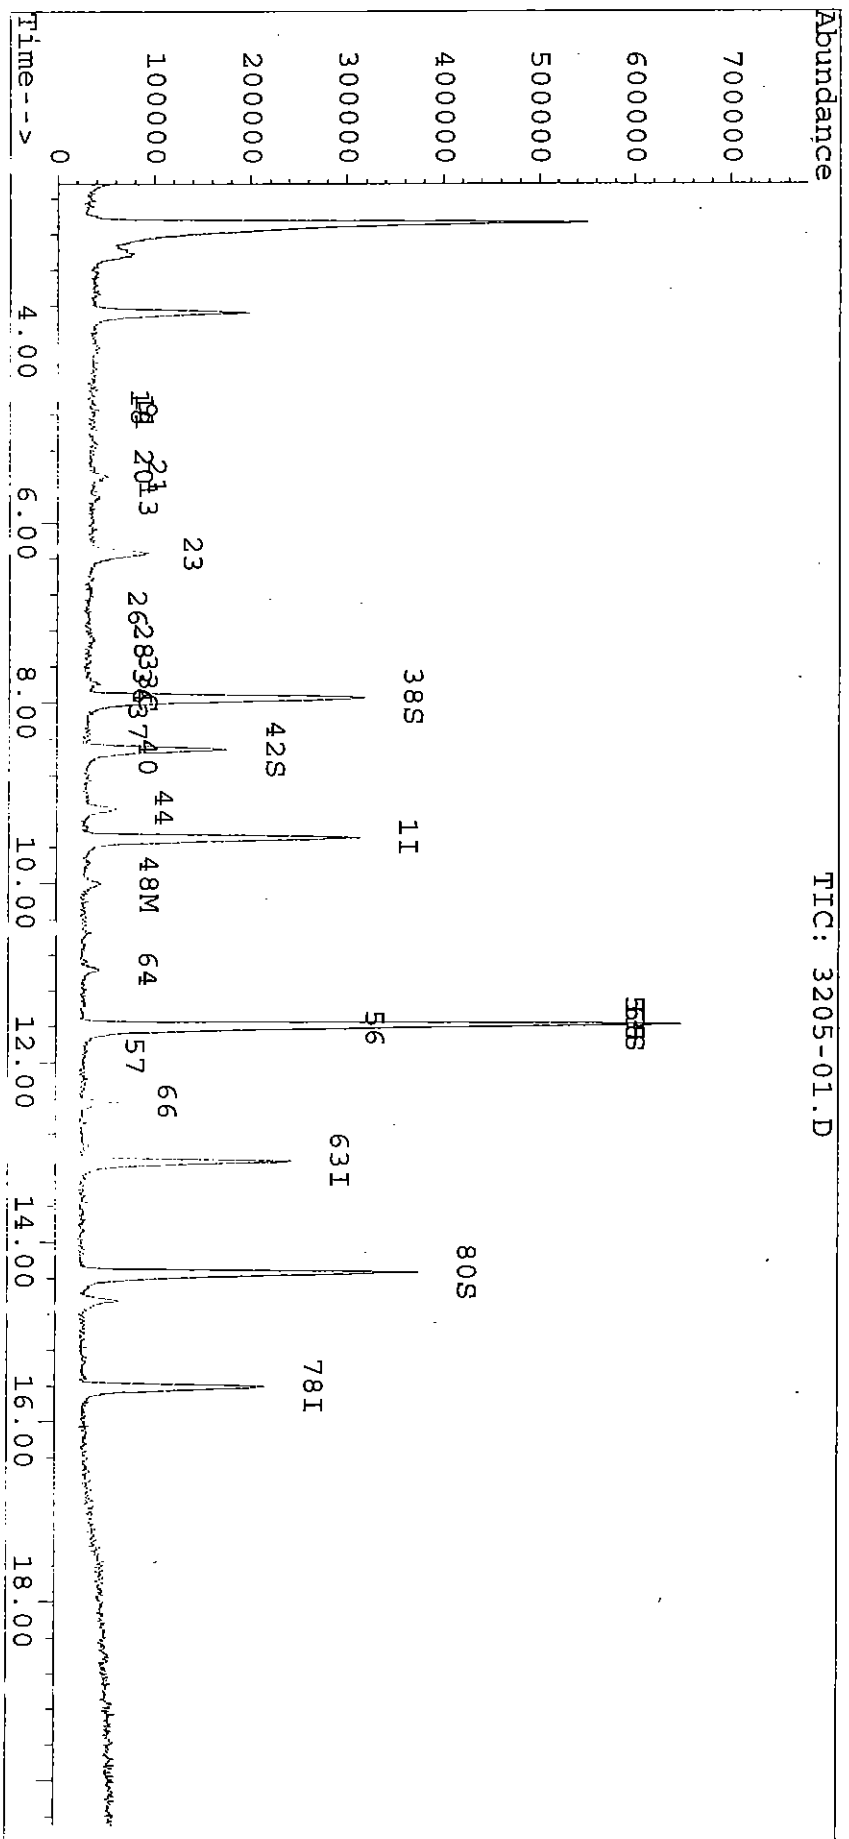

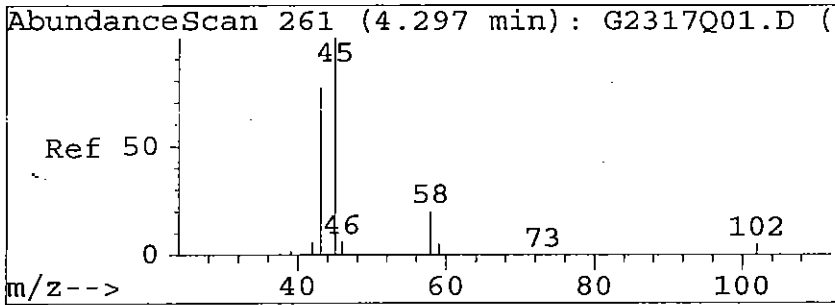




#9
 111 isopropyl alcohol x10
 Concen: 15.02 ppb
 RT: 4.75 min Scan# 318
 Delta R.T. -0.01 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Ratio	Lower	Upper
45	100		
43	49.3	77.0	115.5#
39	8.8	13.3	19.9#
0	0.0	0.0	0.0

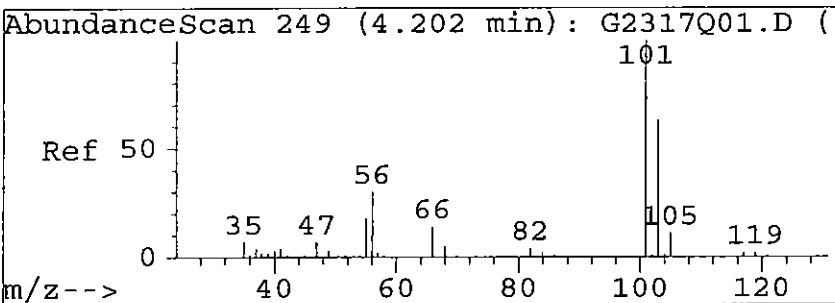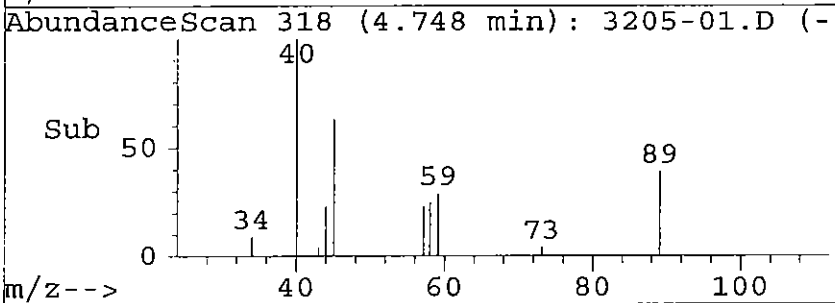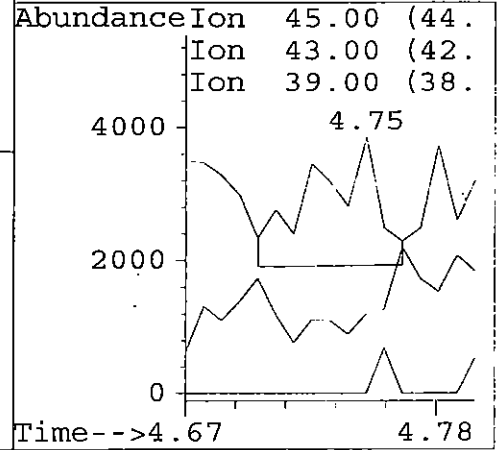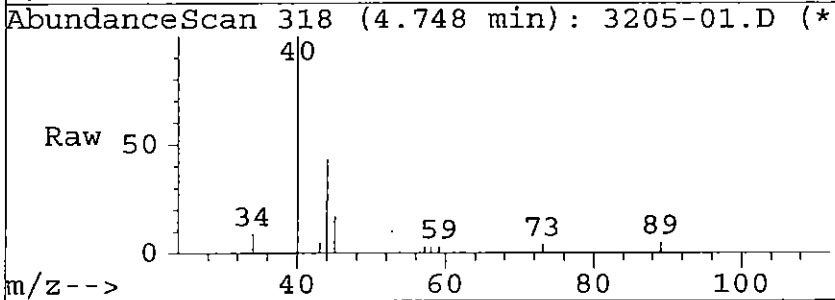

#11
 102 Acrolein x10
 Concen: 4.56 ppb
 RT: 4.78 min Scan# 322
 Delta R.T. 0.11 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am





Tgt Ion	Ratio	Lower	Upper
56	100		
55	120.8	29.2	87.5#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

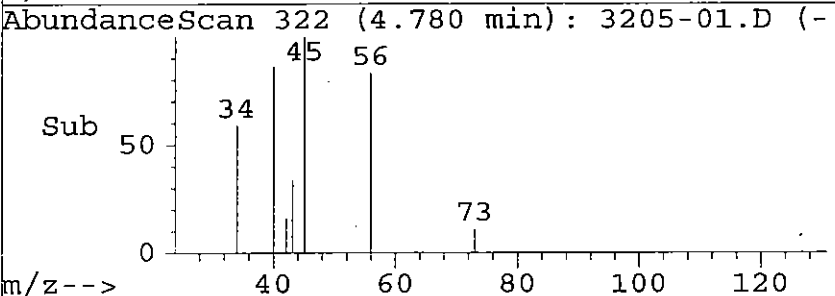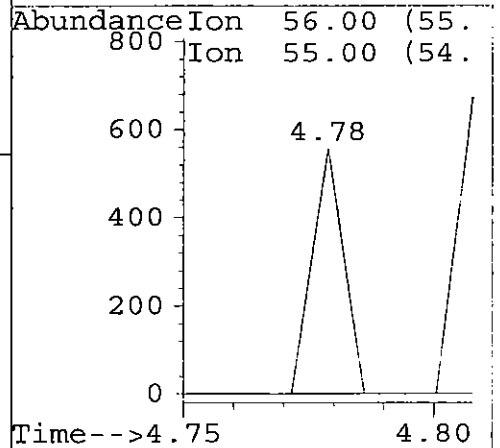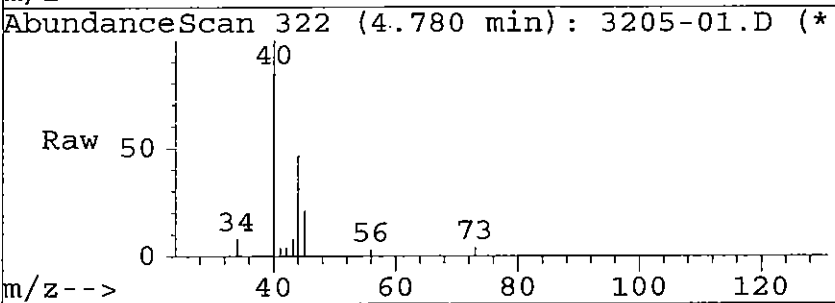

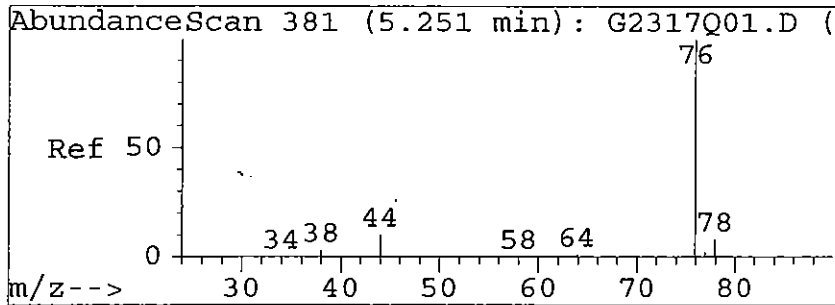




#13
 104 Carbon disulfide
 Concen: 0.65 ppb
 RT: 5.74 min Scan# 443
 Delta R.T. -0.00 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Resp	Lower	Upper
76	25145		
78	3.2	4.5	13.4#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

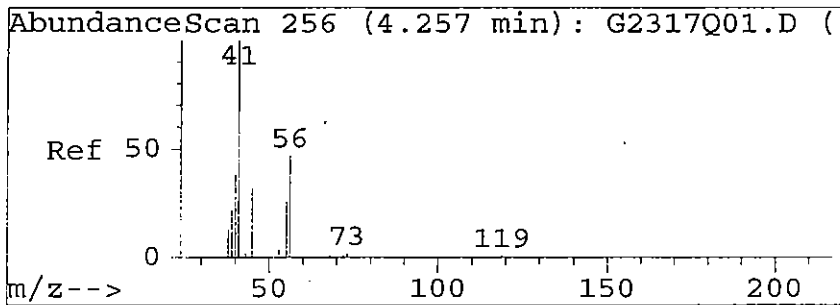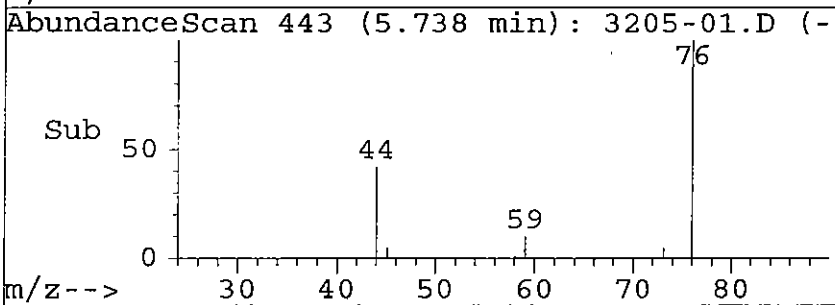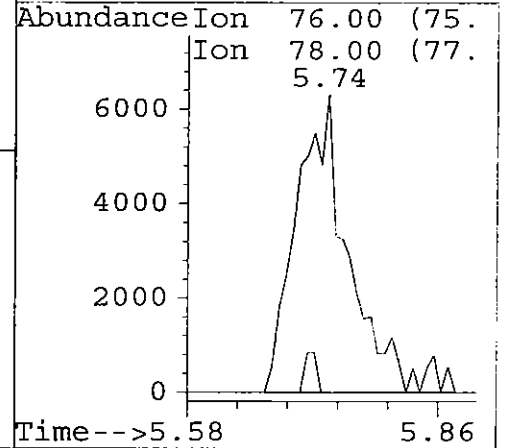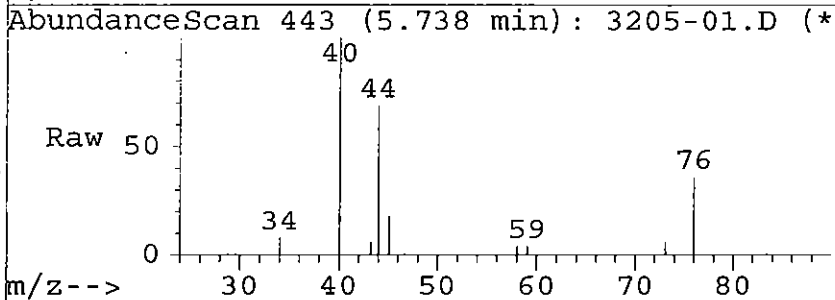

#18
 101 Acetonitrilex10
 Concen: 11.01 ppb
 RT: 4.72 min Scan# 314
 Delta R.T. 0.01 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am





Tgt Ion	Resp	Lower	Upper
41	606		
40	0.0	151.7	227.5#
39	0.0	17.3	25.9#
0	0.0	0.0	0.0

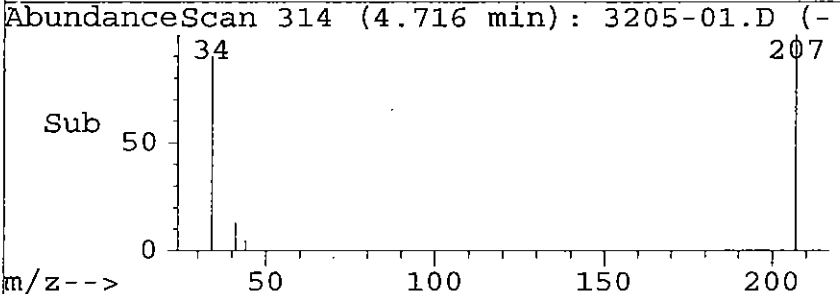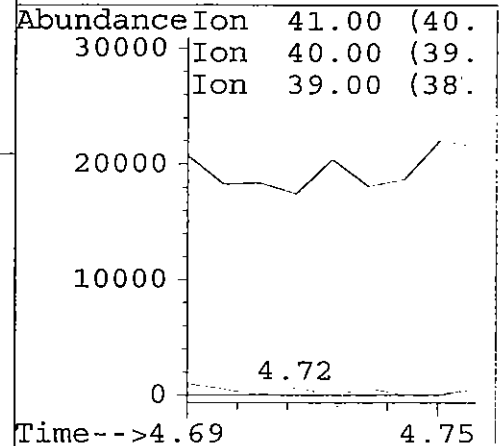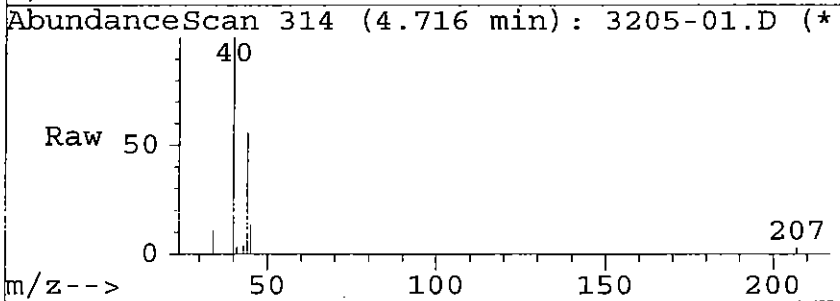

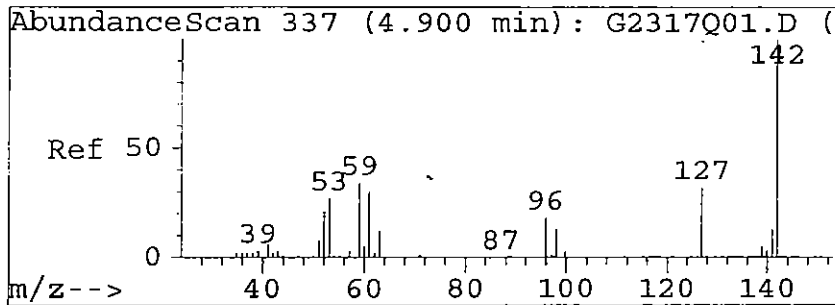




#20
 113 Tert butyl alcohol x10
 Concen: 0.65 ppb
 RT: 5.38 min Scan# 398
 Delta R.T. -0.00 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Resp	Lower	Upper
59	100		
57	0.0	5.8	8.7#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

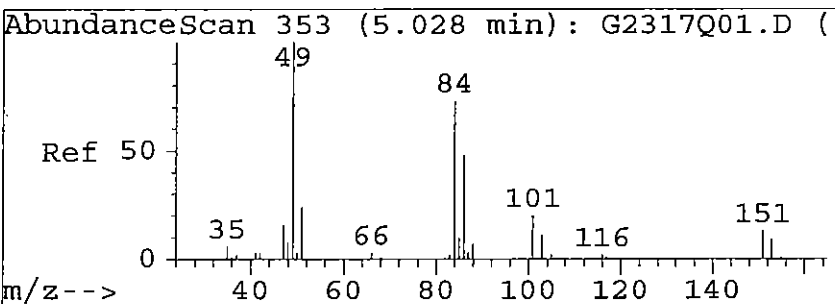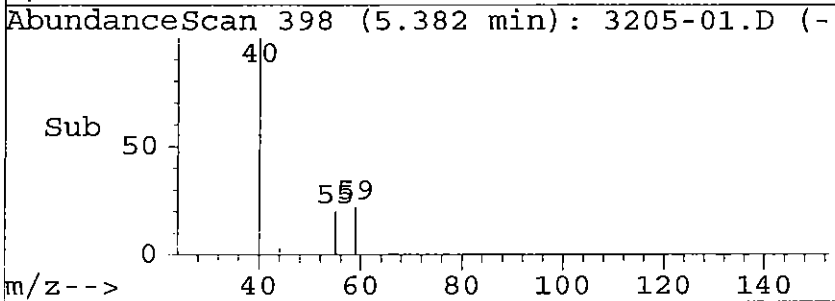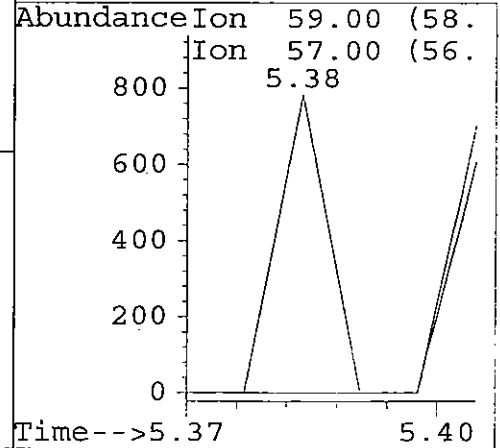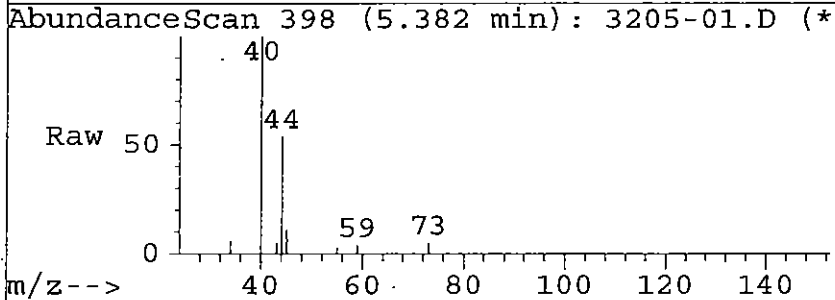

#21
 18 methylene chloride 49 84
 Concen: 1.29 ppb
 RT: 5.49 min Scan# 412
 Delta R.T. -0.01 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am





Tgt Ion	Resp	Lower	Upper
84	100		
49	132.7	62.9	188.5
0	0.0	0.0	0.0
0	0.0	0.0	0.0

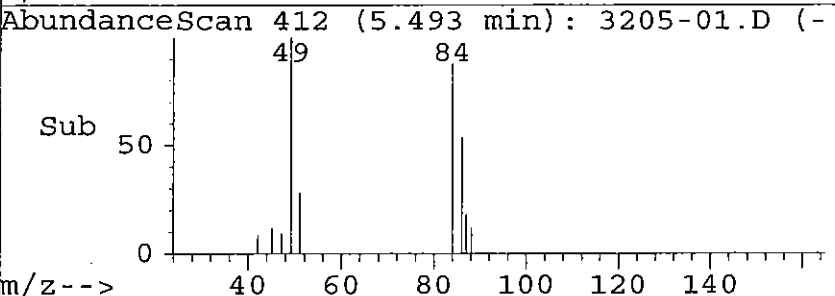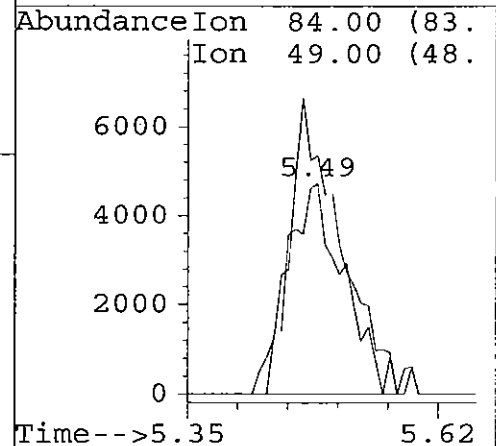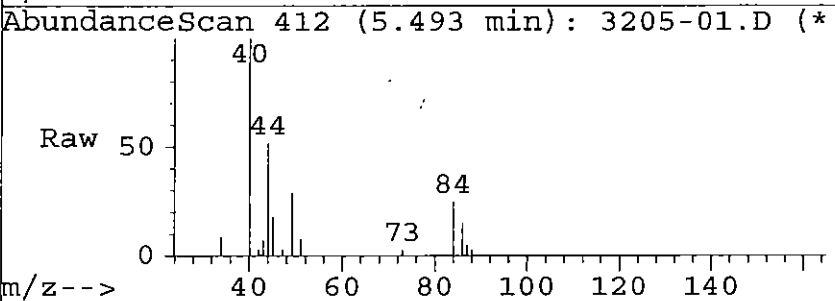

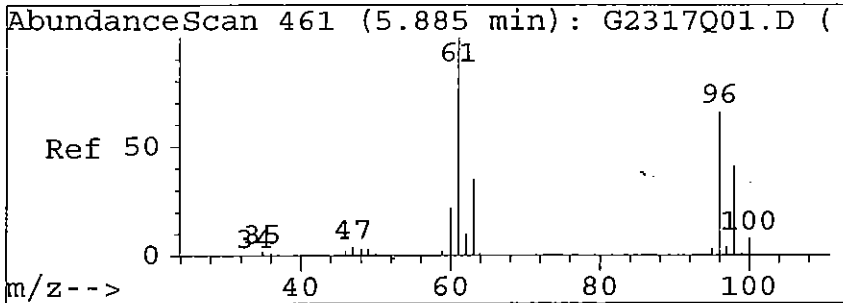




#23
 200 Nitro methane x10
 Concen: 0.45 ppb
 RT: 6.36 min Scan# 522
 Delta R.T. -0.02 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Resp	Lower	Upper
61	1087		
46	33.7	2.5	3.8#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

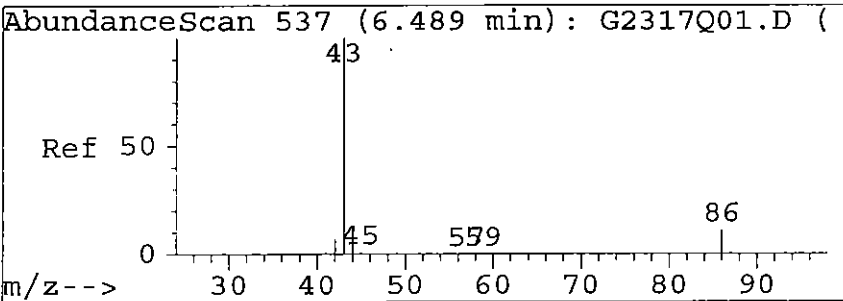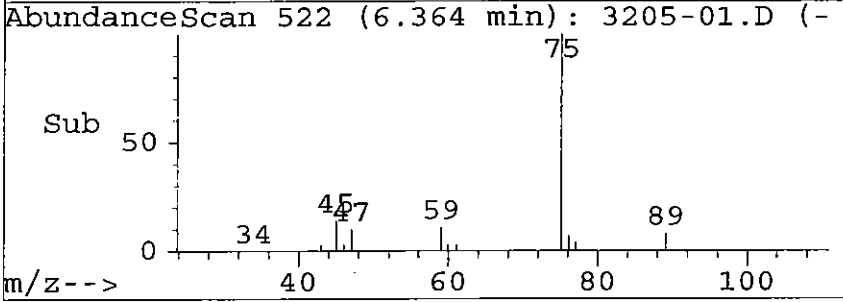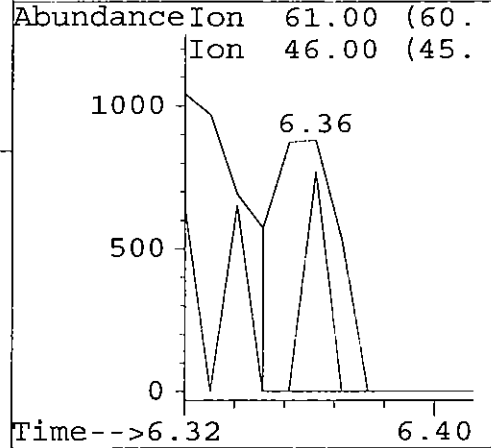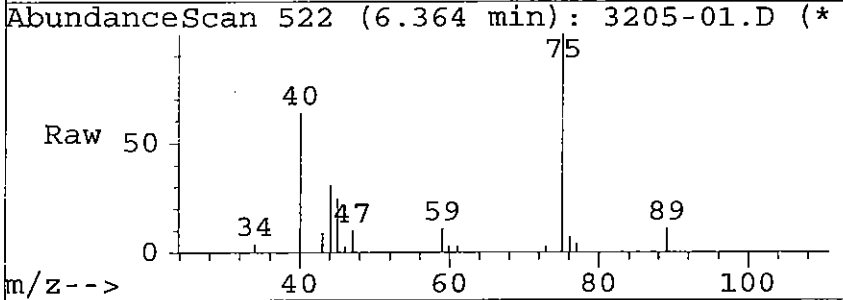

#26
 98 Vinyl acetate x5
 Concen: 12.61 ppb
 RT: 6.96 min Scan# 597
 Delta R.T. -0.01 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am





Tgt Ion	Resp	Lower	Upper
43	1559		
86	0.0	9.5	14.2#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

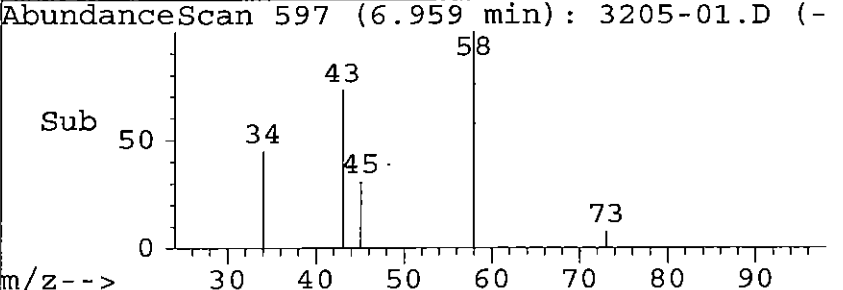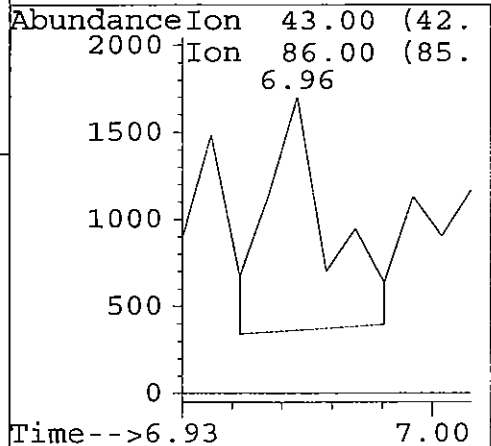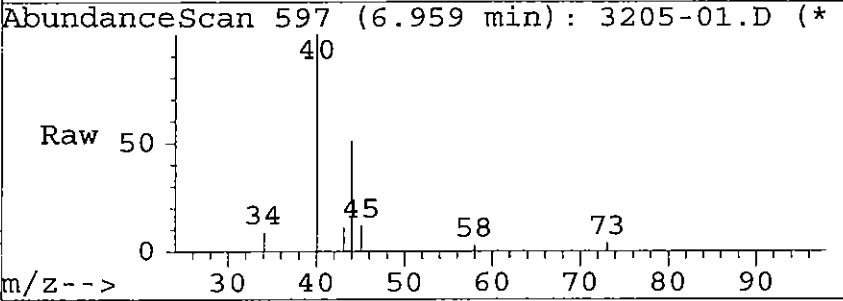

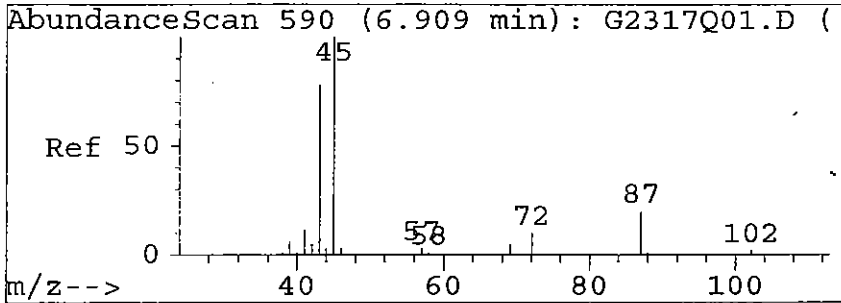




#28
 91 2-butanone MEKx10
 Concen: 1.10 ppb
 RT: 7.32 min Scan# 643
 Delta R.T. -0.05 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Ratio	Lower	Upper
43	100		
72	4.2	9.0	13.5#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

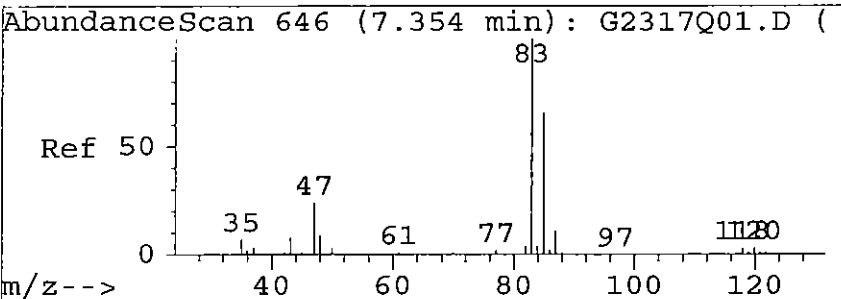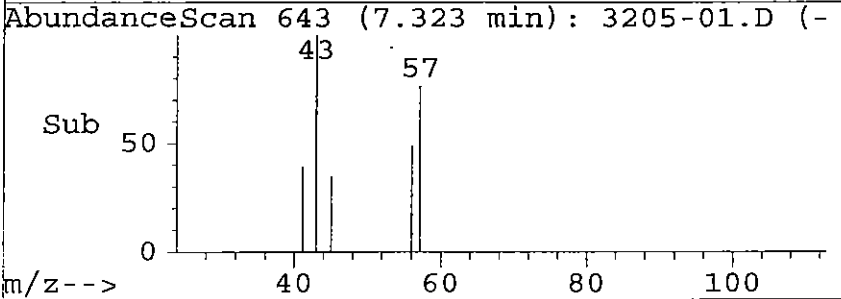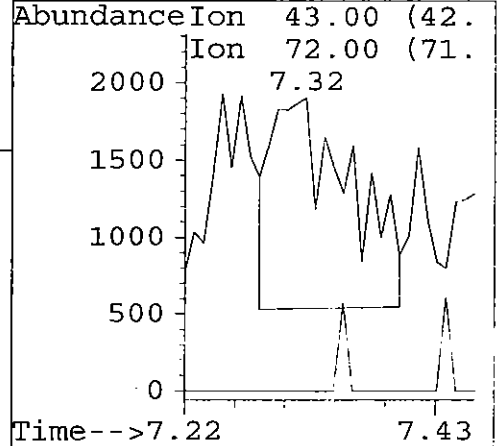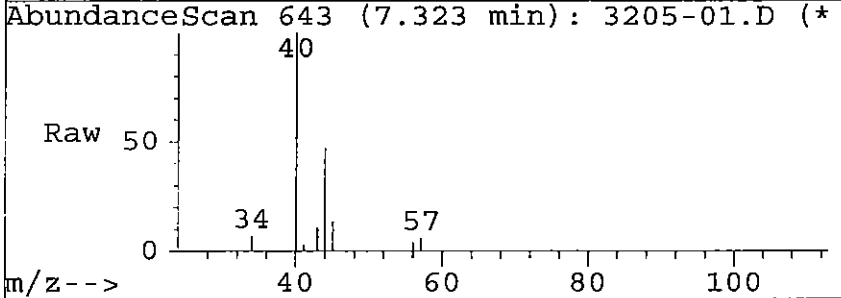

#33
 25 chloroform 83 85
 Concen: 0.76 ppb
 RT: 7.78 min Scan# 701
 Delta R.T. -0.03 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am





Tgt Ion	Ratio	Lower	Upper
83	100		
85	59.3	33.5	100.3
0	0.0	0.0	0.0
0	0.0	0.0	0.0

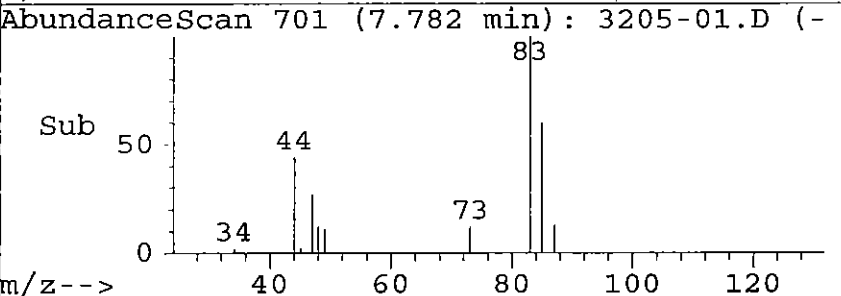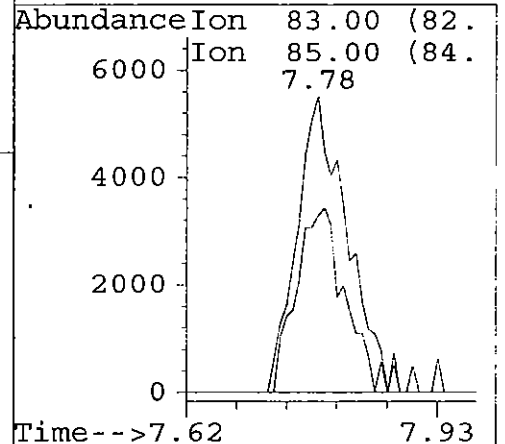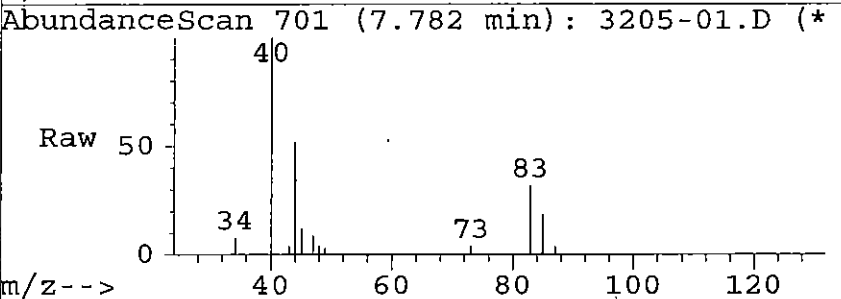

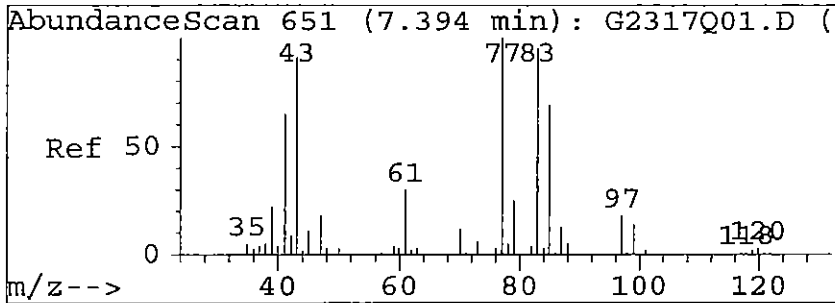




#34
 201 Ethyl acetate x2
 Concen: 4.52 ppb
 RT: 7.82 min Scan# 706
 Delta R.T. -0.01 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Ratio	Lower	Upper
43	100		
61	0.0	19.1	28.6#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

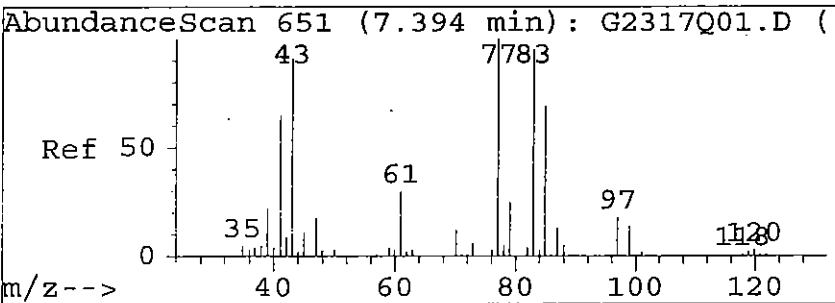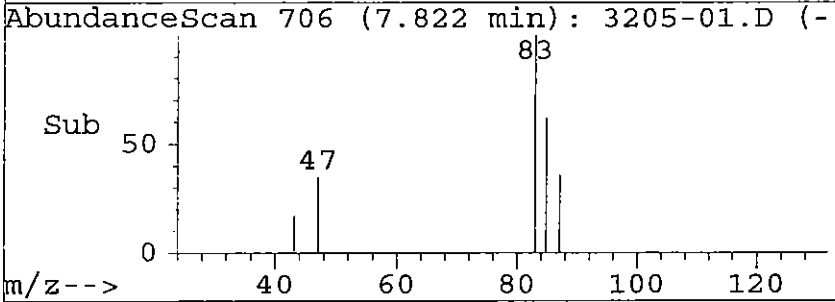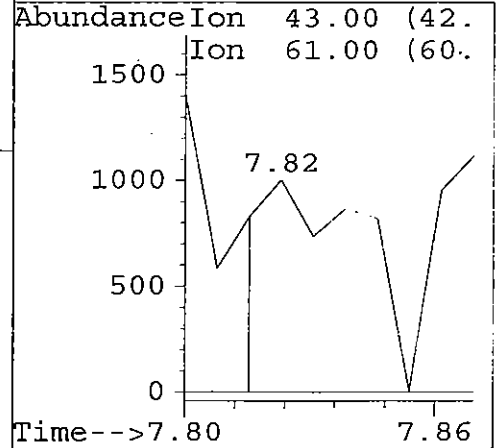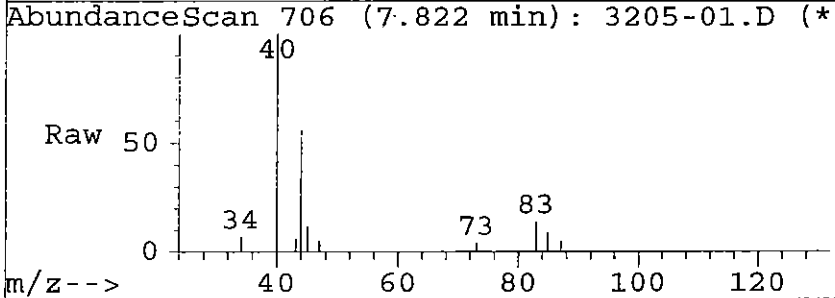

#36
 117 Iso-butyl alcohol X10
 Concen: 14.66 ppb
 RT: 7.82 min Scan# 706
 Delta R.T. -0.01 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am





Tgt Ion	Ratio	Lower	Upper
43	100		
42	15.0	7.3	10.9#
41	15.4	39.7	59.5#
0	0.0	0.0	0.0

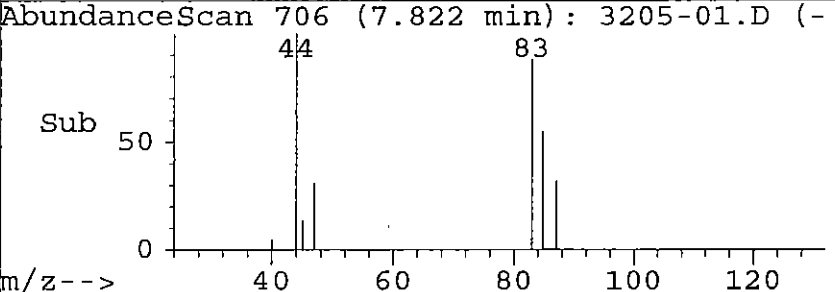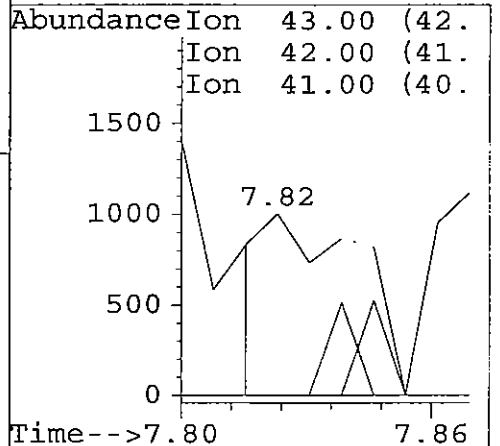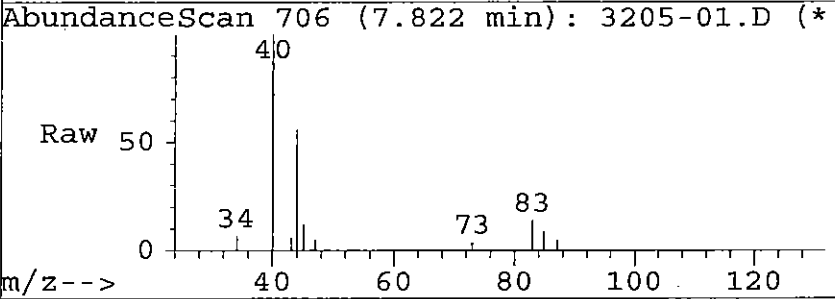

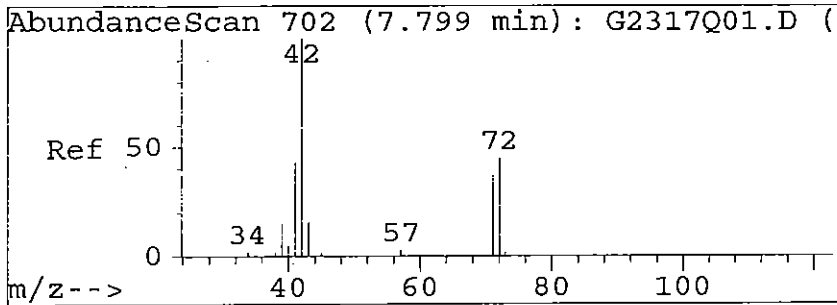




#37
 26 tetrahydrofuranx5
 Concen: 0.37 ppb
 RT: 8.22 min Scan# 756
 Delta R.T. -0.01 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Ratio	Lower	Upper
72	100		
42	304.5	99.5	298.3#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

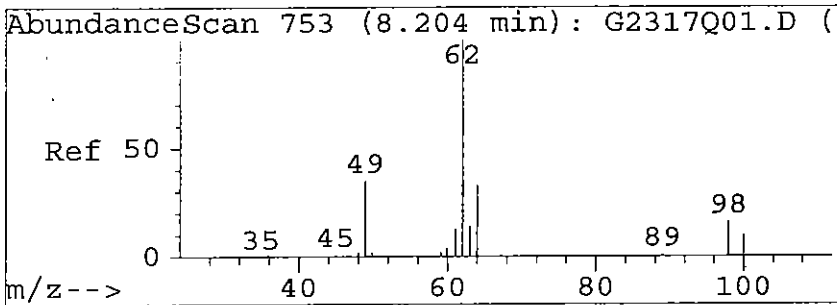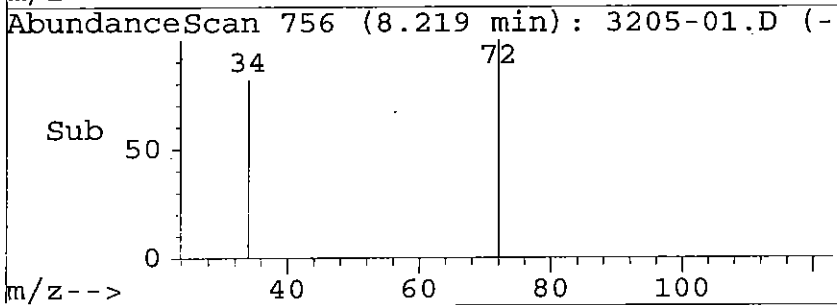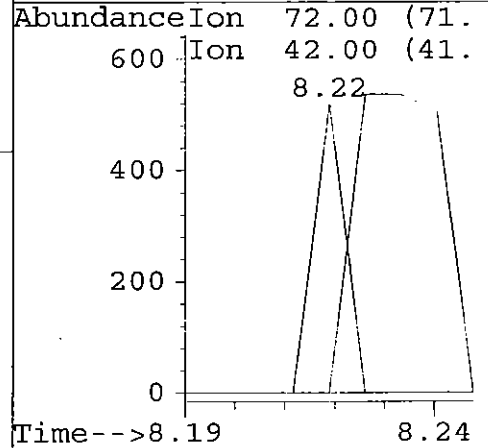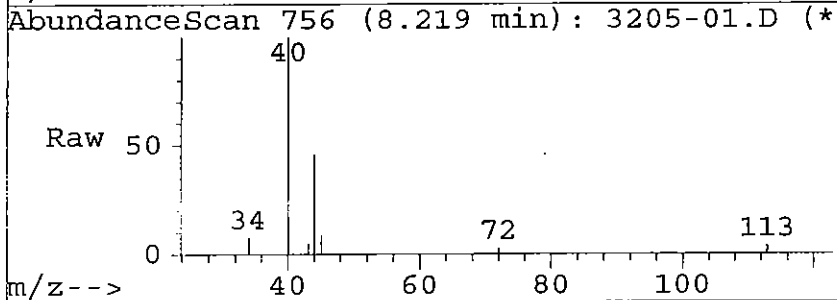

#40
 30 12-dichloroethane 64 62
 Concen: 0.90 ppb
 RT: 8.61 min Scan# 806
 Delta R.T. -0.02 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am





Tgt Ion	Ratio	Lower	Upper
62	100		
64	0.0	13.1	53.1#
49	0.0	16.2	56.2#
0	0.0	0.0	0.0

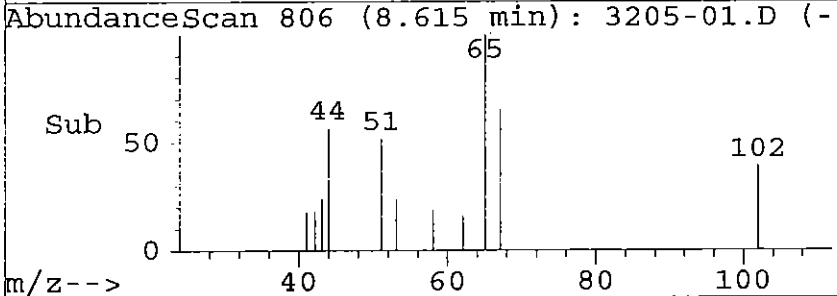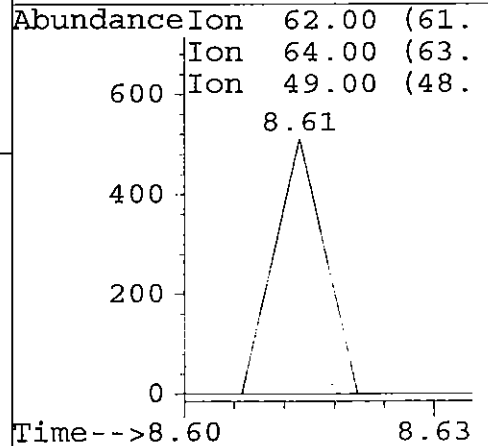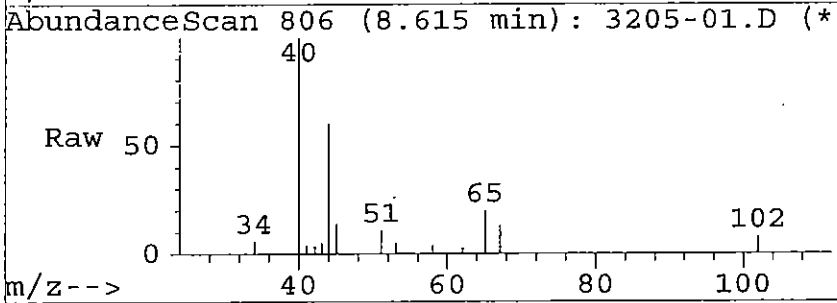

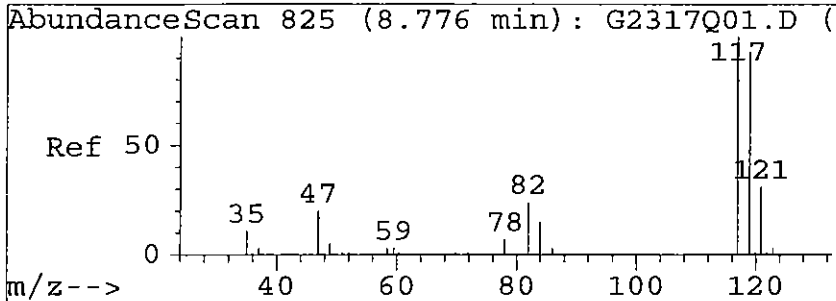




#44
 37 CCl4 117 119
 Concen: 2.37 ppb
 RT: 9.18 min Scan# 877
 Delta R.T. -0.01 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Resp	Lower	Upper
117	52742		
119	94.4	80.3	120.3
0	0.0	0.0	0.0
0	0.0	0.0	0.0

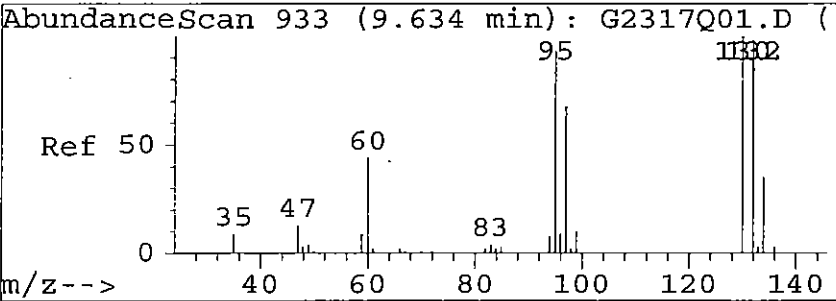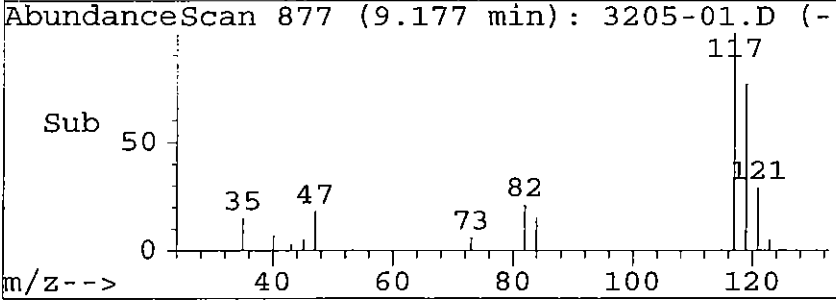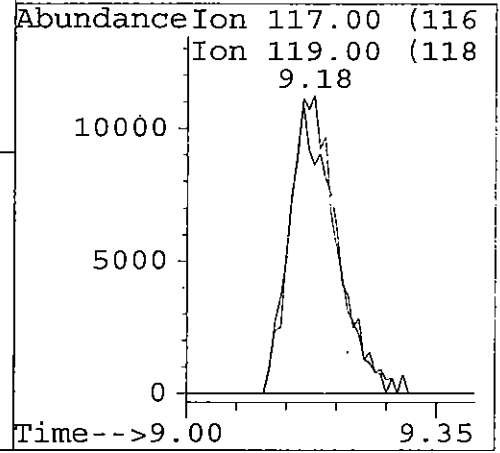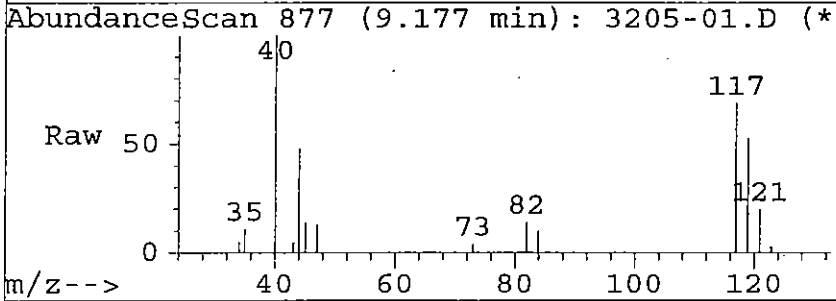

#48
 40 trichloroethene 130 132
 Concen: 0.88 ppb
 RT: 10.00 min Scan# 981
 Delta R.T. -0.02 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am





Tgt Ion	Resp	Lower	Upper
130	16550		
132	115.6	47.4	142.1
0	0.0	0.0	0.0
0	0.0	0.0	0.0

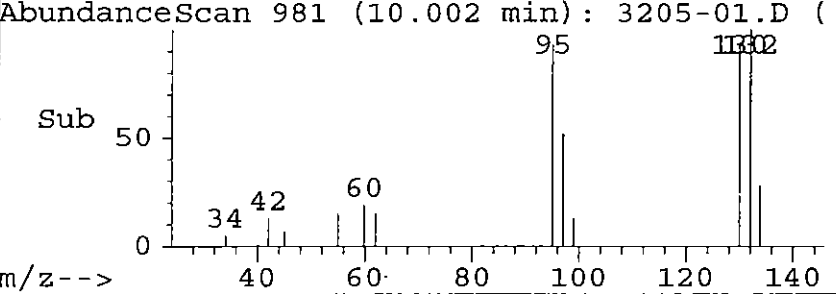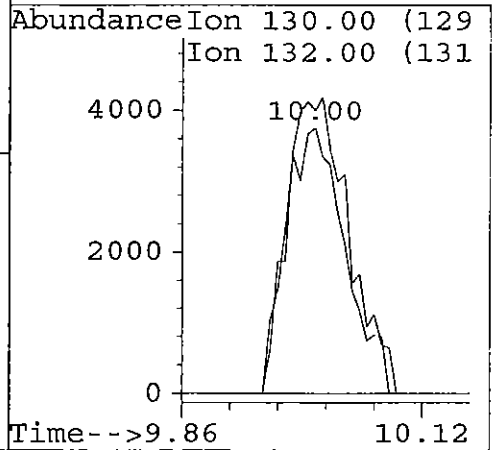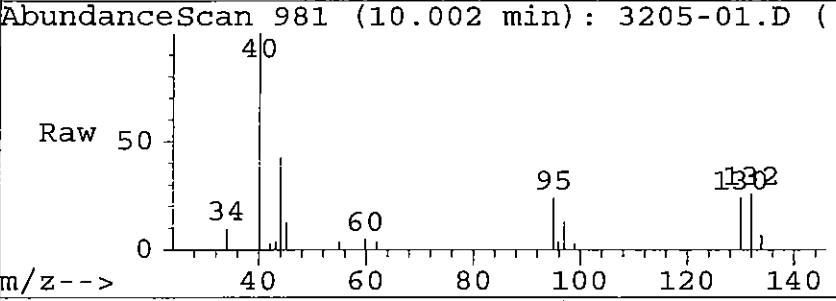

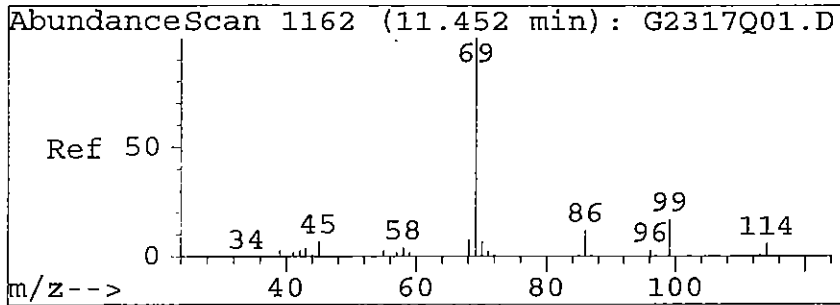




#56
 107 Et methacrylate
 Concen: 1.65 ppb
 RT: 11.63 min Scan# 1187
 Delta R.T. -0.16 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am


Tgt Ion	Resp	Lower	Upper
69	100		
99	0.0	9.4	28.0#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

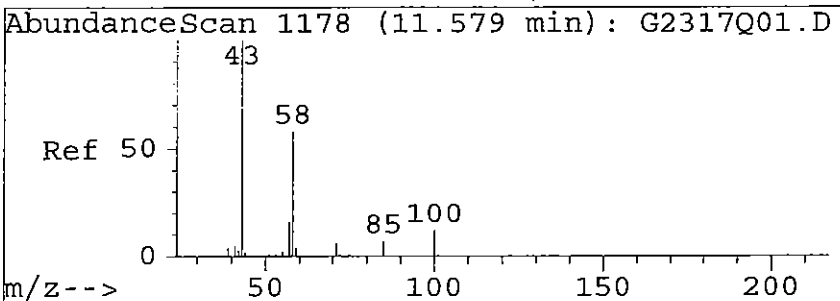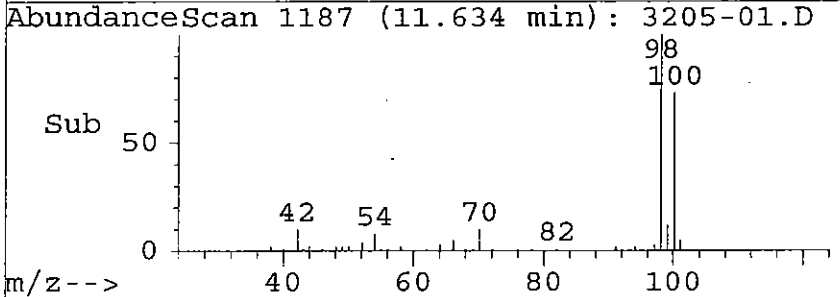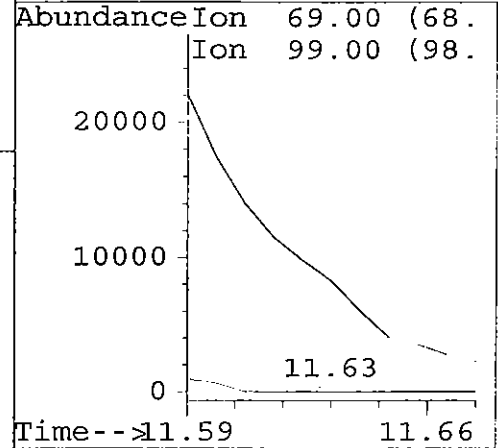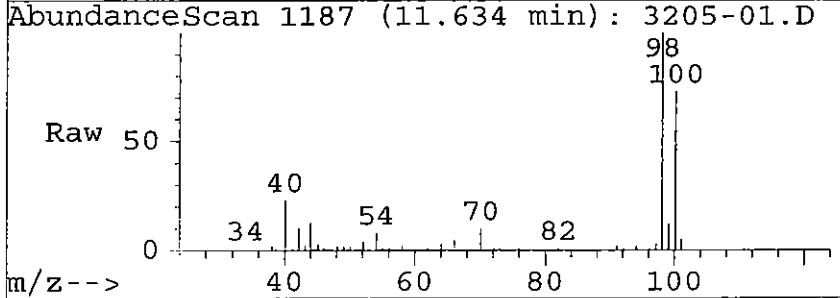


#57
 93 2-Hexanone x5
 Concen: 6.21 ppb
 RT: 11.93 min Scan# 1224
 Delta R.T. -0.00 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am

Tgt Ion	Resp	Lower	Upper
43	100		
58	11.8	44.5	66.8#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

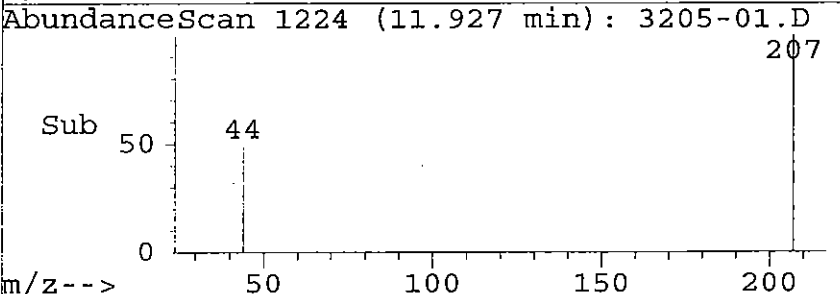
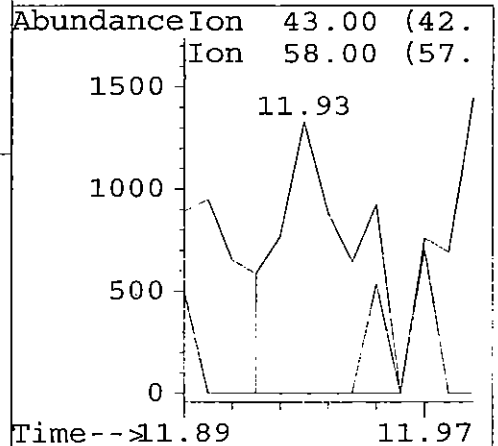
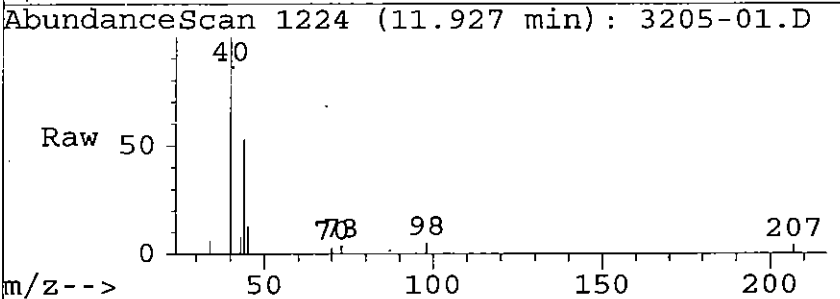


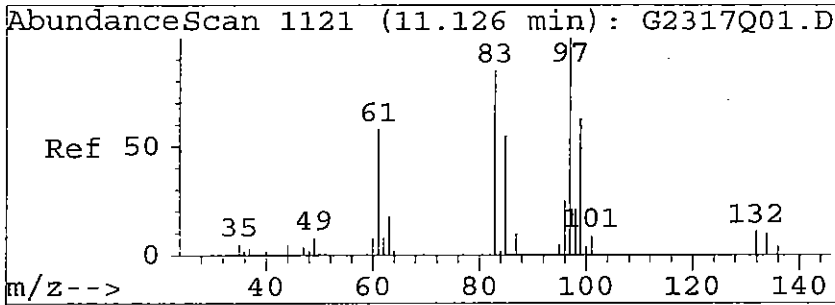


#58
 48 112-tri-Cl-Et 97 83
 Concen: 3.30 ppb
 RT: 11.59 min Scan# 1181
 Delta R.T. 0.10 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am

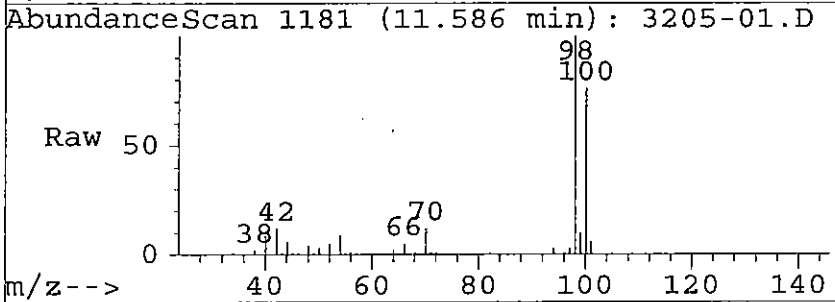



Tgt Ion:97 Resp: 24201
 Ion Ratio Lower Upper
 97 100
 83 0.0 41.5 124.4#
 0 0.0 0.0 0.0
 0 0.0 0.0 0.0

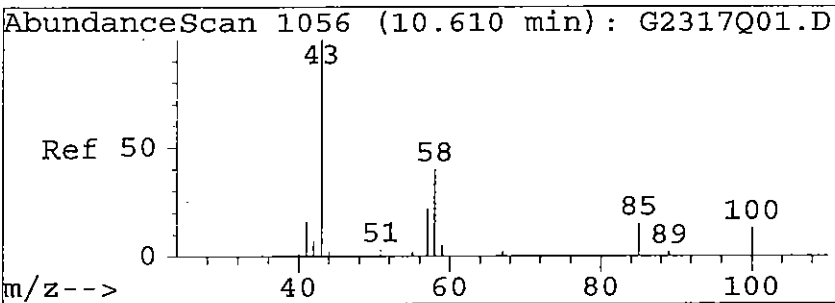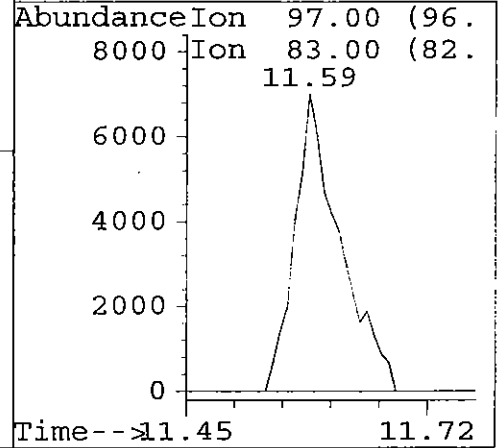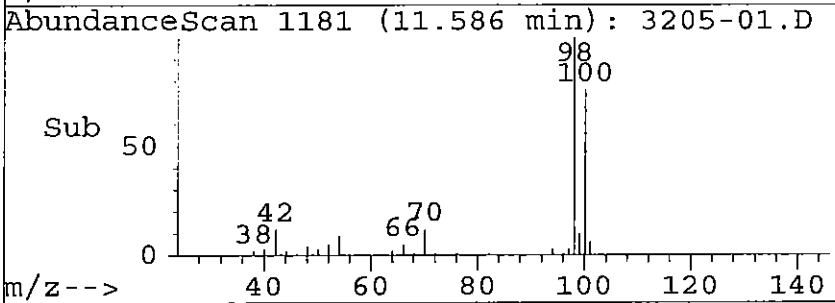


#64
 54 MIBK
 Concen: 6.04 ppb
 RT: 10.96 min Scan# 1102
 Delta R.T. -0.03 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am

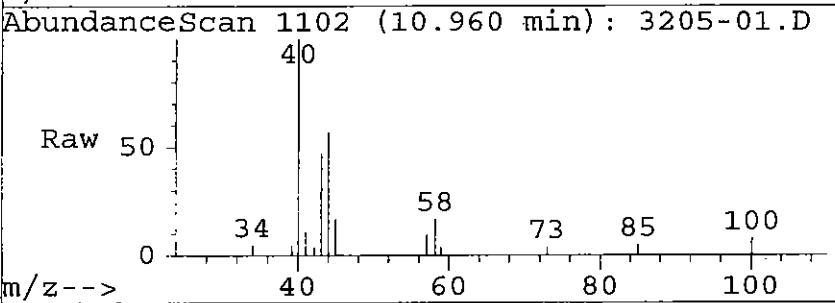





Tgt Ion:43 Resp: 33262
 Ion Ratio Lower Upper
 43 100
 58 38.2 17.5 57.5
 0 0.0 0.0 0.0
 0 0.0 0.0 0.0

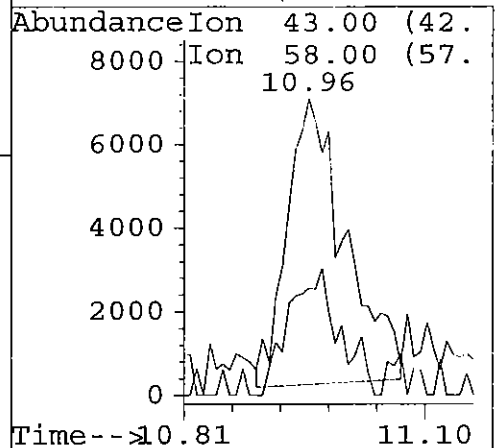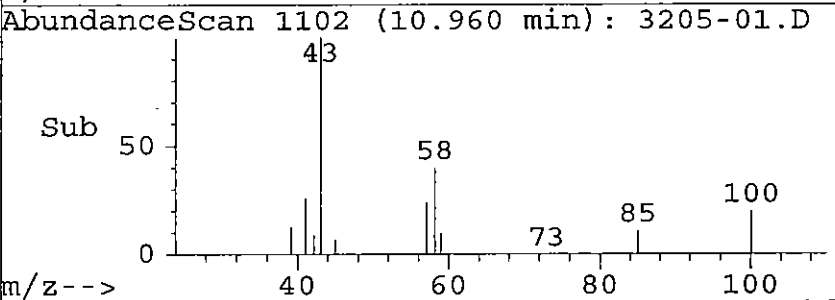

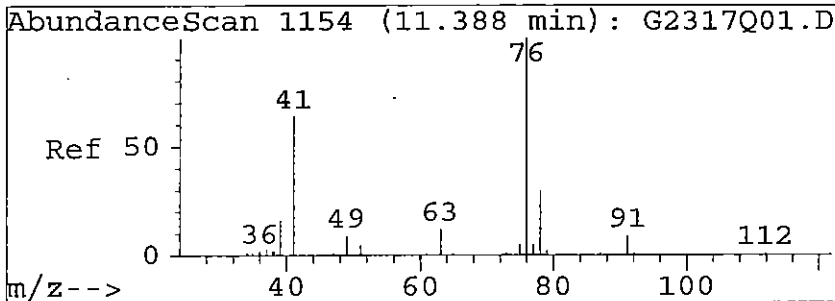




#65
 49 1,3-di-cl-propane 76 78
 Concen: 0.60 ppb
 RT: 11.59 min Scan# 1181
 Delta R.T. -0.17 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am

Tgt Ion	76	78	0	0	Resp:	7263	Lower	Upper
Ion Ratio	100	48.2	0.0	0.0				
		27.9	0.0	0.0				
		41.8#	0.0	0.0				

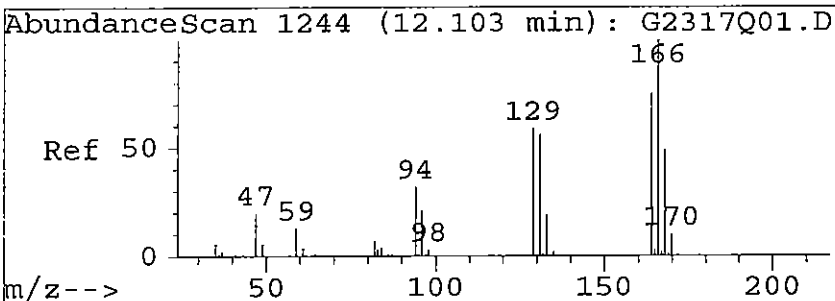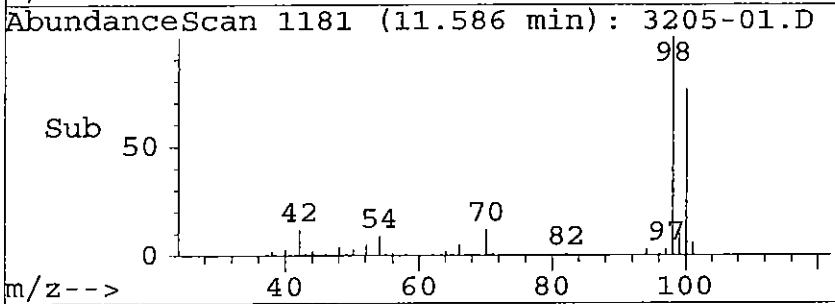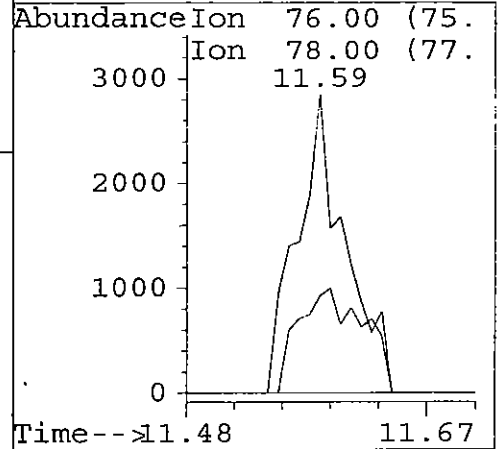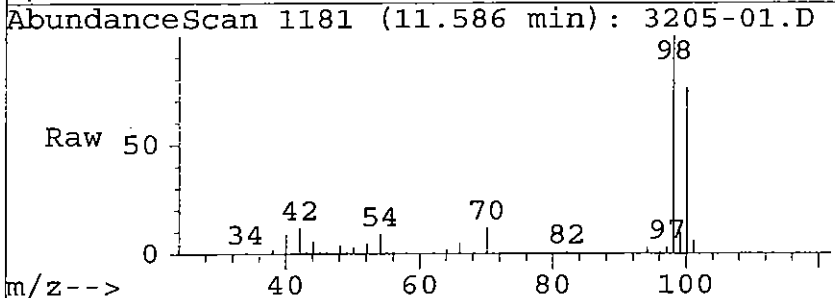

#66
 59 tetra-Cl-ethene 166 168
 Concen: 1.90 ppb
 RT: 12.43 min Scan# 1288
 Delta R.T. -0.03 min
 Lab File: 3205-01.D
 Acq: 20 May 03 12:32 am

Tgt Ion	166	168	0	0	Resp:	27911	Lower	Upper
Ion Ratio	100	50.9	0.0	0.0				
		24.4	0.0	0.0				
		73.0	0.0	0.0				

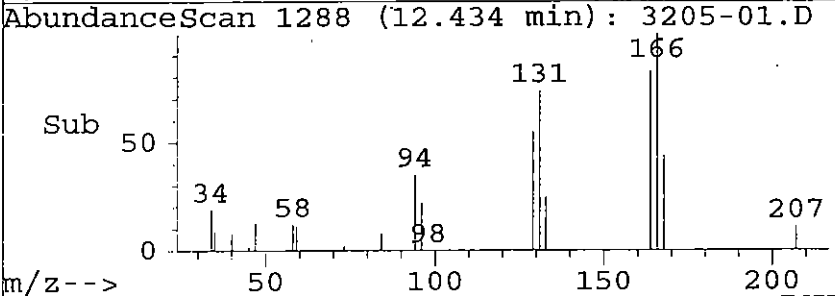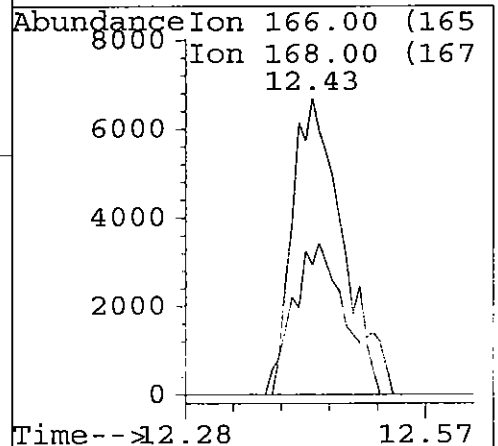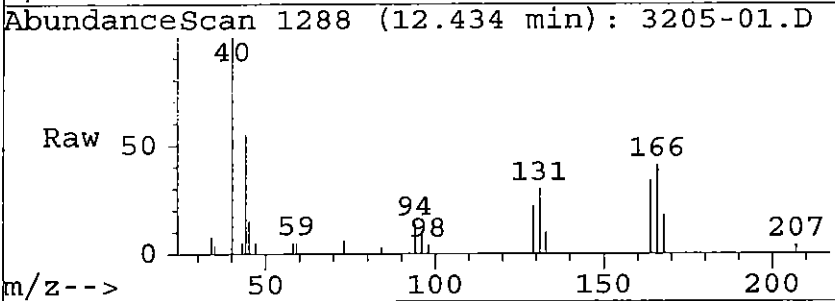

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/13/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: EB-13-5/13/03	Lab Sample ID: 03-3205-2	Received Date: 05/13/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/20/03	Anal. Date: 05/20/03
Data File Name: 3205-02	Prep. No: -	Anal. Time: 01:02
Methanol Vol: -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1 (a)	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	4	J
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8 (a)	<1.8	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	112TRICHLORO-122TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	102	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	91	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	99	
4	TOLUENE-D8	2037-26-5		73-129	105	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	89	
2	1,4-DICHLOROBENZENE-D4	3855-82-1		50-200	100	
3	FLUOROBENZENE	462-06-6		50-200	100	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

(a)MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/13/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: MW-18-1	Lab Sample ID: 03-3205-3	Received Date: 05/13/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/20/03	Anal. Date: 05/20/03
Data File Name: 3205-03	Prep. No: -	Anal. Time: 01:31
Methanol Vol. -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1 (a)	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	4	J
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8 (a)	<1.8	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TETRACHLOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates

			Control Limit, %	Surro. Rec.%
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	97
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	82
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	93
4	TOLUENE-D8	2037-26-5	73-129	98
# of out-of-control				0

Internal Standard

			Control Limit, %	IS Rec.%
1	CHLOROBENZENE-D5	3114-55-4	50-200	100
2	1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	108
3	FLUOROBENZENE	462-06-6	50-200	111
# of out-of-control				0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

(a)MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/13/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: MW-18-2	Lab Sample ID: 03-3205-4	Received Date: 05/13/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/20/03	Anal. Date: 05/20/03
Data File Name: 3205-04	Prep. No: -	Anal. Time: 02:01
Methanol Vol. -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1 (a)	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	4	J
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8 (a)	<1.8	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	100	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	89	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	96	
4	TOLUENE-D8	2037-26-5		73-129	100	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	99	
2	1,4-DICHLOROETHANE-D4	3855-82-1		50-200	109	
3	FLUOROBENZENE	462-06-6		50-200	112	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

(a)MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/13/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: MW-18-3	Lab Sample ID: 03-3205-5	Received Date: 05/13/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/20/03	Anal. Date: 05/20/03
Data File Name: 3205-05	Prep. No: -	Anal. Time: 02:31
Methanol Vol. -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	1.2	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1 (a)	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	4	J
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8 ^(a)	<1.8	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	0.4	J
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	103	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	95	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	100	
4	TOLUENE-D8	2037-26-5		73-129	106	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	99	
2	1,4-DICHLOROETHANE-D4	3855-82-1		50-200	109	
3	FLUOROBENZENE	462-06-6		50-200	109	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

^(a)MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/13/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: MW-18-4	Lab Sample ID: 03-3205-6	Received Date: 05/13/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/20/03	Anal. Date: 05/20/03
Data File Name: 3205-06	Prep. No: -	Anal. Time: 03:00
Methanol Vol. -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	2.4	
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	0.9	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1 (a)	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	7	J
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8 (a)	<1.8	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	2.1	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	1.0	
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TETRACHLOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	99	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	94	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	102	
4	TOLUENE-D8	2037-26-5		73-129	107	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	94	
2	1,4-DICHLOROETHANE-D4	3855-82-1		50-200	108	
3	FLUOROBENZENE	462-06-6		50-200	103	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

(a)MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/13/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: MW-18-5	Lab Sample ID: 03-3205-7	Received Date: 05/13/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/20/03	Anal. Date: 05/20/03
Data File Name: 3205-07	Prep. No: -	Anal. Time: 03:29
Methanol Vol. -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1 (a)	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	5	J
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8 (a)	<1.8	U
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	108	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	101	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	109	
4	TOLUENE-D8	2037-26-5		73-129	113	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	92	
2	1,4-DICHLOROETHANE-D4	3855-82-1		50-200	101	
3	FLUOROBENZENE	462-06-6		50-200	100	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

(a)MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 05/13/2003
Project ID: JPL GW Mon-2Q03	Service ID: 33205	Collected by:
Sample ID: TB-13-5/13/03	Lab Sample ID: 03-3205-8	Received Date: 05/13/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: G
Batch No: 03G2534	Prep. Date: 05/20/03	Anal. Date: 05/20/03
Data File Name: 3205-08	Prep. No: -	Anal. Time: 03:59
Methanol Vol. -	Sample Amount: 25 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	1.1 (a)	<1.1	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	6	J
42	METHYLENE CHLORIDE	75-09-2	µg/L	1.8 (a)	3.9	B
43	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	105	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	91	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	99	
4	TOLUENE-D8	2037-26-5		73-129	106	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	96	
2	1,4-DICHLOROETHANE-D4	3855-82-1		50-200	106	
3	FLUOROBENZENE	462-06-6		50-200	110	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

(a)MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

FORM-2A

Applied P & Ch Laboratory

Surrogate Recovery Summary for Method 524.2

Client Name: GEOFON, Inc.

Contract No:

Lab Code: APCL

Case No:

SAS No:

SDG Number: 033205

Project ID: JPL GW Mon-2Q03

Project No: 04-4428.10

Sample Matrix: Water

Batch No: 03G2534

#	Client Sample No	Lab Sample ID	S1 % #	S2 % #	S3 % #	S4 % #	TOT OUT
1	03G2534-LCS-01	03G2534-LCS-01	88	105	102	99	0
2	MW-22-1MS	03-3130-2MS	87	97	95	94	0
3	MW-22-1MSD	03-3130-2MSD	96	111	107	103	0
4	03G2534-MB-01	03G2534-MB-01	107	98	104	107	0
5	DUPE-7-2Q03	03-3205-1	112	99	107	111	0
6	EB-13-5/13/03	03-3205-2	102	91	99	105	0
7	MW-18-1	03-3205-3	97	82	93	98	0
8	MW-18-2	03-3205-4	100	89	96	100	0
9	MW-18-3	03-3205-5	103	95	100	106	0
10	MW-18-4	03-3205-6	99	94	102	107	0
11	MW-18-5	03-3205-7	108	101	109	113	0
12	TB-13-5/13/03	03-3205-8	105	91	99	106	0
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							

QC Control Limit

S1 = 1-BROMO-4-FLUOROBENZENE (4-BROMOFL 70-129
 S2 = 1,2-DICHLOROETHANE-D4 70-129
 S3 = DIBROMOFLUOROMETHANE 70-122
 S4 = TOLUENE-D8 73-129

Column to be used to flag recovery values:

* - Values outside of contract required QC Limits D - Surrogate diluted out I - Matrix Interference

FORM-3A

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 524.2

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 33205
Project ID: JPL GW Mon-2Q03	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03G2534	
LCS Filename: G2534L01	Date Analyzed: 051903	Time Analyzed: 17:18
LCSD Filename: -	Date Analyzed: -	Time Analyzed: -

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
BENZENE	µg/L	20	0	20.1	101	65-120
CHLOROBENZENE	µg/L	20	0	20.4	102	65-134
1,1-DICHLOROETHENE	µg/L	20	0	20.0	100	65-127
TOLUENE	µg/L	20	0	19.2	96	65-134
TRICHLOROETHENE	µg/L	20	0	20.0	100	67-122
# of Out-of-control					0	

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____
