



Applied Physics & Chemistry Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel. (909) 590-1828 Fax (909) 590-1498

July 07, 2003

GEOFON, Inc.
Attention: Leo Williamson
22632 Golden Spring Dr Ste 270
Diamond Bar CA 91765

Dear Leo Williamson,

This package contains samples in our Service ID 03-3414 and your project : 04-4428.10 JPL GW Mon-2Q03.

Enclosed please find:

- (1) Original analytical report.
- (2) Original Chain of Custody.
- (3) One diskette containing EDD deliverable.
- (4) One original Level C Data Package Deliverable.

If anything is missing or you have any questions, please feel free to contact me.

Respectfully submitted,

A handwritten signature in black ink, appearing to read 'R. Kirakozova', is written over the printed name.

Regina Kirakozova
Associate QA/QC Director
Applied P & Ch Laboratory

Applied P & Ch Laboratory

13780 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Submitted to:
 GEOFFON, Inc.
 Attention: Leo Williamson.
 22632 Golden Spring Dr Ste 270
 Diamond Bar CA 91765
 Tel: (909)396-7662 Fax: (909)396-1455

APCL Analytical Report

Service ID #: 801-033414 Received: 05/28/03
 Collected by: Leo Williamson Extracted: 05/29/03
 Collected on: 05/28/03 Tested: 05/28-06/03/03
 Reported: 06/11/03

Sample Description: Water
 Project Description: 04-4428.10 JPL

Analysis of Water Samples

| Component Analyzed | Method | Unit | PQL | Analysis Result | |
|---------------------------------------|----------|-------------------------|------|--------------------|--------------------|
| | | | | MW-5 03-03414-1 | MW-8 03-03414-2 |
| BICARBONATE | SM2320B | mg/L | 2 | 146 | 153 |
| CARBONATE | SM2320B | mg-CaCO ₃ /L | 2 | <2 | <2 |
| PH | 9040B | pH unit | 0.01 | 6.84 | 7.00 |
| SOLIDS, TOTAL DISSOLVED (TDS) | 160.1 | mg/L | 10 | 263 | 277 |
| CHROMIUM (VI) | 7196 | mg/L | 0.01 | <0.01 | <0.01 |
| Dilution Factor | | | | 1 | 1 |
| PERCHLORATE | 314.0 | µg/L | 4 | <4 | 4.2 |
| Dilution Factor | | | | 2 | 2 |
| CHLORIDE CL ⁻ | 300.0 | mg/L | 0.2 | 9.0 | 14.1 |
| NITRATE AS N | 300.0 | mg/L | 0.04 | 2.3 | 1.4 |
| SULFATE SO ₄ ⁻² | 300.0 | mg/L | 0.5 | 22.1 | 36.4 |
| Dilution Factor | | | | 1 | 1 |
| ARSENIC | 200.9 | µg/L | 5 | <5 | <5 |
| CALCIUM | 200.7 | µg/L | 200 | 45,300 | 52,300 |
| IRON | 200.7 | µg/L | 50 | 357 | 48.7J |
| MAGNESIUM | 200.7 | µg/L | 100 | 13,800 | 16,500 |
| POTASSIUM | 200.7 | µg/L | 400 | 2,740 | 2,450 |
| SODIUM | 200.7 | µg/L | 2000 | 16,500 | 18,000 |
| Dilution Factor | | | | 1 | 1 |
| 1,4-DIOXANE | 8270-SIM | µg/L | 1 | <1 | - |

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|-----------------------------------|--------|------|-----|--------------------|--------------------|-----------------------------|
| | | | | MW-5 03-03414-1 | MW-8 03-03414-2 | TB-15-5/28/03 03-03414-3 |
| VOLATILE ORGANIC COMPOUNDS | | | | | | |
| Dilution Factor | | | | 1 | 1 | 1 |
| BENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMOBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMOCHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMODICHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMOFORM | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| BROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| N-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| SEC-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TERT-BUTYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 2-BUTANONE | 524.2 | µg/L | 10 | <10 | <10 | <10 |
| CARBON TETRACHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLORODIBROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROFORM | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CHLOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 2-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|---|--------|------|---------|--------------------|--------------------|-----------------------------|
| | | | | MW-5 03-03414-1 | MW-8 03-03414-2 | TB-15-5/28/03 03-03414-3 |
| 4-CHLOROTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DIBROMO-3-CHLOROPROPANE | 524.2 | µg/L | 1.1 (a) | <1.1 | <1.1 | <1.1 |
| 1,2-DIBROMOETHANE (EDB) | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| DIBROMOMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,3-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,4-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| DICHLORODIFLUOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CIS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TRANS-1,2-DICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,3-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 2,2-DICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| CIS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TRANS-1,3-DICHLOROPROPENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| ETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| HEXACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| ISOPROPYLBENZENE (CUMENE) | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| P-ISOPROPYLTOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| METHYLENE CHLORIDE | 524.2 | µg/L | 1.8 (a) | <1.8 | 3.7 | 3.8 |
| 4-METHYL-2-PENTANONE (MIBK) | 524.2 | µg/L | 10 | 5J | 5J | 5J |
| METHYL-T-BUTYL ETHER (MTBE) | 524.2 | µg/L | 1 | <1 | <1 | <1 |
| NAPHTHALENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| N-PROPYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| STYRENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,1,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2,2-TETRACHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TETRACHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TOLUENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,3-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,4-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,1-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2-TRICHLOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TRICHLOROETHENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| TRICHLOROFLUOROMETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,3-TRICHLOROPROPANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,1,2,2-TRICHLORO-1,2,2-TRIFLUOROETHANE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,2,4-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| 1,3,5-TRIMETHYLBENZENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| VINYL CHLORIDE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |

APCL Analytical Report

| Component Analyzed | Method | Unit | PQL | Analysis Result | | |
|--------------------|--------|------|-----|--------------------|--------------------|-----------------------------|
| | | | | MW-5 03-03414-1 | MW-8 03-03414-2 | TB-15-5/28/03 03-03414-3 |
| O-XYLENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |
| M/P-XYLENE | 524.2 | µg/L | 0.5 | <0.5 | <0.5 | <0.5 |


PQL: Practical Quantitation Limit. MDL: Method Detection Limit. CRDL: Contract Required Detection Limit

N.D.: Not Detected or less than the practical quantitation limit. "-": Analysis is not required.

J: Reported between PQL and MDL.

Listed Dilution Factors (DF) are relative to the method default DF. All unlisted DFs are 1.0

(a) MDL reported.

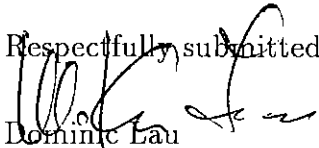Respectfully submitted,

Dominic Lau
Laboratory Director
Applied P & Ch Laboratory

Level C Data Package Deliverables

General Information

Project: 04-4428.10 JPL

APCL Service ID: 03-3414



Applied P & Ch Laboratory

13760 Magnolia Ave. Chino, CA 91710

Telephone (909)590-1828

Fax (909)590-1498

Case Narrative

Project: JPL/04-4428.10

For GEOFON, Inc.

APCL Service No: 03-3414

1. Sample Identification

The sample identifications are listed in the following table:

| GEOFON, Inc. Sample ID | APCL Sample ID |
|------------------------|----------------|
| MW-5 | 03-03414-1 |
| MW-8 | 03-03414-2 |
| TB-15-5/28/03 | 03-03414-3 |

2. Analytical Methodology

Samples are analyzed by EPA methods

524.2 (Volatile Organic Compounds),

7196A (Chromium (VI)),

314.0 (Perchlorate, low level),

300.0 (Anions, by IC),

SM2320B (Bicarbonate, Carbonate),

9040B (pH),

160.1 (Solids, Total Dissolved (TDS)),

200.7 (Metals, by ICP),

200.9 (Arsenic, As, by GFAA),

8270C-SIM (1,4-Dioxane),

3. Holding Time

All samples were extracted, digested and analyzed within the holding times defined by the appropriate EPA methods of the analyses.

4. Preservation

All samples were preserved and stored according to the appropriate EPA methods.

5. Tele-log

None


6. Anomaly

(1) EPA 524.2:


Methylene Chloride in the amount of 5.9 ug/L was detected in the Method Blank of batch 03G2684. Methylene Chloride was also detected in the associated field samples, due to lab contamination.

"I certify that these data are technically accurate, complete, and in compliance with the terms and conditions of the contract, for other than the conditions detailed above. Release of the data contained in the hardcopy data package and its electronic data deliverable submitted on diskette had been authorized by the Laboratory Manager or her/his designee, as verified by the following signature."

Respectfully submitted,



Regina Kirakozova
Associate QA/QC Director
Applied P & Ch Laboratory



INCORPORATED
22632 GOLDEN SPRINGS DR., SUITE 270
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

GEOFON

CHAIN-OF-CUSTODY RECORD

SHALLOW WELLS

0036

LABORATORY COPY

| Item | Sample Identifier | Matrix | Date | Time | Preserved | # of Cont. | QC Level | T.A.T | Analyses | | | | | | | | | | Comments | | |
|------|-------------------|--------|--------|------|-----------|------------|----------|-------|----------|--------|-----|-----|------|------|------|-----|-----|--------|----------|---|---|
| | | | | | | | | | H2O | Sp4/03 | B30 | HCl | None | MIB3 | 3+1+ | 1+1 | ITC | Normal | | X | X |
| 1 | MW-5 | H2O | Sp4/03 | B30 | | | | | X | X | X | X | X | X | X | X | X | X | X | X | |
| 2 | MW-8 | | | | | | | | X | X | X | X | X | X | X | X | X | X | X | X | |
| 3 | | | | | | | | | | | | | | | | | | | | | |
| 4 | | | | | | | | | | | | | | | | | | | | | |
| 5 | TB-15-5/20/03 | H2O | Sp4/03 | | | | | | X | X | X | X | X | X | X | X | X | X | X | X | |
| 6 | | | | | | | | | | | | | | | | | | | | | |
| 7 | | | | | | | | | | | | | | | | | | | | | |
| 8 | | | | | | | | | | | | | | | | | | | | | |
| 9 | | | | | | | | | | | | | | | | | | | | | |
| 10 | | | | | | | | | | | | | | | | | | | | | |

3114

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager

SAMPLES COLLECTED BY: Leo W. Williamson COURIER AND AIR BILL NUMBER: _____
 RELINQUISHED BY: Leo W. Williamson RECEIVED BY: S. Bush DATE: 5/29/03 TIME: 12:40
S. Bush DATE: 5/29/03 TIME: 15:30

COOLER TEMPERATURE UPON RECEIPT: _____
 SAMPLE'S CONDITION UPON RECEIPT: _____



INCORPORATED
 22632 GOLDEN SPRINGS DR., SUITE 270
 DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

SHALLOW WELLS

0037

| Item | Sample Identifier | Matrix | Date | Time | Preserved | # of Cont | QC Level | T.A.T. | Analyses | Comments |
|---|-------------------|------------------|---------|------|-----------|-----------|----------|--------|----------|----------|
| | | | | | | | | | | |
| GEOPON, LAB COORDINATOR LAB COORDINATOR'S PHONE: (909) 396-7662 LAB COORDINATOR'S FAX: (909) 396-1455 PROJECT NAME: JPL LAM Mon-2903 PROJECT LOCATION: MW-5 PROJECT PHONE NUMBER: (714) 920-8729 CITY, STATE AND ZIP CODE: Pasadena, CA CLIENT: US NAVY SNOW PROJECT MANAGER'S PHONE: (909) 396-7662 PROJECT MANAGER'S FAX: (909) 396-7662 LABORATORY PHONE: (909) 590-1828 LABORATORY FAX: (909) 590-1498 LABORATORY ADDRESS: 13760 Magnolia Ave CITY, STATE AND ZIP CODE: Chino, CA, 91710 RECIPIENT NAME: GEOFON, INC. ADDRESS: 22632 Golden Springs Dr #270 CITY, STATE AND ZIP CODE: Diamond Bar, CA 91765 | | | | | | | | | | |
| 1 | MW-5 | H ₂ O | 5/19/03 | 830 | None | 2 | III | Normal | X | |
| 2 | | | | | | | | | | |
| 3 | | | | | | | | | | |
| 4 | | | | | | | | | | |
| 5 | | | | | | | | | | |
| 6 | | | | | | | | | | |
| 7 | | | | | | | | | | |
| 8 | | | | | | | | | | |
| 9 | | | | | | | | | | |
| 10 | | | | | | | | | | |
| SAMPLES COLLECTED BY: Leo W. Williamson RELINQUISHED BY: Leo W. Williamson COURIER AND AIR BILL NUMBER: 9-29-03 RECEIVED BY: G. Barkley DATE: 5/19/03 TIME: 1530 COOLER TEMPERATURE UPON RECEIPT: SAMPLE'S CONDITION UPON RECEIPT: | | | | | | | | | | |

3114

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager

Sample Receiving Checklist

APCL ServiceID: **3414** Client Name/Project: Gordon / JPL

1. Sample Arrival

Date/Time Received 5/28/03 1530 Date/Time Opened 5/28/03 1530 By (name): Kenneth Chan
Custody Transfer: Client Golden State UPS US Mail FedEx APCL Empl: Scott B.

2. Chain-of-Custody (CoC)

With Samples? Faxed? Client has Copy? Signed, dated? By: _____
 Project ID? Analyses Clear? Hold Samples? #on Hold _____ # Received 3
 CoC/Docs Zip-Locked under lid? Compos. #: _____ #Samples OK? _____
 Discrepancies? Client notified? Response (attach docs): _____

3. Shipping Container/Cooler

Cooler Used? # of 1 Cooled by: Ice Blue Ice Dry Ice None
Temp °C 3.9
(Cooler temperature measured from temp blank if present, otherwise measured from the cooler).
Cooler Custody Seal? Absent Intact Tampered?

4. Sample Preservation

pH <2 pH >12
If Not, pH = _____ Preserved by: Client APCL Third Party _____

5. Holding-time Requirements

pH 24hr BACT 6/24hr Cr^{VI} 24hr NO₃ 48hr BOD 48hr
 Cl₂ ASAP Turbidity 48hr DO ASAP Fe(II) ASAP
 HT Expired? Client notified?

6. Sample Container Condition

Intact? Broken? Documented? Number: _____
Type: plastic glass Tube: brass/SS Tedlar Bag
 Quantity OK? Leaking? Anomaly?
 Caps tight? Air Bubbles? Anomaly?
Labels: Unique ID? Date/Time Preserved?

7. Turn Around Time

RUSH TAT: _____ Std (7-10 days) Not Marked

8. Sample Matrix

Drinking H₂O Other Liq Soil Wipe Polymer Air Other: _____
 Ground H₂O Sludge Filter Oil/Petro Paint W. Water Extract Unknown

9. Pre-Login Check List Completed & OK?

ALL OK? (if not, attach docs) Client Contact? (Name: _____) Date/Time: _____
Received/Checked by: [Signature] Date: 28 May 2003 Time: 7:39 a.m.

*HT: Samples must be analyzed for results to reflect total concentrations. Results generated outside required of holding times are considered minimal values and may be used to define waste as hazardous but not as non-hazardous.

Sample Login: Check List

03-03414 (0470_ 151) (2202777_ 151)

05/28/03

Part 1: General Information

| | | | |
|--------------------------|--------------------------|----------------------|--|
| <input type="checkbox"/> | Company Information | Name: | <i>GEOFON, Inc.</i> |
| | | Address: | <i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i> |
| <input type="checkbox"/> | Project Information | Project Description: | <i>JPL</i> |
| | | Project #: | <i>04-4428.10</i> |
| <input type="checkbox"/> | Billing Information | P.O. #: | |
| | | Bill Address: | <i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i> |
| | | Lab Project ID: | |
| | | Client Database #: | <i>3</i> |
| <input type="checkbox"/> | Receiving Information | Who Received Sample? | <i>Kenny Chan</i> |
| | | Receiving Date/Time: | <i>05/28/03 1530</i> |
| | | COC No. | |
| <input type="checkbox"/> | Shipping Information | Shipping Company | <i>APCL pick up</i> |
| | | Packing Information: | <i>Cooler/Ice Chester</i> |
| | | Cooler Temperature: | <i>3.9 °C</i> |
| <input type="checkbox"/> | Container Information | Container Provider: | <i>Client</i> |
| <input type="checkbox"/> | Sampling Information | Sampling Person: | |
| | | Sampling Company: | <i>Client</i> |
| <input type="checkbox"/> | Turn-Around-Time Option: | | <i>Rush 5 working day(s)</i> |
| <input type="checkbox"/> | QC Option: | | <i>NEESA C</i> |
| <input type="checkbox"/> | Disposal Option: | | <i>Not specify</i> |

Part 2: Sample Information

| Seq. # | Sample ID (on COC) | Sample Sub-ID | APCL Sample ID | Matrix | Cont-tainer | Preser-vative | Vol, ml Am. g | # of Replica | Condition G, L, B | Collected mmmddyy | Hold ? | Composite Group | TAT Days |
|--------|--------------------|---------------|----------------------|--------|-------------|---------------|---------------|--------------|-------------------|-------------------|--------|-----------------|----------------------------|
| 1 | MW-5 | VOC | 03-03414-1- α | W | V | C | 40 | 3 | G | 052803 | N | 0 | 7 <input type="checkbox"/> |
| | MW-5 | Metal | 03-03414-1- β | W | P | N | 500 | 1 | G | 052803 | N | 0 | 7 <input type="checkbox"/> |
| | MW-5 | 300 | 03-03414-1- γ | W | P | | 1000 | 1 | G | 052803 | N | 0 | 7 <input type="checkbox"/> |
| | MW-5 | Dioxane | 03-03414-1- δ | W | G | | 1000 | 2 | G | 052803 | N | 0 | 7 <input type="checkbox"/> |
| 2 | MW-8 | VOC | 03-03414-2- α | W | V | C | 40 | 3 | G | 052803 | N | 0 | 7 <input type="checkbox"/> |
| | MW-8 | Metal | 03-03414-2- β | W | P | N | 500 | 1 | G | 052803 | N | 0 | 7 <input type="checkbox"/> |
| | MW-8 | 300 | 03-03414-2- γ | W | P | | 1000 | 1 | G | 052803 | N | 0 | 7 <input type="checkbox"/> |
| 3 | TB-15-5/28/03 | VOC | 03-03414-3 | W | V | C | 40 | 2 | G | 052803 | N | 0 | 7 <input type="checkbox"/> |

Part 3: Analysis Information

| | | |
|-------------|--|---------------------------------|
| Test Items: | <input type="checkbox"/> 524.2 | Volatile Organic Compounds |
| | <input type="checkbox"/> 7196A | Chromium (VI) |
| | <input type="checkbox"/> 314.0/300.0 | Perchlorate, low level |
| | <input type="checkbox"/> 300.0 | Chloride Cl^- by IC |
| | <input type="checkbox"/> 300.0 | Sulfate (SO_4^{--}), by IC |
| | <input type="checkbox"/> 300.0/SM4500NO3 | Nitrate (NO_3^-) as N by IC |
| | <input type="checkbox"/> SM2320B | Carbonate |
| | <input type="checkbox"/> SM2320B | Bicarbonate |
| | <input type="checkbox"/> 9040B/150.1 | pH |
| | <input type="checkbox"/> 160.1 | Solids, Total Dissolved (TDS) |
| | <input type="checkbox"/> 200.7/6010B | Sodium, Na, by ICP |
| | <input type="checkbox"/> 200.7/6010B | Calcium, Ca, by ICP |
| | <input type="checkbox"/> 200.7/6010B | Potassium, K, by ICP |
| | <input type="checkbox"/> 200.7/6010B | Magnesium, Mg, by ICP |
| | <input type="checkbox"/> 200.7/6010B | Iron, Fe, by ICP |
| | <input type="checkbox"/> 206.2/7060A | Arsenic, As, by GFAA |
| | <input type="checkbox"/> 8270-SIM | 1,4-Dioxane |

| Seq. # | Client's Sample ID (as given on COC) | Sample Sub-ID | APCL Sample ID | Matrix | 524.2 | CHROMIUM | PERCH | CL | SO4 | NO3 | CARBON | BICARB |
|--------|--------------------------------------|---------------|----------------------|--------|-------|----------|-------|----|-----|-----|--------|--------------------------|
| 1 | MW-5 | VOC | 03-03414-1- α | W | X | | | | | | | <input type="checkbox"/> |
| | MW-5 | Metal | 03-03414-1- β | W | | | | | | | | <input type="checkbox"/> |
| | MW-5 | 300 | 03-03414-1- γ | W | | X | X | X | X | X | X | <input type="checkbox"/> |
| | MW-5 | Dioxane | 03-03414-1- δ | W | | | | | | | | <input type="checkbox"/> |

Level C Data Package Deliverables

Volatile Organics



Applied P & Ch Laboratory

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|------------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 05/29/2003 |
| Project ID: JPL | Service ID: 33414 | Collected by: |
| Sample ID: 03G2684-MB-01 | Lab Sample ID: 03G2684-MB-01 | Received Date: 05/29/2003 |
| Sample Type: Method Blank | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: G |
| Batch No: 03G2684 | Prep. Date: 05/29/03 | Anal. Date: 05/29/03 |
| Data File Name: G2684K01 | Prep. No: - | Anal. Time: 14:10 |
| Methanol Vol: - | Sample Amount: 25 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|-----|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | < 0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | < 0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | < 0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | < 0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | < 0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | < 0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | < 0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | < 0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | < 0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | < 10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | < 0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | < 0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | < 0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | < 0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | < 0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | < 0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | < 0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | < 0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 1.1 | < 1.1 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | < 0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | < 0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | < 0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | < 0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | < 0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | < 0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | < 0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | < 0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | < 0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | < 0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | < 0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | < 0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | < 0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | < 0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | < 0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | < 0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | < 0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | < 0.5 | U |
| 38 | HEXACHLOROBTADIENE | 87-68-3 | µg/L | 0.5 | < 0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | < 0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---------------------------------------|-----------|------|-----|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 1.8 | 5.9 | |
| 42 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | <10 | U |
| 43 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROBENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROBENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | Control Limit, % | Surro. Rec.% | |
|---------------------|-----------------------------|------------------|--------------|-----|
| 1 | 4-BROMO-FLUOROBENZENE (BFB) | 460-00-4 | 70-129 | 98 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 95 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 101 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 106 |
| # of out-of-control | | | 0 | |

Internal Standard

| | | Control Limit, % | IS Rec.% | |
|---------------------|-----------------------|------------------|----------|----|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 81 |
| 2 | 1,4-DICHLOROETHANE-D4 | 3855-82-1 | 50-200 | 87 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 89 |
| # of out-of-control | | | 0 | |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 05/28/2003 |
| Project ID: JPL | Service ID: 33414 | Collected by: |
| Sample ID: MW-5 | Lab Sample ID: 03-3414-1 | Received Date: 05/28/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: G |
| Batch No: 03G2684 | Prep. Date: 05/29/03 | Anal. Date: 05/29/03 |
| Data File Name: 3414-01 | Prep. No: - | Anal. Time: 16:09 |
| Methanol Vol: - | Sample Amount: 25 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|--------------------|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | < 0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | < 0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | < 0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | < 0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | < 0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | < 0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | < 0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | < 0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | < 0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | < 10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | < 0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | < 0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | < 0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | < 0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | < 0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | < 0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | < 0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | < 0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 1.1 ^(a) | < 1.1 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | < 0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | < 0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | < 0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | < 0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | < 0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | < 0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | < 0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | < 0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | < 0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | < 0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | < 0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | < 0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | < 0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | < 0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | < 0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | < 0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | < 0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | < 0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | < 0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | < 0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---|-----------|------|--------------------|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 1.8 ^(a) | <1.8 | U |
| 42 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | 5 | J |
| 43 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | | Control Limit, % | Surro. Rec.% |
|---------------------|-------------------------------------|------------|------------------|--------------|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 109 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 87 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 96 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 104 |
| # of out-of-control | | | | 0 |

Internal Standard

| | | | Control Limit, % | IS Rec.% |
|---------------------|-----------------------|-----------|------------------|----------|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 89 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 89 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 102 |
| # of out-of-control | | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

^(a) MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 05/28/2003 |
| Project ID: JPL | Service ID: 33414 | Collected by: |
| Sample ID: MW-8 | Lab Sample ID: 03-3414-2 | Received Date: 05/28/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: G |
| Batch No: 03G2684 | Prep. Date: 05/29/03 | Anal. Date: 05/29/03 |
| Data File Name: 3414-02 | Prep. No: - | Anal. Time: 16:39 |
| Methanol Vol: - | Sample Amount: 25 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|--------------------|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | <0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | <0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | <0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | <0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | <0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | <0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | <0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | <0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | <0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | <10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | <0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | <0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | <0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | <0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | <0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | <0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | <0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | <0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 1.1 ^(a) | <1.1 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | <0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | <0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | <0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | <0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | <0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | <0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | <0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | <0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | <0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | <0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | <0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | <0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | <0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | <0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | <0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | <0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | <0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | <0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | <0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | <0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---|-----------|------|--------------------|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 1.8 ^(a) | 3.7 | B |
| 42 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | 5 | J |
| 43 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | | Control Limit, % | Surro. Rec.% |
|---------------------|-------------------------------------|------------|------------------|--------------|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 102 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 86 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 97 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 103 |
| # of out-of-control | | | | 0 |

Internal Standard

| | | | Control Limit, % | IS Rec.% |
|---------------------|-----------------------|-----------|------------------|----------|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 93 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 96 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 104 |
| # of out-of-control | | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

(a) MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

| | | |
|---------------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 05/28/2003 |
| Project ID: JPL | Service ID: 33414 | Collected by: |
| Sample ID: TB-15-5/28/03 | Lab Sample ID: 03-3414-3 | Received Date: 05/28/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: |
| Anal. Method: 524.2 | Prep. Method: 5030 | Instrument ID: GC/MS: G |
| Batch No: 03G2684 | Prep. Date: 05/29/03 | Anal. Date: 05/29/03 |
| Data File Name: 3414-03 | Prep. No: - | Anal. Time: 17:09 |
| Methanol Vol. - | Sample Amount: 25 mL | Dilution Factor: 1 |
| Test Level: Low | Sparge Size: 25 mL | Heated Purge: (Y/N) N |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|-----------------------------|------------|------|--------------------|--------|-----------|
| 1 | BENZENE | 71-43-2 | µg/L | 0.5 | < 0.5 | U |
| 2 | BROMOBENZENE | 108-86-1 | µg/L | 0.5 | < 0.5 | U |
| 3 | BROMOCHLOROMETHANE | 74-97-5 | µg/L | 0.5 | < 0.5 | U |
| 4 | BROMODICHLOROMETHANE | 75-27-4 | µg/L | 0.5 | < 0.5 | U |
| 5 | BROMOFORM | 75-25-2 | µg/L | 0.5 | < 0.5 | U |
| 6 | BROMOMETHANE | 74-83-9 | µg/L | 0.5 | < 0.5 | U |
| 7 | N-BUTYLBENZENE | 104-51-8 | µg/L | 0.5 | < 0.5 | U |
| 8 | SEC-BUTYLBENZENE | 135-98-8 | µg/L | 0.5 | < 0.5 | U |
| 9 | TERT-BUTYLBENZENE | 98-06-6 | µg/L | 0.5 | < 0.5 | U |
| 10 | 2-BUTANONE | 78-93-3 | µg/L | 10 | < 10 | U |
| 11 | CARBON TETRACHLORIDE | 56-23-5 | µg/L | 0.5 | < 0.5 | U |
| 12 | CHLOROBENZENE | 108-90-7 | µg/L | 0.5 | < 0.5 | U |
| 13 | CHLORODIBROMOMETHANE | 124-48-1 | µg/L | 0.5 | < 0.5 | U |
| 14 | CHLOROETHANE | 75-00-3 | µg/L | 0.5 | < 0.5 | U |
| 15 | CHLOROFORM | 67-66-3 | µg/L | 0.5 | < 0.5 | U |
| 16 | CHLOROMETHANE | 74-87-3 | µg/L | 0.5 | < 0.5 | U |
| 17 | 2-CHLOROTOLUENE | 95-49-8 | µg/L | 0.5 | < 0.5 | U |
| 18 | 4-CHLOROTOLUENE | 106-43-4 | µg/L | 0.5 | < 0.5 | U |
| 19 | 1,2-DIBROMO-3-CHLOROPROPANE | 96-12-8 | µg/L | 1.1 ^(a) | < 1.1 | U |
| 20 | 1,2-DIBROMOETHANE (EDB) | 106-93-4 | µg/L | 0.5 | < 0.5 | U |
| 21 | DIBROMOMETHANE | 74-95-3 | µg/L | 0.5 | < 0.5 | U |
| 22 | 1,2-DICHLOROBENZENE | 95-50-1 | µg/L | 0.5 | < 0.5 | U |
| 23 | 1,3-DICHLOROBENZENE | 541-73-1 | µg/L | 0.5 | < 0.5 | U |
| 24 | 1,4-DICHLOROBENZENE | 106-46-7 | µg/L | 0.5 | < 0.5 | U |
| 25 | DICHLORODIFLUOROMETHANE | 75-71-8 | µg/L | 0.5 | < 0.5 | U |
| 26 | 1,1-DICHLOROETHANE | 75-34-3 | µg/L | 0.5 | < 0.5 | U |
| 27 | 1,2-DICHLOROETHANE | 107-06-2 | µg/L | 0.5 | < 0.5 | U |
| 28 | 1,1-DICHLOROETHENE | 75-35-4 | µg/L | 0.5 | < 0.5 | U |
| 29 | CIS-1,2-DICHLOROETHENE | 156-59-2 | µg/L | 0.5 | < 0.5 | U |
| 30 | TRANS-1,2-DICHLOROETHENE | 156-60-5 | µg/L | 0.5 | < 0.5 | U |
| 31 | 1,2-DICHLOROPROPANE | 78-87-5 | µg/L | 0.5 | < 0.5 | U |
| 32 | 1,3-DICHLOROPROPANE | 142-28-9 | µg/L | 0.5 | < 0.5 | U |
| 33 | 2,2-DICHLOROPROPANE | 594-20-7 | µg/L | 0.5 | < 0.5 | U |
| 34 | 1,1-DICHLOROPROPENE | 563-58-6 | µg/L | 0.5 | < 0.5 | U |
| 35 | CIS-1,3-DICHLOROPROPENE | 10061-01-5 | µg/L | 0.5 | < 0.5 | U |
| 36 | TRANS-1,3-DICHLOROPROPENE | 10061-02-6 | µg/L | 0.5 | < 0.5 | U |
| 37 | ETHYLBENZENE | 100-41-4 | µg/L | 0.5 | < 0.5 | U |
| 38 | HEXACHLOROBUTADIENE | 87-68-3 | µg/L | 0.5 | < 0.5 | U |
| 39 | ISOPROPYLBENZENE (CUMENE) | 98-82-8 | µg/L | 0.5 | < 0.5 | U |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----|---|-----------|------|--------------------|--------|-----------|
| 40 | P-ISOPROPYLTOLUENE | 99-87-6 | µg/L | 0.5 | <0.5 | U |
| 41 | METHYLENE CHLORIDE | 75-09-2 | µg/L | 1.8 ^(a) | 3.8 | B |
| 42 | 4-METHYL-2-PENTANONE (MIBK) | 108-10-1 | µg/L | 10 | 5 | J |
| 43 | METHYL-T-BUTYL ETHER (MTBE) | 1634-04-4 | µg/L | 1 | <1 | U |
| 44 | NAPHTHALENE | 91-20-3 | µg/L | 0.5 | <0.5 | U |
| 45 | N-PROPYLBENZENE | 103-65-1 | µg/L | 0.5 | <0.5 | U |
| 46 | STYRENE | 100-42-5 | µg/L | 0.5 | <0.5 | U |
| 47 | 1,1,1,2-TETRACHLOROETHANE | 630-20-6 | µg/L | 0.5 | <0.5 | U |
| 48 | 1,1,2,2-TETRACHLOROETHANE | 79-34-5 | µg/L | 0.5 | <0.5 | U |
| 49 | TETRACHLOROETHENE | 127-18-4 | µg/L | 0.5 | <0.5 | U |
| 50 | TOLUENE | 108-88-3 | µg/L | 0.5 | <0.5 | U |
| 51 | 1,2,3-TRICHLOROENZENE | 87-61-6 | µg/L | 0.5 | <0.5 | U |
| 52 | 1,2,4-TRICHLOROENZENE | 120-82-1 | µg/L | 0.5 | <0.5 | U |
| 53 | 1,1,1-TRICHLOROETHANE | 71-55-6 | µg/L | 0.5 | <0.5 | U |
| 54 | 1,1,2-TRICHLOROETHANE | 79-00-5 | µg/L | 0.5 | <0.5 | U |
| 55 | TRICHLOROETHENE | 79-01-6 | µg/L | 0.5 | <0.5 | U |
| 56 | TRICHLOROFLUOROMETHANE | 75-69-4 | µg/L | 0.5 | <0.5 | U |
| 57 | 1,2,3-TRICHLOROPROPANE | 96-18-4 | µg/L | 0.5 | <0.5 | U |
| 58 | 1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE | 76-13-1 | µg/L | 0.5 | <0.5 | U |
| 59 | 1,2,4-TRIMETHYLBENZENE | 95-63-6 | µg/L | 0.5 | <0.5 | U |
| 60 | 1,3,5-TRIMETHYLBENZENE | 108-67-8 | µg/L | 0.5 | <0.5 | U |
| 61 | VINYL CHLORIDE | 75-01-4 | µg/L | 0.5 | <0.5 | U |
| 62 | O-XYLENE | 95-47-6 | µg/L | 0.5 | <0.5 | U |
| 63 | M/P-XYLENE | 108-38-3 | µg/L | 0.5 | <0.5 | U |

Surrogates

| | | | Control Limit, % | Surro. Rec.% |
|---------------------|-------------------------------------|------------|------------------|--------------|
| 1 | 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) | 460-00-4 | 70-129 | 96 |
| 2 | 1,2-DICHLOROETHANE-D4 | 17060-07-0 | 70-129 | 84 |
| 3 | DIBROMOFLUOROMETHANE | 1868-53-7 | 70-122 | 92 |
| 4 | TOLUENE-D8 | 2037-26-5 | 73-129 | 99 |
| # of out-of-control | | | | 0 |

Internal Standard

| | | | Control Limit, % | IS Rec.% |
|---------------------|-----------------------|-----------|------------------|----------|
| 1 | CHLOROBENZENE-D5 | 3114-55-4 | 50-200 | 98 |
| 2 | 1,4-DICHLOROENZENE-D4 | 3855-82-1 | 50-200 | 103 |
| 3 | FLUOROBENZENE | 462-06-6 | 50-200 | 107 |
| # of out-of-control | | | | 0 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

^(a) MDL reported.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

FORM-2C

Applied P & Ch Laboratory

Surrogate Recovery Summary for Method 524.2

Client Name: GEOFON, Inc.
 Case No:
 Project ID: JPL

Contract No:
 SAS No:
 Project No: 04-4428.10
 Batch No: 03G2684

Lab Code: APCL
 SDG Number: 033414
 Sample Matrix: Water

| # | Client Sample No | Lab Sample ID | S1 % # | S2 % # | S3 % # | S4 % # | TOT OUT |
|----|------------------|----------------|--------|--------|--------|--------|---------|
| 1 | 03G2684-LCS-01 | 03G2684-LCS-01 | 89 | 103 | 102 | 100 | 0 |
| 2 | MW-5MS | 03-3414-1MS | 105 | 116 | 110 | 108 | 0 |
| 3 | MW-5MSD | 03-3414-1MSD | 108 | 110 | 108 | 107 | 0 |
| 4 | 03G2684-MB-01 | 03G2684-MB-01 | 98 | 95 | 101 | 106 | 0 |
| 5 | MW-5 | 03-3414-1 | 109 | 87 | 96 | 104 | 0 |
| 6 | MW-8 | 03-3414-2 | 102 | 86 | 97 | 103 | 0 |
| 7 | TB-15-5/28/03 | 03-3414-3 | 96 | 84 | 92 | 99 | 0 |
| 8 | | | | | | | |
| 9 | | | | | | | |
| 10 | | | | | | | |
| 11 | | | | | | | |
| 12 | | | | | | | |
| 13 | | | | | | | |
| 14 | | | | | | | |
| 15 | | | | | | | |
| 16 | | | | | | | |
| 17 | | | | | | | |
| 18 | | | | | | | |
| 19 | | | | | | | |
| 20 | | | | | | | |
| 21 | | | | | | | |
| 22 | | | | | | | |
| 23 | | | | | | | |
| 24 | | | | | | | |
| 25 | | | | | | | |

QC Control Limit

S1 = 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) 70-129
 S2 = 1,2-DICHLOROETHANE-D4 70-129
 S3 = DIBROMOFLUOROMETHANE 70-122
 S4 = TOLUENE-D8 73-129

Column to be used to flag recovery values:

* - Values outside of contract required QC Limits D - Surrogate diluted out I - Matrix Interference

FORM-3A

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 524.2

| | | |
|---------------------------|------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03G2684 | |
| LCS Filename: G2684L01 | Date Analyzed: 052903 | Time Analyzed: 11:16 |
| LCSID Filename: - | Date Analyzed: - | Time Analyzed: - |

| Spiked Components | Unit | Spike Added | Concentration | | LCS Rec% # | QC Limit % REC |
|---------------------|------|-------------|---------------|------|------------|----------------|
| | | | Unspiked | LCS | | |
| BENZENE | µg/L | 20 | 0 | 19.6 | 98 | 65-120 |
| CHLOROBENZENE | µg/L | 20 | 0 | 19.6 | 98 | 65-134 |
| 1,1-DICHLOROETHENE | µg/L | 20 | 0 | 18.2 | 91 | 65-127 |
| TOLUENE | µg/L | 20 | 0 | 18.8 | 94 | 65-134 |
| TRICHLOROETHENE | µg/L | 20 | 0 | 18.9 | 95 | 67-122 |
| # of Out-of-control | | | | | 0 | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-3A

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 524.2

| | | |
|---------------------------|--------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03G2684 | |
| MS Filename: G2684M01 | Date Analyzed: 052903 | Time Analyzed: 11:44 |
| MSD Filename: G2684N01 | Date Analyzed: 052903 | Time Analyzed: 12:43 |
| MS Sample No: MW-5 | Sample Lab ID: 03-3414-1 | |

| Spiked Components | Unit | Spike Added | Concentration | | MS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|------|-----------|-----------------|
| | | | Unspiked | MS | | |
| BENZENE | µg/L | 20 | 0 | 21.4 | 107 | 65-121 |
| CHLOROBENZENE | µg/L | 20 | 0 | 22.5 | 113 | 65-134 |
| 1,1-DICHLOROETHENE | µg/L | 20 | 0 | 21.1 | 106 | 65-127 |
| TOLUENE | µg/L | 20 | 0 | 21.1 | 106 | 65-134 |
| TRICHLOROETHENE | µg/L | 20 | 0 | 21.3 | 107 | 65-125 |
| # of Out-of-control | | | | | 0 | |

| Spiked Components | Unit | Spike Added | MSD Concentration | MSD Rec% # | RPD% # | QC Limit, % | |
|---------------------|------|-------------|-------------------|------------|--------|-------------|--------|
| | | | | | | RPD | REC |
| BENZENE | µg/L | 20 | 20.8 | 104 | 3 | 28 | 65-121 |
| CHLOROBENZENE | µg/L | 20 | 22.3 | 112 | 1 | 35 | 65-134 |
| 1,1-DICHLOROETHENE | µg/L | 20 | 20.3 | 102 | 4 | 31 | 65-127 |
| TOLUENE | µg/L | 20 | 20.7 | 104 | 2 | 35 | 65-134 |
| TRICHLOROETHENE | µg/L | 20 | 21.3 | 107 | 0 | 30 | 65-125 |
| # of Out-of-control | | | | 0 | 0 | | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-4A

Applied P & Ch Laboratory

Method Blank Summary for Method 524.2


| | | |
|------------------------------|--------------------------|-------------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Analysis Date: 05/29/03 |
| Sample ID: 03G2684-MB-01 | Sample Matrix: Water | Analysis Time: 14:10 |
| Lab Sample ID: 03G2684-MB-01 | Batch No: 03G2684 | Instrument ID: GC/MS: G |
| | Data File Name: G2684K01 | GC Column: DB-VEX |
| | Heated Purge: (Y/N) N | Column ID: 0.45 mm |

This Method Blank applies to the following samples and QC samples:

| # | Client Sample No | Lab Sample ID | Sample Type | Data Filename | Analysis Date | Analysis Time |
|----|------------------|----------------|------------------------|---------------|---------------|---------------|
| 1 | 03G2684-LCS-01 | 03G2684-LCS-01 | Lab Control Spike | G2684L01 | 05/29/03 | 11:16 |
| 2 | MW-5MS | 03-3414-1MS | Matrix Spike | G2684M01 | 05/29/03 | 11:44 |
| 3 | MW-5MSD | 03-3414-1MSD | Matrix Spike Duplicate | G2684N01 | 05/29/03 | 12:43 |
| 4 | MW-5 | 03-3414-1 | Field Sample | 3414-01 | 05/29/03 | 16:09 |
| 5 | MW-8 | 03-3414-2 | Field Sample | 3414-02 | 05/29/03 | 16:39 |
| 6 | TB-15-5/28/03 | 03-3414-3 | Field Sample | 3414-03 | 05/29/03 | 17:09 |
| 7 | | | | | | |
| 8 | | | | | | |
| 9 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |
| 26 | | | | | | |
| 27 | | | | | | |
| 28 | | | | | | |

Data File : C:\HPCHEM\1\DATA\03G2404\G2404P01.D Vial: 18
 Acq On : 15 May 03 10:18 am Operator: Eddie
 Sample : ##03g2404, w Inst : GCMS-G
 Misc : Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P & Ch Lab** EPA 524.2



Peak Apex is scan: 1388

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result |
|-------------|--------------|--------------|--------------|-----------|---------|--------|
| 50 | 95 | 15 | 40 | 16.7 | 17208 | PASS |
| 75 | 95 | 30 | 60 | 43.0 | 44184 | PASS |
| 95 | 95 | 100 | 100 | 100.0 | 102784 | PASS |
| 96 | 95 | 5 | 9 | 6.1 | 6301 | PASS |
| 173 | 174 | 0 | 2 | 0.0 | 0 | PASS |
| 174 | 95 | 50 | 100 | 84.8 | 87112 | PASS |
| 175 | 174 | 5 | 9 | 7.7 | 6735 | PASS |
| 176 | 174 | 95 | 101 | 97.9 | 85240 | PASS |
| 177 | 176 | 5 | 9 | 6.8 | 5764 | PASS |

5A
VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name : APPLIED P & CH LAB Contract: _____
 Lab Code: _____ Case No.: _____ SAS No.: _____ SDG No.: 033414
 Lab File ID: G2404 P01 BFB Injection Date: 05/15/2003
 Instrument ID: GCMS-G BFB Injection Time: 1018
 GC Column: VOCOL ID: 0.32 (mm) Heated Purge: (Y/N) N

| m/e | ION ABUNDANCE CRITERIA | %RELATIVE ABUNDANCE |
|-----|------------------------------------|---------------------|
| 50 | 15.0 - 40.0% of mass 95 | 16.7 |
| 75 | 30.0 - 60.0% of mass 95 | 43.0 |
| 95 | Base peak, 100% relative abundance | 100.0 |
| 96 | 5.0 - 9.0% of mass 95 | 6.1 |
| 173 | Less than 2.0% of mass 174 | 0.0 (0.0)1 |
| 174 | 50.0 - 100.0% of mass 95 | 84.8 |
| 175 | 5.0 - 9.0% of mass 174 | 6.6 (7.7)1 |
| 176 | 95.0 - 101.0% of mass 174 | 82.9 (97.9)1 |
| 177 | 5.0 - 9.0% of mass 176 | 5.6 (6.8)2 |

1-Value is % mass 174

2-Value is % mass 176

This check applies to the following SAMPLES, MS, MSD, BLANKS and STANDARDS:

| | EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|----------------|---------------|-------------|---------------|---------------|
| 01 | VSTD003 | 004-003 | 004-0003.D | 05/15/03 | 1047 |
| 02 | VSTD002 | 004-002 | 004-0002.D | 05/15/03 | 1145 |
| 03 | VSTD010 | 004-0010 | 004-0010.D | 05/15/03 | 1214 |
| 04 | VSTD020 | 004-0020 | 004-0020.D | 05/15/03 | 1243 |
| 05 | VSTD040 | 004-0040 | 004-0040.D | 05/15/03 | 1312 |
| 06 | VSTD080 | 004-0080 | 004-0080.D | 05/15/03 | 1341 |
| 07 | | | | | |
| 08 | | | | | |
| 09 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

INITIAL CALIBRATION SUMMARY

Method File E524G004
 Last Calibration Update Fri May 16 10:36:26 2003

| Level 1 File Name | Level 2 File Name | Level 3 File Name | Level 4 File Name | Level 5 File Name | Level 6 File Name | Level 7 File Name | Level 1 ID | Level 2 ID | Level 3 ID | Level 4 ID | Level 5 ID | Level 6 ID | Level 7 ID |
|-------------------|-------------------|-------------------|-------------------|-------------------|-------------------|-------------------|------------|------------|------------|------------|------------|------------|------------|
| 4-003.D | 4-002.D | 4-010.D | 4-020.D | 4-040.D | 4-080.D | 4-020.D | 0.3 | 2 | 10 | 20 | 40 | 80 | CC |

| Compound Name | Level 1 Response | Level 2 Response | Level 3 Response | Level 4 Response | Level 5 Response | Level 6 Response | Level 7 Response | Coef X ^{v0} | Coef X ^{v1} / ave RF | Coef X ^{v2} | R ^{v2} / RSD |
|-----------------------------|------------------|------------------|------------------|------------------|------------------|------------------|------------------|----------------------|-------------------------------|----------------------|-----------------------|
| 1 Fluorobenzene l1 1 | 815158 | 799651 | 824804 | 746757 | 764394 | 689688 | -1 | ----- | ----- | ----- | ----- |
| 3 di-Cl-di-F-methane 85 87 | 4181 | 35493 | 168476 | 314256 | 706635 | 1288384 | -1 | 0.0000 | 0.2120 | 0.0000 | 0.1090 |
| 4 Chloromethane 50 52 | 1706 | 19850 | 102587 | 246113 | 534218 | 1069891 | -1 | -0.0408 | 0.1954 | 0.0000 | 0.9966 |
| 9 F114 85 135 | 4199 | 44804 | 220942 | 386132 | 819274 | 1556249 | -1 | -0.0188 | 0.2815 | 0.0000 | 0.9991 |
| 5 vinyl chloride 62 64 | 3355 | 33999 | 162051 | 300841 | 621901 | 1167862 | -1 | 0.0000 | 0.1938 | 0.0000 | 0.1466 |
| 6 bromomethane 94 96 | 4372 | 26980 | 129267 | 267214 | 519945 | 1000442 | -1 | 0.0000 | 0.1724 | 0.0000 | 0.0536 |
| 7 Chloroethane 64 66 | 3179 | 26106 | 123679 | 236431 | 478026 | 873637 | -1 | 0.0000 | 0.1527 | 0.0000 | 0.0781 |
| 8 tri-Cl-F-methane 101 103 | 8951 | 64415 | 295972 | 594414 | 1265977 | 2395096 | -1 | 0.0000 | 0.3956 | 0.0000 | 0.0724 |
| 111 isopropyl alcohol x10 | 3587 | 6299 | 29925 | 70395 | 1111196 | 226721 | -1 | 0.0000 | 0.0040 | 0.0000 | 0.1113 |
| 100 ethyl ether x5 | 26492 | 132391 | 571623 | 1090032 | 2124645 | 3947698 | -1 | 0.0028 | 0.1423 | 0.0000 | 0.9997 |
| 102 Acrolein x10 | 1454 | 15421 | 124387 | 164659 | 294058 | 649263 | -1 | -0.0048 | 0.0115 | 0.0000 | 0.9858 |
| 119 methyl acetate | 7468 | 34881 | 93789 | 329077 | 525452 | 898426 | -1 | 0.0239 | 0.1624 | 0.0000 | 0.9860 |
| 104 Carbon disulfide | 15360 | 108670 | 470593 | 924294 | 1876377 | 3448920 | -1 | 0.0000 | 0.6226 | 0.0000 | 0.0560 |
| 103 Acrylonitrile x10 | 4460 | 38141 | 123788 | 403095 | 766254 | 1455017 | -1 | 0.0000 | 0.0268 | 0.0000 | 0.9965 |
| 95 Acetone x10 | 18003 | 42021 | 146218 | 266351 | 522927 | 928171 | -1 | 0.0183 | 0.0166 | 0.0000 | 0.9999 |
| 108 F-113 | 7993 | 56604 | 258951 | 515229 | 1098171 | 2025833 | -1 | 0.0000 | 0.3443 | 0.0000 | 0.0590 |
| 13 11-dichloroethene 61 96 | 8587 | 60316 | 284348 | 535921 | 1112083 | 2068506 | -1 | 0.0000 | 0.3617 | 0.0000 | 0.0355 |
| 101 Acetonitrile x10 | 2831 | 10077 | 31282 | 102405 | 196047 | 363830 | -1 | -0.0063 | 0.0067 | 0.0000 | 0.9966 |
| 109 Iodomethane | 6929 | 75147 | 336586 | 628909 | 1205092 | 2300947 | -1 | -0.0067 | 0.4140 | 0.0000 | 0.9991 |
| 113 Tert butyl alcohol x10 | 1373 | 18588 | 77974 | 138129 | 265783 | 388696 | -1 | 0.0000 | 0.0092 | 0.0000 | 0.1787 |
| 18 methylene chloride 49 84 | -1 | 48402 | 184549 | 355095 | 696481 | 1289109 | -1 | 0.0000 | 0.2451 | 0.0000 | 0.1330 |

| | | | | | | | | | | | | |
|-------------------------------|-----------------|-----------------|-----------------|-----------------|-----------------|-----------------|-----------------|-------------|---------------------|-------------|-------------|--------|
| 112 Allyl chloride | 13441 | 77142 | 331252 | 615063 | 1148799 | 1977528 | -1 | 0.0468 | 0.3564 | 0.0000 | 0.9986 | |
| 200 Nitro methane x10 | 6304 | 66437 | 325452 | 650702 | 1254351 | 2397871 | -1 | 0.0000 | 0.0391 | 0.0000 | 0.1719 | |
| 10 t-Bu-Me-ether | 73 57 | 91189 | 366763 | 722425 | 1502372 | 2824413 | -1 | 0.0000 | 0.4955 | 0.0000 | 0.0864 | |
| 19 t-12-di-Cl-ethene | 96 61 | 5258 | 44435 | 215839 | 423127 | 799696 | -1 | 0.0000 | 0.2634 | 0.0000 | 0.0869 | |
| 98 Vinyl acetate x5 | 3645 | 167151 | 292003 | 1342007 | 2982123 | 5784036 | -1 | -0.2666 | 0.2134 | 0.0000 | 0.9933 | |
| 21 11-dichloroethane | 63 83 | 11126 | 88915 | 412703 | 833014 | 1647004 | -1 | 0.0000 | 0.5252 | 0.0000 | 0.0765 | |
| 91 2-butanolone MEKx10 | 25733 | 153111 | 642126 | 1432839 | 2827847 | 5285771 | -1 | 0.0000 | 0.0938 | 0.0000 | 0.0952 | |
| 115 Diisoprop ether | 40820 | 232542 | 1079994 | 2060781 | 4081017 | 7613956 | -1 | 0.0000 | 1.4212 | 0.0000 | 0.0923 | |
| 22 c-12-di-Cl-ethene | 96 61 | 6716 | 44823 | 222557 | 432230 | 852613 | -1 | 0.0000 | 0.2812 | 0.0000 | 0.0324 | |
| 23 22-Dichloropropane | 77 97 | 11379 | 71432 | 324674 | 629042 | 1268689 | -1 | 0.0000 | 0.4280 | 0.0000 | 0.0585 | |
| 24 Br-Cl-methane | 128 130 | 619 | 19664 | 94361 | 180264 | 365219 | -1 | -0.0056 | 0.1234 | 0.0000 | 0.9997 | |
| 25 chloroform | 83 85 | 15134 | 81585 | 381866 | 741343 | 1478585 | -1 | 0.0000 | 0.5124 | 0.0000 | 0.1068 | |
| 201 Ethyl acetate x2 | 2846 | 46100 | 136924 | 355515 | 703484 | 2772452 | -1 | -0.0563 | 0.1306 | 0.0000 | 0.9958 | |
| 116 ETBE | 33538 | 144136 | 644550 | 1245123 | 2437411 | 4486393 | -1 | 0.0049 | 0.8099 | 0.0000 | 0.9998 | |
| 117 Iso-butyl alcohol X10 | 940 | 62706 | 135151 | 357401 | 710558 | 1430613 | -1 | -0.0353 | 0.0259 | 0.0000 | 0.9953 | |
| 26 tetrahydrofuranx5 | 257 | 8307 | 43847 | 84254 | 161549 | 290888 | -1 | 0.0000 | 0.0107 | 0.0000 | 0.0325 | |
| 27 Di-Br-F-Methane (S1) | 111 1 | 8284 | 60816 | 289627 | 568312 | 1126216 | -1 | 0.0000 | 0.3713 | 0.0000 | 0.0331 | |
| 34 111-tri-Cl-ethane | 97 99 | 8942 | 65770 | 311389 | 599971 | 1237882 | -1 | 0.0000 | 0.3993 | 0.0000 | 0.0616 | |
| 30 12-dichloroethane | 64 62 | 1802 | 33229 | 153871 | 310815 | 631494 | -1 | -0.0194 | 0.2197 | 0.0000 | 0.9990 | |
| 35 11-Di-Cl-propene | 75 110 | 8689 | 58001 | 275836 | 532605 | 1078521 | -1 | 0.0000 | 0.3543 | 0.0000 | 0.0301 | |
| 29 1,2-di-Cl-ethane-d4 [Surf] | 10 | 4884 | 26465 | 134448 | 261823 | 505671 | -1 | 0.0000 | 0.1688 | 0.0000 | 0.0341 | |
| 36 benzene | 78 52 | 20191 | 142907 | 668867 | 1302042 | 2578473 | -1 | 0.0000 | 0.8512 | 0.0000 | 0.0359 | |
| 37 CCl4 | 117 119 | 8483 | 58348 | 273728 | 543038 | 1134691 | -1 | 0.0000 | 0.3590 | 0.0000 | 0.0461 | |
| 97 thiophene | 9443 | 75171 | 331986 | 649163 | 1291816 | 2373848 | -1 | 0.0000 | 0.4243 | 0.0000 | 0.0680 | |
| 118 TAME | 2423 | 114119 | 445234 | 894867 | 1715454 | 3200762 | -1 | -0.0058 | 0.5780 | 0.0000 | 0.9994 | |
| 39 12-di-Cl-propane | 63 76 | 5331 | 41840 | 206799 | 390600 | 777542 | -1 | 0.0000 | 0.2514 | 0.0000 | 0.0677 | |
| 40 trichloroethene | 130 132 | 7533 | 51222 | 233771 | 454200 | 926225 | -1 | 0.0000 | 0.3044 | 0.0000 | 0.0393 | |
| 96 Me-methacrylate | 1437 | 15341 | 47596 | 161499 | 295494 | 591170 | -1 | -0.0168 | 0.1076 | 0.0000 | 0.9949 | |
| 42 Br-di-Cl-methane | 83 85 | 12659 | 54887 | 257854 | 508851 | 988624 | -1 | -0.0042 | 0.3328 | 0.0000 | 0.9996 | |
| 41 dibromomethane | 174 172 | 618 | 19288 | 93298 | 195812 | 390733 | -1 | -0.0102 | 0.1342 | 0.0000 | 0.9994 | |
| Compound | Level 1 | Level 2 | Level 3 | Level 4 | Level 5 | Level 6 | Level 7 | Coef | Coef | Coef | Rv2/ | |
| Name | Response | Response | Response | Response | Response | Response | Response | X^0 | X^1 / ave RF | X^2 | RSD | |
| 45 c-13-di-Cl-propene | 75 110 | 7615 | 48884 | 239463 | 477602 | 948616 | 1759634 | -1 | 0.0000 | 0.5038 | 0.0000 | 0.0376 |
| 55 toluene-d8(S2) | 100 99 | 13666 | 83281 | 390496 | 768293 | 1521774 | 2828221 | -1 | 0.0000 | 0.0259 | 0.0000 | 0.0904 |
| 92 2-ClEt-VI-ether10 | 5311 | 41678 | 205749 | 413282 | 830636 | 1543091 | -1 | 0.0000 | 0.8174 | 0.0000 | 0.1033 | |
| 56 toluene | 91 92 | 24063 | 127484 | 612856 | 1179183 | 2400670 | 4445368 | -1 | 0.0000 | 0.0000 | 0.0000 | 0.1033 |

| | | | | | | | | | | | |
|-----------------------|---------|--------|--------|--------|--------|---------|----|---------|--------|--------|--------|
| 107 Et methacrylate | 3479 | 23955 | 53825 | 215372 | 441923 | 820108 | -1 | -0.0241 | 0.1510 | 0.0000 | 0.9952 |
| 93 2-Hexanone x5 | 1510 | 42848 | 144809 | 430950 | 860345 | 1584358 | -1 | -0.0326 | 0.0581 | 0.0000 | 0.9977 |
| 48 112-tri-Cl-Et | 97 83 | 906 | 19429 | 109523 | 367637 | 694437 | -1 | -0.0023 | 0.1252 | 0.0000 | 0.9994 |
| 58 1,2-di-br-ethane | 107 109 | 1824 | 20769 | 99010 | 395372 | 752280 | -1 | -0.0087 | 0.1362 | 0.0000 | 0.9993 |
| 51 di-Br-Cl-methane | 129 127 | 7347 | 33435 | 155803 | 605212 | 1437349 | -1 | -0.0082 | 0.2056 | 0.0000 | 0.9995 |
| 46 t-13-di-cl-propene | 75 110 | 7615 | 48884 | 239463 | 948616 | 1759634 | -1 | 0.0000 | 0.3094 | 0.0000 | 0.0348 |
| 105 1-Chlorohexane | | 11922 | 55414 | 207900 | 393247 | 824539 | -1 | -0.0003 | 0.2692 | 0.0000 | 0.9998 |
| 47 Cl-benzene-d5, 12 | | 231880 | 227963 | 249245 | 222899 | 243736 | -1 | 0.0000 | 1.0000 | 0.0000 | 0.0000 |
| 54 MIBK | | 4406 | 1842 | 61603 | 163289 | 585241 | -1 | 0.0022 | 0.3172 | 0.0000 | 0.9942 |
| 49 1,3-di-cl-propane | 76 78 | 5042 | 34635 | 178128 | 648825 | 1196619 | -1 | 0.0000 | 0.7083 | 0.0000 | 0.0687 |
| 59 tetra-Cl-ethene | 166 168 | 5645 | 43932 | 206527 | 398332 | 812967 | -1 | 0.0000 | 0.8560 | 0.0000 | 0.0716 |

| Compound | Level 1 | | Level 2 | | Level 3 | | Level 4 | | Level 5 | | Level 6 | | Level 7 | | Coeff X^0 | Coeff X^1 / ave RF | Coeff X^2 | R^2 / RSD |
|-----------------------------|------------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|--|--------------|-----------------------|--------------|--------------|
| | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | Response | | | | | |
| 60 chlorobenzene | 112 77 | 11129 | 80876 | 394322 | 752942 | 1478617 | 2729365 | -1 | 0.0000 | 0.7212 | 0.0000 | 0.0707 | | | | | | |
| 61 1112-tetra-Cl-Et | 131 133 | 4438 | 35454 | 177813 | 344569 | 695345 | 1340863 | -1 | 0.0000 | 0.7212 | 0.0000 | 0.0707 | | | | | | |
| 64 ethylbenzene | 91 106 | 21645 | 144618 | 668986 | 1270086 | 2566878 | 4842788 | -1 | 0.0000 | 2.8368 | 0.0000 | 0.0896 | | | | | | |
| 65 m/p-Xylenes x2 | | 30844 | 222047 | 1015495 | 1972002 | 3905278 | 7205695 | -1 | 0.0000 | 2.1361 | 0.0000 | 0.0886 | | | | | | |
| 99 1-4-di-Cl-butane | | 6740 | 36572 | 153006 | 301374 | 572112 | 1066373 | -1 | 0.0798 | 0.5616 | 0.0000 | 0.9979 | | | | | | |
| 52 bromoform | 173 175 | 2520 | 15462 | 69675 | 136091 | 278788 | 522738 | -1 | 0.0000 | 0.3083 | 0.0000 | 0.1137 | | | | | | |
| 66 styrene | 104 78 | 15564 | 84384 | 382712 | 759242 | 1511886 | 2814241 | -1 | 0.1396 | 1.4904 | 0.0000 | 0.9987 | | | | | | |
| 67 o-xylene | 91 106 | 15170 | 107821 | 489526 | 954644 | 1857499 | 3377446 | -1 | 0.0000 | 2.0583 | 0.0000 | 0.1015 | | | | | | |
| 68 1122-Tetra-Cl-Et | 83 85 | 2369 | 17006 | 81453 | 170717 | 330326 | 601304 | -1 | 0.0000 | 0.3469 | 0.0000 | 0.0735 | | | | | | |
| 110 t-1,4-dichloro-2-butene | | 598 | 5155 | 17689 | 36488 | 58046 | 107382 | -1 | 0.0000 | 0.0781 | 0.0000 | 0.2649 | | | | | | |
| 106 Cl-benzyl | | 1709 | 34984 | 130453 | 246745 | 493146 | 894786 | -1 | 0.0686 | 0.4730 | 0.0000 | 0.9980 | | | | | | |
| 62 1,4-DCB-d4 | 150 152 13 | 220209 | 211064 | 218269 | 198057 | 195846 | 179706 | -1 | 0.0000 | 1.0000 | 0.0000 | 0.0000 | | | | | | |
| 69 123-tri-Cl-Pr | 110 97 | 247 | 4417 | 25007 | 46613 | 92169 | 179941 | -1 | 0.0000 | 0.1159 | 0.0000 | 0.0641 | | | | | | |
| 70 4-Br-1-F-Bz (S3) | 174 95 | 7551 | 36349 | 170967 | 334015 | 639559 | 1173651 | -1 | 0.0000 | 0.8241 | 0.0000 | 0.0360 | | | | | | |
| 71 isopropylbenzene | 105 120 | 20338 | 154289 | 681700 | 1327629 | 2705126 | 5006864 | -1 | 0.0000 | 3.3574 | 0.0000 | 0.0661 | | | | | | |
| 72 bromobenzene | 156 158 | 3634 | 32102 | 153148 | 304357 | 590583 | 1107164 | -1 | 0.0000 | 0.7174 | 0.0000 | 0.1196 | | | | | | |
| 73 n-propylbenzene | 120 78 | 5459 | 46356 | 210844 | 394872 | 801684 | 1463801 | -1 | 0.0000 | 0.9881 | 0.0000 | 0.0916 | | | | | | |
| 74 2-Cl-Tl | 126 128 | 3366 | 25894 | 120864 | 249899 | 481903 | 908178 | -1 | 0.0000 | 0.5924 | 0.0000 | 0.0839 | | | | | | |
| 75 4-Cl-Tl | 126 128 | 4268 | 41895 | 196931 | 372201 | 722805 | 1334882 | -1 | 0.0000 | 0.8886 | 0.0000 | 0.1380 | | | | | | |
| 76 135-tri-Me-Bz | 105 120 | 17066 | 117538 | 539476 | 1018963 | 2059638 | 3828683 | -1 | 0.0000 | 2.6173 | 0.0000 | 0.0399 | | | | | | |
| 79 tert-butylbenzene | 119 91 | 16192 | 139975 | 610164 | 1182229 | 2412602 | 4386919 | -1 | 0.0000 | 2.9464 | 0.0000 | 0.1001 | | | | | | |
| 78 124-tri-Me-Bz | 105 120 | 13993 | 99021 | 441266 | 843153 | 1722397 | 3314335 | -1 | 0.0000 | 2.1864 | 0.0000 | 0.0560 | | | | | | |
| 80 13-di-Cl-Bz | 146 148 | 8334 | 52974 | 229141 | 454607 | 873397 | 1637769 | -1 | 0.0000 | 1.1613 | 0.0000 | 0.0711 | | | | | | |

| | | | | | | | | | | | | |
|---------------------|---------|-------|--------|--------|---------|---------|---------|----|---------|--------|--------|--------|
| 82 14-di-Cl-Bz | 146 148 | 9119 | 77324 | 360564 | 688087 | 1350534 | 2427479 | -1 | 0.0000 | 1.6689 | 0.0000 | 0.0921 |
| 81 sec-butylbenzene | 105 134 | 27562 | 188712 | 808141 | 1585357 | 3307792 | 5902646 | -1 | 0.0000 | 4.1126 | 0.0000 | 0.0619 |
| 77 4-iso-Pr-toluene | 119 134 | 19882 | 146089 | 661221 | 1200767 | 2437020 | 4387114 | -1 | 0.0000 | 3.1156 | 0.0000 | 0.0554 |
| 84 12-di-Cl-benzene | 146 148 | 6500 | 51953 | 234009 | 454651 | 862171 | 1667156 | -1 | 0.0000 | 1.1158 | 0.0000 | 0.0757 |
| 85 n-butylbenzene | 91 134 | 17225 | 125422 | 538366 | 1017966 | 2160614 | 4022017 | -1 | 0.0000 | 2.6951 | 0.0000 | 0.0677 |
| 86 12-diBr-3-Cl-Pra | 157 155 | -1 | 1829 | 14905 | 28995 | 56245 | 114486 | -1 | -0.0147 | 0.0803 | 0.0000 | 0.9979 |
| 87 124-tri-Cl-Bz | 180 182 | 2922 | 30767 | 135221 | 262726 | 578192 | 1051545 | -1 | -0.0553 | 0.7381 | 0.0000 | 0.9992 |
| 88 naphthalene | 128 129 | 1954 | 26649 | 107459 | 235161 | 598470 | 1033706 | -1 | -0.0995 | 0.7367 | 0.0000 | 0.9955 |
| 90 123-tri-Cl-Bz | 180 182 | 1279 | 22090 | 101362 | 206041 | 447433 | 779205 | -1 | -0.0222 | 0.5495 | 0.0000 | 0.9986 |
| 89 hx-Cl-butadiene | 225 260 | 4633 | 32362 | 134569 | 257067 | 538819 | 952000 | -1 | 0.0000 | 0.6806 | 0.0000 | 0.0759 |

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Fri May 16 10:36:26 2003
 Response via : Initial Calibration

Calibration Files
 0.3 =4-003.D 2 =4-002.D 10 =4-010.D
 20 =4-020.D 40 =4-040.D 80 =4-080.D

| Compound | 0.3 | 2 | 10 | 20 | 40 | 80 | Avg | %RSD | |
|-----------------------------|-------|-------|-------|-------|-------|-------|--------|--------|-------|
| 1) I 1 Fluorobenzene I1 | 0.171 | 0.222 | 0.204 | 0.210 | 0.231 | 0.234 | 0.212 | 10.90 | |
| 2) 3 dl-Cl-di-F-metha | 0.070 | 0.124 | 0.124 | 0.165 | 0.175 | 0.194 | 0.142 | 31.72# | 0.996 |
| 3) P 4 Chloromethane | 0.172 | 0.280 | 0.268 | 0.259 | 0.268 | 0.282 | 0.255 | 16.33 | 0.999 |
| 4) 9 F114 85 135 | 0.137 | 0.213 | 0.196 | 0.201 | 0.203 | 0.212 | 0.194 | 14.66 | |
| 5) C 5 vinyl chloride | 0.179 | 0.169 | 0.157 | 0.179 | 0.170 | 0.181 | 0.172 | 5.36 | |
| 6) 6 bromomethane | 0.130 | 0.163 | 0.150 | 0.158 | 0.156 | 0.158 | 0.153 | 7.81 | |
| 7) 7 Chloroethane | 0.366 | 0.403 | 0.359 | 0.398 | 0.414 | 0.434 | 0.396 | 7.24 | |
| 8) 8 tri-Cl-F-methane | 0.004 | 0.004 | 0.005 | 0.005 | 0.004 | 0.004 | 0.004# | 11.13 | 1.000 |
| 9) 111 isopropyl alcch | 0.166 | 0.139 | 0.146 | 0.146 | 0.139 | 0.143 | 0.158 | 19.19 | 0.986 |
| 10) 100 ethyl ether x5 | 0.010 | 0.015 | 0.011 | 0.010 | 0.010 | 0.012 | 0.011# | 19.61 | 0.986 |
| 11) 102 Acrolein x10 | 0.218 | 0.114 | 0.220 | 0.172 | 0.172 | 0.163 | 0.177 | 24.90 | 0.980 |
| 12) 119 methyl acetate | 0.679 | 0.571 | 0.619 | 0.614 | 0.614 | 0.625 | 0.623 | 5.60 | 0.996 |
| 13) 104 Carbon disulfid | 0.024 | 0.015 | 0.027 | 0.025 | 0.025 | 0.026 | 0.023# | 20.79 | 1.000 |
| 14) 103 Acrylonitrilex1 | 0.026 | 0.018 | 0.018 | 0.018 | 0.017 | 0.017 | 0.019# | 20.91 | |
| 15) 95 Acetone x10 | 0.327 | 0.354 | 0.314 | 0.345 | 0.359 | 0.367 | 0.344 | 5.90 | |
| 16) 108 F-113 | 0.351 | 0.377 | 0.345 | 0.359 | 0.364 | 0.375 | 0.362 | 3.55 | |
| 17) M,C 13 11-dichloroethen | 0.012 | 0.006 | 0.004 | 0.007 | 0.006 | 0.007 | 0.007# | 36.67 | 0.996 |
| 18) 101 Acetonitrilex1 | 0.470 | 0.408 | 0.421 | 0.394 | 0.417 | 0.417 | 0.399 | 15.58 | 0.999 |
| 19) 109 Iodomethane | 0.012 | 0.009 | 0.009 | 0.009 | 0.009 | 0.007 | 0.009# | 17.87 | |
| 20) 113 Tert butyl alco | 0.303 | 0.224 | 0.238 | 0.228 | 0.228 | 0.234 | 0.245 | 13.30 | |
| 21) 18 methylene chlori | 0.550 | 0.482 | 0.402 | 0.412 | 0.376 | 0.358 | 0.430 | 16.86 | 0.998 |
| 22) 112 Allyl chloride | 0.026 | 0.042 | 0.039 | 0.044 | 0.041 | 0.043 | 0.039# | 17.19 | |
| 23) 200 Nitro methane x | 0.471 | 0.570 | 0.445 | 0.484 | 0.491 | 0.512 | 0.496 | 8.64 | |
| 24) 10 t-Bu-Me-ether | 0.215 | 0.278 | 0.262 | 0.283 | 0.262 | 0.281 | 0.263 | 9.69 | |
| 25) 19 t-12-di-Cl-ethen | 0.030 | 0.209 | 0.071 | 0.180 | 0.195 | 0.210 | 0.149 | 52.56 | 0.993 |
| 26) 98 Vinyl acetate x5 | 0.455 | 0.556 | 0.500 | 0.558 | 0.539 | 0.544 | 0.525 | 7.65 | |
| 27) P 21 11-dichloroethan | 0.105 | 0.096 | 0.078 | 0.096 | 0.092 | 0.096 | 0.094 | 9.52 | |
| 28) 91 2-butanone MEKx1 | | | | | | | | | |

(#) = Out of Range
 E524G004.M Fri May 16 10:37:12 2003

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Fri May 16 10:36:26 2003
 Response via : Initial Calibration

Calibration Files
 0.3 =4-003.D 2 =4-002.D 10 =4-010.D
 20 =4-020.D 40 =4-040.D 80 =4-080.D

| Compound | 0.3 | 2 | 10 | 20 | 40 | 80 | Avg | %RSD | R ² |
|---------------------------|-------|-------|-------|-------|-------|-------|--------|-------|----------------|
| 29) 115 Di isoprop ethe | 1.669 | 1.454 | 1.309 | 1.380 | 1.335 | 1.380 | 1.421 | 9.23 | |
| 30) 22 c-12-di-Cl-ethen | 0.275 | 0.280 | 0.270 | 0.289 | 0.279 | 0.294 | 0.281 | 3.24 | |
| 31) 23 22-Dichloropropan | 0.465 | 0.447 | 0.394 | 0.421 | 0.415 | 0.426 | 0.428 | 5.85 | |
| 32) 24 Br-Cl-methane | 0.025 | 0.123 | 0.114 | 0.121 | 0.119 | 0.123 | 0.104 | 37.24 | 1.000 |
| 33) 25 chloroform | 0.619 | 0.510 | 0.463 | 0.496 | 0.484 | 0.502 | 0.512 | 10.68 | |
| 34) 201 Ethyl acetate x | 1.371 | 0.901 | 0.781 | 0.834 | 0.797 | 0.813 | 0.916 | 19.14 | 0.996 |
| 35) 116 ETBE | 0.004 | 0.039 | 0.016 | 0.024 | 0.023 | 0.026 | 0.022# | 52.71 | 1.000 |
| 36) 117 Iso-butyl alcch | 0.010 | 0.011 | 0.011 | 0.011 | 0.011 | 0.011 | 0.011# | 3.25 | 0.995 |
| 37) 26 tetrahydrofuranx | 0.380 | 0.351 | 0.378 | 0.402 | 0.405 | 0.435 | 0.399 | 6.16 | |
| 38) 27 Di-Br-F-Methane | 0.366 | 0.411 | 0.378 | 0.402 | 0.405 | 0.435 | 0.399 | 3.31 | |
| 39) 34 111-tri-Cl-ethan | 0.074 | 0.208 | 0.187 | 0.208 | 0.207 | 0.220 | 0.184 | 29.91 | 0.999 |
| 40) 30 12-dichloroethan | 0.355 | 0.363 | 0.334 | 0.357 | 0.353 | 0.364 | 0.354 | 3.01 | |
| 41) 35 11-Di-Cl-propene | 0.165 | 0.163 | 0.175 | 0.175 | 0.165 | 0.175 | 0.169 | 3.41 | |
| 42) 29 1,2-di-Cl-ethane | 0.826 | 0.894 | 0.811 | 0.872 | 0.843 | 0.862 | 0.851 | 3.59 | |
| 43) M 36 benzene | 0.347 | 0.365 | 0.332 | 0.364 | 0.371 | 0.376 | 0.359 | 4.61 | |
| 44) 37 CCl4 | 0.386 | 0.470 | 0.403 | 0.435 | 0.422 | 0.430 | 0.424 | 6.80 | |
| 45) 97 thiophene | 0.099 | 0.714 | 0.540 | 0.599 | 0.561 | 0.580 | 0.515 | 41.29 | 0.999 |
| 46) 118 TAME | 0.218 | 0.262 | 0.251 | 0.262 | 0.254 | 0.262 | 0.251 | 6.77 | |
| 47) C 39 12-di-Cl-propane | 0.308 | 0.320 | 0.283 | 0.304 | 0.303 | 0.307 | 0.304 | 3.93 | |
| 48) M 40 trichloroethene | 0.059 | 0.096 | 0.058 | 0.108 | 0.097 | 0.107 | 0.087 | 26.49 | 0.994 |
| 49) 96 Me-methacrylate | 0.518 | 0.343 | 0.313 | 0.341 | 0.323 | 0.334 | 0.362 | 21.31 | 1.000 |
| 50) 42 Br-di-Cl-methane | 0.025 | 0.121 | 0.113 | 0.131 | 0.128 | 0.134 | 0.109 | 38.23 | 0.999 |
| 51) 41 dibromomethane | 0.311 | 0.306 | 0.290 | 0.320 | 0.310 | 0.319 | 0.309 | 3.48 | |
| 52) 45 c-13-di-Cl-prope | 0.521 | 0.473 | 0.514 | 0.498 | 0.513 | 0.504 | 0.504 | 3.76 | |
| 53) S 55 toluene-d8(S2) | 0.022 | 0.026 | 0.025 | 0.028 | 0.027 | 0.028 | 0.026# | 9.04 | |
| 54) 92 2-ClEt-Vi-ether1 | 0.984 | 0.797 | 0.743 | 0.790 | 0.785 | 0.806 | 0.817 | 10.33 | 0.995 |
| 55) M C 56 toluene | 0.142 | 0.150 | 0.065 | 0.144 | 0.145 | 0.149 | 0.132 | 24.94 | |
| 56) 107 Et methacrylate | 0.012 | 0.054 | 0.035 | 0.058 | 0.056 | 0.057 | 0.045# | 40.36 | 0.998 |
| 57) 93 2-Hexanone x5 | | | | | | | | | |

(#) = Out of Range
 E524G004.M Fri May 16 10:37:17 2003

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Fri May 16 10:36:26 2003
 Response via : Initial Calibration

Calibration Files
 0.3 =4-003.D 2 =4-002.D 10 =4-010.D
 20 =4-020.D 40 =4-040.D 80 =4-080.D

| Compound | 0.3 | 2 | 10 | 20 | 40 | 80 | Avg | %RSD | r ² |
|-----------------------------|----------------|-------|-------|-------|-------|-------|-------|-------|----------------|
| 58) 48 112-tri-Cl-Et | 0.037 | 0.121 | 0.133 | 0.123 | 0.120 | 0.126 | 0.110 | 32.76 | 0.999 |
| 59) 58 1,2-di-br-ethane | 0.075 | 0.130 | 0.120 | 0.133 | 0.129 | 0.136 | 0.121 | 19.23 | 0.999 |
| 60) 51 di-Br-Cl-methane | 0.300 | 0.209 | 0.189 | 0.201 | 0.198 | 0.206 | 0.217 | 19.04 | 1.000 |
| 61) 46 t-13-di-Cl-prope | 0.311 | 0.306 | 0.290 | 0.320 | 0.310 | 0.319 | 0.309 | 3.48 | |
| 62) 105 1-Chlorohexane | 0.488 | 0.346 | 0.252 | 0.263 | 0.270 | 0.270 | 0.315 | 28.95 | 1.000 |
| 63) I 47 Cl-benzene-d5, I2 | -----ISTD----- | | | | | | | | |
| 64) 54 MIBK | 0.633 | 0.040 | 0.247 | 0.366 | 0.338 | 0.311 | 0.323 | 59.49 | 0.993 |
| 65) 49 1,3-di-Cl-propan | 0.725 | 0.760 | 0.715 | 0.750 | 0.665 | 0.635 | 0.708 | 6.87 | |
| 66) 59 tetra-Cl-ethene | 0.811 | 0.964 | 0.829 | 0.894 | 0.834 | 0.805 | 0.856 | 7.16 | |
| 67) M P 60 chlorobenzene | 1.600 | 1.774 | 1.582 | 1.689 | 1.517 | 1.449 | 1.602 | 7.29 | |
| 68) 61 112-tetra-Cl-Et | 0.638 | 0.778 | 0.713 | 0.773 | 0.713 | 0.712 | 0.721 | 7.07 | |
| 69) C 64 ethylbenzene | 3.112 | 3.172 | 2.684 | 2.849 | 2.633 | 2.571 | 2.837 | 8.96 | |
| 70) 65 m/p-Xylenes x2 | 2.217 | 2.435 | 2.037 | 2.212 | 2.003 | 1.913 | 2.136 | 8.86 | |
| 71) 99 1-4-di-Cl-butane | 0.969 | 0.802 | 0.614 | 0.676 | 0.587 | 0.566 | 0.702 | 22.19 | 0.997 |
| 72) P 52 bromoform | 0.362 | 0.339 | 0.280 | 0.305 | 0.286 | 0.278 | 0.308 | 11.37 | |
| 73) 66 styrene | 2.237 | 1.851 | 1.535 | 1.703 | 1.551 | 1.494 | 1.729 | 16.33 | 0.998 |
| 74) 67 o-xylene | 2.181 | 2.365 | 1.964 | 2.141 | 1.905 | 1.793 | 2.058 | 10.15 | |
| 75) P 68 112-Tetra-Cl-Et | 0.341 | 0.373 | 0.327 | 0.383 | 0.339 | 0.319 | 0.347 | 7.35 | |
| 76) 110 t-1,4-dichloro- | 0.086 | 0.113 | 0.071 | 0.082 | 0.060 | 0.057 | 0.078 | 26.49 | |
| 77) 106 Cl-benzyl | 0.246 | 0.767 | 0.523 | 0.553 | 0.506 | 0.475 | 0.512 | 32.62 | 0.997 |
| 78) I 62 1,4-DCB-d4 150 152 | -----ISTD----- | | | | | | | | |
| 79) 69 123-tri-Cl-Pr | 0.105 | 0.115 | 0.118 | 0.118 | 0.118 | 0.125 | 0.116 | 6.41 | |
| 80) S 70 4-Br-1-F-Bz (S3) | 0.861 | 0.783 | 0.843 | 0.816 | 0.816 | 0.816 | 0.824 | 3.60 | |
| 81) 71 isopropylbenzene | 3.079 | 3.655 | 3.123 | 3.352 | 3.453 | 3.483 | 3.357 | 6.61 | |
| 82) 72 bromobenzene | 0.550 | 0.760 | 0.702 | 0.768 | 0.754 | 0.770 | 0.717 | 11.96 | |
| 83) 73 n-propylbenzene | 0.826 | 1.098 | 0.966 | 0.997 | 1.023 | 1.018 | 0.988 | 9.16 | |
| 84) 74 2-Cl-Tl 126 | 0.510 | 0.613 | 0.554 | 0.631 | 0.615 | 0.632 | 0.592 | 8.39 | |

(#) = Out of Range
 E524G004.M Fri May 16 10:37:22 2003

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P &ch Lab** EPA 524.2
 Last Update : Fri May 16 10:36:26 2003
 Response via : Initial Calibration

Calibration Files
 0.3 =4-003.D 2 =4-002.D 10 =4-010.D
 20 =4-020.D 40 =4-040.D 80 =4-080.D

| Compound | 0.3 | 2 | 10 | 20 | 40 | 80 | Avg | %RSD |
|-------------------------|-------|-------|-------|-------|-------|-------|-------|-------|
| 85) 75 4-Cl-Tl 126 | 0.646 | 0.992 | 0.902 | 0.940 | 0.923 | 0.929 | 0.889 | 13.80 |
| 86) 76 135-tri-Me-Bz | 2.583 | 2.784 | 2.472 | 2.572 | 2.629 | 2.663 | 2.617 | 3.99 |
| 87) 79 tert-butylbenzen | 2.451 | 3.316 | 2.795 | 2.985 | 3.080 | 3.051 | 2.946 | 10.01 |
| 88) 78 124-tri-Me-Bz | 2.118 | 2.346 | 2.022 | 2.129 | 2.199 | 2.305 | 2.186 | 5.60 |
| 89) 80 13-di-Cl-Bz 146 | 1.262 | 1.255 | 1.050 | 1.148 | 1.115 | 1.139 | 1.161 | 7.11 |
| 90) 82 14-di-Cl-Bz 146 | 1.380 | 1.832 | 1.652 | 1.737 | 1.724 | 1.689 | 1.669 | 9.21 |
| 91) 81 sec-butylbenzene | 4.172 | 4.470 | 3.703 | 4.002 | 4.222 | 4.106 | 4.113 | 6.19 |
| 92) 77 4-iso-Pr-toluene | 3.010 | 3.461 | 3.029 | 3.031 | 3.111 | 3.052 | 3.116 | 5.54 |
| 93) 84 12-di-Cl-benzene | 0.984 | 1.231 | 1.072 | 1.148 | 1.101 | 1.160 | 1.116 | 7.57 |
| 94) 85 n-butylbenzene | 2.607 | 2.971 | 2.467 | 2.570 | 2.758 | 2.798 | 2.695 | 6.77 |
| 95) 86 12-diBr-3-Cl-Pra | 0.043 | 0.068 | 0.073 | 0.072 | 0.072 | 0.080 | 0.067 | 20.80 |
| 96) 87 124-tri-Cl-Bz | 0.442 | 0.729 | 0.620 | 0.663 | 0.738 | 0.731 | 0.654 | 17.40 |
| 97) 88 naphthalene | 0.296 | 0.631 | 0.492 | 0.594 | 0.764 | 0.719 | 0.583 | 29.17 |
| 98) 90 123-tri-Cl-Bz | 0.194 | 0.523 | 0.464 | 0.520 | 0.571 | 0.542 | 0.469 | 29.72 |
| 99) 89 hx-Cl-butadiene | 0.701 | 0.767 | 0.617 | 0.649 | 0.688 | 0.662 | 0.681 | 7.59 |

0.998
 0.999
 0.999
 0.999

(#) = Out of Range
 E524G004.M Fri May 16 10:37:26 2003

Data File : C:\HPCHEM\1\DATA\03G2684\G2684Q01.D

Acq On : 29 May 03 10:45 am


Sample : #03g2684, w

Misc :

Vial: 19
Operator: Eddie
Inst : GCMS-G
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\E524G004.M

Title : **Applied P & ch Lab** EPA 524.2



Peak Apex is scan: 1522

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result |
|-------------|--------------|--------------|--------------|-----------|---------|--------|
| 50 | 95 | 15 | 40 | 16.3 | 13677 | PASS |
| 75 | 95 | 30 | 60 | 42.7 | 35832 | PASS |
| 95 | 95 | 100 | 100 | 100.0 | 83864 | PASS |
| 96 | 95 | 5 | 9 | 7.2 | 6077 | PASS |
| 173 | 174 | 0 | 2 | 0.0 | 0 | PASS |
| 174 | 95 | 50 | 100 | 81.1 | 68048 | PASS |
| 175 | 174 | 5 | 9 | 6.8 | 4621 | PASS |
| 176 | 174 | 95 | 101 | 97.1 | 66048 | PASS |
| 177 | 176 | 5 | 9 | 6.2 | 4072 | PASS |

FORM-5A

Applied P & Ch Laboratory

Volatile Organic Instrument Performance Check for Method 524.2

Bromofluorobenzene (BFB), Part II

| | | | | |
|-----------------|--------------|---------------------|--------------|---------|
| Client Name: | GEOFON, Inc. | Contract No: | Lab Code: | APCL |
| Case No: | | SAS No: | Service ID: | 033414 |
| Project ID: | JPL | BFB Inj. Date: | Batch No: | 03G2684 |
| | | BFB Inj. Time: | Sequence No: | 03G2684 |
| Project No: | 04-4428.10 | Instrument ID: | GC Column: | DB-VEX |
| Data File Name: | G2684Q01 | Heated Purge: (Y/N) | Column ID: | 0.45 mm |

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS AND STANDARDS:

| # | Client Sample No | Lab Sample ID | Data File Name | Date Analyzed | Time Analyzed |
|----|------------------|----------------|----------------|---------------|---------------|
| 1 | 03G2697-CCV-01 | 03G2684-CCV-01 | G2684Q01 | 05/29/03 | 10:45 |
| 2 | 03G2684-LCS-01 | 03G2684-LCS-01 | G2684L01 | 05/29/03 | 11:16 |
| 3 | MW-5MS | 03-3414-1MS | G2684M01 | 05/29/03 | 11:44 |
| 4 | MW-5MSD | 03-3414-1MSD | G2684N01 | 05/29/03 | 12:43 |
| 5 | 03G2684-MB-01 | 03G2684-MB-01 | G2684K01 | 05/29/03 | 14:10 |
| 6 | MW-5 | 03-3414-1 | 3414-01 | 05/29/03 | 16:09 |
| 7 | MW-8 | 03-3414-2 | 3414-02 | 05/29/03 | 16:39 |
| 8 | TB-15-5/28/03 | 03-3414-3 | 3414-03 | 05/29/03 | 17:09 |
| 9 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |
| 23 | | | | | |
| 24 | | | | | |
| 25 | | | | | |

Evaluate Continuing Calibration Report

Data File : C:\HPCHEM\1\DATA\03G2684\G2684Q01.D
 Acq On : 29 May 03 10:45 am
 Sample : ##03g2684, w
 Misc :

Vial: 19
 Operator: Eddie
 Inst : GCMS-G
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P & Sch Lab** EPA 524.2
 Last Update : Fri May 16 10:36:26 2003
 Response via : Multiple Level Calibration

Min. RRF : 0.050 Min. Rel. Area : 35% Max. R.T. Dev 0.50min
 Max. RRF Dev : 20% Max. Rel. Area : 150%

| Compound | AvGRF | CCRF | %Dev | Area | Area% | Dev(min) |
|----------------------------------|-------|--------|--------|------|-------|----------|
| 1 I 1 Fluorobenzene I1 1 | 1.000 | 1.000 | 0.0 | 96 | 0.00 | |
| 2 3 di-Cl-di-F-methane 85 8 | 0.212 | 0.192 | 9.3 | 87 | 0.00 | |
| 3 P 4 Chloromethane 50 5 | 0.142 | 0.158 | -11.3 | 92 | 0.00 | |
| 4 9 F114 85 135 | 0.255 | 0.232 | 9.1 | 86 | 0.00 | |
| 5 C 5 vinyl chloride 62 6 | 0.194 | 0.188 | 2.9 | 89 | 0.00 | |
| 6 6 bromomethane 94 9 | 0.172 | 0.192 | -11.5 | 103 | 0.00 | |
| 7 7 Chloroethane 64 66 | 0.153 | 0.150 | 2.0 | 90 | 0.00 | |
| 8 8 tri-Cl-F-methane 101 10 | 0.396 | 0.362 | 8.6 | 87 | 0.00 | |
| 9 111 isopropyl alcohol x10 | 0.004 | 0.005# | -20.8# | 98 | 0.00 | |
| 10 100 ethyl ether x5 | 0.158 | 0.150 | 5.2 | 98 | 0.00 | |
| 11 102 Acrolein x10 | 0.011 | 0.008# | 26.4# | 73 | 0.00 | |
| 12 119 methyl acetate | 0.177 | 0.156 | 12.2 | 68 | 0.00 | |
| 13 104 Carbon disulfide | 0.623 | 0.546 | 12.2 | 84 | 0.00 | |
| 14 103 Acrylonitrile x10 | 0.023 | 0.028# | -17.3 | 97 | 0.00 | |
| 15 95 Acetone x10 | 0.019 | 0.021# | -11.9 | 115 | 0.00 | |
| 16 108 F-113 | 0.344 | 0.312 | 9.4 | 86 | 0.00 | |
| 17 M,C 13 11-dichloroethene 61 9 | 0.362 | 0.329 | 9.0 | 88 | 0.00 | |
| 18 101 Acetonitrile x10 | 0.007 | 0.008# | -10.0 | 106 | 0.00 | |
| 19 109 Iodomethane | 0.399 | 0.250 | 37.2# | 57 | 0.00 | |
| 20 113 Tert butyl alcohol x10 | 0.009 | 0.011# | -21.5# | 116 | 0.00 | |
| 21 18 methylene chloride 49 8 | 0.245 | 0.319 | -30.1# | 128 | 0.00 | |
| 22 112 Allyl chloride | 0.430 | 0.376 | 12.6 | 87 | 0.00 | |
| 23 200 Nitro methane x10 | 0.039 | 0.040# | -2.4 | 88 | 0.00 | |
| 24 10 t-Bu-Me-ether 73 57 | 0.496 | 0.522 | -5.4 | 103 | 0.00 | |
| 25 19 t-12-di-Cl-ethene 96 6 | 0.263 | 0.255 | 3.1 | 86 | 0.00 | |
| 26 98 Vinyl acetate x5 | 0.149 | 0.293 | -96.3# | 156# | 0.00 | |
| 27 P 21 11-dichloroethane 63 8 | 0.525 | 0.538 | -2.5 | 92 | 0.00 | |

(#) = Out of Range
 G2684Q01.D E524G004.M Thu May 29 13:21:21 2003

Evaluate Continuing Calibration Report

Data File : C:\HPCHEM\1\DATA\03G2684\G2684Q01.D Vial: 19
 Acq On : 29 May 03 10:45 am Operator: Eddie
 Sample : ##03g2684, w Inst : GCMS-G
 Misc : Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P & Sch Lab** EPA 524.2
 Last Update : Fri May 16 10:36:26 2003
 Response via : Multiple Level Calibration

Min. RRF : 0.050 Min. Rel. Area : 35% Max. R.T. Dev 0.50min
 Max. RRF Dev : 20% Max. Rel. Area : 150%

| Compound | AVGRF | CCRF | %Dev | Area | % Dev | Area | % Dev | Area | % Dev | Area | % Dev |
|----------|-------------------------------|-------|--------|--------|-------|------|-------|------|-------|------|-------|
| 28 | 91 2-butanone MEKx10 | 0.094 | 0.100 | -6.5 | 100 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 29 | 115 Di isoprop ether | 1.421 | 1.382 | 2.8 | 96 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 30 | 22 c-12-di-Cl-ethene | 0.281 | 0.283 | -0.6 | 93 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 31 | 23 22-Dichloropropane | 0.428 | 0.418 | 2.4 | 95 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 32 | 24 Br-Cl-methane | 0.104 | 0.127 | -21.5# | 100 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 33 | 25 chloroform | 0.512 | 0.491 | 4.1 | 95 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 34 | 201 Ethyl acetate x2 | 0.118 | 0.154 | -30.2# | 123 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 35 | 116 ETBE | 0.916 | 0.875 | 4.5 | 100 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 36 | 117 Iso-butyl alcohol X10 | 0.022 | 0.031# | -41.1# | 124 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 37 | 26 tetrahydrofuranx5 | 0.011 | 0.012# | -7.7 | 97 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 38 | S 27 Di-Br-F-Methane (S1) | 0.371 | 0.381 | -2.7 | 96 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 39 | 34 111-tri-Cl-ethane | 0.399 | 0.389 | 2.5 | 93 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 40 | 30 12-dichloroethane | 0.184 | 0.213 | -15.9 | 98 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 41 | 35 11-Di-Cl-propene | 0.354 | 0.333 | 6.1 | 89 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 42 | S 29 1,2-di-Cl-ethane-d4 [Sur | 0.169 | 0.176 | -4.0 | 96 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 43 | M 36 benzene | 0.851 | 0.848 | 0.4 | 93 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 44 | 37 CCl4 | 0.359 | 0.343 | 4.4 | 90 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 45 | 97 thiophene | 0.424 | 0.429 | -1.0 | 94 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 46 | 118 TAME | 0.515 | 0.614 | -19.0 | 98 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 47 | C 39 12-di-Cl-propane | 0.251 | 0.265 | -5.3 | 97 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 48 | M 40 trichloroethene | 0.304 | 0.290 | 4.6 | 91 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 49 | 96 Me-methacrylate | 0.087 | 0.104 | -19.0 | 92 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 50 | 42 Br-di-Cl-methane | 0.362 | 0.336 | 7.1 | 94 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 51 | 41 dibromomethane | 0.109 | 0.130 | -19.3 | 95 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 52 | 45 c-13-di-Cl-propene | 0.309 | 0.321 | -3.7 | 96 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 53 | S 55 toluene-d8 (S2) | 0.504 | 0.503 | 0.1 | 94 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 54 | 92 2-ClEt-Vi-ether10 | 0.026 | 0.028# | -8.1 | 97 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |

(#) = Out of Range
 G2684Q01.D E524G004.M Thu May 29 13:21:26 2003

Evaluate Continuing Calibration Report

Data File : C:\HPCHEM\1\DATA\03G2684\G2684Q01.D

Acq On : 29 May 03 10:45 am
 Sample : ##03G2684, w
 Misc :

Vial: 19
 Operator: Eddie
 Inst : GCMS-G
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P & Ch Lab** EPA 524.2
 Last Update : Fri May 16 10:36:26 2003
 Response via : Multiple Level Calibration

Min. RRF : 0.050 Min. Rel. Area : 35% Max. R.T. Dev 0.50min
 Max. RRF Dev : 20% Max. Rel. Area : 150%

| Compound | AVGRF | CCRF | %Dev | Area% | Dev(min) | | | |
|----------|-----------------------------|------|------|-------|----------|--------|-----|------|
| 55 M C | 56 toluene | 91 | 9 | 0.817 | 0.772 | 5.6 | 93 | 0.00 |
| 56 | 107 Et methacrylate | | | 0.132 | 0.201 | -51.9# | 133 | 0.00 |
| 57 | 93 2-Hexanone x5 | | | 0.045 | 0.066 | -45.7# | 110 | 0.00 |
| 58 | 48 112-tri-Cl-Et | | | 0.110 | 0.126 | -14.3 | 98 | 0.00 |
| 59 | 58 1,2-di-br-ethane | 107 | 109 | 0.121 | 0.133 | -10.5 | 96 | 0.00 |
| 60 | 51 di-Br-Cl-methane | 129 | 12 | 0.217 | 0.210 | 3.2 | 100 | 0.00 |
| 61 | 46 t-13-di-Cl-propene | 75 | 11 | 0.309 | 0.321 | -3.7 | 96 | 0.00 |
| 62 | 105 1-Chlorohexane | | | 0.315 | 0.250 | 20.7# | 91 | 0.00 |
| 63 I | 47 Cl-benzene-d5, I2 | | | 1.000 | 1.000 | 0.0 | 100 | 0.00 |
| 64 | 54 MTBK | | | 0.323 | 0.375 | -16.2 | 103 | 0.00 |
| 65 | 49 1,3-di-Cl-propane | 76 | 78 | 0.708 | 0.684 | 3.4 | 92 | 0.00 |
| 66 | 59 tetra-Cl-ethene | 166 | 16 | 0.856 | 0.793 | 7.4 | 89 | 0.00 |
| 67 M P | 60 chlorobenzene | 112 | 7 | 1.602 | 1.597 | 0.3 | 95 | 0.00 |
| 68 | 61 1112-tetra-Cl-Et | 131 | 13 | 0.721 | 0.752 | -4.3 | 98 | 0.00 |
| 69 C | 64 ethylbenzene | 91 | 10 | 2.837 | 2.639 | 7.0 | 93 | 0.00 |
| 70 | 65 m/p-Xylenes x2 | | | 2.136 | 2.006 | 6.1 | 91 | 0.00 |
| 71 | 99 1-4-di-Cl-butane | | | 0.702 | 0.649 | 7.6 | 96 | 0.00 |
| 72 P | 52 bromoform | 173 | 17 | 0.308 | 0.315 | -2.3 | 104 | 0.00 |
| 73 | 66 styrene | 104 | 7 | 1.729 | 1.559 | 9.8 | 92 | 0.00 |
| 74 | 67 o-xylene | 91 | 10 | 2.058 | 1.913 | 7.1 | 90 | 0.00 |
| 75 P | 68 1122-Tetra-Cl-Et | 83 | 8 | 0.347 | 0.376 | -8.4 | 99 | 0.00 |
| 76 | 110 t-1,4-dichloro-2-butene | | | 0.078 | 0.075 | 4.4 | 92 | 0.00 |
| 77 | 106 Cl-benzyl | | | 0.512 | 0.625 | -22.0# | 113 | 0.00 |

| | | | | | | | | | |
|------|------------------|-----|-----|----|-------|-------|------|-----|------|
| 78 I | 62 1,4-DCB-d4 | 150 | 152 | I3 | 1.000 | 1.000 | 0.0 | 103 | 0.00 |
| 79 | 69 123-tri-Cl-Pr | | 110 | 9 | 0.116 | 0.122 | -5.4 | 106 | 0.00 |

(#) = Out of Range

G2684Q01.D E524G004.M Thu May 29 13:21:30 2003

Evaluate Continuing Calibration Report

Data File : C:\HPCHEM\1\DATA\03G26884\G26884Q01.D

Vial: 19

Acq On : 29 May 03 10:45 am
 Sample : ##03g26884, w
 Misc :
 Operator: Eddie
 Inst : GCMS-G
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\E524G004.M
 Title : **Applied P & Ch Lab** EPA 524.2

Last Update : Fri May 16 10:36:26 2003
 Response via : Multiple Level Calibration

Min. RRF : 0.050 Min. Rel. Area : 35% Max. R.T. Dev 0.50min
 Max. RRF Dev : 20% Max. Rel. Area : 150%

| Compound | AVGRF | CCRF | %Dev | Area% Dev(min) | | | | | |
|----------|-------|-------------------|------|----------------|-------|-------|--------|-----|------|
| 80 S | 70 | 4-Br-1-F-Bz (S3) | 174 | 9 | 0.824 | 0.764 | 7.3 | 93 | 0.00 |
| 81 | 71 | isopropylbenzene | 105 | 12 | 3.357 | 2.963 | 11.8 | 91 | 0.00 |
| 82 | 72 | bromobenzene | 156 | 15 | 0.717 | 0.701 | 2.3 | 93 | 0.00 |
| 83 | 73 | n-propylbenzene | 120 | 7 | 0.988 | 0.884 | 10.5 | 91 | 0.00 |
| 84 | 74 | 2-Cl-Tl | 126 | 128 | 0.592 | 0.575 | 2.9 | 93 | 0.00 |
| 85 | 75 | 4-Cl-Tl | 126 | 128 | 0.889 | 0.840 | 5.4 | 92 | 0.00 |
| 86 | 76 | 135-tri-Me-Bz | 105 | 12 | 2.617 | 2.347 | 10.3 | 94 | 0.00 |
| 87 | 79 | tert-butylbenzene | 119 | 9 | 2.946 | 2.618 | 11.1 | 90 | 0.00 |
| 88 | 78 | 124-tri-Me-Bz | 105 | 12 | 2.186 | 2.053 | 6.1 | 99 | 0.00 |
| 89 | 80 | 13-di-Cl-Bz | 146 | 148 | 1.161 | 1.101 | 5.2 | 98 | 0.00 |
| 90 | 82 | 14-di-Cl-Bz | 146 | 148 | 1.669 | 1.505 | 9.8 | 89 | 0.00 |
| 91 | 81 | sec-butylbenzene | 105 | 13 | 4.113 | 3.457 | 15.9 | 89 | 0.00 |
| 92 | 77 | 4-iso-Pr-toluene | 119 | 13 | 3.116 | 2.725 | 12.5 | 92 | 0.00 |
| 93 | 84 | 12-di-Cl-benzene | 146 | 14 | 1.116 | 1.052 | 5.7 | 94 | 0.00 |
| 94 | 85 | n-butylbenzene | 91 | 13 | 2.695 | 2.322 | 13.9 | 93 | 0.00 |
| 95 | 86 | 12-diBr-3-Cl-Pra | 157 | 15 | 0.067 | 0.071 | -5.9 | 100 | 0.00 |
| 96 | 87 | 124-tri-Cl-Bz | 180 | 18 | 0.654 | 0.703 | -7.5 | 109 | 0.00 |
| 97 | 88 | naphthalene | 128 | 12 | 0.583 | 0.736 | -26.3# | 127 | 0.00 |
| 98 | 90 | 123-tri-Cl-Bz | 180 | 18 | 0.469 | 0.546 | -16.4 | 108 | 0.00 |
| 99 | 89 | hx-Cl-butadiene | 225 | 26 | 0.681 | 0.582 | 14.5 | 92 | 0.00 |

(#) = Out of Range
 G26884Q01.D E524G004.M SPPC'S out = 0 CCC'S out = 0
 Thu May 29 13:21:34 2003

Continuing Calibration Concentration Summary

Data File G2684Q01.D

Method File E524G004

| <u>Compound Name</u> | <u>Amount</u> | <u>Actual</u> | <u>Units</u> | <u>%Dev</u> | <u>Target Response</u> |
|----------------------------------|---------------|---------------|--------------|-------------|------------------------|
| 1 Fluorobenzene l1 1 | 10 | 10.00 | ppb | 0.00 | 713991 |
| 3 di-Cl-di-F-methane 85 87 | 20 | 18.14 | ppb | 9.32 | 274560 |
| 4 Chloromethane 50 52 | 20 | 18.25 | ppb | 8.73 | 225545 |
| 9 F114 85 135 | 20 | 17.12 | ppb | 14.42 | 330605 |
| 5 vinyl chloride 62 64 | 20 | 19.42 | ppb | 2.92 | 268660 |
| 6 bromomethane 94 96 | 20 | 22.30 | ppb | 11.50 | 274520 |
| 7 Chloroethane 64 66 | 20 | 19.60 | ppb | 2.02 | 213631 |
| 8 tri-Cl-F-methane 101 103 | 20 | 18.28 | ppb | 8.58 | 516479 |
| 111 isopropyl alcohol x10 | 200 | 241.66 | ppb | 20.83 | 69108 |
| 100 ethyl ether x5 | 100 | 105.10 | ppb | 5.10 | 1070002 |
| 102 Acrolein x10 | 200 | 151.07 | ppb | 24.47 | 120095 |
| 119 methyl acetate | 20 | 17.71 | ppb | 11.46 | 222394 |
| 104 Carbon disulfide | 20 | 17.55 | ppb | 12.25 | 780208 |
| 103 Acrylonitrilex10 | 200 | 222.22 | ppb | 11.11 | 392999 |
| 95 Acetone x10 | 200 | 247.02 | ppb | 23.51 | 306038 |
| 108 F-113 | 20 | 18.11 | ppb | 9.45 | 445250 |
| 13 11-dichloroethene 61 96 | 20 | 18.20 | ppb | 9.00 | 470082 |
| 101 Acetonitrilex10 | 200 | 238.50 | ppb | 19.25 | 108757 |
| 109 Iodomethane | 20 | 12.26 | ppb | 38.71 | 357555 |
| 113 Tert butyl alcohol x10 | 200 | 243.08 | ppb | 21.54 | 159886 |
| 18 methylene chloride 49 84 | 20 | 26.01 | ppb | 30.07 | 455282 |
| 112 Allyl chloride | 20 | 19.78 | ppb | 1.12 | 536616 |
| 200 Nitro methane x10 | 200 | 204.72 | ppb | 2.36 | 572067 |
| 10 t-Bu-Me-ether 73 57 | 20 | 21.08 | ppb | 5.40 | 745816 |
| 19 t-12-di-Cl-ethene 96 61 | 20 | 19.38 | ppb | 3.12 | 364371 |
| 98 Vinyl acetate x5 | 100 | 149.57 | ppb | 49.57 | 2088805 |
| 21 11-dichloroethane 63 83 | 20 | 20.49 | ppb | 2.45 | 768428 |
| 91 2-butanone MEKx10 | 200 | 213.06 | ppb | 6.53 | 1427520 |
| 115 Di isoprop ether | 20 | 19.45 | ppb | 2.76 | 1973456 |
| 22 c-12-di-Cl-ethene 96 61 | 20 | 20.12 | ppb | 0.62 | 404019 |
| 23 22-Dichloropropane 77 97 | 20 | 19.52 | ppb | 2.41 | 596517 |
| 24 Br-Cl-methane 128 130 | 20 | 21.00 | ppb | 5.01 | 181074 |
| 25 chloroform 83 85 | 20 | 19.18 | ppb | 4.12 | 701522 |
| 201 Ethyl acetate x2 | 40 | 51.40 | ppb | 28.50 | 438906 |
| 116 ETBE | 20 | 21.54 | ppb | 7.71 | 1249183 |
| 117 Iso-butyl alcohol X10 | 200 | 254.67 | ppb | 27.33 | 444917 |
| 26 tetrahydrofuranx5 | 100 | 107.66 | ppb | 7.66 | 82114 |
| 27 Di-Br-F-Methane (S1) 111 1 | 20 | 20.53 | ppb | 2.66 | 544331 |
| 34 111-tri-Cl-ethane 97 99 | 20 | 19.49 | ppb | 2.55 | 555606 |
| 30 12-dichloroethane 64 62 | 20 | 20.26 | ppb | 1.32 | 304010 |
| 35 11-Di-Cl-propene 75 110 | 20 | 18.78 | ppb | 6.12 | 474973 |
| 29 1,2-di-Cl-ethane-d4 [Surr] 10 | 20 | 20.80 | ppb | 4.00 | 250639 |
| 36 benzene 78 52 | 20 | 19.92 | ppb | 0.40 | 1210640 |
| 37 CCl4 117 119 | 20 | 19.12 | ppb | 4.39 | 490183 |

| | | | | | |
|------------------------------|-----|--------|-----|------|--------|
| 97 thiophene | 20 | 20.21 | ppb | 1.04 | 612241 |
| 118 TAME | 20 | 21.33 | ppb | 6.66 | 876255 |
| 39 12-di-Cl-propane 63 76 | 20 | 21.06 | ppb | 5.29 | 377963 |
| 40 trichloroethene 130 132 | 20 | 19.08 | ppb | 4.60 | 414626 |
| 96 Me-methacrylate | 20 | 20.89 | ppb | 4.43 | 148538 |
| 42 Br-di-Cl-methane 83 85 | 20 | 20.32 | ppb | 1.61 | 479894 |
| 41 dibromomethane 174 172 | 20 | 20.08 | ppb | 0.40 | 185088 |
| 45 c-13-di-Cl-propene 75 110 | 20 | 20.74 | ppb | 3.68 | 458065 |
| 55 toluene-d8(S2) 100 99 | 20 | 19.98 | ppb | 0.11 | 718585 |
| 92 2-ClEt-Vi-ether10 | 200 | 216.14 | ppb | 8.07 | 400033 |

| <u>Compound Name</u> | <u>Amount</u> | <u>Actual</u> | <u>Units</u> | <u>%Dev</u> | <u>Target Response</u> |
|------------------------------|---------------|---------------|--------------|-------------|------------------------|
| 56 toluene 91 92 | 20 | 18.88 | ppb | 5.58 | 1102151 |
| 107 Et methacrylate | 20 | 28.25 | ppb | 41.23 | 287320 |
| 93 2-Hexanone x5 | 100 | 119.46 | ppb | 19.46 | 472510 |
| 48 112-tri-Cl-Et 97 83 | 20 | 20.29 | ppb | 1.46 | 179727 |
| 58 1,2-di-br-ethane 107 109 | 20 | 20.19 | ppb | 0.96 | 190228 |
| 51 di-Br-Cl-methane 129 127 | 20 | 20.86 | ppb | 4.29 | 300332 |
| 46 t-13-di-cl-propene 75 110 | 20 | 20.74 | ppb | 3.68 | 458065 |
| 105 1-Chlorohexane | 20 | 18.56 | ppb | 7.20 | 356499 |
| 47 Cl-benzene-d5, I2 | 10 | 10.00 | ppb | 0.00 | 223967 |
| 54 MIBK | 20 | 23.57 | ppb | 17.84 | 167900 |
| 49 1,3-di-cl-propane 76 78 | 20 | 19.31 | ppb | 3.43 | 306418 |
| 59 tetra-Cl-ethene 166 168 | 20 | 18.52 | ppb | 7.39 | 355107 |
| 60 chlorobenzene 112 77 | 20 | 19.94 | ppb | 0.31 | 715260 |
| 61 1112-tetra-Cl-Et 131 133 | 20 | 20.86 | ppb | 4.29 | 336911 |
| 64 ethylbenzene 91 106 | 20 | 18.61 | ppb | 6.96 | 1182269 |

| <u>Compound Name</u> | <u>Amount</u> | <u>Actual</u> | <u>Units</u> | <u>%Dev</u> | <u>Target Response</u> |
|-----------------------------|---------------|---------------|--------------|-------------|------------------------|
| 65 m/p-Xylenes x2 | 40 | 37.55 | ppb | 6.11 | 1796677 |
| 99 1-4-di-Cl-butane | 20 | 21.69 | ppb | 8.43 | 290641 |
| 52 bromoform 173 175 | 20 | 20.46 | ppb | 2.29 | 141252 |
| 66 styrene 104 78 | 20 | 19.99 | ppb | 0.05 | 698529 |
| 67 o-xylene 91 106 | 20 | 18.59 | ppb | 7.05 | 856934 |
| 68 1122-Tetra-Cl-Et 83 85 | 20 | 21.69 | ppb | 8.45 | 168513 |
| 110 t-1,4-dichloro-2-butene | 20 | 19.12 | ppb | 4.38 | 33438 |
| 106 Cl-benzyl | 20 | 24.96 | ppb | 24.79 | 279752 |
| 62 1,4-DCB-d4 150 152 I3 | 10 | 10.00 | ppb | 0.00 | 203050 |
| 69 123-tri-Cl-Pr 110 97 | 20 | 21.08 | ppb | 5.40 | 49625 |
| 70 4-Br-1-F-Bz (S3) 174 95 | 20 | 18.55 | ppb | 7.25 | 310388 |
| 71 isopropylbenzene 105 120 | 20 | 17.65 | ppb | 11.76 | 1203154 |
| 72 bromobenzene 156 158 | 20 | 19.53 | ppb | 2.34 | 284539 |
| 73 n-propylbenzene 120 78 | 20 | 17.90 | ppb | 10.52 | 359075 |
| 74 2-Cl-TI 126 128 | 20 | 19.42 | ppb | 2.90 | 233607 |
| 75 4-Cl-TI 126 128 | 20 | 18.91 | ppb | 5.43 | 341260 |
| 76 135-tri-Me-Bz 105 120 | 20 | 17.93 | ppb | 10.34 | 953050 |
| 79 tert-butylbenzene 119 91 | 20 | 17.77 | ppb | 11.14 | 1063215 |
| 78 124-tri-Me-Bz 105 120 | 20 | 18.78 | ppb | 6.12 | 833554 |
| 80 13-di-Cl-Bz 146 148 | 20 | 18.96 | ppb | 5.20 | 447112 |
| 82 14-di-Cl-Bz 146 148 | 20 | 18.04 | ppb | 9.80 | 611359 |
| 81 sec-butylbenzene 105 134 | 20 | 16.81 | ppb | 15.94 | 1403967 |

| | | | | | | |
|---------------------|---------|-----|-------|-----|-------|---------|
| 77 4-iso-Pr-toluene | 119 134 | .20 | 17.49 | ppb | 12.55 | 1106502 |
| 84 12-di-Cl-benzene | 146 148 | 20 | 18.86 | ppb | 5.69 | 427356 |
| 85 n-butylbenzene | 91 134 | 20 | 17.23 | ppb | 13.85 | 942893 |
| 86 12-diBr-3-Cl-Pra | 157 155 | 20 | 19.56 | ppb | 2.18 | 28929 |
| 87 124-tri-Cl-Bz | 180 182 | 20 | 19.79 | ppb | 1.05 | 285358 |
| 88 naphthalene | 128 129 | 20 | 21.33 | ppb | 6.66 | 298891 |
| 90 123-tri-Cl-Bz | 180 182 | 20 | 20.27 | ppb | 1.36 | 221675 |

Ave.% Dev 8.20

FORM-8A

Applied P & Ch Laboratory

Internal Standard Area and RT Summary for Method 524.2

Client Name: GEOFON, Inc. Contract No: Lab Code: APCL
 Case No: SAS No: Service ID: 033414
 Project ID: JPL Project No: 04-4428.10 Sample Matrix: Water
 CCV Data File: G2684Q01 Instrument ID: G
 Batch No: 03G2684

| # | Client Sample No | Lab Sample ID | Analysis Date & Time | IS-1 | | IS-2 | | IS-3 | |
|-----------------|------------------|----------------|----------------------|---------|------|--------|-------|--------|-------|
| | | | | Area # | RT # | Area # | RT # | Area # | RT # |
| 12 Hour CCV STD | | | 05/29/03 10:45 | 713991 | 9.48 | 223967 | 13.07 | 203050 | 15.59 |
| CCV Upper Limit | | | | 1427982 | 9.98 | 447934 | 13.57 | 406100 | 16.09 |
| CCV Lower Limit | | | | 356995 | 8.98 | 111983 | 12.57 | 101525 | 15.09 |
| 1 | 03G2684-LCS-01 | 03G2684-LCS-01 | 05/29/03 11:16 | 708791 | 9.47 | 220328 | 13.07 | 209010 | 15.58 |
| 2 | MW-5MS | 03-3414-1MS | 05/29/03 11:44 | 638973 | 9.49 | 197185 | 13.09 | 178464 | 15.60 |
| 3 | MW-5MSD | 03-3414-1MSD | 05/29/03 12:43 | 632200 | 9.52 | 187812 | 13.13 | 165478 | 15.65 |
| 4 | 03G2684-MB-01 | 03G2684-MB-01 | 05/29/03 14:10 | 638085 | 9.48 | 180507 | 13.10 | 176069 | 15.59 |
| 5 | MW-5 | 03-3414-1 | 05/29/03 16:09 | 729302 | 9.47 | 200248 | 13.07 | 181489 | 15.59 |
| 6 | MW-8 | 03-3414-2 | 05/29/03 16:39 | 743133 | 9.47 | 208530 | 13.07 | 195818 | 15.58 |
| 7 | TB-15-5/28/03 | 03-3414-3 | 05/29/03 17:09 | 760474 | 9.47 | 220283 | 13.07 | 209259 | 15.59 |
| 8 | | | | | | | | | |
| 9 | | | | | | | | | |
| 10 | | | | | | | | | |
| 11 | | | | | | | | | |
| 12 | | | | | | | | | |
| 13 | | | | | | | | | |
| 14 | | | | | | | | | |
| 15 | | | | | | | | | |
| 16 | | | | | | | | | |
| 17 | | | | | | | | | |
| 18 | | | | | | | | | |
| 19 | | | | | | | | | |
| 20 | | | | | | | | | |
| 21 | | | | | | | | | |

IS-1 = FLUOROBENZENE
 IS-2 = CHLOROBENZENE-D5
 IS-3 = 1,4-DICHLOROBENZENE-D4

Area Upper Limit = +100% of CCV internal standard area
 Area Lower Limit = - 50% of CCV internal standard area
 RT Upper Limit = +0.50 minutes of CCV internal standard RT
 RT Lower Limit = - 0.50 minutes of CCV internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits

GP
 W. P. & Ch Laboratory

Magolia Ave. Chino CA 91710
 (909) 590-1828 Fax: (909) 590-1498

VOC Analysis General Logbook

0269 2684 Batch # 0269 2684 Matrix: W Date: 5-29-03 Analyst: Eddie

IS/Surrogate: GC-15114/15115 Methanol(mark-M): PEG (mark-PEG): Defoaming(mark-DF):

Ini. Batch Initial Batch; Middle Batch; Final Batch. Internal Study Datafile Path:

| Type | Sample ID | Method | V/X=f ₁ | V _i /V _i =f ₂ | V _{esp} /V _{inj} =f ₃ | F | A-# | Datafile | Note | pH |
|--------|-----------|--------|--------------------|--|--|---|-----|----------|---------|--------|
| SW | 6284 P01 | E5246 | 251 25=1 | = | = | = | | 6284 P01 | | |
| WW | 001 | 00A | = | = | = | | | 001 | 5-24-03 | |
| LM | L01 | | = | = | = | | | L01 | 5-4-03 | 66/6/6 |
| MS | M01 | | = | = | = | | | M01 | 3414-01 | LV |
| MSD | M01 | | = | = | = | | | M01 | 3414-01 | LV |
| MB | K01 | | = | = | = | | | K01 | | |
| Sample | 33911-01 | | = | = | = | | | 33911-01 | | LV |
| | 02 | | = | = | = | | | 02 | | |
| | 03 | | = | = | = | | | 03 | th | |
| | 3414-01 | | = | = | = | | | 3414-01 | | |
| | 02 | | = | = | = | | | 02 | | |
| | 03 | | = | = | = | | | 03 | th | ↓ |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |
| | | | = | = | = | | | | | |

| Type | Op # | STD Lot # | C _{std} (ng/μL) × V _{std} (μL) / X(g or mL) = T | Op # | STD Lot # | C _{std} (ng/μL) × V _{std} (μL) / X(g or mL) = T |
|-------|-----------|-----------|---|------|-----------|---|
| /LCSD | 3447 | GC- | x / X = ppb | | GC- | x / X = ppb |
| /MSD | 3448/3449 | GC-15162 | 200 x / X = 20 ppb | | GC- | x / X = ppb |

Note/Anomaly:

Applied P & Ch Laboratory

180 Magnolia Ave. Chino CA 91710
 (909) 590-1828 Fax: (909) 590-1498

VOC Analysis General Logbook

02692404 Batch # 02692404 Matrix: W Date: 5-15-03 Analyst: Eddie

IS/Surrogate: GC-15114/15115 Methanol(mark-M): _____ PEG (mark-PEG): _____ Defoaming(mark-DF): _____

Calib. + Ini. Batch Initial Batch; Middle Batch; Final Batch. Internal Study Datafile Path: _____

| # | Type | Sample ID | Method | $V_i/X = f_1$ | $V_j/V_i = f_2$ | $V_{avg}/V_{inj} = f_3$ | F | A-# | Datafile | Note | pH |
|------|--------|-----------|--------|---------------|-----------------|-------------------------|---|-----|----------|---------------------------|------|
| 3817 | SP | 62404P01 | E246 | 25125 = 1 | 1 = | 1 = | 1 | | 62404P01 | 5-15-03 10:18 AM | 6.45 |
| 3818 | Calib | 4-003 | 004 | 1 = | 1 = | 1 = | | | 4-003 | GC15137 | |
| 3819 | | 4-002 | | 1 = | 1 = | 1 = | | | 4-002 | | |
| 3820 | | 4-010 | | 1 = | 1 = | 1 = | | | 4-010 | | |
| 3821 | | 4-020 | | 1 = | 1 = | 1 = | | | 4-020 | | |
| 3822 | | 4-040 | | 1 = | 1 = | 1 = | | | 4-040 | | |
| 3823 | | 4-080 | | 1 = | 1 = | 1 = | | | 4-080 | | |
| 3824 | CV | 62404R01 | | 1 = | 1 = | 1 = | | | 62404R01 | CWICW 5-16-03 10:08 AM | |
| 3825 | LY | L01 | | 1 = | 1 = | 1 = | | | L01 | 6.45 | |
| 3826 | M7 | M01 | | 1 = | 1 = | 1 = | | | M01 | 37082-04 C2 | |
| 3827 | M7D | N01 | | 1 = | 1 = | 1 = | | | N01 | 37082-04 C2 | |
| 3828 | M7 | K01 | | 1 = | 1 = | 1 = | | | K01 | | |
| 3829 | Sample | 3082-01 | | 1 = | 1 = | 1 = | | | 3082-01 | | C2 |
| 3830 | | 02 | | 1 = | 1 = | 1 = | | | 02 | | |
| 3831 | | 03 | | 1 = | 1 = | 1 = | | | 03 | | |
| | | 04 | | 1 = | 1 = | 1 = | | | 04 | M7 | |
| | | 05 | | 1 = | 1 = | 1 = | | | 05 | | |
| 3834 | | 06 | | 1 = | 1 = | 1 = | | | 06 | | |
| 3835 | | 07 | | 1 = | 1 = | 1 = | | | 07 | | |
| 3836 | | 3102-01 | | 1 = | 1 = | 1 = | | | 3102-01 | | |
| 3837 | | 02 | | 1 = | 1 = | 1 = | | | 02 | | |
| 3838 | | 03 | | 1 = | 1 = | 1 = | | | 03 | | |
| 3839 | | 04 | | 1 = | 1 = | 1 = | | | 04 | | |
| 3840 | | 05 | | 1 = | 1 = | 1 = | | | 05 | | |
| 3841 | | 06 | | 1 = | 1 = | 1 = | | | 06 | | |
| 3842 | | 07 | | 1 = | 1 = | 1 = | | | 07 | | |
| 3843 | | 08 | | 1 = | 1 = | 1 = | | | 08 | | |
| 3844 | | 3115-01 | | 1 = | 1 = | 1 = | | | 3115-01 | | |
| 3845 | | 02 | | 1 = | 1 = | 1 = | | | 02 | | |
| 3846 | | 03 | | 1 = | 1 = | 1 = | | | 03 | | |
| 3847 | ✓ | 04 | ✓ | 1 = | 1 = | 1 = | ✓ | | 04 | pass 12/11/03 | |
| 3848 | | | | 1 = | 1 = | 1 = | | | | | |

| Type | Op # | STD Lot # | $C_{std}(ng/\mu L) \times V_{std}(\mu L) / X(g \text{ or } mL) = T$ | Op # | STD Lot # | $C_{std}(ng/\mu L) \times V_{std}(\mu L) / X(g \text{ or } mL) = T$ |
|----------|-----------|-----------|---|------|-----------|---|
| LCS/LCSD | 3825 | GC-15138 | $20 \times 2.5 / X =$ ppb | | GC- | $x / X =$ ppb |
| MS/MSD | 3826/3827 | GC-15138 | $20 \times 2.5 / X = 20$ ppb | | GC- | $x / X =$ ppb |

Site/Anomaly:

Level C Data Package Deliverables

8270-SIM



Applied P & Ch Laboratory
13760 Magnolia Ave. Chino, CA 91710
Telephone (909)590-1828
Fax (909)590-1498

Applied P & Ch Laboratory
Organic Analysis Results for Method 8270-SIM

| | | |
|---------------------------------|------------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 05/29/2003 |
| Project ID: JPL | Service ID: 33414 | Collected by: |
| Sample ID: 03G2697-MB-01 | Lab Sample ID: 03G2697-MB-01 | Received Date: 05/29/2003 |
| Sample Type: Method Blank | Sample Matrix: Water | Moisture %: -- |
| Anal. Method: 8270-SIM | Prep. Method: 3520 | Instrument ID: GC/MS: M |
| Batch No: 03G2697 | Prep. Date: 05/29/03 | Anal. Date: 06/03/03 |
| Data File Name: G2697K01 | Prep. No: 1 of 1 | Anal. Time: 16:07 |
| Extract Vol. 1.0 mL | Sample Amount: 1000 mL | Dilution Factor: 1 |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|--------------------------|----------------|------------|------|-------------------------|-----------------|-----------|
| 1 | 1,4-DIOXANE | 123-91-1 | µg/L | 1 | <1 | U |
| Internal Standard | | | | Control Limit, % | IS Rec.% | |
| 1 | 1,4-DIOXANE-D8 | 17647-74-4 | | 50-200 | 84 | |
| # of out-of-control | | | | | 0 | |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

| | |
|--|--|
| Qualifier: U - Not Detected or less than MDL | E - Exceed calibration range |
| J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC) | B - A positive value was found in the method blank |
| | D - Diluted |

Applied P & Ch Laboratory
Organic Analysis Results for Method 8270-SIM

| | | |
|---------------------------|--------------------------|-----------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Collection Date: 05/28/2003 |
| Project ID: JPL | Service ID: 33414 | Collected by: |
| Sample ID: MW-5 | Lab Sample ID: 03-3414-1 | Received Date: 05/28/2003 |
| Sample Type: Field Sample | Sample Matrix: Water | Moisture %: - |
| Anal. Method: 8270-SIM | Prep. Method: 3520 | Instrument ID: GC/MS: M |
| Batch No: 03G2697 | Prep. Date: 05/29/03 | Anal. Date: 06/03/03 |
| Data File Name: 3414-01 | Prep. No: 1 of 1 | Anal. Time: 23:44 |
| Extract Vol. 1.0 mL | Sample Amount: 1000 mL | Dilution Factor: 1 |

| # | Component Name | CAS No | Unit | RL | Result | Qualifier |
|----------------------------|----------------|------------|------|-------------------------|------------------|-----------|
| 1 | 1,4-DIOXANE | 123-91-1 | µg/L | 1 | < t | U |
| Internal Standard | | | | Control Limit, % | IS Rec. % | |
| 1 | 1,4-DIOXANE-D8 | 17647-74-4 | | 50-200 | 74 | |
| # of out-of-control | | | | | 0 | |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

| | |
|--|--|
| Qualifier: U - Not Detected or less than MDL | E - Exceed calibration range |
| J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC) | B - A positive value was found in the method blank |
| | D - Diluted |

FORM-3C

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 8270-SIM

Client Name: GEOFON, Inc.

Contract No:

Lab Code: APCL

Case No:

SAS No:

Service ID: 33414

Project ID: JPL

Project No: 04-4428.10

Sample Matrix: Water

Batch No: 03G2697

LCS Filename: G2697L01

Date Analyzed: 060303

Time Analyzed: 16:30

LCSD Filename: G2697J01

Date Analyzed: 060303

Time Analyzed: 16:56

| Spiked Components | Unit | Spike Added | Concentration | | LCS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|------|------------|-----------------|
| | | | Unspiked | LCS | | |
| 1,4-DIOXANE | µg/L | 20 | 0 | 19.1 | 96 | 40-140 |
| # of Out-of-control | | | | | 0 | |

| Spiked Components | Unit | Spike Added | LCSD Concentration | LCSD Rec% # | RPD% # | QC Limit, % | |
|---------------------|------|-------------|--------------------|-------------|--------|-------------|--------|
| | | | | | | RPD | REC |
| 1,4-DIOXANE | µg/L | 20 | 19.1 | 96 | 0 | 30 | 40-140 |
| # of Out-of-control | | | | 0 | 0 | | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-3C

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 8270-SIM

| | | |
|----------------------------|--------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03G2697 | |
| MS Filename: G2697M02 | Date Analyzed: 060303 | Time Analyzed: 18:10 |
| MSD Filename: G2697N02 | Date Analyzed: 060303 | Time Analyzed: 18:36 |
| MS Sample No: 09MW-01-1-GW | Sample Lab ID: 03-3401-1 | |

| Spiked Components | Unit | Spike Added | Concentration | | MS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|------|-----------|-----------------|
| | | | Unspiked | MS | | |
| 1,4-DIOXANE | µg/L | 20 | 0.7 | 20.8 | 101 | 40-140 |
| # of Out-of-control | | | | | 0 | |

| Spiked Components | Unit | Spike Added | MSD Concentration | MSD Rec% # | RPD% # | QC Limit, % RPD REC | |
|---------------------|------|-------------|-------------------|------------|--------|---------------------|------|
| | | | | | | 1,4-DIOXANE | µg/L |
| # of Out-of-control | | | | | 0 | 0 | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-4B

Applied P & Ch Laboratory

Method Blank Summary for Method 8270-SIM

| | | |
|------------------------------|--------------------------|-------------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Analysis Date: 06/03/03 |
| Sample ID: 03G2697-MB-01 | Sample Matrix: Water | Analysis Time: 16:07 |
| Lab Sample ID: 03G2697-MB-01 | Batch No: 03G2697 | Instrument ID: GC/MS: M |
| | Data File Name: G2697K01 | GC Column: DB-5.625 |
| | | Column ID: 0.25 mm |


This Method Blank applies to the following samples and QC samples:

| # | Client Sample No | Lab Sample ID | Sample Type | Data Filename | Analysis Date | Analysis Time |
|----|------------------|----------------|-----------------------------|---------------|---------------|---------------|
| 1 | 03G2697-LCS-01 | 03G2697-LCS-01 | Lab Control Spike | G2697L01 | 06/03/03 | 16:30 |
| 2 | 03G2697-LSD-01 | 03G2697-LSD-01 | Lab Control Spike Duplicate | G2697J01 | 06/03/03 | 16:56 |
| 3 | 09MW-01-1-GWMS | 03-3401-1MS | Matrix Spike | G2697M02 | 06/03/03 | 18:10 |
| 4 | 09MW-01-1-GWMSD | 03-3401-1MSD | Matrix Spike Duplicate | G2697N02 | 06/03/03 | 18:36 |
| 5 | MW-5 | 03-3414-1 | Field Sample | 3414-01 | 06/03/03 | 23:44 |
| 6 | | | | | | |
| 7 | | | | | | |
| 8 | | | | | | |
| 9 | | | | | | |
| 10 | | | | | | |
| 11 | | | | | | |
| 12 | | | | | | |
| 13 | | | | | | |
| 14 | | | | | | |
| 15 | | | | | | |
| 16 | | | | | | |
| 17 | | | | | | |
| 18 | | | | | | |
| 19 | | | | | | |
| 20 | | | | | | |
| 21 | | | | | | |
| 22 | | | | | | |
| 23 | | | | | | |
| 24 | | | | | | |
| 25 | | | | | | |

Data File : C:\HPCHEM\1\DATA\02G5027\G5027P01.D
 Acq On : 17 Dec 02 2:19 pm
 Sample : #02g5027,w dftpp gc14349
 Misc :

Vial: 99
 Operator: Andy Huang
 Inst : GC/MS - M
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\DIOSIM06.M
 Title : * Applied P & Ch Lab * GC/MS 8270



Peak Apex is scan: AVERAGE

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result |
|-------------|--------------|--------------|--------------|-----------|---------|--------|
| 51 | 198 | 30 | 80 | 44.9 | 254307 | PASS |
| 68 | 69 | 0 | 2 | 0.0 | 0 | PASS |
| 69 | 198 | 1 | 100 | 78.3 | 443243 | PASS |
| 70 | 69 | 0 | 2 | 0.3 | 1277 | PASS |
| 127 | 198 | 25 | 75 | 46.2 | 261139 | PASS |
| 197 | 198 | 0 | 1 | 0.0 | 0 | PASS |
| 198 | 198 | 100 | 100 | 100.0 | 565803 | PASS |
| 199 | 198 | 5 | 9 | 6.7 | 37981 | PASS |
| 275 | 198 | 10 | 30 | 27.4 | 155040 | PASS |
| 365 | 198 | 1 | 100 | 3.7 | 20870 | PASS |
| 441 | 443 | 1 | 99 | 78.6 | 52501 | PASS |
| 442 | 198 | 40 | 110 | 61.8 | 349717 | PASS |
| 443 | 442 | 15 | 24 | 19.1 | 66784 | PASS |

5B
SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name : APPLIED P & CH LAB Contract: _____
 Lab Code: _____ Case No.: _____ SAS No.: _____ SDG No.: 033414
 Lab File ID: G5027P01 DFTPP Injection Date: 12/17/02
 Instrument ID: GCMS-M DFTPP Injection Time: 1419

| m/e | ION ABUNDANCE CRITERIA | %RELATIVE ABUNDANCE |
|-----|-------------------------------------|---------------------|
| 51 | 30.0 - 60.0% of mass 198 | 44.9 |
| 68 | Less than 2.0% of mass 69 | 0.0 (0.0)1 |
| 69 | Mass 69 relative abundance | 78.3 |
| 70 | Less than 2.0% of mass 69 | 0.2 (0.3)1 |
| 127 | 40.0 - 60.0% of mass 198 | 46.2 |
| 197 | Less than 1.0% of mass 198 | 0.0 |
| 198 | Base Peak, 100 % relative abundance | 100.0 |
| 199 | 5.0 - 9.0% of mass 198 | 6.7 |
| 275 | 10.0 - 30.0% of mass 198 | 27.4 |
| 365 | Greater than 0.75% of mass 198 | 3.7 |
| 441 | Present, but less than mass 443 | 9.3 (78.6)3 |
| 442 | 40.0 - 100.0% of mass 198 | 61.8 |
| 443 | 17.0 - 23.0% of mass 442 | 11.8 (19.1)2 |

1-Value is % mass 69 2-Value is % mass 442 3-Value is % mass 443

This check applies to the following SAMPLES, MS, MSD, BLANKS and STANDARDS:

| | EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED | TIME ANALYZED |
|----|----------------|---------------|-------------|---------------|---------------|
| 01 | SSTD040 | DS006-40 | DS006-040.D | 12/17/2002 | 1438 |
| 02 | SSTD030 | DS006-30 | DS006-030.D | 12/17/2002 | 1457 |
| 03 | SSTD020 | DS006-20 | DS006-020.D | 12/17/2002 | 1516 |
| 04 | SSTD010 | DS006-10 | DS006-10.D | 12/17/2002 | 1536 |
| 05 | SSTD001 | DS006-01 | DS006-01.D | 12/17/2002 | 1555 |
| 06 | | | | | |
| 07 | | | | | |
| 08 | | | | | |
| 09 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |
| 23 | | | | | |

Method : C:\HPCHEM\1\METHODS\DIOSIM06.M
 Title : * Applied P & Ch Lab * GC/MS 8270
 Last Update : Tue Dec 17 16:08:23 2002
 Response via : Initial Calibration

Calibration Files
 30 =M06-030.D 20 =M06-020.D 10 =M06-010.D
 1 =M06-001.D 40 =M06-040.D


| Compound | 30 | 20 | 10 | 1 | 40 | Avg | %RSD |
|-----------------------|-------|-------|-------|-------|-------|-------|------|
| 1) I 1 1.4-Dioxane-d8 | | | | | | | |
| 2) 2 1,4-Dioxane | 1.151 | 1.165 | 1.216 | 1.379 | 1.165 | 1.215 | 7.81 |

(#) = Out of Range
 DIOSIM06.M Tue Dec 17 16:08:40 2002 5972

Data File : C:\HPCHEM\1\DATA\03G2739\G2739P02.D
 Acq On : 3 Jun 03 3:15 pm
 Sample : dftpp gc14349
 Misc :

Vial: 99
 Operator: Andy Huang
 Inst : GC/MS - M
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\DIOSIM06.M
 Title : * Applied P & Ch Lab * GC/MS 8270



Peak Apex is scan: 88

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result |
|-------------|--------------|--------------|--------------|-----------|---------|--------|
| 51 | 198 | 30 | 80 | 54.6 | 331904 | PASS |
| 68 | 69 | 0 | 2 | 0.0 | 0 | PASS |
| 69 | 198 | 1 | 100 | 85.2 | 517952 | PASS |
| 70 | 69 | 0 | 2 | 0.0 | 0 | PASS |
| 127 | 198 | 25 | 75 | 46.6 | 283392 | PASS |
| 197 | 198 | 0 | 1 | 0.0 | 0 | PASS |
| 198 | 198 | 100 | 100 | 100.0 | 607808 | PASS |
| 199 | 198 | 5 | 9 | 6.6 | 40096 | PASS |
| 275 | 198 | 10 | 30 | 27.7 | 168576 | PASS |
| 365 | 198 | 1 | 100 | 3.7 | 22656 | PASS |
| 441 | 443 | 1 | 99 | 80.2 | 73952 | PASS |
| 442 | 198 | 40 | 110 | 77.1 | 468352 | PASS |
| 443 | 442 | 15 | 24 | 19.7 | 92192 | PASS |

FORM-5B

Applied P & Ch Laboratory

**Semivolatile Organic Instrument Performance Check for Method 8270-SIM
Decafluorotriphenylphosphine (DFTPP), Part II**

| | | |
|---------------------------|----------------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 033414 |
| Project ID: JPL | DFTPP Inj. Date: <u>06/03/03</u> | Batch No: 03G2697 |
| | DFTPP Inj. Time: <u>15:15</u> | Sequence No: 03G2739 |
| Project No: 04-4428.10 | Instrument ID: M | GC Column: DB-5.625 |
| Data File Name: G2739P02 | | Column ID: 0.25 mm |

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS AND STANDARDS:

| # | Client Sample No | Lab Sample ID | Data File Name | Date Analyzed | Time Analyzed |
|----|------------------|----------------|----------------|---------------|---------------|
| 1 | 03G2697-CCV-01 | 03G2697-CCV-01 | G2739Q02 | 06/03/03 | 15:45 |
| 2 | 03G2697-MB-01 | 03G2697-MB-01 | G2697K01 | 06/03/03 | 16:07 |
| 3 | 03G2697-LCS-01 | 03G2697-LCS-01 | G2697L01 | 06/03/03 | 16:30 |
| 4 | 03G2697-LSD-01 | 03G2697-LSD-01 | G2697J01 | 06/03/03 | 16:56 |
| 5 | 09MW-01-1-GWMS | 03-3401-1MS | G2697M02 | 06/03/03 | 18:10 |
| 6 | 09MW-01-1-GWMSD | 03-3401-1MSD | G2697N02 | 06/03/03 | 18:36 |
| 7 | MW-5 | 03-3414-1 | 3414-01 | 06/03/03 | 23:44 |
| 8 | | | | | |
| 9 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |
| 23 | | | | | |
| 24 | | | | | |
| 25 | | | | | |

FORM-7B

Applied P & Ch Laboratory

CCV Recovery for Method 8270-SIM

Client Name: GEOFON, Inc.
 Case No:
 Project ID: JPL
 CCV File: G2739Q02

Contract No.:
 SAS No.:
 Project No.: 04-4428.10
 Batch No.: 03G2697
 Date Analyzed: 06/03/2003

Lab Code: APCL
 Service ID: 33414
 Instrument: M
 Sequence No.: 03G2739
 Time Analyzed: 15:45

Target Components

| # | Component Name | Unit | Expe- cted | Test Result | Rec. % | Dev. % | Flag | Control Limit, % | by |
|---------------------------------|----------------|------|---------------|----------------|-----------|-----------|------|---------------------|-----|
| 1 | 1,4-DIOXANE | mg/L | 20 | 19.4 | 97 | -3 | ✓ | 80-120 | CCV |
| Total CCV Out of Control | | | | | | | 0 | | |

FORM-8B

Applied P & Ch Laboratory

Internal Standard Area and RT Summary for Method 8270-SIM

Client Name: GEOFON, Inc. Contract No: Lab Code: APCL
 Case No: SAS No: Service ID: 033414
 Project ID: JPL Project No: 04-4428.10 Sample Matrix: Water
 CCV Data File: G2739Q02 Instrument ID: M
 Batch No: 03G2697

| # | Client Sample No | Lab Sample ID | Analysis Date & Time | IS-1 | |
|-----------------|------------------|----------------|----------------------|--------|------|
| | | | | Area # | RT # |
| 12 Hour CCV STD | | | 06/03/03 15:45 | 483801 | 4.03 |
| CCV Upper Limit | | | | 967602 | 4.53 |
| CCV Lower Limit | | | | 241900 | 3.53 |
| 1 | 03G2697-MB-01 | 03G2697-MB-01 | 06/03/03 16:07 | 403974 | 4.14 |
| 2 | 03G2697-LCS-01 | 03G2697-LCS-01 | 06/03/03 16:30 | 348169 | 4.21 |
| 3 | 03G2697-LSD-01 | 03G2697-LSD-01 | 06/03/03 16:56 | 357813 | 4.18 |
| 4 | 09MW-01-1-GWMS | 03-3401-1MS | 06/03/03 18:10 | 352352 | 4.19 |
| 5 | 09MW-01-1-GWMSD | 03-3401-1MSD | 06/03/03 18:36 | 347620 | 4.15 |
| 6 | MW-5 | 03-3414-1 | 06/03/03 23:44 | 357841 | 4.36 |
| 7 | | | | | |
| 8 | | | | | |
| 9 | | | | | |
| 10 | | | | | |
| 11 | | | | | |
| 12 | | | | | |
| 13 | | | | | |
| 14 | | | | | |
| 15 | | | | | |
| 16 | | | | | |
| 17 | | | | | |
| 18 | | | | | |
| 19 | | | | | |
| 20 | | | | | |
| 21 | | | | | |
| 22 | | | | | |

IS-1 = 1,4-DIOXANE-D8

Area Upper Limit = +100% of CCV internal standard area
 Area Lower Limit = - 50% of CCV internal standard area
 RT Upper Limit = +0.50 minutes of CCV internal standard RT
 RT Lower Limit = - 0.50 minutes of CCV internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits

Applied P & Ch Laboratory

Log-121

13760 Magnolia Ave. Chino CA 91710
Tel: (909) 590-1828 Fax: (909) 590-1498

Organic Sample Preparation Logbook

Batch # 0242697 Matrix: W Target method: 1,4-Dioxane EXT Method: 3520C
Solvent: CH2Cl2 Lot # 027471 Exchange Solvent: NA Lot # NA
Lot #: Surr.: GC Conc.: _____ ppm Na2SO4: Ke 0078

Date: 5/29/03
Analyst: rdl

| Op. # | Sample Type | Sample ID # | Smpl Amnt (mL or g) | Surr. Vol mL | Extract sub-ID | Final Vol. mL | Dilution F=V/X | Note & Anomaly |
|-------|-------------|-------------|---------------------|--------------|----------------|---------------|----------------|----------------|
| 4601 | MB | 0342697-K01 | 1000.0 | NA | 1,4-Dioxane | 1.00 | 0.001 | |
| 4602 | LCS | -201 | 1000.0 | | | | | |
| 4603 | LCSD | -501 | 1000.0 | | | | | |
| 4604 | Sample-1 | 3381-1 | 1000.0 | | | | | |
| 4605 | MS | -5 | 1000.0 | | | | | |
| 4606 | MSD | -5 | 1000.0 | | | | | |
| 4607 | Sample-2 | -2 | 1000.0 | | | | | |
| 4608 | Sample-3 | -3 | 1000.0 | | | | | |
| 4609 | Sample-4 | -4 | 1000.0 | | | | | |
| 4610 | Sample-5 | -5 | 1000.0 | | | | | |
| 4611 | Sample-6 | -6 | 1000.0 | | | | | |
| 4612 | Sample-7 | -7 | 1000.0 | | | | | |
| 4613 | Sample-8 | 3391-1 | 1000.0 | | | | | |
| 4614 | Sample-9 | -2 | 1000.0 | | | | | |
| 4615 | Sample-10 | 3401-1 | 1000.0 | | | | | |
| 4616 | Sample-11 | -2 | 1000.0 | | | | | |
| 4617 | Sample-12 | -3 | 1000.0 | | | | | |
| 4618 | Sample-13 | 3414-1 | 1000.0 | | | | | |
| 4619 | Sample-14 | 3421-8 | 1000.0 | | | | | |
| 4620 | Sample-15 | | | | | | | |
| 4621 | Sample-16 | | | | | | | |
| 4622 | Sample-17 | | | | | | | |
| 4623 | Sample-18 | | | | | | | |
| 4624 | Sample-19 | | | | | | | |
| 4625 | Sample-20 | | | | | | | |
| 4626 | MTX Dup. | | | | | | | |
| 4627 | LCS' | | | | | | | |
| 4628 | LCSD' | | | | | | | |
| 4629 | MS' | 3401-1 | 1000.0 | NA | 1,4-Dioxane | 1.00 | 0.001 | |
| 4630 | MSD' | -1 | 1000.0 | | | | | |

rdl
5/29/03

| Type | Op # | STD Lot # | $C_{std}(ppm) \times V_{std}(mL) / X(g \text{ or } mL) = T$ | Op # | STD Lot # | $C_{std}(ppm) \times V_{std}(mL) / X(g \text{ or } mL) = T$ |
|------------|------|-----------|---|------|-----------|---|
| LCS/LCSD | 4602 | GC-15154 | $1000 \times 20.0 \times 1.00 / X =$ ppb | 4603 | GC-15154 | $1000 \times 20.0 \times 1.00 / X =$ ppb |
| MS/MSD | 4605 | GC- ↓ | $1000 \times \downarrow \times \downarrow / X =$ ppb | 4606 | GC- ↓ | $1000 \times \downarrow \times \downarrow / X =$ ppb |
| LCS'/LCSD' | | GC- | $1000 \times \times / X =$ ppb | | GC- | $1000 \times \times / X =$ ppb |
| MS'/MSD' | 4629 | GC- ↓ | $1000 \times \downarrow \times \downarrow / X =$ ppb | 4630 | GC- ↓ | $1000 \times \downarrow \times \downarrow / X =$ ppb |

Supervisor Initial rdl

Organic Sample Preparation

Extraction method: 1 3510-separate funnel; 2 3520-L-L continue extraction; 3 3550-Ultrasonic; 4 LUFT-Shaker; 5 3540-Soxhlet;
6 Solid phase Extraction; 7 Microextraction; 8 SFE; 9 Dilution; 10 Concentration; 11 Other, specify.

Service ID: 3381 Batch # 03G2697 Matrix W GC, GC/MS Method 14 Dioxane Ext Method 3520C

Sample Extraction
OP. by jde Date 5/29/03 Surro Lot GC-NA Conc. NA pp
LCS Lot GC-15154 Conc. 20.0 pp MS Lot GC-15154 Conc. 20.0 pp
Ext. solv. CH₂Cl₂ Lot # 027471 Exchange solv. NA Lot # NA

Sample ID -K01 -L01 -J01 -5115 -5 MSD -1 -2 -3

Sample Matrix W

Sample Amount, X (g/mL) 1000.0 1000.0 1000.0 1000.0 1000.0 1000.0 1000.0 1000.0

Any TCLP, EP, WET, SPLP ? _____

Surr. STD used, mL NA

Spike STD used, mL 1.00

[Extracted at pH] 1 1 1 1 1 1 1 1

Solvent amount, mL 300 X X X X X X X

Final volume, V_i mL 1.00

Extraction DF f_e = V_i/X 0.001

Sub-ID of extracts 1,4 Dioxane

Anomaly Footnote† : _____

Sample Cleanup Op. by _____ Date / / (For details, see Cleanup worksheet)

Cleanup method: _____

Cleanup DF, f_c _____

Preparation DF, f₁ = f_e f_c _____

Pre-injection* : Op. by _____ Date / / IS Lot : GC Conc. _____ pp

2nd dilution, f₂ (1) _____

V_i, μL (40) _____

Single Extract GC, GC/MS Analysis:

V₂ = V_i/f₂, μL (40/f₂) _____

V_{solvent} = V_i - V₂, μL _____

Double Extract GC, GC/MS Analysis:

V_> = 1/2 V_i/f₂, μL (20/f₂) _____

V_< = 1/2 V_i f_</f_>, μL (20 f_</f_>) _____

V_{solvent} = V_i - V_> - V_< _____

IS volume, μL (10) _____

Final Conc. of IS (40 ppm) _____

Total F = 2 f₁ f_> or f₁ f₂ _____

† Extraction Anomaly Footnote:

- | | | |
|--|--|----------------------------|
| 1. Difficult to concentrate to 1.0 mL. | 5. Too much precipitate during extraction. | 9. Sample has strong stink |
| 2. Extract is dark color | 6. There is an oil layer above the sample. | 10. Some solvent suspected |
| 3. Extract is sticky | 7. Mixture of soil & water. | 11. special color, specify |
| 4. Heterogenous matrix. | 8. BN-extract is interfered, A-extract only. | |

* For double extract analysis (ABN), f_> = max[f_A, f_B] and f_< = min[f_A, f_B], where f_A, f_B are f₁ for A and BN extracts, respectively. The values in () is the typical case for 625/8270 ABN analysis.

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Organic Sample Preparation

Extraction method: 1 3510-separate funnel; 2 3520-L-L continue extraction; 3 3550-Ultrasonic; 4 LUFT-Shaker; 5 3540-Soxhlet;
6 Solid phase Extraction; 7 Microextraction; 8 SFE; 9 Dilution; 10 Concentration; 11 Other, specify.

Service ID: 3414 Batch # 0242697 Matrix W GC, GC/MS Method 14 Dioxane Ext Method 3520C

Sample Extraction
 OP. by jde Date 5/29/03 Surro Lot GC-NA Conc. NA pp
 LCS Lot GC-15154 Conc. 20.0 pp MS Lot GC-15154 Conc. 20.0 pp
 Ext. solv. CH₂Cl₂ Lot # 027471 Exchange solv. NA Lot # NA

Sample ID -1
 Sample Matrix W
 Sample Amount, X (g/mL) 1000.0
 Any TCLP, EP, WET, SPLP ?
 Surr. STD used, mL NA
 Spike STD used, mL
 [Extracted at pH] 1 1 1 1 1 1 1 1
 Solvent amount, mL 200 X X X X X X X
 Final volume, V, mL 1.00
 Extraction DF $f_e = V/X$ 0.001
 Sub-ID of extracts 1,4 Dioxane
 Anomaly Footnote† :

Sample Cleanup
 Op. by _____ Date / / (For details, see Cleanup worksheet)
 Cleanup method:
 Cleanup DF, f_c
 Preparation DF, $f_1 = f_e f_c$

Pre-injection* : Op. by _____ Date / / IS Lot : GC- Conc. _____ pp
 2nd dilution, f_2 (1) _____
 $V_t, \mu L$ (40) _____

Single Extract GC, GC/MS Analysis:
 $V_2 = V_t / f_2, \mu L$ (40/ f_2) _____
 $V_{solvent} = V_t - V_2, \mu L$ _____

Double Extract GC, GC/MS Analysis:
 $V_{>} = \frac{1}{2} V_t / f_2, \mu L$ (20/ f_2) _____
 $V_{<} = \frac{1}{2} \frac{V_t f_{<}}{f_2 f_{>}}, \mu L$ ($\frac{20 f_{<}}{f_2 f_{>}}$) _____
 $V_{solvent} = V_t - V_{>} - V_{<}$ _____
 IS volume, μL (10) _____
 Final Conc. of IS (40 ppm) _____
 Total $F = 2 f_1 f_{>} \text{ or } f_1 f_2$ _____

† Extraction Anomaly Footnote:

- | | | |
|--|--|----------------------------|
| 1. Difficult to concentrate to 1.0 mL. | 5. Too much precipitate during extraction. | 9. Sample has strong stink |
| 2. Extract is dark color | 6. There is an oil layer above the sample. | 10. Some solvent suspected |
| 3. Extract is sticky | 7. Mixture of soil & water. | 11. special color, specify |
| 4. Heterogenous matrix. | 8. BN-extract is interfered, A-extract only. | |

* For double extract analysis (ABN), $f_{>} = \max[f_A, f_B]$ and $f_{<} = \min[f_A, f_B]$, where f_A, f_B are f_1 for A and BN extracts, respectively.
 The values in () is the typical case for 625/8270 ABN analysis.

Sequence # 0362739

Starting Date: 6/2/03 Time 4:49 pm Analyst: JH

Seq. type: Cal. Ini. Batch Middle Final Continue Study

Datafile Path: E:\APCL\BEM\11\DATA\0362739

Routine Maintenance: Replace Septum Replace Liner Replace Seal Cut Guid Column Cut Column Others

| Op. # | Batch-No | MTX | S Type* | Sample ID | Method** | f ₂ | F | A-# | Datafile | OK ?† | Note†† |
|-------|----------|-----|---------|-----------|----------|----------------|--------|-----|----------|-------|--------------------|
| 1241 | | | SP | 62739P01 | DFTPP625 | | | 99 | 62739P01 | / | 6/2/03 4:49 pm. |
| 1242 | | | CCV | 0201 | DIOSIM06 | | | 100 | 0201 | / | GC14349 |
| 1243 | 0362739 | S | MB | K01 | | | 0.0333 | 1 | K01 | / | GC15755 |
| 1244 | | | LCS | L01 | | | | 2 | L01 | / | |
| 1245 | | | LCSD | J01 | | | | 3 | J01 | / | |
| 1246 | | | MS | M01 | | | | 4 | M01 | / | #3475-02 |
| 1247 | | | MSD | N01 | | | | 5 | N01 | / | 1 |
| 1248 | | | | 3475-02 | | | | 6 | 3475-02 | / | |
| 1249 | | | | 3475-04 | | | | 7 | -04 | / | |
| 1250 | 0362739 | W | SP | 62739P02 | DFTPP625 | | | 99 | 62739P02 | / | 6/3/03 3:25 pm. |
| 1251 | | | CCV | 0202 | DIOSIM06 | | | 100 | 62739P02 | / | GC14349 |
| 1252 | | | MB | 62697K01 | | | 0.001 | 1 | 62697K01 | / | GC15155 |
| 1253 | | | LCS | L01 | | | | 2 | L01 | / | |
| 1254 | | | LCSD | J01 | | | | 3 | J01 | / | |
| 1255 | | | MS | M01 | | | | 4 | M01 | / | |
| 1256 | | | MSD | N01 | | | | 5 | N01 | / | |
| 1257 | | | MS' | M02 | | | | 6 | M02 | / | |
| 1258 | | | MSD' | N02 | | | | 7 | N02 | / | |
| 1259 | | | | 3381-01 | | | | 8 | 3381-01 | / | |
| 1260 | | | | -02 | | | | 9 | -02 | / | |
| 1261 | | | | -03 | | | | 10 | -03 | / | |
| 1262 | | | | -04 | | | | 11 | -04 | / | |
| 1263 | | | | -05 | | | | 12 | -05 | / | |
| 1264 | | | | -06 | | | | 13 | -06 | / | |
| 1265 | | | | -07 | | | | 14 | -07 | / | |
| 1266 | | | | 3391-01 | | | | 15 | 3391-01 | / | |
| 1267 | | | | -02 | | | | 16 | -02 | / | |
| 1268 | | | | 3401-01 | | | | 17 | 3401-01 | / | |
| 1269 | | | | -02 | | | | 18 | -02 | / | |
| 1270 | | | | -03 | | | | 19 | -03 | / | |

Footnote/Anomaly:

* Sample type such as, SP(BFB, or DFTPP), CCV, CVA, CVB, LCS, LCSD, MS, MSD, MD, CLS etc. For field samples leave as blank.
 ** Method name: [MMMM][S][nnn]. [MMMM] - method code, per SOP C-88. Special codes: DSL2: Diesel #2; FP30: Fuel Finger Print (C8-C30); FP40: Fuel Finger Print (C8-C40); EGLY: Ethylene Glycol; FORM: Formaldehyde; MEOH: Methyl Alcohol. [S] - APCL system code; [nnn] - initial calibration number.
 † Specify the result of the injection is accepted (✓), or denied (X), or need Re-run (R) or use as a reference data (ref).
 †† Lot # for CCV/Closing, Time for SP (e.g. DFTPP) must be recorded.

656

Semi-VOC Analysis Logbook

M

Sequence # 0362739

Starting Date: 6/2/03 Time 4:49 pm Analyst: J-F

Seq. type: Cal. Ini. Batch Middle Final Continue Study

Datafile Path: 01\PPCH\BGM\1\DATA\0362739

Routine Maintenance: Replace Septum Replace Liner Replace Seal Cut Guid Column Cut Column Others

| Op. # | Batch-No | MTX | S Type* | Sample ID | Method** | f ₂ | F | A-# | Datafile | OK ?† | Note†† |
|-------|----------|-----|---------|-----------|----------|----------------|-------|-----|----------|-------|--------|
| 1271 | 0362739 | W | | 3414-01 | D10S0106 | | 0.001 | 20 | 3414-01 | / | |
| 1272 | 1 | 1 | | 3421-08 | 1 | | 1 | 21 | 3421-08 | / | |
| 1273 | | | | | | | | | | | |
| 1274 | | | | | | | | | | | |
| 1275 | | | | | | | | | | | |
| 1276 | | | | | | | | | | | |
| 1277 | | | | | | | | | | | |
| 1278 | | | | | | | | | | | |
| 1279 | | | | | | | | | | | |
| 1280 | | | | | | | | | | | |
| 1281 | | | | | | | | | | | |
| 1282 | | | | | | | | | | | |
| 1283 | | | | | | | | | | | |
| 1284 | | | | | | | | | | | |
| 1285 | | | | | | | | | | | |
| 1286 | | | | | | | | | | | |
| 1287 | | | | | | | | | | | |
| 1288 | | | | | | | | | | | |
| 1289 | | | | | | | | | | | |
| 1290 | | | | | | | | | | | |
| 1291 | | | | | | | | | | | |
| 1292 | | | | | | | | | | | |
| 1293 | | | | | | | | | | | |
| 1294 | | | | | | | | | | | |
| 1295 | | | | | | | | | | | |
| 1296 | | | | | | | | | | | |
| 1297 | | | | | | | | | | | |
| 1298 | | | | | | | | | | | |
| 1299 | | | | | | | | | | | |
| 1300 | | | | | | | | | | | |

Com 6/2/03

Footnote/Anomaly:

* Sample type such as, SP(BFB, or DFTPP), CCV, CVA, CVB, LCS, LCSD, MS, MSD, MD, CLS etc. For field samples leave as blank.
 ** Method name: [MMMM][S][nnn]. [MMMM] - method code, per SOP C-88. Special codes: DSL2: Diesel #2; FP30: Fuel Finger Print (C8-C30); FP40: Fuel Finger Print (C8-C40); EGLY: Ethylene Glycol; FORM: Formaldehyde; MEQH: Methyl Alcohol. [S] - APCL system code; [nnn] - initial calibration number.
 † Specify the result of the injection is accepted (✓), or denied (X), or need Re-run (R) or use as a reference data (ref).
 †† Lot # for CCV/Closing, Time for SP (e.g. DFTPP) must be recorded.

Supervisor Initial

[Signature]

Semi-VOC Analysis Logbook

M LOG-063

Sample # 026502

Starting Date: 12-17-02 Time 2:19 pm Analyst: J.Y.

Sample type: Cal. Ini. Batch Middle Final Continue Study
 Line Maintenance: Replace Septum Replace Liner Replace Seal Cut Guid Column Cut Column Others

Datafile Path: _____

| Batch-No | MTX | S Type* | Sample ID | Method** | f ₂ | F | A-# | Datafile | OK ?† | Note†† |
|----------|-----|---------|-----------|----------|----------------|----------|-----|----------|-------|---------------------|
| | | SP | 65027P01 | DFTPP625 | | | 99 | 65027P01 | ✓ | 12-17-02 2:19 pm |
| | | Cali- | M06-040 | D10S1M06 | | | 1 | M06-040 | ✓ | Koppin 6214354 |
| | | | -030 | | | | 2 | -030 | ✓ | 30 |
| | | | -020 | | | | 3 | -020 | ✓ | 20 |
| | | | -010 | | | | 4 | -010 | ✓ | 10 |
| | | | -001 | | | | 5 | -001 | ✓ | 1 |
| | | CCV | 65027Q01 | | | | 100 | 65027Q01 | ✓ | 6214354 |
| 026502 | W | MR | K01 | | | 0.001 | 6 | K01 | - | |
| | | LCS | L01 | | | | 7 | L01 | - | |
| | | LCSD | J01 | | | | 8 | J01 | - | |
| | | MS | M01 | | | | 9 | M01 | - | \$6556-03 |
| | | MSD | N01 | | | | 10 | N01 | - | 1 |
| | | MS' | M02 | | | 0.000962 | 11 | M02 | - | \$6587-01 |
| | | MSD' | N02 | | | | 12 | N02 | - | 1 |
| | | | 6587-01 | | | | 13 | 6587-01 | - | |
| | | | -02 | | | | 14 | -02 | - | |
| | | | -03 | | | | 15 | -03 | - | |
| | | | 6556-01 | | | 0.002 | 16 | 6556-01 | - | |
| | | | -02 | | | 0.001 | 17 | -02 | - | |
| | | | -03 | | | | 18 | -03 | - | |
| | | | 6588-01 | | | 0.000962 | 19 | 6588-01 | - | |
| | | | 6603-01 | | | | 20 | 6603-01 | - | |
| | | | -02 | | | | 21 | -02 | - | |
| | | | 6558-01 | | | | 22 | 6558-01 | - | |
| | | | -03 | | | 0.001 | 23 | -03 | - | |
| | | | 6586-02 | | | | 24 | 6586-02 | - | |
| | | | -04 | | | | 25 | -04 | - | |
| | | | -05 | | | | 26 | -05 | - | |
| | | | -06 | | | | 27 | -06 | - | Reverse side |
| | | | -08 | | | | 28 | -08 | ↓ | ✓ |

Footnote/Anomaly:

* Sample type such as, SP(BFB, or DFTPP), CCV, CVA, CVB, LCS, LCSD, MS, MSD, MD, CLS etc. For field samples leave as blank.
 ** Method name: [MMMM][S][nnn]. [MMMM] - method code, per SOP C-88. Special codes: DSL2: Diesel #2; FP30: Fuel Finger Print (C8-C30); FP40: Fuel Finger Print (C8-C40); EGLY: Ethylene Glycol; FORM: Formaldehyde; MEOH: Methyl Alcohol. [S] - APCL system code; [nnn] - initial calibration number.
 † Specify the result of the injection is accepted (✓), or denied (X), or need Re-run (R) or use as a reference data (ref).
 †† Lot # for CCV/Closing, Time for SP (e.g. DFTPP) must be recorded.

Level C Data Package Deliverables

Metals



Applied P & Ch Laboratory

Applied P & Ch Laboratory
Metal Analysis Results

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 33414

Collection Date: 06/02/2003
 Collected by:

Sample ID: 03M1535-MB-01
 Sample Type: Method Blank

Lab Sample ID: 03M1535-MB-01
 Sample Matrix: Water

Received Date: 06/02/2003
 Moisture %: --

| Element Name | CAS No | Unit | RL | Result | C | M | Q | Batch | D-Date | A-Date | DF | Method |
|--------------|-----------|------|------|--------|---|---|---|----------|----------|----------|----|--------|
| ARSENIC | 7440-38-2 | µg/L | 5 | < 5 | U | F | | 03M1535E | 06/02/03 | 06/02/03 | 1 | 200.9 |
| CALCIUM | 7440-70-2 | µg/L | 200 | < 200 | U | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| IRON | 7439-89-6 | µg/L | 50 | 5.1 | B | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| MAGNESIUM | 7439-95-4 | µg/L | 100 | 49.4 | B | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| POTASSIUM | 7440-09-7 | µg/L | 400 | 156 | B | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| SODIUM | 7440-23-5 | µg/L | 2000 | < 2000 | U | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: RL: PQL (EQL) or CRDL D-Date: Digestion Date; A-Date: Analysis Date; DF: Dilution Factor

C Qualifier: U - Not Detected or less than IDL

B - Less than RL (PQL, EQL or CRDL), but greater than IDL.

Q Qualifier: N - Spike recovery out of control

* - Duplicate analysis out of control

W - Post digestion spike for GFAA out of control

E - Serial dilution difference out of control

M Qualifier: P - ICP

A - FLAA

F - GFAA

CV - Cold Vapor

Applied P & Ch Laboratory
Metal Analysis Results

Client Name: GEOFON, Inc.
Project ID: JPL
Sample ID: MW-5
Sample Type: Field Sample

Project No: 04-4428.10
Service ID: 33414
Lab Sample ID: 03-3414-1
Sample Matrix: Water

Collection Date: 05/28/2003
Collected by:
Received Date: 05/28/2003
Moisture %: -

| Element Name | CAS No | Unit | RL | Result | C | M | Q | Batch | D-Date | A-Date | DF | Method |
|--------------|-----------|------|------|--------|---|---|---|----------|----------|----------|----|--------|
| ARSENIC | 7440-38-2 | µg/L | 5 | < 5 | U | F | | 03M1535E | 06/02/03 | 06/02/03 | 1 | 200.9 |
| CALCIUM | 7440-70-2 | µg/L | 200 | 45300 | | | P | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| IRON | 7439-89-6 | µg/L | 50 | 357 | | | P | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| MAGNESIUM | 7439-95-4 | µg/L | 100 | 13800 | | | P | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| POTASSIUM | 7440-09-7 | µg/L | 400 | 2740 | | | P | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| SODIUM | 7440-23-5 | µg/L | 2000 | 16500 | | | P | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: RL: PQL (EQL) or CRDL D-Date: Digestion Date; A-Date: Analysis Date; DF: Dilution Factor

C Qualifier: U - Not Detected or less than IDL

B - Less than RL (PQL, EQL or CRDL), but greater than IDL.

Q Qualifier: N - Spike recovery out of control

* - Duplicate analysis out of control

W - Post digestion spike for GFAA out of control

E - Serial dilution difference out of control

M Qualifier: P - ICP

A - FLAA

F - GFAA

CV - Cold Vapor

Applied P & Ch Laboratory
Metal Analysis Results

Client Name: GEOFON, Inc.

Project No: 04-4428.10

Collection Date: 05/28/2003

Project ID: JPL

Service ID: 33414

Collected by:

Lab Sample ID: 03-3414-2

Received Date: 05/28/2003

Sample ID: MW-8

Sample Matrix: Water

Moisture %: -

Sample Type: Field Sample

| Element Name | CAS No | Unit | RL | Result | C | M | Q | Batch | D-Date | A-Date | DF | Method |
|--------------|-----------|------|------|--------|---|---|---|----------|----------|----------|----|--------|
| ARSENIC | 7440-38-2 | µg/L | 5 | 2.0 | B | F | | 03M1535E | 06/02/03 | 06/02/03 | 1 | 200.9 |
| CALCIUM | 7440-70-2 | µg/L | 200 | 52300 | | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| IRON | 7439-89-6 | µg/L | 50 | 48.7 | B | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| MAGNESIUM | 7439-95-4 | µg/L | 100 | 16500 | | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| POTASSIUM | 7440-09-7 | µg/L | 400 | 2450 | | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |
| SODIUM | 7440-23-5 | µg/L | 2000 | 18000 | | P | | 03M1525L | 05/29/03 | 05/29/03 | 1 | 200.7 |

Note: RL: PQL (EQL) or CRDL D-Date: Digestion Date; A-Date: Analysis Date; DF: Dilution Factor

C Qualifier: U - Not Detected or less than IDL

B - Less than RL (PQL, EQL or CRDL), but greater than IDL.

Q Qualifier: N - Spike recovery out of control

* - Duplicate analysis out of control

W - Post digestion spike for GFAA out of control

E - Serial dilution difference out of control

M Qualifier: P - ICP

A - FLAA

F - GFAA

CV - Cold Vapor

FORM-2A Metal
Applied P & Ch Laboratory
Initial and Continuing Calibration Verification

Client Name: GEOFON, Inc.

Project No: 04-4428.10

Lab Code: APCI

Project Name: JPL

Service ID: 033414

Sequence No.: 03M15251

Instrument: ICP -L

Method: 200.9

Batch No.(s): 03M1525

Analysis Date: 05/29/03

Concentration Units: UG/L

| # | Analyte | ICV 11:48 | | | CCV 12:07 | | | CCV 13:04 | | | CCV 13:42 | | |
|----|------------|-----------|-----------|-------|-----------|-----------|-------|-----------|----------|------|-----------|----------|------|
| | | True | Result | %R | True | Result | %R | True | Result | %R | True | Result | %R |
| 1 | Aluminum | 10000.0 | 9961.00 | 99.6 | 5000.0 | 5302.64 | 106.1 | 5000.0 | 4794.09 | 95.9 | 5000.0 | 4825.23 | 96.5 |
| 2 | Antimony | 4000.0 | 3994.99 | 99.9 | 2000.0 | 2051.36 | 102.6 | 2000.0 | 1961.18 | 98.1 | 2000.0 | 1970.19 | 98.5 |
| 3 | Arsenic | 1000.0 | 995.39 | 99.5 | 500.0 | 507.93 | 101.6 | 500.0 | 480.98 | 96.2 | 500.0 | 489.86 | 98.0 |
| 4 | Barium | 10000.0 | 9779.38 | 97.8 | 5000.0 | 5159.57 | 103.2 | 5000.0 | 4778.21 | 95.6 | 5000.0 | 4906.47 | 98.1 |
| 5 | Beryllium | 1000.0 | 986.85 | 98.7 | 500.0 | 497.96 | 99.6 | 500.0 | 465.29 | 93.1 | 500.0 | 480.06 | 96.0 |
| 6 | Cadmium | 2000.0 | 1969.19 | 98.5 | 1000.0 | 1033.76 | 103.4 | 1000.0 | 984.24 | 98.4 | 1000.0 | 994.41 | 99.4 |
| 7 | Calcium | 100000.0 | 101169.99 | 101.2 | 50000.0 | 50933.90 | 101.9 | 50000.0 | 48533.82 | 97.1 | 50000.0 | 48869.72 | 97.7 |
| 8 | Chromium | 1000.0 | 985.56 | 98.6 | 500.0 | 517.87 | 103.6 | 500.0 | 484.29 | 96.9 | 500.0 | 488.64 | 97.7 |
| 9 | Cobalt | 4000.0 | 3928.68 | 98.2 | 2000.0 | 2079.33 | 104.0 | 2000.0 | 1970.50 | 98.5 | 2000.0 | 1989.71 | 99.5 |
| 10 | Copper | 4000.0 | 3985.57 | 99.6 | 2000.0 | 2058.27 | 102.9 | 2000.0 | 1978.06 | 98.9 | 2000.0 | 1995.25 | 99.8 |
| 11 | Iron | 10000.0 | 9841.19 | 98.4 | 5000.0 | 5228.99 | 104.6 | 5000.0 | 4841.45 | 96.8 | 5000.0 | 4881.64 | 97.6 |
| 12 | Lead | 1000.0 | 975.57 | 97.6 | 500.0 | 502.74 | 100.5 | 500.0 | 474.40 | 94.9 | 500.0 | 475.12 | 95.0 |
| 13 | Magnesium | 50000.0 | 48949.84 | 97.9 | 25000.0 | 25608.29 | 102.4 | 25000.0 | 23506.31 | 94.0 | 25000.0 | 23732.96 | 94.9 |
| 14 | Manganese | 4000.0 | 3925.63 | 98.1 | 2000.0 | 2058.65 | 102.9 | 2000.0 | 1926.86 | 96.3 | 2000.0 | 1983.50 | 99.2 |
| 15 | Nickel | 4000.0 | 3917.81 | 97.9 | 2000.0 | 2074.07 | 103.7 | 2000.0 | 1964.22 | 98.2 | 2000.0 | 1985.35 | 99.3 |
| 16 | Potassium | 30000.0 | 29967.49 | 99.9 | 15000.0 | 14859.19 | 99.1 | 15000.0 | 13933.23 | 92.9 | 15000.0 | 14346.56 | 95.6 |
| 17 | Selenium | 1000.0 | 989.38 | 98.9 | 500.0 | 510.16 | 102.0 | 500.0 | 475.47 | 95.1 | 500.0 | 480.02 | 96.0 |
| 18 | Silver | 2000.0 | 1999.98 | 100.0 | 1000.0 | 1031.29 | 103.1 | 1000.0 | 980.77 | 98.1 | 1000.0 | 978.16 | 97.8 |
| 19 | Sodium | 200000.0 | 199352.77 | 99.7 | 100000.0 | 102633.21 | 102.6 | 100000.0 | 96864.63 | 96.9 | 100000.0 | 97874.49 | 97.9 |
| 20 | Thallium | 1000.0 | 993.55 | 99.4 | 500.0 | 517.53 | 103.5 | 500.0 | 483.60 | 96.7 | 500.0 | 484.59 | 96.9 |
| 21 | Vanadium | 4000.0 | 3976.86 | 99.4 | 2000.0 | 2059.93 | 103.0 | 2000.0 | 1939.43 | 97.0 | 2000.0 | 1954.53 | 97.7 |
| 22 | Zinc | 4000.0 | 3916.62 | 97.9 | 2000.0 | 2062.38 | 103.1 | 2000.0 | 1964.56 | 98.2 | 2000.0 | 1989.94 | 99.5 |
| 23 | Molybdenum | 4000.0 | 3953.31 | 98.8 | 2000.0 | 2064.50 | 103.2 | 2000.0 | 1929.98 | 96.5 | 2000.0 | 1938.82 | 96.9 |

(a) ICV Control Limit 95-105%; For Hg, 90-110%.

(b) CCV Control Limit 90-110%; For Hg, 80-120%.

FORM-2A Metal
Applied P & Ch Laboratory
Initial and Continuing Calibration Verification

Client Name: GEOFON, Inc.
Project Name: JPL

Project No: 04-4428.10 Lab Code: APCL
Service ID: 033414 Sequence No.: 03M1525L
Instrument: ICP -L Method: 200.9

Batch No.(s): 03M1525

Analysis Date: 05/29/03

Concentration Units: UG/L

| # | Analyte | CCV 14:25 | | | True | Result | %R | True | Result | %R | True | Result | %R |
|----|------------|-----------|----------|-------|------|--------|----|------|--------|----|------|--------|----|
| | | True | Result | %R | | | | | | | | | |
| 1 | Aluminum | 5000.0 | 4977.98 | 99.6 | | | | | | | | | |
| 2 | Antimony | 2000.0 | 2022.25 | 101.1 | | | | | | | | | |
| 3 | Arsenic | 500.0 | 499.39 | 99.9 | | | | | | | | | |
| 4 | Barium | 5000.0 | 4965.33 | 99.3 | | | | | | | | | |
| 5 | Beryllium | 500.0 | 485.85 | 97.2 | | | | | | | | | |
| 6 | Cadmium | 1000.0 | 1012.67 | 101.3 | | | | | | | | | |
| 7 | Calcium | 50000.0 | 50133.41 | 100.3 | | | | | | | | | |
| 8 | Chromium | 500.0 | 499.22 | 99.8 | | | | | | | | | |
| 9 | Cobalt | 2000.0 | 2036.50 | 101.8 | | | | | | | | | |
| 10 | Copper | 2000.0 | 2035.28 | 101.8 | | | | | | | | | |
| 11 | Iron | 5000.0 | 5046.78 | 100.9 | | | | | | | | | |
| 12 | Lead | 500.0 | 484.64 | 96.9 | | | | | | | | | |
| 13 | Magnesium | 25000.0 | 24068.38 | 96.3 | | | | | | | | | |
| 14 | Manganese | 2000.0 | 2013.71 | 100.7 | | | | | | | | | |
| 15 | Nickel | 2000.0 | 2026.52 | 101.3 | | | | | | | | | |
| 16 | Potassium | 15000.0 | 14550.52 | 97.0 | | | | | | | | | |
| 17 | Selenium | 500.0 | 491.35 | 98.3 | | | | | | | | | |
| 18 | Silver | 1000.0 | 992.29 | 99.2 | | | | | | | | | |
| 19 | Sodium | 100000.0 | 99701.57 | 99.7 | | | | | | | | | |
| 20 | Thallium | 500.0 | 498.11 | 99.6 | | | | | | | | | |
| 21 | Vanadium | 2000.0 | 1998.07 | 99.9 | | | | | | | | | |
| 22 | Zinc | 2000.0 | 2026.05 | 101.3 | | | | | | | | | |
| 23 | Molybdenum | 2000.0 | 1977.61 | 98.9 | | | | | | | | | |

(a) ICV Control Limit 95-105%; For Hg, 90-110%.

(b) CCV Control Limit 90-110%; For Hg, 80-120%.

FORM-2A Metal
Applied P & Ch Laboratory
Initial and Continuing Calibration Verification

Client Name: GEOFON, Inc.
Project Name: JPL
Batch No.(s): 03M1535

Project No: 04-4428.10 Lab Code: APCL
Service ID: 033414 Sequence No.: 03M1535F
Instrument: GFAA-E Method: 200.9

Analysis Date: 06/02/03

Concentration Units: UG/L

| # | Analyte | ICV 15:36 | | | CCV 16:53 | | | CCV 18:08 | | | CCV 18:27 | | |
|---|---------|-----------|--------|-------|-----------|--------|-------|-----------|--------|-------|-----------|--------|-------|
| | | True | Result | %R | True | Result | %R | True | Result | %R | True | Result | %R |
| 1 | Arsenic | 50.0 | 51.00 | 102.0 | 50.0 | 50.70 | 101.4 | 50.0 | 50.00 | 100.0 | 50.0 | 50.70 | 101.4 |

(a) ICV Control Limit 95-105%; For Hg, 90-110%.

(b) CCV Control Limit 90-110%; For Hg, 80-120%.

FORM-2B Metal
Applied P & Ch Laboratory
CRDL Standard For AA and ICP

Client Name: GEOFON, Inc.
Project Name: JPL

Project No: 04-4428.10
Service ID: 033414
Instrument: ICP -L

Lab Code: APCI
Sequence No.: 03M1525L
Method: 200.9

Batch No.(s): 03M1525

Analysis Date: 05/29/03

Concentration Units: UG/L

| # | Analyte | True | 11:57 Found | R% | Time Found | R% |
|----|------------|--------|----------------|-------|---------------|----|
| 1 | Aluminum | 200.0 | 203.75 | 101.9 | | |
| 2 | Antimony | 20.0 | 19.23 | 96.2 | | |
| 3 | Arsenic | 20.0 | 22.30 | 111.5 | | |
| 4 | Barium | 10.0 | 12.03 | 120.3 | | |
| 5 | Beryllium | 4.0 | 4.42 | 110.6 | | |
| 6 | Cadmium | 5.0 | 5.11 | 102.2 | | |
| 7 | Calcium | 1000.0 | 1025.08 | 102.5 | | |
| 8 | Chromium | 10.0 | 10.62 | 106.2 | | |
| 9 | Cobalt | 20.0 | 22.54 | 112.7 | | |
| 10 | Copper | 10.0 | 10.52 | 105.2 | | |
| 11 | Iron | 50.0 | 54.39 | 108.8 | | |
| 12 | Lead | 10.0 | 9.09 | 90.9 | | |
| 13 | Magnesium | | 23.70 | | | |
| 14 | Manganese | 10.0 | 11.17 | 111.7 | | |
| 15 | Nickel | 20.0 | 21.35 | 106.7 | | |
| 16 | Potassium | | 156.42 | | | |
| 17 | Selenium | 10.0 | 6.87 | 68.7 | | |
| 18 | Silver | 10.0 | 11.43 | 114.3 | | |
| 19 | Sodium | | 13.36 | | | |
| 20 | Thallium | 10.0 | 9.23 | 92.3 | | |
| 21 | Vanadium | 10.0 | 10.84 | 108.4 | | |
| 22 | Zinc | 20.0 | 21.88 | 109.4 | | |
| 23 | Molybdenum | 15.0 | 14.58 | 97.2 | | |

FORM-3 Metal
Applied P & Ch Laboratory
Metal ICB/CCB Summary

Client Name: GEOFON, Inc.
Project Name: JPL

Project No: 04-4428.10
Service ID: 033414
Instrument: ICP -L

Lab Code: APCL
Sequence No.: 03M1525L
Method: 200.9

Batch No.(s): 03M1525

Analysis Date: 05/29/03

Concentration Units: UG/L

| # | Analyte | ICB 11:54 | | CCB 12:13 | | CCB 13:07 | | CCB 13:46 | | CCB 14:29 | |
|----|------------|-----------|---|-----------|---|-----------|---|-----------|---|-----------|---|
| | | Result | C | Result | C | Result | C | Result | C | Result | C |
| 1 | Aluminum | 11.00 | U | 11.00 | U | 11.00 | U | 11.00 | U | 11.00 | U |
| 2 | Antimony | 3.00 | U | 3.00 | U | 3.00 | U | 3.00 | U | 3.00 | U |
| 3 | Arsenic | 2.40 | U | 2.40 | U | 2.40 | U | 2.40 | U | 2.40 | U |
| 4 | Barium | 2.25 | B | 0.63 | U | 1.44 | B | 2.36 | B | 0.72 | B |
| 5 | Beryllium | 0.15 | B | 0.12 | B | 0.26 | B | 0.15 | B | 0.19 | B |
| 6 | Cadmium | 0.21 | U | 0.21 | U | 0.21 | U | 0.28 | B | 0.21 | U |
| 7 | Calcium | 83.00 | U | 83.00 | U | 83.00 | U | 98.11 | B | 83.00 | U |
| 8 | Chromium | 0.19 | U | 0.19 | U | 0.19 | U | 0.19 | U | 0.19 | U |
| 9 | Cobalt | 0.29 | U | 0.29 | U | 0.51 | B | 1.04 | B | 0.29 | U |
| 10 | Copper | 0.71 | U | 0.71 | U | 1.83 | B | 1.74 | B | 1.40 | B |
| 11 | Iron | 2.48 | B | 4.87 | B | 4.85 | B | 5.51 | B | 12.65 | B |
| 12 | Lead | -1.57 | B | -1.89 | B | 1.40 | U | -1.91 | B | -2.12 | B |
| 13 | Magnesium | 31.76 | B | 38.66 | B | 61.02 | B | 45.61 | B | 15.00 | B |
| 14 | Manganese | 0.87 | B | 0.62 | B | 1.03 | B | 1.43 | B | 0.68 | B |
| 15 | Nickel | 0.35 | U | 0.35 | U | 0.35 | U | 0.39 | B | 0.35 | U |
| 16 | Potassium | 154.78 | B | 154.19 | B | 156.87 | B | 153.25 | B | 153.43 | B |
| 17 | Selenium | 2.60 | U | 2.60 | U | 2.60 | U | 2.60 | U | 2.60 | U |
| 18 | Silver | 1.49 | B | 1.28 | B | 1.39 | B | 1.20 | U | 1.20 | U |
| 19 | Sodium | 198.00 | U | 198.00 | U | 198.00 | U | 198.00 | U | 198.00 | U |
| 20 | Thallium | 1.60 | U | 1.60 | U | 1.60 | U | 1.60 | U | 1.60 | U |
| 21 | Vanadium | 0.44 | U | 0.55 | B | 0.44 | U | 0.44 | U | 0.44 | U |
| 22 | Zinc | 0.81 | U | 0.81 | U | 0.81 | U | 1.01 | B | 0.81 | U |
| 23 | Molybdenum | 2.96 | B | 1.23 | B | 2.23 | B | 2.59 | B | 1.58 | B |

FORM-3 Metal
 Applied P & Ch Laboratory
Metal ICB/CCB Summary

Client Name: GEOFON, Inc.

Project No: 04-4428.10

Lab Code: APCL

Project Name: JPL

Service ID: 033414

Sequence No.: 03M1535E

Instrument: GFAA-E

Method: 200.9

Batch No.(s): 03M1535

Analysis Date: 06/02/03

Concentration Units: UG/L

| # | Analyte | ICB 15:42 | | CCB 16:59 | | CCB 18:15 | | CCB 18:34 | | CCB Time | |
|---|---------|-----------|---|-----------|---|-----------|---|-----------|---|----------|---|
| | | Result | C | Result | C | Result | C | Result | C | Result | C |
| 1 | Arsenic | 1.80 | U | 1.80 | U | 1.80 | U | 1.80 | U | | |

FORM-4 Metal
Applied P & Ch Laboratory
ICP Interference Check Sample

Client Name: GEOFON, Inc.
Project Name: JPL

Project No: 04-4428.10
Service ID: 033414
ICP ID Number: ICP -L

Lab Code: APCL
Sequence No.: 03M1525L

Batch No.(s): 03M1525

Analysis Date: 05/29/03

Concentration Units: UG/L

| # | Analyte | Expected | | Initial | Found | %R | Final | Found | %R |
|----|------------|----------|---------|---------|----------|-------|--------|----------|-------|
| | | Sol. A | Sol. AB | 12:01 | 12:03 | | 14:19 | 14:22 | |
| 1 | Aluminum | 500000 | 500000 | 478855 | 476912.5 | 95.4 | 462381 | 462803.2 | 92.6 |
| 2 | Antimony | 0 | 1000 | -5 | 926.6 | 92.7 | -4 | 969.9 | 97.0 |
| 3 | Arsenic | 0 | 1000 | -1 | 906.4 | 90.6 | -1 | 941.1 | 94.1 |
| 4 | Barium | 0 | 500 | 0 | 497.8 | 99.6 | 1 | 477.0 | 95.4 |
| 5 | Beryllium | 0 | 500 | 0 | 466.8 | 93.4 | 0 | 459.0 | 91.8 |
| 6 | Cadmium | 0 | 1000 | -1 | 922.0 | 92.2 | -1 | 941.4 | 94.1 |
| 7 | Calcium | 500000 | 500000 | 520048 | 530570.4 | 106.1 | 518507 | 523503.5 | 104.7 |
| 8 | Chromium | 0 | 500 | 7 | 466.8 | 93.4 | 7 | 468.7 | 93.7 |
| 9 | Cobalt | 0 | 500 | 4 | 447.0 | 89.4 | 4 | 456.4 | 91.3 |
| 10 | Copper | 0 | 500 | 7 | 504.6 | 100.9 | 5 | 495.1 | 99.0 |
| 11 | Iron | 200000 | 200000 | 177289 | 172041.1 | 86.0 | 170684 | 167465.0 | 83.7 |
| 12 | Lead | 0 | 1000 | 4 | 890.9 | 89.1 | 3 | 900.5 | 90.0 |
| 13 | Magnesium | 500000 | 500000 | 476850 | 468214.2 | 93.6 | 447866 | 446223.6 | 89.2 |
| 14 | Manganese | 0 | 500 | -2 | 477.8 | 95.6 | 0 | 469.4 | 93.9 |
| 15 | Nickel | 0 | 1000 | 4 | 864.6 | 86.5 | 3 | 880.0 | 88.0 |
| 16 | Potassium | 0 | 0 | 191 | 183.5 | | 189 | 179.7 | |
| 17 | Selenium | 0 | 1000 | -7 | 895.3 | 89.5 | -6 | 919.7 | 92.0 |
| 18 | Silver | 0 | 1000 | 5 | 1009.3 | 100.9 | 5 | 971.7 | 97.2 |
| 19 | Sodium | 0 | 0 | -192 | -69.7 | | 29 | -32.8 | |
| 20 | Thallium | 0 | 1000 | -2 | 895.5 | 89.5 | -4 | 881.5 | 88.1 |
| 21 | Vanadium | 0 | 500 | 1 | 476.9 | 95.4 | 1 | 464.8 | 93.0 |
| 22 | Zinc | 0 | 1000 | 10 | 937.9 | 93.8 | 10 | 958.2 | 95.8 |
| 23 | Molybdenum | 0 | 1000 | 2 | 881.9 | 88.2 | 1 | 877.4 | 87.7 |

FORM-5A Metal

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 200.9

| | | |
|---------------------------|--------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03M1535E | |
| MS Filename: - | Date Analyzed: 060203 | Time Analyzed: 16:27 |
| MSD Filename: - | Date Analyzed: 060203 | Time Analyzed: 16:33 |
| MS Sample No: MW-6 | Sample Lab ID: 03-3444-1 | |

| Spiked Components | Unit | Spike Added | Concentration | | MS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|------|-----------|-----------------|
| | | | Unspiked | MS | | |
| ARSENIC | µg/L | 50 | 0 | 50.0 | 97 | 75-125 |
| # of Out-of-control | | | | | 0 | |

| Spiked Components | Unit | Spike Added | MSD Concentration | MSD Rec% # | RPD% # | QC Limit, % | |
|---------------------|------|-------------|-------------------|------------|--------|-------------|--------|
| | | | | | | RPD | REC |
| ARSENIC | µg/L | 50 | 50.3 | 97 | 0 | 20 | 75-125 |
| # of Out-of-control | | | | 0 | 0 | | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-5A Metal

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 200.7

| | | |
|---------------------------|--------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCI |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03M1525L | |
| MS Filename: - | Date Analyzed: 052903 | Time Analyzed: 12:46 |
| MSD Filename: - | Date Analyzed: 052903 | Time Analyzed: 12:50 |
| MS Sample No: AE420 | Sample Lab ID: 03-3389-9 | |

| Spiked Components | Unit | Spike Added | Concentration | | MS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|--------|-----------|-----------------|
| | | | Unspiked | MS | | |
| CALCIUM | µg/L | 20000 | 473000 | 444000 | -144 * | 75-125 |
| IRON | µg/L | 1000 | 0 | 904 | 90 | 75-125 |
| MAGNESIUM | µg/L | 10000 | 201000 | 175000 | -259 * | 75-125 |
| POTASSIUM | µg/L | 5000 | 4890 | 12000 | 142 * | 75-125 |
| SODIUM | µg/L | 40000 | 452000 | 437000 | -36 * | 75-125 |
| # of Out-of-control | | | | | 4 | |

| Spiked Components | Unit | Spike Added | MSD Concentration | MSD Rec% # | RPD% # | QC Limit, % | |
|---------------------|------|-------------|-------------------|------------|--------|-------------|--------|
| | | | | | | RPD | REC |
| CALCIUM | µg/L | 20000 | 452000 | -104 * | -31 * | 20 | 75-125 |
| IRON | µg/L | 1000 | 924 | 92 | 2 | 20 | 75-125 |
| MAGNESIUM | µg/L | 10000 | 184000 | -169 * | -41 * | 20 | 75-125 |
| POTASSIUM | µg/L | 5000 | 12300 | 148 * | 4 | 20 | 75-125 |
| SODIUM | µg/L | 40000 | 447000 | -11 * | -105 * | 20 | 75-125 |
| # of Out-of-control | | | | 4 | 3 | | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-5B Metal
Applied P & Ch Laboratory
Post Digest Spike Sample Recovery

| | | |
|-------------------------------|-------------------------|----------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Lab Code: APCL |
| Project Name: JPL | Service ID: 033414 | Sequence No: 03M1525 |
| Spike Sample No. : 03-3389-09 | Batch No.: 03M1525 | Method: 200.9 |
| Client Sample No.: AE420 | Matrix: WATER | Instrument: ICP-AE |
| | Analysis Date: 05/29/03 | |

Concentration Units: UG/L

| # | Analyte | Spiked Sample Result(SSR) | 12:53 C | Sample Result(SR) | 12:36 C | Spike Added(SA) | % Rec. | Control Limit | Q |
|----|------------|------------------------------|------------|----------------------|------------|--------------------|--------|---------------|---|
| 1 | Aluminum | 2039.2191 | | 2.3639 | U | 2000.00 | 102.0 | 75-125 | |
| 2 | Antimony | 514.5115 | | -3.2971 | U | 500.00 | 102.9 | 75-125 | |
| 3 | Arsenic | 520.0990 | | -0.3470 | U | 500.00 | 104.0 | 75-125 | |
| 4 | Barium | 3886.2036 | | 21.6237 | | 4000.00 | 96.6 | 75-125 | |
| 5 | Beryllium | 182.4957 | | 0.0856 | B | 200.00 | 91.2 | 75-125 | |
| 6 | Cadmium | 245.0381 | | -0.2405 | U | 250.00 | 98.0 | 75-125 | |
| 7 | Calcium | 460043.0000 | | 472930.9375 | | 20000.00 | -64.4 | | |
| 8 | Chromium | 964.8719 | | 0.7463 | B | 1000.00 | 96.4 | 75-125 | |
| 9 | Cobalt | 972.9851 | | 0.1124 | U | 1000.00 | 97.3 | 75-125 | |
| 10 | Copper | 1031.5735 | | 5.8847 | B | 1000.00 | 102.6 | 75-125 | |
| 11 | Iron | 947.2427 | | -16.7129 | U | 1000.00 | 94.7 | 75-125 | |
| 12 | Lead | 2646.3032 | | 0.2839 | U | 3000.00 | 88.2 | 75-125 | |
| 13 | Magnesium | 190576.2500 | | 201450.0313 | | 10000.00 | -108.7 | | |
| 14 | Manganese | 1083.0605 | | 179.7312 | | 1000.00 | 90.3 | 75-125 | |
| 15 | Nickel | 956.3861 | | -0.4838 | U | 1000.00 | 95.6 | 75-125 | |
| 16 | Potassium | 12693.7490 | | 4892.3813 | | 5000.00 | 156.0 | 75-125 | N |
| 17 | Selenium | 645.6242 | | 144.8367 | | 500.00 | 100.2 | 75-125 | |
| 18 | Silver | 1043.8335 | | 5.4342 | B | 1000.00 | 103.8 | 75-125 | |
| 19 | Sodium | 453064.9688 | | 452185.6563 | | 40000.00 | 2.2 | | |
| 20 | Thallium | 457.8111 | | -0.1159 | U | 500.00 | 91.6 | 75-125 | |
| 21 | Vanadium | 1922.8342 | | 0.9157 | B | 2000.00 | 96.1 | 75-125 | |
| 22 | Zinc | 492.5609 | | -0.6638 | U | 500.00 | 98.5 | 75-125 | |
| 23 | Molybdenum | 2001.3403 | | 6.4245 | | 2000.00 | 99.7 | 75-125 | |

FORM-5B Metal
Applied P & Ch Laboratory
Post Digest Spike Sample Recovery

| | | |
|-------------------------------|-------------------------|------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Lab Code: APCL |
| Project Name: JPL | Service ID: 033414 | Sequence No.: 03M1535E |
| Spike Sample No. : 03-3444-01 | Batch No.: 03M1535 | Method: 200.9 |
| Client Sample No.: MW-6 | Matrix: WATER | Instrument: GFAA-E |
| | Analysis Date: 06/02/03 | |

Concentration Units: UG/L

| # | Analyte | Spiked Sample 16:40 | | Sample 16:07 | | Spike Added(SA) | % Rec. | Control Limit | Q |
|---|---------|---------------------|---|--------------|---|-----------------|--------|---------------|---|
| | | Result(SSR) | C | Result(SR) | C | | | | |
| 1 | Arsenic | 49.5000 | | 1.7000 | U | 50.00 | 99.0 | 75-125 | |

FORM-6 Metal
Applied P & Ch Laboratory
Duplicates Verification

Client Name: GEOFON, Inc.
Project Name: JPL

Project No: 04-4428.10
Service ID: 033414
Batch No.: 03M1525
Matrix: WATER
% Solid: 0.00

Lab Code: APCL
Sequence No.: 03M15251
Method: 200.9
Instrument: ICP -L
Analysis Date: 05/29/03

Spike Sample No. 03-3389-09
Client Sample No. AE420

Concentration Unit: UG/L

| # | Analyte | 12:36 | | 12:39 | | RPD(%) | Q |
|----|------------|-------------|---|-------------|---|--------|---|
| | | Sample(s) | C | Duplicate | C | | |
| 1 | Aluminum | 2.3639 | U | 2.0582 | U | | |
| 2 | Antimony | -3.2971 | U | -3.6534 | U | | |
| 3 | Arsenic | -0.3470 | U | -0.4985 | U | | |
| 4 | Barium | 21.6237 | | 21.2824 | | 1.6 | |
| 5 | Beryllium | 0.0856 | B | 0.0803 | B | 6.4 | |
| 6 | Cadmium | -0.2405 | U | -0.1131 | U | | |
| 7 | Calcium | 472930.9375 | | 465575.6875 | | 1.6 | |
| 8 | Chromium | 0.7463 | B | 0.7498 | B | 0.5 | |
| 9 | Cobalt | 0.1124 | U | 0.1288 | U | | |
| 10 | Copper | 5.8847 | B | 3.5322 | B | 50.0 | |
| 11 | Iron | -16.7129 | U | -15.4709 | U | | |
| 12 | Lead | 0.2839 | U | -0.2411 | U | | |
| 13 | Magnesium | 201450.0313 | | 193420.1406 | | 4.1 | |
| 14 | Manganese | 179.7312 | | 174.8012 | | 2.8 | |
| 15 | Nickel | -0.4838 | U | -0.5836 | U | | |
| 16 | Potassium | 4892.3813 | | 4819.2373 | | 1.5 | |
| 17 | Selenium | 144.8367 | | 141.2172 | | 2.5 | |
| 18 | Silver | 5.4342 | B | 5.3839 | B | 0.9 | |
| 19 | Sodium | 452185.6563 | | 443773.3750 | | 1.9 | |
| 20 | Thallium | -0.1159 | U | -2.2162 | U | | |
| 21 | Vanadium | 0.9157 | B | 0.8254 | B | 10.4 | |
| 22 | Zinc | -0.6638 | U | -0.4959 | U | | |
| 23 | Molybdenum | 6.4245 | | 4.3417 | B | 38.7 | |

FORM-6 Metal
Applied P & Ch Laboratory
Duplicates Verification

| | | |
|-----------------------------|------------------------|-------------------------|
| Client Name: GEOFON, Inc. | Project No: 04-4428.10 | Lab Code: APCL |
| Project Name: JPL | Service ID: 033414 | Sequence No.: 03M1535F |
| | Batch No.: 03M1535 | Method: 200.9 |
| Spike Sample No. 03-3444-01 | Matrix: WATER | Instrument: GFAA-E |
| Client Sample No. MW-6 | % Solid: 0.00 | Analysis Date: 06/02/03 |

Concentration Unit: UG/L

| # | Analyte | 16:07 Sample(s) | C | 16:14 Duplicate | C | RPD(%) | Q |
|---|---------|--------------------|---|--------------------|---|--------|---|
| 1 | Arsenic | 1.7000 | U | 1.0000 | U | | |

FORM-7 Metal

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 200.9

| | | |
|---------------------------|------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03M1535E | |
| LCS Filename: - | Date Analyzed: 060203 | Time Analyzed: 15:55 |
| LCSD Filename: - | Date Analyzed: 060203 | Time Analyzed: 16:01 |

| Spiked Components | Unit | Spike Added | Concentration | | LCS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|------|------------|-----------------|
| | | | Unspiked | LCS | | |
| ARSENIC | µg/L | 50 | 0 | 46.7 | 93 | 80-120 |
| # of Out-of-control | | | | | 0 | |

| Spiked Components | Unit | Spike Added | LCSD Concentration | LCSD Rec% # | RPD% # | QC Limit, % REC | |
|---------------------|------|-------------|--------------------|-------------|--------|-----------------|--------|
| | | | | | | RPD | REC |
| ARSENIC | µg/L | 50 | 46.3 | 93 | 0 | 20 | 80-120 |
| # of Out-of-control | | | | 0 | 0 | | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-7 Metal

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 200.7

| | | |
|---------------------------|------------------------|----------------------|
| Client Name: GEOFON, Inc. | Contract No: | Lab Code: APCL |
| Case No: | SAS No: | Service ID: 33414 |
| Project ID: JPL | Project No: 04-4428.10 | Sample Matrix: Water |
| | Batch No: 03M1525L | |
| LCS Filename: - | Date Analyzed: 052903 | Time Analyzed: 12:29 |
| LCSD Filename: - | Date Analyzed: 052903 | Time Analyzed: 12:32 |

| Spiked Components | Unit | Spike Added | Concentration | | LCS Rec% # | QC Limit, % REC |
|---------------------|------|-------------|---------------|-------|------------|-----------------|
| | | | Unspiked | LCS | | |
| CALCIUM | µg/L | 20000 | 0 | 19700 | 99 | 80-120 |
| IRON | µg/L | 1000 | 0 | 1030 | 103 | 80-120 |
| MAGNESIUM | µg/L | 10000 | 0 | 9700 | 97 | 80-120 |
| POTASSIUM | µg/L | 5000 | 0 | 4560 | 91 | 80-120 |
| SODIUM | µg/L | 40000 | 0 | 38500 | 96 | 80-120 |
| # of Out-of-control | | | | | 0 | |

| Spiked Components | Unit | Spike Added | LCSD Concentration | LCSD Rec% # | RPD% # | QC Limit, % | |
|---------------------|------|-------------|--------------------|-------------|--------|-------------|--------|
| | | | | | | RPD | REC |
| CALCIUM | µg/L | 20000 | 19700 | 99 | 0 | 20 | 80-120 |
| IRON | µg/L | 1000 | 1020 | 102 | 1 | 20 | 80-120 |
| MAGNESIUM | µg/L | 10000 | 9550 | 96 | 1 | 20 | 80-120 |
| POTASSIUM | µg/L | 5000 | 4500 | 90 | 1 | 20 | 80-120 |
| SODIUM | µg/L | 40000 | 37700 | 94 | 2 | 20 | 80-120 |
| # of Out-of-control | | | | | 0 | 0 | |

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-9 Metal
Applied P & Ch Laboratory
Serial Dilution

| | | | | | |
|----------------------|--------------|----------------|------------|---------------|----------|
| Client Name: | GEOFON, Inc. | Project No: | 04-4428.10 | Lab Code: | APCL |
| Project Name: | JPL | Service ID: | 033414 | Sequence No.: | 03M1525L |
| | | Batch No.: | 03M1525 | Method: | 200.9 |
| Dilution Sample No.: | 03-3389-09 | Matrix: | WATER | Instrument: | ICP -L |
| Client Sample No.: | AE420 | Analysis Date: | 05/29/03 | | |

Concentration Units: UG/L

| # | Analyte | Initial Sample | | Serial Dilut | | % Diff. | Q |
|----|------------|----------------|------------|--------------|------------|---------|---|
| | | Results(I) | 12:36 C | Results(S) | 12:43 C | | |
| 1 | Aluminum | 2.36 | U | -0.33 | U | | |
| 2 | Antimony | -3.30 | U | -10.22 | U | | |
| 3 | Arsenic | -0.35 | U | 2.86 | U | | |
| 4 | Barium | 21.62 | | 21.39 | B | 1.1 | |
| 5 | Beryllium | 0.09 | B | 0.74 | B | 762.7 | |
| 6 | Cadmium | -0.24 | U | -1.23 | U | | |
| 7 | Calcium | 472930.94 | | 431954.97 | | 8.7 | |
| 8 | Chromium | 0.75 | B | 1.23 | B | 65.1 | |
| 9 | Cobalt | 0.11 | U | 0.17 | U | | |
| 10 | Copper | 5.88 | B | 10.19 | B | 73.1 | |
| 11 | Iron | -16.71 | U | -2.16 | U | | |
| 12 | Lead | 0.28 | U | -5.77 | U | | |
| 13 | Magnesium | 201450.03 | | 181858.98 | | 9.7 | |
| 14 | Manganese | 179.73 | | 173.58 | | 3.4 | |
| 15 | Nickel | -0.48 | U | -3.06 | U | | |
| 16 | Potassium | 4892.38 | | 3626.44 | | 25.9 | F |
| 17 | Selenium | 144.84 | | 130.47 | | 9.9 | |
| 18 | Silver | 5.43 | B | 8.58 | B | 57.8 | |
| 19 | Sodium | 452185.66 | | 437142.31 | | 3.3 | |
| 20 | Thallium | -0.12 | U | -3.90 | U | | |
| 21 | Vanadium | 0.92 | B | 1.40 | U | 100.0 | |
| 22 | Zinc | -0.66 | U | -1.21 | U | | |
| 23 | Molybdenum | 6.42 | | 6.57 | B | 2.3 | |

FORM-9 Metal
Applied P & Ch Laboratory
Serial Dilution

| | | | | | |
|----------------------|--------------|----------------|------------|---------------|----------|
| Client Name: | GEOFON, Inc. | Project No: | 04-4428.10 | Lab Code: | APCL |
| Project Name: | JPL | Service ID: | 033414 | Sequence No.: | 03M1535E |
| Dilution Sample No.: | 03-3444-01 | Batch No.: | 03M1535 | Method: | 200.9 |
| Client Sample No.: | MW-6 | Matrix: | WATER | Instrument: | GEAA E |
| | | Analysis Date: | 06/02/03 | | |

Concentration Units: UG/L

| # | Analyte | Initial Sample Results(I) | 16:07 C | Serial Dilut Results(S) | 16:20 C | % Diff. | Q |
|---|---------|------------------------------|------------|----------------------------|------------|---------|---|
| 1 | Arsenic | 1.70 | U | 9.00 | B | | |

FORM-13 Metal
Applied P & Ch Laboratory
Preparation Log

Client Name: GEOFON, Inc.
Project Name: JPL

Project No: 04-4428.10
Service ID: 033414
Batch No.: 03M1525
Instrument: ICP -L

Lab Code: APCL
Sequence No.: 03M1525L
Method: 200.9

Preparation Matrix: WATER

| # | Client Sample No. | APCL Sample No. | Preparation Date | Weight (gram) | Volume (ml) |
|----|-------------------|-----------------|------------------|---------------|-------------|
| 1 | AE420 | 03-3389-09DM | 05/29/03 | | 50.0 |
| 2 | AE127 | 03-3389-04 | 05/29/03 | | 50.0 |
| 3 | AE128 | 03-3389-05 | 05/29/03 | | 50.0 |
| 4 | 1 | 03-3388-01TC | 05/29/03 | | 50.0 |
| 5 | MW-13 | 03-3391-01 | 05/29/03 | | 50.0 |
| 6 | MW-16 | 03-3391-02 | 05/29/03 | | 50.0 |
| 7 | AE142 | 03-3394-11 | 05/29/03 | | 50.0 |
| 8 | AE143 | 03-3394-12 | 05/29/03 | | 50.0 |
| 9 | AE144 | 03-3394-13 | 05/29/03 | | 50.0 |
| 10 | AE020 | 03-3396-01 | 05/29/03 | | 50.0 |
| 11 | AE021 | 03-3396-02 | 05/29/03 | | 50.0 |
| 12 | AE022 | 03-3396-03 | 05/29/03 | | 50.0 |
| 13 | AE023 | 03-3396-04 | 05/29/03 | | 50.0 |
| 14 | 051EB1-14822 | 03-3405-01 | 05/29/03 | | 50.0 |
| 15 | AE145 | 03-3413-01 | 05/29/03 | | 50.0 |
| 16 | MW-5 | 03-3414-01 | 05/29/03 | | 50.0 |
| 17 | MW-8 | 03-3414-02 | 05/29/03 | | 50.0 |
| 18 | | 03M1525MB | 05/29/03 | | 50.0 |
| 19 | | 03M1525LCS | 05/29/03 | | 50.0 |
| 20 | | 03M1525LCSD | 05/29/03 | | 50.0 |
| 21 | AE420 Dup. | 03M1525MD | 05/29/03 | | 50.0 |
| 22 | AE420 MS | 03M1525MS | 05/29/03 | | 50.0 |
| 23 | AE420 MSD | 03M1525MSD | 05/29/03 | | 50.0 |

FORM-13 Metal
Applied P & Ch Laboratory
Preparation Log

| | | | | | |
|---------------------|--------------|-------------|------------|---------------|----------|
| Client Name: | GEOFON, Inc. | Project No: | 04-4428.10 | Lab Code: | APCL |
| Project Name: | JPL | Service ID: | 033414 | Sequence No.: | 03M1535E |
| | | Batch No.: | 03M1535 | Method: | 200.9 |
| Preparation Matrix: | WATER | Instrument: | GFAA-E | | |

| # | Client Sample No. | APCL Sample No. | Preparation Date | Weight (gram) | Volume (ml) |
|----|-------------------|-----------------|------------------|---------------|-------------|
| 1 | MW-13 | 03-3391-01 | 06/02/03 | | 50.0 |
| 2 | MW-16 | 03-3391-02 | 06/02/03 | | 50.0 |
| 3 | MW-5 | 03-3414-01 | 06/02/03 | | 50.0 |
| 4 | MW-8 | 03-3414-02 | 06/02/03 | | 50.0 |
| 5 | MW-6 | 03-3444-01DM | 06/02/03 | | 50.0 |
| 6 | MW-7 | 03-3444-02 | 06/02/03 | | 50.0 |
| 7 | MW-15 | 03-3444-03 | 06/02/03 | | 50.0 |
| 8 | MW-1 | 03-3465-01 | 06/02/03 | | 50.0 |
| 9 | MW-9 | 03-3465-02 | 06/02/03 | | 50.0 |
| 10 | MW-10 | 03-3465-03 | 06/02/03 | | 50.0 |
| 11 | | 03M1535MB | 06/02/03 | | 50.0 |
| 12 | | 03M1535LCS | 06/02/03 | | 50.0 |
| 13 | | 03M1535LCSD | 06/02/03 | | 50.0 |
| 14 | MW-6 Dup. | 03M1535MD | 06/02/03 | | 50.0 |
| 15 | MW-6 MS | 03M1535MS | 06/02/03 | | 50.0 |
| 16 | MW-6 MSD | 03M1535MSD | 06/02/03 | | 50.0 |

FORM-14 Metal
Applied P & Ch Laboratory
Analysis Run Log

Client Name: GEOFON, Inc.
Project Name: JPL

Project No: 04-4428.10
Service ID: 033414
Instrument: ICP -L
Start Date: 05/29/03

Lab Code: APCL
Sequence No.: 03M1525L
Method: 200.9
End Date: 05/29/03

Batch No.(s): 03M1525

| # | APCL Sample No. | D/F | Time | Al | Sb | As | Ba | Be | Cd | Ca | Cr | Co | Cu | Fe | Pb | Mg | Mn | Hg | Ni | K | Se | Ag | Na | Tl | V | Zn | Mo | Sr | Ti | Sn | Li | B | Si |
|----|-----------------|------|-------|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|---|----|----|----|----|---|----|----|----|----|----|----|---|----|
| 41 | 3388-1TC F=2 | 2.00 | 14:14 | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ |
| 42 | ICSA 1441 | 1.00 | 14:19 | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ |
| 43 | ICSAB 1443 | 1.00 | 14:22 | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ |
| 44 | CCV 1447B | 1.00 | 14:25 | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ |
| 45 | CCB | 1.00 | 14:29 | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ |
| 46 | DLC A1427 | 1.00 | 14:32 | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ | √ |

FORM-14 Metal
Applied P & Ch Laboratory
Analysis Run Log

Client Name: GEOFON, Inc.
Project Name: JPL
Batch No.(s): 03M1535

Project No: 04-4428.10
Service ID: 033414
Instrument: GFAA-E
Start Date: 06/02/03

Lab Code: APCL
Sequence No.: 03M1535E
Method: 200.9
End Date: 06/02/03

| # | APCL Sample No. | D/F | Time | Al | Sb | As | Ba | Be | Cd | Ca | Cr | Co | Cu | Fe | Pb | Mg | Mn | Hg | Ni | K | Se | Ag | Na | Ti | V | Zn | Mo | Sr | Ti | Sn | Li | B | Si | | |
|----|-----------------|------|-------|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|---|----|----|----|----|---|----|----|----|----|----|----|---|----|--|--|
| 1 | Calib. Blank | 1.00 | 15:00 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 2 | 1/2 STD1 1472A | 1.00 | 15:06 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 3 | STD1 1472A | 1.00 | 15:12 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 4 | STD2 1472B | 1.00 | 15:18 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 5 | STD3 1472C | 1.00 | 15:25 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 6 | ICV A1474 | 1.00 | 15:36 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 7 | ICB | 1.00 | 15:42 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 8 | M-BL 03M1535 | 1.00 | 15:48 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 9 | LCS-03M1535 | 1.00 | 15:55 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 10 | LCSD-03M1535 | 1.00 | 16:01 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 11 | 3444-1 S F=1 | 1.00 | 16:07 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 12 | 3444-1 D F=1 | 1.00 | 16:14 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 13 | 3444-1 1/5 F=5 | 5.00 | 16:20 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 14 | 3444-1 MS F=1 | 1.00 | 16:27 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 15 | 3444-1 MSD F=1 | 1.00 | 16:33 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 16 | 3444-1 PS F=1 | 1.00 | 16:40 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 17 | 3444-2 F=1 | 1.00 | 16:46 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 18 | CCV A1474 | 1.00 | 16:53 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 19 | CCB | 1.00 | 16:59 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 20 | 3444-3 F=1 | 1.00 | 17:24 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 21 | 3391-1 F=1 | 1.00 | 17:31 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 22 | 3391-2 F=1 | 1.00 | 17:37 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 23 | 3414-1 F=1 | 1.00 | 17:43 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 24 | 3414-2 F=1 | 1.00 | 17:49 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 25 | 3465-1 F=1 | 1.00 | 17:56 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 26 | 3465-2 F=1 | 1.00 | 18:02 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 27 | CCV A1474 | 1.00 | 18:08 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 28 | CCB | 1.00 | 18:15 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 29 | 3465-3 F=1 | 1.00 | 18:21 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 30 | CCV A1474 | 1.00 | 18:27 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 31 | CCB | 1.00 | 18:34 | | | ✓ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

Analysis Anomaly Record

Batch #: 03M1525 Method: 6010B Matrix: W Date: 5/29/03

Samples Involved: 3389, 3391, 3394, 3396, 3413, 3405, 3414

• Anomaly for MS/MSD/MD

- 1. MS/MSD out of control limit, sample matrix interference suspected
- 2. MS or MSD out of control limit, but \overline{MS} is O.K.
- 3. One of MS/MSD, and \overline{MS} out of control limit, but not enough sample for re-analysis
- 4. Not enough sample for MS/MSD, LCS/LCSD may be used
- 5. Spiked samples contain high concentration of analytes ($>4 \times$ spiked concentration) *K Na Ca Mg*
- 6. MS/MSD out of control limit, but post spike is O.K.
- 7. MS/MSD out of control limit, due to the heterogenous matrix
- 8. MS/MSD out of control limit, due to the very special matrix
- 9. Not enough sample for matrix duplicate (MD)

• Anomaly for Holding time (HT)

- 10. HT has been exceeded when received, authorized by the Client to carry on with the analyses
- 11. Extraction HT was passed, authorized by the Client to carry on with the analyses
- 12. Analysis HT was passed, authorized by the Client to carry on with the analyses

• Surrogates Anomaly

- 13. Surrogate recovery out of control limit (see Level-1 Part III), sample matrix interference suspected
- 14. Surrogate recovery out of control limit (see Level-1 Part III), but not enough sample for re-analysis
- 15. Surrogate recovery out of control limit, due to very special matrix
- 16. Surrogate diluted out (for highly contaminated samples)
- 17. Lower surrogate recovery due to cleanup process

• Chromatogram Pattern Anomaly

- 18. Not a typical gasoline chromatogram pattern
- 19. Not a typical diesel chromatogram pattern
- 20. Not a typical diesel chromatogram pattern, but similar to heavy-oil or motor oil
- 21. Not a typical kerosene chromatogram pattern
- 22. Not a typical jet fuel chromatogram pattern
- 23. Not a complete PCB chromatogram pattern, interference/degradation suspected

• Other anomaly

Problem Description: _____

Reason: _____

Analyst: N.7 Date: 5/29/03

Note: _____

1760 Magnolia Ave. Chino CA 91710

Metal Digestion (3010/3050) Worksheet

Phone: (909) 590-1828 Fax: (909) 590-1498

Batch # 03M1525 Matrix: W Method used: 3010A Date: 5/29/03 Digested by: XI Diluted by: N.F.

Lot #: ASTM Type I water RW1413 HNO₃ 1102/20 H₂SO₄ _____ HCl 4102050 H₂O₂ _____

| OP # | Type | Samp ID /Lot # | X (g or mL) | V _{digest} /X = f ₁ | V ₁ /V _i = f ₂ | V _j /V _i = f ₃ | F = f ₁ f ₂ f ₃ | Note |
|------|--------------|------------------------|-------------|---|---|---|--|-----------------|
| 2899 | Method Blank | Bl. Lot: <u>RW1413</u> | <u>50</u> | <u>50/X = 1</u> | <u>1 =</u> | <u>1 =</u> | | <u>23 Me</u> |
| 2900 | LCS1 | Bl. Lot: <u>11</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2901 | Sample-1 | <u>3389 -9</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2902 | MS1 on S-1 | <u>-9</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | <u>T = 95°C</u> |
| 2903 | MS2 on S-1 | <u>-9</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2904 | Sample 2 | <u>-4</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2905 | Sample 3 | <u>-5</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2906 | Sample 4 | <u>3391 -1</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2907 | Sample 5 | <u>-2</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2908 | Sample 6 | <u>3394 -11</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2909 | Sample 7 | <u>-12</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2910 | Sample 8 | <u>-13</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2911 | Sample 9 | <u>3414 -1</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2912 | Sample 10 | <u>-2</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2913 | LCS2 | Bl. Lot: <u>RW1413</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2914 | Sample 11 | <u>3396 -1</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2915 | Sample 12 | <u>-2</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2916 | Sample 13 | <u>-3</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2917 | Sample 14 | <u>-4</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2918 | Sample 15 | <u>3413 -1</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2919 | Sample 16 | <u>3405 -1</u> | | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2920 | Sample 17 | <u>Tc Blank</u> | | <u>/X =</u> | <u>10/5 = 2</u> | <u>/ =</u> | <u>2</u> | |
| 2921 | Sample 18 | <u>3388 -1 Tc</u> | <u>↓</u> | <u>↓ /X =</u> | <u>10/5 = 2</u> | <u>/ =</u> | <u>2</u> | |
| 2922 | Sample 19 | | <u>X1</u> | <u>/X =</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2923 | Sample 20 | | | <u>5/29/03</u> | <u>/ =</u> | <u>/ =</u> | | |
| 2924 | Duplicate | <u>3389 -9</u> | <u>50</u> | <u>50/X = 1</u> | <u>/ =</u> | <u>/ =</u> | | |

Specification of matrix spike and lab control spike

| QC Type | Spiked Element * | Spike Stock Solution Lot # | Spike Stock (Rep.) Conc. C _s , µg/mL | Spike Stock Volum Used V _s mL | Spike Level T' = C _s V _s /V ppm or mg/L | Sample Spike T, ppm |
|---------|---------------------------|---------------------------------|---|--|---|---------------------|
| MS1 | /As/Se/Sb/M ₂₀ | AA- /AA- /AA- <u>1A143</u> | <u>/ / / 25</u> | <u>/ / / 2</u> | <u>/ / / /</u> | |
| MS2 | /As/Se/Sb/M ₂₀ | AA- /AA- /AA- /AA- <u>11</u> | <u>/ / /</u> | <u>/ / /</u> | <u>/ / / /</u> | |
| LCS1 | /As/Se/Sb/M ₂₀ | AA- /AA- /AA- /AA- <u>1A142</u> | <u>/ / /</u> | <u>/ / /</u> | <u>/ / / /</u> | |
| LCS2 | /As/Se/Sb/M ₂₀ | AA- /AA- /AA- /AA- <u>11</u> | <u>/ / /</u> | <u>/ / /</u> | <u>/ / / /</u> | |

* Notation: T - rep. sample spike level. T' - digest solution spike level. T = f T' = C_sV_s/X. M20 (or Mj) represents 20 (or j) metals, (see STD logbook).
 If digest needs dilution for different metals, use dilution worksheet.

Supervisor Initial Y.680

13760 Magnolia Ave. Chino CA 91710

Metal Digestion (3010/3050) Worksheet

Tel: (909) 590-1828 Fax: (909) 590-1498

Batch # B3M535 Matrix: W Method used: 3020A Date: 6/2/03 Digested by: Xi Diluted by: YCW

Lot #: ASTM Type I water RW1414 HNO₃ 1102/20 H₂SO₄ _____ HCl _____ H₂O₂ _____

| OP # | Type | Samp ID /Lot # | X (g or mL) | V _{digest} /X = f ₁ | V ₁ /V _i = f ₂ | V _j /V _i = f ₃ | F = f ₁ f ₂ f ₃ | Note |
|------|--------------|-----------------------|-------------|---|---|---|--|----------------|
| 3107 | Methqd Blank | Bl. Lot <u>RW1414</u> | <u>50</u> | <u>50/X = 1</u> | <u>1 =</u> | <u>1 =</u> | | <u>GFAA/AS</u> |
| 3108 | LCS1 | Bl. Lot: (1) | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3109 | Sample-1 | <u>3444 -1</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3110 | MS1 on S-1 | <u>3444 -1</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3111 | MS2 on S-1 | <u>Xi 6/2/03 -1</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3112 | Sample 2 | <u>-2</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | <u>MS/MSD</u> |
| 3113 | Sample 3 | <u>-3</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3114 | Sample 4 | <u>3391 -1</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3115 | Sample 5 | <u>-2</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3116 | Sample 6 | <u>3414 -1</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3117 | Sample 7 | <u>-2</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3118 | Sample 8 | <u>3465 -1</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3119 | Sample 9 | <u>-2</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3120 | Sample 10 | <u>-3</u> | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3121 | LCS2 | Bl. Lot <u>RW1414</u> | <u>√</u> | <u>√/X = √</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3122 | Sample 11 | | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3123 | Sample 12 | | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3124 | Sample 13 | | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3125 | Sample 14 | | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3126 | Sample 15 | | | <u>Xi /X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3127 | Sample 16 | | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3128 | Sample 17 | | | <u>6/2/03 /X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3129 | Sample 18 | | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3130 | Sample 19 | | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3131 | Sample 20 | | | <u>/X =</u> | <u>1 =</u> | <u>1 =</u> | | |
| 3132 | Duplicate | <u>3444 -1</u> | <u>50</u> | <u>50/X = 1</u> | <u>1 =</u> | <u>1 =</u> | | |

Specification of matrix spike and lab control spike

| QC Type | Spiked Element * | Spike Stock Solution Lot # | Spike Stock (Rep.) Conc. C _s , µg/mL | Spike Stock Volum Used V _s , mL | Spike Level T' = C _s V _s /V ppm or mg/L | Sample Spike T, ppm |
|---------|---------------------------|-------------------------------|---|--|---|---------------------|
| MS1 | /As/Sc/Sb/M ₂₀ | AA- /AA- /AA- /AA- <u>473</u> | <u>1 1 1 5</u> | <u>1 1 10.5</u> | <u>1 1 10.05</u> | |
| MS2 | /As/Sc/Sb/M ₂₀ | AA- /AA- /AA- /AA- <u>11</u> | <u>1 1 1</u> | <u>1 1 1</u> | <u>1 1 1</u> | |
| LCS1 | /As/Sc/Sb/M ₂₀ | AA- /AA- /AA- /AA- <u>471</u> | <u>1 1 1</u> | <u>1 1 1</u> | <u>1 1 1</u> | |
| LCS2 | /As/Sc/Sb/M ₂₀ | AA- /AA- /AA- /AA- <u>11</u> | <u>1 1 1</u> | <u>1 1 1</u> | <u>1 1 1</u> | |

* Notation: T - rep. sample spike level. T' - digest solution spike level. T = T' = C_sV_s/X. M20 (or M_j) represents 20 (or j) metals, (see STD logbook). If digest needs dilution for different metals, use dilution worksheet.

Supervisor Initial YCW