

Level C Data Package Deliverables

Wet Chemistry



Applied P & Ch Laboratory

Applied P & Ch Laboratory
Wet Analysis Results for Method 314.0

Client Name: GEOFON, Inc.
 Project ID: JPL

Project No: 04-4428.10
 Service ID: 34406

Anal. Method 314.0
 Collected by:

Component Name: Perchlorate
 CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-4406-1	DUPE-1-3Q03	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	<4	U
03-4406-2	EB-2-7/30/03	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	<4	U
03-4406-3	MW-3-2	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	8.9	
03-4406-4	MW-3-3	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	<4	U
03-4406-5	MW-3-4	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	<4	U
03-4406-6	MW-17-2	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	10.9	
03-4406-7	MW-17-3	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	20	209	
03-4406-8	MW-17-4	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	<4	U
03-4406-9	MW-19-1	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	<4	U
03-4406-10	MW-19-2	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	3.6	B
03-4406-11	MW-19-3	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	3.0	B
03-4406-12	MW-19-4	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	<4	U
03-4406-13	MW-19-5	Water	07/30/03	07/30/03	07/31/03	03W3913	µg/L	4	<4	U
03W3913-MB-01	03W3913-MB-01	Water	07/31/03	07/31/03	07/31/03	03W3913	µg/L	4	<4	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory
Wet Analysis Results for Method 7196

Client Name: GEOFON, Inc.
Project ID: JPL

Project No: 04-4428.10
Service ID: 34406

Anal. Method 7196
Collected by:

Component Name: Chromium (VI)
CAS No: 1333-82-0

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-4406-3	MW-3-2	Water	07/30/03	07/30/03	07/30/03	03W3907	mg/L	0.01	<0.01	U
03-4406-4	MW-3-3	Water	07/30/03	07/30/03	07/30/03	03W3907	mg/L	0.01	<0.01	U
03-4406-5	MW-3-4	Water	07/30/03	07/30/03	07/30/03	03W3907	mg/L	0.01	<0.01	U
03-4406-6	MW-17-2	Water	07/30/03	07/30/03	07/30/03	03W3907	mg/L	0.01	<0.01	U
03-4406-7	MW-17-3	Water	07/30/03	07/30/03	07/30/03	03W3907	mg/L	0.01	<0.01	U
03-4406-8	MW-17-4	Water	07/30/03	07/30/03	07/30/03	03W3907	mg/L	0.01	<0.01	U
03W3907-MB-01	03W3907-MB-01	Water	07/30/03	07/30/03	07/30/03	03W3907	mg/L	0.01	<0.01	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

FORM-3

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 314.0

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34406
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W3913	
LCS Filename: -	Date Analyzed: 073103	Time Analyzed:
LCSD Filename: -	Date Analyzed: -	Time Analyzed: -

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
PERCHLORATE	µg/L	25	0	25.5	102	80-120
# of Out-of-control					0	

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 314.0

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34406
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W3913	
MS Filename: -	Date Analyzed: 073103	Time Analyzed:
MSD Filename: -	Date Analyzed: 073103	Time Analyzed:
MS Sample No: MW-19-2	Sample Lab ID: 03-4406-10	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
PERCHLORATE	µg/L	50	3.6	60.5	114	75-125
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
PERCHLORATE	µg/L	50	59.7	112	2	20	75-125
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 7196

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34406
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W3907	
LCS Filename: -	Date Analyzed: 073003	Time Analyzed: 13:59
LCSD Filename: -	Date Analyzed: 073003	Time Analyzed: 13:59

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
CHROMIUM (VI)	mg/L	0.25	0	0.230	92	80-115
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	LCSD Concentration	LCSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
CHROMIUM (VI)	mg/L	0.25	0.236	94	2	19	80-115
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-3

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 7196

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34406
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W3907	
MS Filename: -	Date Analyzed: 073003	Time Analyzed: 13:59
MSD Filename: -	Date Analyzed: 073003	Time Analyzed: 13:59
MS Sample No: MW-3-3	Sample Lab ID: 03-4406-4	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
CHROMIUM (VI)	mg/L	0.25	0	0.223	89	78-115
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
CHROMIUM (VI)	mg/L	0.25	0.228	91	2	19	78-115
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

6A
INITIAL CALIBRATION DATA

Lab Name: Applied P & Ch Lab Contract: 34406

Analysis: Chromium (VI) Calibration Date: 07/28/2003

Concentration (mg/L)	0.000	0.0125	0.050	0.125	0.250	0.50
Absorbance	0.000	0.007	0.017	0.107	0.212	0.420

A=-0.001+ 0.846C

A=Absorbance

C=Concentration (mg/L)

r= 0.9999

FORM-7

Applied P & Ch Laboratory

CCV Recovery for Wet Analysis

Client Name: GEOFON, Inc.

Contract No.:

Lab Code:

APCL

Case No:

SAS No.:

Service ID:

34406

Project ID: JPL

Project No.: 04-4428.10

#	Component Name	Method	Batch No.	Unit	Expected	Test Result	Rec. %	Dev. %	Flag	Control Limit, %	Test Date
1	Perchlorate	314.0	03W3913	µg/L	50	55.2	110	10	✓	85-115	07/31/2003
	Perchlorate	314.0	03W3913	µg/L	50	55.6	111	11	✓	85-115	07/31/2003
	Perchlorate	314.0	03W3913	µg/L	50	55.4	111	11	✓	85-115	07/31/2003
	Perchlorate	314.0	03W3913	µg/L	50	54.9	110	10	✓	85-115	07/31/2003
2	Chromium (VI)	7196	03W3907	mg/L	0.25	0.249	100	0	✓	90-110	07/30/2003
	Chromium (VI)	7196	03W3907	mg/L	0.25	0.240	96	-4	✓	90-110	07/30/2003

Line	Sample	Sample Type	Level	Method	Data File	Volume	Dilution
1	##03w3913kw ipc 25ppb w8032	Sample		e314-011.met	c:\data\03w3913k\w3913k ipc 25ppb	1	1
2	ccv 50ppb w8082	Sample		e314-011.met	c:\data\03w3913k\w3913k q01	1	1
3	lcs 25ppb w8087	Sample		e314-011.met	c:\data\03w3913k\w3913k l01	1	1
4	LCS 18PPB W8033a	Sample		e314-011.met	c:\data\03w3913k\w3913k j01	1	1
5	ICCS 4ppb w8088	Sample		e314-011.met	c:\data\03w3913k\w3913k iccs 4ppb	1	1
6	mb	Sample		e314-011.met	c:\data\03w3913k\w3913k k01	1	1
7	4406-10 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-10	1	1
8	4389-02 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-02	1	1
9	4389-03 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-03	1	1
0	4389-04 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-04	1	1
1	4389-05 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-05	1	1
2	4389-06 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-06	1	1
3	ccv 50ppb w8082	Sample		e314-011.met	c:\data\03w3913k\w3913k q02	1	1
4	ccb	Sample		e314-011.met	c:\data\03w3913k\w3913k k02	1	1
5	4406-10 ms 50ppb f=1 w8033b	Sample		e314-011.met	c:\data\03w3913k\w3913k m01	1	1
6	4406-10 msd 50ppb f=1 w8033b	Sample		e314-011.met	c:\data\03w3913k\w3913k n01	1	1
7	4406-01 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-01	1	1
8	4406-02 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-02	1	1
9	4406-03 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-03	1	1
0	4406-04 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-04	1	1
1	4406-05 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-05	1	1
2	4406-06 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-06	1	1
3	4406-07 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-07	1	1
4	ccv 50ppb w8082	Sample		e314-011.met	c:\data\03w3913k\w3913k q03	1	1
5	ccb	Sample		e314-011.met	c:\data\03w3913k\w3913k k03	1	1
6	4389-01 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-01	1	1
7	4406-08 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-08	1	1
8	4406-09 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-09	1	1
9	4406-11 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-11	1	1
0	4406-12 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-12	1	1
1	4406-13 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-13	1	1
2	4406-07 f=5	Sample		e314-011.met	c:\data\03w3913k\4406-07a	1	5
3	ccv 50ppb w8082	Sample		e314-011.met	c:\data\03w3913k\w3913k q04	1	1
4		Sample		aastopcl.met		1	1

Analyst Wesley Way
Date 7/31/03
Instrument LC-K

Line	Weight	Int. Std.	Comment
1	1	1	
2	1	1	
3	1	1	
4	1	1	
5	1	1	
6	1	1	
7	1	1	
8	1	1	
9	1	1	
0	1	1	
1	1	1	
2	1	1	
3	1	1	
4	1	1	
5	1	1	
6	1	1	
7	1	1	
8	1	1	
9	1	1	
0	1	1	
1	1	1	
2	1	1	
3	1	1	
4	1	1	
5	1	1	
6	1	1	
7	1	1	
8	1	1	
9	1	1	
0	1	1	
1	1	1	
2	1	1	
3	1	1	
4	1	1	

Default Method Path: C:\PEAKNET\METHOD
Default Data Path: C:\DATA\03W3650K
Comment:

APCL Perchlorate Analysis Report

Sample Name : 4406-01 f=1

Data File Name : C:\DATA\03W3913K\4406-01_017.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 2:31:45 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

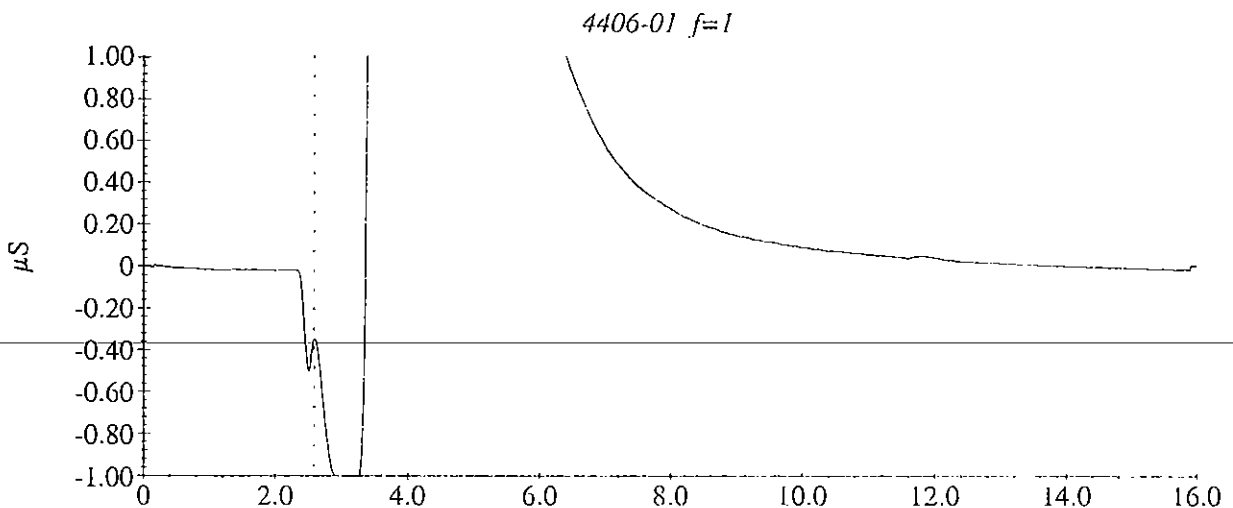

APCL Perchlorate Analysis Report

Sample Name : 4406-02 f=1

Data File Name : C:\DATA\03W3913K\4406-02_018.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 2:50:08 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

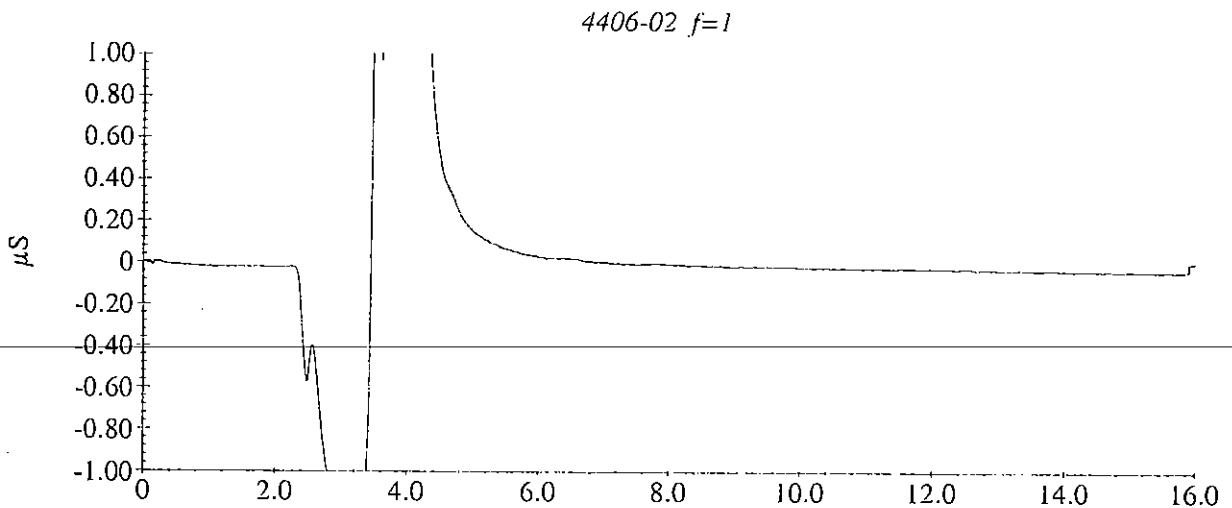

APCL Perchlorate Analysis Report

Sample Name : 4406-03 f=1

Data File Name : C:\DATA\03W3913K\4406-03_019.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 3:08:33 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.78	8.92	15138.00	750.25

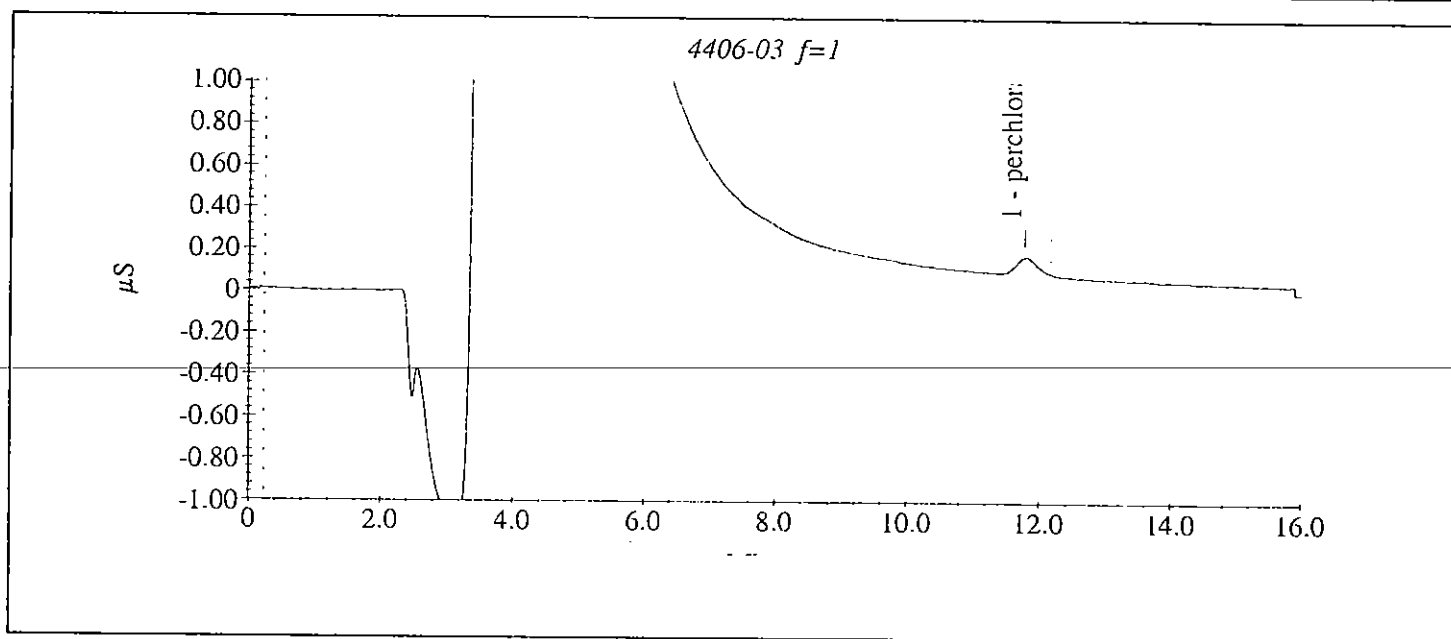

APCL Perchlorate Analysis Report

Sample Name : 4406-04 f=1

Data File Name : C:\DATA\03W3913K\4406-04_020.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 3:26:56 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

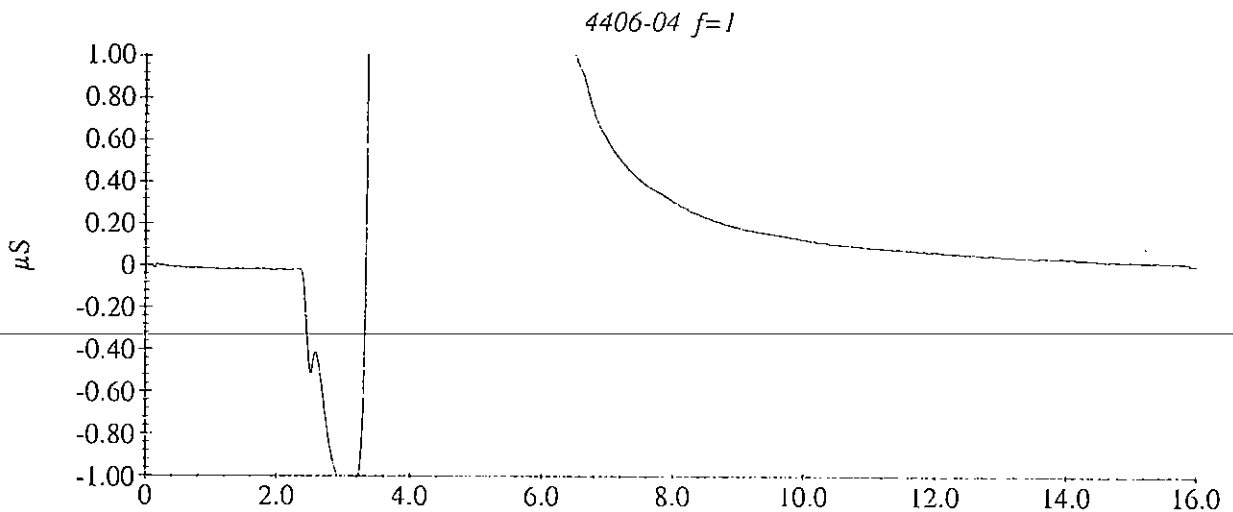

APCL Perchlorate Analysis Report

Sample Name : 4406-05 f=1

Data File Name : C:\DATA\03W3913K\4406-05_021.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 3:45:20 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
	perchlorate				

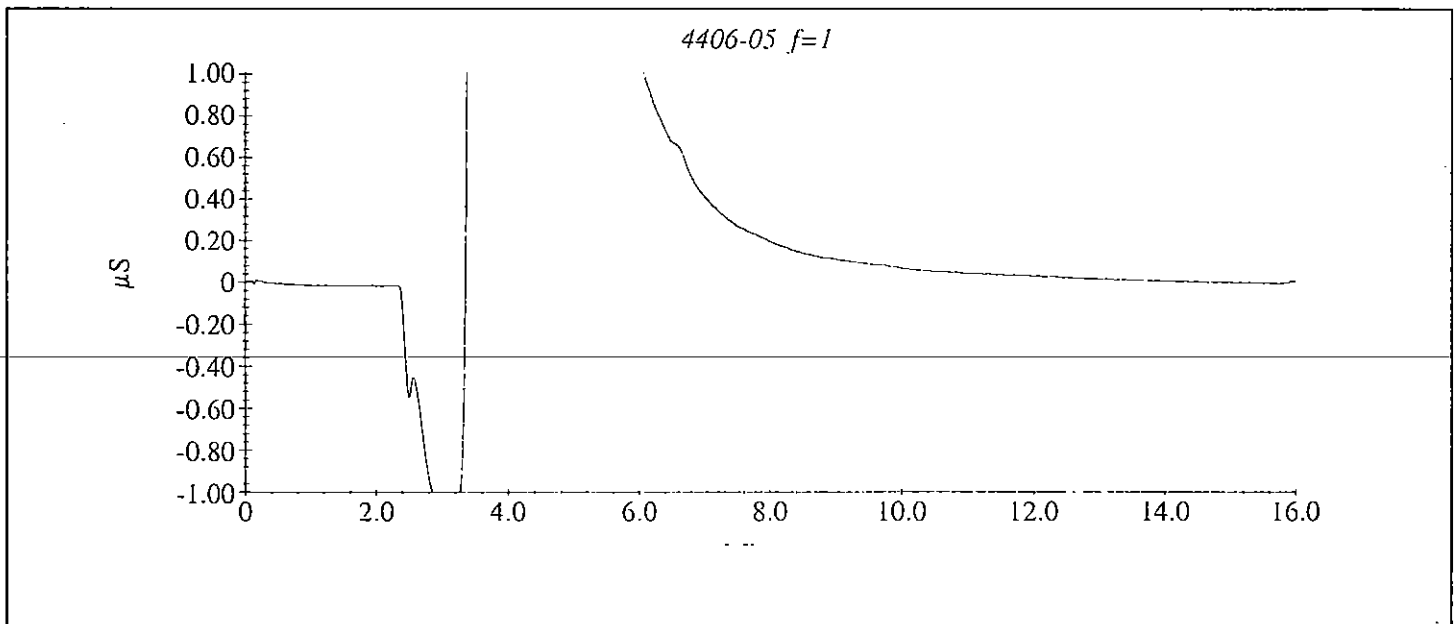

APCL Perchlorate Analysis Report

Sample Name : 4406-06 f=1

Data File Name : C:\DATA\03W3913K\4406-06_022.DXD

Method File Name : c:\peaknet\method\ve314-011.met


Date Time Collected : 07/31/2003 4:03:44 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.82	10.89	18488.75	914.27

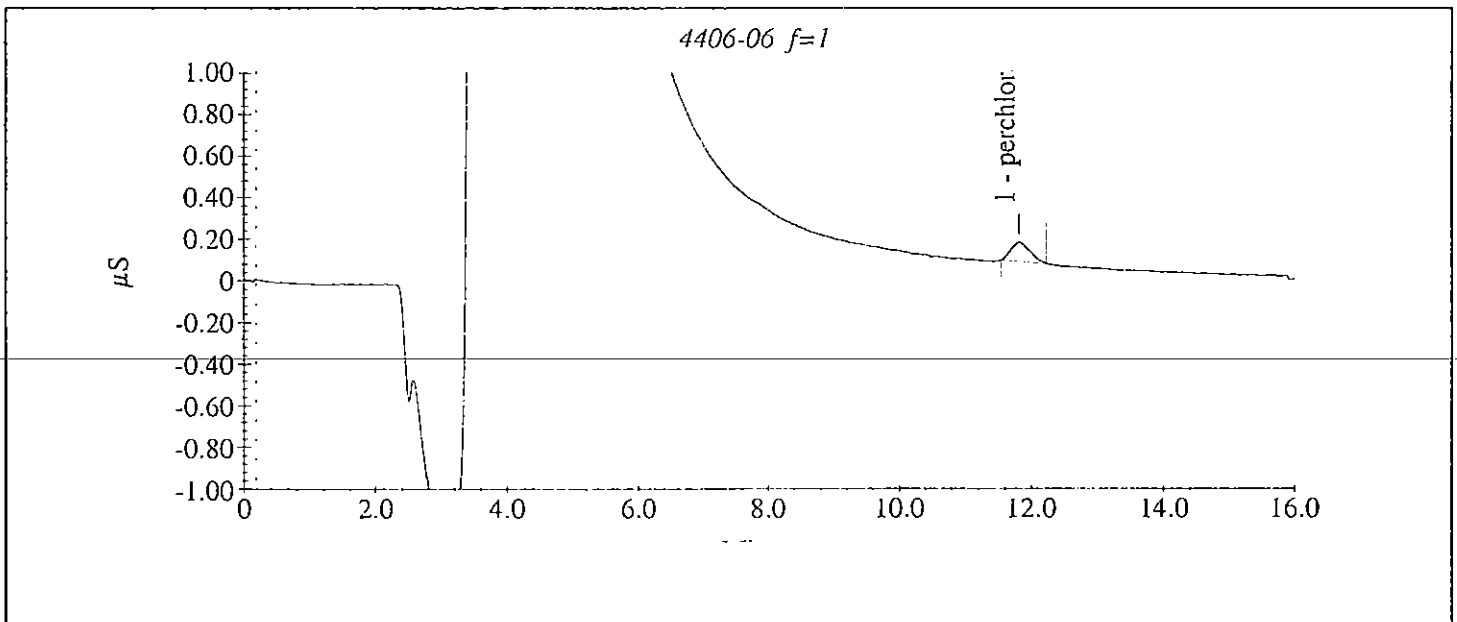

APCL Perchlorate Analysis Report

Sample Name : 4406-07 f=5

Data File Name : C:\DATA\03W3913K\4406-07A_032.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 7:07:49 PM

System Operator : C.W and W.W

Dilution Factor : 5.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.67	209.14	70985.50	3145.42

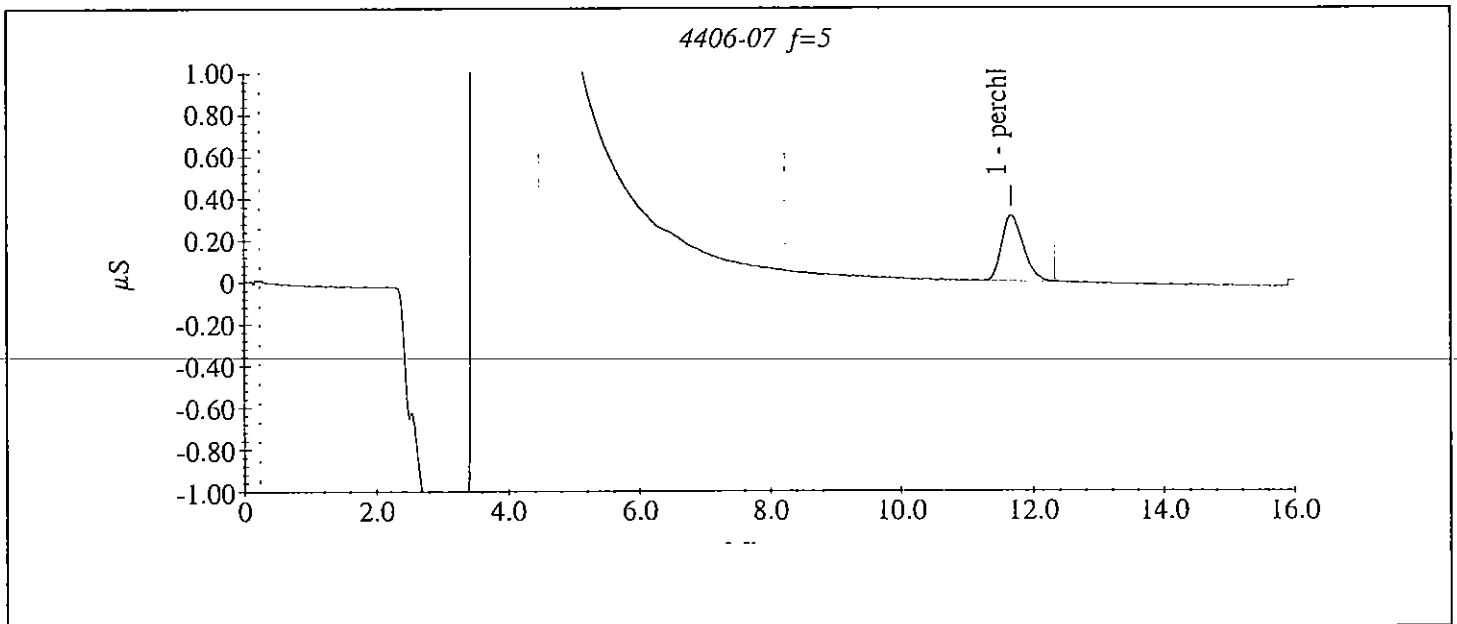

APCL Perchlorate Analysis Report

Sample Name : 4406-07 f=1

Data File Name : C:\DATA\03W3913K\4406-07_023.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 4:22:08 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.75	220.04	373421.70	16505.57

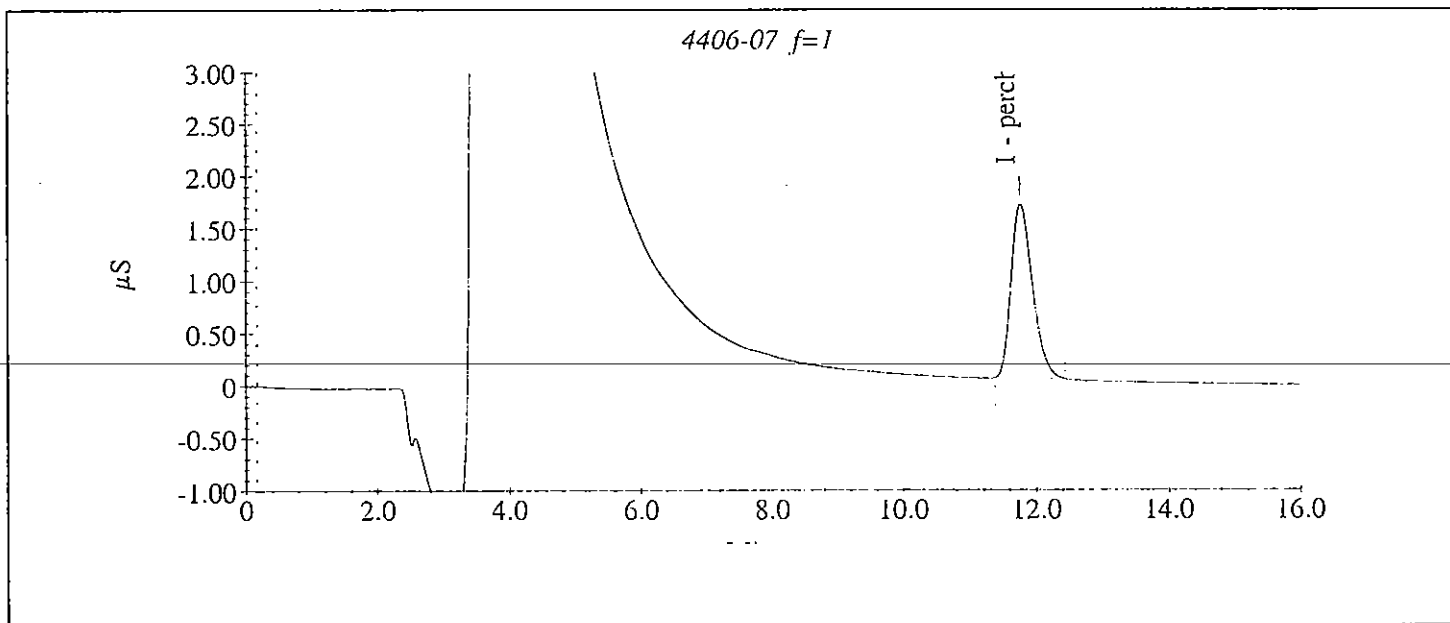

for reference



APCL Perchlorate Analysis Report

Sample Name : 4406-08 f=1

Data File Name : C:\DATA\03W3913K\4406-08_027.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 5:35:43 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

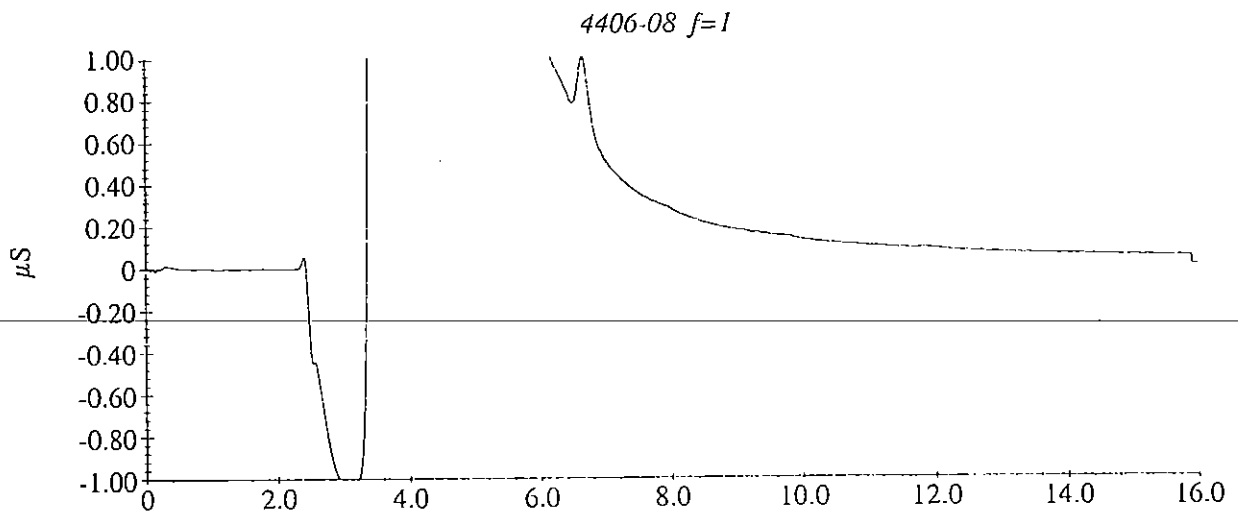

APCL Perchlorate Analysis Report

Sample Name : 4406-09 f=1

Data File Name : C:\DATA\03W3913K\4406-09_028.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 5:54:06 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height

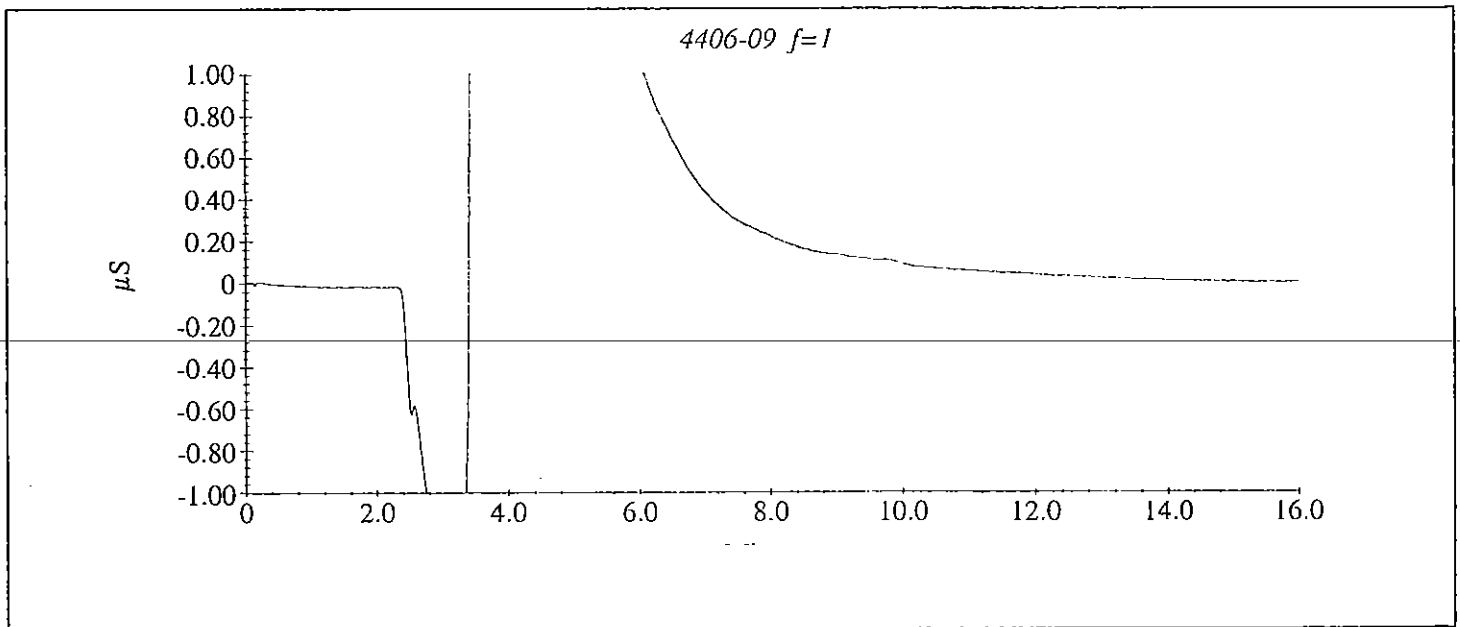

APCL Perchlorate Analysis Report

Sample Name : 4406-10 f=1

Data File Name : C:\DATA\03W3913K\4406-10_007.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 11:27:49 AM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.85	3.63	6160.30	344.81

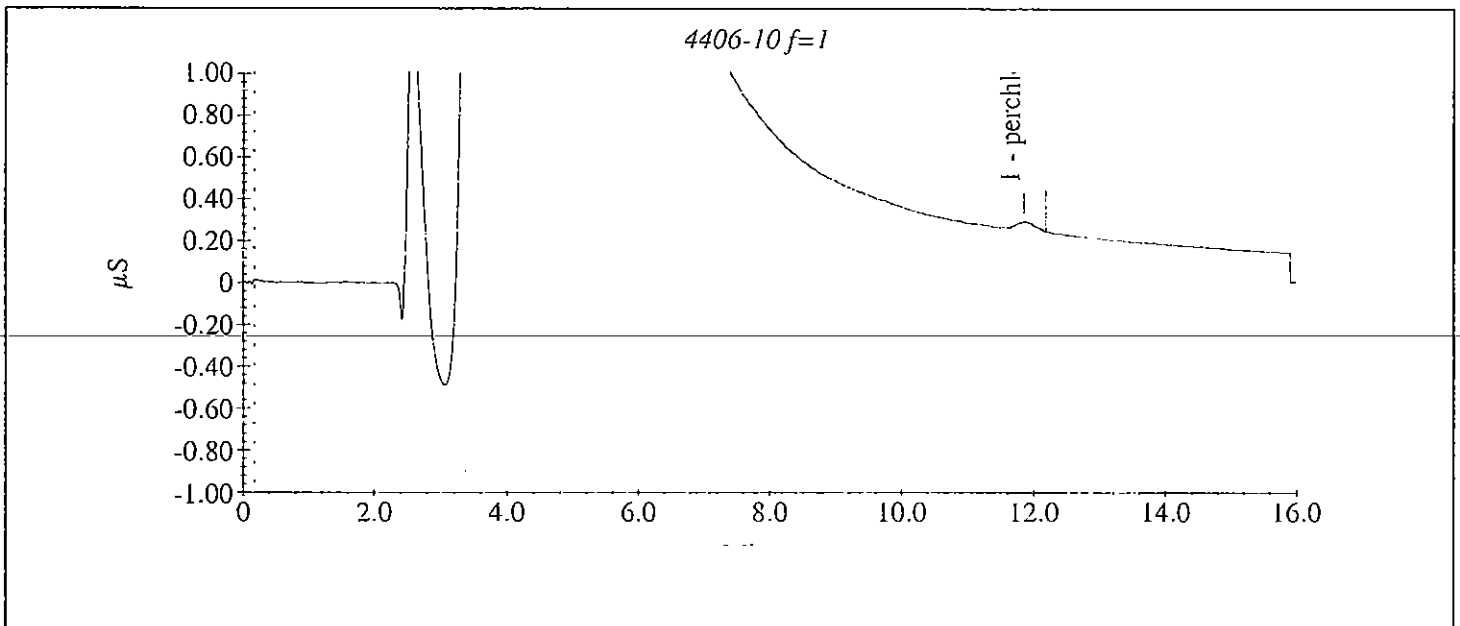

APCL Perchlorate Analysis Report

Sample Name : 4406-11 f=1

Data File Name : C:\DATA\03W3913K\4406-11_029.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 6:12:31 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.87	3.03	5136.10	284.05

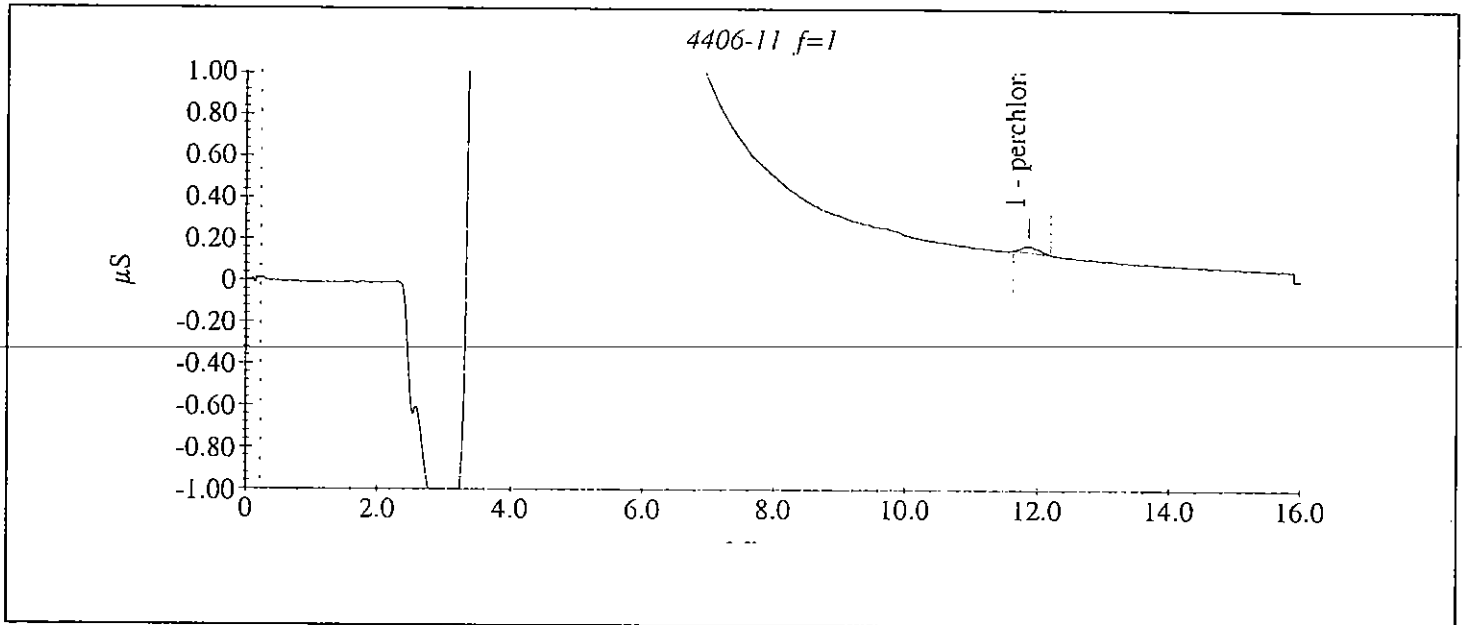

APCL Perchlorate Analysis Report

Sample Name : 4406-12 f=1

Data File Name : C:\DATA\03W3913K\4406-12_030.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 6:30:54 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

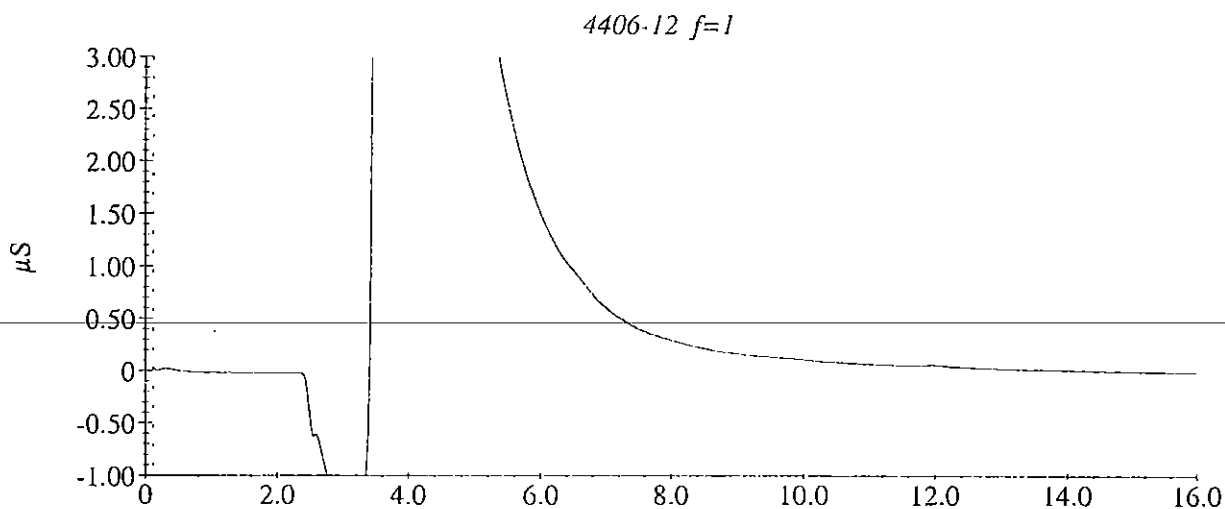

APCL Perchlorate Analysis Report

Sample Name : 4406-13 f=1

Data File Name : C:\DATA\03W3913K\4406-13_031.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 6:49:20 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

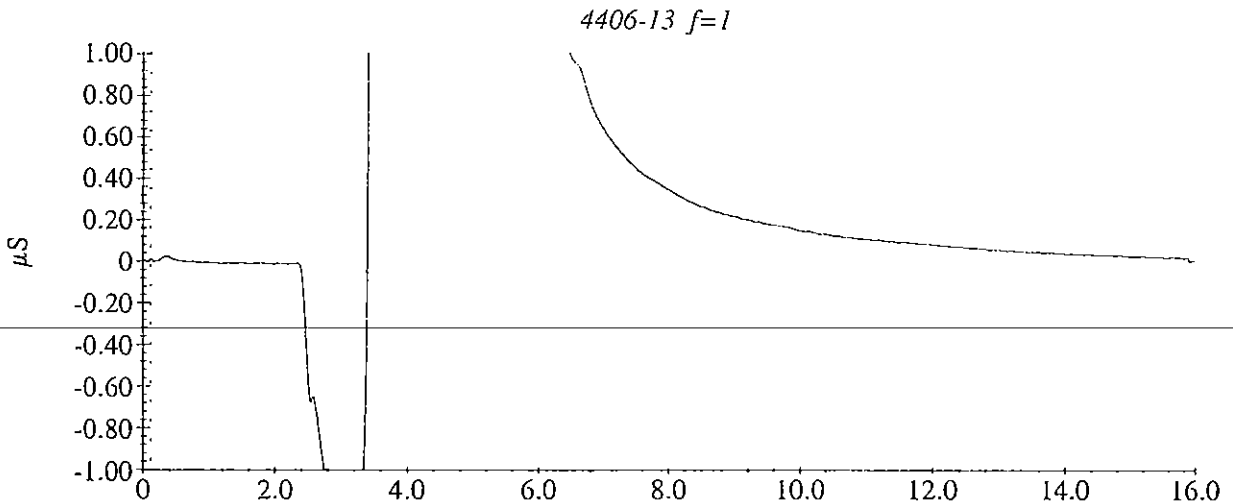

APCL Perchlorate Analysis Report

Sample Name : 4406-10 ms 50ppb f=1 w8033b

Data File Name : C:\DATA\03W3913K\W3913K M01_015.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 1:54:57 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.82	60.51	102685.10	4579.38

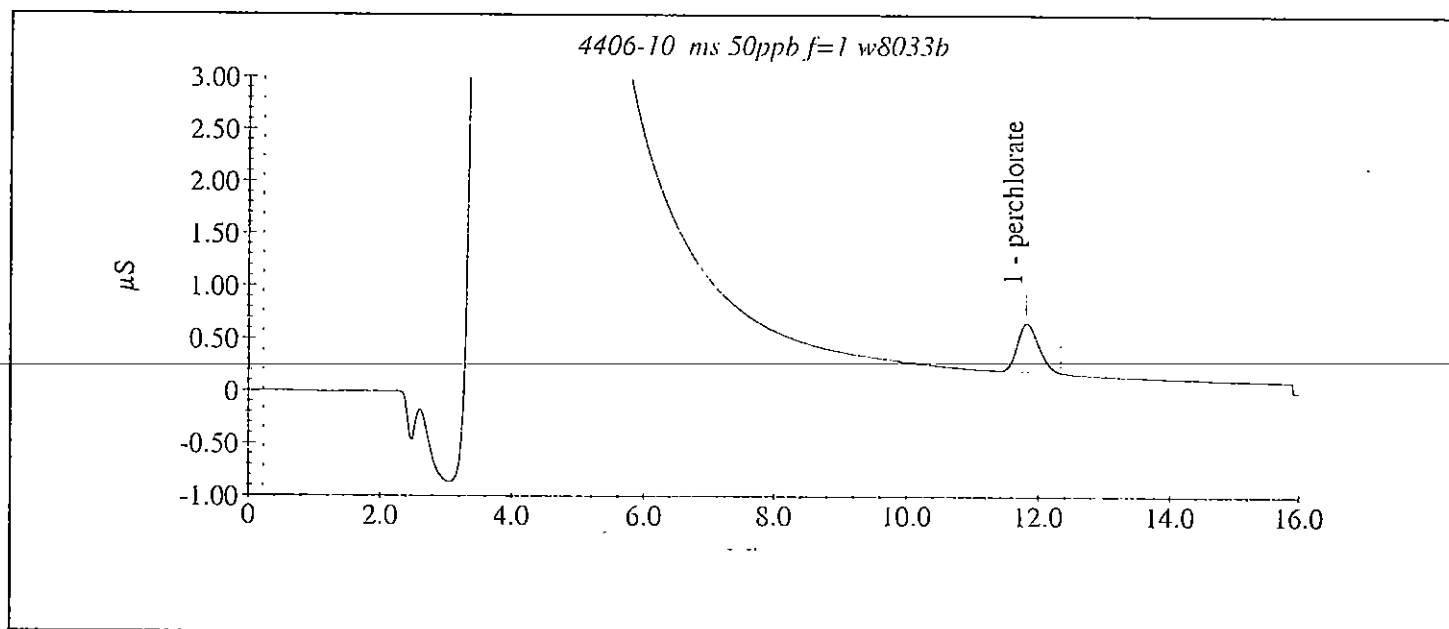

Rec 113.76%



APCL Perchlorate Analysis Report

Sample Name : 4406-10 msd 50ppb f=1 w8033b

Data File Name : C:\DATA\03W3913K\W3913K N01_016.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 2:13:21 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.85	59.68	101278.00	4553.16

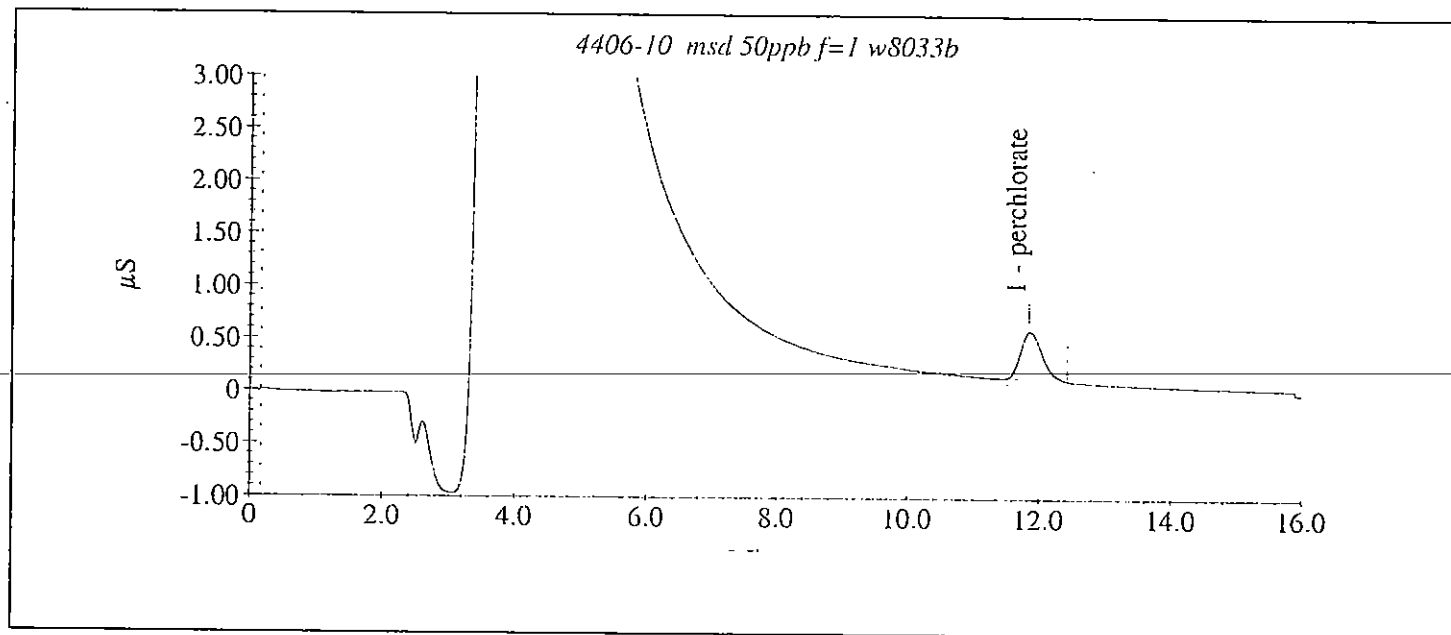

Rec 112.10%



APCL Perchlorate Analysis Report

Sample Name : ccv 50ppb w8082

Data File Name : C:\DATA\03W3913K\W3913K Q01_002.DXD

Method File Name : c:\peaknet\method\ve314-011.met


Date Time Collected : 07/31/2003 9:54:45 AM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.73	55.18	93651.90	4281.52

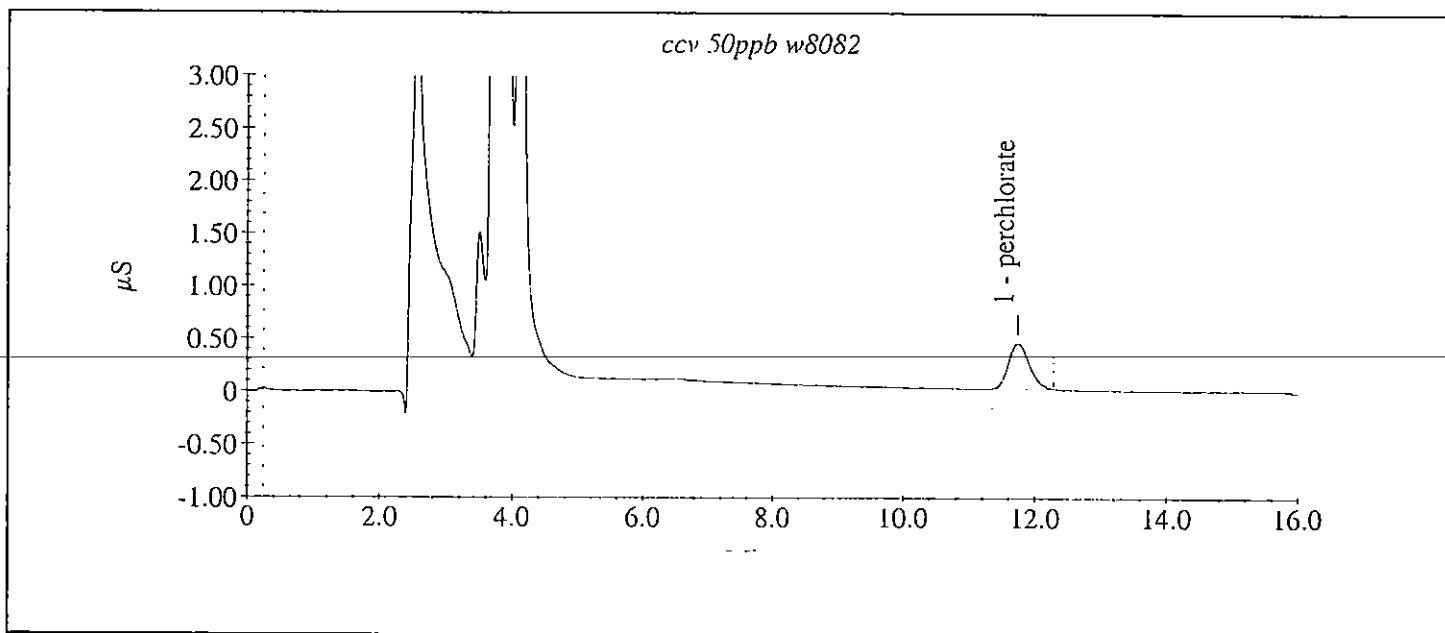

APCL Perchlorate Analysis Report

Sample Name : ccv 50ppb w8082

Data File Name : C:\DATA\03W3913K\W3913K Q02_013.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 1:18:09 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.85	55.56	94289.35	4170.73

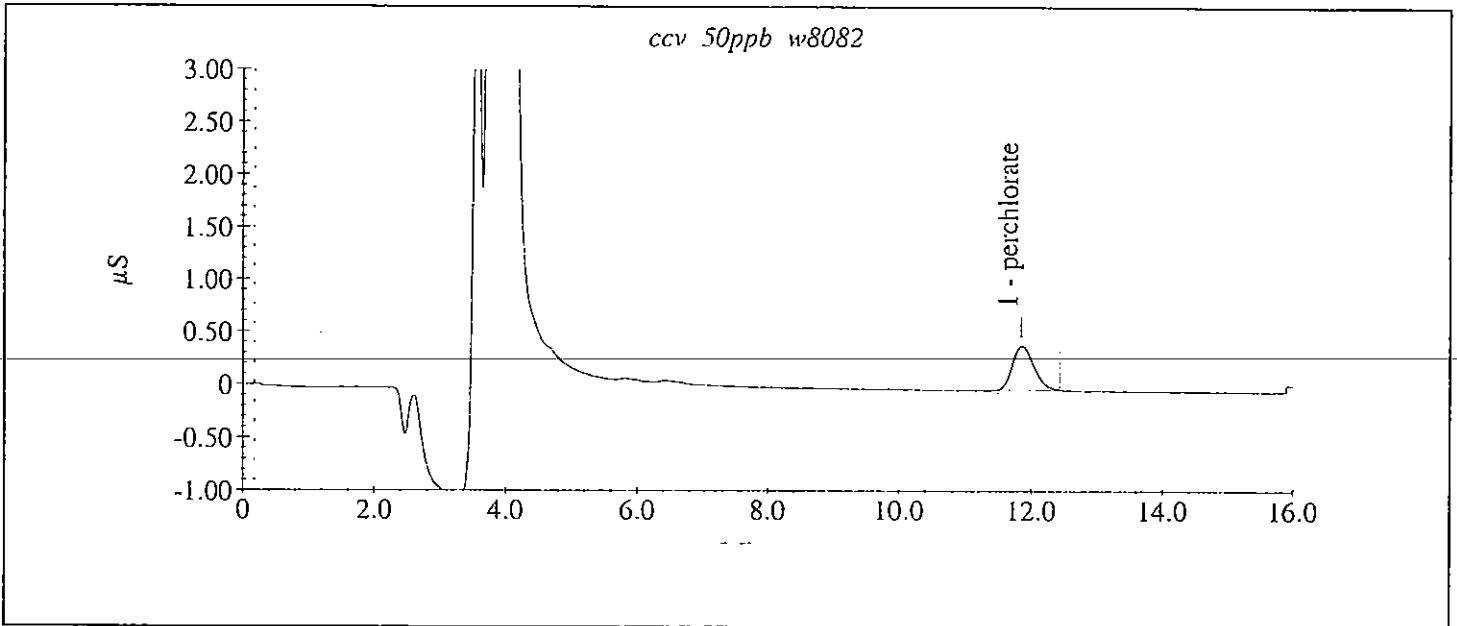

APCL Perchlorate Analysis Report

Sample Name : ccv 50ppb w8082

Data File Name : C:\DATA\03W3913K\W3913K Q03_024.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 4:40:32 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.77	55.38	93981.30	4225.00

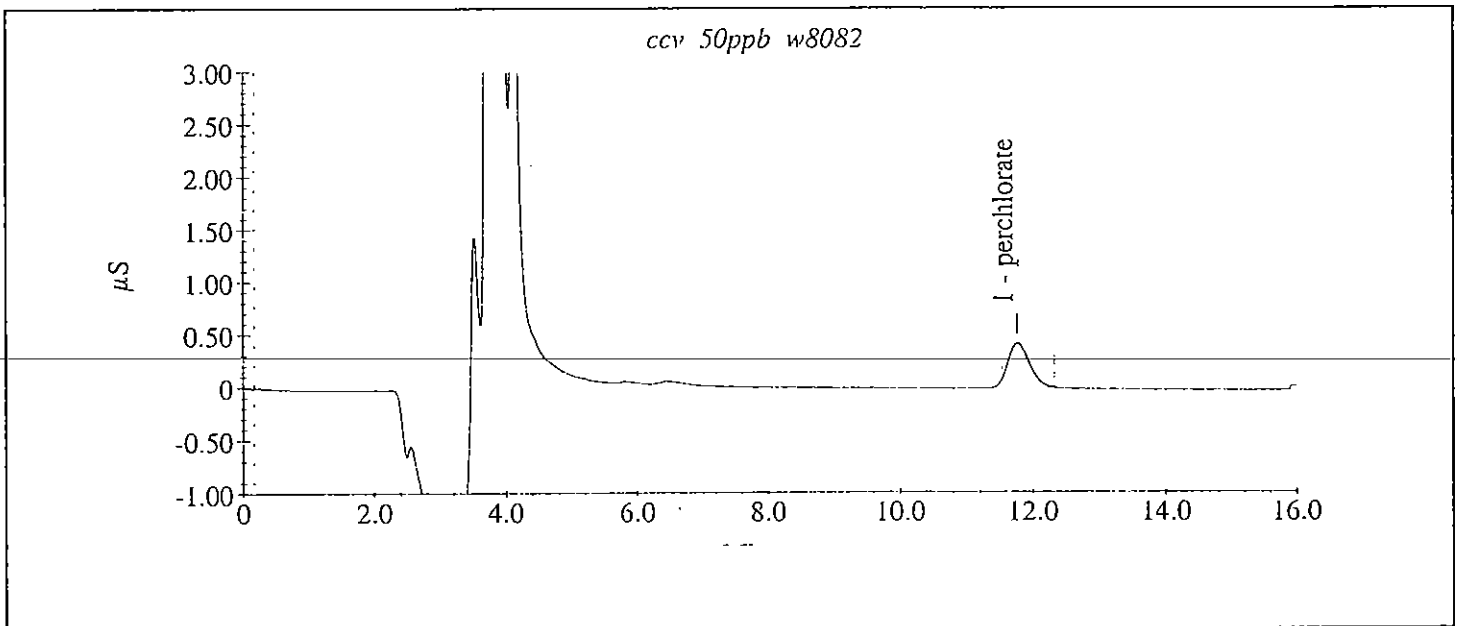

APCL Perchlorate Analysis Report

Sample Name : ccv 50ppb w8082

Data File Name : C:\DATA\03W3913K\W3913K Q04_033.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 7:26:14 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
2	perchlorate	11.60	54.90	93170.05	4266.66

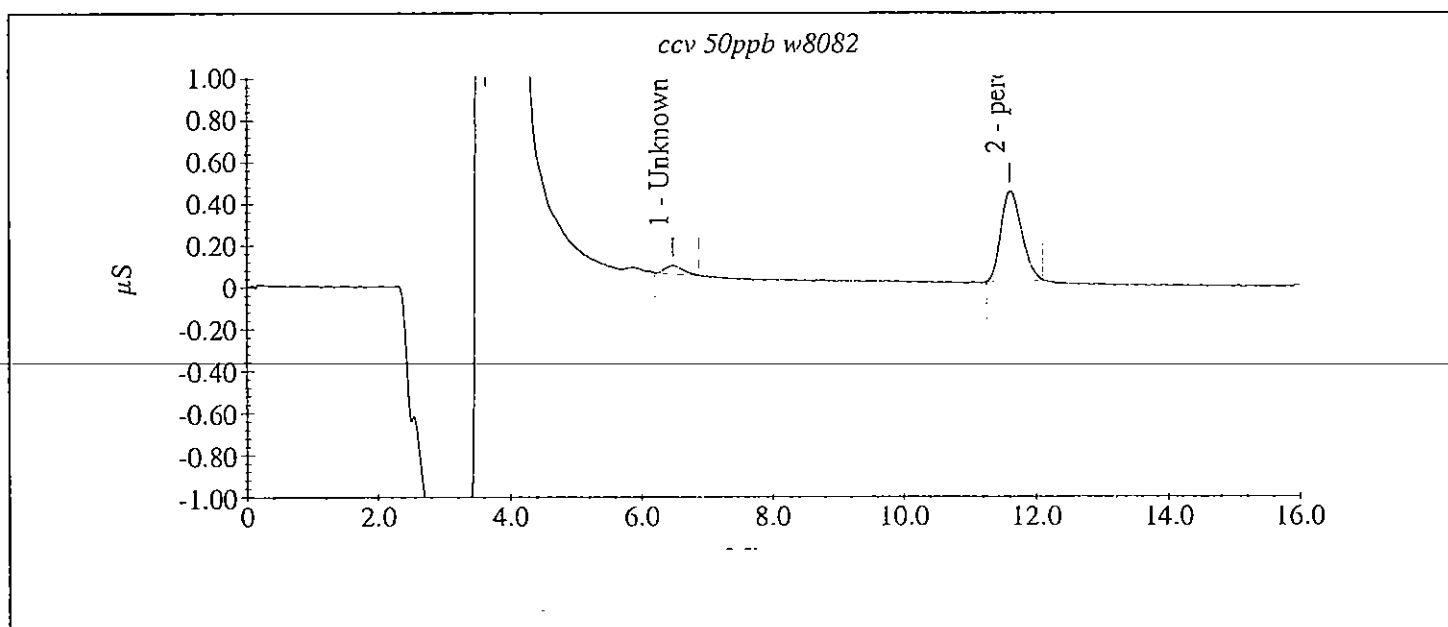

APCL Perchlorate Analysis Report

Sample Name : mb

Data File Name : C:\DATA\03W3913K\W3913K K01_006.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 11:08:31 AM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

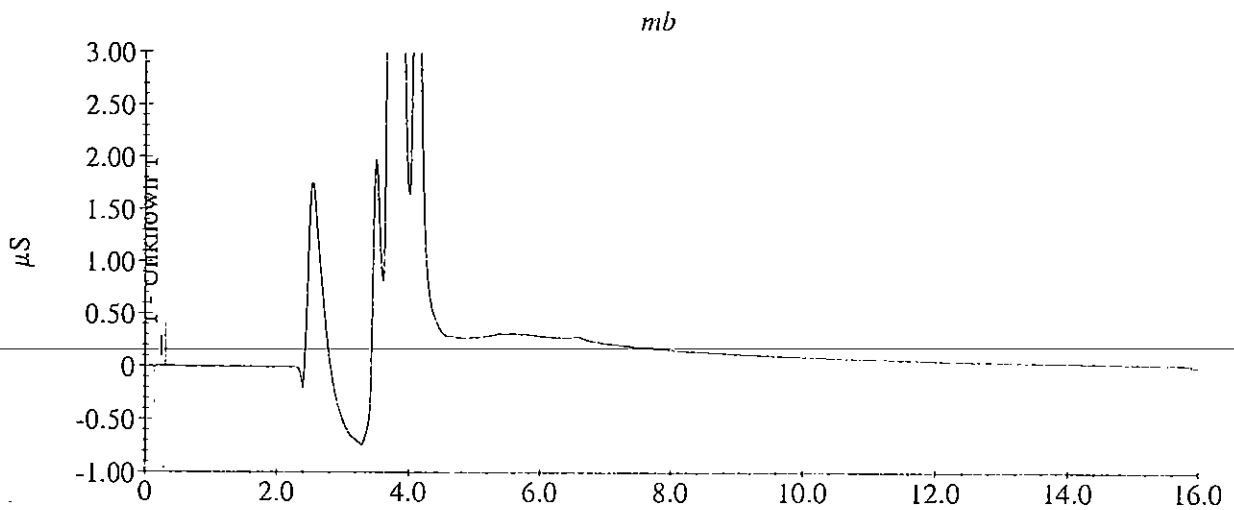

APCL Perchlorate Analysis Report

Sample Name : LCS 18PPB W8033a

Data File Name : C:\DATA\03W3913K\W3913K J01_004.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 10:31:41 AM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.85	18.96	32180.60	1492.49

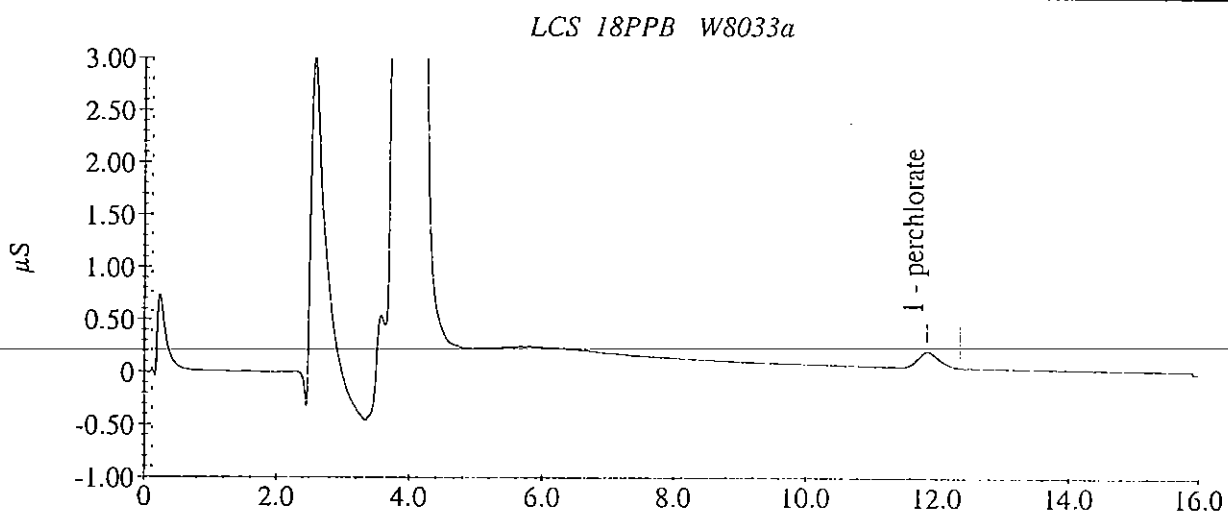

APCL Perchlorate Analysis Report

Sample Name : lcs 25ppb w8087

Data File Name : C:\DATA\03W3913K\W3913K L01_003.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 10:13:15 AM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.73	25.52	43302.60	2033.75

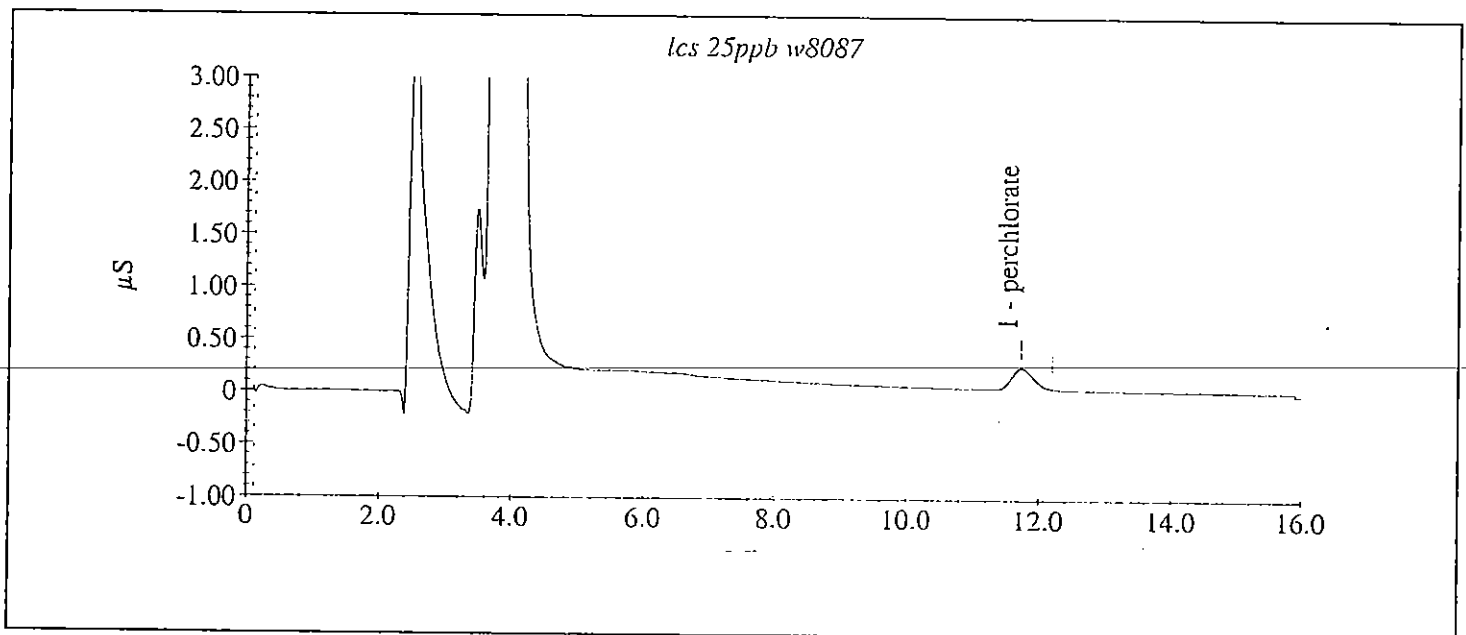

APCL Perchlorate Analysis Report

Sample Name : ICCS 4ppb w8088

Data File Name : C:\DATA\03W3913K\W3913K ICCS 4PPB_005.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 10:50:06 AM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.77	4.19	7110.80	379.71

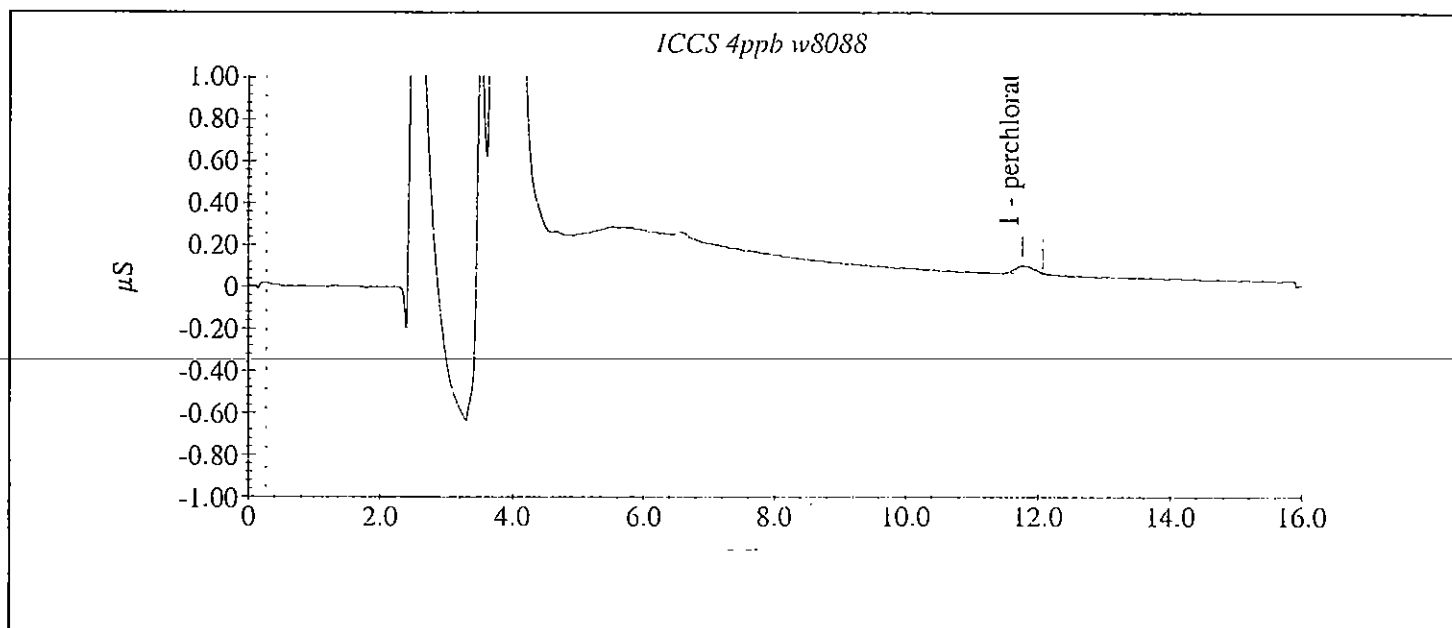

APCL Perchlorate Analysis Report

Sample Name : ccb

Data File Name : C:\DATA\03W3913K\W3913K K02_014.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 1:36:33 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

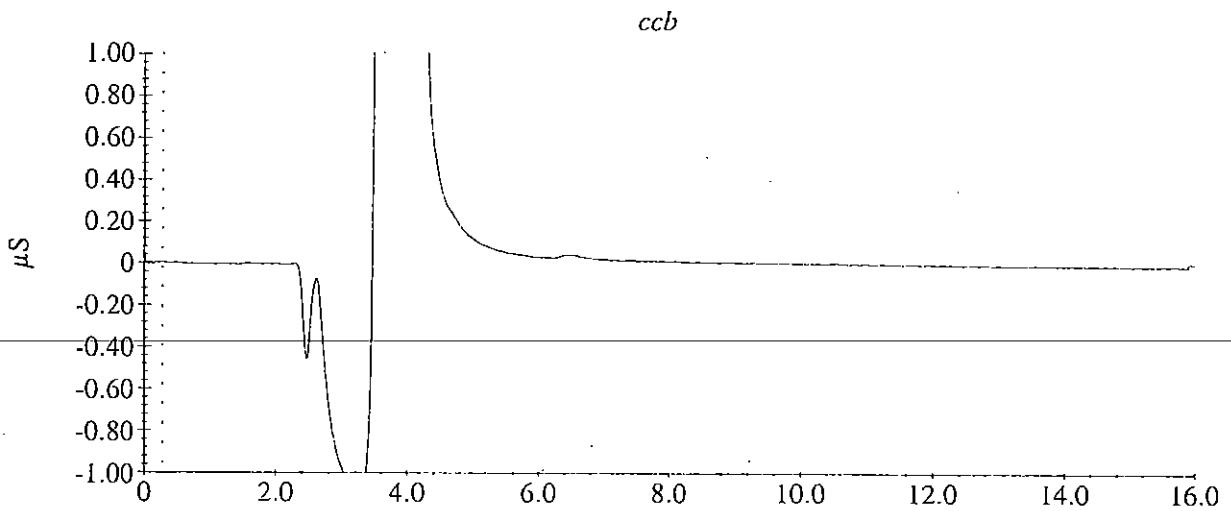

APCL Perchlorate Analysis Report

Sample Name : ##03w3913kw ipc 25ppb w8032

Data File Name : C:\DATA\03W3913K\W3913K IPC 25PPB_001.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 9:33:02 AM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
1	perchlorate	11.77	27.05	45909.00	2002.14

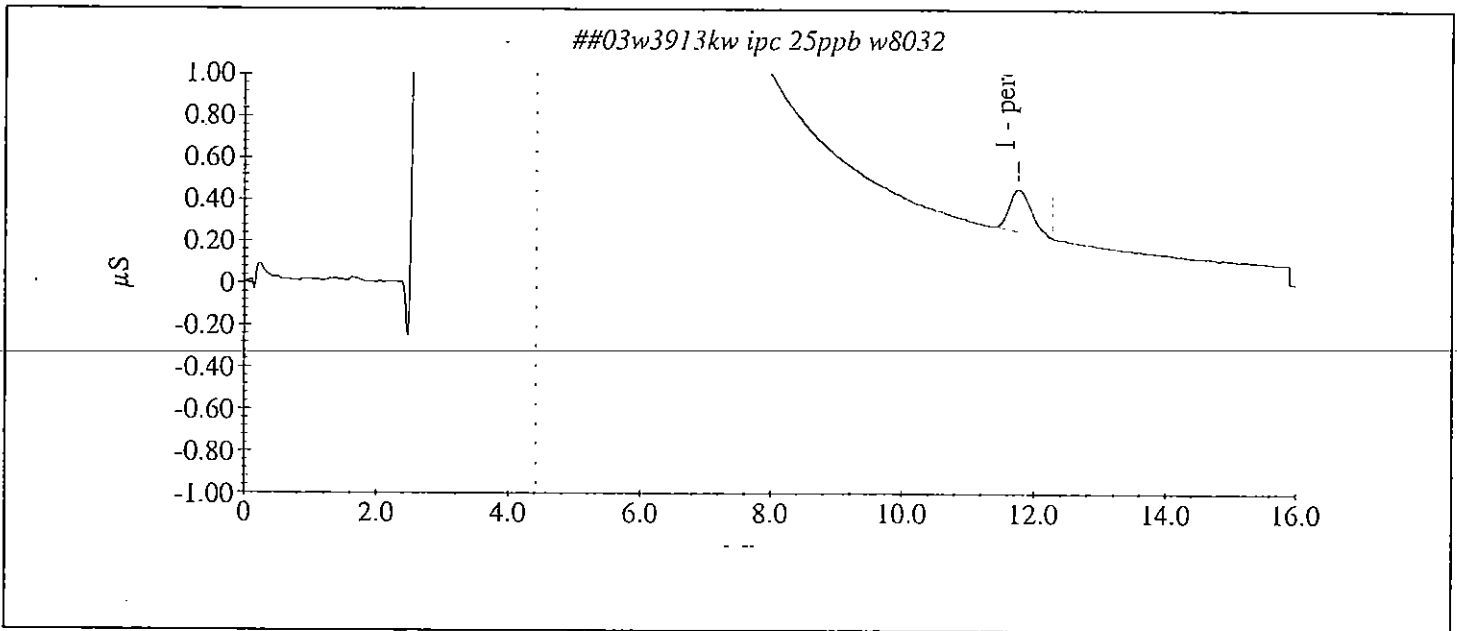

APCL Perchlorate Analysis Report

Sample Name : ccb

Data File Name : C:\DATA\03W3913K\W3913K K03_025.DXD

Method File Name : c:\peaknet\method\314-011.met


Date Time Collected : 07/31/2003 4:58:55 PM

System Operator : C.W and W.W

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

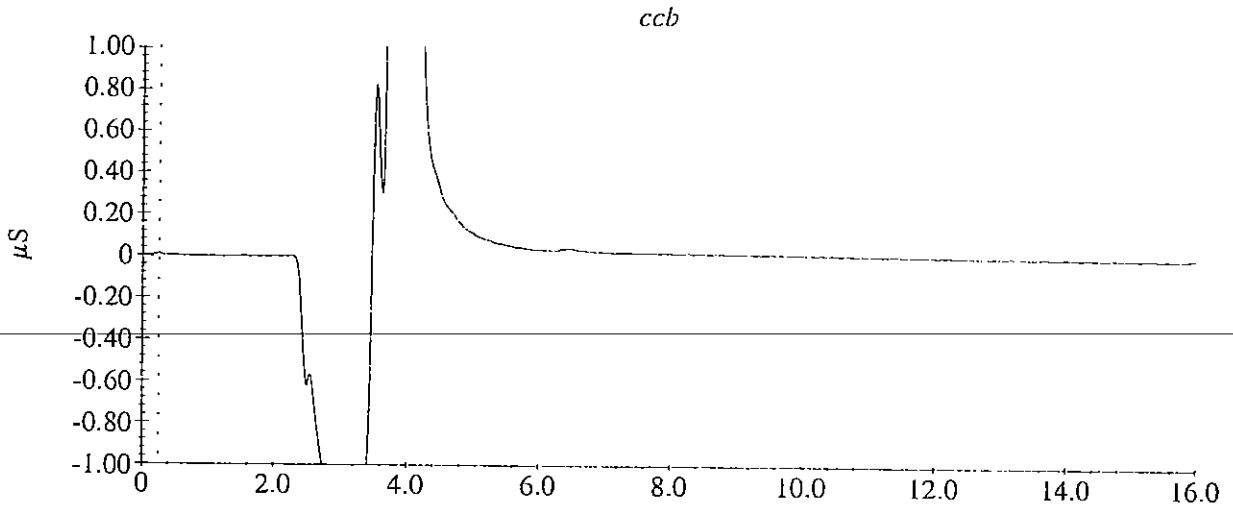

Applied P & Ch Laboratory

760 Magnolia Ave. Chino CA 91710
Tel: (909) 590-1828 Fax: (909) 590-1498

Chromium (VI) (7196) Worksheet

Batch # PC Matrix: WHS [Holding Time: 24 hours!!]

Test Date: 7/28/03 Analyst: [Signature]

Lot #: Reagent Water Diphenylcazide solution Test Time: _____ SOP: _____

Calibration	STD Lot #	$C_{std} \times V_{std} / V_j = C_i$	A_i	$RF_i = A_i / C_i$	Calibration results	Note
STD-1	W-7757	x / = 0.00 mg/L	0.000		Least Square [RF]=	Cal. Code:
STD-2	W-	x / = 0.01 mg/L	0.007		Average RF=	
STD-3	W-	x / = 0.02 mg/L	0.017		C.C. <u>0.999</u> (≥ 0.995)	
STD-4	W-	x / = 0.05 mg/L	0.107		RSD= % ($\leq 15\%$)	
STD-5	W-	x / = 0.10 mg/L	0.212		Ref. page	
STD-6	W-	x / = 0.50 mg/L	0.420		$A = -0.001 + 0.846C$	

Analysis Type	Sample ID or Lot #	Samp. Amt X_0 (g or mL)	Dilu./Ext $X/X_0 = f_1$	Treat. Ratio $V/X = f_2$	540 nm A	Concentration $C' = A / RF$	C (Sample) $C = f_1 f_2 C'$	Ano N
CCV	Lot: W-7853	Expected Conc.: x	1	= 0.05 mg/L	0.218	0.259 mg/L	REC. %	90-1
Method Blank	Bl. Lot:		$X_0 =$	95.0/ =	0.000	0.000 mg/L	ppm	
LCS1	Bl. Lot:		$X_0 =$	95.0/ =	0.210	0.250 mg/L	ppm	
Sample-1	4177-37	1ml \rightarrow 100ml $X_0 = 1$		95.0/ = 2	0.290	0.689 mg/L	ppm	
MS on S-1	37	0.5ml \rightarrow 100ml $X_0 =$		95.0/ = 2	0.287	0.682 mg/L	ppm	report
MSD on S-1	4175-15	10.0g \rightarrow 500mg $X_0 = 5$		95.0/ = 10	0.050	3.04 mg/L	ppm	
Sample 2	15		$X_0 =$	95.0/ = 2	0.247	2.94 mg/L	ppm	report
Sample 3			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 4			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 5			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 6			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 7			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 8			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 9			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 10			$X_0 =$	95.0/ =		mg/L	ppm	
Blank	Lot:		$X_0 =$	95.0/ =		mg/L	ppm	
LCS2	Bl. Lot:		$X_0 =$	95.0/ =		mg/L	ppm	
Sample 11			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 12			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 13			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 14			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 15			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 16			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 17			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 18			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 19			$X_0 =$	95.0/ =		mg/L	ppm	
Sample 20			$X_0 =$	95.0/ =		mg/L	ppm	
MTX Dup.	<u>Lot: 405.90 mg/L</u>		$X_0 =$	95.0/ =	0.248	0.259 mg/L	ppm	

Type	STD Lot #	$C_{STD}(\mu\text{s/mL}) \times V_{STD}(\text{mL}) / X(\text{g or mL}) = T$	Spike Rec.	Ctl Limit (W/S)	PQL/MDL (in ppm)
MS	W-	x / = ppm	%	80-120 %/80-120 %	PQL(w) 0.01
MSD	W-	x / = ppm	%	PQL(s) 0.05
LCS	W-	x / = ppm	%	80-120 %/80-120 %	MDL(w) 0.005
LCSD	W-	x / = ppm	%	MDL(s) 0.025

1778

Chromium (VI) (7196) Worksheet

#03W3907

Matrix: W

[Holding Time: 24 hours!!]

Test Date: 7/30/03

Analyst: hr

Test Time: 13:59

SOP: G-22

Lot #: Reagent Water

Diphenylcazide solution


Calibration	STD Lot #	$C_{std} \times V_{std} / V_j = C_i$	A_i	$RF_i = A_i / C_i$	Calibration results	Note
STD-1	W-	x / = mg/L			Least Square [RF]=	Cal. Code:
STD-2	W-	x / = mg/L			Average RF=	
STD-3	W-	x / = mg/L			C.C.=0.999 (> 0.995)	
STD-4	W-	x / = mg/L			RSD= % (< 15%)	
STD-5	W-	x / = mg/L			Ref. page	
STD-6	W-	x / = mg/L				

$A = -0.001 + 0.846C$

Analysis Type	Sample ID or Lot #	Samp. Amnt X_0 (g or mL)	Dilu./Ext $X/X_0 = f_1$	Treat. Ratio $V/X = f_2$	540 nm A	Concentration $C' = A/RF$	C (Sample) $C = f_1 f_2 C'$	Anomaly Note
CCV	Lot: W- 7757	Expected Conc.: x	1	= 2.25 mg/L	0.210	0.249 mg/L	REC.	% 90-110 %
Method Blank	Bl. Lot: 7117		$1/X_0 =$	95.0/ =	0.000	mg/L	0.001 ppm	
LCS1	Bl. Lot: 11		$1/X_0 =$	95.0/ =	0.194	mg/L	0.230 ppm	
Sample 1	4406-3		$1/X_0 =$	95.0/ =	0.001	mg/L	0.002 ppm	
MS on S-1	4		$1/X_0 =$	95.0/ =	0.188	mg/L	0.223 ppm	
MSD on S-1	4		$1/X_0 =$	95.0/ =	0.192	mg/L	0.228 ppm	
Sample 2	4		$1/X_0 =$	95.0/ =	0.002	mg/L	0.004 ppm	
Sample 3	5		$1/X_0 =$	95.0/ =	0.003	mg/L	0.005 ppm	
Sample 4	6		$1/X_0 =$	95.0/ =	0.002	mg/L	0.004 ppm	
Sample 5	7		$1/X_0 =$	95.0/ =	0.003	mg/L	0.005 ppm	
Sample 6	8		$1/X_0 =$	95.0/ =	0.001	mg/L	0.002 ppm	
Sample 7			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 8			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 9			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 10			$1/X_0 =$	95.0/ =		mg/L	ppm	
Blank	Lot: 7117		$1/X_0 =$	95.0/ =		mg/L	ppm	
LCS2	Bl. Lot: 7117		$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 11			$1/X_0 =$	95.0/ =	0.199	mg/L	0.236 ppm	
Sample 12			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 13			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 14			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 15			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 16			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 17			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 18			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 19			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 20			$1/X_0 =$	95.0/ =		mg/L	ppm	
MTX Dup.			$1/X_0 =$	95.0/ =	0.202	0.240 mg/L	ppm	

Type	STD Lot #	$C_{STD} (\mu\text{g/mL}) \times V_{STD} (\text{mL}) / X (\text{g or mL}) = T$	Spike Rec.	Ctrl Limit (W/S)	PQL/MDL (in ppm)
MS	W- 7757	x / = 0.25 ppm	%	80-120 %/80-120 %	PQL(w) 0.01
MSD	W-	x / = ppm	%	PQL(s) 0.05
LCS	W- 7853	x / = ppm	%	80-120 %/80-120 %	MDL(w) 0.005
LCSD	W-	x / = ppm	%	MDL(s) 0.025

1. Component: perchlorate
Standard: External Fit Type: Linear
Origin: Force Calibration: Area
 $r^2=0.999492$
Amt=0.0005893*Resp+0

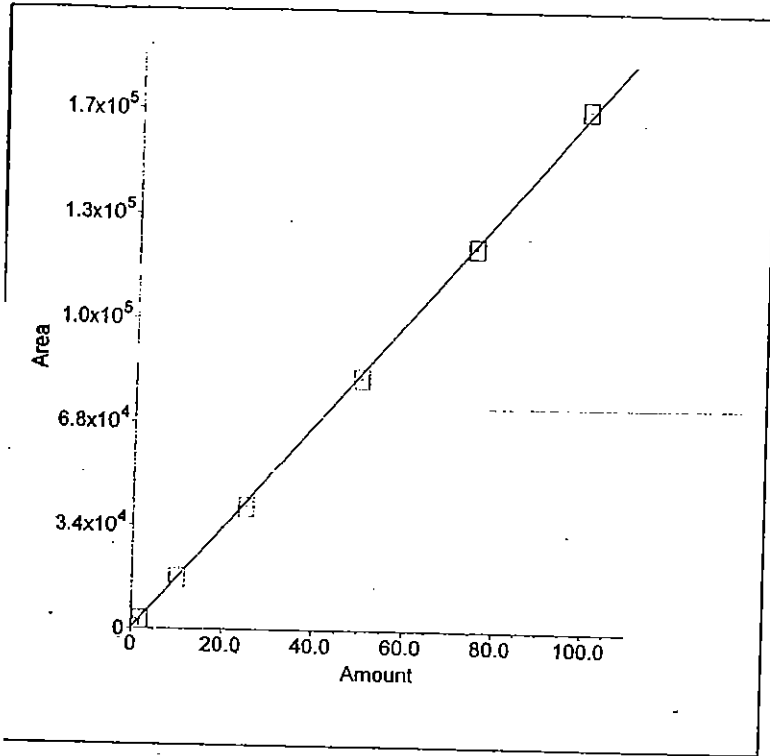

Calibration : 7 points , 0, 2, 10, 25, 50, 75, 100 ppb

Analyst C.W
Date 03/12/03
Instrument IC-10

APCL Perchlorate Analysis Report

Sample Name : Cal blank

Data File Name : C:\data\E314-011\Mb_001.DXD

Method File Name : c:\peaknet\method\e314-011.met


Date Time Collected : 03/12/2003 5:55:39 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

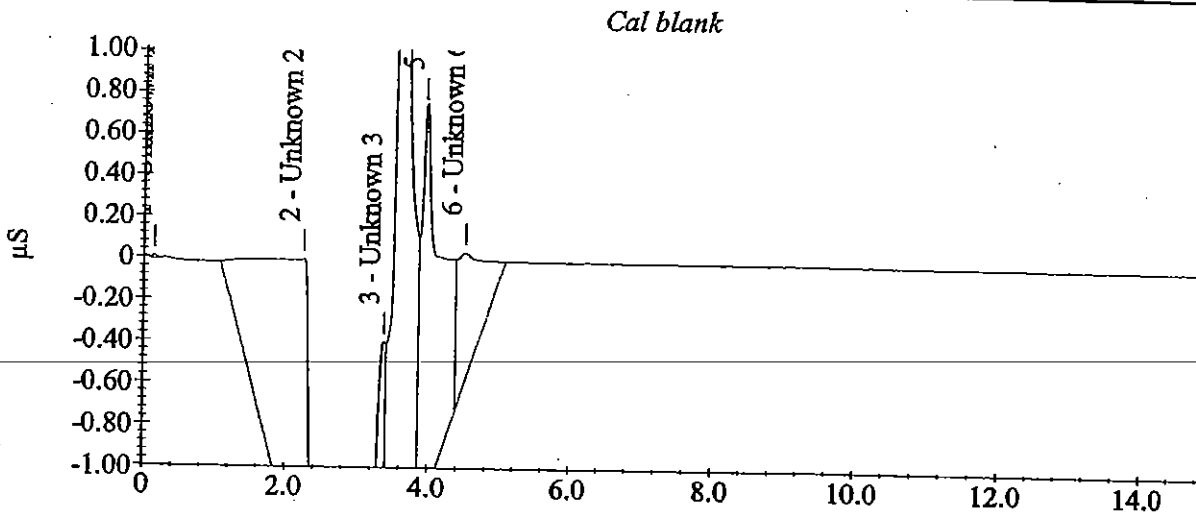

APCL Perchlorate Analysis Report

Sample Name : cal standard 2ppb W7827a

Data File Name : C:\DATA\E314-011\std-2pb_002.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 6:13:12 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.62	1.92	2910	164

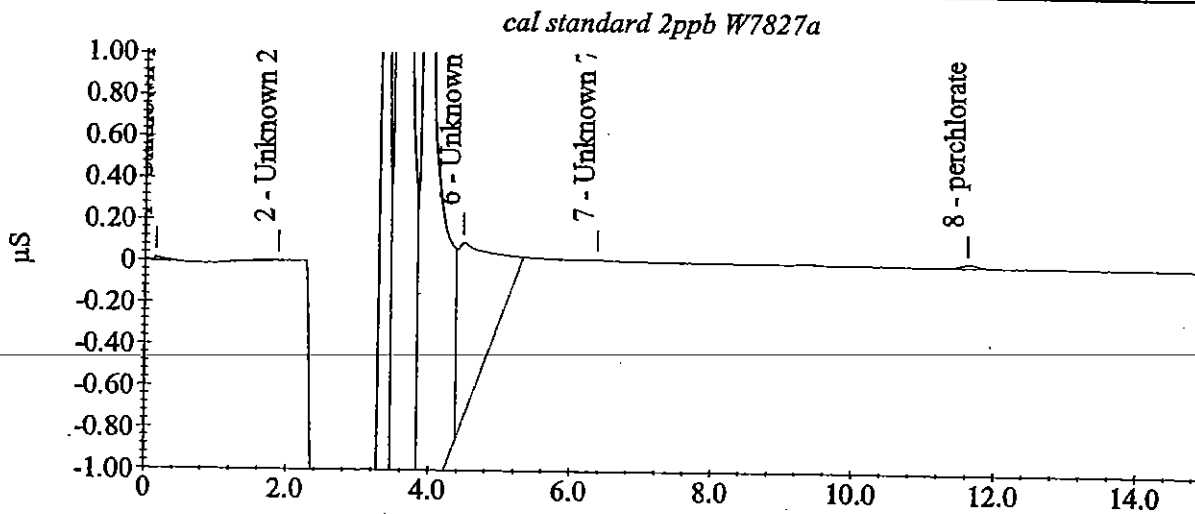

APCL Perchlorate Analysis Report

Sample Name : cal standard 10ppb W7827c

Data File Name : C:\DATA\E314-011\std-10pb_004.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 6:48:21 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
7	perchlorate	11.70	11.16	16917	879

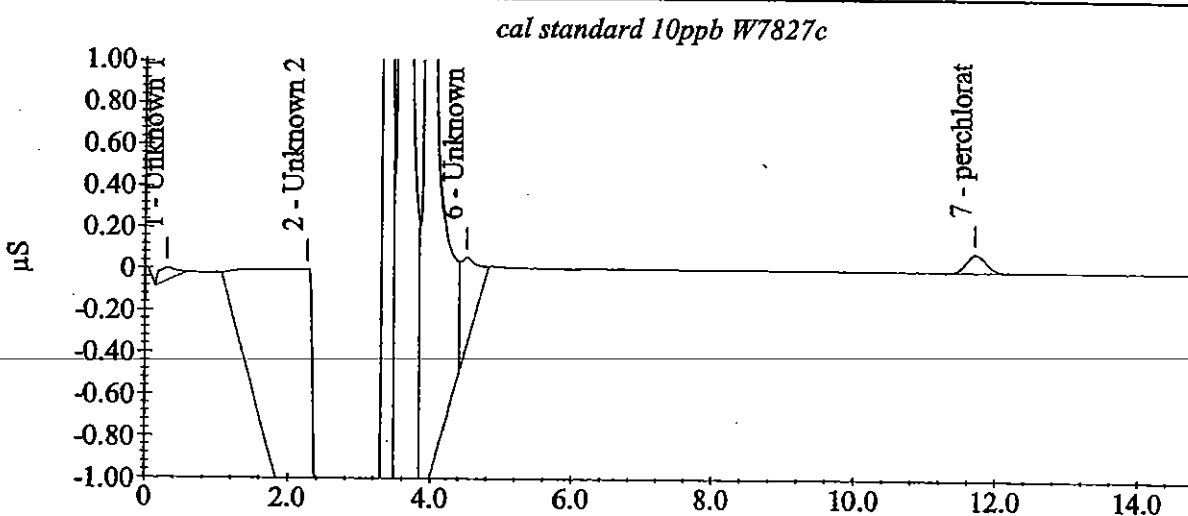

APCL Perchlorate Analysis Report

Sample Name : cal standard 25ppb W7827d

Data File Name : C:\DATA\E314-011\std-25pb_005.DXD

Method File Name : C:\PEAKNET\METHOD\E314-011.met


Date Time Collected : 03/12/2003 7:05:54 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.60	26.84	40702	2125

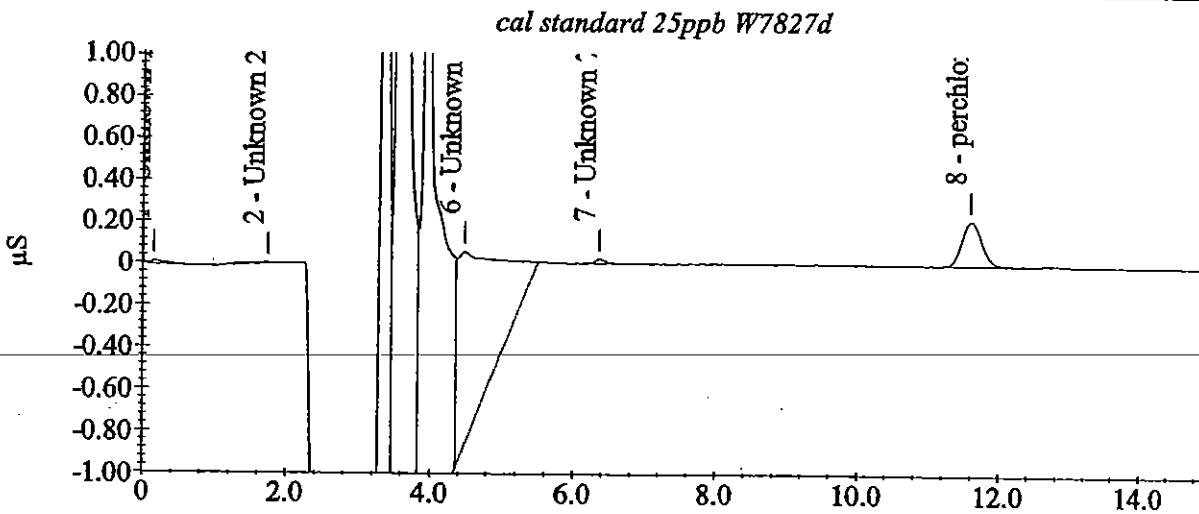

APCL Perchlorate Analysis Report

Sample Name : cal standard 50ppb W7827e

Data File Name : C:\DATA\E314-011\std-50pb_006.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 7:23:30 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.67	54.89	83240	4320

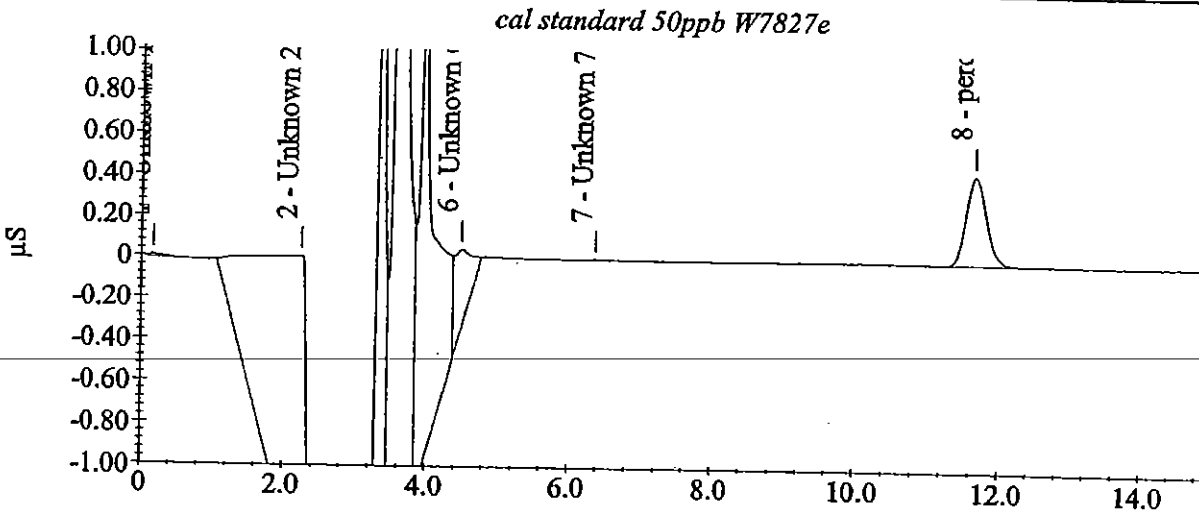

APCL Perchlorate Analysis Report

Sample Name : cal standard 75ppb W7827f

Data File Name : C:\DATA\E314-011\std-75pb_007.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 7:41:05 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
7	perchlorate	11.62	83.23	126224	6553

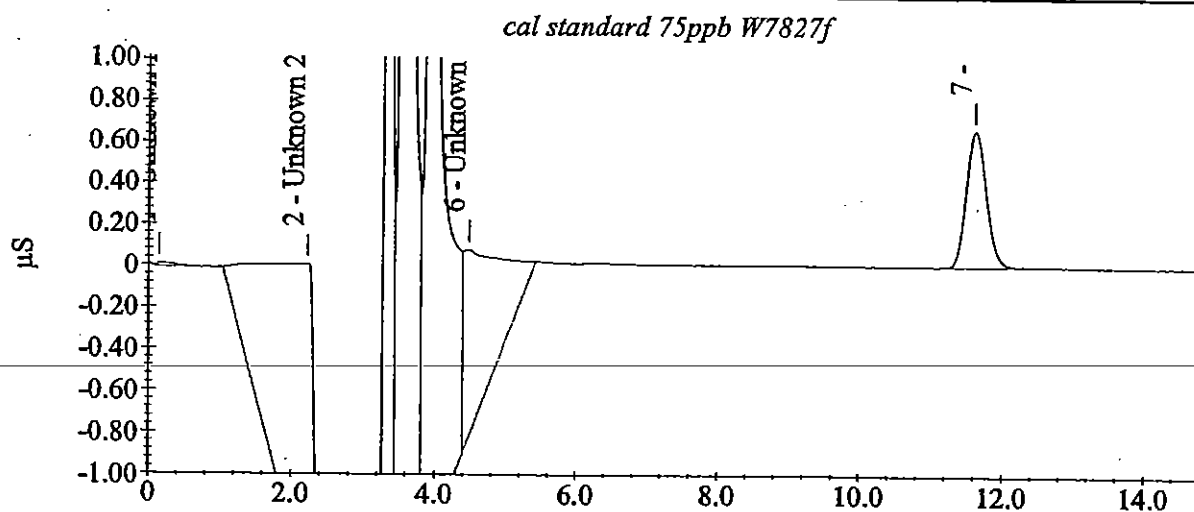

APCL Perchlorate Analysis Report

Sample Name : cal standard 100ppb W7827g

Data File Name : C:\DATA\E314-011\std-100pb_008.DXD

Method File Name : C:\PEAKNET\METHOD\ve314-011.met


Date Time Collected : 03/12/2003 7:58:39 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.62	113.21	171686	892

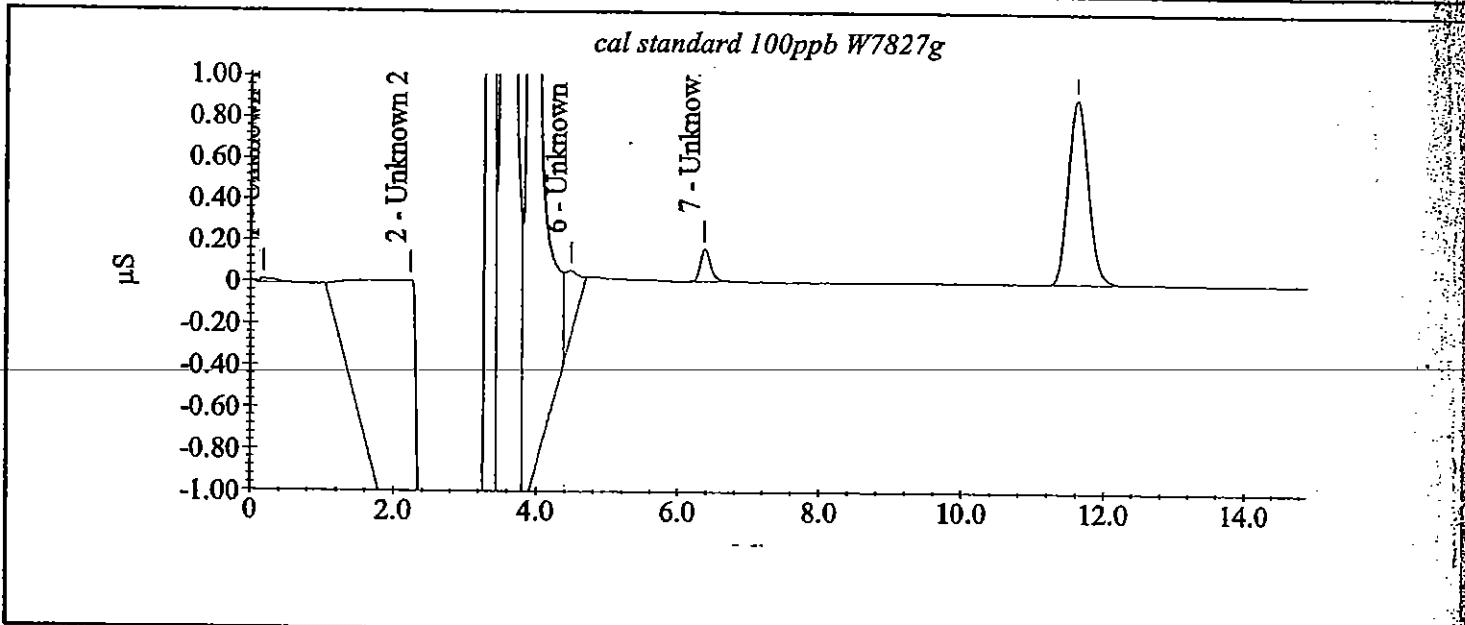

APCL Perchlorate Analysis Report

Sample Name : ICV 50 ppb w7828a

Data File Name : C:\DATA\E314-011\icv-50pb_009.DXD

Method File Name : C:\PEAKNET\METHOD\E314-011.met


Date Time Collected : 03/12/2003 8:16:15 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.65	49.49	83990	4321

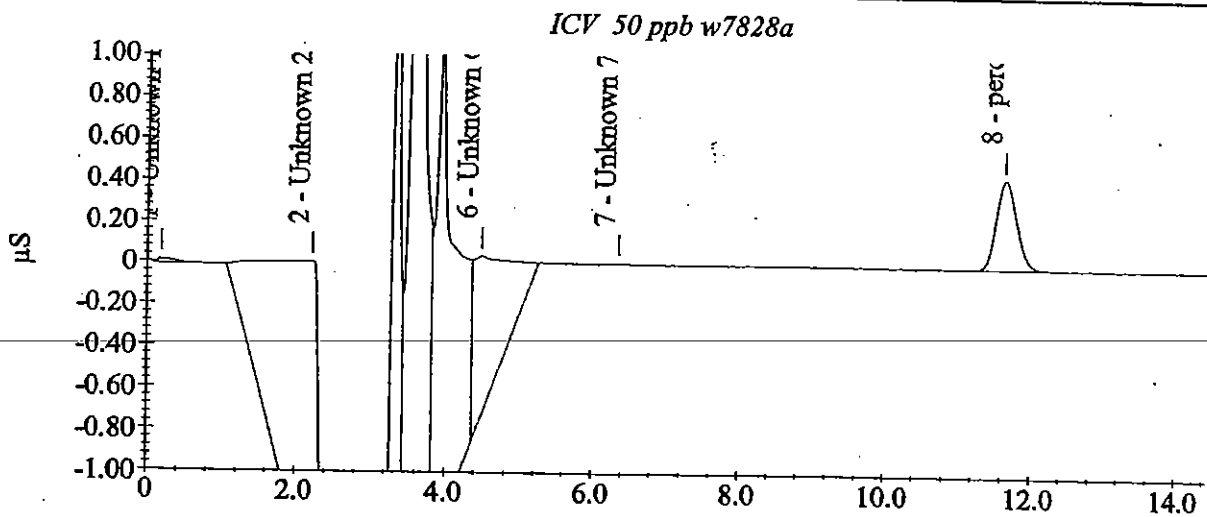

APCL Perchlorate Analysis Report

Sample Name : icb

Data File Name : C:\DATA\E314-011\ICB_010.DXD

Method File Name : c:\PeakNet\method\E314-011.met


Date Time Collected : 03/12/2003 8:33:51 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

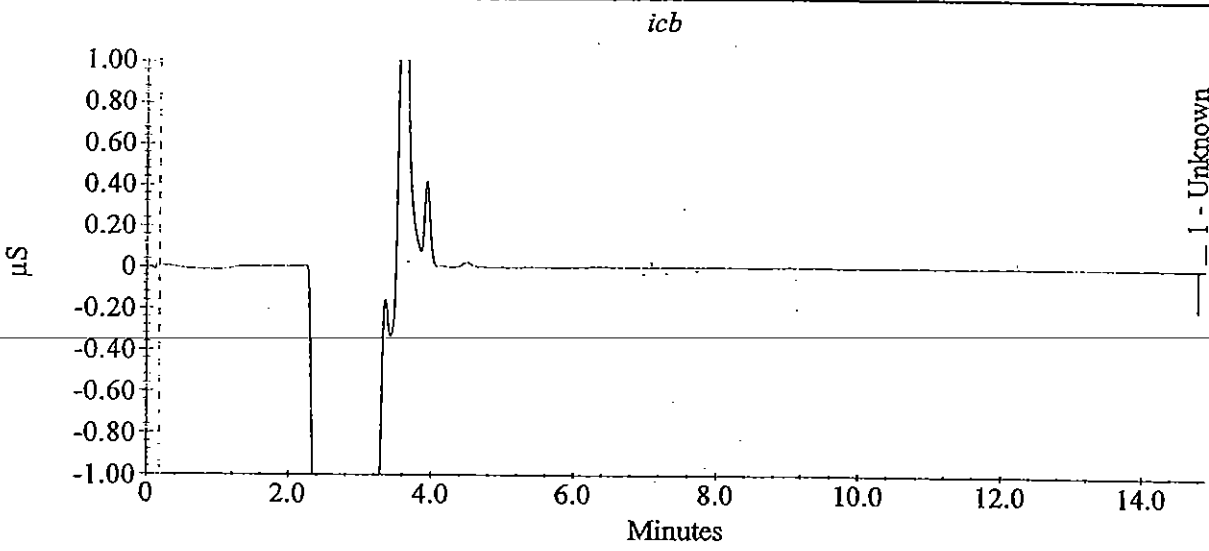

Line	Sample	Sample Type	Level	Method	Data File	Volume	Dilution
1	Cal blank	Sample		e314-011.met	c:\data\314-01\mb_001.dxd	1	1
2	cal standard 2ppb W7827a	Sample		e314-011.met	c:\data\314-01\std-2pb_002.dxd	1	1
3	cal standard 4ppb W7827b	Sample		e314-011.met	c:\data\314-01\std-4pb_003.dxd	1	1
4	cal standard 10ppb W7827c	Sample		e314-011.met	c:\data\314-01\std-10pb_004.dxd	1	1
5	cal standard 25ppb W7827d	Sample		e314-011.met	c:\data\314-01\std-25pb_005.dxd	1	1
6	cal standard 50ppb W7827e	Sample		e314-011.met	c:\data\314-01\std-50pb_006.dxd	1	1
7	cal standard 75ppb W7827f	Sample		e314-011.met	c:\data\314-01\std-75pb_007.dxd	1	1
8	cal standard 100ppb W7827g	Sample		e314-011.met	c:\data\314-01\std-100pb_008.dxd	1	1
9	ICV 50 ppb w7828a	Sample		e314-011.met	c:\data\314-01\icv-50pb_009.dxd	1	1
10	icb	Sample		e314-011.met	c:\data\314-01\icb_010.dxd	1	1
11	anion 100pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\mct-100_011.dxd	1	1
12	anion 200pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\mct-200_012.dxd	1	1
13	anion 300pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\mct-300_013.dxd	1	1
14	anion 400pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\mct-400_014.dxd	1	1
15	anion 500pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\mct-500_015.dxd	1	1
16	anion 600pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\mct-600_016.dxd	1	1
17	anion 800pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\mct-800_017.dxd	1	1
18	anion 1000pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-01\mct-1000_018.dxd	1	1
19	anion 400pm each 2pb	Sample		e314-011.met	c:\data\314-01\ipc-2pb_019.dxd	1	1
20	anion 400pm each 4pb	Sample		e314-011.met	c:\data\314-01\ipc-4pb_020.dxd	1	1
21	anion 400pm each 25pb	Sample		e314-011.met	c:\data\314-01\ipc-25pb_021.dxd	1	1
22	ICV 50 ppb	Sample		e314-011.met	c:\data\314-01\iccv-50pb	1	1
23	MDL 4pb	Sample		e314-011.met	c:\data\314-01\mdl-02_023.dxd	1	1
24	MDL 4pb	Sample		e314-011.met	c:\data\314-01\mdl-03_024.dxd	1	1
25	MDL 4pb	Sample		e314-011.met	c:\data\314-01\mdl-04	1	1
26	MDL 4pb	Sample		e314-011.met	c:\data\314-01\mdl-05	1	1
27	MDL 4pb	Sample		e314-011.met	c:\data\314-01\mdl-06	1	1
28	MDL 4pb	Sample		e314-011.met	c:\data\314-01\mdl-07	1	1
29	MDL 4pb	Sample		e314-011.met	c:\data\314-01\mdl-08	1	1
30	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\idap-25pb	1	1
31	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\idap-25pb	1	1
32	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\idap-25pb	1	1
33	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\idap-25pb	1	1
34	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\idap-25pb	1	1
35	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\idap-25pb	1	1
36	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-01\idap-25pb	1	1
37	MCT anion 800pm each, 25pbCLO4	Sample		e314-011.met	c:\data\314-01\ipo-25pb	1	1
38	MCT anion 800pm each, 25pbCLO4	Sample		e314-011.met	c:\data\314-01\ipc-25pb	1	1
39	MCT anion 800pm each, 4pbCLO4	Sample		e314-011.met	c:\data\314-01\ipc-4pb	1	1
40	MCT anion 800pm each, 4pbCLO4	Sample		e314-011.met	c:\data\314-01\ipc-4pb	1	1
41	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\mdl-s01	1	5
42	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\mdl-s02	1	5
43	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\mdl-s03	1	5
44	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\mdl-s04	1	5
45	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\mdl-s05	1	5
46	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\mdl-s06	1	5
47	MDL 20pb soil	Sample		e314-011.met	c:\data\314-01\mdl-s07	1	5
48	standard 25ppb W7827d	Sample		e314-011.met	c:\data\314-01\std-25pb	1	1
49	anion 100pm each,4pb CLO4	Sample		e314-011.met	c:\data\314-01\lam-100-4pb	1	1
50	anion 200pm each ,4pb CLO4	Sample		e314-011.met	c:\data\314-01\lam-200-4pb	1	1
51	anion 300pm each ,4pb CLO4	Sample		e314-011.met	c:\data\314-01\lam-300-4pb	1	1
52	anion 100pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-01\lam-100-2pb	1	1
53	anion 200pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-01\lam-200-2pb	1	1
54	anion 300pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-01\lam-300-2pb	1	1
55	1982-01 B S.C 4450us/cm	Sample		e314-011.met	c:\data\314-01\1982-01	1	1
56	1982-01 B S.C 4450us/cm	Sample		e314-011.met	c:\data\314-01\1982-01	1	2
57	1982-02 f=10	Sample		e314-011.met	c:\data\314-01\1982-02_057.dxd	1	10
58		Sample		aastopcl.met		1	1

Line	Weight	Int. Std.	Comment
1	1	1	
2	1	1	
3	1	1	
4	1	1	
5	1	1	
6	1	1	
7	1	1	
8	1	1	
9	1	1	
10	1	1	
11	1	1	
12	1	1	
13	1	1	
14	1	1	
15	1	1	
16	1	1	
17	1	1	
18	1	1	
19	1	1	
20	1	1	
21	1	1	
22	1	1	
23	1	1	
24	1	1	
25	1	1	
26	1	1	
27	1	1	
28	1	1	
29	1	1	
30	1	1	
31	1	1	
32	1	1	
33	1	1	
34	1	1	
35	1	1	
36	1	1	
37	1	1	
38	1	1	
39	1	1	
40	1	1	
41	1	1	
42	1	1	
43	1	1	
44	1	1	
45	1	1	
46	1	1	
47	1	1	
48	1	1	
49	1	1	
50	1	1	
51	1	1	
52	1	1	
53	1	1	
54	1	1	
55	1	1	
56	1	1	
57	1	1	
58	1	1	

Default Method Path: C:\PEAKNET\METHOD
 Default Data Path: C:\DATA\03W1286K
 Comment:
 Remark:

Condition information:

1. Column

Separator column: AS16 4mm

Guard column: AS16 4mm

2. Eluent: NaOH 38mM

3. Flow rate: 1.2mL/min

4. Suppressor: ASRS-ULTRA 4mm

5. Detector: CD20

6. Analyst: Charles Wu and Wei Wang

7. Date: 03 / 12 / 2003

8. Instrument: IC-K DX-500 Dionex



A P C L

Applied Physics & Chemistry Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel. (909) 590-1828 Fax (909) 590-1498

Sep 02, 2003

GEOFON, Inc.
Attention: Brad Shojaee
22632 Golden Spring Dr Ste 270
Diamond Bar CA 91765

Dear Brad,

This package contains samples in our Service ID 03-4455 and your project : 04-4428.10 JPL
Enclosed please find:

- (1) Original analytical report.
- (2) Original Chain of Custody.
- (3) One diskette containing EDD deliverable.
- (4) One original Level C Data Package Deliverable.

If anything is missing or you have any questions, please feel free to contact me.

Respectfully submitted,

Regina Kirakozova
Associate QA/QC Director
Applied P & Ch Laboratory

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Submitted to:

GEOFON, Inc.

Attention: Brad Shojaee.

22632 Golden Spring Dr Ste 270

Diamond Bar CA 91765

Tel: (909)396-7662 Fax: (909)396-1455

APCL Analytical Report

Service ID #: 801-034455

Received: 08/04/03

Collected by: Leo Williamson

Extracted: N/A

Collected on: 08/04/03

Tested: 08/04-08/03

Reported: 08/18/03

Sample Description: Water from MW-18,4.

Project Description: 04-4428.10 JPL

Analysis of Water Samples

Component Analyzed	Method	Unit	PQL	Analysis Result			
				DUPE-3-3-Q03	EB-4-8-4-03	MW-4-1	MW-4-2
				03-04455-1	03-04455-2	03-04455-3	03-04455-4
CHROMIUM (VI)	7196	mg/L	0.01	<0.01	<0.01	<0.01	<0.01
Dilution Factor				1	1	1	1
PERCHLORATE	314.0	µg/L	4	<4	<4	<4	9.0
VOLATILE ORGANIC COMPOUNDS							
Dilution Factor				1	1	1	1
BENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOCHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMODICHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOFORM	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2-BUTANONE	524.2	µg/L	10	<10	<10	<10	<10
N-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
SEC-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TERT-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CARBON TETRACHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLORODIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROFORM	524.2	µg/L	0.5	<0.5	<0.5	<0.5	0.5J
CHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
4-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DIBROMO-3-CHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DIBROMOETHANE (EDB)	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
DIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,4-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
DICHLORODIFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	0.6
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CIS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5

APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result			
				DUPE-3-3-Q03	EB-4-8-4-03	MW-4-1	MW-4-2
				03-04455-1	03-04455-2	03-04455-3	03-04455-4
TRANS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,2-DICHLOROPROPANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,3-DICHLOROPROPANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
2,2-DICHLOROPROPANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,1-DICHLOROPROPENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
CIS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
TRANS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
ETHYLBENZENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
HEXACHLOROBUTADIENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
ISOPROPYLBENZENE (CUMENE)	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
P-ISOPROPYLTOLUENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
METHYLENE CHLORIDE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
METHYL-T-BUTYL ETHER (MTBE)	524.2	µg/L	1	< 1	< 1	< 1	< 1
4-METHYL-2-PENTANONE (MIBK)	524.2	µg/L	10	< 10	< 10	< 10	< 10
NAPHTHALENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
N-PROPYLBENZENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
STYRENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,1,1,2-TETRACHLOROETHANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
TETRACHLOROETHENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	1.3
TOLUENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,2,3-TRICHLOROBENZENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,2,4-TRICHLOROBENZENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,1,1-TRICHLOROETHANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,1,2-TRICHLOROETHANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
TRICHLOROETHENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	0.7
TRICHLOROFLUOROMETHANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,2,3-TRICHLOROPROPANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,2,4-TRIMETHYLBENZENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
1,3,5-TRIMETHYLBENZENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
VINYL CHLORIDE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
O-XYLENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5
M/P-XYLENE	524.2	µg/L	0.5	< 0.5	< 0.5	< 0.5	< 0.5

APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result		
				MW-4-3	MW-18-2	MW-18-3
				03-04455-5	03-04455-6	03-04455-7
CHROMIUM (VI)	7196	mg/L	0.01	<0.01	<0.01	<0.01
Dilution Factor				1	1	1
PERCHLORATE	314.0	µg/L	4	<4	<4	1.3J
VOLATILE ORGANIC COMPOUNDS						
Dilution Factor				1	1	1
BENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOCHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMODICHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOFORM	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
N-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
SEC-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TERT-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2-BUTANONE	524.2	µg/L	10	<10	<10	<10
CARBON TETRACHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLORODIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLOROFORM	524.2	µg/L	0.5	<0.5	<0.5	1.5
CHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
4-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DIBROMO-3-CHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DIBROMOETHANE (EDB)	524.2	µg/L	0.5	<0.5	<0.5	<0.5
DIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,4-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
DICHLORODIFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CIS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TRANS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CIS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TRANS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5

APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result		
				MW-4-3	MW-18-2	MW-18-3
				03-04455-5	03-04455-6	03-04455-7
ETHYLBENZENE	524.2	µg/L	0.5	4.5	<0.5	<0.5
HEXACHLOROBUTADIENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
ISOPROPYLBENZENE (CUMENE)	524.2	µg/L	0.5	<0.5	<0.5	<0.5
P-ISOPROPYLTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
METHYLENE CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
METHYL-T-BUTYL ETHER (MTBE)	524.2	µg/L	1	<1	<1	<1
4-METHYL-2-PENTANONE (MIBK)	524.2	µg/L	10	<10	<10	<10
NAPHTHALENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
N-PROPYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
STYRENE	524.2	µg/L	0.5	0.5J	<0.5	<0.5
1,1,1,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TETRACHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	0.3J
TOLUENE	524.2	µg/L	0.5	0.6	<0.5	<0.5
1,2,3-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,4-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,1-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TRICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	0.4J
TRICHLOROFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,4-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3,5-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
VINYL CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
O-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
M/P-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5

Component Analyzed	Method	Unit	PQL	Analysis Result		
				MW-18-4	MW-18-5	TB-4-8-4-03
				03-04455-8	03-04455-9	03-04455-10
CHROMIUM (VI)	7196	mg/L	0.01	<0.01	-	-
Dilution Factor				1	1	1
PERCHLORATE	314.0	µg/L	4	15.0	<4	-

APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result		
				MW-18-4 03-04455-8	MW-18-5 03-04455-9	TB-4-8-4-03 03-04455-10
VOLATILE ORGANIC COMPOUNDS						
Dilution Factor				1	1	1
BENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOCHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMODICHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOFORM	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2-BUTANONE	524.2	µg/L	10	<10	<10	<10
N-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
SEC-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TERT-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CARBON TETRACHLORIDE	524.2	µg/L	0.5	3.3	<0.5	<0.5
CHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLORODIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLOROFORM	524.2	µg/L	0.5	1.0	<0.5	<0.5
CHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
4-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DIBROMO-3-CHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DIBROMOETHANE (EDB)	524.2	µg/L	0.5	<0.5	<0.5	<0.5
DIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,4-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
DICHLORODIFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CIS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TRANS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CIS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TRANS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
ETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
HEXACHLOROBUTADIENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
ISOPROPYLBENZENE (CUMENE)	524.2	µg/L	0.5	<0.5	<0.5	<0.5

APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result		
				MW-18-4	MW-18-5	TB-4-8-4-03
				03-04455-8	03-04455-9	03-04455-10
P-ISOPROPYLTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
METHYLENE CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	0.6
METHYL-T-BUTYL ETHER (MTBE)	524.2	µg/L	1	<1	<1	<1
4-METHYL-2-PENTANONE (MIBK)	524.2	µg/L	10	<10	<10	<10
NAPHTHALENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
N-PROPYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
STYRENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,1,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TETRACHLOROETHENE	524.2	µg/L	0.5	1.9	<0.5	<0.5
TOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,4-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,1-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TRICHLOROETHENE	524.2	µg/L	0.5	1.1	<0.5	<0.5
TRICHLOROFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,4-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3,5-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
VINYL CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
O-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
M/P-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5


PQL: Practical Quantitation Limit. MDL: Method Detection Limit. CRDL: Contract Required Detection Limit

N.D.: Not Detected or less than the practical quantitation limit. "-": Analysis is not required.

J: Reported between PQL and MDL.

Listed Dilution Factors (DF) are relative to the method default DF. All unlisted DFs are 1.0

Respectfully submitted,

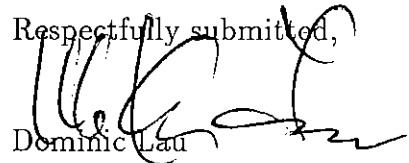

Dominic Lau
Laboratory Director
Applied P & Ch Laboratory

Level C Data Package Deliverables

General Information

Project: 04-4428.10 JPL

APCL Service ID: 03-4455



Applied P & Ch Laboratory

13760 Magnolia Ave. Chino, CA 91710

Telephone (909)590-1828

Fax (909)590-1498

Case Narrative

Project: JPL/MW-18,4./04-4428.10

For GEOFON, Inc.

APCL Service No: 03-4455

1. Sample Identification

The sample identifications are listed in the following table:

GEOFON, Inc. Sample ID	APCL Sample ID
MW-18-5	03-04455-9
MW-18-4	03-04455-8
MW-18-3	03-04455-7
MW-18-2	03-04455-6
EB-4-8-4-03	03-04455-2
TB-4-8-4-03	03-04455-10
MW-4-3	03-04455-5
MW-4-2	03-04455-4
MW-4-1	03-04455-3
DUPE-3-3-Q03	03-04455-1

2. Analytical Methodology

Samples are analyzed by EPA methods

524.2 (Volatile Organic Compounds),

7196 (Chromium (VI)),

314.0 (Perchlorate, low level),

3. Holding Time

All samples were extracted, digested and analyzed within the holding times defined by the appropriate EPA methods of the analyses.

4. Preservation

All samples were preserved and stored according to the appropriate EPA methods.

5. Tele-log


None

6. Anomaly

None

"I certify that these data are technically accurate, complete, and in compliance with the terms and conditions of the contract, for other than the conditions detailed above. Release of the data contained in the hardcopy data package and its electronic data deliverable submitted on diskette had been authorized by the Laboratory Manager or her/his designee, as verified by the following signature."

Respectfully submitted,

A handwritten signature in black ink, appearing to read 'R. Kirakozova', written in a cursive style.

Regina Kirakozova
Associate QA/QC Director
Applied P & Ch Laboratory



INCORPORATED
22632 GOLDEN SPRINGS DR., SUITE 270
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

MW-18

0076

GEOFFON LAB COORDINATOR		LAB COORDINATOR'S PHONE		LAB COORDINATOR'S FAX		LABORATORY SERVICE ID		LABORATORY CONTACT		MAIL REPORT (COMPLAINANT NAME)	
Brad Shjaeger		(909) 396-7662		(909) 396-1455		—		Kenny Chan		GEOFFON, INC.	
PROJECT NAME: JPL Lab/MW-3903		PROJECT LOCATION MW-18 (Ahtedda & Henrich)		PROJECT NUMBER 04-442810		LABORATORY PHONE (909) 590-1828		LABORATORY FAX (909) 590-1498		RECIPIENT NAME Tony Ford	
PROJECT CONTACT J. Robinson		PROJECT PHONE NUMBER (949) 295-7884		PROJECT FAX (909) 396-1455		LABORATORY ADDRESS 13760 Magnolia Ave		LABORATORY CITY, STATE AND ZIP CODE Chico, CA 91110		ADDRESS 22632 Golden Springs Dr. #270	
PROJECT ADDRESS 4800 Cat Lane Dr.		CITY, STATE AND ZIP CODE Pasadena, CA		CLIENT US NAVY SWDIR		LABORATORY CITY, STATE AND ZIP CODE Chico, CA		LABORATORY CITY, STATE AND ZIP CODE 91110		CITY, STATE AND ZIP CODE Diamond Bar, CA 91765	
PROJECT MANAGER Asrar Fabeem		PROJECT MANAGER'S PHONE (909) 396-7662		PROJECT MANAGER'S FAX (909) 396-1455		ANALYSES 524.2 (NOCS) 314.0 (Recl. lead) 317.6 (Hex Chrome) 202.8 (Total Chrome)				Comments	
Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont.	QC Level	T.A.T			
1	MW-18-5	H ₂ O	8/1/03	0801	H ₂	3+1	III	unknown	X	X	
2	MW-18-4			0830	H ₂	3+1			X	X	
3	MW-18-3			0819	H ₂				X	X	
4	MW-18-2			0812	H ₂				X	X	
5	EB-4-8-4-03			0810	H ₂	5			X	X	
6	TB-4-8-4-03				H ₂	2			X	X	
7											
8											
9											
10											

1455

SAMPLES COLLECTED BY: Leah Williamson COURIER AND AIR BILL NUMBER: _____ COOL DR. TEMPERATURE UPON RECEIPT: _____

RELINQUISHED BY: Leah Williamson RECEIVED BY: [Signature] DATE: 8/1/03 TIME: 1000 SAMPLE'S CONDITION UPON RECEIPT: _____

[Signature] [Signature] DATE: 8-1-03 13:30 DATE: 8-4-03 15:35

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager



INCORPORATED
 22632 GOLDEN SPRINGS DR., SUITE 270
 DIAMOND BAR, CA 91765 • (909) 396-7862 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

MW-4

0047

Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont.	QC Level	T.A.T	Analyses			Comments
									H2O	H2O	H2O	
1	MW-4-3	H2O	8/11/03	1010	3+1+1	III	NORMAL	X	X	X		
2	MW-4-2			1031				X	X	X		HS/MSN
3	MW-4-1			1104				X	X	X		
4	Dupe - 3-3-003			1129		IV		X	X	X		
5												
6												
7												
8												
9												
10												

4455

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager

Sample Receiving Checklist

APCL ServiceID: **4455** Client Name/Project: Geolon/JPL

1. Sample Arrival

Date/Time Received 8/4/03 1535 Date/Time Opened 8/4/03 1535 By (name): Kennu Chan
Custody Transfer: Client Golden State UPS US Mail FedEx APCL Empl: Scat B.

2. Chain-of-Custody (CoC)

With Samples? Faxed? Client has Copy? Signed, dated? By: _____
 Project ID? Analyses Clear? Hold Samples? #on Hold _____ # Received 10
 CoC/Docs Zip-Locked under lid? Compos.#: _____ #Samples OK? _____
 Discrepancies? Client notified? Response (attach docs): _____

3. Shipping Container/Cooler

Cooler Used? # of 1 Cooled by: Ice Blue Ice Dry Ice None
Temp °C 4.2
(Cooler temperature measured from temp blank if present, otherwise measured from the cooler).
Cooler Custody Seal? Absent Intact Tampered?

4. Sample Preservation

pH <2 pH >12
If Not, pH = _____ Preserved by: Client APCL Third Party _____

5. Holding-time Requirements

pH 24hr BACT 6/24hr Cr^{VI} 24hr NO₃ 48hr BOD 48hr
 Cl₂ ASAP Turbidity 48hr DO ASAP Fe(II) ASAP
 HT Expired? Client notified?

6. Sample Container Condition

Intact? Broken? Documented? Number: _____
Type: plastic glass Tube: brass/SS Tedlar Bag
 Quantity OK? Leaking? Anomaly?
 Caps tight? Air Bubbles? Anomaly?
Labels: Unique ID? Date/Time Preserved?

7. Turn Around Time

RUSH TAT: _____ Std (7-10 days) Not Marked

8. Sample Matrix

Drinking H₂O Other Liq Soil Wipe Polymer Air Other: _____
 Ground H₂O Sludge Filter Oil/Petro Paint W. Water Extract Unknown

9. Pre-Login Check List Completed & OK?

ALL OK? (if not, attach docs) Client Contact? (Name: _____) Date/Time: _____
Received/Checked by: Kennu Chan Printed: 4 Aug 2003 8:27 a.m.

*HT: Samples must be analyzed for results to reflect total concentrations. Results generated outside required of holding times are considered minimal values and may be used to define waste as hazardous but not as non-hazardous.

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Sample Login: Check List

03-04455 (0470_ 160) (2202777_ 160)

08/04/03

Part 1: General Information

<input type="checkbox"/>	Company Information	Name:	<i>GEOFON, Inc.</i>
		Address:	<i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i>
<input type="checkbox"/>	Project Information	Project Description:	<i>JPL</i>
		Project #:	<i>04-4428.10</i>
<input type="checkbox"/>	Billing Information	P.O. #:	
		Bill Address:	<i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i>
		Lab Project ID:	
		Client Database #:	<i>3</i>
<input type="checkbox"/>	Receiving Information	Who Received Sample?	<i>Kenny Chan</i>
		Receiving Date/Time:	<i>08/04/03 1535</i>
		COC No.	
<input type="checkbox"/>	Shipping Information	Shipping Company	<i>APCL pick up</i>
		Packing Information:	<i>Cooler/Ice Chester</i>
		Cooler Temperature:	<i>4.2 °C</i>
<input type="checkbox"/>	Container Information	Container Provider:	<i>Client</i>
<input type="checkbox"/>	Sampling Information	Sampling Person:	
		Sampling Company:	<i>Client</i>
<input type="checkbox"/>	Turn-Around-Time Option:		<i>Rush 5 working day(s)</i>
<input type="checkbox"/>	QC Option:		<i>NEESA C</i>
<input type="checkbox"/>	Disposal Option:		<i>Not specify</i>

Part 2: Sample Information

Seq. #	Sample ID (on COC)	Sample Sub-ID	APCL Sample ID	Matrix	Cont- tainer	Preser- vative	Vol, ml Am. g	# of Replica	Condition G, L, B	Collected mmddyy	Hold ?	Composite Group	TAT Days	
1	MW-18-5	VOC	03-04455-9- α	W	V	C	40	3	G	080403	N	0	6	<input type="checkbox"/>
	MW-18-5	Perch	03-04455-9- β	W	P		500	1	G	080403	N	0	6	<input type="checkbox"/>
2	MW-18-4	VOC	03-04455-8- α	W	V	C	40	3	G	080403	N	0	6	<input type="checkbox"/>
	MW-18-4	CRVI/Perch	03-04455-8- β	W	P		500	1	G	080403	N	0	6	<input type="checkbox"/>
3	MW-18-3	VOC	03-04455-7- α	W	V	C	40	3	G	080403	N	0	6	<input type="checkbox"/>
	MW-18-3	CRVI/Perch	03-04455-7- β	W	P		500	1	G	080403	N	0	6	<input type="checkbox"/>
4	MW-18-2	VOC	03-04455-6- α	W	V	C	40	3	G	080403	N	0	6	<input type="checkbox"/>
	MW-18-2	CRVI/Perch	03-04455-6- β	W	P		500	1	G	080403	N	0	6	<input type="checkbox"/>
5	EB-4-8-4-03	VOC	03-04455-2- α	W	V	C	40	3	G	080403	N	0	6	<input type="checkbox"/>
	EB-4-8-4-03	CRVI/Perch	03-04455-2- β	W	P		500	1	G	080403	N	0	6	<input type="checkbox"/>
6	TB-4-8-4-03	VOC	03-04455-10	W	V	C	40	2	G	080403	N	0	6	<input type="checkbox"/>
7	MW-4-3	VOC	03-04455-5- α	W	V	C	40	3	G	080403	N	0	6	<input type="checkbox"/>
	MW-4-3	CRVI/Perch	03-04455-5- β	W	P		500	1	G	080403	N	0	6	<input type="checkbox"/>
8	MW-4-2	VOC	03-04455-4- α	W	V	C	40	6	G	080403	N	0	6	<input type="checkbox"/>
	MW-4-2	CRVI/Perch	03-04455-4- β	W	P		500	2	G	080403	N	0	6	<input type="checkbox"/>
9	MW-4-1	VOC	03-04455-3- α	W	V	C	40	3	G	080403	N	0	6	<input type="checkbox"/>
	MW-4-1	CRVI/Perch	03-04455-3- β	W	P		500	1	G	080403	N	0	6	<input type="checkbox"/>
10	DUPE-3-3-Q03	VOC	03-04455-1- α	W	V	C	40	3	G	080403	N	0	6	<input type="checkbox"/>
	DUPE-3-3-Q03	CRVI/Perch	03-04455-1- β	W	P		500	1	G	080403	N	0	6	<input type="checkbox"/>

Part 3: Analysis Information

Test Items:	<input type="checkbox"/> 524.2	Volatile Organic Compounds
	<input type="checkbox"/> 7196A	Chromium (VI)
	<input type="checkbox"/> 314.0/300.0	Perchlorate, low level
	<input type="checkbox"/> 300.0	Chloride Cl^- by IC
	<input type="checkbox"/> 300.0	Sulfate (SO_4^{--}), by IC
	<input type="checkbox"/> 300.0/SM4500NO3	Nitrate (NO_3^-) as N by IC
	<input type="checkbox"/> SM2320B	Carbonate
	<input type="checkbox"/> SM2320B	Bicarbonate
	<input type="checkbox"/> 9040B/150.1	pH
	<input type="checkbox"/> 160.1	Solids, Total Dissolved (TDS)
	<input type="checkbox"/> 200.7/6010B	Sodium, Na, by ICP
	<input type="checkbox"/> 200.7/6010B	Calcium, Ca, by ICP
	<input type="checkbox"/> 200.7/6010B	Potassium, K, by ICP
	<input type="checkbox"/> 200.7/6010B	Magnesium, Mg, by ICP
	<input type="checkbox"/> 200.7/6010B	Iron, Fe, by ICP

Level C Data Package Deliverables

Volatile Organics



Applied P & Ch Laboratory

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/07/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: 03G3595-MB-01	Lab Sample ID: 03G3595-MB-01	Received Date: 08/07/2003
Sample Type: Method Blank	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: G3595K01	Prep. No: -	Anal. Time: 13:17
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYL BENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYL BENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYL BENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLORO BENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLORO BENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLORO BENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TETRACHLOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	4-BROMO-FLUOROBENZENE (BFB)	460-00-4		70-129	96	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	110	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	105	
4	TOLUENE-D8	2037-26-5		73-129	98	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4		50-200	98	
2	1,4-DICHLOROETHANE-D4	3855-82-1		50-200	96	
3	FLUOROBENZENE	462-06-6		50-200	94	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL
 J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)
 E - Exceed calibration range
 B - A positive value was found in the method blank
 D - Diluted

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595K01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 13:17 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:12 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:12 2003
 Miscellaneous :


ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
Internal Standards											
1	Fluorobenzene	7.65	7.63	0.003	96	70	719.160	10.00		0.02	
47	Chlorobenzene-d5	11.55	11.54	0.000	117	82	584.537	10.00		0.00	
62	1,4-Dichlorobenze	13.84	13.84	0.000	152	150	301.712	10.00		0.00	


System Monitoring Compounds (Surrogate)											
27	Di-Br-F-Me (surr)	6.60	6.58	0.002	111	113	376.521	21.01		21.0	105.04%
29	1,2-Di-Cl-Et-d4 (7.11	7.08	0.002	65	102	319.939	22.04		22.0	110.21%
55	toluene-d8	9.91	9.89	0.000	98	100	1433.527	19.46		19.5	97.28%
70	4-Br-1-F-Bz (S3)	12.74	12.74	0.000	174	95	478.479	19.17		19.2	95.87%

Target Compounds											
<<<	I1 : ISTD ID = 1	>>>									
91	Acetonitrile X10	4.08	4.04	0.005	41	40	1.150	0.36		0.4	6
95	Tert butyl alcoho	4.48	4.47	0.002	59	57	0.101	24.27		24.3	100
<<<	I2 : ISTD ID = 47	>>>									
54	MIBK	9.91	9.76	0.013	43	58	4.438	0.52		0.5	1
57	2-hexanone X5	10.77	10.75	0.002	43	58	2.469	0.43		0.4	88

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06





Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595K01.D Sample : f=1
Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
Acq. Time : Aug 7 13:17 2003 RF via : Multiple Level Calibration
Method Update: Thu Jul 24 12:40 2003 Operator: zou
Quant. Time : Aug 08 13:12 2003 Multiplr: 1.000000
Print Time : Fri Aug 08 13:12 2003
Miscellaneous :

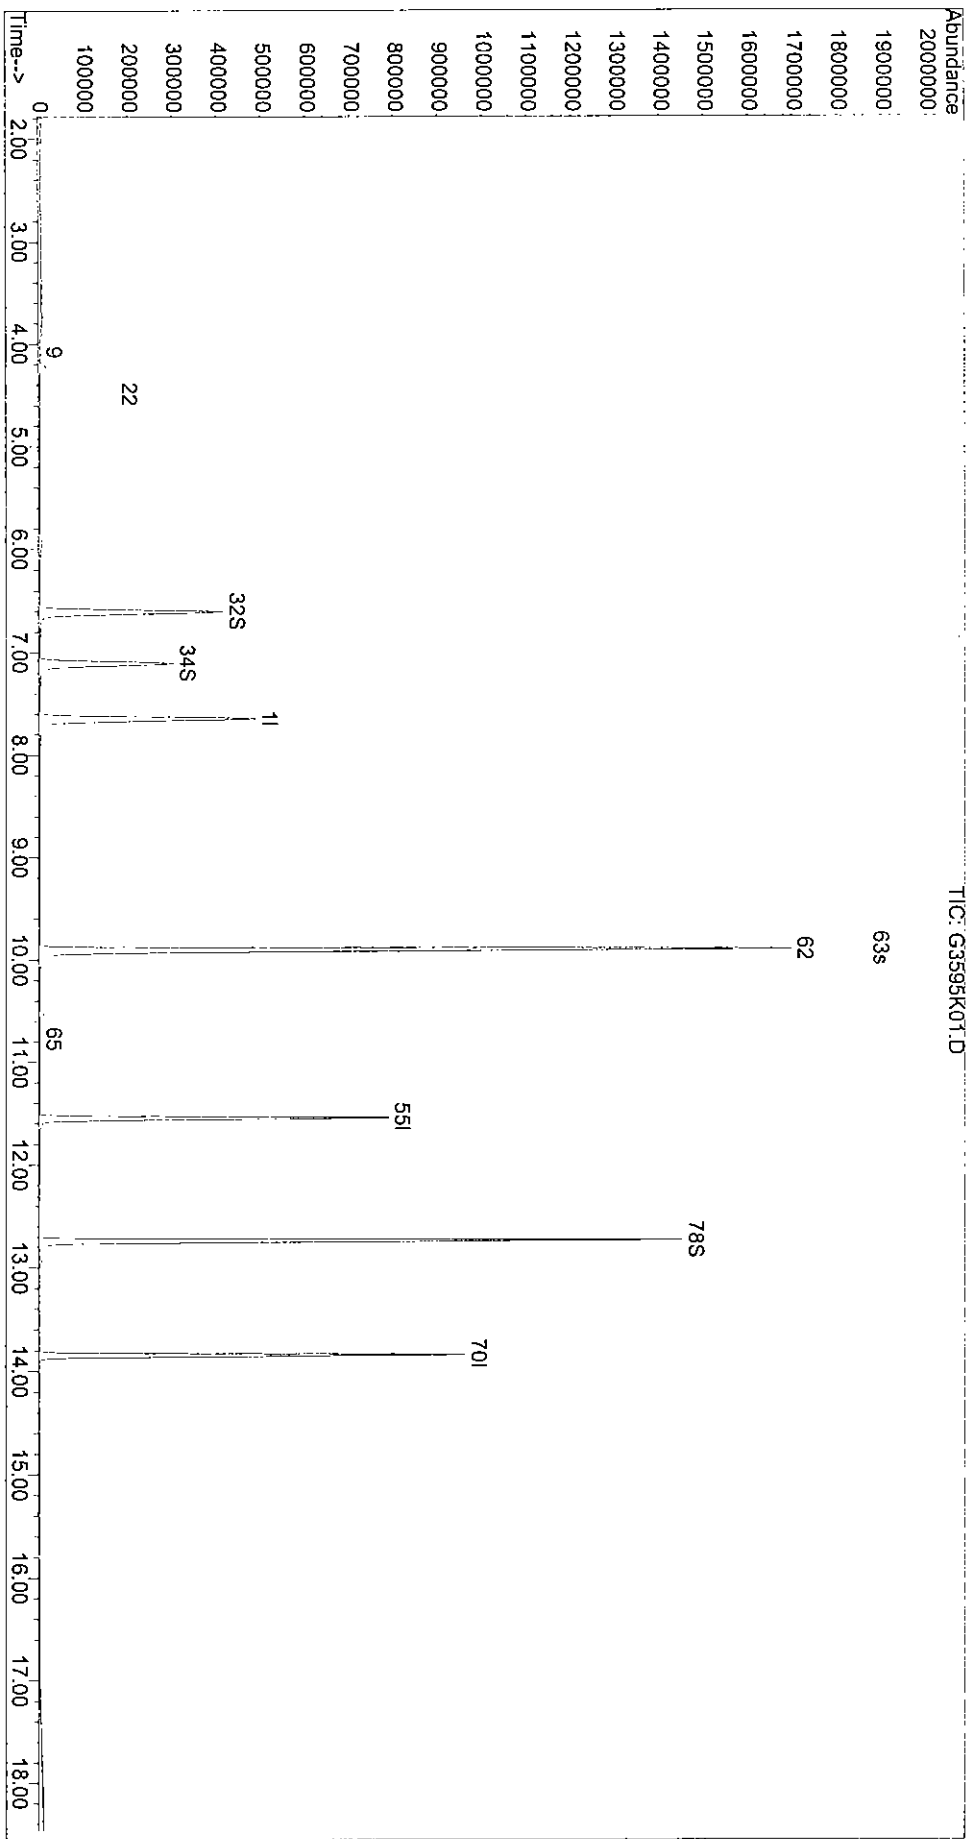

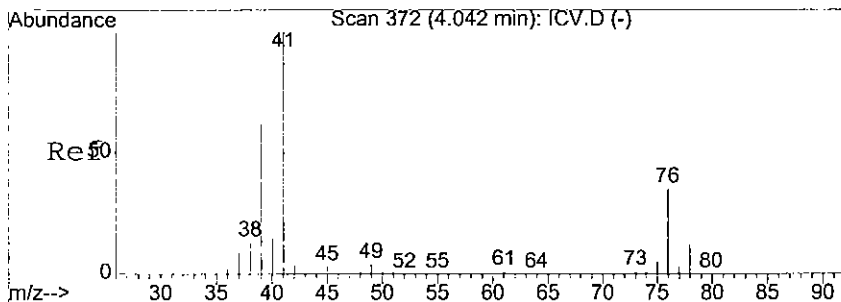




#9
 91 Acetonitrile X10
 Concen: 0.36 ppb
 RT: 4.08 min Scan# 378
 Delta R.T. 0.04 min
 Lab File: G3595K01.D
 Acq: 7 Aug 2003 1:17 pm


Tgt Ion	Resp	Lower	Upper
41	1150		
40	74.7	0.0	33.0#
39	0.0	44.6	84.6#
0	0.0	0.0	0.0

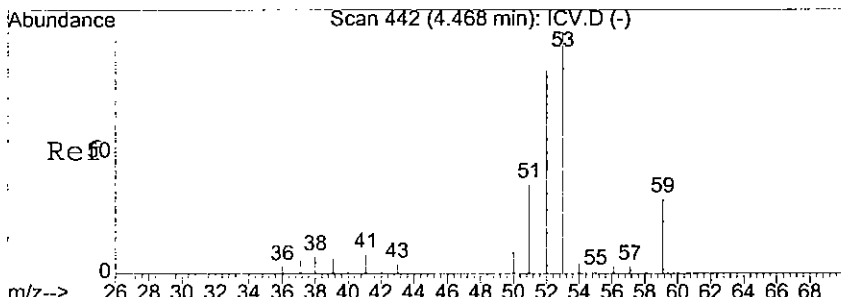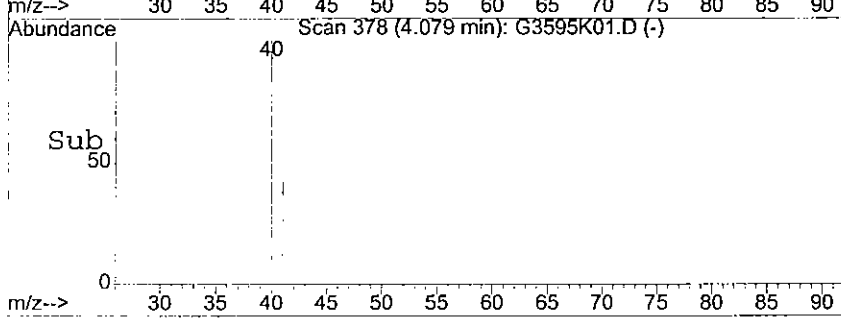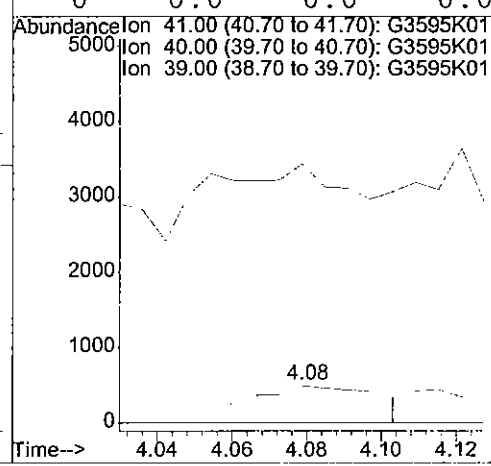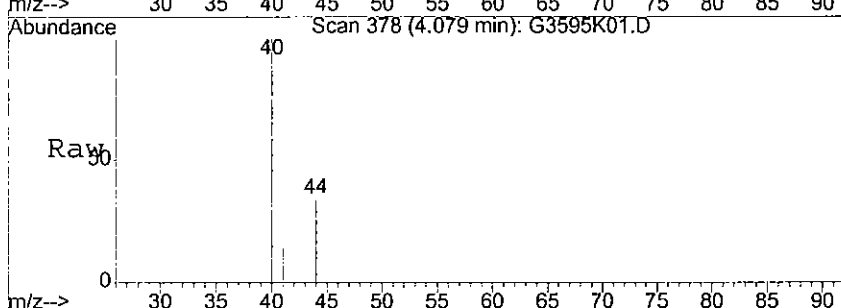

#22
 95 Tert butyl alcoholx10
 Concen: 24.27 ppb
 RT: 4.48 min Scan# 444
 Delta R.T. 0.01 min
 Lab File: G3595K01.D
 Acq: 7 Aug 2003 1:17 pm





Tgt Ion	Resp	Lower	Upper
59	101		
59	100		
57	0.0	0.0	0.0
0	0.0	0.0	0.0
0	0.0	0.0	0.0

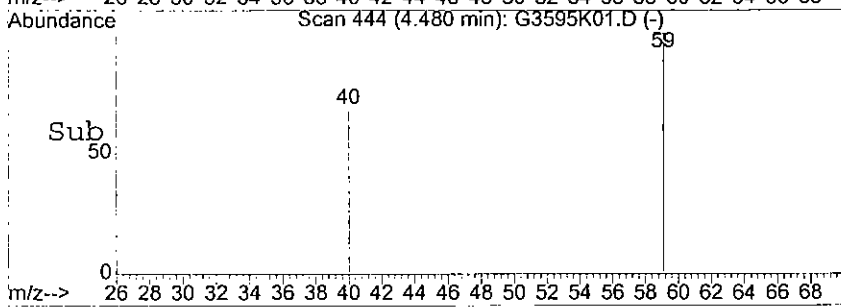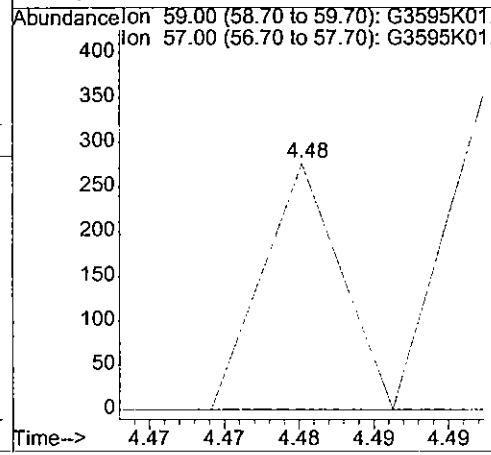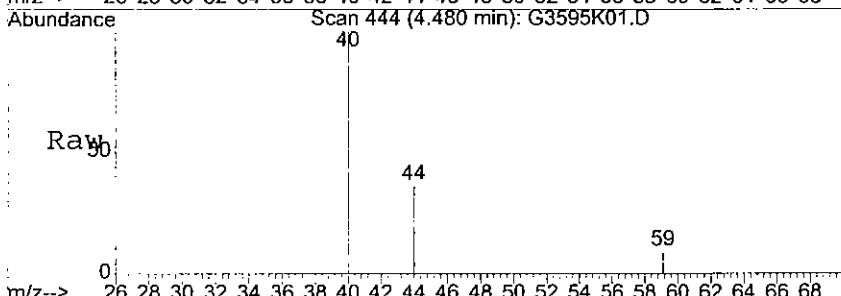

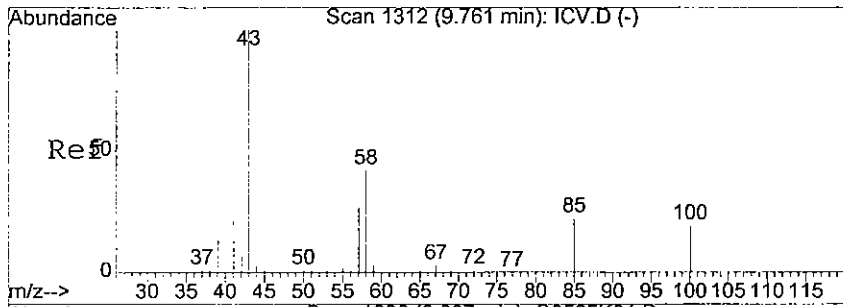




#62
 54 MIBK
 Concen: 0.52 ppb
 RT: 9.91 min Scan# 1336
 Delta R.T. 0.15 min
 Lab File: G3595K01.D
 Acq: 7 Aug 2003 1:17 pm

Tgt Ion	Resp	Lower	Upper
43	4438		
58	222.8	20.1	60.1#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

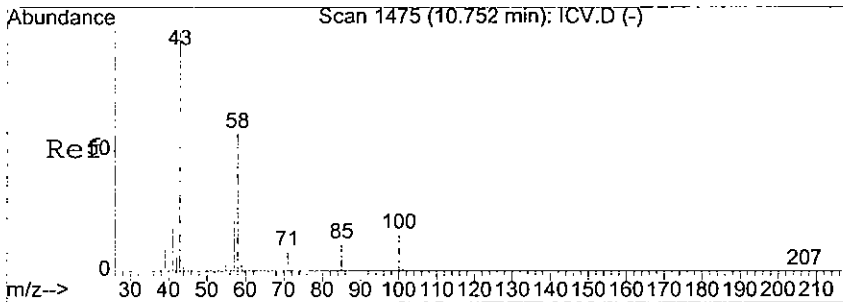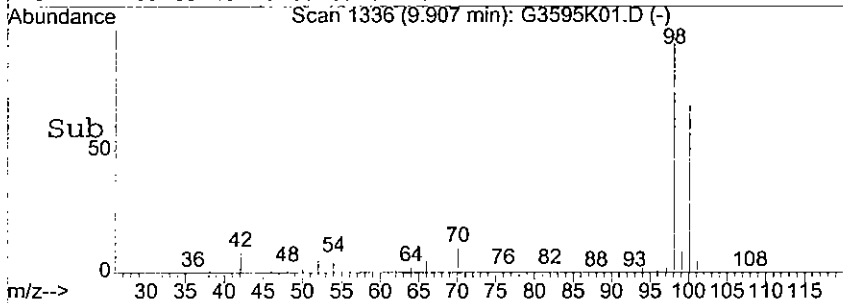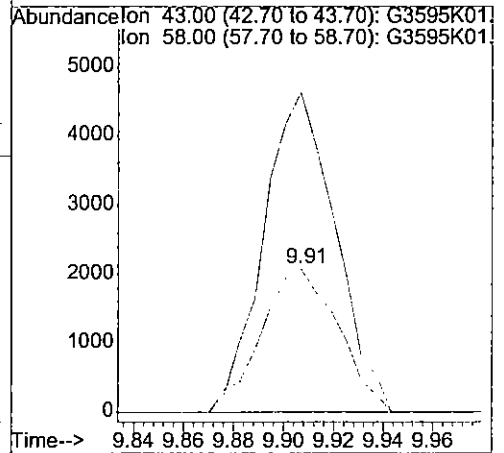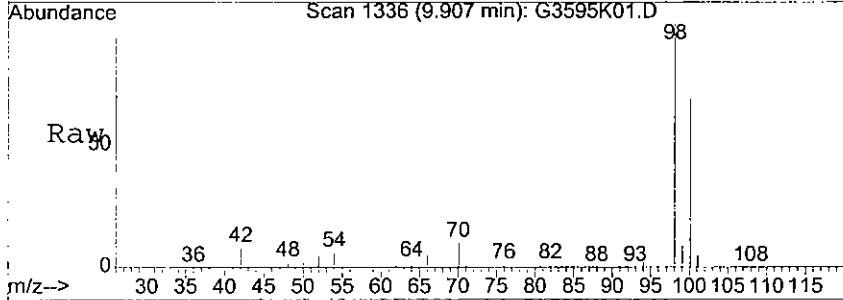

#65
 57 2-hexanone X5
 Concen: 0.43 ppb
 RT: 10.77 min Scan# 1478
 Delta R.T. 0.02 min
 Lab File: G3595K01.D
 Acq: 7 Aug 2003 1:17 pm

Tgt Ion	Resp	Lower	Upper
43	2469		
58	49.4	38.4	78.4
0	0.0	0.0	0.0
0	0.0	0.0	0.0

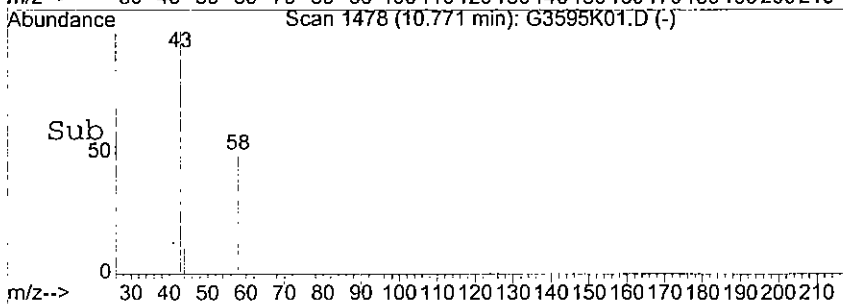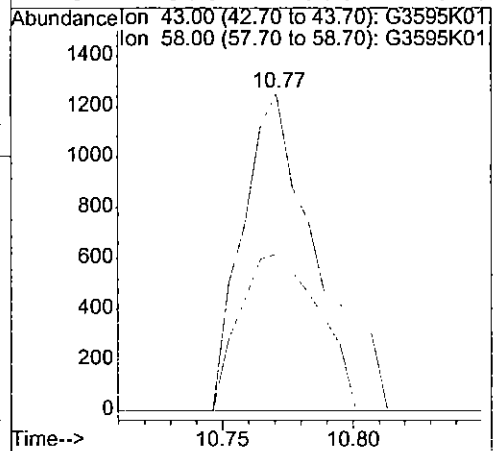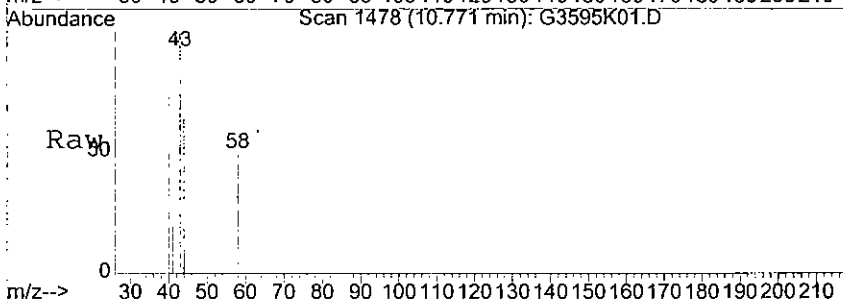

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/08/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: 03G3619-MB-01	Lab Sample ID: 03G3619-MB-01	Received Date: 08/08/2003
Sample Type: Method Blank	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3619	Prep. Date: 08/08/03	Anal. Date: 08/08/03
Data File Name: G3619K01	Prep. No: -	Anal. Time: 13:25
Methanol Vol: -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates

		Control Limit, %	Surro. Rec. %	
1	4-BROMO-FLUOROBENZENE (BFB)	460-00-4	70-129	96
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	110
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	106
4	TOLUENE-D8	2037-26-5	73-129	97
# of out-of-control			0	

Internal Standard

		Control Limit, %	IS Rec. %	
1	CHLOROBENZENE-D5	3114-55-4	50-200	97
2	1,4-DICHLOROETHANE-D4	3855-82-1	50-200	96
3	FLUOROBENZENE	462-06-6	50-200	93
# of out-of-control			0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: DUPE-3-3-Q03	Lab Sample ID: 03-4455-1	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-01	Prep. No: -	Anal. Time: 19:01
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROETHANE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROETHANE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROETHANE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	97	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	114	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	109	
4	TOLUENE-D8	2037-26-5		73-129	99	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4		50-200	94	
2	1,4-DICHLOROENZENE-D4	3855-82-1		50-200	94	
3	FLUOROBENZENE	462-06-6		50-200	91	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Data Filename: C:\MSDCHEM\1\DATA\03G35595\4455-01.D
 Method : C:\MSDCHEM\1\METHODS\E524A002.M
 Acq. Time : Aug 7 19:01 2003
 Method Update: Thu Jul 24 12:40 2003
 Quant. Time : Aug 08 11:35 2003
 Print Time : Fri Aug 08 11:35 2003
 Miscellaneous :

Sample : f=1 dup
 Inst. : GCMS-A
 RF via : Multiple
 Operator: zou
 Multiplr: 1.000000

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
----	----------------	------	-----	------	------	----	---------	--------	-------	---------	------

Internal Standards

1	Fluorobenzene	7.65	7.63	0.003	96	70	694.155	10.00		0.02	
47	Chlorobenzene-d5	11.55	11.54	0.000	117	82	562.650	10.00		0.00	
62	1,4-Dichlorobenze	13.85	13.84	0.000	152	150	294.291	10.00		0.00	

System Monitoring Compounds (Surrogate)


27	Di-Br-F-Me (surr)	6.60	6.58	0.002	111	113	374.639	21.66		21.7	108.28%
29	1,2-Di-Cl-Et-d4 (7.11	7.08	0.002	65	102	317.458	22.66		22.7	113.29%
55	toluene-d8	9.91	9.89	0.000	98	100	1397.177	19.70		19.7	98.52%
70	4-Br-1-F-Bz (S3)	12.74	12.74	0.000	174	95	471.020	19.35		19.4	96.75%


Target Compounds

ID	Compound	RT	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note	
11	ISTD ID = 1	>>>									
95	Tert butyl alcoho	4.41	4.47	-0.007	59	57	0.685	24.90		24.9	100
92	Nitro Methane(x10	5.90	5.80	0.014	61	46	4.572	11.86		11.9	37
54	MIBK	9.91	9.76	0.013	43	58	3.983	0.49		0.5	1


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\4455-01.D
Method : C:\MSDCHEM\1\METHODS\E524A002.M
Acq. Time : Aug 7 19:01 2003
Method Update: Thu Jul 24 12:40 2003
Quant. Time : Aug 08 11:35 2003
Print Time : Fri Aug 08 11:35 2003
Miscellaneous :
Sample : F=1 dup
Inst. : GCMS-A
RF via : Multiple Level Calibration
Operator: zou
Multiplier: 1.000000



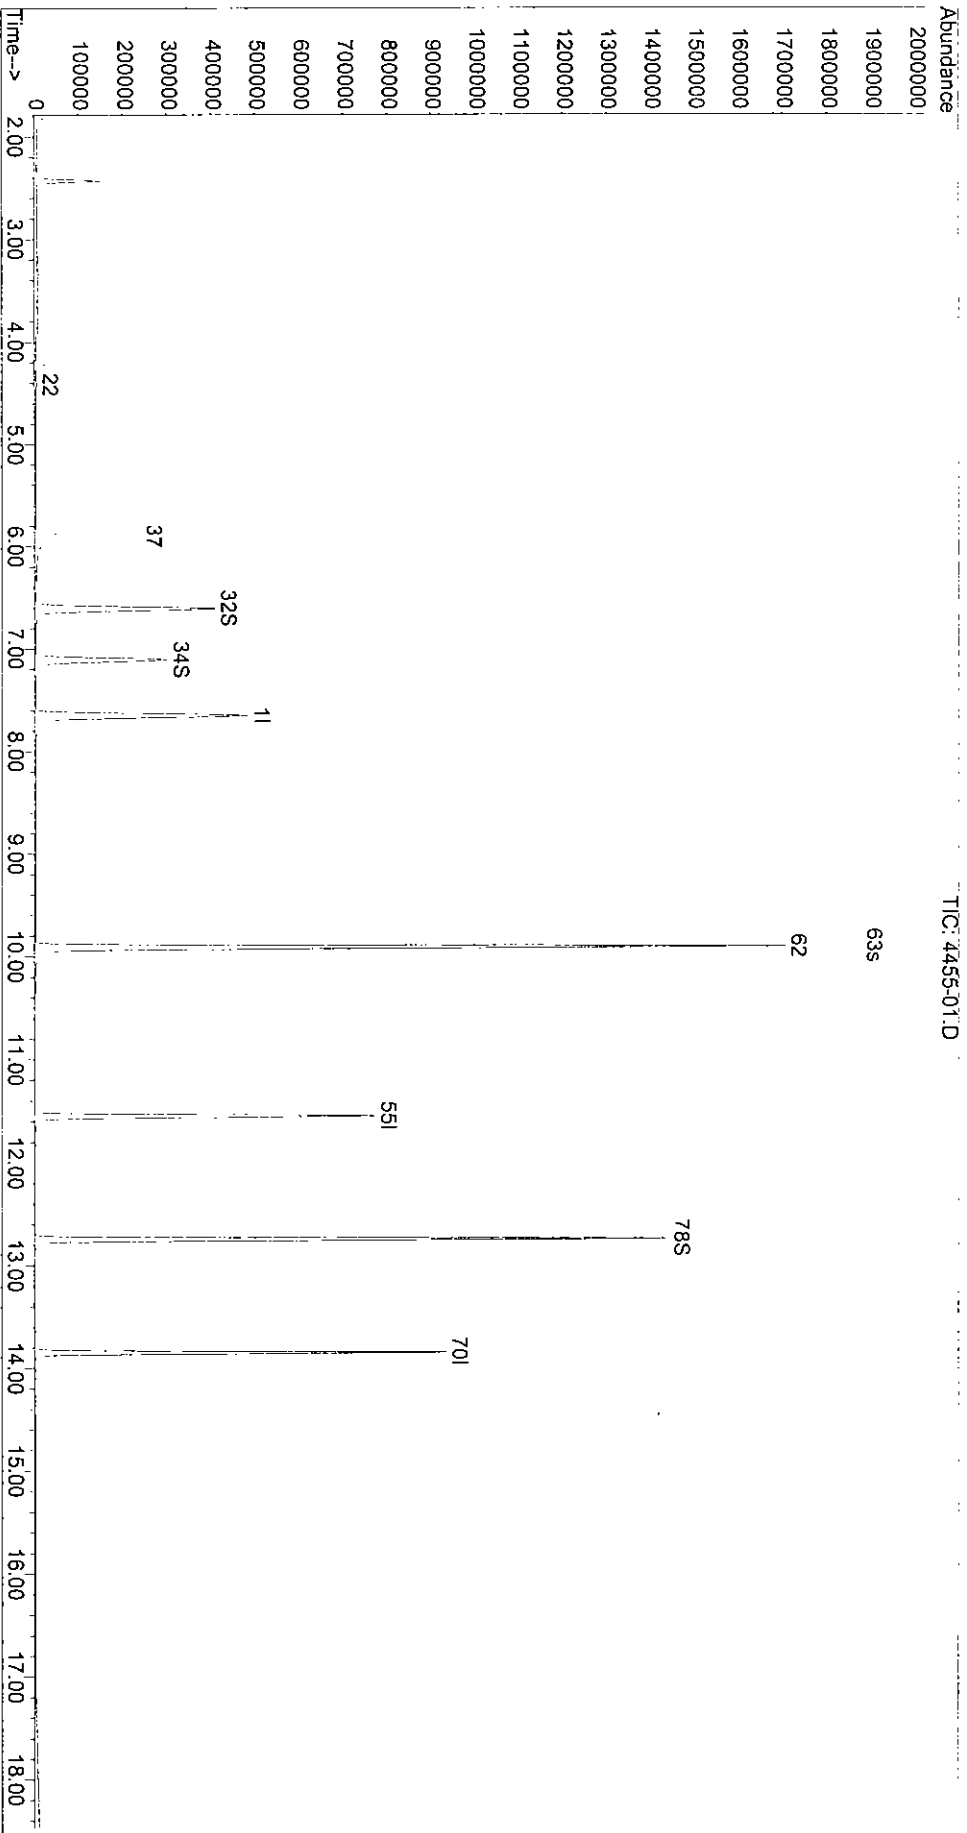


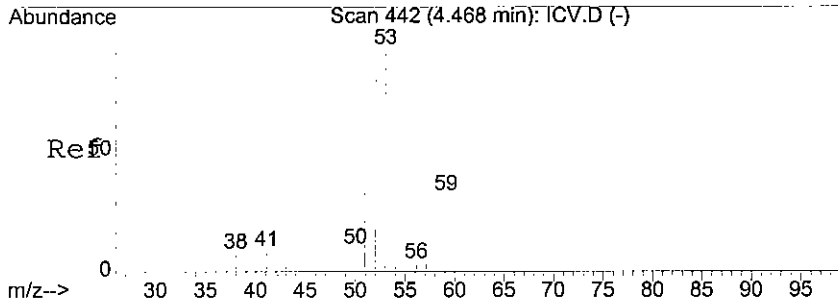


#22
 95 Tert butyl alcoholx10
 Concen: 24.90 ppb
 RT: 4.41 min Scan# 433
 Delta R.T. -0.05 min
 Lab File: 4455-01.D
 Acq: 7 Aug 2003 7:01 pm

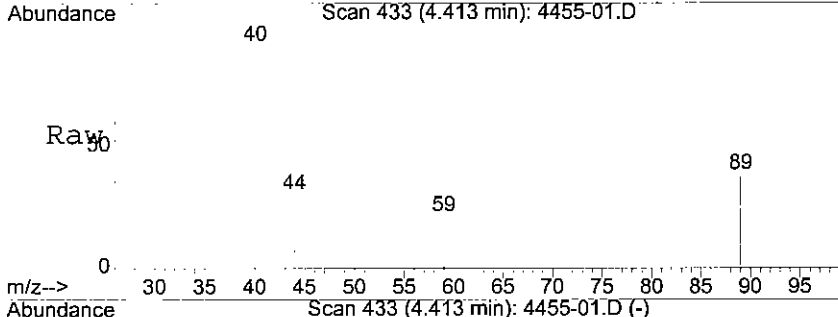



Tgt Ion	Resp	Lower	Upper
59	100		
57	0.0	0.0	0.0
0	0.0	0.0	0.0
0	0.0	0.0	0.0

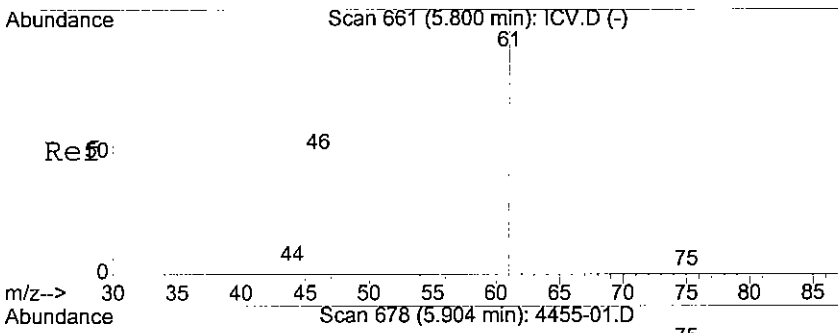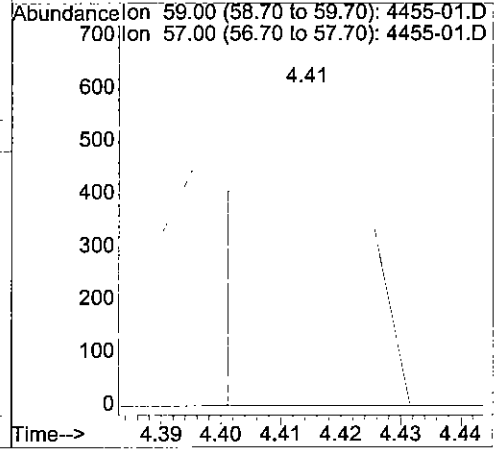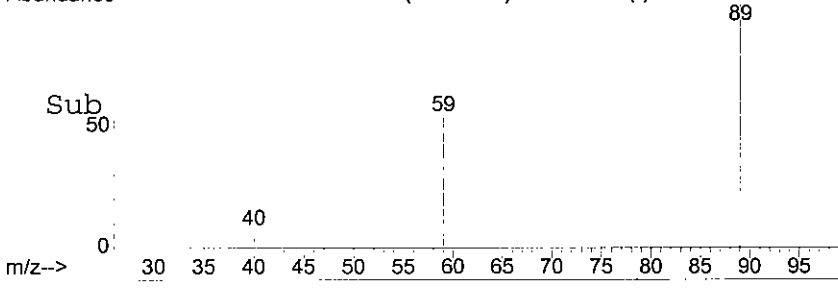


#37
 92 Nitro Methane(x10)
 Concen: 11.86 ppb
 RT: 5.90 min Scan# 678
 Delta R.T. 0.10 min
 Lab File: 4455-01.D
 Acq: 7 Aug 2003 7:01 pm

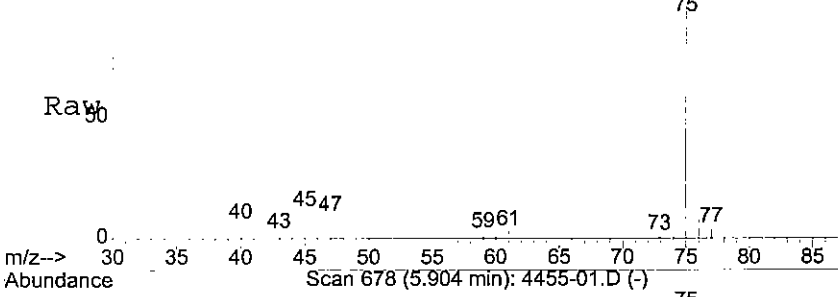


Tgt Ion	Resp	Lower	Upper
61	100		
46	17.3	48.0	88.0#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

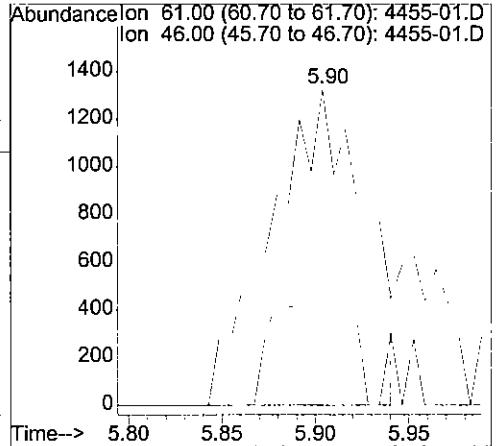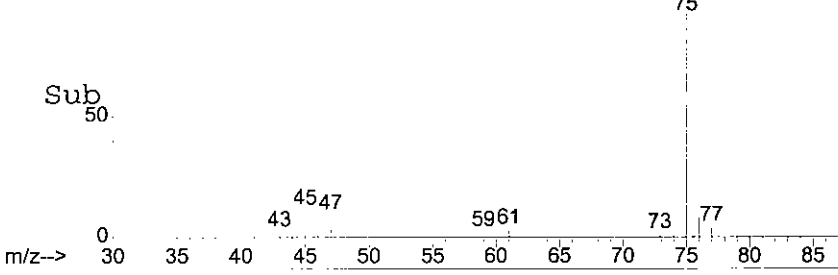

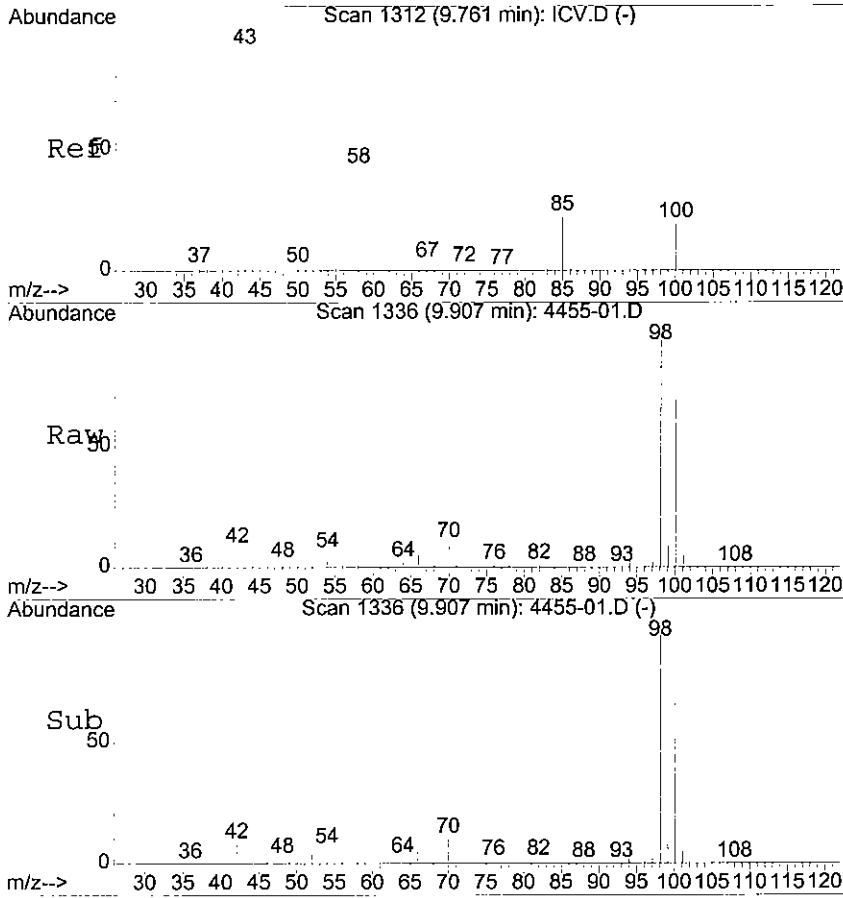

#62
 54 MIBK
 Concen: 0.49 ppb
 RT: 9.91 min Scan# 1336
 Delta R.T. 0.15 min
 Lab File: 4455-01.D
 Acq: 7 Aug 2003 7:01 pm

Tgt Ion	Resp	Lower	Upper
43	3983		
43	100		
58	204.8	20.1	60.1#
0	0.0	0.0	0.0
0	0.0	0.0	0.0

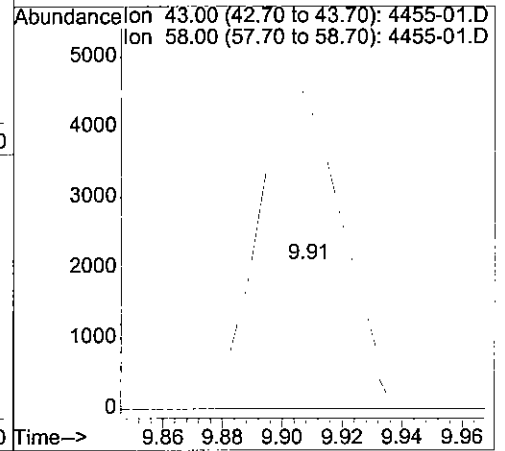

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: EB-4-8-4-03	Lab Sample ID: 03-4455-2	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-02	Prep. No: -	Anal. Time: 15:56
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYL BENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYL BENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYL BENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLORO BENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLORO BENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLORO BENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYL BENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYL BENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	97	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	111	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	107	
4	TOLUENE-D8	2037-26-5		73-129	100	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4		50-200	94	
2	1,4-DICHLOROENZENE-D4	3855-82-1		50-200	94	
3	FLUOROBENZENE	462-06-6		50-200	92	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank
D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: MW-4-1	Lab Sample ID: 03-4455-3	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-03	Prep. No: -	Anal. Time: 19:28
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROETHANE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROETHANE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROETHANE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	94	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	115	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	110	
4	TOLUENE-D8	2037-26-5		73-129	98	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4		50-200	94	
2	1,4-DICHLOROENZENE-D4	3855-82-1		50-200	97	
3	FLUOROENZENE	462-06-6		50-200	91	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank
D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: MW-4-2	Lab Sample ID: 03-4455-4	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3619	Prep. Date: 08/08/03	Anal. Date: 08/08/03
Data File Name: 4455-04	Prep. No: -	Anal. Time: 14:18
Methanol Vol: -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	0.5	J
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROETHANE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROETHANE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROETHANE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	0.6	J
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	1.3	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	0.7	
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	95
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	109
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	107
4	TOLUENE-D8	2037-26-5	73-129	99
# of out-of-control				0

Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4	50-200	95
2	1,4-DICHLOROENZENE-D4	3855-82-1	50-200	93
3	FLUOROBENZENE	462-06-6	50-200	91
# of out-of-control				0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: MW-4-3	Lab Sample ID: 03-4455-5	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-05	Prep. No: -	Anal. Time: 19:54
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROETHANE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROETHANE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROETHANE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	4.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	0.5	J
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	0.6	
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	96	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	112	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	109	
4	TOLUENE-D8	2037-26-5		73-129	98	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4		50-200	95	
2	1,4-DICHLOROENZENE-D4	3855-82-1		50-200	97	
3	FLUOROBENZENE	462-06-6		50-200	90	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank
D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: MW-18-2	Lab Sample ID: 03-4455-6	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-06	Prep. No: -	Anal. Time: 20:20
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROENZENE (4-BROMOFL)	460-00-4		70-129	96	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	112	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	109	
4	TOLUENE-D8	2037-26-5		73-129	99	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4		50-200	94	
2	1,4-DICHLOROENZENE-D4	3855-82-1		50-200	93	
3	FLUROENZENE	462-06-6		50-200	90	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank
D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: MW-18-3	Lab Sample ID: 03-4455-7	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-07	Prep. No: -	Anal. Time: 20:46
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	1.5	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	0.3	J
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	0.4	J
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
Surrogates				Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	97	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	117	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	109	
4	TOLUENE-D8	2037-26-5		73-129	99	
# of out-of-control					0	
Internal Standard				Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4		50-200	93	
2	1,4-DICHLOROENZENE-D4	3855-82-1		50-200	93	
3	FLUOROBENZENE	462-06-6		50-200	89	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank
D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: MW-18-4	Lab Sample ID: 03-4455-8	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-08	Prep. No: -	Anal. Time: 21:12
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	3.3	
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	1.0	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	1.9	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	1.1	
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	97
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	113
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	109
4	TOLUENE-D8	2037-26-5	73-129	100
# of out-of-control			0	

Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4	50-200	92
2	1,4-DICHLOROENZENE-D4	3855-82-1	50-200	93
3	FLUOROBENZENE	462-06-6	50-200	89
# of out-of-control			0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank
D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: MW-18-5	Lab Sample ID: 03-4455-9	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-09	Prep. No: -	Anal. Time: 21:39
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	112TRICHLORO-122TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	96
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	114
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	109
4	TOLUENE-D8	2037-26-5	73-129	100
# of out-of-control			0	

Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4	50-200	92
2	1,4-DICHLOROETHANE-D4	3855-82-1	50-200	93
3	FLUOROBENZENE	462-06-6	50-200	88
# of out-of-control			0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank
D - Diluted

Applied P & Ch Laboratory
Organic Analysis Results for Method 524.2

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/04/2003
Project ID: JPL	Service ID: 34455	Collected by:
Sample ID: TB-4-8-4-03	Lab Sample ID: 03-4455-10	Received Date: 08/04/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3595	Prep. Date: 08/07/03	Anal. Date: 08/07/03
Data File Name: 4455-10	Prep. No: -	Anal. Time: 15:29
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	0.6	
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,2,2,2-TETRAFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	96
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	113
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	108
4	TOLUENE-D8	2037-26-5	73-129	97
#	of out-of-control			0

Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4	50-200	96
2	1,4-DICHLOROENZENE-D4	3855-82-1	50-200	95
3	FLUOROBENZENE	462-06-6	50-200	91
#	of out-of-control			0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

E - Exceed calibration range

B - A positive value was found in the method blank

D - Diluted

FORM-2A

Applied P & Ch Laboratory

Surrogate Recovery Summary for Method 524.2

Client Name: GEOFON, Inc.
 Case No:
 Project ID: JPL

Contract No:
 SAS No:
 Project No: 04-4428.10
 Batch No: 03G3595

Lab Code: APCL
 SDG Number: 034455
 Sample Matrix: Water

#	Client Sample No	Lab Sample ID	S1 % #	S2 % #	S3 % #	S4 % #	TOT OUT
1	03G3595-LCS-01	03G3595-LCS-01	91	95	97	95	0
2	MW-20-4MS	03-4425-6MS	99	95	98	98	0
3	MW-20-4MSD	03-4425-6MSD	96	97	98	96	0
4	03G3595-MB-01	03G3595-MB-01	96	110	105	98	0
5	TB-4-8-4-03	03-4455-10	96	113	108	97	0
6	EB-4-8-4-03	03-4455-2	97	111	107	100	0
7	DUPE-3-3-Q03	03-4455-1	97	114	109	99	0
8	MW-4-1	03-4455-3	94	115	110	98	0
9	MW-4-3	03-4455-5	96	112	109	98	0
10	MW-18-2	03-4455-6	96	112	109	99	0
11	MW-18-3	03-4455-7	97	117	109	99	0
12	MW-18-4	03-4455-8	97	113	109	100	0
13	MW-18-5	03-4455-9	96	114	109	100	0
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							

QC Control Limit

S1 = 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) 70-129
 S2 = 1,2-DICHLOROETHANE-D4 70-129
 S3 = DIBROMOFLUOROMETHANE 70-122
 S4 = TOLUENE-D8 73-129

Column to be used to flag recovery values:

* - Values outside of contract required QC Limits D - Surrogate diluted out I - Matrix Interference

FORM-2A

Applied P & Ch Laboratory

Surrogate Recovery Summary for Method 524.2

Client Name: GEOFON, Inc.
 Case No:
 Project ID: JPL

Contract No:
 SAS No:
 Project No: 04-4428.10
 Batch No: 03G3619

Lab Code: APCL
 Service ID: 034455
 Sample Matrix: Water

#	Client Sample No	Lab Sample ID	S1 % #	S2 % #	S3 % #	S4 % #	TOT OUT
1	03G3619-LCS-01	03G3619-LCS-01	95	98	99	97	0
2	MW-4-2MS	03-4455-4MS	100	90	97	102	0
3	MW-4-2MSD	03-4455-4MSD	96	95	98	96	0
4	03G3619-MB-01	03G3619-MB-01	96	110	106	97	0
5	MW-4-2	03-4455-4	95	109	107	99	0
6							
7							
8							
9							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							

QC Control Limit

S1 = 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) 70-129
 S2 = 1,2-DICHLOROETHANE-D4 70-129
 S3 = DIBROMOFLUOROMETHANE 70-122
 S4 = TOLUENE-D8 73-129

Column to be used to flag recovery values:

* - Values outside of contract required QC Limits D - Surrogate diluted out I - Matrix Interference

FORM-3A

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 524.2

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34455
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03G3595	
LCS Filename: G3595L01	Date Analyzed: 080703	Time Analyzed: 11:06
LCSD Filename: -	Date Analyzed: -	Time Analyzed: -

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
BENZENE	µg/L	20	0	18.6	93	65-120
CHLOROBENZENE	µg/L	20	0	20.1	101	65-134
1,1-DICHLOROETHENE	µg/L	20	0	19.4	97	65-127
TOLUENE	µg/L	20	0	19.1	96	65-134
TRICHLOROETHENE	µg/L	20	0	19.5	98	67-122
# of Out-of-control					0	

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595L01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:06 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:02 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:02 2003
 Miscelaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
Internal Standards											
1	Fluorobenzene	7.65	7.63	0.003	96	70	793.930	10.00		0.02	
47	Chlorobenzene-d5	11.55	11.54	0.000	117	82	618.724	10.00		0.00	
62	1,4-Dichlorobenzene	13.84	13.84	0.000	152	150	326.278	10.00		0.00	

System Monitoring Compounds (Surrogate)											
27	Di-Br-F-Me (surr)	6.60	6.58	0.002	111	113	382.390	19.33	19.3	96.63%	
29	1,2-Di-Cl-Et-d4 (7.11	7.08	0.002	65	102	305.597	19.07	19.1	95.35%	
55	toluene-d8	9.91	9.89	0.000	98	100	1484.506	19.04	19.0	95.19%	
70	4-Br-1-F-Bz (S3)	12.74	12.74	0.000	174	95	493.594	18.29	18.3	91.45%	

Target Compounds
 <<< I1 : ISTD ID = 1 >>> Qvalue

3	di-Cl-di-F-methan	1.89	1.85	0.005	85	87	369.276	18.53	18.5	99	
4	Chloromethane	2.11	2.07	0.006	50	52	304.199	18.07	18.1	98	
2	F114	2.04	2.00	0.006	85	135	207.161	19.88	19.9	60	
5	vinyl chloride	2.23	2.19	0.005	62	64	359.079	18.66	18.7	99	
6	bromomethane	2.61	2.58	0.005	94	96	194.910	21.08	21.1	97	
7	chloroethane	2.73	2.70	0.004	64	66	218.671	19.09	19.1	99	
8	tri-Cl-F-methane	3.03	3.00	0.005	101	103	546.331	19.16	19.2	100	
91	Acetonitrile X10	4.07	4.04	0.004	41	40	631.430	181.28	181.3	90	
9	acrolein X10	3.51	3.48	0.005	56	55	400.955	212.92	212.9	99	
11	acetone X10	3.73	3.69	0.005	43	58	650.146	363.67	363.7	0	
12	ethyl ether X5	3.37	3.34	0.005	59	74	918.938	107.82	107.8	92	
13	11-dichloroethene	3.64	3.60	0.005	61	96	442.380	19.44	19.4	96	
14	Iodomethane	3.82	3.78	0.005	142	127	283.922	14.11	14.1	95	
15	F-113	3.65	3.62	0.005	101	151	337.835	21.61	21.6	89	
16	acrylonitrile X10	4.52	4.49	0.004	53	52	619.965	174.68	174.7	98	
17	carbon disulfide	3.90	3.87	0.004	76	78	1085.914	18.77	18.8	100	
94	Isopropyl Alcohol	4.10	4.01	0.012	45	43	87.466	175.76	175.8	100	
18	methylene chlorid	4.22	4.19	0.004	84	49	373.497	18.49	18.5	99	
19	t-12-di-Cl-ethene	4.58	4.55	0.004	96	61	403.208	18.80	18.8	93	

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

m
08/08/03
08/08/03
08/08/03

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595I01.D
 Method : C:\MSDCHEM\1\METHODS\E524A002.M
 Acq. Time : Aug 7 11:06 2003
 Method Update: Thu Jul 24 12:40 2003
 Quant. Time : Aug 08 13:02 2003
 Print Time : Fri Aug 08 13:03 2003
 Miscleous :

Sample : F=1
 Inst. : GCMS-A
 RF via : Multiple Level Calibration
 Operator: zou
 Multiplr: 1.000000

2
4
8
11

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
20	t-Bu-Me-ether	4.60	4.56	0.005	73	57	679.306	19.03	19.0	95	? \
95	Tert butyl alcohol	4.50	4.47	0.004	59	57	178.587	190.90	190.9	100	m? De
94	allyl chloride	4.07	4.04	0.004	41	76	631.430	20.22	20.2	87	#? 8/8/03
21	11-dichloroethane	5.12	5.09	0.004	63	83	619.320	18.00	18.0	99	
97	propionitrile	6.03	5.99	0.004	54	51	24.827	18.64	18.6	100	#?
22	c-12-di-Cl-ethene	5.92	5.89	0.003	96	61	410.531	18.99	19.0	86	?
23	22-Dichloropropan	5.92	5.89	0.004	77	97	545.825	25.22	25.2	99	?
24	Br-Cl-methane	6.25	6.23	0.003	128	130	192.595	18.37	18.4	100	?
25	chloroform	6.38	6.35	0.003	83	85	651.929	20.10	20.1	100	
26	tetrahydrofuranX5	6.35	6.32	0.003	42	72	233.474	89.54	89.5	95	
98	Diisopropyl ether	5.24	5.22	0.003	45	87	993.491	18.75	18.7	98	
99	ETBE	5.74	5.72	0.003	59	87	816.157	20.15	20.1	98	
30	12-dichloroethane	7.22	7.20	0.003	64	62	114.311	20.42	20.4	93	?
32	vinyl acetate X5	5.20	5.17	0.004	43	86	2461.337	99.36	99.4	99	
92	Nitro Methane (x10	5.83	5.80	0.004	61	46	82.946	188.13	188.1	84	
33	2-butanoneMEK X10	5.95	5.92	0.003	43	72	822.173	246.70	246.7	97	?
93	Ethyl Acetate x2	6.04	6.02	0.002	43	61	321.252	37.07	37.1	89	#?
34	111-trichloroetha	6.65	6.63	0.002	97	99	617.465	19.30	19.3	98	
35	11-Di-Cl-propene	6.91	6.88	0.003	75	110	503.514	20.83	20.8	91	?
36	benzene	7.21	7.19	0.003	78	52	1502.217	18.64	18.6	98	?
37	CCl4	6.91	6.89	0.003	117	119	592.977	20.11	20.1	100	?
100	Isobutyl alcohol	7.17	7.39	-0.030	43	42	67.268	183.84	183.8	92	m? 8/8/03
38	thiophene	7.53	7.51	0.003	84	58	779.187	19.45	19.5	98	
39	12-di-Cl-propane	8.56	8.54	0.002	63	76	333.738	18.51	18.5	95	
40	trichloroethene	8.24	8.23	0.002	130	132	488.601	19.45	19.5	100	
41	dibromomethane	8.73	8.71	0.002	174	172	209.626	18.33	18.3	100	
101	TAME	7.41	7.39	0.002	73	43	714.381	20.34	20.3	97	
42	Br-di-Cl-methane	8.96	8.95	0.002	83	85	467.835	19.81	19.8	99	
43	Me-methacrylate	8.76	8.75	0.002	69	100	165.240	18.01	18.0	92	
44	2-ClEt-Vi-ether10	9.38	9.37	0.000	63	43	237.296	118.57	118.6	96	
45	c-13-di-Cl-propen	9.56	9.55	0.002	75	110	534.067	20.38	20.4	92	
46	t-1,3-dichloropro	10.25	10.24	0.000	75	110	434.279	20.84	20.8	92	

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595L01.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:06 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:02 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:03 2003
 Miscellaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	CO,ppb	C,ppb	Quality	Note
<<<	I2 : ISTD ID = 47 >>>										
48	112-tri-Cl-Et	10.46	10.45	0.000	97	83	266.282	17.83	17.8	96	
49	13-di-Cl-propane	10.65	10.64	0.000	76	78	425.025	18.05	18.0	100	?
50	Et methacrylate	10.37	10.37	0.000	69	99	352.814	18.85	18.8	93	
51	di-Br-Cl-methane	10.91	10.90	0.000	129	127	360.265	19.22	19.2	100	
52	bromoform	12.42	12.41	0.000	173	174	206.684	18.03	18.0	100	
53	1,4-dichlorobutan	12.68	12.67	0.000	55	41	385.529	17.58	17.6	96	
54	MIBK	9.77	9.76	0.000	43	58	167.522	18.59	18.6	93	
56	toluene	9.99	9.98	0.000	91	92	1713.697	19.12	19.1	98	
57	2-hexanone X5	10.76	10.75	0.000	43	58	638.973	104.47	104.5	94	
58	12-dibromoethane	11.03	11.03	0.000	107	109	264.841	17.98	18.0	98	
59	tetra-Cl-ethene	10.64	10.64	0.000	166	168	514.519	19.22	19.2	98	?
60	chlorobenzene	11.57	11.57	0.000	112	77	1169.530	20.06	20.1	92	?
61	1112-tetra-Cl-Et	11.66	11.66	0.000	131	133	418.584	18.35	18.4	99	
<<<	I3 : ISTD ID = 62 >>>										
63	1-chlorohexane	11.56	11.56	0.000	93	55	220.620	20.73	20.7	97	?
64	Et-Bz	11.70	11.69	0.000	91	106	1969.836	19.29	19.3	97	
65	m/p-Xylenes X2	11.82	11.82	0.000	91	106	3028.780	39.24	39.2	98	
66	styrene	12.24	12.23	0.000	104	78	1168.041	19.91	19.9	93	?
67	o-xylene	12.22	12.22	0.000	91	106	1557.202	20.11	20.1	96	?
68	1122-Tetra-Cl-Et	12.87	12.87	0.000	83	85	286.399	16.62	16.6	99	
69	123-tri-Cl-Pr	12.91	12.91	0.000	110	97	89.557	17.36	17.4	98	?
71	isopropylbenzene	12.60	12.59	0.000	105	120	2074.435	20.91	20.9	98	
72	bromobenzene	12.89	12.89	0.000	156	158	504.142	18.92	18.9	99	?
92	t-1,4-dichloro-2-	12.92	12.92	0.000	89	53	53.051	18.16	18.2	89	?
73	n-propylbenzene	13.00	12.99	0.000	120	78	638.876	20.56	20.6	92	
74	2-Cl-Toluene	13.08	13.08	0.000	126	128	542.111	19.74	19.7	98	
75	4-Cl-Toluene	13.19	13.18	0.000	126	128	540.239	19.34	19.3	99	?
76	135-tri-Me-Benzen	13.16	13.16	0.000	105	120	1765.629	20.68	20.7	98	?
77	4-iso-Pr-toluene	13.81	13.81	0.000	119	134	1999.950	20.97	21.0	98	?
78	124-tri-Me-Benzen	13.52	13.51	0.000	105	120	1791.811	20.15	20.1	96	
79	tert-butylbenzene	13.47	13.47	0.000	119	91	1659.210	20.35	20.3	94	


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595L01.D Sample : F=1
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:06 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:02 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:03 2003
 Miscellaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
80	13-DCB	13.79	13.78	0.000	146	148	1042.667	18.62	18.6	100	?
81	sec-butylbenzene	13.68	13.68	0.000	105	134	2413.449	21.03	21.0	97	
82	14-DCB	13.87	13.87	0.000	146	148	1033.426	19.40	19.4	98	
83	Cl-benzyl	13.98	13.98	0.000	126	91	140.844	26.10	26.1	75	#
84	12-DCB	14.21	14.21	0.000	146	148	923.354	18.51	18.5	100	?
85	n-butylbenzene	14.18	14.18	0.000	134	91	564.528	20.19	20.2	87	#?
86	12-dIBr-2-Cl-Pra	14.88	14.88	0.000	157	155	62.189	17.71	17.7	97	
87	124-tri-Cl-Bz	15.58	15.58	0.000	180	182	689.242	21.34	21.3	100	
88	naphthalene	15.79	15.78	0.000	128	129	1114.456	19.02	19.0	99	
89	hx-Cl-butadiene	15.72	15.72	0.000	225	258	388.066	19.85	19.8	97	
90	123-Tri-Cl-Bz	15.98	15.98	0.000	180	182	586.574	20.24	20.2	100	

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595L01.D Sample : f=1
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:06 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: Zou
 Quant. Time : Aug 08 13:02 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:03 2003
 Miscellaneous :

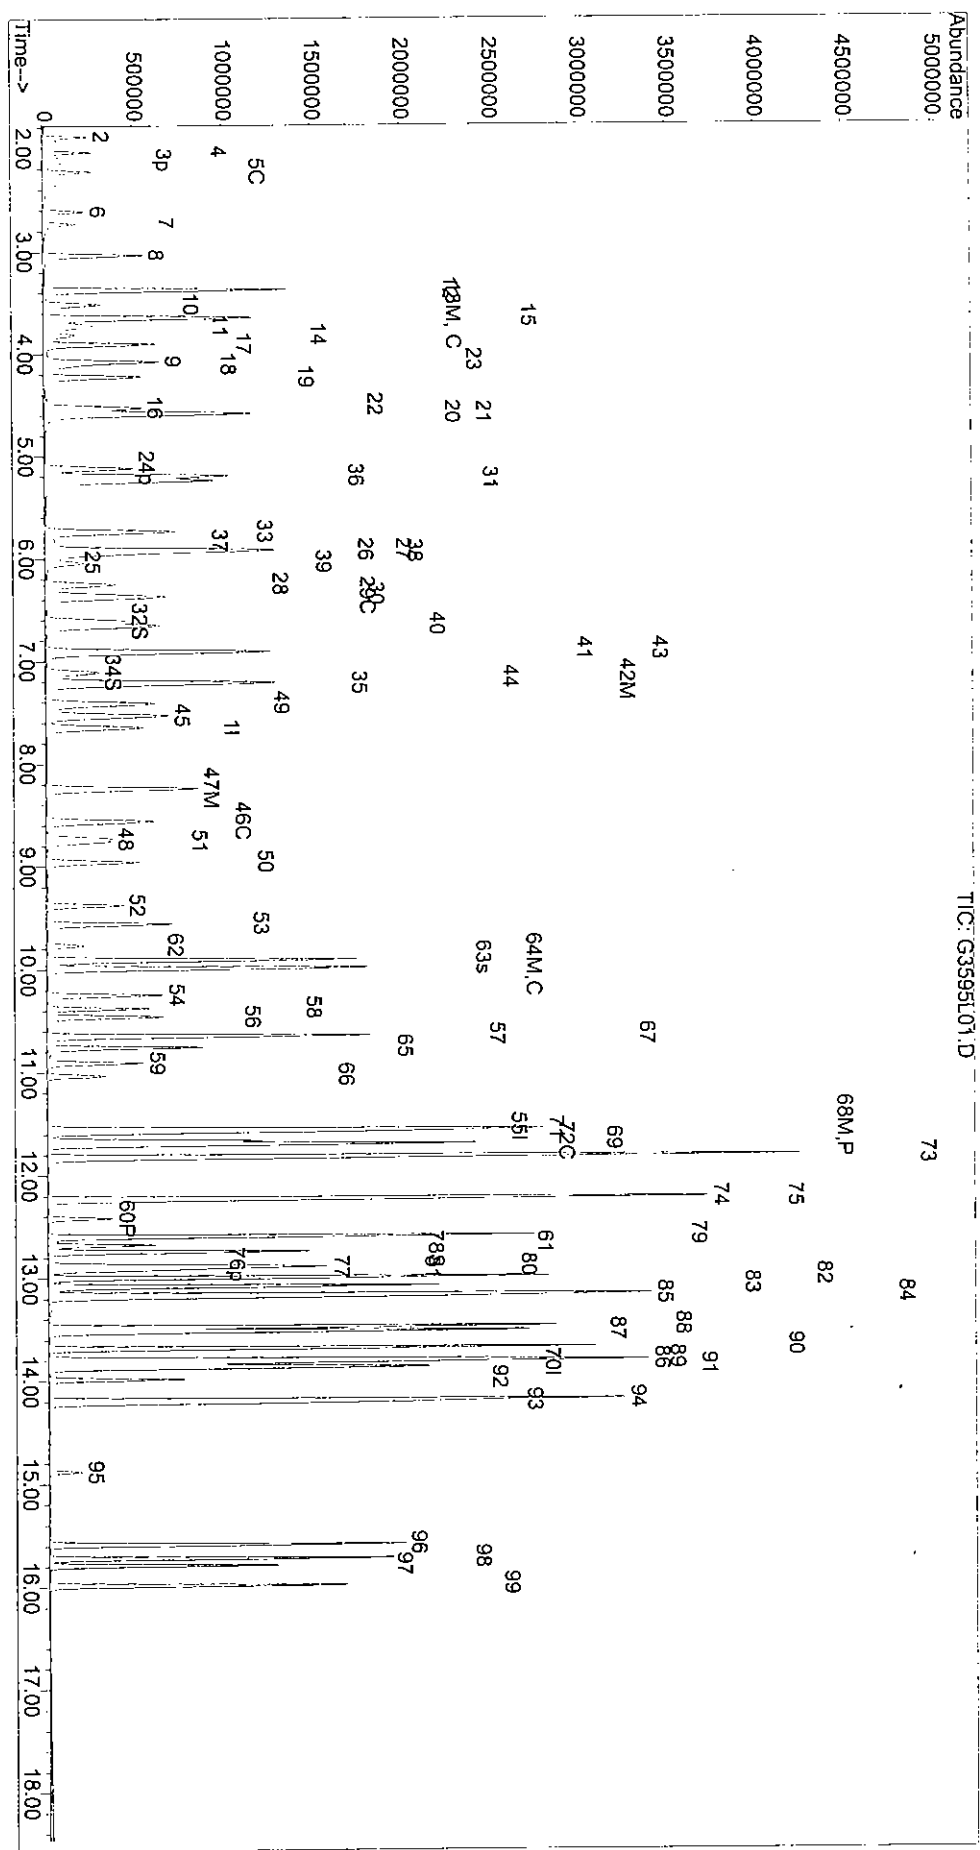

FORM-3A

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 524.2

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34455
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03G3595	
MS Filename: G3595M01	Date Analyzed: 080703	Time Analyzed: 11:32
MSD Filename: G3595N01	Date Analyzed: 080703	Time Analyzed: 11:58
MS Sample No: MW-20-4	Sample Lab ID: 03-4425-6	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
BENZENE	µg/L	20	0	18.8	94	65-121
CHLOROBENZENE	µg/L	20	0	20.5	103	65-134
1,1-DICHLOROETHENE	µg/L	20	0	19.5	98	65-127
TOLUENE	µg/L	20	0	19.4	97	65-134
TRICHLOROETHENE	µg/L	20	0	19.8	99	65-125
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
BENZENE	µg/L	20	18.9	95	1	28	65-121
CHLOROBENZENE	µg/L	20	20.3	102	1	35	65-134
1,1-DICHLOROETHENE	µg/L	20	19.2	96	2	31	65-127
TOLUENE	µg/L	20	19.3	97	0	35	65-134
TRICHLOROETHENE	µg/L	20	19.7	99	0	30	65-125
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595M01.D Sample : F=1 \$4425-06
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:32 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:06 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:06 2003
 Miscellaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
Internal Standards											
1	Fluorobenzene	7.65	7.63	0.003	96	70	813.408	10.00		0.02	
47	Chlorobenzene-d5	11.54	11.54	0.000	117	82	623.673	10.00		0.00	
62	1,4-Dichlorobenze	13.84	13.84	0.000	152	150	310.405	10.00		0.00	

System Monitoring Compounds (Surrogate)											
27	Di-Br-F-Me (surr)	6.60	6.58	0.002	111	113	395.218	19.50		19.5	97.48%
29	1,2-Di-Cl-Et-d4 (7.11	7.08	0.002	65	102	311.505	18.97		19.0	94.87%
55	toluene-d8	9.91	9.89	0.000	98	100	1535.715	19.54		19.5	97.69%
70	4-Br-1-F-Bz (S3)	12.74	12.74	0.000	174	95	510.658	19.89		19.9	99.45%

Target Compounds <<< 11 : ISTD ID = 1 >>> Qvalue

3	di-Cl-di-F-methan	1.89	1.85	0.005	85	87	381.912	18.70		18.7	100	
4	Chloromethane	2.12	2.07	0.006	50	52	299.727	17.35		17.3	100	
2	F114	2.04	2.00	0.006	85	135	217.241	20.35		20.3	59	
5	vinyl chloride	2.23	2.19	0.005	62	64	371.362	18.83		18.8	98	
6	bromomethane	2.61	2.58	0.005	94	96	132.682	14.01		14.0	99	
7	chloroethane	2.73	2.70	0.004	64	66	225.408	19.21		19.2	99	
8	tri-Cl-F-methane	3.03	3.00	0.005	101	103	573.102	19.62		19.6	100	
91	Acetonitrile X10	4.07	4.04	0.004	41	40	647.925	181.56		181.6	90	
9	acrolein X10	3.51	3.48	0.005	56	55	332.192	169.55		169.6	98	
11	acetone X10	3.72	3.69	0.004	43	58	375.738	192.11		192.1	100	
12	ethyl ether X5	3.37	3.34	0.005	59	74	935.434	107.07		107.1	91	
13	11-dichloroethene	3.64	3.60	0.005	61	96	454.299	19.48		19.5	98	
14	Iodomethane	3.82	3.78	0.005	142	127	483.819	23.47		23.5	94	
15	F-113	3.65	3.62	0.005	101	151	348.580	21.77		21.8	89	
16	acrylonitrile X10	4.52	4.49	0.004	53	52	639.436	175.85		175.9	97	
17	carbon disulfide	3.91	3.87	0.005	76	78	1191.042	20.09		20.1	100	
94	Isopropyl Alcohol	4.07	4.01	0.008	45	43	93.168	182.56		182.6	100	
18	methylene chlorid	4.22	4.19	0.005	84	49	394.484	19.10		19.1	100	
19	t-12-di-Cl-ethene	4.58	4.55	0.004	96	61	418.205	19.03		19.0	93	

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

m *08/08/03*
? *08/08/03*
? *08/08/03*
? *08/08/03*

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595M01.D Sample : F=1 \$4425-06
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:32 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:06 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:06 2003
 Miscellaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
20	t-Bu-Me-ether	4.60	4.56	0.005	73	57	708.053	19.36	19.4	96	?
95	Tert butyl alcoho	4.49	4.47	0.003	59	57	200.206	206.61	206.6	100	me 8/16/03
94	allyl chloride	4.07	4.04	0.004	41	76	647.925	20.25	20.2	86	#?
21	11-dichloroethane	5.12	5.09	0.004	63	83	644.781	18.29	18.3	100	
97	propionitrile	6.01	5.99	0.002	54	51	27.591	20.22	20.2	100	#
22	C-12-di-Cl-ethene	5.92	5.89	0.003	96	61	425.635	19.21	19.2	91	?
23	22-Dichloropropan	5.92	5.89	0.003	77	97	587.004	26.52	26.5	98	?
24	Br-Cl-methane	6.25	6.23	0.003	128	130	198.167	18.45	18.4	94	?
25	chloroform	6.37	6.35	0.003	83	85	676.723	20.37	20.4	98	?
26	tetrahydrofuranX5	6.35	6.32	0.003	42	72	241.522	90.41	90.4	96	?
98	Diisopropyl ether	5.24	5.22	0.003	45	87	1021.207	18.81	18.8	99	?
99	ETBE	5.74	5.72	0.003	59	87	843.058	20.31	20.3	98	?
30	12-dichloroethane	7.22	7.20	0.003	64	62	117.841	20.55	20.5	94	?
32	vinyl acetate X5	5.20	5.17	0.004	43	86	2484.946	97.91	97.9	100	
92	Nitro Methane(X10	5.82	5.80	0.003	61	46	95.645	211.74	211.7	82	
33	2-butanoneMEK X10	5.95	5.92	0.003	43	72	650.570	188.62	188.6	97	#
93	Ethyl Acetate x2	6.04	6.02	0.003	43	61	334.180	37.64	37.6	90	
34	111-trichloroetha	6.65	6.63	0.002	97	99	638.865	19.50	19.5	99	?
35	11-Di-Cl-propene	6.91	6.88	0.003	75	110	527.807	21.32	21.3	90	?
36	benzene	7.21	7.19	0.003	78	52	1554.235	18.83	18.8	98	?
37	CCl4	6.91	6.89	0.003	117	119	610.151	20.19	20.2	100	?
100	Isobutyl alcohol	7.17	7.39	-0.030	43	42	67.710	180.79	180.8	96	me 8/16/03
38	thiophene	7.53	7.51	0.002	84	58	807.069	19.66	19.7	98	
39	12-di-Cl-propane	8.56	8.54	0.002	63	76	345.921	18.73	18.7	97	
40	trichloroethene	8.24	8.23	0.002	130	132	509.410	19.80	19.8	99	
41	di bromomethane	8.73	8.71	0.002	174	172	216.661	18.49	18.5	99	
101	TAME	7.41	7.39	0.002	73	43	747.246	20.76	20.8	97	
42	Br-di-Cl-methane	8.96	8.95	0.002	83	85	476.893	19.71	19.7	100	
43	Me-methacrylate	8.76	8.75	0.002	69	100	170.901	18.18	18.2	92	
44	2-ClEt-Vi-ether10	9.57	9.37	0.026	63	43	2.421	16.44	16.4	28	#?
45	C-13-di-Cl-propen	9.56	9.55	0.002	75	110	545.702	20.33	20.3	93	?
46	t-1,3-dichloropro	10.25	10.24	0.000	75	110	446.469	20.91	20.9	93	

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595M01.D Sample : F=1 \$4425-06
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:32 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:06 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:06 2003
 Miscleous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
<<< 12	: ISTD ID = 47 >>>										
48	112-tri-Cl-Et	10.46	10.45	0.000	97	83	268.579	17.84	17.8	96	
49	13-di-Cl-propane	10.65	10.64	0.001	76	78	430.303	18.12	18.1	100	?
50	Et methacrylate	10.38	10.37	0.000	69	99	364.301	19.28	19.3	94	
51	di-Br-Cl-methane	10.91	10.90	0.000	129	127	368.083	19.48	19.5	99	
52	bromoform	12.42	12.41	0.000	173	174	209.966	18.17	18.2	100	
53	1,4-dichlorobutan	12.68	12.67	0.000	55	41	387.686	17.54	17.5	95	
54	MIBK	9.77	9.76	0.000	43	58	170.391	18.76	18.8	92	
56	toluene	9.99	9.98	0.001	91	92	1749.406	19.37	19.4	99	
57	2-hexanone X5	10.76	10.75	0.000	43	58	574.987	93.27	93.3	95	
58	12-dibromoethane	11.03	11.03	0.000	107	109	271.410	18.28	18.3	98	
59	tetra-Cl-ethene	10.65	10.64	0.001	166	168	531.592	19.70	19.7	98	?
60	chlorobenzene	11.58	11.57	0.000	112	77	1202.279	20.46	20.5	91	?
61	1112-tetra-Cl-Et	11.66	11.66	0.000	131	133	425.717	18.52	18.5	98	
<<< 13	: ISTD ID = 62 >>>										
63	1-chlorohexane	11.56	11.56	0.000	93	55	226.646	22.39	22.4	96	?
64	Et-Bz	11.70	11.69	0.000	91	106	2026.841	20.87	20.9	96	
65	m/p-Xylenes X2	11.82	11.82	0.000	91	106	3115.832	42.44	42.4	97	
66	styrene	12.24	12.23	0.000	104	78	1208.705	21.65	21.7	93	?
67	o-xylene	12.22	12.22	0.000	91	106	1605.946	21.80	21.8	97	?
68	1122-Tetra-Cl-Et	12.87	12.87	0.000	83	85	290.212	17.70	17.7	98	
69	123-tri-Cl-Pr	12.91	12.91	0.000	110	97	88.445	18.02	18.0	100	?
71	isopropylbenzene	12.60	12.59	0.000	105	120	2124.998	22.52	22.5	98	
72	bromobenzene	12.89	12.89	0.000	156	158	515.846	20.35	20.4	98	?
92	t-1,4-dichloro-2-	12.92	12.92	0.000	89	53	55.583	19.87	19.9	83	#?
73	n-propylbenzene	13.00	12.99	0.000	120	78	656.002	22.19	22.2	91	
74	2-Cl-Toluene	13.08	13.08	0.000	126	128	555.051	21.25	21.2	98	
75	4-Cl-Toluene	13.19	13.18	0.000	126	128	552.258	20.78	20.8	99	?
76	135-tri-Me-Benzene	13.16	13.16	0.000	105	120	1814.924	22.34	22.3	97	?
77	4-iso-Pr-toluene	13.81	13.81	0.000	119	134	2053.468	22.63	22.6	98	?
78	124-tri-Me-Benzene	13.52	13.51	0.000	105	120	1831.600	21.65	21.6	96	
79	tert-butylbenzene	13.47	13.47	0.000	119	91	1702.030	21.94	21.9	94	


= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595M01.D Sample : F=1 \$4425-06
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:32 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zcu
 Quant. Time : Aug 08 13:06 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:06 2003
 Miscellaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
80	13-DCB	13.79	13.78	0.000	146	148	1067.975	20.04	20.0	100	?
81	sec-butylbenzene	13.68	13.68	0.000	105	134	2471.219	22.63	22.6	97	
82	14-DCB	13.87	13.87	0.000	146	148	1052.303	20.77	20.8	99	
83	Cl-benzyl	13.98	13.98	0.000	126	91	146.524	28.54	28.5	74	#
84	12-DCB	14.21	14.21	0.000	146	148	935.960	19.73	19.7	100	?
85	n-butylbenzene	14.18	14.18	0.000	134	91	578.129	21.71	21.7	84	#?
86	12-diBr-2-Cl-Pra	14.88	14.88	0.000	157	155	65.296	19.54	19.5	100	
87	124-tri-Cl-Bz	15.58	15.58	0.000	180	182	706.807	23.01	23.0	100	
88	naphthalene	15.79	15.78	0.000	128	129	1132.987	20.32	20.3	100	
89	hx-Cl-butadiene	15.72	15.72	0.000	225	258	391.640	21.06	21.1	97	
90	123-Tri-Cl-Bz	15.98	15.98	0.000	180	182	589.534	21.38	21.4	99	

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595M01.D Sample : F=1 \$4425-06
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:32 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:06 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:06 2003
 Miscellaneous :

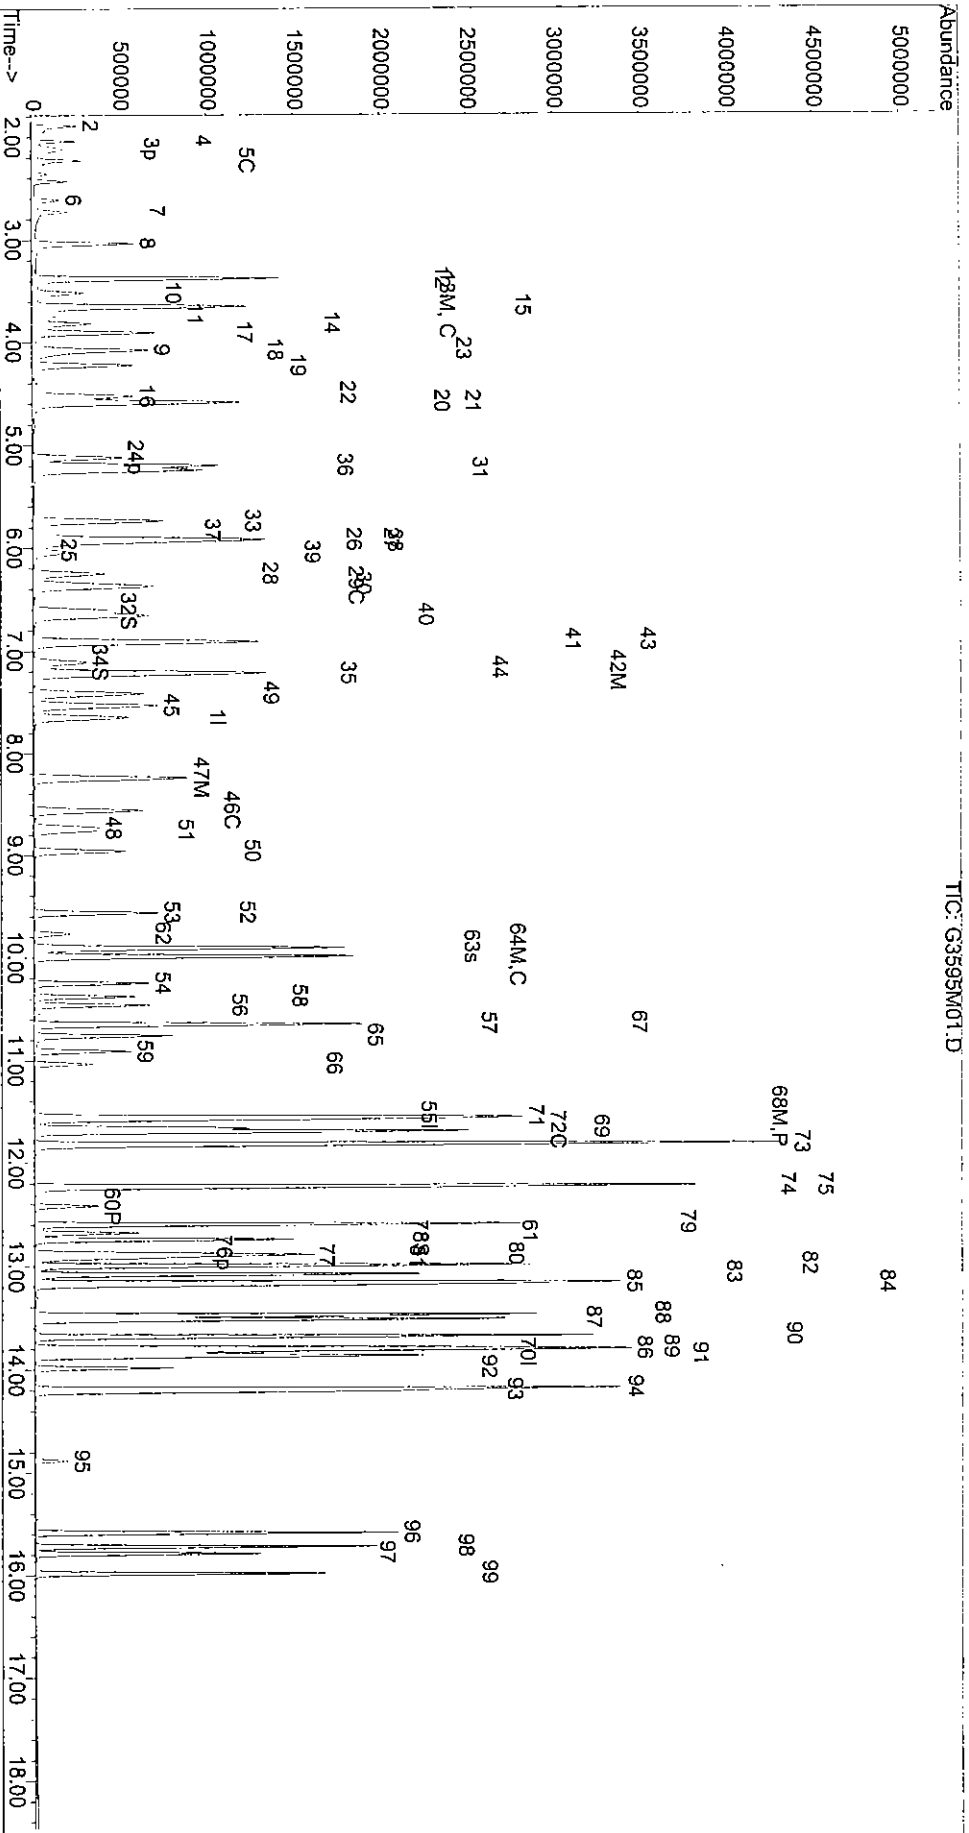

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595N01.D Sample : F#1 \$4425-06
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:58 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:11 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:11 2003
 Miscellaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
20	t-Bu-Me-ether	4.60	4.56	0.005	73	57	753.421	20.43	20.4	95	? #? 8/8/03
95	Tert butyl alcoho	4.51	4.47	0.006	59	57	215.385	218.83	218.8	100	#? 8/8/03
94	allyl chloride	4.07	4.04	0.004	41	76	663.719	20.57	20.6	85	
21	11-dichloroethane	5.12	5.09	0.004	63	83	653.135	18.37	18.4	99	
97	propionitrile	6.03	5.99	0.004	54	51	28.168	20.47	20.5	100	#?
22	c-12-di-cl-ethene	5.92	5.89	0.003	96	61	429.744	19.24	19.2	94	?
23	22-Dichloropropan	5.92	5.89	0.004	77	97	576.534	25.81	25.8	96	?
24	Br-Cl-methane	6.25	6.23	0.003	128	130	204.795	18.91	18.9	96	?
25	chloroform	6.37	6.35	0.002	83	85	686.182	20.49	20.5	99	?
26	tetrahydrofuranX5	6.35	6.32	0.003	42	72	262.264	97.37	97.4	98	?
98	Disopropyl ether	5.24	5.22	0.003	45	87	1041.256	19.02	19.0	99	?
99	ETBE	5.74	5.72	0.003	59	87	889.082	21.25	21.2	97	?
30	12-dichloroethane	7.22	7.20	0.003	64	62	119.758	20.71	20.7	98	?
32	vinyl acetate X5	5.20	5.17	0.004	43	86	2594.186	101.38	101.4	99	?
92	Nitro Methane(X10	5.82	5.80	0.003	61	46	98.539	216.35	216.4	78	?
33	2-butanoneMEK X10	5.95	5.92	0.003	43	72	700.851	202.10	202.1	98	?
93	Ethyl Acetate x2	6.04	6.02	0.003	43	61	368.573	41.18	41.2	93	#?
34	111-trichloroetha	6.65	6.63	0.002	97	99	638.649	19.33	19.3	99	?
35	11-Di-Cl-propene	6.90	6.88	0.002	75	110	530.655	21.25	21.3	91	?
36	benzene	7.21	7.19	0.003	78	52	1572.880	18.89	18.9	99	?
37	CCl4	6.91	6.89	0.003	117	119	611.152	20.06	20.1	98	?
100	Isobutyl alcohol	7.18	7.39	-0.029	43	42	73.697	194.37	194.4	96	?
38	thiophene	7.53	7.51	0.002	84	58	821.203	19.84	19.8	99	?
39	12-di-Cl-propane	8.56	8.54	0.002	63	76	350.588	18.82	18.8	96	?
40	trichloroethene	8.24	8.23	0.002	130	132	511.760	19.72	19.7	100	?
41	diBromomethane	8.73	8.71	0.002	174	172	227.281	19.24	19.2	98	?
101	TAME	7.41	7.39	0.002	73	43	787.712	21.71	21.7	97	?
42	Br-di-Cl-methane	8.96	8.95	0.002	83	85	488.256	20.02	20.0	99	?
43	Me-methacrylate	8.76	8.75	0.002	69	100	184.494	19.39	19.4	92	?
44	2-ClEt-Vi-ether10	9.57	9.37	0.026	63	43	2.385	16.41	16.4	28	#?
45	c-13-di-Cl-propen	9.56	9.55	0.002	75	110	559.203	20.66	20.7	93	?
46	t-1,3-dichloropro	10.25	10.24	0.000	75	110	464.859	21.60	21.6	92	?

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595N01.D Sample : F=1 \$4425-06
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:58 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:11 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:11 2003
 Miscellaneous :

ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
<<< 12	: ISTD ID = 47 >>>										
48	112-tri-Cl-Et	10.46	10.45	0.000	97	83	285.102	18.50	18.5	94	
49	13-di-Cl-propane	10.65	10.64	0.000	76	78	452.321	18.61	18.6	99	?
50	Et methacrylate	10.38	10.37	0.000	69	99	391.052	20.17	20.2	94	
51	di-Br-Cl-methane	10.91	10.90	0.000	129	127	380.853	19.68	19.7	99	
52	bromoform	12.42	12.41	0.000	173	174	221.249	18.71	18.7	99	
53	1,4-dichlorobutan	12.68	12.67	0.000	55	41	412.254	18.22	18.2	95	
54	MIBK	9.77	9.76	0.000	43	58	189.992	20.43	20.4	94	
56	toluene	9.99	9.98	0.000	91	92	1779.849	19.25	19.2	98	
57	2-hexanone X5	10.76	10.75	0.000	43	58	634.630	100.55	100.6	94	
58	12-dibromoethane	11.03	11.03	0.000	107	109	287.036	18.88	18.9	98	
59	tetra-Cl-ethene	10.64	10.64	0.000	166	168	533.355	19.30	19.3	98	
60	chlorobenzene	11.57	11.57	0.000	112	77	1218.144	20.25	20.2	92	?
61	1112-tetra-Cl-Et	11.66	11.66	0.000	131	133	440.606	18.72	18.7	99	
<<< 13	: ISTD ID = 62 >>>										
63	1-chlorohexane	11.56	11.56	0.000	93	55	231.400	21.81	21.8	95	?
64	Et-Bz	11.70	11.69	0.000	91	106	2045.202	20.09	20.1	96	
65	m/p-Xylenes X2	11.82	11.82	0.000	91	106	3149.058	40.91	40.9	95	
66	styrene	12.24	12.23	0.000	104	78	1231.281	21.04	21.0	92	?
67	o-xylene	12.22	12.22	0.000	91	106	1631.513	21.13	21.1	96	?
68	1122-Tetra-Cl-Et	12.87	12.87	0.000	83	85	308.178	17.93	17.9	99	
69	123-tri-Cl-Pr	12.91	12.91	0.000	110	97	96.138	18.68	18.7	98	?
71	isopropylbenzene	12.60	12.59	0.000	105	120	2159.861	21.83	21.8	97	
72	bromobenzene	12.89	12.89	0.000	156	158	527.990	19.87	19.9	99	?
92	t-1,4-dichloro-2-	12.92	12.92	0.000	89	53	59.319	20.21	20.2	82	#?
73	n-propylbenzene	13.00	12.99	0.000	120	78	660.240	21.31	21.3	92	
74	2-Cl-Toluene	13.08	13.08	0.000	126	128	560.793	20.48	20.5	98	
75	4-Cl-Toluene	13.19	13.18	0.000	126	128	557.665	20.02	20.0	98	?
76	135-tri-Me-Benzen	13.16	13.16	0.000	105	120	1818.466	21.35	21.4	96	?
77	4-iso-Pr-toluene	13.81	13.81	0.000	119	134	2090.132	21.98	22.0	98	?
78	124-tri-Me-Benzen	13.51	13.51	0.000	105	120	1856.326	20.93	20.9	97	
79	tert-butylbenzene	13.47	13.47	0.000	119	91	1722.730	21.18	21.2	95	

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Quantitation Report: **Applied P &ch Lab** EPA 524.2


Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595N01.D Sample : F=1 \$4425-06
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 11:58 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 13:11 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:11 2003
 Miscelaneous :

ID	Component Name	R.T.	RT0	DRRT	QIon	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
80	13-DCB	13.79	13.78	0.000	146	148	1088.428	19.49	19.5	100	?
81	sec-butylbenzene	13.68	13.68	0.000	105	134	2493.990	21.79	21.8	96	
82	14-DCB	13.87	13.87	0.000	146	148	1076.495	20.27	20.3	97	
83	Cl-benzyl	13.98	13.98	0.000	126	91	153.423	28.50	28.5	73	#
84	12-DCB	14.21	14.21	0.000	146	148	957.896	19.26	19.3	99	?
85	n-butylbenzene	14.18	14.18	0.000	134	91	582.965	20.89	20.9	87	#?
86	12-diBr-2-Cl-Pra	14.88	14.88	0.000	157	155	70.819	20.22	20.2	99	
87	124-tri-Cl-Bz	15.58	15.58	0.000	180	182	728.613	22.62	22.6	100	
88	naphthalene	15.79	15.78	0.000	128	129	1213.693	20.77	20.8	99	
89	hx-Cl-butadiene	15.72	15.72	0.000	225	258	399.169	20.47	20.5	98	
90	123-Tri-Cl-Bz	15.98	15.98	0.000	180	182	623.335	21.57	21.6	98	

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\G3595N01.D
 Method : C:\MSDCHEM\1\METHODS\E524A002.M
 Acq. Time : Aug 7 11:58 2003
 Method Update: Thu Jul 24 12:40 2003
 Quant. Time : Aug 08 13:11 2003
 Print Time : Fri Aug 08 13:11 2003
 Miscellaneous :

Sample : F=1 \$4425-06
 Inst. : GCMS-A
 RF via : Multiple Level Calibration
 Operator: zou
 Multiplr: 1.000000

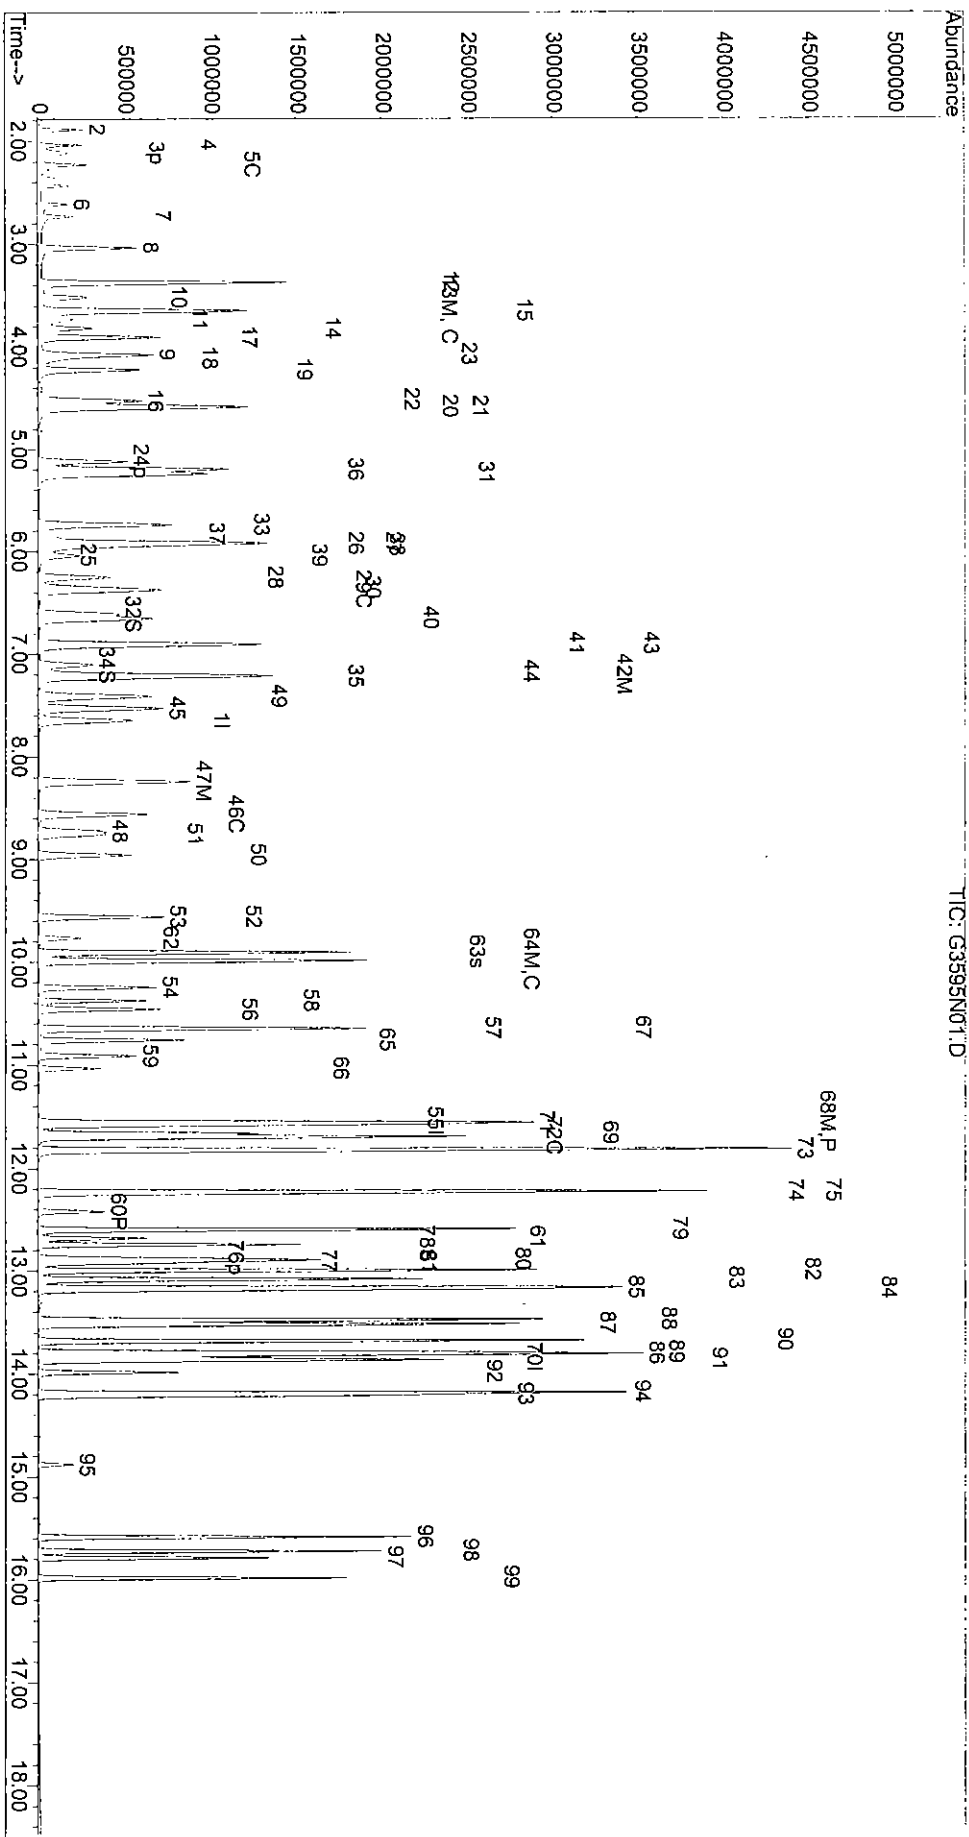

Data Filename: C:\MSDCHEM\1\DATA\03G3595\4425-06.D Sample : F=1 ms
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 16:22 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 11:35 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:12 2003
 Miscellaneous :


ID	Component Name	R.T.	RT0	DRRT	Qion	Q1	RF/1000	C0,ppb	C,ppb	Quality	Note
Internal Standards											
1	Fluorobenzene	7.65	7.63	0.003	96	70	704.743	10.00		0.02	
47	Chlorobenzene-d5	11.54	11.54	0.000	117	82	574.822	10.00		0.00	
62	1,4-Dichlorobenze	13.84	13.84	0.000	152	150	298.518	10.00		0.00	

System Monitoring Compounds (Surrogate)											
27	Di-Br-F-Me (surr)	6.60	6.58	0.002	111	113	377.276	21.48		21.5	107.41%
29	1,2-Di-Cl-Et-d4 (7.11	7.08	0.002	65	102	315.939	22.21		22.2	111.05%
55	toluene-d8	9.91	9.89	0.000	98	100	1394.529	19.25		19.2	96.25%
70	4-Br-1-F-Bz (S3)	12.74	12.74	0.000	174	95	476.109	19.28		19.3	96.41%

Target Compounds											
<<<	I1 : ISTD ID = 1	>>>									
5	vinyl chloride	2.43	2.19	0.031	62	64	6.684	0.39		0.4	95
95	Tert butyl alcoho	4.41	4.47	-0.007	59	57	1.525	25.77		25.8	100
92	Nitro Methane(x10	5.89	5.80	0.012	61	46	6.502	16.61		16.6	35
<<<	I2 : ISTD ID = 47	>>>									
54	MIBK	9.91	9.76	0.013	43	58	3.977	0.48		0.5	1

= qualifier out of range, m = manual integration, ? = RT coelution, * = DRRT > 0.06

Data Filename: C:\MSDCHEM\1\DATA\03G3595\4425-06.D Sample : F=1 ms
 Method : C:\MSDCHEM\1\METHODS\E524A002.M Inst. : GCMS-A
 Acq. Time : Aug 7 16:22 2003 RF via : Multiple Level Calibration
 Method Update: Thu Jul 24 12:40 2003 Operator: zou
 Quant. Time : Aug 08 11:35 2003 Multiplr: 1.000000
 Print Time : Fri Aug 08 13:12 2003
 Miscellaneous :

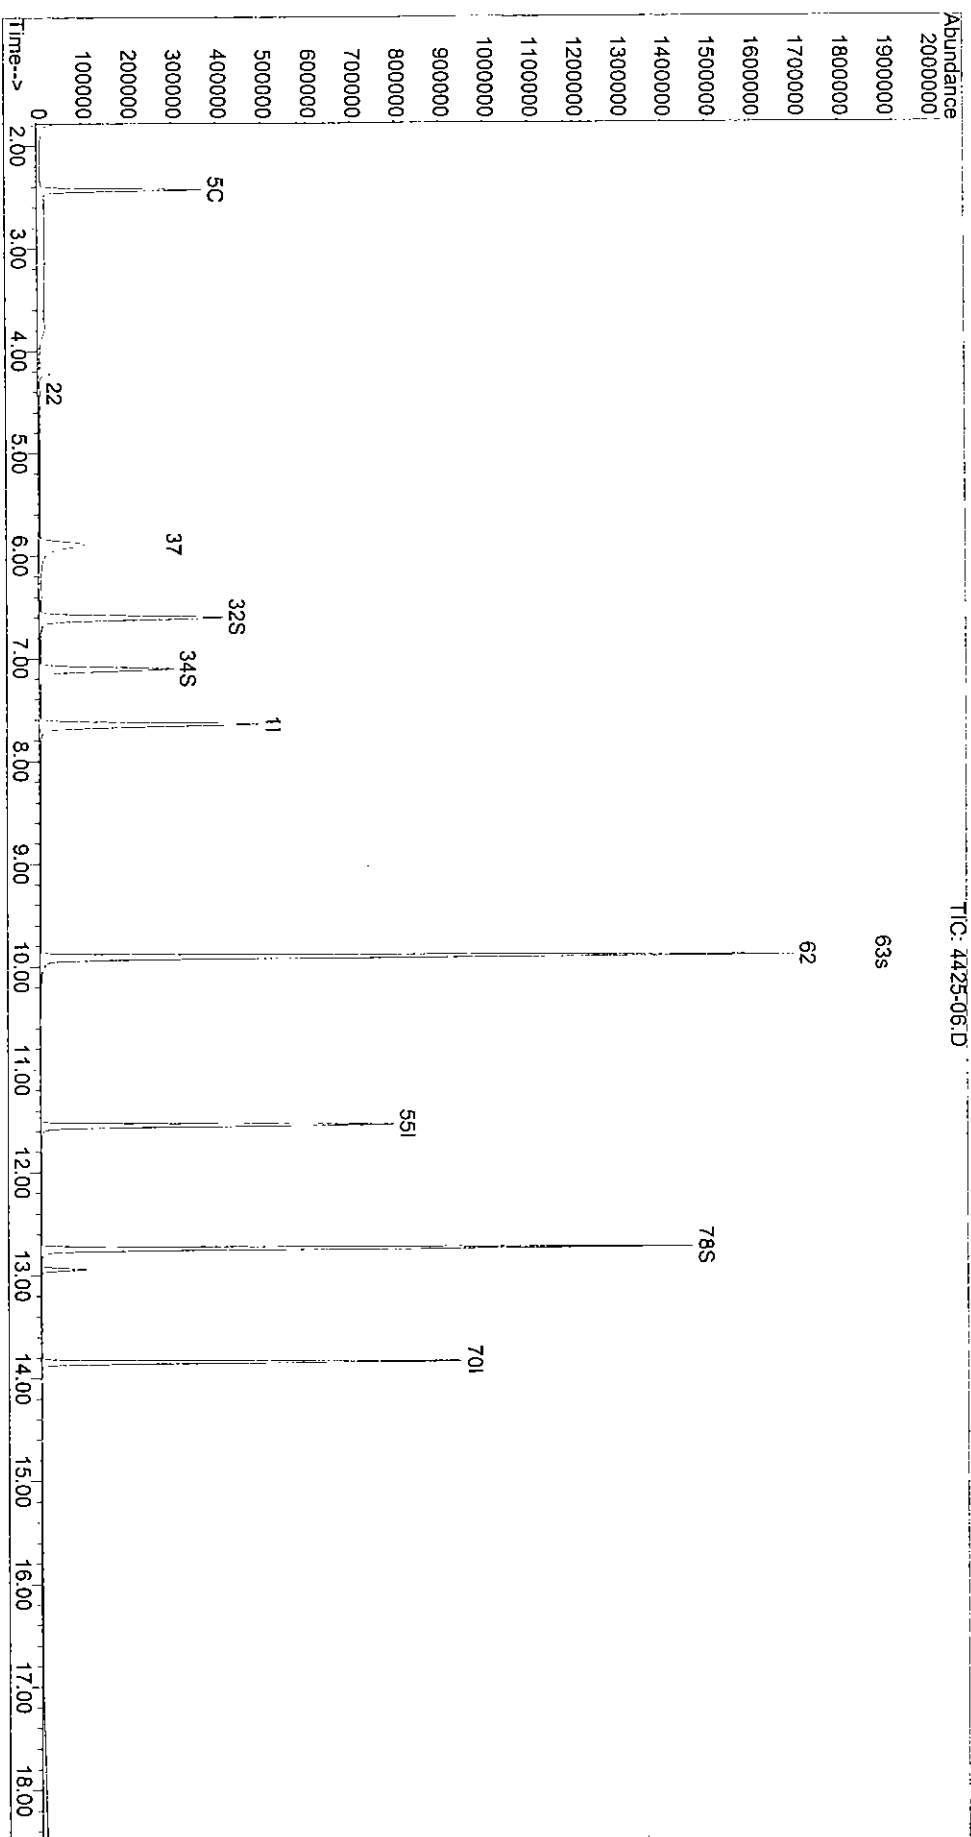

FORM-3A

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 524.2

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34455
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03G3619	
LCS Filename: G3619L01	Date Analyzed: 080803	Time Analyzed: 11:12
LCSD Filename: -	Date Analyzed: -	Time Analyzed: -

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
BENZENE	µg/L	20	0	19.1	96	65-120
CHLOROBENZENE	µg/L	20	0	20.7	104	65-134
1,1-DICHLOROETHENE	µg/L	20	0	19.7	99	65-127
TOLUENE	µg/L	20	0	19.5	98	65-134
TRICHLOROETHENE	µg/L	20	0	20.0	100	67-122
# of Out-of-control					0	

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits D - Spiked components diluted out

Comments: _____

FORM-3A

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 524.2

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34455
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03G3619	
MS Filename: G3619M01	Date Analyzed: 080803	Time Analyzed: 11:40
MSD Filename: G3619N01	Date Analyzed: 080803	Time Analyzed: 12:06
MS Sample No: MW-4-2	Sample Lab ID: 03-4455-4	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
BENZENE	µg/L	20	0	19.2	96	65-121
CHLOROBENZENE	µg/L	20	0	21.1	106	65-134
1,1-DICHLOROETHENE	µg/L	20	0	20.2	101	65-127
TOLUENE	µg/L	20	0	20.3	102	65-134
TRICHLOROETHENE	µg/L	20	0.7	21.3	103	65-125
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
BENZENE	µg/L	20	18.8	94	2	28	65-121
CHLOROBENZENE	µg/L	20	20.3	102	4	35	65-134
1,1-DICHLOROETHENE	µg/L	20	19.3	97	4	31	65-127
TOLUENE	µg/L	20	19.3	97	5	35	65-134
TRICHLOROETHENE	µg/L	20	20.4	99	4	30	65-125
# of Out-of-control				0	0		

Column to be used to flag recovery and RPD values:

* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: _____
