



A P C L

Applied Physics & Chemistry Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel. (909) 590-1528 Fax (909) 590-1498

Aug 20, 2003

GEOFON, Inc.

Attention: ~~Leo Williamson~~ *Brad Shojae*

22632 Golden Spring Dr Ste 270

Diamond Bar CA 91765

Dear Leo Williamson,

This package contains samples in our Service ID 03-4389 and your project : 04-4428.10 JPL

Enclosed please find:

- (1) Original analytical report.
- (2) Original Chain of Custody.
- (3) One diskette containing EDD deliverable.
- (4) One original Level C Data Package Deliverable.

If anything is missing or you have any questions, please feel free to contact me.

Respectfully submitted,

Regina Kirakozova  
Associate QA/QC Director  
Applied P & Ch Laboratory

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Submitted to:

GEOFON, Inc.

Attention: Brad Shojaee.

22632 Golden Spring Dr Ste 270

Diamond Bar CA 91765

Tel: (909)396-7662 Fax: (909)396-1455

# APCL Analytical Report

Service ID #: 801-034389

Received: 07/29/03

Collected by: Leo Williamson

Extracted: N/A

Collected on: 07/29/03

Tested: 07/29-08/06/03

Reported: 08/11/03

Sample Description: Water from MW-21 (Hahamonga Park)

Project Description: 04-4428.10 JPL

## Analysis of Water Samples

Component Analyzed	Method	Unit	PQL	Analysis Result		
				EB-1-7-29-03	MW-21-1	MW-21-2
				03-04389-1	03-04389-2	03-04389-3
<b>CHROMIUM (VI)</b>	7196	mg/L	0.01	<0.01	<0.01	<0.01
Dilution Factor				1	1	1
<b>PERCHLORATE</b>	314.0	µg/L	4	<4	5.2	2.1J
<b>VOLATILE ORGANIC COMPOUNDS</b>				1	1	1
Dilution Factor						
BENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOCHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMODICHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOFORM	524.2	µg/L	0.5	<0.5	<0.5	<0.5
BROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2-BUTANONE	524.2	µg/L	10	7J	<10	<10
N-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
SEC-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TERT-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CARBON TETRACHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLORODIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CHLOROFORM	524.2	µg/L	0.5	<0.5	1.7	<0.5
CHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
4-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DIBROMO-3-CHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DIBROMOETHANE (EDB)	524.2	µg/L	0.5	<0.5	<0.5	<0.5
DIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,4-DICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
DICHLORODIFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	0.7	<0.5
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CIS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5

# APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result		
				EB-1-7-29-03	MW-21-1	MW-21-2
				03-04389-1	03-04389-2	03-04389-3
TRANS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
2,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
CIS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TRANS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
ETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
HEXACHLOROBUTADIENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
ISOPROPYLBENZENE (CUMENE)	524.2	µg/L	0.5	<0.5	<0.5	<0.5
P-ISOPROPYLTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
METHYLENE CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
METHYL-T-BUTYL ETHER (MTBE)	524.2	µg/L	1	<1	<1	<1
4-METHYL-2-PENTANONE (MIBK)	524.2	µg/L	10	<10	<10	<10
NAPHTHALENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
N-PROPYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
STYRENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,1,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TETRACHLOROETHENE	524.2	µg/L	0.5	<0.5	1.0	1.3
TOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,4-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,1-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
TRICHLOROETHENE	524.2	µg/L	0.5	<0.5	11.0	0.5J
TRICHLOROFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,2,4-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
1,3,5-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
VINYL CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
O-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5
M/P-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5


# APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result			
				MW-21-3	MW-21-4	MW-21-5	TB-1-7-29-03
				03-04389-4	03-04389-5	03-04389-6	03-04389-7
<b>CHROMIUM (VI)</b>	7196	mg/L	0.01	<0.01	<0.01	<0.01	-
Dilution Factor				1	1	1	1
<b>PERCHLORATE</b>	314.0	µg/L	4	2.7J	2.7J	2.6J	-
<b>VOLATILE ORGANIC COMPOUNDS</b>							
Dilution Factor				1	1	1	1
BENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOCHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMODICHLOROMETHANE	524.2	µg/L	0.5	<0.5	0.5	<0.5	<0.5
BROMOFORM	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
BROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
N-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
SEC-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TERT-BUTYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2-BUTANONE	524.2	µg/L	10	<10	<10	<10	<10
CARBON TETRACHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLORODIBROMOMETHANE	524.2	µg/L	0.5	0.4J	0.7	<0.5	<0.5
CHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CHLOROFORM	524.2	µg/L	0.5	0.5J	3.2	3.6	<0.5
CHLOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
4-CHLOROTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DIBROMO-3-CHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DIBROMOETHANE (EDB)	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
DIBROMOMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,4-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
DICHLORODIFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CIS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	0.4J	2.2	2.5	<0.5
TRANS-1,2-DICHLOROETHENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
2,2-DICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
CIS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TRANS-1,3-DICHLOROPROPENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5

# APCL Analytical Report

Component Analyzed	Method	Unit	PQL	Analysis Result			
				MW-21-3	MW-21-4	MW-21-5	TB-1-7-29-03
				03-04389-4	03-04389-5	03-04389-6	03-04389-7
ETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
HEXACHLOROBUTADIENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
ISOPROPYLBENZENE (CUMENE)	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
P-ISOPROPYLTOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
METHYLENE CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	2.5
METHYL-T-BUTYL ETHER (MTBE)	524.2	µg/L	1	<1	<1	<1	<1
4-METHYL-2-PENTANONE (MIBK)	524.2	µg/L	10	<10	<10	<10	2J
NAPHTHALENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
N-PROPYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
STYRENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,1,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2,2-TETRACHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TETRACHLOROETHENE	524.2	µg/L	0.5	1.8	15.4	20.2	<0.5
TOLUENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,4-TRICHLOROBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,1-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2-TRICHLOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
TRICHLOROETHENE	524.2	µg/L	0.5	1.0	1	1	<0.5
TRICHLOROFLUOROMETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,3-TRICHLOROPROPANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,1,2,2,2-TRICHLORO-1,1,1,2,2,2-TRIFLUOROETHANE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,2,4-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
1,3,5-TRIMETHYLBENZENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
VINYL CHLORIDE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
O-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5
M/P-XYLENE	524.2	µg/L	0.5	<0.5	<0.5	<0.5	<0.5

PQL: Practical Quantitation Limit. MDL: Method Detection Limit. CRDL: Contract Required Detection Limit  
 N.D.: Not Detected or less than the practical quantitation limit. "": Analysis is not required.  
 J: Reported between PQL and MDL.  
 Listed Dilution Factors (DF) are relative to the method default DF. All unlisted DFs are 1.0

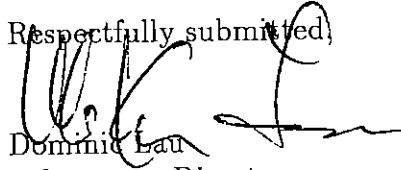Respectfully submitted,  
  
 Dominic Lau  
 Laboratory Director  
 Applied P & Ch Laboratory

Level C Data Package Deliverables

## General Information

Project: 04-4428.10 JPL

APCL Service ID: 03-4389



Applied P & Ch Laboratory

13760 Magnolia Ave. Chino, CA 91710

Telephone (909)590-1828

Fax (909)590-1498

# Case Narrative

**Project: JPL/MW-21. (Hahamonga Park)/04-4428.10**

**For GEOFON, Inc.**

**APCL Service No: 03-4389**

## 1. Sample Identification

The sample identifications are listed in the following table:

GEOFON, Inc. Sample ID	APCL Sample ID
MW-21-5	03-04389-6
MW-21-4	03-04389-5
MW-21-3	03-04389-4
MW-21-2	03-04389-3
MW-21-1	03-04389-2
TB-1-7-29-03	03-04389-7
EB-1-7-29-03	03-04389-1

## 2. Analytical Methodology

Samples are analyzed by EPA methods  
524.2 (Volatile Organic Compounds ),  
7196 (Chromium (VI) ),  
314.0 (Perchlorate, low level ),

## 3. Holding Time

All samples were extracted, digested and analyzed within the holding times defined by the appropriate EPA methods of the analyses.

## 4. Preservation

All samples were preserved and stored according to the appropriate EPA methods.

## 5. Tele-log


None

## 6. Anomaly

None

"I certify that these data are technically accurate, complete, and in compliance with the terms and conditions of the contract, for other than the conditions detailed above. Release of the data contained in the hardcopy data package and its electronic data deliverable submitted on diskette had been authorized by the Laboratory Manager or her/his designee, as verified by the following signature."

Respectfully submitted,



Regina Kirakozova  
Associate QA/QC Director  
Applied P & Ch Laboratory





INCORPORATED  
 22632 GOLDEN SPRINGS DR., SUITE 270  
 DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

MW-21 0041

Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont	QC Level	T.A.T	Analyses	Comments
1	MW-21-5	H <sub>2</sub> O	7/29/03	1149	HCl MNO <sub>3</sub> None	3+1+1	III	Normal	X X X	
2	MW-21-4			1221					X X X	
3	MW-21-3			1250					X X X	
4	MW-21-2			1321					X X X	
5	MW-21-1			1355					X X X	
6										
7	TB-1-7-29-03	H <sub>2</sub> O	7/29/03		HCl	3	III	Normal	X	
8	EB-1-7-29-03			1230	HCl MNO <sub>3</sub> None	3+1+1			X X X	
9										
10										

4389

SAMPLES COLLECTED BY: Leo W. Williamson COURIER AND AIR BILL NUMBER: \_\_\_\_\_  
 RELINQUISHED BY: \_\_\_\_\_ RECEIVED BY: \_\_\_\_\_ DATE: 7/29/03 TIME: 14:39  
 SAMPLE'S CONDITION UPON RECEIPT: \_\_\_\_\_

PROJECT CONTACT: J.S. Ford PROJECT PHONE NUMBER: (909) 920 8729 PROJECT FAX: (909) 396-1455  
 PROJECT ADDRESS: 7800 CITY, STATE AND ZIP CODE: Pasadena CA CLIENT: US Navy SWD  
 PROJECT MANAGER: Asrar Yehya PROJECT MANAGER'S PHONE: (909) 396-7662 PROJECT MANAGER'S FAX: (909) 396-1455  
 LABORATORY PHONE: (909) 580-1828 LABORATORY ADDRESS: 13760 Magnolia Ave  
 LABORATORY SERVICE ID: \_\_\_\_\_ CITY, STATE AND ZIP CODE: 91710 LABORATORY CONTACT: Kenny Chan  
 MAIL REPORT (COMPANY NAME): GEOFON, INC.  
 RECIPIENT NAME: Tony Ford  
 ADDRESS: 22632 Golden Springs Dr #270  
 CITY, STATE AND ZIP CODE: Diamond Bar, CA 91765

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager

# Sample Receiving Checklist

APCL ServiceID: **4389** Client Name/Project: Geoson SPL

### 1. Sample Arrival

Date/Time Received 7/29/03 10:45 Date/Time Opened 7/29/03 10:45 By (name): Kenny Chem  
Custody Transfer:  Client  Golden State  UPS  US Mail  FedEx  APCL Empl: Scott P.

### 2. Chain-of-Custody (CoC)

With Samples?  Faxed?  Client has Copy?  Signed, dated? By: \_\_\_\_\_  
 Project ID?  Analyses Clear?  Hold Samples? # on Hold \_\_\_\_\_ # Received 7  
 CoC/Docs Zip-Locked under lid?  Compos.#: \_\_\_\_\_  #Samples OK?  
 Discrepancies?  Client notified?  Response (attach docs): \_\_\_\_\_

### 3. Shipping Container/Cooler

Cooler Used? # of 1 Cooled by:  Ice  Blue Ice  Dry Ice  None  
Temp °C 3.9  
(Cooler temperature measured from temp blank if present, otherwise measured from the cooler).  
Cooler Custody Seal?  Absent  Intact  Tampered?

### 4. Sample Preservation

pH <2  pH >12  
If Not, pH = \_\_\_\_\_ Preserved by:  Client  APCL  Third Party \_\_\_\_\_

### 5. Holding-time Requirements

pH 24hr  BACT 6/24hr  Cr<sup>VI</sup> 24hr  NO<sub>3</sub><sup>-</sup> 48hr  BOD 48hr  
 Cl<sub>2</sub> ASAP  Turbidity 48hr  DO ASAP  Fe(II) ASAP  
 HT Expired?  Client notified?

### 6. Sample Container Condition

Intact?  Broken?  Documented? Number: \_\_\_\_\_  
Type:  plastic  glass  Tube: brass/SS  Tedlar Bag  
 Quantity OK?  Leaking?  Anomaly?  
 Caps tight?  Air Bubbles?  Anomaly?  
Labels:  Unique ID?  Date/Time  Preserved?

### 7. Turn Around Time

RUSH TAT: \_\_\_\_\_  Std (7-10 days)  Not Marked

### 8. Sample Matrix

Drinking H<sub>2</sub>O  Other Liq  Soil  Wipe  Polymer  Air  Other: \_\_\_\_\_  
 Ground H<sub>2</sub>O  Sludge  Filter  Oil/Petro  Paint  W. Water  Extract  Unknown

### 9. Pre-Login Check List Completed & OK?

ALL OK? (if not, attach docs)  Client Contact? (Name: \_\_\_\_\_) Date/Time: \_\_\_\_\_

Received/Checked by: [Signature] Printed: 29 Jul 2003 7:31 a.m.

\* HT: Samples must be analyzed for results to reflect total concentrations. Results generated outside required of holding times are considered minimal values and may be used to define waste as hazardous but not as non-hazardous.

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

# Sample Login: Check List

03-04389 (0470\_ 156) (2202777\_ 156)

07/30/03

## Part 1: General Information

---

<input type="checkbox"/>	Company Information	Name:	<i>GEOFON, Inc.</i>
		Address:	<i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i>
<input type="checkbox"/>	Project Information	Project Description:	<i>JPL</i>
		Project #:	<i>04-4428.10</i>
<input type="checkbox"/>	Billing Information	P.O. #:	
		Bill Address:	<i>22632 Golden Spring Dr Ste 270 ,Diamond Bar ,CA 91765</i>
		Lab Project ID:	
		Client Database #:	<i>3</i>
<input type="checkbox"/>	Receiving Information	Who Received Sample?	<i>Kenny Chan</i>
		Receiving Date/Time:	<i>07/29/03 1645</i>
		COC No.	
<input type="checkbox"/>	Shipping Information	Shipping Company	<i>APCL pick up</i>
		Packing Information:	<i>Cooler/Ice Chester</i>
		Cooler Temperature:	<i>3.9 °C</i>
<input type="checkbox"/>	Container Information	Container Provider:	<i>Client</i>
<input type="checkbox"/>	Sampling Information	Sampling Person:	
		Sampling Company:	<i>Client</i>
<input type="checkbox"/>	Turn-Around-Time Option:		<i>Rush 5 working day(s)</i>
<input type="checkbox"/>	QC Option:		<i>NEESA C</i>
<input type="checkbox"/>	Disposal Option:		<i>Not specify</i>

---

## Part 2: Sample Information

Seq. #	Sample ID (on COC)	Sample Sub-ID	APCL Sample ID	Matrix	Cont- tainer	Preser- vative	Vol, ml Am. g	# of Replica	Condition G, L, B	Collected mmddyy	Hold ?	Composite Group	TAT Days	
1	MW-21-5	VOC	03-04389-6- $\alpha$	W	V	C	40	3	G	072903	N	0	7	<input type="checkbox"/>
	MW-21-5	CRVI/Perch	03-04389-6- $\beta$	W	P		500	1	G	072903	N	0	7	<input type="checkbox"/>
2	MW-21-4	VOC	03-04389-5- $\alpha$	W	V	C	40	3	G	072903	N	0	7	<input type="checkbox"/>
	MW-21-4	CRVI/Perch	03-04389-5- $\beta$	W	P		500	1	G	072903	N	0	7	<input type="checkbox"/>
3	MW-21-3	VOC	03-04389-4- $\alpha$	W	V	C	40	3	G	072903	N	0	7	<input type="checkbox"/>
	MW-21-3	CRVI/Perch	03-04389-4- $\beta$	W	P		500	1	G	072903	N	0	7	<input type="checkbox"/>
4	MW-21-2	VOC	03-04389-3- $\alpha$	W	V	C	40	3	G	072903	N	0	7	<input type="checkbox"/>
	MW-21-2	CRVI/Perch	03-04389-3- $\beta$	W	P		500	1	G	072903	N	0	7	<input type="checkbox"/>
5	MW-21-1	VOC	03-04389-2- $\alpha$	W	V	C	40	3	G	072903	N	0	7	<input type="checkbox"/>
	MW-21-1	CRVI/Perch	03-04389-2- $\beta$	W	P		500	1	G	072903	N	0	7	<input type="checkbox"/>
6	TB-1-7-29-03	VOC	03-04389-7	W	V	C	40	3	G	072903	N	0	7	<input type="checkbox"/>
7	EB-1-7-29-03	VOC	03-04389-1- $\alpha$	W	V	C	40	3	G	072903	N	0	7	<input type="checkbox"/>
	EB-1-7-29-03	CRVI/Perch	03-04389-1- $\beta$	W	P		500	1	G	072903	N	0	7	<input type="checkbox"/>

## Part 3: Analysis Information

Test Items:	<input type="checkbox"/> 524.2	Volatile Organic Compounds
	<input type="checkbox"/> 7196A	Chromium (VI)
	<input type="checkbox"/> 314.0/300.0	Perchlorate, low level
	<input type="checkbox"/> 300.0	Chloride $Cl^-$ by IC
	<input type="checkbox"/> 300.0	Sulfate ( $SO_4^{--}$ ), by IC
	<input type="checkbox"/> 300.0/SM4500NO3	Nitrate ( $NO_3^-$ ) as N by IC
	<input type="checkbox"/> SM2320B	Carbonate
	<input type="checkbox"/> SM2320B	Bicarbonate
	<input type="checkbox"/> 9040B/150.1	pH
	<input type="checkbox"/> 160.1	Solids, Total Dissolved (TDS)
	<input type="checkbox"/> 200.7/6010B	Sodium, Na, by ICP
	<input type="checkbox"/> 200.7/6010B	Calcium, Ca, by ICP
	<input type="checkbox"/> 200.7/6010B	Potassium, K, by ICP
	<input type="checkbox"/> 200.7/6010B	Magnesium, Mg, by ICP
	<input type="checkbox"/> 200.7/6010B	Iron, Fe, by ICP
	<input type="checkbox"/> 206.2/7060A	Arsenic, As, by GFAA
	<input type="checkbox"/> 8270-SIM	1,4-Dioxane

Seq. #	Client's Sample ID (as given on COC)	Sample Sub-ID	APCL Sample ID	Matrix	524.2	CHROMIUM	PERCH	CL	SO4	NO3	CARBON	BICARB
--------	--------------------------------------	---------------	----------------	--------	-------	----------	-------	----	-----	-----	--------	--------

Level C Data Package Deliverables

# **Volatile Organics**



Applied P & Ch Laboratory

Applied P & Ch Laboratory  
**Organic Analysis Results for Method 524.2**

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 08/06/2003
Project ID: JPL	Service ID: 34389	Collected by:
Sample ID: <b>03G3570-MB-01</b>	Lab Sample ID: 03G3570-MB-01	Received Date: 08/06/2003
Sample Type: Method Blank	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3570	Prep. Date: 08/06/03	Anal. Date: 08/06/03
Data File Name: G3570K01	Prep. No: -	Anal. Time: 13:08
Methanol Vol: -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

## Surrogates

		Control Limit, %	Surro. Rec.%	
1	4-BROMO-FLUOROBENZENE (BFB)	460-00-4	70-129	94
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	105
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	104
4	TOLUENE-D8	2037-26-5	73-129	98

# of out-of-control

0

## Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4	50-200	96
2	1,4-DICHLOROETHANE-D4	3855-82-1	50-200	98
3	FLUOROBENZENE	462-06-6	50-200	92

# of out-of-control

0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory  
**Organic Analysis Results for Method 524.2**

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 07/29/2003
Project ID: JPL	Service ID: 34389	Collected by:
Sample ID: <b>EB-1-7-29-03</b>	Lab Sample ID: 03-4389-1	Received Date: 07/29/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3570	Prep. Date: 08/06/03	Anal. Date: 08/06/03
Data File Name: 4389-01	Prep. No: -	Anal. Time: 14:01
Methanol Vol: -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	7	J
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U



#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

**Surrogates**

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	96
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	107
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	106
4	TOLUENE-D8	2037-26-5	73-129	98

# of out-of-control

0

**Internal Standard**

		Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4	50-200	95
2	1,4-DICHLOROENZENE-D4	3855-82-1	50-200	97
3	FLUOROBENZENE	462-06-6	50-200	91

# of out-of-control

0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank  
D - Diluted

Applied P & Ch Laboratory  
**Organic Analysis Results for Method 524.2**

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 07/29/2003
Project ID: JPL	Service ID: 34389	Collected by:
Sample ID: MW-21-1	Lab Sample ID: 03-4389-2	Received Date: 07/29/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3570	Prep. Date: 08/06/03	Anal. Date: 08/06/03
Data File Name: 4389-02	Prep. No: -	Anal. Time: 14:53
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	1.7	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	0.7	
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	1.0	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	11.0	
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	112TRICHLORO-122TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

## Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	96
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	110
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	105
4	TOLUENE-D8	2037-26-5	73-129	98

# of out-of-control

0

## Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4	50-200	96
2	1,4-DICHLOROETHANE-D4	3855-82-1	50-200	98
3	FLUOROBENZENE	462-06-6	50-200	92

# of out-of-control

0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank  
D - Diluted

Applied P & Ch Laboratory  
**Organic Analysis Results for Method 524.2**

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 07/29/2003
Project ID: JPL	Service ID: 34389	Collected by:
Sample ID: MW-21-2	Lab Sample ID: 03-4389-3	Received Date: 07/29/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3570	Prep. Date: 08/06/03	Anal. Date: 08/06/03
Data File Name: 4389-03	Prep. No: -	Anal. Time: 15:19
Methanol Vol: -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	< 0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	< 0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	< 0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	< 0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	< 0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	< 0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	< 10	U
8	N-BUTYL BENZENE	104-51-8	µg/L	0.5	< 0.5	U
9	SEC-BUTYL BENZENE	135-98-8	µg/L	0.5	< 0.5	U
10	TERT-BUTYL BENZENE	98-06-6	µg/L	0.5	< 0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	< 0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	< 0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	< 0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	< 0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	< 0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	< 0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	< 0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	< 0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	< 0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	< 0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	< 0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	< 0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	< 0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	< 0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	< 0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	< 0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	< 0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	< 0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	< 0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	< 0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	< 0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	< 0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	< 0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	< 0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	< 0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	< 0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	< 0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	< 0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	< 0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	1.3	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	0.5	J
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2-TRICHLORO-1,1,2,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U
<b>Surrogates</b>				<b>Control Limit, %</b>	<b>Surro. Rec.%</b>	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4		70-129	96	
2	1,2-DICHLOROETHANE-D4	17060-07-0		70-129	110	
3	DIBROMOFLUOROMETHANE	1868-53-7		70-122	106	
4	TOLUENE-D8	2037-26-5		73-129	98	
# of out-of-control					0	
<b>Internal Standard</b>				<b>Control Limit, %</b>	<b>IS Rec.%</b>	
1	CHLOROENZENE-D5	3114-55-4		50-200	96	
2	1,4-DICHLOROENZENE-D4	3855-82-1		50-200	97	
3	FLUOROENZENE	462-06-6		50-200	92	
# of out-of-control					0	

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank  
D - Diluted

Applied P & Ch Laboratory  
**Organic Analysis Results for Method 524.2**

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 07/29/2003
Project ID: JPL	Service ID: 34389	Collected by:
Sample ID: MW-21-3	Lab Sample ID: 03-4389-4	Received Date: 07/29/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3570	Prep. Date: 08/06/03	Anal. Date: 08/06/03
Data File Name: 4389-04	Prep. No: -	Anal. Time: 15:46
Methanol Vol: -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	0.4	J
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	0.5	J
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	0.4	J
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	1.8	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	1.0	
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	112TRICHLORO-122TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

## Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	96
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	110
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	105
4	TOLUENE-D8	2037-26-5	73-129	97

# of out-of-control

0

## Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROENZENE-D5	3114-55-4	50-200	96
2	1,4-DICHLOROENZENE-D4	3855-82-1	50-200	97
3	FLUOROENZENE	462-06-6	50-200	92

# of out-of-control

0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory  
**Organic Analysis Results for Method 524.2**

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 07/29/2003
Project ID: JPL	Service ID: 34389	Collected by:
Sample ID: MW-21-4	Lab Sample ID: 03-4389-5	Received Date: 07/29/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3570	Prep. Date: 08/06/03	Anal. Date: 08/06/03
Data File Name: 4389-05	Prep. No: -	Anal. Time: 16:12
Methanol Vol: -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	0.5	
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	0.7	
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	3.2	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	2.2	
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U



#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	15.4	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	1	
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	112TRICHLORO-122TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

## Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	96
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	111
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	107
4	TOLUENE-D8	2037-26-5	73-129	97

# of out-of-control

0

## Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4	50-200	96
2	1,4-DICHLOROBENZENE-D4	3855-82-1	50-200	97
3	FLUOROBENZENE	462-06-6	50-200	91

# of out-of-control

0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory  
**Organic Analysis Results for Method 524.2**

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 07/29/2003
Project ID: JPL	Service ID: 34389	Collected by:
Sample ID: MW-21-5	Lab Sample ID: 03-4389-6	Received Date: 07/29/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3570	Prep. Date: 08/06/03	Anal. Date: 08/06/03
Data File Name: 4389-06	Prep. No: -	Anal. Time: 16:39
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Spurge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	3.6	
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	2.5	
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	<0.5	U
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	<10	U
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	20.2	
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	1	
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

## Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	96
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	109
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	106
4	TOLUENE-D8	2037-26-5	73-129	97

# of out-of-control

0

## Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4	50-200	96
2	1,4-DICHLOROENZENE-D4	3855-82-1	50-200	96
3	FLUOROBENZENE	462-06-6	50-200	91

# of out-of-control

0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

Applied P & Ch Laboratory  
**Organic Analysis Results for Method 524.2**

Client Name: GEOFON, Inc.	Project No: 04-4428.10	Collection Date: 07/29/2003
Project ID: JPL	Service ID: 34389	Collected by:
Sample ID: <b>TB-1-7-29-03</b>	Lab Sample ID: 03-4389-7	Received Date: 07/29/2003
Sample Type: Field Sample	Sample Matrix: Water	Moisture %: -
Anal. Method: 524.2	Prep. Method: 5030	Instrument ID: GC/MS: A
Batch No: 03G3570	Prep. Date: 08/06/03	Anal. Date: 08/06/03
Data File Name: 4389-07	Prep. No: -	Anal. Time: 13:34
Methanol Vol. -	Sample Amount: 25.0 mL	Dilution Factor: 1
Test Level: Low	Sparge Size: 25 mL	Heated Purge: (Y/N) N

#	Component Name	CAS No	Unit	RL	Result	Qualifier
1	BENZENE	71-43-2	µg/L	0.5	<0.5	U
2	BROMOBENZENE	108-86-1	µg/L	0.5	<0.5	U
3	BROMOCHLOROMETHANE	74-97-5	µg/L	0.5	<0.5	U
4	BROMODICHLOROMETHANE	75-27-4	µg/L	0.5	<0.5	U
5	BROMOFORM	75-25-2	µg/L	0.5	<0.5	U
6	BROMOMETHANE	74-83-9	µg/L	0.5	<0.5	U
7	2-BUTANONE	78-93-3	µg/L	10	<10	U
8	N-BUTYLBENZENE	104-51-8	µg/L	0.5	<0.5	U
9	SEC-BUTYLBENZENE	135-98-8	µg/L	0.5	<0.5	U
10	TERT-BUTYLBENZENE	98-06-6	µg/L	0.5	<0.5	U
11	CARBON TETRACHLORIDE	56-23-5	µg/L	0.5	<0.5	U
12	CHLOROBENZENE	108-90-7	µg/L	0.5	<0.5	U
13	CHLORODIBROMOMETHANE	124-48-1	µg/L	0.5	<0.5	U
14	CHLOROETHANE	75-00-3	µg/L	0.5	<0.5	U
15	CHLOROFORM	67-66-3	µg/L	0.5	<0.5	U
16	CHLOROMETHANE	74-87-3	µg/L	0.5	<0.5	U
17	2-CHLOROTOLUENE	95-49-8	µg/L	0.5	<0.5	U
18	4-CHLOROTOLUENE	106-43-4	µg/L	0.5	<0.5	U
19	1,2-DIBROMO-3-CHLOROPROPANE	96-12-8	µg/L	0.5	<0.5	U
20	1,2-DIBROMOETHANE (EDB)	106-93-4	µg/L	0.5	<0.5	U
21	DIBROMOMETHANE	74-95-3	µg/L	0.5	<0.5	U
22	1,2-DICHLOROBENZENE	95-50-1	µg/L	0.5	<0.5	U
23	1,3-DICHLOROBENZENE	541-73-1	µg/L	0.5	<0.5	U
24	1,4-DICHLOROBENZENE	106-46-7	µg/L	0.5	<0.5	U
25	DICHLORODIFLUOROMETHANE	75-71-8	µg/L	0.5	<0.5	U
26	1,1-DICHLOROETHANE	75-34-3	µg/L	0.5	<0.5	U
27	1,2-DICHLOROETHANE	107-06-2	µg/L	0.5	<0.5	U
28	1,1-DICHLOROETHENE	75-35-4	µg/L	0.5	<0.5	U
29	CIS-1,2-DICHLOROETHENE	156-59-2	µg/L	0.5	<0.5	U
30	TRANS-1,2-DICHLOROETHENE	156-60-5	µg/L	0.5	<0.5	U
31	1,2-DICHLOROPROPANE	78-87-5	µg/L	0.5	<0.5	U
32	1,3-DICHLOROPROPANE	142-28-9	µg/L	0.5	<0.5	U
33	2,2-DICHLOROPROPANE	594-20-7	µg/L	0.5	<0.5	U
34	1,1-DICHLOROPROPENE	563-58-6	µg/L	0.5	<0.5	U
35	CIS-1,3-DICHLOROPROPENE	10061-01-5	µg/L	0.5	<0.5	U
36	TRANS-1,3-DICHLOROPROPENE	10061-02-6	µg/L	0.5	<0.5	U
37	ETHYLBENZENE	100-41-4	µg/L	0.5	<0.5	U
38	HEXACHLOROBUTADIENE	87-68-3	µg/L	0.5	<0.5	U
39	ISOPROPYLBENZENE (CUMENE)	98-82-8	µg/L	0.5	<0.5	U

#	Component Name	CAS No	Unit	RL	Result	Qualifier
40	P-ISOPROPYLTOLUENE	99-87-6	µg/L	0.5	<0.5	U
41	METHYLENE CHLORIDE	75-09-2	µg/L	0.5	2.5	
42	METHYL-T-BUTYL ETHER (MTBE)	1634-04-4	µg/L	1	<1	U
43	4-METHYL-2-PENTANONE (MIBK)	108-10-1	µg/L	10	2	J
44	NAPHTHALENE	91-20-3	µg/L	0.5	<0.5	U
45	N-PROPYLBENZENE	103-65-1	µg/L	0.5	<0.5	U
46	STYRENE	100-42-5	µg/L	0.5	<0.5	U
47	1,1,1,2-TETRACHLOROETHANE	630-20-6	µg/L	0.5	<0.5	U
48	1,1,2,2-TETRACHLOROETHANE	79-34-5	µg/L	0.5	<0.5	U
49	TETRACHLOROETHENE	127-18-4	µg/L	0.5	<0.5	U
50	TOLUENE	108-88-3	µg/L	0.5	<0.5	U
51	1,2,3-TRICHLOROBENZENE	87-61-6	µg/L	0.5	<0.5	U
52	1,2,4-TRICHLOROBENZENE	120-82-1	µg/L	0.5	<0.5	U
53	1,1,1-TRICHLOROETHANE	71-55-6	µg/L	0.5	<0.5	U
54	1,1,2-TRICHLOROETHANE	79-00-5	µg/L	0.5	<0.5	U
55	TRICHLOROETHENE	79-01-6	µg/L	0.5	<0.5	U
56	TRICHLOROFLUOROMETHANE	75-69-4	µg/L	0.5	<0.5	U
57	1,2,3-TRICHLOROPROPANE	96-18-4	µg/L	0.5	<0.5	U
58	1,1,2,2-TRICHLORO-1,1,2,2-TRIFLUOROETHANE	76-13-1	µg/L	0.5	<0.5	U
59	1,2,4-TRIMETHYLBENZENE	95-63-6	µg/L	0.5	<0.5	U
60	1,3,5-TRIMETHYLBENZENE	108-67-8	µg/L	0.5	<0.5	U
61	VINYL CHLORIDE	75-01-4	µg/L	0.5	<0.5	U
62	O-XYLENE	95-47-6	µg/L	0.5	<0.5	U
63	M/P-XYLENE	108-38-3	µg/L	0.5	<0.5	U

## Surrogates

		Control Limit, %	Surro. Rec.%	
1	1-BROMO-4-FLUOROBENZENE (4-BROMOFL)	460-00-4	70-129	95
2	1,2-DICHLOROETHANE-D4	17060-07-0	70-129	105
3	DIBROMOFLUOROMETHANE	1868-53-7	70-122	103
4	TOLUENE-D8	2037-26-5	73-129	99

# of out-of-control

0

## Internal Standard

		Control Limit, %	IS Rec.%	
1	CHLOROBENZENE-D5	3114-55-4	50-200	96
2	1,4-DICHLOROETHANE-D4	3855-82-1	50-200	97
3	FLUOROBENZENE	462-06-6	50-200	92

# of out-of-control

0

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Qualifier: U - Not Detected or less than MDL

E - Exceed calibration range

J - Less than RL (PQL, EQL or CRDL), but greater than MDL, or an estimated result (e.g. for TIC)

B - A positive value was found in the method blank

D - Diluted

FORM-2A

Applied P & Ch Laboratory

**Surrogate Recovery Summary for Method 524.2**

Client Name: GEOFON, Inc.  
 Case No:  
 Project ID: JPL

Contract No:  
 SAS No:  
 Project No: 04-4428.10  
 Batch No: 03G3570

Lab Code: APCL  
 SDG Number: 034389  
 Sample Matrix: Water

#	Client Sample No	Lab Sample ID	S1 % #	S2 % #	S3 % #	S4 % #	TOT OUT
1	03G3570-LCS-01	03G3570-LCS-01	93	96	97	95	0
2	MW-19-2MS	03-4406-10MS	97	95	97	99	0
3	MW-19-2MSD	03-4406-10MSD	95	94	97	96	0
4	03G3570-MB-01	03G3570-MB-01	94	105	104	98	0
5	TB-1-7-29-03	03-4389-7	95	105	103	99	0
6	EB-1-7-29-03	03-4389-1	96	107	106	98	0
7	MW-21-1	03-4389-2	96	110	105	98	0
8	MW-21-2	03-4389-3	96	110	106	98	0
9	MW-21-3	03-4389-4	96	110	105	97	0
10	MW-21-4	03-4389-5	96	111	107	97	0
11	MW-21-5	03-4389-6	96	109	106	97	0
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							

QC Control Limit

S1 = 1-BROMO-4-FLUOROBENZENE (4-BROMOFL) 70-129  
 S2 = 1,2-DICHLOROETHANE-D4 70-129  
 S3 = DIBROMOFLUOROMETHANE 70-122  
 S4 = TOLUENE-D8 73-129

# Column to be used to flag recovery values:

\* - Values outside of contract required QC Limits    D - Surrogate diluted out    I - Matrix Interference

FORM-3A

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 524.2

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34389
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03G3570	
LCS Filename: G3570L01	Date Analyzed: 080603	Time Analyzed: 10:58
LCSD Filename: -	Date Analyzed: -	Time Analyzed: -

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
BENZENE	µg/L	50	0	46.6	93	65-120
CHLOROBENZENE	µg/L	50	0	49.8	100	65-134
1,1-DICHLOROETHENE	µg/L	50	0	48.3	97	65-127
TOLUENE	µg/L	50	0	47.2	94	65-134
TRICHLOROETHENE	µg/L	50	0	48.9	98	67-122
# of Out-of-control					0	

# Column to be used to flag recovery and RPD values:

\* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: \_\_\_\_\_  
 \_\_\_\_\_

FORM-3A

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 524.2

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34389
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03G3570	
MS Filename: G3570M01	Date Analyzed: 080603	Time Analyzed: 11:24
MSD Filename: G3570N01	Date Analyzed: 080603	Time Analyzed: 11:50
MS Sample No: MW-19-2	Sample Lab ID: 03-4406-10	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
BENZENE	µg/L	50	0	47.5	95	65-121
CHLOROBENZENE	µg/L	50	0	51.0	102	65-134
1,1-DICHLOROETHENE	µg/L	50	0	49.6	99	65-127
TOLUENE	µg/L	50	0	49.0	98	65-134
TRICHLOROETHENE	µg/L	50	0.6	50.8	100	65-125
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
BENZENE	µg/L	50	46.8	94	1	28	65-121
CHLOROBENZENE	µg/L	50	50.0	100	2	35	65-134
1,1-DICHLOROETHENE	µg/L	50	48.0	96	3	31	65-127
TOLUENE	µg/L	50	47.7	95	3	35	65-134
TRICHLOROETHENE	µg/L	50	49.7	98	2	30	65-125
# of Out-of-control					0	0	

# Column to be used to flag recovery and RPD values:

\* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: \_\_\_\_\_



FORM-4A

Applied P & Ch Laboratory

Method Blank Summary for Method 524.2

Client Name: GEOFON, Inc.

Contract No:

Lab Code: APCL

Case No:

SAS No:

Service ID: 34389

Project ID: JPL

Project No: 04-4428.10

Analysis Date: 08/06/03

Sample Matrix: Water

Analysis Time: 13:08

Sample ID: 03G3570-MB-01

Batch No: 03G3570

Instrument ID: GC/MS: A

Lab Sample ID: 03G3570-MB-01

Data File Name: G3570K01

GC Column: HP-VOC

Heated Purge: (Y/N) N


Column ID: 0.20 mm

This Method Blank applies to the following samples and QC samples:

#	Client Sample No	Lab Sample ID	Sample Type	Data Filename	Analysis Date	Analysis Time
1	03G3570-LCS-01	03G3570-LCS-01	Lab Control Spike	G3570L01	08/06/03	10:58
2	MW-19-2MS	03-4406-10MS	Matrix Spike	G3570M01	08/06/03	11:24
3	MW-19-2MSD	03-4406-10MSD	Matrix Spike Duplicate	G3570N01	08/06/03	11:50
4	TB-1-7-29-03	03-4389-7	Field Sample	4389-07	08/06/03	13:34
5	EB-1-7-29-03	03-4389-1	Field Sample	4389-01	08/06/03	14:01
6	MW-21-1	03-4389-2	Field Sample	4389-02	08/06/03	14:53
7	MW-21-2	03-4389-3	Field Sample	4389-03	08/06/03	15:19
8	MW-21-3	03-4389-4	Field Sample	4389-04	08/06/03	15:46
9	MW-21-4	03-4389-5	Field Sample	4389-05	08/06/03	16:12
10	MW-21-5	03-4389-6	Field Sample	4389-06	08/06/03	16:39
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						

Data File : C:\MSDCHEM\1\DATA\03G3415\G3415P01.D  
 Acq On : 22 Jul 2003 5:08 pm  
 Sample : ##03G3415, w 50 ng  
 Misc :  
 MS Integration Params: Lscint.P  
 Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P &ch Lab\*\* EPA 524.2

Vial: 2  
 Operator: zou  
 Inst : GCMS-A  
 Multiplr: 1.00

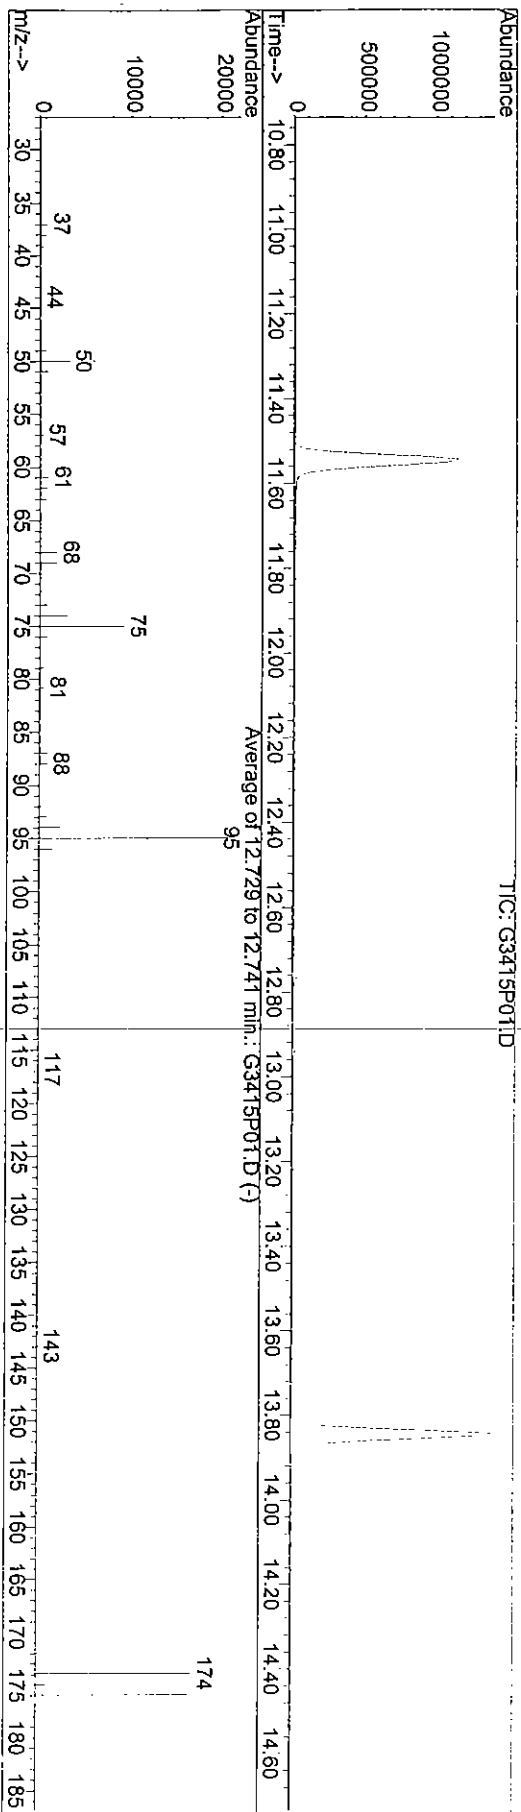

Spectrum Information: Average of 12.729 to 12.741 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	15.3	3208	PASS
75	95	30	60	44.1	9259	PASS
95	95	100	100	100.0	20984	PASS
96	95	5	9	7.0	1467	PASS
173	174	0.00	2	0.7	120	PASS
174	95	50	100	81.3	17069	PASS
175	174	5	9	7.1	1218	PASS
176	174	95	101	98.6	16830	PASS
177	176	5	9	7.6	1277	PASS

5A  
VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
BROMOFLUOROBENZENE (BFB)

Lab Name : APPLIED P & CH LAB Contract: \_\_\_\_\_  
 Lab Code: \_\_\_\_\_ Case No.: \_\_\_\_\_ SAS No.: \_\_\_\_\_ SDG No.: 034389  
 Lab File ID: G3415 P01 BFB Injection Date: 07/22/2003  
 Instrument ID: GCMS-A BFB Injection Time: 1708  
 GC Column: HP-VOC ID: 0.20 (mm) Heated Purge: (Y/N) N

m/e	ION ABUNDANCE CRITERIA	%RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	15.3
75	30.0 - 60.0% of mass 95	44.1
95	Base peak, 100% relative abundance	100.0
96	5.0 - 9.0% of mass 95	7.0
173	Less than 2.0% of mass 174	0.6 ( 0.7 )1
174	50.0 - 100.0% of mass 95	81.3
175	5.0 - 9.0% of mass 174	5.8 ( 7.1 )1
176	95.0 - 101.0% of mass 174	80.2 ( 98.6 )1
177	5.0 - 9.0% of mass 176	6.1 ( 7.6 )2

1-Value is % mass 174

2-Value is % mass 176

This check applies to the following SAMPLES, MS, MSD, BLANKS and STANDARDS:

	EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
01	VSTD0003	20-0003	20-00003.D	07/22/2003	1925
02	VSTD002	20-0002	20-0002.D	07/22/2003	2111
03	VSTD010	20-0010	20-0010.D	07/22/2003	2137
04	VSTD020	20-0020	20-0020.D	07/22/2003	2256
05	VSTD040	20-0040	20-0040.D	07/23/2003	0043
06	VSTD060	20-0060	20-0060.D	07/23/2003	0245
07					
08					
09					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					

Response Factor Report GCMS-A

Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P & Ch Lab\*\* EPA 524.2  
 Last Update : Thu Jul 24 12:40:35 2003  
 Response via : Initial Calibration

Calibration Files  
 .3 =2-00003.D 2 =2-0002A.D 10 =2-00010.D  
 20 =2-00020.D 40 =2-00040.D 60 =2-00060.D

Compound	.3	2	10	20	40	60	Avg	%RSD
1) I Fluorobenzene	0.279	0.253	0.228	0.251	0.250	0.246	0.251	6.61
2) di-Cl-di-F-m	0.300	0.265	0.208	0.221	0.218	0.200	0.235	16.51
3) P Chloromethan	0.116	0.138	0.126	0.136	0.137	0.133	0.131	6.45
4) F114	0.268	0.267	0.219	0.239	0.240	0.223	0.242	8.61
5) C vinyl chlori	0.143	0.128	0.105	0.113	0.104	0.106	0.116	13.63
6) bromomethane	0.162	0.171	0.136	0.131	0.138	0.129	0.144	12.08
7) chloroethane	0.426	0.367	0.310	0.357	0.356	0.338	0.359	10.76
8) tri-Cl-F-met	0.055	0.041	0.041	0.042	0.041	0.040	0.044	14.16
9) Acetonitrile	0.034	0.034	0.026	0.025	0.024	0.022	0.028	18.73
10) acrolein	0.106	0.053	0.028	0.024	0.024	0.021	0.043	77.29
11) acetone X	0.162	0.157	0.117	0.117	0.110	0.098	0.127	20.67
12) ethyl ether	0.345	0.312	0.258	0.277	0.275	0.253	0.287	12.31#
13) M, Cl3 11-dichloroe	0.266	0.286	0.244	0.262	0.258	0.205	0.253	10.75
14) Iodomethane	0.313	0.246	0.193	0.211	0.205	0.185	0.225	21.21
15) F-113	0.053	0.052	0.042	0.041	0.040	0.040	0.045	13.61
16) acrylonitril	0.838	0.780	0.654	0.729	0.722	0.649	0.729	10.00
17) carbon disul	0.015	0.008	0.005	0.006	0.007	0.006	0.008	46.15
18) Isopropyl Al	1.323	0.482	0.257	0.251	0.242	0.244	0.467	92.15
19) methylene ch	0.297	0.305	0.248	0.262	0.256	0.253	0.270	8.99
20) t-12-di-Cl-e	0.474	0.509	0.419	0.427	0.427	0.442	0.450	7.81
21) t-Bu-Me-ethe	0.014	0.010	0.010	0.010	0.012	0.013	0.012	16.51
22) Tert butyl a	0.549	0.412	0.417	0.307	0.307	0.282	0.393	26.97
23) allyl chlori	0.518	0.484	0.380	0.407	0.403	0.409	0.433	12.52
24) p 11-dichloroe	0.020	0.014	0.016	0.016	0.016	0.017	0.017	14.53
25) propionitril	0.296	0.311	0.252	0.263	0.257	0.255	0.272	9.12
26) c-12-di-Cl-e	0.392	0.360	0.280	0.290	0.277	0.262	0.310	16.98
27) 22-Dichlorop	0.158	0.150	0.117	0.123	0.122	0.122	0.132	13.12
28) Br-Cl-methan								

*Handwritten mark*

*0.996*

*0.997*

*0.994*

*0.995*

*0.990*

*0.998*

(#) = Out of Range  
 E524A002.M Thu Jul 24 12:41:07 2003

Response Factor Report GCMS-A

Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P & Ch Lab\*\* EPA 524.2  
 Last Update : Thu Jul 24 12:40:35 2003  
 Response via : Initial Calibration

Calibration Files  
 .3 =2-00003.D 2 =2-0002A.D 10 =2-00010.D  
 20 =2-00020.D 40 =2-00040.D 60 =2-00060.D

Compound	.3	2	40	10	20	40	60	Avg	%RSD
29) C 25 chloroform	0.724	0.528	0.396	0.413	0.403	0.406	0.478	27.21#	1.00
30) 26 tetrahydrofu	0.036	0.035	0.031	0.031	0.032	0.032	0.033	6.66	
31) 98 Disopropyl	0.648	0.792	0.634	0.653	0.636	0.641	0.667	9.23	
32) S 27 Di-Br-F-Me (	0.294	0.230	0.240	0.239	0.243	0.249	10.27	10.27	
33) 99 FTBE	0.437	0.534	0.485	0.524	0.532	0.549	0.510	8.20	
34) S 29 1,2-Di-Cl-Et	0.248	0.186	0.191	0.191	0.192	0.202	12.96	12.96	
35) 30 12-dichloroe	0.094	0.093	0.070	0.070	0.070	0.070	0.078	15.50	1.00
36) 32 vinyl acetat	0.319	0.377	0.321	0.291	0.285	0.280	0.312	11.53	
37) 92 Nitro Methan	0.006	0.005	0.005	0.005	0.006	0.006	0.006	9.09	
38) 33 2-butanoneME	0.081	0.061	0.044	0.043	0.042	0.041	0.052	30.99	1.00
39) 93 Ethyl Acetat	0.175	0.135	0.110	0.107	0.107	0.110	0.124	22.07	0.999
40) 34 111-trichlor	0.479	0.436	0.353	0.387	0.385	0.378	0.403	11.36	
41) 35 11-Di-Cl-pro	0.271	0.306	0.284	0.325	0.324	0.316	0.304	7.40	
42) M 36 benzene	1.117	1.160	0.923	0.983	0.960	0.948	1.015	9.69	
43) 37 CCl4	0.434	0.397	0.329	0.361	0.358	0.350	0.371	10.20	
44) 100 Isobutyl al	0.002	0.005	0.004	0.004	0.005	0.005	0.004	30.78	0.997
45) 38 thiophene	0.471	0.573	0.471	0.505	0.504	0.503	0.505	7.36	
46) C 39 12-di-Cl-pro	0.247	0.251	0.204	0.220	0.221	0.220	0.227	7.93#	
47) M 40 trichloroeth	0.354	0.335	0.274	0.312	0.315	0.309	0.316	8.59	
48) 41 dibromometha	0.177	0.159	0.126	0.133	0.134	0.135	0.144	13.68	
49) 101 TAME	0.352	0.451	0.420	0.462	0.472	0.498	0.442	11.61	1.00
50) 42 Br-di-Cl-met	0.433	0.359	0.280	0.298	0.298	0.297	0.327	17.81	0.999
51) 43 Me-methacryl	0.065	0.098	0.100	0.112	0.117	0.121	0.102	20.03	0.999
52) 44 2-ClEt-Vl-et	0.010	0.016	0.019	0.025	0.029		0.020	37.07	0.992
53) 45 c-13-di-Cl-p	0.312	0.358	0.307	0.333	0.335	0.336	0.330	5.59	
54) 46 t-1,3-dichlo	0.227	0.272	0.247	0.270	0.278	0.281	0.262	8.00	
55) I 47 Chlorobezene-d5	0.288	0.275	0.213	0.222	0.224	0.226	0.241	13.17	
56) 48 112-tri-Cl-E									

(#) = Out of Range  
 E524A002.M Thu Jul 24 12:41:08 2003

Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P & Ch Lab\*\* EPA 524.2  
 Last Update : Thu Jul 24 12:40:35 2003  
 Response via : Initial Calibration

Calibration Files  
 .3 =2-00003.D 2 =2-0002A.D 10 =2-00010.D  
 20 =2-00020.D 40 =2-00040.D 60 =2-00060.D

Compound	.3	2	10	20	40	60	Avg	%RSD
57) 49 13-di-Cl-pro	0.436	0.432	0.347	0.357	0.359	0.353	0.381	10.91
58) 50 Et methacryl	0.189	0.269	0.272	0.287	0.301	0.321	0.273	16.74
59) .51 di-Br-Cl-met	0.422	0.341	0.275	0.296	0.304	0.309	0.325	16.16
60) P .52 bromoform	0.222	0.192	0.159	0.171	0.181	0.187	0.185	11.70
61) 53 1,4-dichloro	0.405	0.396	0.312	0.330	0.340	0.344	0.354	10.53
62) 54 MIBK	0.132	0.144	0.134	0.144	0.155	0.166	0.146	8.89
63) s 55 toluene-d8	1.345	1.364	1.130	1.244	1.257	1.223	1.260	6.78
64) M,C 56 toluene	1.448	1.627	1.315	1.441	1.448	1.412	1.448	6.98
65) 57 2-hexanone X	0.100	0.109	0.092	0.094	0.098	0.100	0.099	5.95
66) 58 12-dibromoet	0.274	0.254	0.210	0.222	0.233	0.235	0.238	9.68
67) 59 tetra-Cl-eth	0.496	0.464	0.378	0.427	0.424	0.408	0.433	9.68
68) M,P 60 chlorobenzen	1.297	1.156	0.893	0.967	0.959	0.919	1.032	15.48
69) 61 1112-tetra-C	0.447	0.412	0.317	0.340	0.348	0.348	0.369	13.47
70) I 62 1,4-Dichlorobenzen	-----ISTD-----							
71) 63 1-chlorohexa	0.269	0.309	0.291	0.356	0.374	0.358	0.326	12.94
72) C 64 Et-Bz	3.072	3.263	2.780	3.211	3.292	3.156	3.129	6.01#
73) 65 m/p-Xylenes	2.292	2.598	2.175	2.438	2.422	2.268	2.365	6.37
74) 66 styrene	1.472	1.978	1.707	1.902	1.915	1.818	1.798	10.32
75) 67 o-xylene	1.955	2.508	2.249	2.527	2.563	2.438	2.373	9.83
76) p 68 1122-Tetra-C	0.659	0.575	0.456	0.475	0.501	0.503	0.528	14.34
77) 69 123-tri-Cl-P	0.186	0.176	0.138	0.146	0.151	0.152	0.158	11.76
78) s 70 4-Br-1-F-Bz	0.953	0.876	0.706	0.798	0.823	0.806	0.827	10.01
79) 71 Isopropylben	2.262	3.010	2.857	3.361	3.462	3.290	3.040	14.58
80) 72 bromobenzene	0.840	0.881	0.719	0.807	0.842	0.810	0.817	6.73
81) 81) 92 t-1,4-dichlo	0.038	0.078	0.075	0.082	0.094	0.095	0.077	27.12
82) 82) 73 n-propylbenz	0.759	0.999	0.867	1.019	1.061	1.009	0.952	12.10
83) 83) 74 2-Cl-Toluene	0.756	0.887	0.758	0.870	0.905	0.873	0.841	7.90
84) 84) 75 4-Cl-Toluene	0.853	0.955	0.757	0.860	0.880	0.830	0.856	7.52

(#) = Out of Range  
 E524A002.M Thu Jul 24 12:41:09 2003

Response Factor Report GCMS-A

1531

Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P & Ch Lab\*\* EPA 524.2  
 Last Update : Thu Jul 24 12:40:35 2003  
 Response via : Initial Calibration

Calibration Files  
 .3 =2-00003.D 2 =2-0002A.D 10 =2-00010.D  
 20 =2-00020.D 40 =2-00040.D 60 =2-00060.D

Compound	.3	2	10	20	40	60	Avg	%RSD
85) 76 135-tri-Me-B	2.031	2.864	2.465	2.815	2.851	2.678	2.617	12.38
86) 77 4-iso-Pr-to1	2.280	3.155	2.726	3.159	3.220	2.998	2.923	12.39
87) 78 124-tri-Me-B	2.267	3.012	2.517	2.854	2.932	2.773	2.726	10.34
88) 79 tert-butylbe	2.041	2.391	2.526	2.636	2.748	2.655	2.499	10.24
89) 80 13-DCB	1.989	1.888	1.484	1.667	1.680	1.592	1.717	10.95
90) 81 sec-butylben	2.715	3.632	3.274	3.857	3.936	3.690	3.517	12.95
91) 82 14-DCB	2.240	1.859	1.457	1.644	1.684	1.613	1.749	15.60
92) 83 Cl-benzyl	0.164	0.159	0.155	0.169	0.181	0.165	0.165	5.41
93) 84 12-DCB	1.762	1.734	1.326	1.464	1.479	1.408	1.529	11.67
94) 85 n-butylbenze	0.528	0.789	0.731	0.875	0.910	0.843	0.779	17.73
95) 86 12-diBr-2-Cl	0.110	0.104	0.091	0.102	0.118	0.120	0.108	10.09
96) 87 124-tri-Cl-B	0.843	0.926	0.884	1.065	1.130	1.091	0.990	12.16
97) 88 naphthalene	2.218	1.820	1.426	1.651	1.832	1.831	1.796	14.50
98) 89 hx-Cl-butadi	0.644	0.621	0.514	0.599	0.629	0.588	0.599	7.74
99) 90 123-Tri-Cl-B	0.849	0.875	0.777	0.914	0.969	0.944	0.888	7.86

*Y*

*0.999*  
*0.997*

(#) = Out of Range  
 E524A002.M Thu Jul 24 12:41:09 2003

# INITIAL CALIBRATION SUMMARY

1532

Method File: E524A002  
 Last Calibration Update: Thu Jul 24 12:40:35 2003

Level	File Name	Level 1 ID	Level 2 ID	Level 3 ID	Level 4 ID	Level 5 ID	Level 6 ID	Level 7 ID
Level 1	File Name	2-00003.D	Level 1 ID	3				
Level 2	File Name	2-0002A.D	Level 2 ID	2				
Level 3	File Name	2-00010.D	Level 3 ID	10				
Level 4	File Name	2-00020.D	Level 4 ID	20				
Level 5	File Name	2-00040.D	Level 5 ID	40				
Level 6	File Name	2-00060.D	Level 6 ID	60				
Level 7	File Name	2-00020.D	Level 7 ID	cc				

Compound Name	Level 1 Response	Level 2 Response	Level 3 Response	Level 4 Response	Level 5 Response	Level 6 Response	Level 7 Response	Coeff X <sup>0</sup>	Coeff X <sup>1</sup> / ave RF	Coeff X <sup>2</sup>	R <sup>2</sup> / RSD
1 Fluorobenzene	919393	1006828	1003977	1015499	990930	980047	-1	-----	-----	-----	-----
3 di-Cl-di-F-methane	7698	51044	228452	508778	990705	1444214	-1	0.0000	0.2510	0.0000	0.0661
4 Chloromethane	8264	53373	208536	448729	864850	1174857	-1	0.0169	0.2027	0.0000	0.9966
2 F114	3209	27835	126949	275940	544934	783345	-1	0.0000	0.1313	0.0000	0.0645
5 vinyl chloride	7381	53695	219399	484855	949966	1312837	-1	0.0000	0.2424	0.0000	0.0861
6 bromomethane	3952	25743	105105	228520	411844	626111	-1	0.0000	0.1165	0.0000	0.1363
7 chloroethane	4460	34347	136103	266250	546077	758703	-1	0.0000	0.1443	0.0000	0.1208
8 tri-Cl-F-methane	11754	73985	311036	724847	1412342	1986417	-1	0.0000	0.3591	0.0000	0.1076
91 Acetonitrile X10	-1	110646	413272	845923	1639456	2365932	-1	0.0000	0.0439	0.0000	0.1416
9 acrolein X10	9511	67561	262941	513017	937791	1313901	-1	0.0306	0.0223	0.0000	0.9978
11 acetone X10	29124	106138	281400	497276	943071	1241915	-1	0.0622	0.0208	0.0000	0.9944
12 ethyl ether X5	22348	158277	587938	1189867	2188257	2883396	-1	0.0885	0.0991	0.0000	0.9929
13 11-dichloroethene	9522	62800	259067	562011	1088836	1490545	-1	0.0000	0.2867	0.0000	0.1231
14 iodomethane	7324	57536	244664	532902	1022337	1206486	-1	0.0000	0.2534	0.0000	0.1075
15 F-113	8636	49466	193654	427782	814332	1086062	-1	0.0189	0.1881	0.0000	0.9947
16 acrylonitrile X10	14700	104060	420553	831510	1601521	2352958	-1	0.0000	0.0447	0.0000	0.1361
17 carbon disulfide	23125	156993	656825	1480814	2862257	3817157	-1	0.0000	0.7288	0.0000	0.1000
94 Isopropyl Alcoholx10	4021	15273	46223	124874	265866	369178	-1	-0.0027	0.0064	0.0000	0.9954
18 methylene chloride	36501	97000	257935	510536	960233	1435510	-1	0.0322	0.2370	0.0000	0.9996
19 t-12-di-Cl-ethene	8180	61414	249312	531623	1015155	1488348	-1	0.0000	0.2701	0.0000	0.0899
20 t-Bu-Me-ether	13066	102540	420692	866584	1693079	2598506	-1	0.0000	0.4496	0.0000	0.0781
95 Tert butyl alcoholx10	-1	28855	98345	205914	482970	785022	-1	-0.0326	0.0135	0.0000	0.9918



Compound Name	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	Level 7	Coeff X^0	Coeff X^1 / ave RF	Coeff X^2	R^2 / RSD
	Response	Response	Response	Response	Response	Response	Response				
94 allyl chloride	-1	110646	413272	845923	1216384	1660968	-1	0.0000	0.3934	0.0000	0.2697
21 1,1-dichloroethane	14292	97373	381929	825889	1598207	2404444	-1	0.0000	0.4335	0.0000	0.1252
97 propionitrile	-1	4103	13637	33328	64498	101359	-1	0.0000	0.0168	0.0000	0.1453
22 c-12-di-Cl-ethene	8154	62676	253306	533706	1019103	1499328	-1	0.0000	0.2723	0.0000	0.0912
23 2,2-Dichloropropane	10809	72464	281116	589735	1098975	1539718	-1	0.0244	0.2629	0.0000	0.9982
24 Br-Cl-methane	4359	30212	117713	250220	483734	716534	-1	0.0000	0.1321	0.0000	0.1312
25 chloroform	19972	106303	398005	838697	1597118	2387736	-1	0.0108	0.4031	0.0000	0.9998
26 tetrahydrofuranX5	4965	35404	154519	318868	624422	946730	-1	0.0000	0.0328	0.0000	0.0666
98 Diisopropyl ether	17882	159533	636576	1326012	2521921	3767835	-1	0.0000	0.6674	0.0000	0.0923
27 Di-Br-F-Me (sur)	-1	59230	230740	486919	949109	1428311	-1	0.0000	0.2492	0.0000	0.1027
99 ETBE	12061	107588	486462	1064815	2106754	3231163	-1	0.0000	0.5102	0.0000	0.0820
29 1,2-Di-Cl-Et-d4 (S1)	-1	50036	187219	388784	757790	411282	-1	0.0000	0.2018	0.0000	0.1296
30 12-dichloroethane	2582	18795	70404	142937	277276	411282	-1	0.0020	0.0695	0.0000	0.9999
32 vinyl acetate X5	43949	379164	1608933	2957025	5653569	8226056	-1	0.0000	0.3120	0.0000	0.1153
92 Nitro Methane(x10)	-1	12060	47784	111334	237578	325914	-1	0.0000	0.0056	0.0000	0.0909
33 2-butanoneMEK X10	22369	123309	444332	875377	1648493	2411259	-1	0.0340	0.0406	0.0000	0.9998
93 Ethyl Acetate x2	9671	54370	220002	434881	845931	1295021	-1	0.0014	0.1088	0.0000	0.9995
34 111-trichloroethane	13204	87716	354801	785718	1524561	2222673	-1	0.0000	0.4029	0.0000	0.1136
35 11-Di-Cl-propene	7463	61583	285223	660985	1285689	1859527	-1	0.0000	0.3044	0.0000	0.0740
36 benzene	30808	233485	926403	1995763	3805709	5575015	-1	0.0000	1.0150	0.0000	0.0969
37 CCl4	11983	79844	329846	732441	1420059	2060040	-1	0.0000	0.3715	0.0000	0.1020
100 Isobutyl alcoholx10	457	10371	40745	87337	182637	287972	-1	-----	-----	-----	-----
38 thiophene	12985	115327	473132	1025220	1999457	2960047	-1	0.0000	0.5046	0.0000	0.0736
39 12-di-Cl-propane	6808	50516	204989	446632	875952	1293157	-1	0.0000	0.2271	0.0000	0.0793
40 trichloroethene	9774	67466	274815	633192	1246934	1815606	-1	0.0000	0.3164	0.0000	0.0859
41 dibromomethane	4889	32002	126997	270225	530196	793122	-1	0.0000	0.1441	0.0000	0.1368
101 TAME	9699	90788	421379	938326	1872529	2927534	-1	0.0000	0.4424	0.0000	0.1161
42 Br-di-Cl-methane	11934	72312	281223	604352	1181950	1745648	-1	0.0014	0.2967	0.0000	0.9998
43 Me-methacrylate	1794	19729	100519	228095	464768	714088	-1	-0.0114	0.1219	0.0000	0.9990
44 2-ClEt-VI-ether10	2834	31796	189485	514977	1130652	-1	-1	-0.0446	0.0290	0.0000	0.9927
45 c-13-di-Cl-propene	8596	71992	308098	676158	1328342	1977341	-1	0.0000	0.3301	0.0000	0.0559
46 t-1,3-dichloropropene	6273	54825	247619	547714	1100371	1653172	-1	0.0000	0.2625	0.0000	0.0800
47 Chlorobezene-d5	683445	775455	774184	772935	739886	736062	-1	0.0000	1.0000	0.0000	0.0000


Compound Name	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	Level 7	Coeff X <sup>1</sup> 0	Coeff X <sup>1</sup> 1 / ave RF	Coeff X <sup>2</sup> 2	R <sup>2</sup> / RSD
	Response	Response	Response	Response	Response	Response	Response				
48 112-tri-Cl-Et	5902	42713	164770	343401	662895	997315	-1	0.0000	0.2413	0.0000	0.1317
49 13-di-Cl-propane	8941	66977	268452	552557	1062190	1558760	-1	0.0000	0.3807	0.0000	0.1091
50 Et methacrylate	3865	41714	210769	443099	890456	1418605	-1	-0.0322	0.3197	0.0000	0.9978
51 di-Br-Cl-methane	8661	52843	213283	456818	899440	1365305	-1	-0.0111	0.3087	0.0000	0.9994
52 bromoform	4560	29809	123106	263988	534402	823804	-1	0.0000	0.1852	0.0000	0.1170
53 1,4-dichlorobutane-2	8296	61397	241554	510059	1005306	1519089	-1	0.0000	0.3544	0.0000	0.1053
54 MIBK	2701	22334	103475	222364	457366	733371	-1	0.0000	0.1456	0.0000	0.0889
55 toluene-d8	27570	211476	874470	1923324	3719816	5400714	-1	0.0000	1.2603	0.0000	0.0678
56 toluene	29681	252340	1018191	2227432	4284454	6235319	-1	0.0000	1.4484	0.0000	0.0698
57 2-hexanone X5	10224	84522	356146	728526	1453530	2205707	-1	0.0000	0.0989	0.0000	0.0595
58 12-dibromoethane	5621	39459	162435	343609	688415	1038913	-1	0.0000	0.2381	0.0000	0.0968
59 tetra-Cl-ethene	10167	72027	292262	659769	1256084	1800306	-1	0.0000	0.4328	0.0000	0.0968
60 chlorobenzene	26600	179300	691236	1494861	2837497	4059222	-1	0.0338	0.9255	0.0000	0.9991
61 1112-tetra-Cl-Et	9159	63898	245258	525072	1031299	1537036	-1	0.0000	0.3686	0.0000	0.1347
62 1,4-Dichlorobenzene-d4	358277	419640	407774	393961	367099	365124	-1	0.0000	1.0000	0.0000	0.0000
63 1-chlorohexane	2893	25946	118729	280119	548810	784184	-1	0.0000	0.3261	0.0000	0.1294
64 Et-Bz	33015	273886	1133719	2529977	4833949	6913463	-1	0.0000	3.1290	0.0000	0.0601
65 m/p-Xylenes X2	49281	436018	1773476	3842318	7112016	9936549	-1	0.0000	2.3654	0.0000	0.0637
66 styrene	15818	166023	695954	1498467	2811895	3981902	-1	0.0000	1.7985	0.0000	0.1032
67 o-xylene	21010	210456	917264	1990843	3763083	5341093	-1	0.0000	2.3732	0.0000	0.0983
68 1122-Tetra-Cl-Et	7086	48249	186045	374484	736112	1101133	-1	0.0000	0.5283	0.0000	0.1434
69 123-tri-Cl-Pr	1994	14801	56224	114784	222436	332760	-1	0.0000	0.1581	0.0000	0.1176
70 4-Br-1-F-Bz (S3)	10243	73535	287803	629095	1208574	1766234	-1	0.0000	0.8271	0.0000	0.1001
71 isopropylbenzene	24316	252585	1164869	2648278	5083237	7208570	-1	0.0000	3.0403	0.0000	0.1458
72 bromobenzene	9030	73980	293172	635461	1236729	1774887	-1	0.0000	0.8166	0.0000	0.0673
92 t-1,4-dichloro-2-butene	406	6524	30509	64587	137632	207953	-1	-0.0118	0.0961	0.0000	0.9978
73 n-propylbenzene	8157	83853	353478	802663	1558540	2210026	-1	0.0000	0.9523	0.0000	0.1210
74 2-Cl-Toluene	8123	74427	309252	685694	1328259	1912837	-1	0.0000	0.8415	0.0000	0.0790
75 4-Cl-Toluene	9172	80121	308786	677984	1291985	1819259	-1	0.0000	0.8560	0.0000	0.0752
76 135-tri-Me-Benzene	21830	240336	1005234	2217776	4186569	5867539	-1	0.0000	2.6173	0.0000	0.1238
77 4-iso-Pr-toluene	24508	264794	1111631	2489320	4727712	6567533	-1	0.0000	2.9230	0.0000	0.1239
78 124-tri-Me-Benzene	24365	252796	1026195	2248874	4305294	6074118	-1	0.0000	2.7257	0.0000	0.1034
79 tert-butylbenzene	21932	200692	1030129	2077031	4034706	5816456	-1	0.0000	2.4995	0.0000	0.1024

80 13-DCB	21374	158442	605258	1313556	2467081	3488098	-1	0.0000	1.7167	0.0000	0.1095
81 sec-butylbenzene	29181	304851	1334960	3039109	5779243	8084394	-1	0.0000	3.5174	0.0000	0.1295
82 14-DCB	24079	155998	594167	1295125	2472135	3533637	-1	-0.0003	1.6325	0.0000	0.9988
83 Cl-benzyI	1764	13306	63403	132793	265795	361085	-1	0.0000	0.1654	0.0000	0.0541
84 12-DCB	18942	145496	540526	1153351	2171646	3083911	-1	0.0000	1.5286	0.0000	0.1167
85 n-butylbenzene	5679	66251	298215	689097	1335543	1846727	-1	-0.0178	0.8660	0.0000	0.9968
86 12-dIBr-2-Cl-Pra	1180	8757	37194	80335	173925	263112	-1	0.0000	0.1076	0.0000	0.1009
87 124-tri-Cl-Bz	9061	77700	360446	838928	1658990	2390948	-1	0.0000	0.9898	0.0000	0.1216
88 naphthalene	23839	152715	581293	1300980	2689379	4011635	-1	0.0000	1.7961	0.0000	0.1450
89 hx-Cl-butadiene	6922	52135	209577	472099	923440	1288580	-1	0.0000	0.5992	0.0000	0.0774
90 123-Tri-Cl-Bz	9124	73440	317007	719921	1423460	2068944	-1	0.0000	0.8881	0.0000	0.0786

1535

Data File : C:\MSDCHEM\1\DATA\03G3570\G3570P01.D  
 Acq On : 6 Aug 2003 10:07 am  
 Sample : #03g3570,w 50ng  
 Misc :  
 MS Integration Params: Lscint.P  
 Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P &h Lab\*\* EPA 524.2

Vial: 1  
 Operator: zou  
 Inst : GCMS-A  
 Multiplr: 1.00

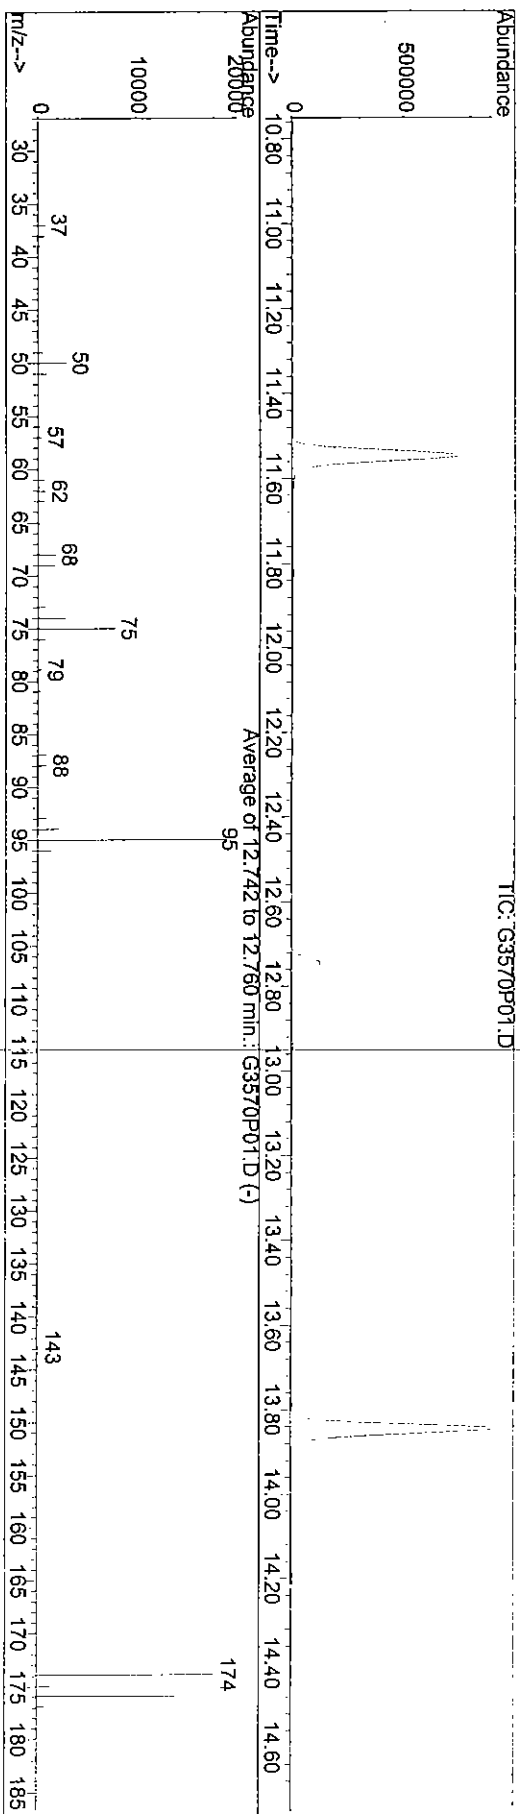

Spectrum Information: Average of 12.742 to 12.760 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	15.1	2944	PASS
75	95	30	60	40.6	7912	PASS
95	95	100	100	100.0	19475	PASS
96	95	5	9	7.0	1357	PASS
173	174	0.00	2	0.4	68	PASS
174	95	50	100	93.6	18225	PASS
175	174	5	9	7.8	1416	PASS
176	174	95	101	98.7	17985	PASS
177	176	5	9	7.8	1394	PASS

FORM-5A

Applied P & Ch Laboratory

Volatile Organic Instrument Performance Check for Method 524.2

Bromofluorobenzene (BFB ), Part II

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 034389
Project ID: JPL	BFB Inj. Date: 08/06/03	Batch No: 03G3570
Project No: 04-4428.10	BFB Inj. Time: 10:07	Sequence No: 03G3570
Data File Name: G3570P01	Instrument ID: A	GC Column: HP-VOC
	Heated Purge: (Y/N) N	Column ID: 0.20 mm

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS AND STANDARDS:

#	Client Sample No	Lab Sample ID	Data File Name	Date Analyzed	Time Analyzed
1	03G3570-CCV-01	03G3570-CCV-01	G3570Q01	08/06/03	10:32
2	03G3570-LCS-01	03G3570-LCS-01	G3570L01	08/06/03	10:58
3	MW-19-2MS	03-4406-10MS	G3570M01	08/06/03	11:24
4	MW-19-2MSD	03-4406-10MSD	G3570N01	08/06/03	11:50
5	03G3570-MB-01	03G3570-MB-01	G3570K01	08/06/03	13:08
6	TB-1-7-29-03	03-4389-7	4389-07	08/06/03	13:34
7	EB-1-7-29-03	03-4389-1	4389-01	08/06/03	14:01
8	MW-21-1	03-4389-2	4389-02	08/06/03	14:53
9	MW-21-2	03-4389-3	4389-03	08/06/03	15:19
10	MW-21-3	03-4389-4	4389-04	08/06/03	15:46
11	MW-21-4	03-4389-5	4389-05	08/06/03	16:12
12	MW-21-5	03-4389-6	4389-06	08/06/03	16:39
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					

# Continuing Calibration Concentration Summary

Data File G3570Q01  
Method File E524A002

<u>Compound Name</u>	<u>Amount</u>	<u>Actual</u>	<u>Units</u>	<u>%Dev</u>	<u>Target Response</u>
1 Fluorobenzene	10	10.00	ppb	0.00	790353
3 di-Cl-di-F-methane	20	18.07	ppb	9.64	358542
4 Chloromethane	20	16.59	ppb	17.06	279095
2 F114	20	19.23	ppb	3.86	199480
5 vinyl chloride	20	17.96	ppb	10.18	344173
6 bromomethane	20	17.74	ppb	11.30	163266
7 chloroethane	20	18.77	ppb	6.14	214063
8 tri-Cl-F-methane	20	18.85	ppb	5.73	535063
91 Acetonitrile X10	200	176.79	ppb	11.60	613006
9 acrolein X10	200	204.92	ppb	2.46	385070
11 acetone X10	200	347.18	ppb	73.59	620100
12 ethyl ether X5	100	104.62	ppb	4.62	889704
13 11-dichloroethane	20	18.87	ppb	5.66	427487
14 Iodomethane	20	10.38	ppb	48.08	207968
15 F-113	20	21.23	ppb	6.15	330645
16 acrylonitrile X10	200	173.06	ppb	13.47	611466
17 carbon disulfide	20	18.48	ppb	7.60	1064381
94 Isopropyl Alcoholx10	200	176.36	ppb	11.82	87379
18 methylene chloride	20	18.04	ppb	9.81	363409
19 t-12-di-Cl-ethene	20	18.24	ppb	8.79	389462
20 t-Bu-Me-ether	20	18.46	ppb	7.71	655909
95 Tert butyl alcoholx10	200	175.44	ppb	12.28	161293
94 allyl chloride	20	19.72	ppb	1.42	613006
21 11-dichloroethane	20	17.50	ppb	12.49	599613
97 propionitrile	20	20.10	ppb	0.50	26651
22 c-12-di-Cl-ethene	20	18.43	ppb	7.87	396616
23 22-Dichloropropane	20	24.81	ppb	24.04	534764
24 Br-Cl-methane	20	17.99	ppb	10.06	187762
25 chloroform	20	19.68	ppb	1.60	635499
26 tetrahydrofuranX5	100	87.94	ppb	12.06	228264
98 Diisopropyl ether	20	17.94	ppb	10.28	946543
27 Di-Br-F-Me (surr)	20	18.80	ppb	5.98	370366
99 ETBE	20	19.53	ppb	2.35	787537
29 1,2-Di-Cl-Et-d4 (S1)	20	18.78	ppb	6.09	299618
30 12-dichloroethane	20	20.11	ppb	0.54	112076
32 vinyl acetate X5	100	97.31	ppb	2.69	2399525
92 Nitro Methane(x10)	200	169.16	ppb	15.42	74246
33 2-butanoneMEK X10	200	230.39	ppb	15.19	766132
93 Ethyl Acetate x2	40	36.69	ppb	8.27	316586
34 111-trichloroethane	20	18.76	ppb	6.19	597390
35 11-Di-Cl-propene	20	20.32	ppb	1.60	488889
36 benzene	20	18.15	ppb	9.26	1455820
37 CCl4	20	19.47	ppb	2.64	571650

<u>Compound Name</u>	<u>Amount</u>	<u>Actual</u>	<u>Units</u>	<u>%Dev</u>	<u>Target Response</u>
100 Isobutyl alcoholx10	200	170.18	ppb	14.91	61706
38 thiophene	20	19.06	ppb	4.69	760139
39 12-di-Cl-propane	20	17.94	ppb	10.30	322021
40 trichloroethene	20	18.93	ppb	5.36	473283
41 dibromomethane	20	17.86	ppb	10.68	203405
101 TAME	20	20.01	ppb	0.06	699756
42 Br-di-Cl-methane	20	19.39	ppb	3.03	455934
43 Me-methacrylate	20	17.50	ppb	12.48	159581
44 2-ClEt-Vi-ether10	200	116.80	ppb	41.60	232170
45 c-13-di-Cl-propene	20	19.78	ppb	1.09	516018
46 t-1,3-dichloropropene	20	20.36	ppb	1.81	422370
47 Chlorobezene-d5	10	10.00	ppb	0.00	610095
48 112-tri-Cl-Et	20	17.61	ppb	11.95	259291
49 13-di-Cl-propane	20	17.77	ppb	11.16	412652
50 Et methacrylate	20	18.39	ppb	8.05	338969

<u>Compound Name</u>	<u>Amount</u>	<u>Actual</u>	<u>Units</u>	<u>%Dev</u>	<u>Target Response</u>
51 di-Br-Cl-methane	20	18.92	ppb	5.41	349560
52 bromoform	20	17.82	ppb	10.92	201352
53 1,4-dichlorobutane-2	20	17.18	ppb	14.10	371406
54 MIBK	20	17.43	ppb	12.86	154861
55 toluene-d8	20	18.67	ppb	6.63	1435838
56 toluene	20	18.71	ppb	6.47	1652885
57 2-hexanone X5	100	94.13	ppb	5.87	567671
58 12-dibromoethane	20	17.75	ppb	11.27	257766
59 tetra-Cl-ethene	20	18.83	ppb	5.84	497251
60 chlorobenzene	20	19.73	ppb	1.37	1134367
61 1112-tetra-Cl-Et	20	17.91	ppb	10.46	402707
62 1,4-Dichlorobenzene-d4	10	10.00	ppb	0.00	311119
63 1-chlorohexane	20	21.04	ppb	5.20	213480
64 Et-Bz	20	19.58	ppb	2.10	1906033
65 m/p-Xylenes X2	40	39.84	ppb	0.40	2931988
66 styrene	20	20.34	PPB	1.72	1138373
67 o-xylene	20	20.49	ppb	2.47	1513242
68 1122-Tetra-Cl-Et	20	17.06	ppb	14.68	280470
69 123-tri-Cl-Pr	20	17.80	ppb	11.00	87570
70 4-Br-1-F-Bz (S3)	20	18.71	ppb	6.45	481440
71 isopropylbenzene	20	21.24	ppb	6.21	2009263
72 bromobenzene	20	19.03	ppb	4.85	483453
92 t-1,4-dichloro-2-butene	20	19.11	ppb	4.44	53439
73 n-propylbenzene	20	20.87	ppb	4.36	618383
74 2-Cl-Toluene	20	20.01	ppb	0.03	523766
75 4-Cl-Toluene	20	19.77	ppb	1.17	526408
76 135-tri-Me-Benzene	20	21.03	ppb	5.14	1712315
77 4-iso-Pr-toluene	20	21.30	ppb	6.52	1937365
78 124-tri-Me-Benzene	20	20.46	ppb	2.32	1735411
79 tert-butylbenzene	20	20.59	ppb	2.95	1601166
80 13-DCB	20	18.95	ppb	5.27	1011879
81 sec-butylbenzene	20	21.32	ppb	6.60	2333010

82 14-DCB	20	19.61	ppb	1.97	995672
83 Cl-benzyl	20	26.70	ppb	33.52	137437
84 12-DCB	20	18.62	ppb	6.92	885389
85 n-butylbenzene	20	20.33	ppb	1.66	542253
86 12-diBr-2-Cl-Pra	20	18.29	ppb	8.57	61240
87 124-tri-Cl-Bz	20	21.43	ppb	7.13	659771
88 naphthalene	20	17.81	ppb	10.94	995381
89 hx-Cl-butadiene	20	19.80	ppb	1.02	369056
90 123-Tri-Cl-Bz	20	20.10	ppb	0.51	555466

Average D % 8.5139949



Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\03G3570\G3570Q01.D  
 Acq On : 6 Aug 2003 10:32 am  
 Sample : f=1  
 Misc :  
 MS Integration Params: Lscint.p

Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P & Sch Lab\*\* EPA 524.2  
 Last Update : Thu Jul 24 12:40:35 2003  
 Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	AvgRRF	CCRF	%Dev	Area#	Dev(min)
1 I	1.000	1.000	0.0	78	0.02
2	0.251	0.227	9.6	70	0.04
3 p	0.235	0.177	24.7#	62	0.04
4	0.131	0.126	3.8	72	0.04
5 C	0.242	0.218	9.9	71	0.04
6	0.116	0.103	11.2	71	0.04
7	0.144	0.135	6.2	80	0.03
8	0.359	0.338	5.8	74	0.04
9	0.044	0.039	11.4	72	0.03
10	0.028	0.024	14.3	75	0.04
11	0.043	0.039	9.3	125	0.04
12	0.127	0.113	11.0	75	0.04
13 M, C	0.287	0.270	5.9	76	0.04
14	0.253	0.132	47.8#	39#	0.04
15	0.225	0.209	7.1	77	0.04
16	0.045	0.039	13.3	74	0.04
17	0.729	0.673	7.7	72	0.04
18	0.008	0.006	25.0#	70	0.10
19	0.467	0.230	50.7#	71	0.04
20	0.270	0.246	8.9	73	0.04
21	0.450	0.415	7.8	76	0.04
22	0.012	0.010	16.7	78	0.11
23	0.393	0.388	1.3	72	0.03
24 p	0.433	0.379	12.5	73	0.03
25	0.017	0.017	0.0	80	0.03
26	0.272	0.251	7.7	74	0.02

(#) = Out of Range  
 G3570Q01.D E524A002.M Thu Aug 07 16:13:47 2003

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\03G3570\G3570Q01.D  
 Acq On : 6 Aug 2003 10:32 am  
 Sample : f=1  
 Misc :  
 MS Integration Params: Lscint.p

Vial: 2  
 Operator: zou  
 Inst : GCMS-A  
 Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P &h Lab\*\* EPA 524.2  
 Last Update : Thu Jul 24 12:40:35 2003  
 Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	AVGRF	CCRF	%Dev Area	% Dev (min)
27 22-Dichloropropane	0.310	0.338	-9.0	91 0.03
28 Br-Cl-methane	0.132	0.119	9.8	75 0.02
29 C 25 chloroform	0.478	0.402	15.9	76 0.03
30 26 tetrahydrofuranX5	0.033	0.029	12.1	72 0.03
31 98 Disopropyl ether	0.667	0.599	10.2	71 0.02
32 S 27 Di-Br-F-Me (surr)	0.249	0.234	6.0	76 0.03
33 99 ETBE	0.510	0.498	2.4	74 0.02
34 S 29 1,2-Di-Cl-Et-d4 (S1)	0.202	0.190	5.9	77 0.03
35 30 12-dichloroethane	0.078	0.071	9.0	78 0.02
36 32 vinyl acetate X5	0.312	0.304	2.6	81 0.03
37 92 Nitro Methane(x10)	0.006	0.005	16.7	67 0.04
38 33 2-butanoneMEK X10	0.052	0.048	7.7	88 0.03
39 93 Ethyl Acetate X2	0.124	0.100	19.4	73 0.02
40 34 111-trichloroethane	0.403	0.378	6.2	76 0.02
41 35 11-Di-Cl-propene	0.304	0.309	-1.6	74 0.02
42 M 36 benzene	1.015	0.921	9.3	73 0.02
43 37 CCl4	0.371	0.362	2.4	78 0.02
44 100 Isobutyl alcoholX10	0.004	0.004	0.0	71 -0.20
45 38 thiophene	0.505	0.481	4.8	74 0.02
46 C 39 12-di-Cl-propane	0.227	0.204	10.1	72 0.02
47 M 40 trichloroethene	0.316	0.299	5.4	75 0.02
48 41 dibromomethane	0.144	0.129	10.4	75 0.01
49 101 TAME	0.442	0.443	-0.2	75 0.02
50 42 Br-di-Cl-methane	0.327	0.288	11.9	75 0.01
51 43 Me-methacrylate	0.102	0.101	1.0	70 0.01
52 44 2-ClEt-VI-ether10	0.020	0.015	25.0#	45# 0.01

(#) = Out of Range

G3570Q01.D E524A002.M

Thu Aug 07 16:13:48 2003

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\03G3570\G3570Q01.D Vial: 2  
 Acq On : 6 Aug 2003 10:32 am Operator: zou  
 Sample : f=1 Inst : GCMS-A  
 Misc : Multiplr: 1.00  
 MS Integration Params: Lscint.p

Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P & Ch Lab\*\* EPA 524.2  
 Last Update : Thu Jul 24 12:40:35 2003  
 Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	AVGRF	CCRF	%Dev Area	% Dev (min)				
53	45	c-13-di-Cl-propene	0.330	0.326	1.2	76	0.01	
54	46	t-1,3-dichloropropene	0.262	0.267	-1.9	77	0.00	
55	I	47	Chlorobezene-d5	1.000	1.000	0.0	79	0.00
56	48	112-tri-Cl-Et	0.241	0.213	11.6	76	0.00	
57	49	13-di-Cl-propane	0.381	0.338	11.3	75	0.01	
58	50	Et methacrylate	0.273	0.278	-1.8	76	0.00	
59	51	di-Br-Cl-methane	0.325	0.286	12.0	77	0.00	
60	P	52	bromoform	0.185	0.165	10.8	76	0.00
61	53	1,4-dichlorobutane-2	0.354	0.304	14.1	73	0.00	
62	54	MTBK	0.146	0.127	13.0	70	0.00	
63	s	55	toluene-d8	1.260	1.177	6.6	75	0.01
64	M,C	56	toluene	1.448	1.355	6.4	74	0.00
65	57	2-hexanone X5	0.099	0.093	6.1	78	0.00	
66	58	12-dibromoethane	0.238	0.211	11.3	75	0.00	
67	59	tetra-Cl-ethene	0.433	0.408	5.8	75	0.00	
68	M,P	60	chlorobenzene	1.032	0.930	9.9	76	0.00
69	61	1112-tetra-Cl-Et	0.369	0.330	10.6	77	0.00	
70	I	62	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	79	0.00
71	63	1-chlorohexane	0.326	0.343	-5.2	76	0.00	
72	C	64	Et-Bz	3.129	3.063	2.1	75	0.00
73	65	m/p-Xylenes X2	2.365	2.356	0.4	76	0.00	
74	66	styrene	1.798	1.829	-1.7	76	0.00	
75	67	o-xylene	2.373	2.432	-2.5	76	0.00	
76	p	68	1122-Tetra-Cl-Et	0.528	0.451	14.6	75	0.00

(#) = Out of Range  
 G3570Q01.D E524A002.M Thu Aug 07 16:13:49 2003

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\03G3570\G3570Q01.D Vial: 2  
 Acq On : 6 Aug 2003 10:32 am Operator: zou  
 Sample : f=1 Inst : GCMS-A  
 Misc : Multiplr: 1.00  
 MS Integration Params: Iscint.p

Method : C:\MSDCHEM\1\METHODS\E524A002.M (RTE Integrator)  
 Title : \*\*Applied P & Ch Lab\*\* EPA 524.2  
 Last Update : Thu Jul 24 12:40:35 2003  
 Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	AVGRF	CCRF	%Dev	Area%	Dev(min)		
77	69	123-tri-Cl-Pr	0.158	0.141	10.8	76	0.00
78	S	70 4-Br-1-F-Bz (S3)	0.827	0.774	6.4	77	0.00
79		71 isopropylbenzene	3.040	3.229	-6.2	76	0.00
80		72 bromobenzene	0.817	0.777	4.9	76	0.00
81		92 t-1,4-dichloro-2-butene	0.077	0.086	-11.7	83	0.00
82		73 n-propylbenzene	0.952	0.994	-4.4	77	0.00
83		74 2-Cl-Toluene	0.841	0.842	-0.1	76	0.00
84		75 4-Cl-Toluene	0.856	0.846	1.2	78	0.00
85		76 135-tri-Me-Benzene	2.617	2.752	-5.2	77	0.00
86		77 4-Iso-Pr-toluene	2.923	3.114	-6.5	78	0.00
87		78 124-tri-Me-Benzene	2.726	2.789	-2.3	77	0.00
88		79 tert-butylbenzene	2.499	2.573	-3.0	77	0.00
89		80 13-DCB	1.717	1.626	5.3	77	0.00
90		81 sec-butylbenzene	3.517	3.749	-6.6	77	0.00
91		82 14-DCB	1.749	1.600	8.5	77	0.00
92		83 Cl-benzy1	0.165	0.221	-33.9#	103	0.00
93		84 12-DCB	1.529	1.423	6.9	77	0.00
94		85 n-butylbenzene	0.779	0.871	-11.8	79	0.00
95		86 12-diBr-2-Cl-Pra	0.108	0.098	9.3	76	0.00
96		87 124-tri-Cl-Bz	0.990	1.060	-7.1	79	0.00
97		88 naphthalene	1.796	1.600	10.9	77	0.00
98		89 hx-Cl-butadiene	0.599	0.593	1.0	78	0.00
99		90 123-Tri-Cl-Bz	0.888	0.893	-0.6	77	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 0  
 G3570Q01.D E524A002.M Thu Aug 07 16:13:49 2003

FORM-8A

Applied P & Ch Laboratory

Internal Standard Area and RT Summary for Method 524.2

Client Name: GEOFON, Inc. Contract No: Lab Code: APCL  
 Case No: SAS No: Service ID: 034389  
 Project ID: JPL Project No: 04-4428.10 Sample Matrix: Water  
 CCV Data File: G3570Q01 Instrument ID: A  
 Batch No: 03G3570

#	Client Sample No	Lab Sample ID	Analysis Date & Time	IS-1		IS-2		IS-3	
				Area #	RT #	Area #	RT #	Area #	RT #
12 Hour CCV STD			08/06/03 10:32	790353	7.65	610095	11.55	311119	13.85
CCV Upper Limit				1580706	8.15	1220190	12.05	622238	14.35
CCV Lower Limit				395176	7.15	305047	11.05	155559	13.35
1	03G3570-LCS-01	03G3570-LCS-01	08/06/03 10:58	829058	7.65	648481	11.54	336853	13.84
2	MW-19-2MS	03-4406-10MS	08/06/03 11:24	818407	7.65	629647	11.54	320116	13.84
3	MW-19-2MSD	03-4406-10MSD	08/06/03 11:50	849231	7.65	658725	11.54	333596	13.84
4	03G3570-MB-01	03G3570-MB-01	08/06/03 13:08	728257	7.65	583860	11.55	305134	13.85
5	TB-1-7-29-03	03-4389-7	08/06/03 13:34	726679	7.65	582655	11.54	302469	13.85
6	EB-1-7-29-03	03-4389-1	08/06/03 14:01	721013	7.65	579030	11.55	300277	13.85
7	MW-21-1	03-4389-2	08/06/03 14:53	730016	7.65	586053	11.54	304526	13.85
8	MW-21-2	03-4389-3	08/06/03 15:19	723916	7.65	586397	11.55	301898	13.85
9	MW-21-3	03-4389-4	08/06/03 15:46	725098	7.65	583534	11.55	302576	13.85
10	MW-21-4	03-4389-5	08/06/03 16:12	718013	7.65	582910	11.54	301795	13.85
11	MW-21-5	03-4389-6	08/06/03 16:39	716053	7.65	585291	11.55	299175	13.85
12									
13									
14									
15									
16									
17									
18									
19									
20									
21									
22									

IS-1 = FLUOROBENZENE  
 IS-2 = CHLOROBENZENE-D5  
 IS-3 = 1,4-DICHLOROBENZENE-D4

Area Upper Limit = +100% of CCV internal standard area  
 Area Lower Limit = - 50% of CCV internal standard area  
 RT Upper Limit = +0.50 minutes of CCV internal standard RT  
 RT Lower Limit = - 0.50 minutes of CCV internal standard RT

# Column used to flag values outside QC limits with an asterisk.  
 \* Values outside of QC limits

United P & Ch Laboratory  
 Magnolia Ave. Chino CA 91710  
 (909) 590-1828 Fax: (909) 590-1498

# VOC Analysis General Logbook

Case # 0383570 Batch # 0383570 Matrix: W Date: 08/06/03 Analyst: Zou

IS/Surrogate: GC-1514/1515 Methanol(mark-M): \_\_\_\_\_ PEG (mark-PEG): \_\_\_\_\_ Defoaming(mark-DF): \_\_\_\_\_

Initial Batch:  Initial Batch;  Middle Batch;  Final Batch.  Internal Study Datafile Path: \_\_\_\_\_

Type	Sample ID	Method	V/X=f <sub>1</sub>	V <sub>i</sub> /V <sub>i</sub> =f <sub>2</sub>	V <sub>spg</sub> /V <sub>inj</sub> =f <sub>3</sub>	F	A-#	Datafile	Note	pH
SP	G357001	ES24A 202	25/25 = 1	/ =	/ =	1		G357001	08/06/03	10:07 am
CCV	Q01		/ =	/ =	/ =			Q01	GC15524	
LCS	L01		/ =	/ =	/ =			L01		
MS	M01		/ =	/ =	/ =			M01	\$4406-10	<2
MSD	N01		/ =	/ =	/ =			N01	↓	↓
MB	✓ K01		/ =	/ =	/ =			✓ K01		
Sample	4389-07		/ =	/ =	/ =			4389-07	#b	<2
	↓ 01		/ =	/ =	/ =			↓ 01	eb	
	4406-10		/ =	/ =	/ =			4406-10	ms	
	4389-02		/ =	/ =	/ =			4389-02		
	03		/ =	/ =	/ =			03		
	04		/ =	/ =	/ =			04		
	05		/ =	/ =	/ =			05		
	✓ 06		/ =	/ =	/ =			↓ 06		
	4406-01		/ =	/ =	/ =			4406-01		
	03		/ =	/ =	/ =			03		
	04		/ =	/ =	/ =			04		
	05		/ =	/ =	/ =			05		
	06		/ =	/ =	/ =			06		
	07		/ =	/ =	/ =			07		
	08		/ =	/ =	/ =			08		
	09		/ =	/ =	/ =			09		
	11		/ =	/ =	/ =			11		
	12		/ =	/ =	/ =			12		
↓	↓ 13	↓	↓	↓	↓	↓		↓ 13		↓

*[Handwritten signature]*  
 08/11/03

type	Op #	STD Lot #	C <sub>std</sub> (ng/μL) × V <sub>std</sub> (μL) / X(g or mL) = T	Op #	STD Lot #	C <sub>std</sub> (ng/μL) × V <sub>std</sub> (μL) / X(g or mL) = T
/LCS	2603	GC-15524	200 × 25 / X = ppb		GC-	x / X = ppb
/MSD	2604/2605	GC-	x / X = ppb		GC-	x / X = ppb

Note/Anomaly:

Applied P & Ch Laboratory

VOC Analysis General Logbook

13760 Magnolia Ave. Chino CA 91710  
Tel: (909) 590-1828 Fax: (909) 590-1498

Sequence # 0393415 Batch # 0393415 Matrix: W Date: 07/24/03 Analyst: Zou  
Lot #: IS/Surrogate: GC-1544/1515 Methanol(mark-M): \_\_\_\_\_ PEG (mark-PEG): \_\_\_\_\_ Defoaming(mark-DF): \_\_\_\_\_

Calib. + Ini. Batch  Initial Batch;  Middle Batch;  Final Batch.  Internal Study Datafile Path: \_\_\_\_\_

Op. #	Type	Sample ID	Method	V/X=f <sub>1</sub>	V <sub>1</sub> /V <sub>i</sub> =f <sub>2</sub>	V <sub>spg</sub> /V <sub>inj</sub> =f <sub>3</sub>	F	A-#	Datafile	Note	pH
2217	SP	G3415 P01	E524A 02	25/25 = 1	/ =	/ =	1		G3415 P01	07/24/03	7.08
2218	Calib.	02-0003		/ =	/ =	/ =			02-0003	0.3 ppb	
2219		0002A		/ =	/ =	/ =			0002A	2 ppb	
2220		00010		/ =	/ =	/ =			00010	10 ppb	
2221		00020		/ =	/ =	/ =			00020	20 ppb	
2222		00040		/ =	/ =	/ =			00040	40 ppb	
2223		00060		/ =	/ =	/ =			00060	60 ppb	
2224				/ =	/ =	/ =					
2225				/ =	/ =	/ =					
2226				/ =	/ =	/ =					
2227				/ =	/ =	/ =					
2228				/ =	/ =	/ =					
2229				/ =	/ =	/ =					
2230				/ =	/ =	/ =					
2231				/ =	/ =	/ =					
2232				/ =	/ =	/ =					
2233				/ =	/ =	/ =					
2234				/ =	/ =	/ =					
2235				/ =	/ =	/ =					
2236				/ =	/ =	/ =					
2237				/ =	/ =	/ =					
2238				/ =	/ =	/ =					
2239				/ =	/ =	/ =					
2240				/ =	/ =	/ =					
2241				/ =	/ =	/ =					
2242				/ =	/ =	/ =					
2243				/ =	/ =	/ =					
2244				/ =	/ =	/ =					
2245				/ =	/ =	/ =					
2246				/ =	/ =	/ =					
2247				/ =	/ =	/ =					
2248				/ =	/ =	/ =					

*Dr*  
*07/23/03*

Type	Op #	STD Lot #	C <sub>std</sub> (ng/μL) × V <sub>std</sub> (μL) / X (g or mL) = T	Op #	STD Lot #	C <sub>std</sub> (ng/μL) × V <sub>std</sub> (μL) / X (g or mL) = T
LCS/LCSD		GC-	x / X = ppb		GC-	x / X = ppb
MS/MSD		GC-	x / X = ppb		GC-	x / X = ppb

Footnote/Anomaly: \_\_\_\_\_

Level C Data Package Deliverables

# Wet Chemistry



Applied P & Ch Laboratory



Applied P & Ch Laboratory  
**Wet Analysis Results for Method 7196**

Client Name: GEOFON, Inc.                      Project No: 04-4428.10                      Anal. Method 7196  
 Project ID: JPL                                      Service ID: 34389                              Collected by:

Component Name: Chromium (VI)  
 CAS No: 1333-82-0

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-4389-1	EB-1-7-29-03	Water	07/29/03	07/29/03	07/29/03	03W3899	mg/L	0.01	<0.01	U
03-4389-2	MW-21-1	Water	07/29/03	07/29/03	07/29/03	03W3899	mg/L	0.01	<0.01	U
03-4389-3	MW-21-2	Water	07/29/03	07/29/03	07/29/03	03W3899	mg/L	0.01	<0.01	U
03-4389-4	MW-21-3	Water	07/29/03	07/29/03	07/29/03	03W3899	mg/L	0.01	<0.01	U
03-4389-5	MW-21-4	Water	07/29/03	07/29/03	07/29/03	03W3899	mg/L	0.01	<0.01	U
03-4389-6	MW-21-5	Water	07/29/03	07/29/03	07/29/03	03W3899	mg/L	0.01	<0.01	U
03W3899-MB-01	03W3899-MB-01	Water	07/29/03	07/29/03	07/29/03	03W3899	mg/L	0.01	<0.01	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

Applied P & Ch Laboratory  
**Wet Analysis Results for Method 314.0**

Client Name: GEOFON, Inc.                      Project No: 04-4428.10                      Anal. Method 314.0  
 Project ID: JPL                                      Service ID: 34389                              Collected by:

Component Name: Perchlorate  
 CAS No:

Lab ID	Sample ID	Matrix	Coll. Date	Rcv Date	Anal. Date	Batch	Unit	RL	Result	Q
03-4389-1	EB-1-7-29-03	Water	07/29/03	07/29/03	07/31/03	03W3913	µg/L	4	<4	U
03-4389-2	MW-21-1	Water	07/29/03	07/29/03	07/31/03	03W3913	µg/L	4	5.2	
03-4389-3	MW-21-2	Water	07/29/03	07/29/03	07/31/03	03W3913	µg/L	4	2.1	B
03-4389-4	MW-21-3	Water	07/29/03	07/29/03	07/31/03	03W3913	µg/L	4	2.7	B
03-4389-5	MW-21-4	Water	07/29/03	07/29/03	07/31/03	03W3913	µg/L	4	2.7	B
03-4389-6	MW-21-5	Water	07/29/03	07/29/03	07/31/03	03W3913	µg/L	4	2.6	B
03W3913-MB-01	03W3913-MB-01	Water	07/31/03	07/31/03	07/31/03	03W3913	µg/L	4	<4	U

Not Detected is shown as PQL, with dilution and moisture corrected if applicable.

Note: Q - Qualifier.

Qualifier: U - Not Detected or less than MDL

B - Less than RL (PQL, EQL or CRDL), but greater than MDL.

FORM-3  
Applied P & Ch Laboratory

**Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 314.0**

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34389
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W3913	
LCS Filename: -	Date Analyzed: 073103	Time Analyzed:
LCSD Filename: -	Date Analyzed: 073103	Time Analyzed:

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
PERCHLORATE	µg/L	50	0	51.0	102	80-120
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	LCSD Concentration	LCSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
PERCHLORATE	µg/L	50	52.7	105	3	20	80-120
# of Out-of-control				0	0		

# Column to be used to flag recovery and RPD values:

\* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: \_\_\_\_\_  
\_\_\_\_\_

FORM-3

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 314.0

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34389
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W3913	
MS Filename: -	Date Analyzed: 073103	Time Analyzed:
MSD Filename: -	Date Analyzed: 073103	Time Analyzed:
MS Sample No: MW-19-2	Sample Lab ID: 03-4406-10	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
PERCHLORATE	µg/L	50	3.6	60.5	114	75-125
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
PERCHLORATE	µg/L	50	59.7	112	2	20	75-125
# of Out-of-control				0	0		

# Column to be used to flag recovery and RPD values:

\* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: \_\_\_\_\_  
 \_\_\_\_\_

FORM-3

Applied P & Ch Laboratory

Lab Control Spike/Lab Control Spike Duplicate Recovery for Method 7196

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34389
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W3899	
LCS Filename: -	Date Analyzed: 072903	Time Analyzed: 16:48
LCSD Filename: -	Date Analyzed: 072903	Time Analyzed: 16:48

Spiked Components	Unit	Spike Added	Concentration		LCS Rec% #	QC Limit, % REC
			Unspiked	LCS		
CHROMIUM (VI)	mg/L	0.25	0	0.266	106	80-115
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	LCSD Concentration	LCSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
CHROMIUM (VI)	mg/L	0.25	0.270	108	2	19	80-115
# of Out-of-control				0	0		

# Column to be used to flag recovery and RPD values:

\* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: \_\_\_\_\_  
 \_\_\_\_\_

FORM-3

Applied P & Ch Laboratory

Matrix Spike/Matrix Spike Duplicate Recovery for Method 7196

Client Name: GEOFON, Inc.	Contract No:	Lab Code: APCL
Case No:	SAS No:	Service ID: 34389
Project ID: JPL	Project No: 04-4428.10	Sample Matrix: Water
	Batch No: 03W3899	
MS Filename: -	Date Analyzed: 072903	Time Analyzed: 16:48
MSD Filename: -	Date Analyzed: 072903	Time Analyzed: 16:48
MS Sample No: MW-21-1	Sample Lab ID: 03-4389-2	

Spiked Components	Unit	Spike Added	Concentration		MS Rec% #	QC Limit, % REC
			Unspiked	MS		
CHROMIUM (VI)	mg/L	0.25	0	0.220	88	78-115
# of Out-of-control					0	

Spiked Components	Unit	Spike Added	MSD Concentration	MSD Rec% #	RPD% #	QC Limit, %	
						RPD	REC
CHROMIUM (VI)	mg/L	0.25	0.217	87	1	19	78-115
# of Out-of-control				0	0		

# Column to be used to flag recovery and RPD values:

\* - Values outside of contract required QC Limits

D - Spiked components diluted out

Comments: \_\_\_\_\_  
 \_\_\_\_\_

6A  
INITIAL CALIBRATION DATA

Lab Name: Applied P & Ch Lab Contract: 34389

Analysis: Chromium (VI) Calibration Date: 07/28/2003

Concentration (mg/L)	0.000	0.0125	0.050	0.125	0.250	0.50
Absorbance	0.000	0.007	0.017	0.107	0.212	0.420

**$A = -0.001 + 0.846C$**

**A=Absorbance**

**C=Concentration (mg/L)**

**r= 0.9999**

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710  
Tel: (909) 590-1828 Fax: (909) 590-1498

Chromium (VI) (7196) Worksheet

Batch # PR Matrix: WRS [ Holding Time: 24 hours!! ]

Test Date: 7/28/03 Analyst: PR

Lot #: Reagent Water Al 7/28/03  
Diphenylcazide solution

Test Time: \_\_\_\_\_ SOP: \_\_\_\_\_

Calibration	STD Lot #	$C_{std} \times V_{std} / V_f = C_i$	$A_i$	$RF_i = A_i / C_i$	Calibration results	Note
STD-1	W-7757	x / = 0.00 mg/L	0.000		Least Square [RF]=	Cal. Code:
STD-2	W-	x / = 0.005 mg/L	0.007		Average RF=	
STD-3	W-	x / = 0.005 mg/L	0.017		C.C. = 0.999 ( $\geq 0.995$ )	
STD-4	W-	x / = 0.015 mg/L	0.107		RSD= % ( $\leq 15\%$ )	
STD-5	W-	x / = 0.100 mg/L	0.212		Ref. page	
STD-6	W-	x / = 0.50 mg/L	0.420		$A = -0.001 + 0.846C$	

Analysis Type	Sample ID or Lot #	Samp. Amnt $X_0$ (g or mL)	Dilu./Ext $X/X_0 = f_1$	Treat. Ratio $V/V = f_2$	540 nm A	Concentration $C' = A / RF$	C (Sample) $C = f_1 f_2 C'$	Ano
CCV	Lot: W-7853	Expected Conc.: x	1	= 0.05 mg/L	0.218	0.259 mg/L	REC.	%
Method Blank	Bl. Lot:		$1/X_0 =$	95.0/	=	0.000	0.000 mg/L	ppm
LCS1	Bl. Lot:		$1/X_0 =$	95.0/	=	0.210	0.250 mg/L	ppm
Sample-1	4177-37	1ml $\rightarrow$ 100ml	$1/X_0 = 1$	95.0/	= 2	0.290	0.681 mg/L	ppm
MS on S-1	37	0.5ml $\rightarrow$ 100ml	$1/X_0 =$	95.0/	= 2	0.287	0.682 mg/L	ppm
MSD on S-1	4175-15	10.0g $\rightarrow$ 100g	$1/X_0 = 5$	95.0/	= 10	0.050	3.04 mg/L	ppm
Sample 2	15		$1/X_0 =$	95.0/	= 2	0.247	2.94 mg/L	ppm
Sample 3			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 4			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 5			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 6			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 7			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 8			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 9			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 10			$1/X_0 =$	95.0/	=		mg/L	ppm
Blank	Lot:		$1/X_0 =$	95.0/	=		mg/L	ppm
LCS2	Bl. Lot:		$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 11			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 12			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 13			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 14			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 15			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 16			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 17			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 18			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 19			$1/X_0 =$	95.0/	=		mg/L	ppm
Sample 20			$1/X_0 =$	95.0/	=		mg/L	ppm
MTX Dup.			$1/X_0 =$	95.0/	=	0.248	0.259 mg/L	ppm

Type	STD Lot #	$C_{STD} (\mu\text{g/mL}) \times V_{STD} (\text{mL}) / X (\text{g or mL}) = T$	Spike Rec.	Ch Limit (W/S)	PQL/MDL (in ppm)
MS	W-	x / = ppm	%	80-120 %/80-120 %	PQL(w) 0.01
MSD	W-	x / = ppm	%	.. ..	PQL(s) 0.05
LCS	W-	x / = ppm	%	80-120 %/80-120 %	MDL(w) 0.005
LCSD	W-	x / = ppm	%	.. ..	MDL(s) 0.025

1556



FORM-7  
Applied P & Ch Laboratory  
CCV Recovery for Wet Analysis

Client Name: GEOFON, Inc.

Contract No.:

Lab Code: APCL

Case No:

SAS No.:

Service ID: 34389

Project ID: JPL

Project No.: 04-4428.10

#	Component Name	Method	Batch No.	Unit	Expected	Test Result	Rec. %	Dev. %	Flag	Control Limit, %	Test Date
1	Perchlorate	314.0	03W3913	µg/L	50	55.2	110	10	✓	85-115	07/31/2003
	Perchlorate	314.0	03W3913	µg/L	50	55.6	111	11	✓	85-115	07/31/2003
	Perchlorate	314.0	03W3913	µg/L	50	55.4	111	11	✓	85-115	07/31/2003
	Perchlorate	314.0	03W3913	µg/L	50	54.9	110	10	✓	85-115	07/31/2003
2	Chromium (VI)	7196	03W3899	mg/L	0.25	0.258	103	3	✓	90-110	07/29/2003
	Chromium (VI)	7196	03W3899	mg/L	0.25	0.248	99	-1	✓	90-110	07/29/2003

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710  
Tel: (909) 590-1828 Fax: (909) 590-1498

Chromium (VI) (7196) Worksheet

Batch # W3899 Matrix: W

[ Holding Time: 24 hours!! ]

Test Date: 7/29/03 Analyst: pr

Lot #: Reagent Water \_\_\_\_\_ Diphenylcazide solution \_\_\_\_\_

Test Time: 16:48 SOP: G-1

Calibration	STD Lot #	$C_{std} \times V_{std} / V_f = C_i$	$A_i$	$RF_i = A_i / C_i$	Calibration results	Note
STD-1	W-	x / = mg/L			Least Square [RF]=	Cal. Code:
STD-2	W-	x / = mg/L			Average RF=	
STD-3	W-	x / = mg/L			C.C. = <u>0.999</u> (> 0.995)	
STD-4	W-	x / = mg/L			RSD = % (< 15%)	
STD-5	W-	x / = mg/L			Ref. page	
STD-6	W-	x / = mg/L				

$A = -0.001 + 0.846C$

Analysis Type	Sample ID or Lot #	Samp. Amnt $X_0$ (g or mL)	Dilu./Ext $X/X_0 = f_1$	Treat. Ratio $V/X = f_2$	540 nm A	Concentration $C' = A/RF$	C (Sample) $C = f_1 f_2 C'$	Anomaly Note
CCV	Lot: W- <u>7757</u>	Expected Conc.: x	1	= 0.25 mg/L	0.217	0.258 mg/L	REC. %	90-110 %
Method Blank	Bl. Lot:		$1/X_0 =$	95.0/ =	0.000	mg/L	0.001 ppm	
LCS1	Bl. Lot:		$1/X_0 =$	95.0/ =	0.224	mg/L	0.266 ppm	
Sample-1	<u>W3899 -2</u>		$1/X_0 =$	95.0/ =	0.002	mg/L	0.003 ppm	
MS on S-1	-2		$1/X_0 =$	95.0/ =	0.185	mg/L	0.220 ppm	
MSD on S-1	-2		$1/X_0 =$	95.0/ =	0.002	mg/L	0.217 ppm	
Sample 2	-3		$1/X_0 =$	95.0/ =	0.002	mg/L	0.003 ppm	
Sample 3	-4		$1/X_0 =$	95.0/ =	0.001	mg/L	0.002 ppm	
Sample 4	-5		$1/X_0 =$	95.0/ =	0.001	mg/L	0.002 ppm	
Sample 5	-6		$1/X_0 =$	95.0/ =	0.000	mg/L	0.001 ppm	
Sample 6	-1		$1/X_0 =$	95.0/ =	0.000	mg/L	0.001 ppm	
Sample 7			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 8			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 9			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 10			$1/X_0 =$	95.0/ =		mg/L	ppm	
Blank	Lot:		$1/X_0 =$	95.0/ =		mg/L	ppm	
LCS2	Bl. Lot:		$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 11			$1/X_0 =$	95.0/ =	0.227	mg/L	0.270 ppm	
Sample 12			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 13			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 14			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 15			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 16			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 17			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 18			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 19			$1/X_0 =$	95.0/ =		mg/L	ppm	
Sample 20			$1/X_0 =$	95.0/ =		mg/L	ppm	
MTX Dup.			$1/X_0 =$	95.0/ =	0.209	0.248 mg/L	ppm	

Type	STD Lot #	$C_{STD} (\mu\text{g/mL}) \times V_{STD} (\text{mL}) / X (\text{g or mL}) = T$	Spike Rec.	Ctrl Limit (W/S)	PQL/MDL (in ppm)
MS	W- <u>7757</u>	x / = 0.25 ppm	%	80-120 %/80-120 %	PQL(w) 0.01
MSD	W- <u>4</u>	x / = ppm	%	..	PQL(s) 0.05
LCS	W- <u>7853</u>	x / = ppm	%	80-120 %/80-120 %	MDL(w) 0.005
LCSD	W- <u>1</u>	x / = ppm	%	..	MDL(s) 0.058

Applied P & Ch Laboratory  
 13760 Magnolia Ave. Chino, CA.91710  
 Tel: (909) 590-1828

**Perchlorate (EPA 314) Batch QC Report**

Batch: 03w3913 Matrix w  
 Test date: 07/31/03 System K  
 MDL: 0.66 ppb MRL: 4 ppb

Service included 03-4406,4389  
 Analyst: ww and Wu  
 MCT: 6462 us/cm

Items	Perchlorate Expt.(ppb)	Results Summary							Acceptance Criteria
		S.C us/cm	6462		Perchlor. Conc.	27.05	Perchlor.Re c %	108.2	
IPC	25	A	45909	H	2002.14	A/H	22.93	P/D % 7.4	R 80-120% PD <25%
MB	0	Conc.	0	OK ?	OK				<= 1/2 MRL
ICCS	4	Conc.	4.19	Rec. %	104.75				70-125%
LCS	25	Conc.	25.52	Rec. %	102.08	A	H	A/H	80-120%
CHECK	18	Conc.	18.96	Rec. %	105.33				85-115%
CCV	50	CCV1 Conc.	55.18	Rec. %	110.36	CCV2 Conc.	55.56	Rec. % 111	85-115%
CCV	50	CCV3 Conc.	55.38	Rec. %	110.76	ECV Conc.	54.9	Rec. % 110	85-115%
MD		RPD%	0	OK ?	OK				<=15%
MS	50	usprike conc.	3.63	MS conc	60.51	MS Rec.%.	113.76		75-125%
MSD	50	usprike conc.	3.63	MSD conc	59.68	MSD Rec.%.	112.1		75-125%

Sample ID for MS/MSD 4406-10 Sample ID for MD

Global QC :  Passed  
 Flag: \_\_\_\_\_  
 Failed: Corrective action \_\_\_\_\_


- Note:
1. IPC: Instrument Performance Check Standard at MCT.
  2. ICCS: Initial Calibration Check.
  3. MCT: Matrix Conductivity Threshold.
  4. PD(A/H): The A/H ratio percent difference between the average A/H ratio for the LFB(A/H) and the A/H ratio of IPC.
  5. A/H : Peak area/peak height.

ie	Sample	Sample Type	Level	Method	Data File	Volume	Dilution
	##03w3913kw ipc 25ppb w8032	Sample		e314-011.met	c:\data\03w3913k\w3913k ipc 25ppb	1	1
	ccv 50ppb w8082	Sample		e314-011.met	c:\data\03w3913k\w3913k q01	1	1
	lcs 25ppb w8087	Sample		e314-011.met	c:\data\03w3913k\w3913k l01	1	1
	LCS 18PPB W8033a	Sample		e314-011.met	c:\data\03w3913k\w3913k j01	1	1
	ICCS 4ppb w8088	Sample		e314-011.met	c:\data\03w3913k\w3913k iccs 4ppb	1	1
	mb	Sample		e314-011.met	c:\data\03w3913k\w3913k k01	1	1
	4406-10 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-10	1	1
	4389-02 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-02	1	1
	4389-03 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-03	1	1
	4389-04 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-04	1	1
	4389-05 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-05	1	1
	4389-06 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-06	1	1
	ccv 50ppb w8082	Sample		e314-011.met	c:\data\03w3913k\w3913k q02	1	1
	ccb	Sample		e314-011.met	c:\data\03w3913k\w3913k k02	1	1
	4406-10 ms 50ppb f=1 w8033b	Sample		e314-011.met	c:\data\03w3913k\w3913k m01	1	1
	4406-10 msd 50ppb f=1 w8033b	Sample		e314-011.met	c:\data\03w3913k\w3913k n01	1	1
	4406-01 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-01	1	1
	4406-02 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-02	1	1
	4406-03 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-03	1	1
	4406-04 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-04	1	1
	4406-05 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-05	1	1
	4406-06 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-06	1	1
	4406-07 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-07	1	1
	ccv 50ppb w8082	Sample		e314-011.met	c:\data\03w3913k\w3913k q03	1	1
	ccb	Sample		e314-011.met	c:\data\03w3913k\w3913k k03	1	1
	4389-01 f=1	Sample		e314-011.met	c:\data\03w3913k\4389-01	1	1
	4406-08 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-08	1	1
	4406-09 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-09	1	1
	4406-11 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-11	1	1
	4406-12 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-12	1	1
	4406-13 f=1	Sample		e314-011.met	c:\data\03w3913k\4406-13	1	1
	4406-07 f=5	Sample		e314-011.met	c:\data\03w3913k\4406-07a	1	5
	ccv 50ppb w8082	Sample		e314-011.met	c:\data\03w3913k\w3913k q04	1	1
		Sample		aastopcl.met		1	1

Analyst Wes' Way  
 Date 7/31/03  
 Instrument IC-K



1. Component: perchlorate  
Standard: External Fit Type: Linear  
Origin: Force Calibration: Area  
 $r^2=0.999492$   
 $Amt=0.0005893*Resp+0$

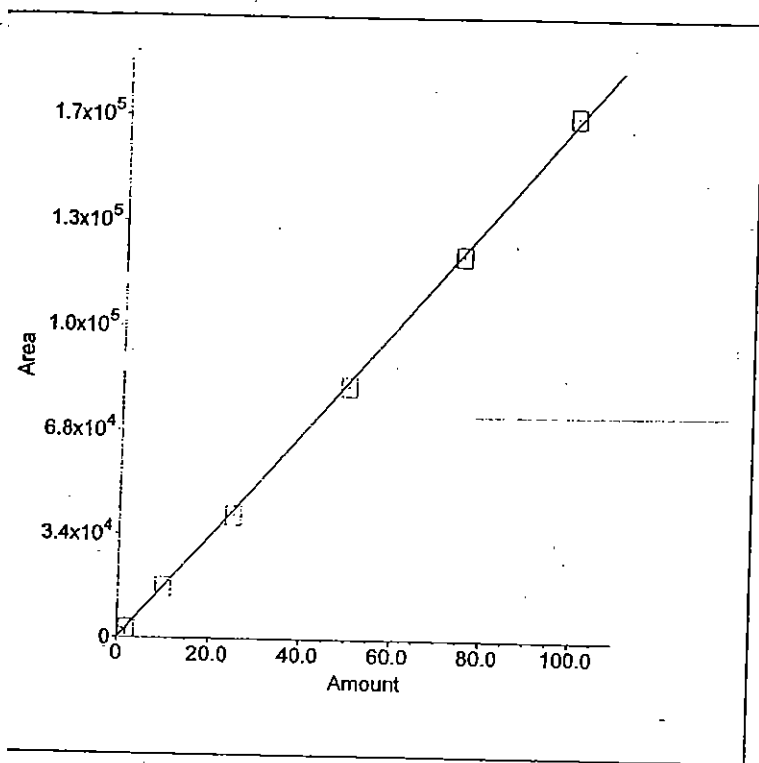

Calibration : 7 points , 0, 2, 10, 25, 50, 75, 100 ppb

Analyst C.W  
Date 03/12/03  
Instrument LC-10

# APCL Perchlorate Analysis Report

Sample Name : Cal blank

Data File Name : C:\data\E314-011\Mb\_001.DXD

Method File Name : c:\peaknet\method\e314-011.met


Date Time Collected : 03/12/2003 5:55:39 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

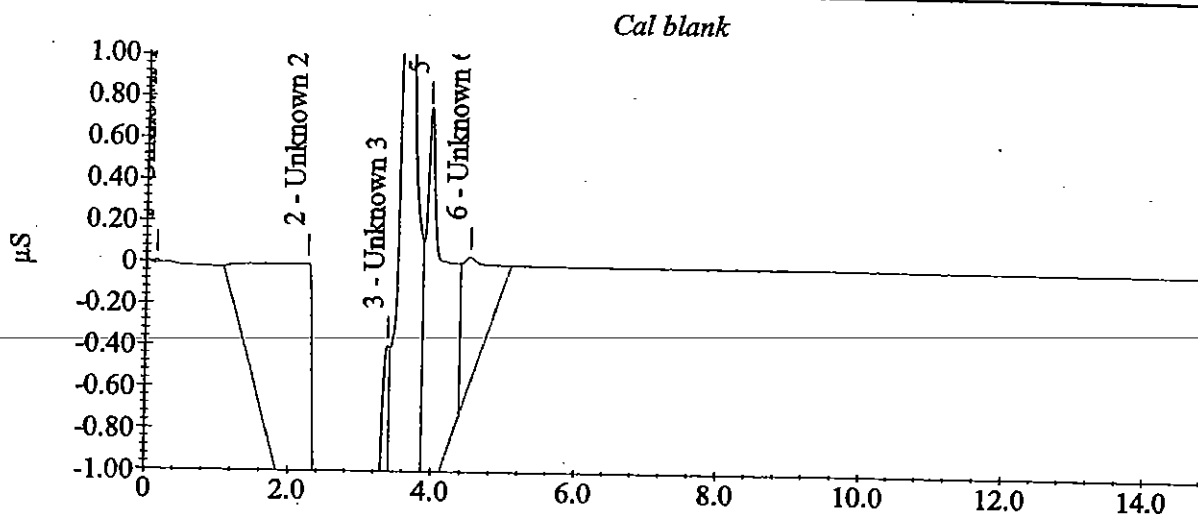

# APCL Perchlorate Analysis Report

Sample Name : cal standard 2ppb W7827a

Data File Name : C:\DATA\E314-011\std-2pb\_002.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 6:13:12 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.62	1.92	2910	164

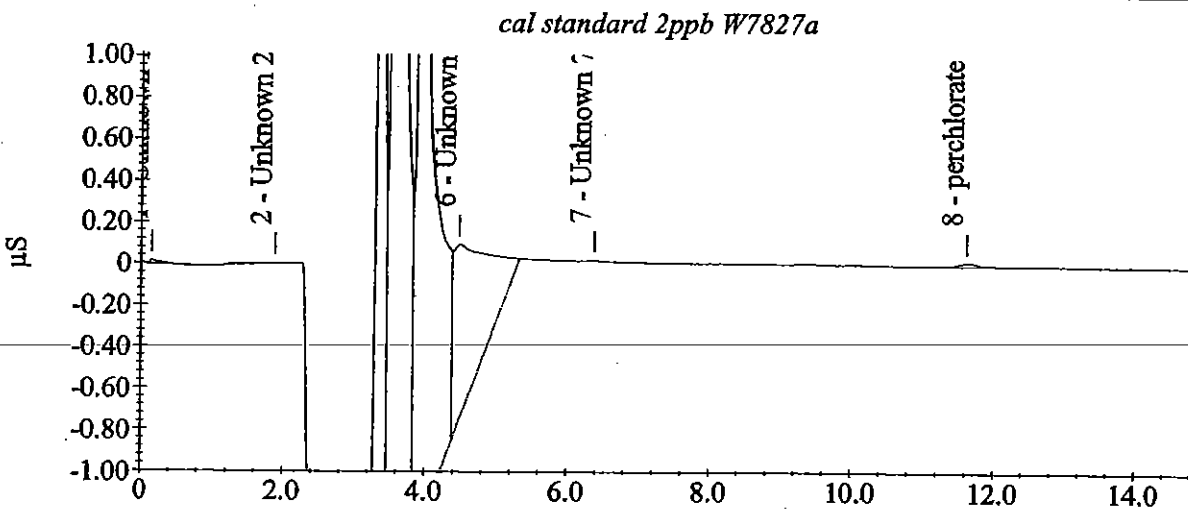



# APCL Perchlorate Analysis Report

Sample Name : cal standard 10ppb W7827c

Data File Name : C:\DATA\E314-011\std-10pb\_004.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 6:48:21 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
7	perchlorate	11.70	11.16	16917	879

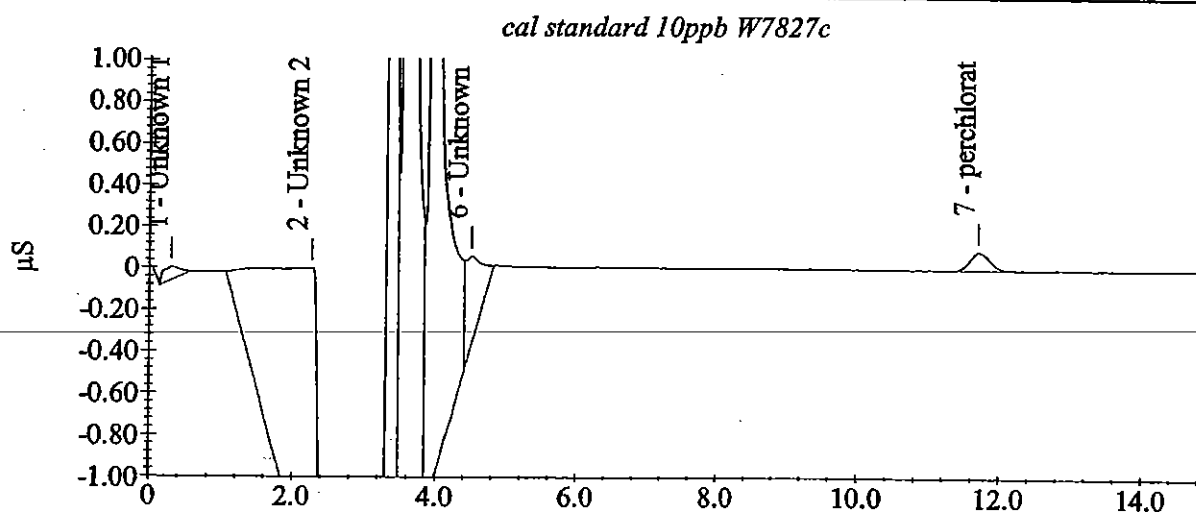

# APCL Perchlorate Analysis Report

Sample Name : cal standard 25ppb W7827d

Data File Name : C:\DATA\E314-011\std-25pb\_005.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 7:05:54 PM

System Operator : wei wang

Dilution Factor : 1.00

## Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.60	26.84	40702	2125

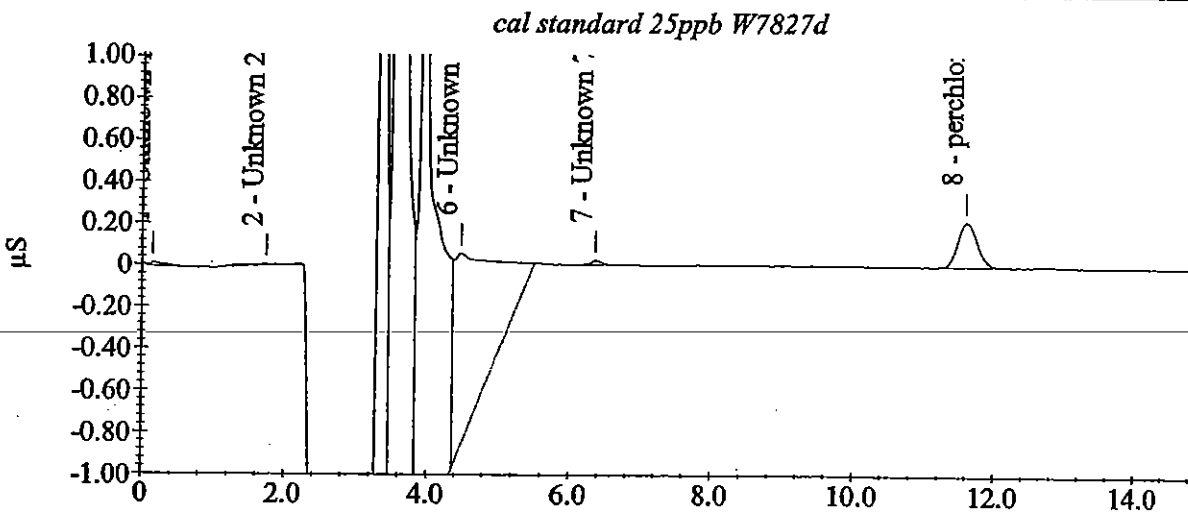

# APCL Perchlorate Analysis Report

Sample Name : cal standard 50ppb W7827e

Data File Name : C:\DATA\E314-011\std-50pb\_006.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 7:23:30 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.67	54.89	83240	4320

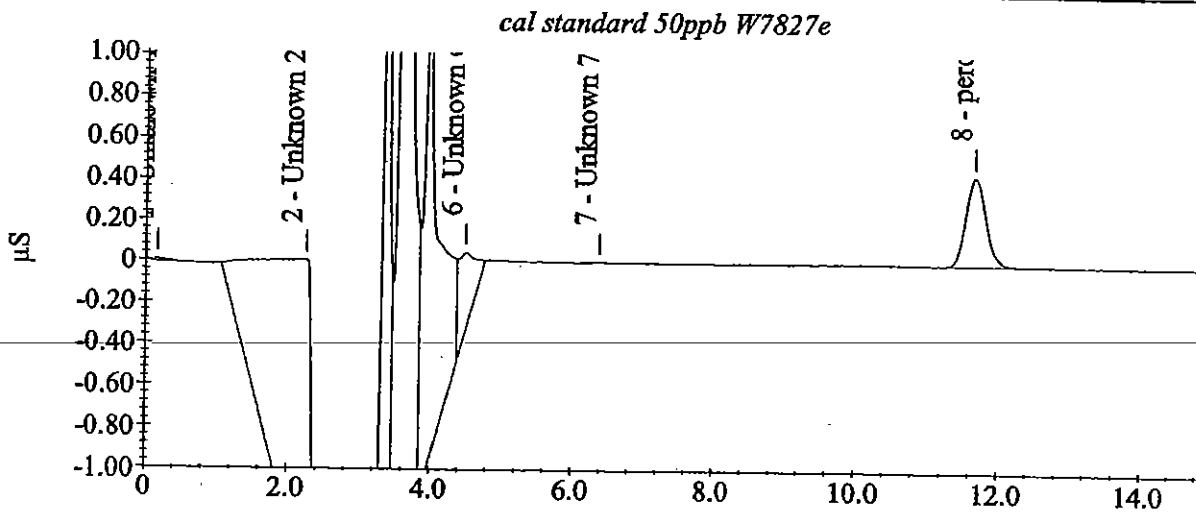

# APCL Perchlorate Analysis Report

Sample Name : cal standard 75ppb W7827f

Data File Name : C:\DATA\E314-011\std-75pb\_007.DXD

Method File Name : C:\PEAKNET\METHOD\e314-011.met


Date Time Collected : 03/12/2003 7:41:05 PM

System Operator : wei wang

Dilution Factor : 1.00

## Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
7	perchlorate	11.62	83.23	126224	6553

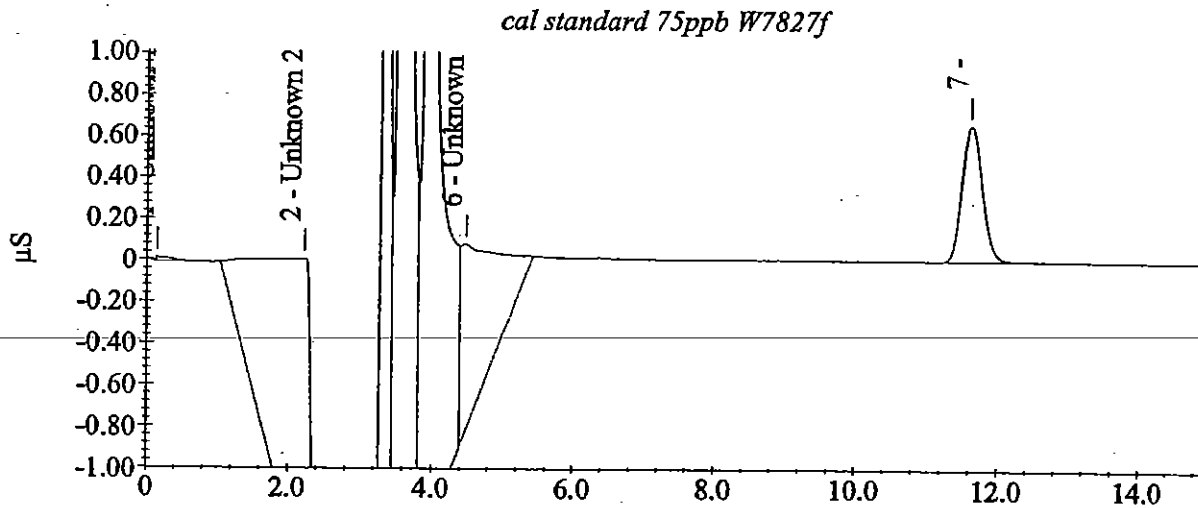

# APCL Perchlorate Analysis Report

Sample Name : cal standard 100ppb W7827g

Data File Name : C:\DATA\E314-011\std-100pb\_008.DXD

Method File Name : C:\PEAKNET\METHOD\314-011.met


Date Time Collected : 03/12/2003 7:58:39 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.62	113.21	171686	89271

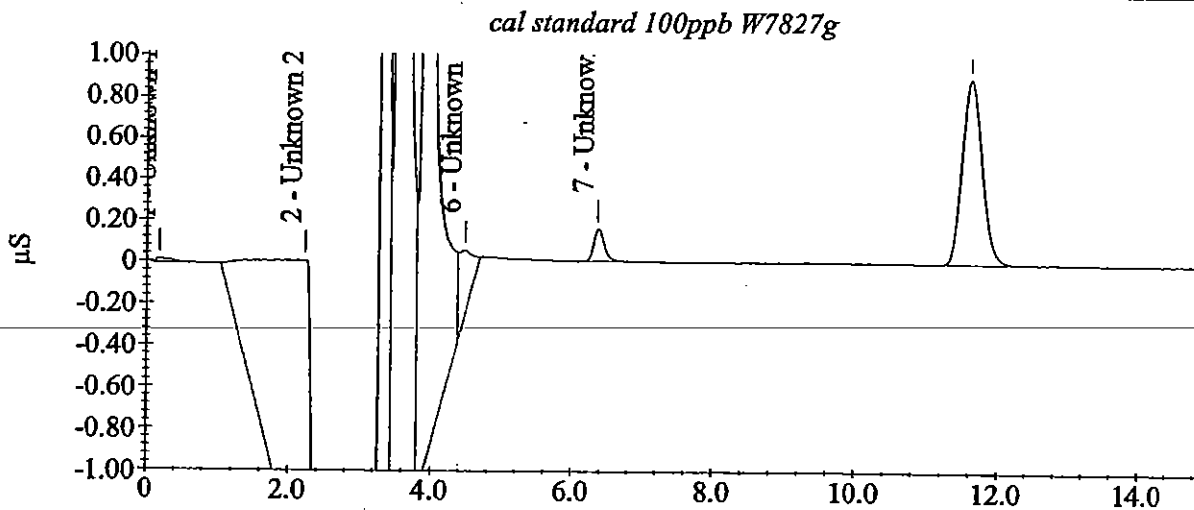

# APCL Perchlorate Analysis Report

Sample Name : ICV 50 ppb w7828a

Data File Name : C:\DATA\E314-011\icv-50pb\_009.DXD

Method File Name : C:\PEAKNET\METHOD\E314-011.met


Date Time Collected : 03/12/2003 8:16:15 PM

System Operator : wei wang

Dilution Factor : 1.00

Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
8	perchlorate	11.65	49.49	83990	4321

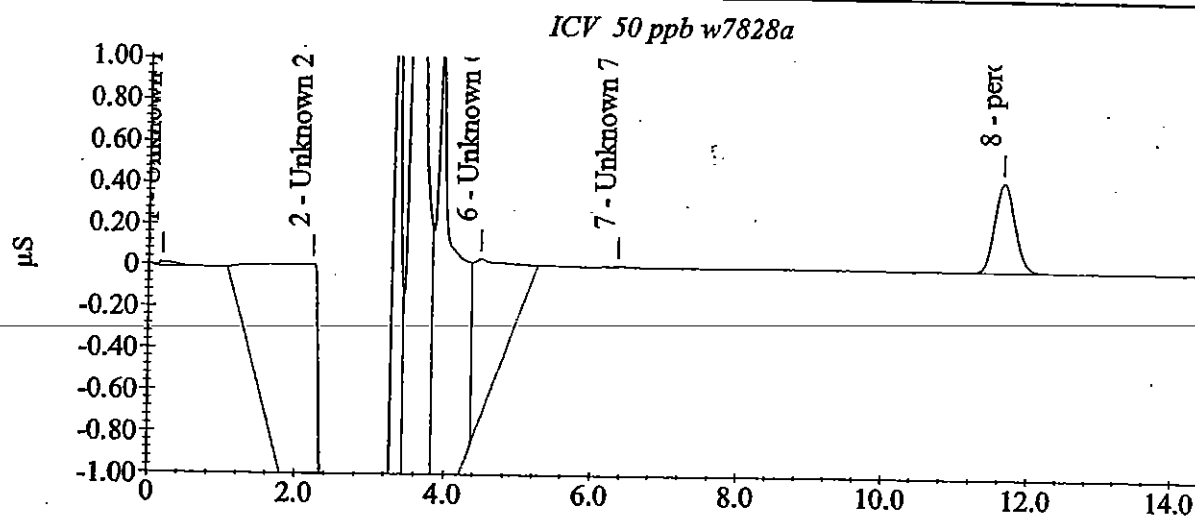

# APCL Perchlorate Analysis Report

Sample Name : icb

Data File Name : C:\DATA\E314-011\ICB\_010.DXD

Method File Name : c:\PeakNet\method\E314-011.met


Date Time Collected : 03/12/2003 8:33:51 PM

System Operator : wei wang

Dilution Factor : 1.00

## Peak Information : All Components

Peak #	Component Name	Retention Time	Amount (ppb)	Peak Area	Peak Height
--------	----------------	----------------	--------------	-----------	-------------

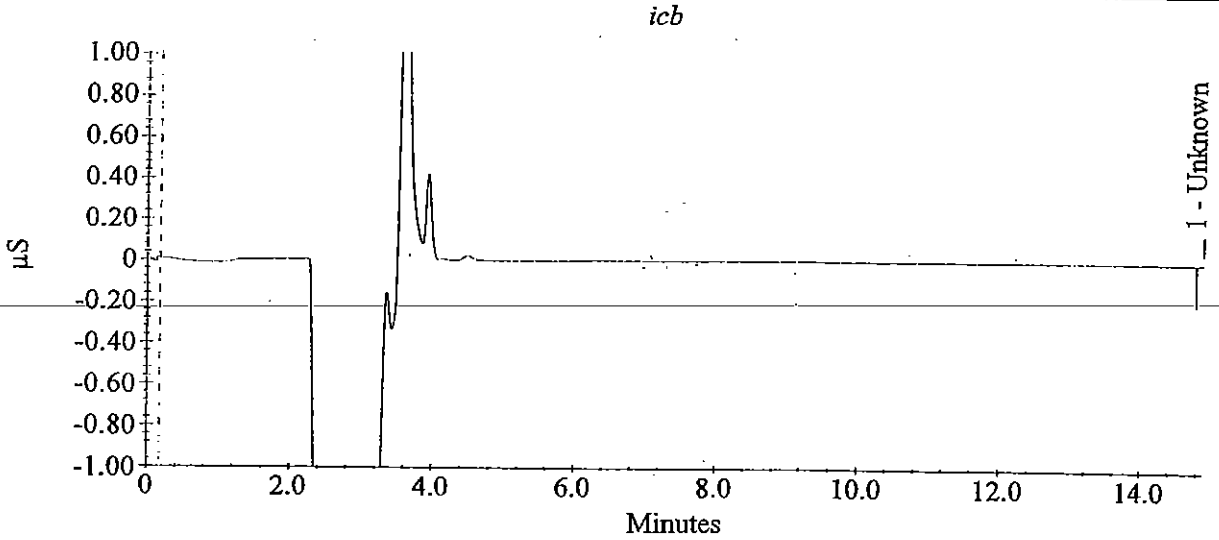

Line	Sample	Sample Type	Level	Method	Data File	Volume	Dilution
1	Cal blank	Sample		e314-011.met	c:\data\314-011\mb_001.dxd	1	1
2	cal standard 2ppb W7827a	Sample		e314-011.met	c:\data\314-011\std-2pb_002.dxd	1	1
3	cal standard 4ppb W7827b	Sample		e314-011.met	c:\data\314-011\std-4pb_003.dxd	1	1
4	cal standard 10ppb W7827c	Sample		e314-011.met	c:\data\314-011\std-10pb_004.dxd	1	1
5	cal standard 25ppb W7827d	Sample		e314-011.met	c:\data\314-011\std-25pb_005.dxd	1	1
6	cal standard 50ppb W7827e	Sample		e314-011.met	c:\data\314-011\std-50pb_006.dxd	1	1
7	cal standard 75ppb W7827f	Sample		e314-011.met	c:\data\314-011\std-75pb_007.dxd	1	1
8	cal standard 100ppb W7827g	Sample		e314-011.met	c:\data\314-011\std-100pb_008.dxd	1	1
9	ICV 50 ppb w7828a	Sample		e314-011.met	c:\data\314-011\icv-50pb_009.dxd	1	1
0	icb	Sample		e314-011.met	c:\data\314-011\icb_010.dxd	1	1
1	anion 100pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-011\mct-100_011.dxd	1	1
2	anion 200pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-011\mct-200_012.dxd	1	1
3	anion 300pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-011\mct-300_013.dxd	1	1
4	anion 400pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-011\mct-400_014.dxd	1	1
5	anion 500pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-011\mct-500_015.dxd	1	1
6	anion 600pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-011\mct-600_016.dxd	1	1
7	anion 800pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-011\mct-800_017.dxd	1	1
8	anion 1000pm each ,25pb CLO4	Sample		e314-011.met	c:\data\314-011\mct-1000_018.dxd	1	1
9	anion 400pm each 2pb	Sample		e314-011.met	c:\data\314-011\ipc-2pb_019.dxd	1	1
0	anion 400pm each 4pb	Sample		e314-011.met	c:\data\314-011\ipc-4pb_020.dxd	1	1
1	anion 400pm each 25pb	Sample		e314-011.met	c:\data\314-011\ipc-25pb_021.dxd	1	1
2	ICV 50 ppb	Sample		e314-011.met	c:\data\314-011\icc-50pb	1	1
3	MDL 4pb	Sample		e314-011.met	c:\data\314-011\mdl-02_023.dxd	1	1
4	MDL 4pb	Sample		e314-011.met	c:\data\314-011\mdl-03_024.dxd	1	1
5	MDL 4pb	Sample		e314-011.met	c:\data\314-011\mdl-04	1	1
6	MDL 4pb	Sample		e314-011.met	c:\data\314-011\mdl-05	1	1
7	MDL 4pb	Sample		e314-011.met	c:\data\314-011\mdl-06	1	1
8	MDL 4pb	Sample		e314-011.met	c:\data\314-011\mdl-07	1	1
9	MDL 4pb	Sample		e314-011.met	c:\data\314-011\mdl-08	1	1
0	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-011\idap-25pb	1	1
1	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-011\idap-25pb	1	1
2	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-011\idap-25pb	1	1
3	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-011\idap-25pb	1	1
4	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-011\idap-25pb	1	1
5	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-011\idap-25pb	1	1
6	IDP and IDA 25pb	Sample		e314-011.met	c:\data\314-011\idap-25pb	1	1
7	MCT anion 800pm each, 25pbCLO4	Sample		e314-011.met	c:\data\314-011\ipc-25pb	1	1
8	MCT anion 800pm each, 25pbCLO4	Sample		e314-011.met	c:\data\314-011\ipc-25pb	1	1
9	MCT anion 800pm each, 4pbCLO4	Sample		e314-011.met	c:\data\314-011\ipc-4pb	1	1
0	MCT anion 800pm each, 4pbCLO4	Sample		e314-011.met	c:\data\314-011\ipc-4pb	1	1
1	MDL 20pb soil	Sample		e314-011.met	c:\data\314-011\mdl-s01	1	5
2	MDL 20pb soil	Sample		e314-011.met	c:\data\314-011\mdl-s02	1	5
3	MDL 20pb soil	Sample		e314-011.met	c:\data\314-011\mdl-s03	1	5
4	MDL 20pb soil	Sample		e314-011.met	c:\data\314-011\mdl-s04	1	5
5	MDL 20pb soil	Sample		e314-011.met	c:\data\314-011\mdl-s05	1	5
6	MDL 20pb soil	Sample		e314-011.met	c:\data\314-011\mdl-s06	1	5
7	MDL 20pb soil	Sample		e314-011.met	c:\data\314-011\mdl-s07	1	5
8	standard 25ppb W7827d	Sample		e314-011.met	c:\data\314-011\std-25pb	1	1
9	anion 100pm each,4pb CLO4	Sample		e314-011.met	c:\data\314-011\lam-100-4pb	1	1
0	anion 200pm each ,4pb CLO4	Sample		e314-011.met	c:\data\314-011\lam-200-4pb	1	1
1	anion 300pm each ,4pb CLO4	Sample		e314-011.met	c:\data\314-011\lam-300-4pb	1	1
2	anion 100pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-011\lam-100-2pb	1	1
3	anion 200pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-011\lam-200-2pb	1	1
4	anion 300pm each,2pb CLO4	Sample		e314-011.met	c:\data\314-011\lam-300-2pb	1	1
5	1982-01 B S.C 4450us/cm	Sample		e314-011.met	c:\data\314-011\1982-01	1	1
6	1982-01 B S.C 4450us/cm	Sample		e314-011.met	c:\data\314-011\1982-01	1	2
7	1982-02 f=10	Sample		e314-011.met	c:\data\314-011\1982-02_057.dxd	1	10
8		Sample		aastopcl.met		1	1



Line	Weight	Int. Std.	Comment
1	1	1	
2	1	1	
3	1	1	
4	1	1	
5	1	1	
6	1	1	
7	1	1	
8	1	1	
9	1	1	
10	1	1	
11	1	1	
12	1	1	
13	1	1	
14	1	1	
15	1	1	
16	1	1	
17	1	1	
18	1	1	
19	1	1	
20	1	1	
21	1	1	
22	1	1	
23	1	1	
24	1	1	
25	1	1	
26	1	1	
27	1	1	
28	1	1	
29	1	1	
30	1	1	
31	1	1	
32	1	1	
33	1	1	
34	1	1	
35	1	1	
36	1	1	
37	1	1	
38	1	1	
39	1	1	
40	1	1	
41	1	1	
42	1	1	
43	1	1	
44	1	1	
45	1	1	
46	1	1	
47	1	1	
48	1	1	
49	1	1	
50	1	1	
51	1	1	
52	1	1	
53	1	1	
54	1	1	
55	1	1	
56	1	1	
57	1	1	
58	1	1	

Default Method Path: C:\PEAKNET\METHOD  
Default Data Path: C:\DATA\03V\1286K  
Comment:  
Remark:

Condition information:

Column

Separator column: AS16 4mm

Guard column: AS16 4mm

Eluent: NaOH 38mM

Flow rate: 1.2mL/min

Suppressor: ASRS-ULTRA 4mm

Detector: CD20

Analyst: Charles Wu and Wei Wang

Date: 03 / 12 / 2003

Instrument: IC-K DX-500 Dionex

Applied P & Ch Laboratory

13760 Magnolia Ave. Chino CA 91710

Tel: (909) 590-1828 Fax: (909) 590-1498

Submitted to:

GEOFON, Inc.

Attention: Brad Shojaee

22632 Golden Spring Dr Ste 270

Diamond Bar 91765

Tel: (909)396-7662 Fax: (909)396-1455

# APCL Analytical Report

Service ID #: 801-034558

Received: 08/07/03

Collected by:

Extracted: N/A

Collected on: 08/04-07/03

Tested: N/A

Reported: 08/19/03

Sample Description: Water

Project Description: JPL

## Analysis of Water Samples

Component Analyzed	Method	Unit	PQL	Analysis Result			
				DUPE-3-3-Q03	DUPE-4-3-Q03	EB-4-8-4-03	EB-5-8-6-03
				03-04558-1	03-04558-2	03-04558-3	03-04558-4

### CHROMIUM (a)

Component Analyzed	Method	Unit	PQL	Analysis Result			
				MW-4-1	MW-4-2	MW-4-3	MW-11-1
				03-04558-5	03-04558-6	03-04558-7	03-04558-8

### CHROMIUM (a)

Component Analyzed	Method	Unit	PQL	Analysis Result			
				MW-11-2	MW-11-3	MW-14-1	MW-14-2
				03-04558-9	03-04558-10	03-04558-11	03-04558-12

### CHROMIUM (a)

Component Analyzed	Method	Unit	PQL	Analysis Result			
				MW-14-3	MW-14-4	MW-18-2	MW-18-3
				03-04558-13	03-04558-14	03-04558-15	03-04558-16

### CHROMIUM (a)

Component Analyzed	Method	Unit	PQL	Analysis Result		
				MW-18-4	MW-23-1	MW-23-2
				03-04558-17	03-04558-18	03-04558-19

### CHROMIUM (a)

Component Analyzed	Method	Unit	PQL	Analysis Result		
				MW-23-3	MW-23-4	MW-24-1
				03-04558-20	03-04558-21	03-04558-22

### CHROMIUM (a)

# APCL Analytical Report

---

Component Analyzed	Method	Unit	PQL	Analysis Result		
				MW-24-2	MW-24-3	MW-24-4
				03-04558-23	03-04558-24	03-04558-25

---

## CHROMIUM <sup>(a)</sup>

PQL: Practical Quantitation Limit. MDL: Method Detection Limit. CRDL: Contract Required Detection Limit


N.D.: Not Detected or less than the practical quantitation limit. "-": Analysis is not required.

J: Reported between PQL and MDL.

Listed Dilution Factors (DF) are relative to the method default DF. All unlisted DFs are 1.0

<sup>(a)</sup> Subcontracted to Advanced Technology Laboratories Inc. See attached.

Respectfully submitted,

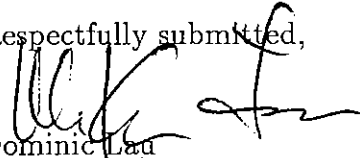

Dominic Lau  
Laboratory Director  
Applied P & Ch Laboratory



INCORPORATED  
22632 GOLDEN SPRINGS DR., SUITE 270  
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX: (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

MW-18

0076

Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont.	QC Level	T.A.T	Analyses		Comments
									524.2 (VOCs)	314.0 (Residuals)	
1	MW-18-5	H <sub>2</sub> O	8/1/03	0801	None	3+1	TTC	None	X	X	
2	MW-18-4			0830	None	3+1	TTC	None	X	X	
3	MW-18-3			0879	None				X	X	
4	MW-18-2			0872	None				X	X	
5	EB-4-8-4-03			0840	None	5			X	X	
6	TB-4-8-4-03				None	3+2			X	X	
7											
8											
9											
10											

4558

SAMPLES COLLECTED BY: Leah Williamson COURIER AND AIR BILL NUMBER: \_\_\_\_\_ RECEIVED BY: \_\_\_\_\_ DATE: 8/1/03 TIME: 1000

REINQUISHED BY: Leah Williamson

LABORATORY SERVICE ID: \_\_\_\_\_ LABORATORY CONTACT: Kenny Chan

LABORATORY PHONE: (909) 590-1828 LABORATORY FAX: (909) 590-1498

LABORATORY ADDRESS: 13760 Magnolia Ave CITY, STATE AND ZIP CODE: Cherry, CA 91710

MAIL REPORT (COMPANY NAME): GEOFON, INC RECIPIENT NAME: Tony Ford

PROJECT NAME: Dr. Lee Mon-3903 PROJECT LOCATION: MW-18 (Athletics & Forecasts) PROJECT NUMBER: 04-442 B/D

PROJECT CONTACT: J. Robinson PROJECT PHONE NUMBER: (949) 295-7884 PROJECT FAX: (909) 396-1455

PROJECT ADDRESS: 4800 Oak Lane Dr. CITY, STATE AND ZIP CODE: Pasadena, CA CLIENT: US Navy Swidiv

PROJECT MANAGER: Arnar Fabean PROJECT MANAGER'S PHONE: (909) 396-7662 PROJECT MANAGER'S FAX: (909) 396-1455

ADDRESS: 22632 Golden Springs Dr #270 CITY, STATE AND ZIP CODE: Diamond Bar, CA 91765

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager



**GEOFFON**  
INCORPORATED

22632 GOLDEN SPRINGS DR., SUITE 270  
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

**CHAIN-OF-CUSTODY RECORD**

LABORATORY COPY

MW-4  
0047

Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont	QC Level	T.A.T	Analyses	Comments
1	MW-4-3	H <sub>2</sub> O	8/11/03	1010	3+1+1	III	NORMAL	X	X	X
2	MW-4-2			1031				X	X	X
3	MW-4-1			1104				X	X	X
4	Dupe-3-3-003			1129		IV		X	X	X
5										
6										
7										
8										
9										
10										

**4558**

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager



**GEOFFON**  
INCORPORATED  
22632 GOLDEN SPRINGS DR., SUITE 270  
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

**CHAIN-OF-CUSTODY RECORD**

LABORATORY COPY

MW-23 0048

GEORGE - LAB COORDINATOR

LAB COORDINATOR'S PHONE

LAB COORDINATOR'S FAX

LABORATORY SERVICE ID

LABORATORY CONTACT

MAIL REPORT (COMPANY NAME)

Brad Shojaee

(909) 396-7662

(909) 396-1455

-

Kenny Chan

GEOFFON, INC.

PROJECT NAME: MW 6w Mon - 3903

PROJECT LOCATION: MW-23 ( N. of Bl 233)

PROJECT NUMBER: 04-442810

LABORATORY PHONE: (909) 590-1828

LABORATORY FAX: (909) 590-1498

RECIPIENT NAME: Tony Ford

PROJECT CONTACT: J. Robinson

PROJECT PHONE NUMBER: (909) 295-7884

PROJECT FAX: (909) 396-1455

LABORATORY ADDRESS: 13760 Magnolia Ave

LABORATORY CITY, STATE AND ZIP CODE: Chino, CA 91710

ADDRESS: 22632 Golden Springs Dr. #270

PROJECT ADDRESS: 4800 Oak Grove Dr.

CITY, STATE AND ZIP CODE: Pasadena, CA

CLIENT: US NAVY Snowir

CITY, STATE AND ZIP CODE: Chino, CA 91710

LABORATORY CONTACT: (909) 590-1828

CITY, STATE AND ZIP CODE: Diamond Bar, CA 91765

PROJECT MANAGER: Astrar Fabeem

PROJECT MANAGER'S PHONE: (909) 396-7662

PROJECT MANAGER'S FAX: (909) 396-1455

LABORATORY SERVICE ID

LABORATORY CONTACT

MAIL REPORT (COMPANY NAME)

PROJECT MANAGER: Astrar Fabeem

PROJECT MANAGER'S PHONE: (909) 396-7662

PROJECT MANAGER'S FAX: (909) 396-1455

LABORATORY SERVICE ID

LABORATORY CONTACT

MAIL REPORT (COMPANY NAME)

PROJECT MANAGER: Astrar Fabeem

PROJECT MANAGER'S PHONE: (909) 396-7662

PROJECT MANAGER'S FAX: (909) 396-1455

LABORATORY SERVICE ID

LABORATORY CONTACT

MAIL REPORT (COMPANY NAME)

PROJECT MANAGER: Astrar Fabeem

PROJECT MANAGER'S PHONE: (909) 396-7662

PROJECT MANAGER'S FAX: (909) 396-1455

LABORATORY SERVICE ID

LABORATORY CONTACT

MAIL REPORT (COMPANY NAME)

Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont.	QC Level	T.A.T	Analyses			Comments
									5242 (Vols)	3140 (Perchlorate)	7196 (Hex Chloro)	
1	MW-23-4	H <sub>2</sub> O	8/6/03	0722	HC1	2441	ITC	Normal	X	X	X	
2	MW-23-3			0748					X	X	X	
3	MW-23-2			0809					X	X	X	
4	MW-23-1			0824					X	X	X	
5	IB-5-8-6-03				HC1	2			X	X	X	
6	IR-5-8-6-03				HC1	5			X	X	X	
7												
8												
9												
10												

4558

8.6.03

SAMPLES COLLECTED BY: Leo W. Williamson

RELINQUISHED BY: Leo W. Williamson

COURIER AND AIR BILL NUMBER:

RECEIVED BY: Leo W. Williamson

DATE: 8/6/03

TIME: 0704

SAMPLE'S CONDITION UPON RECEIPT

RELINQUISHED BY: Leo W. Williamson

RECEIVED BY: Leo W. Williamson

COURIER AND AIR BILL NUMBER:

DATE: 8/6/03

TIME: 1531

SAMPLE'S CONDITION UPON RECEIPT

RELINQUISHED BY: Leo W. Williamson

RECEIVED BY: Leo W. Williamson

COURIER AND AIR BILL NUMBER:

DATE: 8/6/03

TIME: 1655

SAMPLE'S CONDITION UPON RECEIPT

RELINQUISHED BY: Leo W. Williamson

RECEIVED BY: Leo W. Williamson


COURIER AND AIR BILL NUMBER:

DATE: 8/6/03

TIME: 1655

SAMPLE'S CONDITION UPON RECEIPT

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager



INCORPORATED  
26592 GOLDEN SPRINGS DR, SUITE 270  
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

PROJECT DATA MANAGERS COPY

MW-2495.9.03 0019

Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont	QC Level	T.A.T	Analyses	Comments
1	ANN-74-9	HO	8/6/03	07:00	2:00	1	III	medium	5242 (VVO) 3140 (Machobane) 7126 (Machobane) 2263 (Machobane)	ADD 3140 for Analysis 8/03
2	ANN-74-3		8/6/03	07:00	2:00	1	III	medium		
3	ANN-74-2		8/6/03	07:00	2:00	1	III	medium		
4	ANN-74-1		8/6/03	07:00	2:00	1	III	medium		
5	DATE-7-5-003		8/6/03	07:00	2:00	1	III	medium		
6										
7										
8										
9										
10										

1552

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager

REUNDRUSHED BY: W.L. G.P. 5/03  
CORNER AND AIR BILL NUMBER: 1552  
RECEIVED BY: [Signature]  
DATE: 8/10/03  
TIME: 10:31

COOLER TEMPERATURE UPON RECEIPT

SAMPLE'S CONDITION UPON RECEIPT



**GEOFON**

INCORPORATED  
22632 GOLDEN SPRINGS DR., SUITE 270  
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

**CHAIN-OF-CUSTODY RECORD**

LABORATORY COPY

MW-24

0049

GEOPON LAB COORDINATOR	LAB COORDINATOR'S PHONE	LAB COORDINATOR'S FAX	LABORATORY SERVICE ID	LABORATORY CONTACT	MAIL REPORT (COMPANY NAME)
Brad Shojae	(909) 396-7662	(909) 396-1455	-	Kenny Chan	GEOFON, INC.

PROJECT NAME	PROJECT LOCATION	PROJECT NUMBER	LABORATORY PHONE	LABORATORY FAX	RECIPIENT NAME
SPC LWR MW-3903	MW-24 (E. of Security Bldg)	04-42810202	(909) 590-1828	(909) 590-1498	Tony Ford

PROJECT CONTACT	PROJECT PHONE NUMBER	PROJECT FAX	LABORATORY ADDRESS	ADDRESS
J. Robinson	(909) 295-7886	(909) 396-1455	13760 Magnolia	22632 Golden Springs Dr #270

PROJECT ADDRESS	CITY, STATE AND ZIP CODE	CLIENT	CITY, STATE AND ZIP CODE	CITY, STATE AND ZIP CODE
4800 Oak Grove Dr.	Pasadena CA.	US NAVY SMOBIC	Ching A.	Diamond Bar, CA. 91765

PROJECT CONTACT	PROJECT PHONE NUMBER	PROJECT FAX	LABORATORY PHONE	LABORATORY FAX
Aster Fsheem	(909) 396-7662	(909) 396-1455	524.2 (VOC)	314.0 (Hex Chrom)

Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont.	QC Level	T.A.T	Analyses		Comments
									X	X	
1	MW-24-4	H <sub>2</sub> O	8/6/03	0926	3141	III	Numerical		X	X	
2	MW-24-3			0950					X	X	
3	MW-24-2			1041					X	X	MSMSD
4	MW-24-1			1123					X	X	
5	Dupe-4-3-003			1018		IV			X	X	4558
6											
7											
8											
9											
10											

SAMPLES COLLECTED BY	REINQUIRED BY	COURIER AND AIR BILL NUMBER	RECEIVED BY	DATE	TIME	COOLER TEMPERATURE UPON RECEIPT
Leo W. Williamson	Leo W. Williamson		Ronald Stewart	8/6/03	0906	
			Ronald Stewart	8/6/03	1531	
			Ronald Stewart	8/6/03	1655	

Distribution: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager





INCORPORATED  
22632 GOLDEN SPRINGS DR., SUITE 270  
DIAMOND BAR, CA 91765 • (909) 396-7662 • FAX (909) 396-1455

CHAIN-OF-CUSTODY RECORD

LABORATORY COPY

MW-11 2050

GEOPON, LAB COORDINATOR: Brad Shojae  
LAB COORDINATOR'S PHONE: (909) 396-7662  
LAB COORDINATOR'S FAX: (909) 396-1455  
LABORATORY SERVICE ID: -  
LABORATORY CONTACT: Kang Chan  
MAIL REPORT (COMPANY NAME): GEOFON, INC.

PROJECT NAME: SPL GW MON-3003  
PROJECT LOCATION: MW-11 (S. of B1 277)  
PROJECT NUMBER: 04-4428.10  
LABORATORY PHONE: (909) 590-1828  
LABORATORY FAX: (909) 590-1498  
RECIPIENT NAME: Tony Ford

PROJECT CONTACT: J. Robinson  
PROJECT PHONE NUMBER: (914) 9208729  
PROJECT FAX: (909) 386-1455  
LABORATORY ADDRESS: 15760 Magnolia Ave  
CITY, STATE AND ZIP CODE: Chino, CA 91710  
ADDRESS: 22632 Golden Springs Dr. #270  
CITY, STATE AND ZIP CODE: Diamond Bar, CA. 91765

PROJECT ADDRESS: 4800 Oak Grove Dr  
CITY, STATE AND ZIP CODE: Pasadena, CA.  
CLIENT: US NAVY SWAIR  
PROJECT MANAGER'S PHONE: (909) 396-7662  
PROJECT MANAGER'S FAX: (909) 396-1455

PROJECT MANAGER: Astrar Faeem

Item	Sample Identifier	Matrix	Date	Time	Preserved	# of Cont	QC Level	T.A.T	Analyses			Comments
									H <sub>2</sub> O	HCl	Normal	
1	MW-11-4	H <sub>2</sub> O	8/1/03	0945	None	3+1+1	III	Normal	X	X	X	
2	MW-11-3								X	X	X	
3	MW-11-2								X	X	X	
4	MW-11-1								X	X	X	
5												
6												
7												
8												
9												
10												

SAMPLES COLLECTED BY: Leo W. Williamson  
COURIER AND AIR BILL NUMBER:  
COOLER TEMPERATURE UPON RECEIPT:

RELINQUISHED BY: Leo W. Williamson  
RECEIVED BY: [Signature]  
DATE: 08/02/03  
TIME: 0802

DISTRIBUTION: White - Laboratory (To be returned with Analytical Report); Goldenrod - Project File; Yellow - Project Data Manager

4558

